


Data Path : Z:\HPCHEM1\BNA E\DATA\BE040816\
Data File : BE091605.D
Acq On : 8 Apr 2016 9:57
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 08 16:48:14 2016

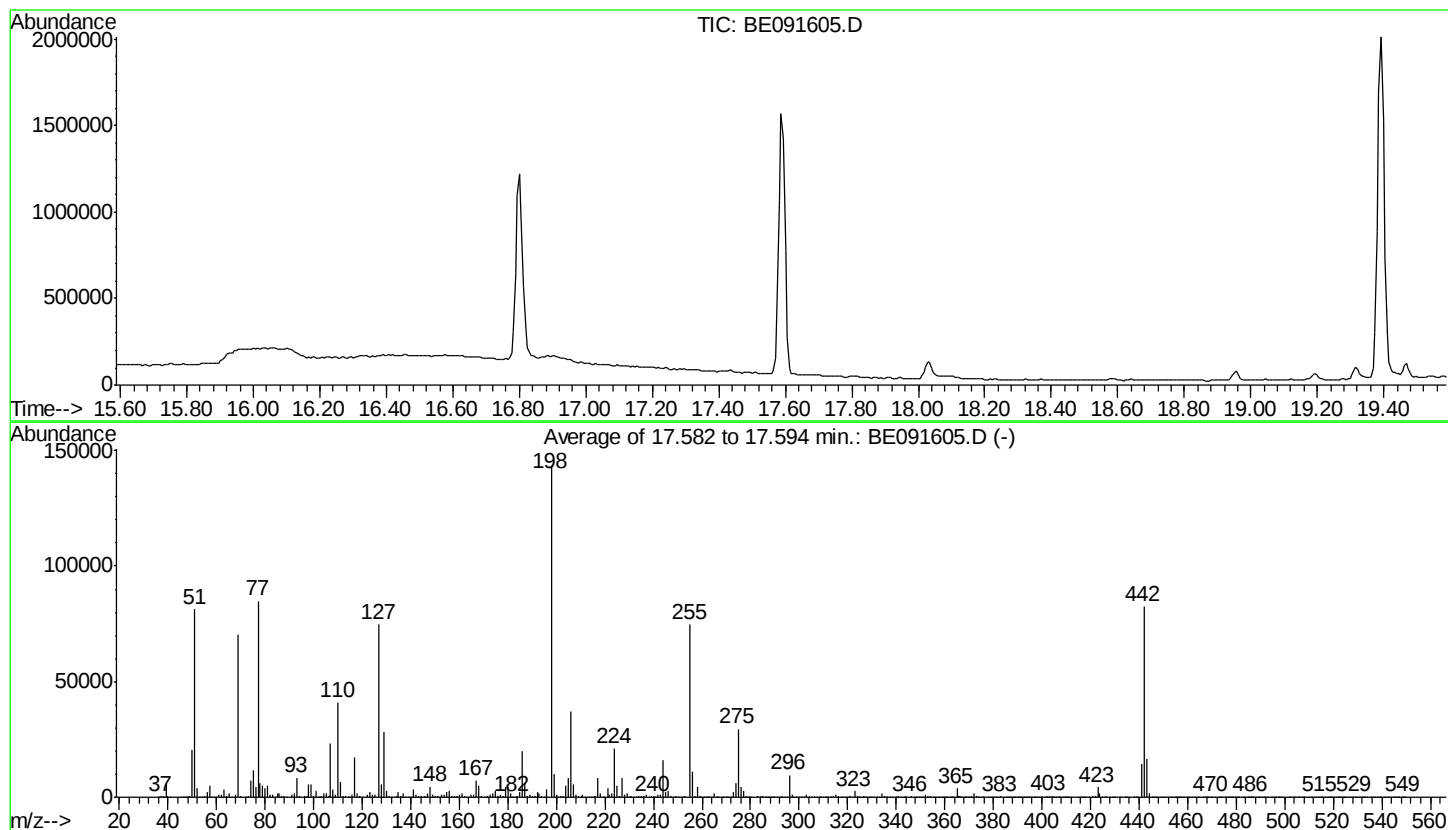

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.7	81301	PASS
68	69	0.00	2	1.8	1247	PASS
69	198	0.00	100	49.1	70416	PASS
70	69	0.00	2	0.5	367	PASS
127	198	10	80	52.1	74745	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143459	PASS
199	198	5	9	7.0	10015	PASS
275	198	10	60	20.5	29404	PASS
365	198	1	100	2.7	3866	PASS
441	442	0.01	24	17.2	14191	PASS
442	198	50	100	57.5	82478	PASS
443	442	15	24	19.8	16366	PASS