

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE040918\
 Data File : BE095964.D
 Acq On : 9 Apr 2018 13:14
 Operator : SJ/JU
 Sample : J2135-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 X2C46

Quant Time: Apr 10 03:57:21 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 03:47:21 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	1980	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5255	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2918	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	7053	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	8946	0.40	ng/ul	0.00
20) Perylene-d12	24.39	264	7188	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.77	152	2588	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	9493	0.33	ng/ul	0.00
Target Compounds				Qvalue		
3) Naphthalene	11.26	128	6929	0.472	ng/ul#	88
5) 2-Methylnaphthalene	12.84	142	5200	0.523	ng/ul	99
7) Acenaphthylene	14.70	152	8521	0.563	ng/ul	97
8) Acenaphthene	15.04	153	6995	0.645	ng/ul	95
11) Pentachlorophenol	17.34	266	2171	1.454	ng/ul	96
13) Anthracene	17.81	178	10889	0.526	ng/ul#	91
17) Pyrene	20.05	202	26203	0.862	ng/ul#	79
19) Chrysene	21.82	228	16778	0.645	ng/ul	97
21) Benzo(b)fluoranthene	23.58	252	19283	0.829	ng/ul	85
22) Benzo(k)fluoranthene	23.64	252	28289	1.221	ng/ul#	85
25) Dibenzo(a,h)anthracene	27.21	278	16965	0.845	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE040918\
Data File : BE095964.D
Acq On : 9 Apr 2018 13:14
Operator : SJ/JU
Sample : J2135-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
X2C46

Quant Time: Apr 10 03:57:21 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 03:47:21 2018
Response via : Initial Calibration

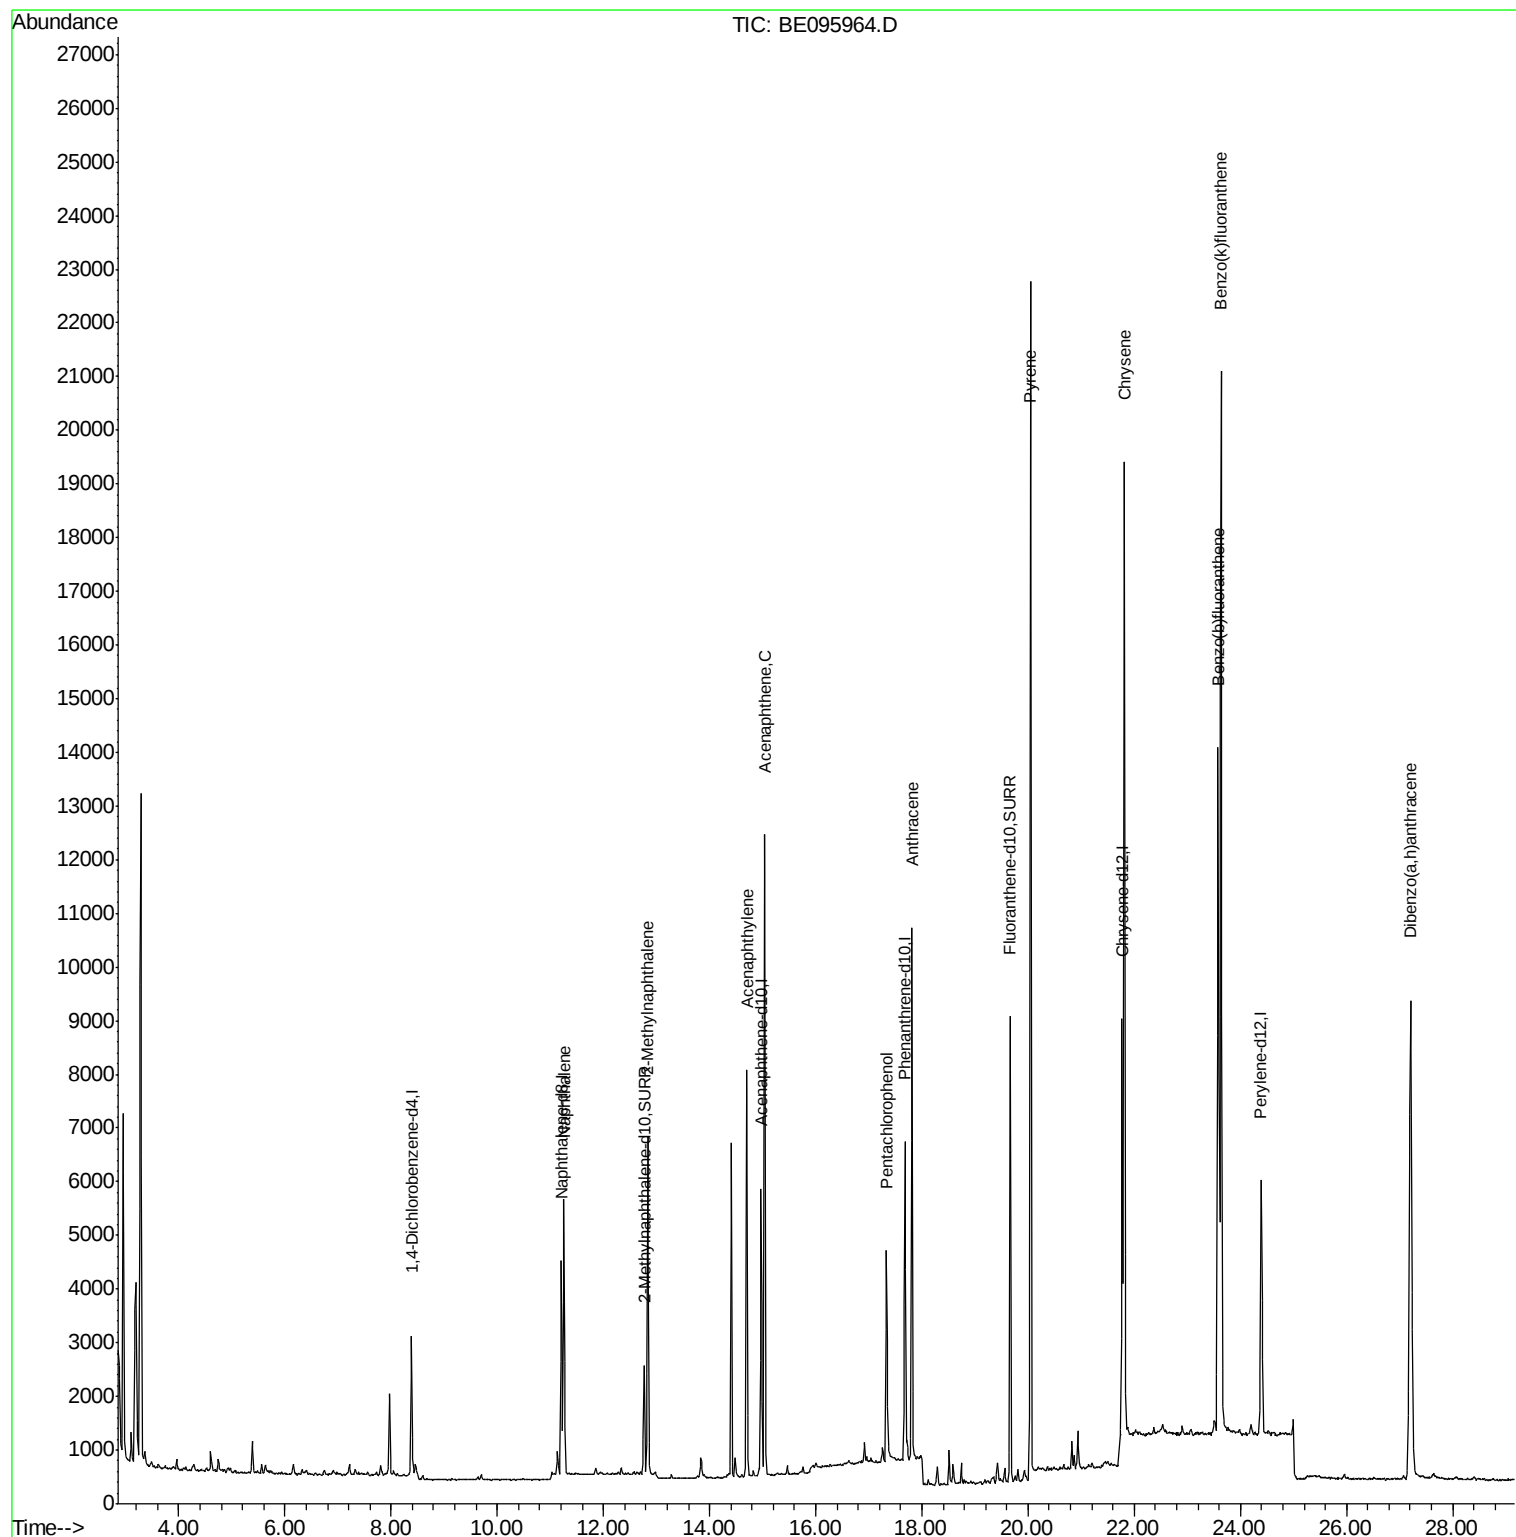

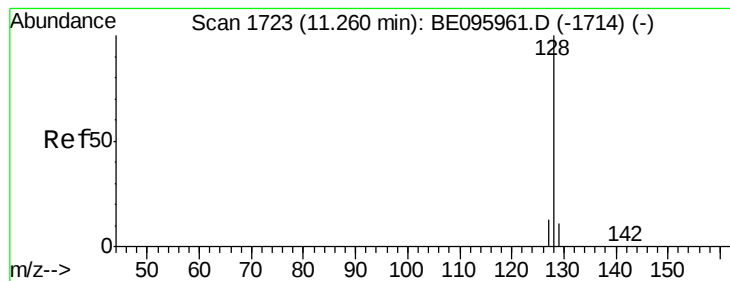

#3

Naphthalene

Concen: 0.472 ng/ul

RT: 11.26 min Scan# 1722

Delta R.T. -0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46


Tgt Ion:128 Resp: 6929

Ion Ratio Lower Upper

128 100

129 11.8 11.3 16.9




127 14.5 4.0 6.0#

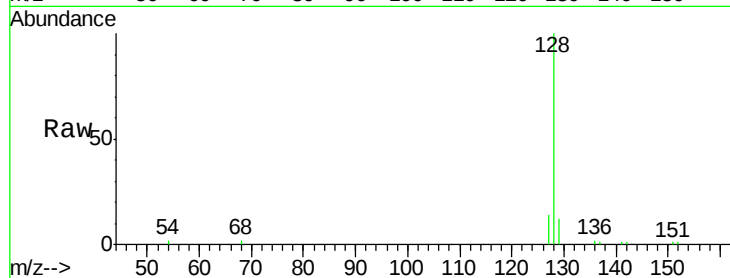

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

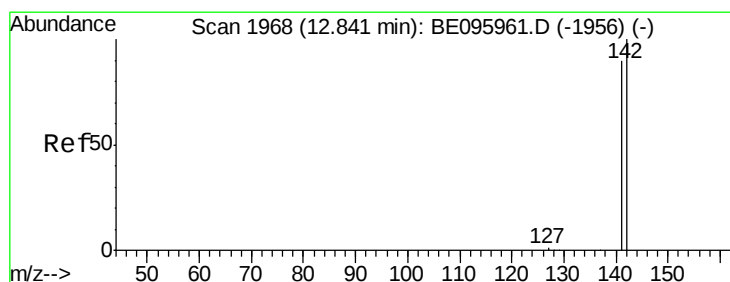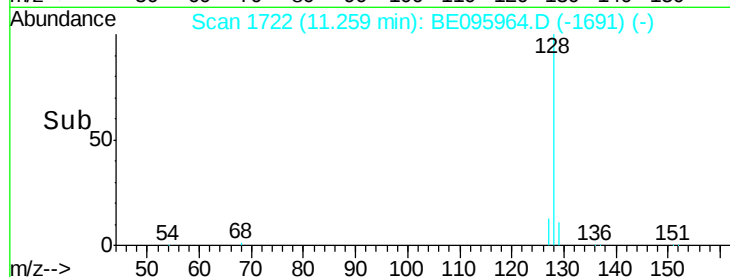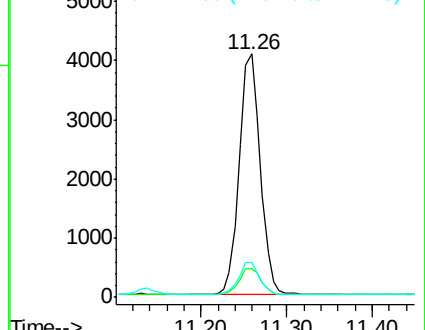

#5

2-Methylnaphthalene

Concen: 0.523 ng/ul

RT: 12.84 min Scan# 1967

Delta R.T. -0.00 min

Lab File: BE095964.D


Acq: 9 Apr 2018 13:14

Tgt Ion:142 Resp: 5200

Ion Ratio Lower Upper



142 100


141 90.0 72.6 108.8

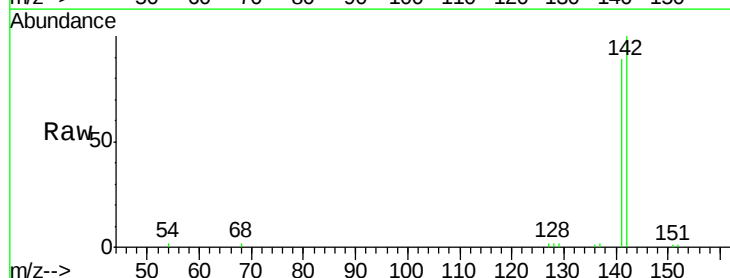

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

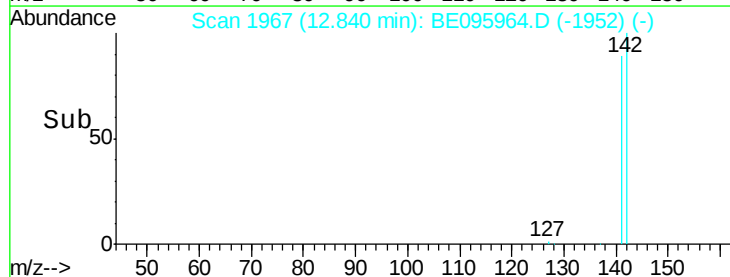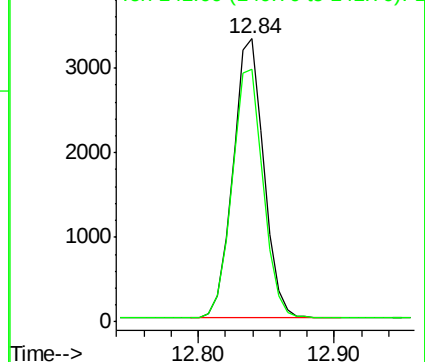

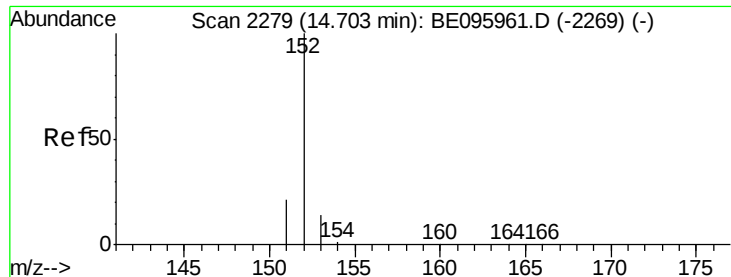

#7

Acenaphthylene

Concen: 0.563 ng/ul

RT: 14.70 min Scan# 2278

Delta R.T. -0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46


Tgt Ion:152 Resp: 8521

Ion Ratio Lower Upper

152 100

151 20.3 17.1 25.7




153 14.1 12.8 19.2

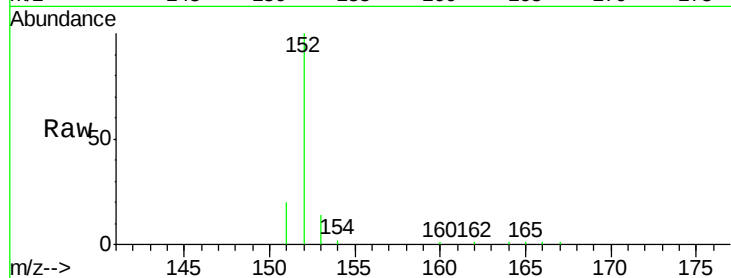

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

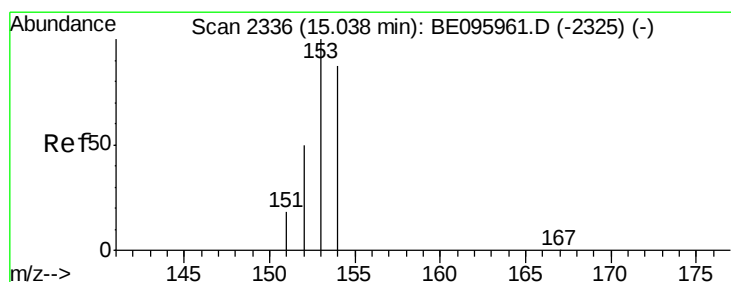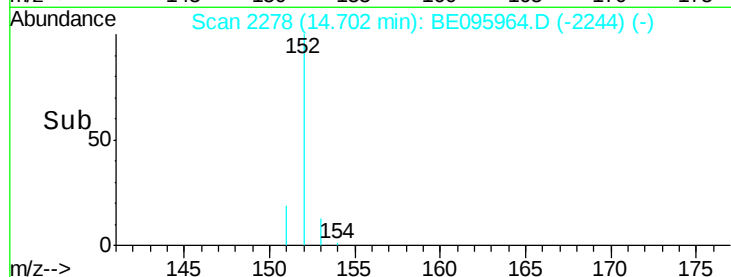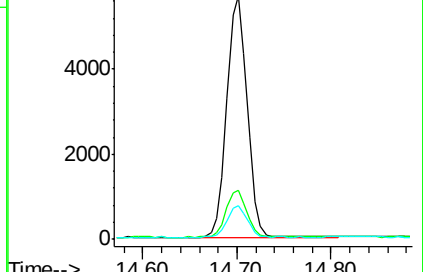

#8

Acenaphthene

Concen: 0.645 ng/ul

RT: 15.04 min Scan# 2335

Delta R.T. -0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14


Tgt Ion:153 Resp: 6995

Ion Ratio Lower Upper

153 100

152 47.2 36.0 54.0



154 84.8 72.0 108.0

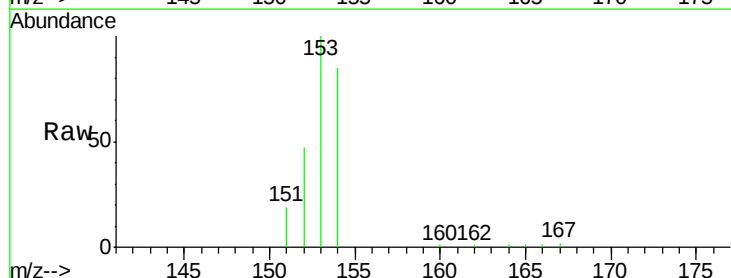


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

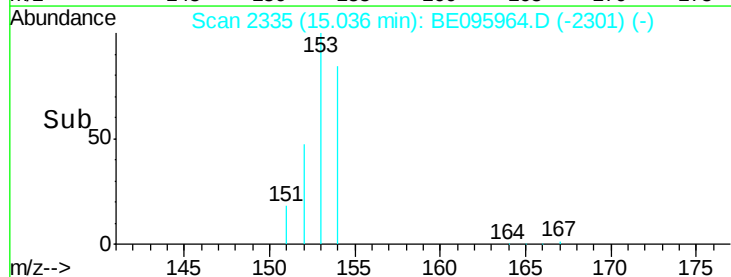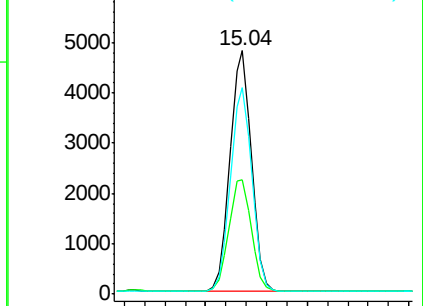

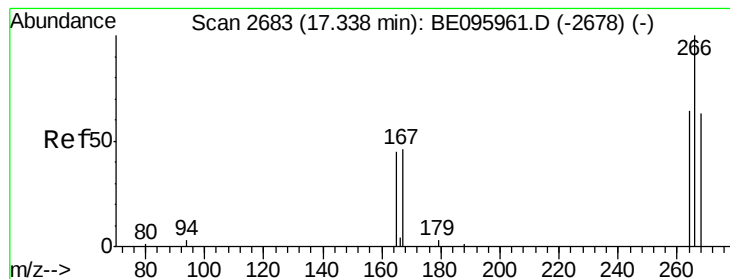

#11

Pentachlorophenol

Concen: 1.454 ng/ul

RT: 17.34 min Scan# 2683

Delta R.T. 0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46


Tgt Ion:266 Resp: 2171

Ion Ratio Lower Upper

266 100

264 63.8 47.9 71.9




268 64.1 49.8 74.8

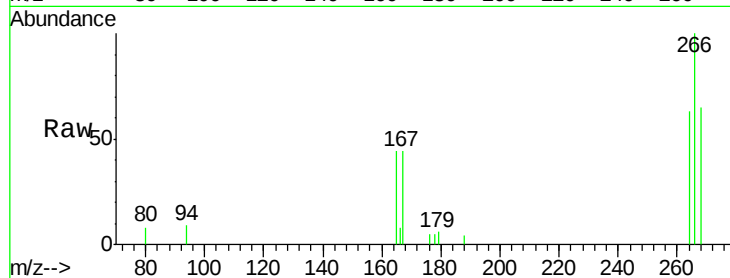

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

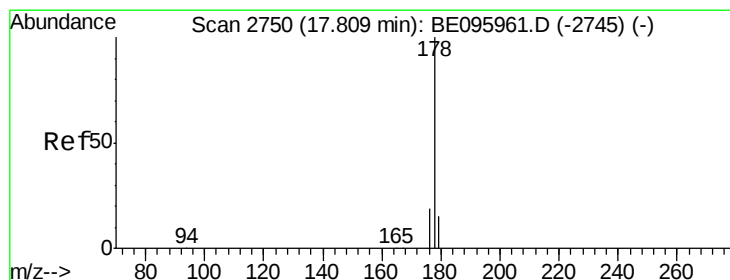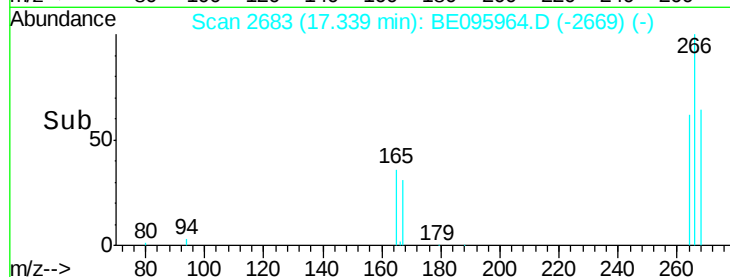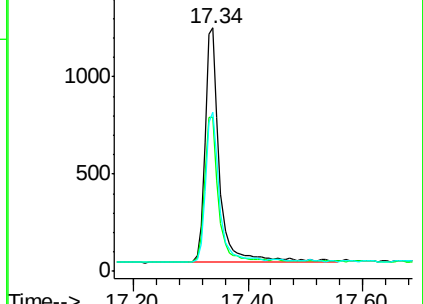

#13

Anthracene

Concen: 0.526 ng/ul

RT: 17.81 min Scan# 2750

Delta R.T. 0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14


Tgt Ion:178 Resp: 10889

Ion Ratio Lower Upper

178 100

179 15.7 18.1 27.1#



176 19.8 14.7 22.1

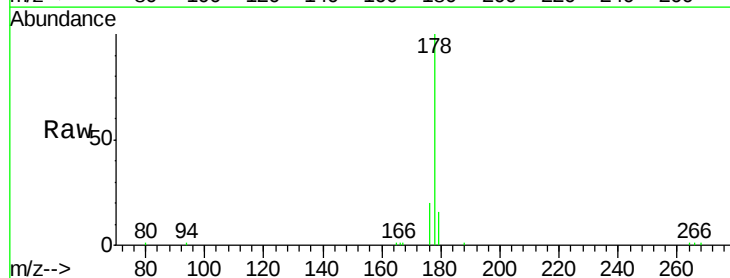


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

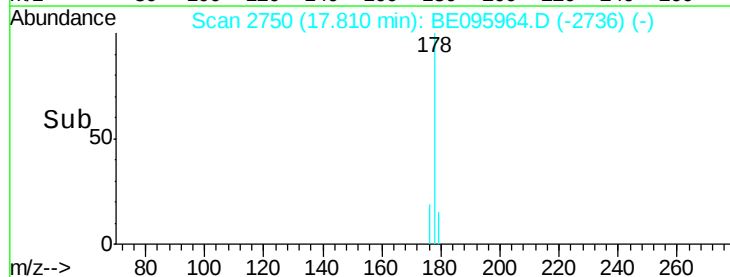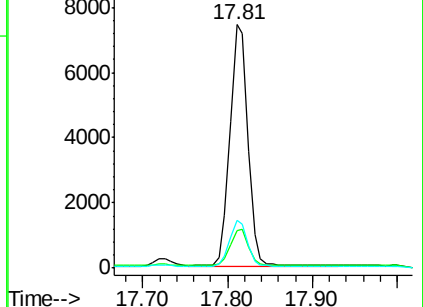

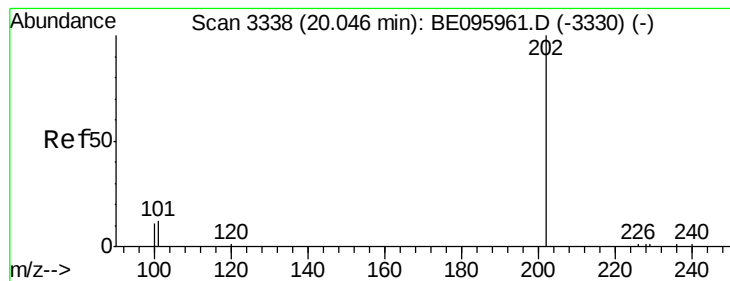

#17

Pyrene

Concen: 0.862 ng/ul

RT: 20.05 min Scan# 3337

Delta R.T. -0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46


Tgt Ion:202 Resp: 26203

Ion Ratio Lower Upper

202 100

101 12.0 18.2 27.4#




100 10.5 15.6 23.4#

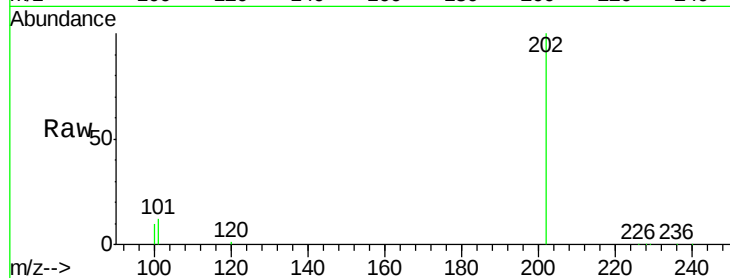

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

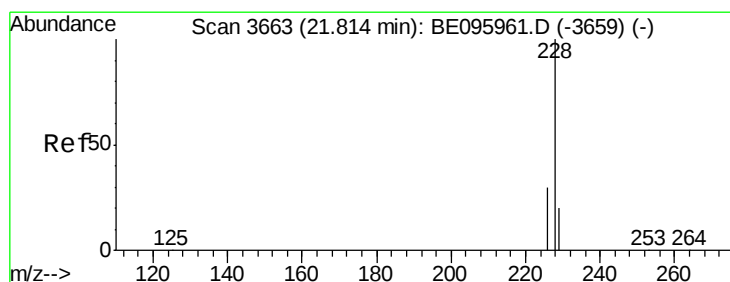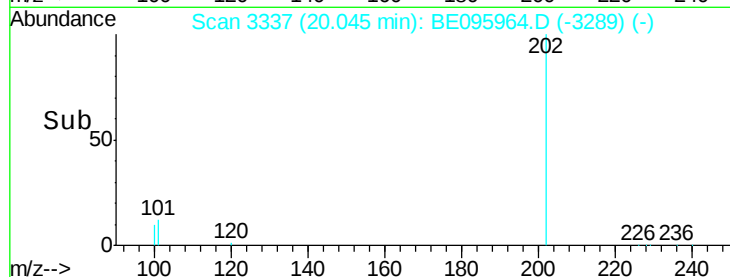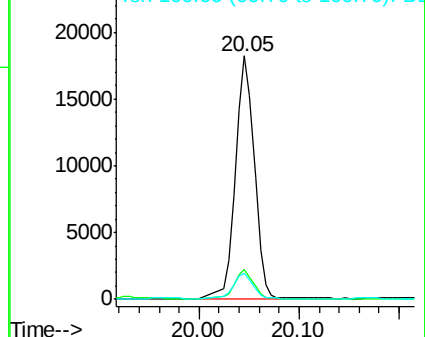

#19

Chrysene

Concen: 0.645 ng/ul

RT: 21.82 min Scan# 3662

Delta R.T. 0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14


Tgt Ion:228 Resp: 16778

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.0



229 20.3 17.7 26.5

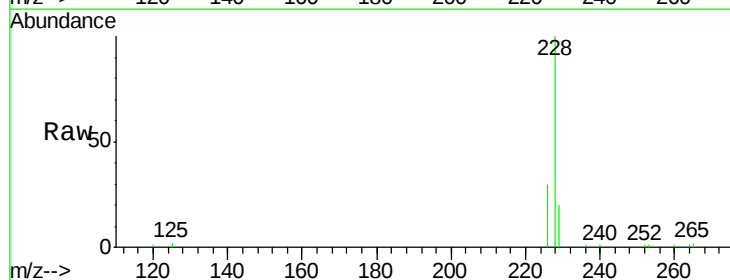


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

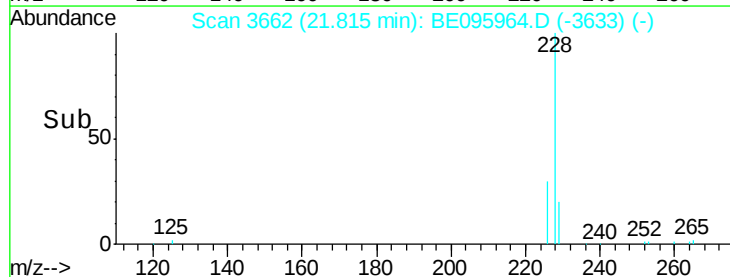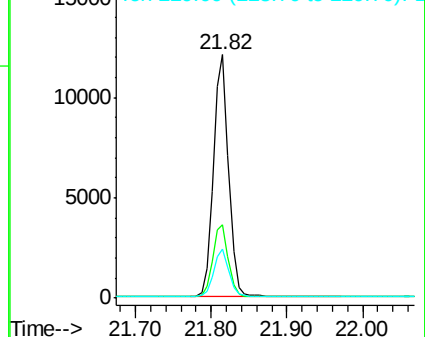

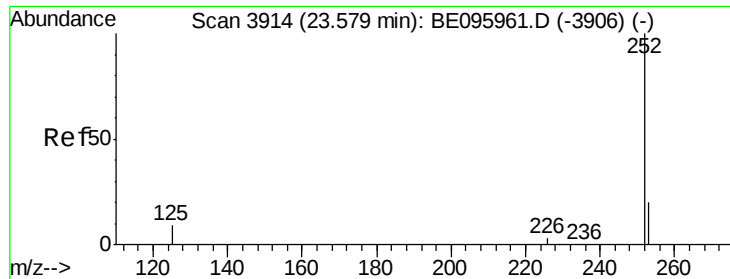

#21

Benzo(b)fluoranthene

Concen: 0.829 ng/ul

RT: 23.58 min Scan# 3913

Delta R.T. 0.00 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46


Tgt Ion:252 Resp: 19283

Ion Ratio Lower Upper

252 100

253 22.9 0.0 64.2




125 11.7 0.0 35.0

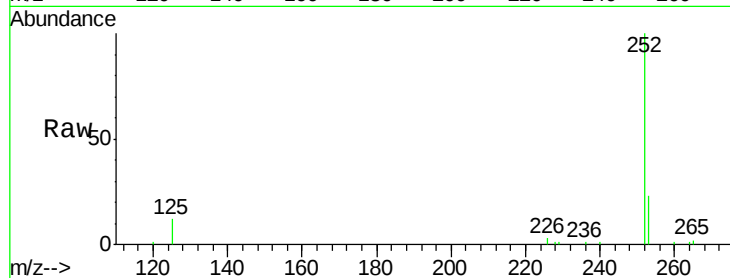

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

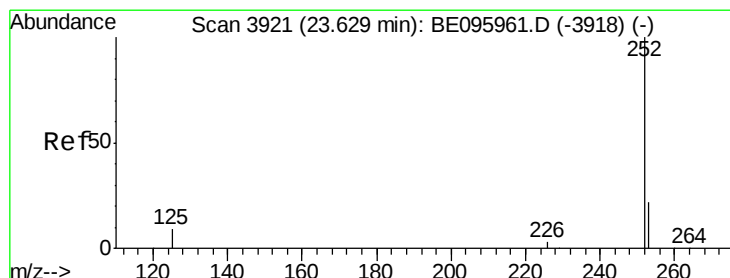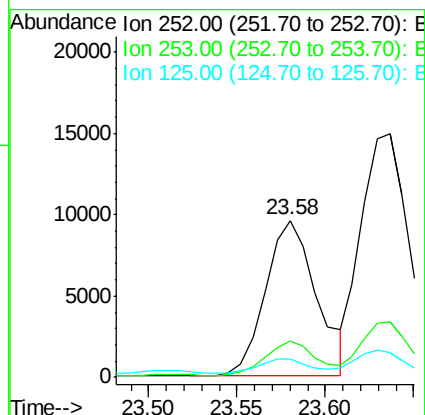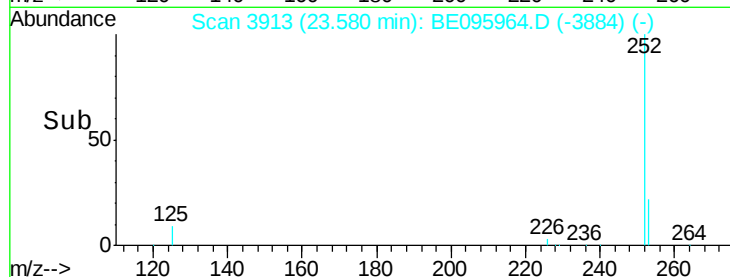

#22

Benzo(k)fluoranthene

Concen: 1.221 ng/ul

RT: 23.64 min Scan# 3921

Delta R.T. 0.01 min

Lab File: BE095964.D

Acq: 9 Apr 2018 13:14


Tgt Ion:252 Resp: 28289

Ion Ratio Lower Upper

252 100

253 22.6 24.5 36.7#



125 10.1 13.7 20.5#

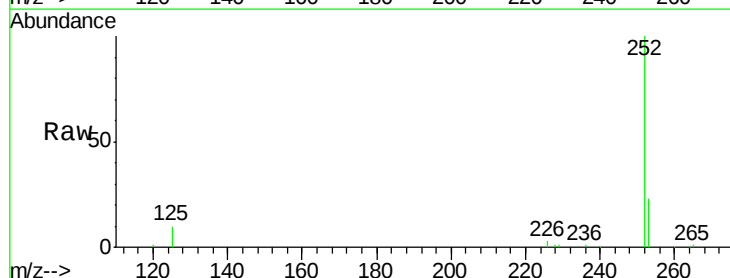


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

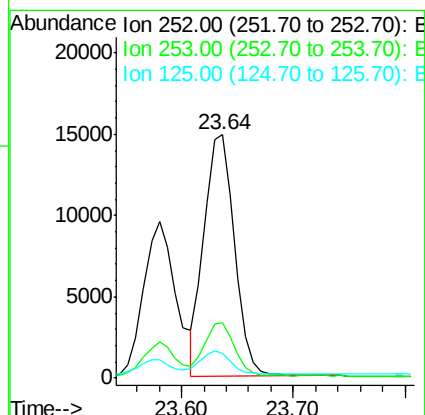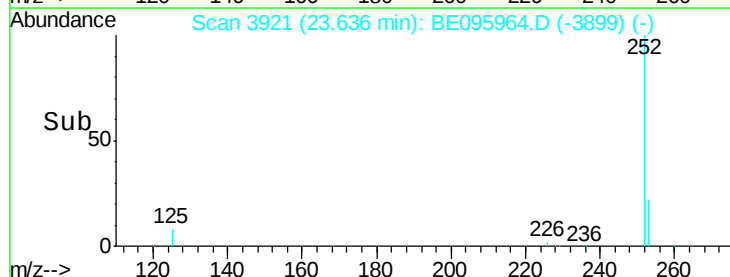

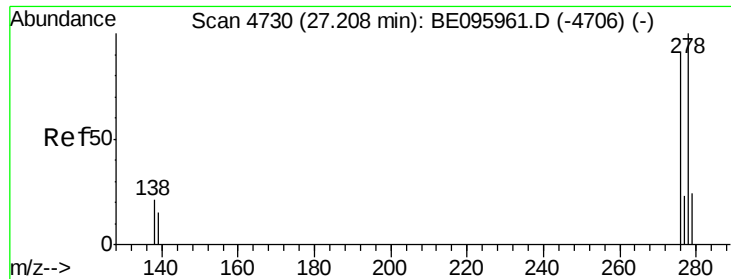

#25

Dibenzo(a,h)anthracene

Concen: 0.845 ng/ul

RT: 27.21 min Scan# 4728

Delta R.T. -0.00 min

Lab File: BE095964.D


Acq: 9 Apr 2018 13:14

Instrument :

BNA_E

ClientSampleId :

X2C46

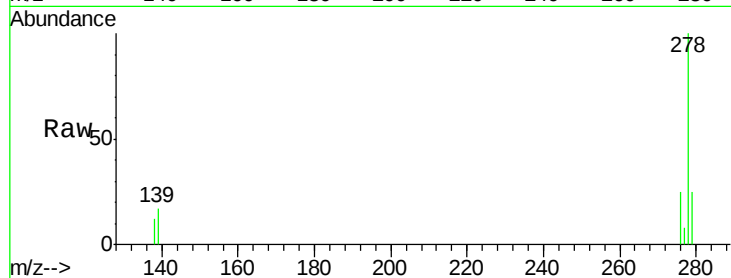

Tgt Ion: 278 Resp: 16965

Ion Ratio Lower Upper

278 100

139 17.1 17.4 26.0#

279 24.7 25.9 38.9#

