
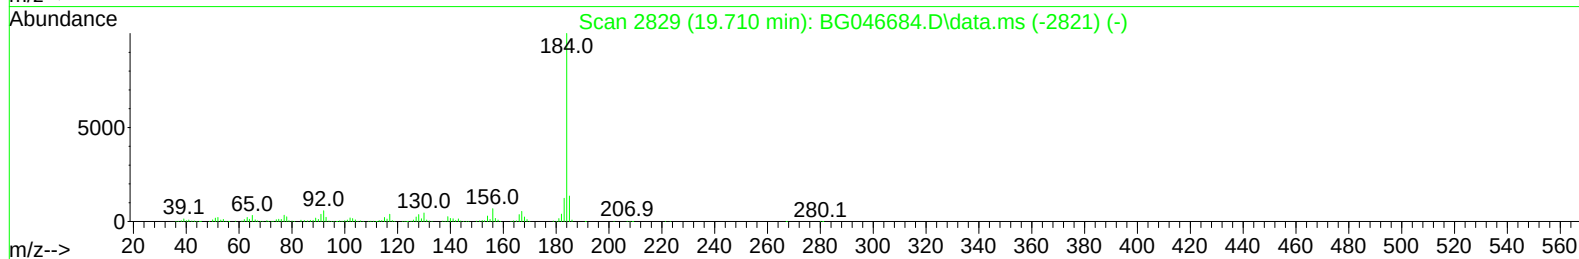
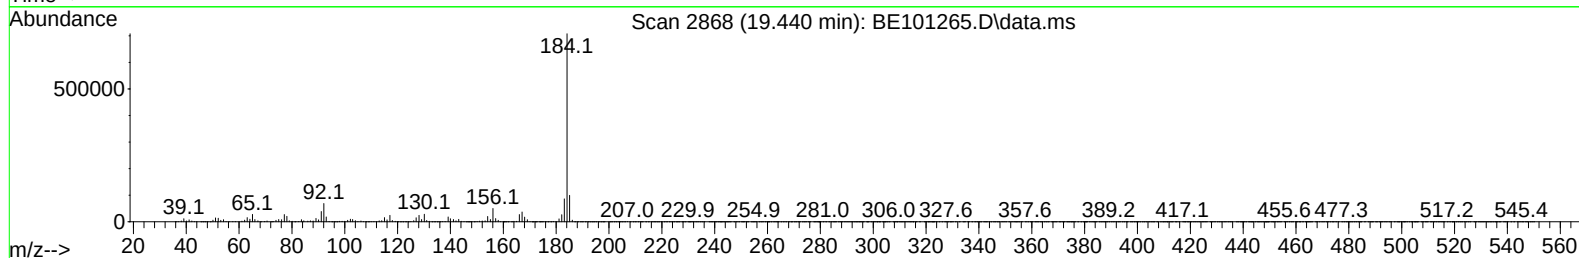


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040921\
Data File : BE101265.D
Acq On : 9 Apr 2021 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 11:05:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

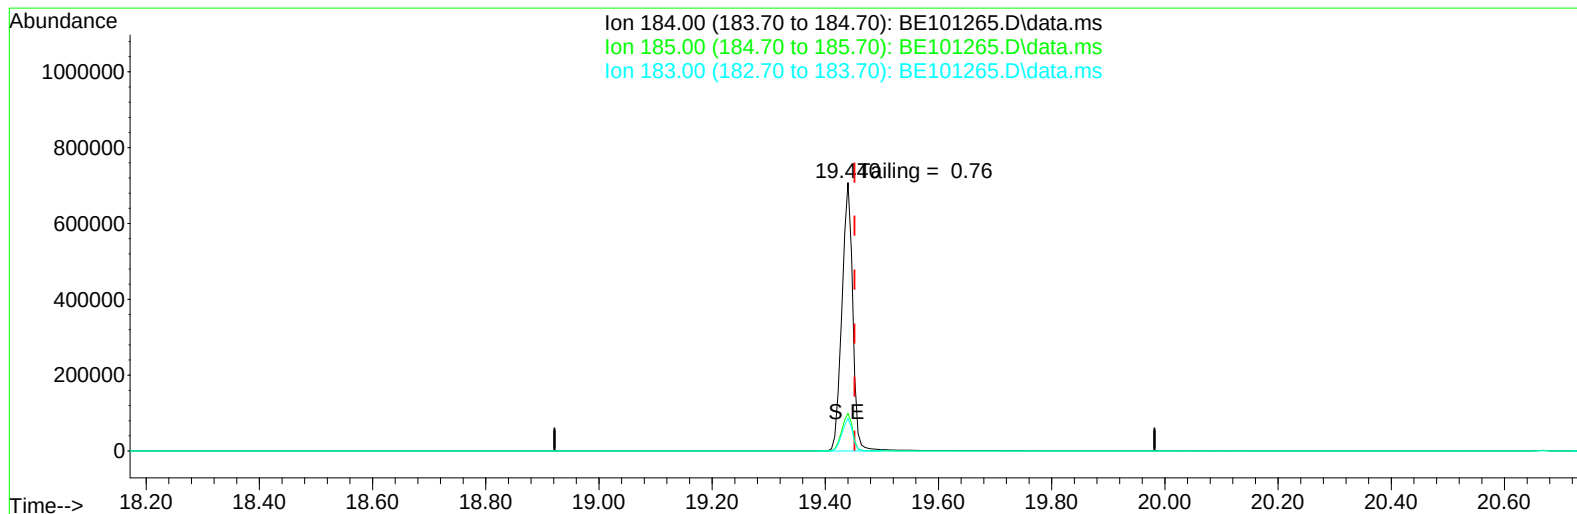




TIC: BE101265.D\data.ms

(77) Benzidine**19.440min (-0.011) 4343.87 ng****response 948423**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040921\
Data File : BE101265.D
Acq On : 9 Apr 2021 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 11:05:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

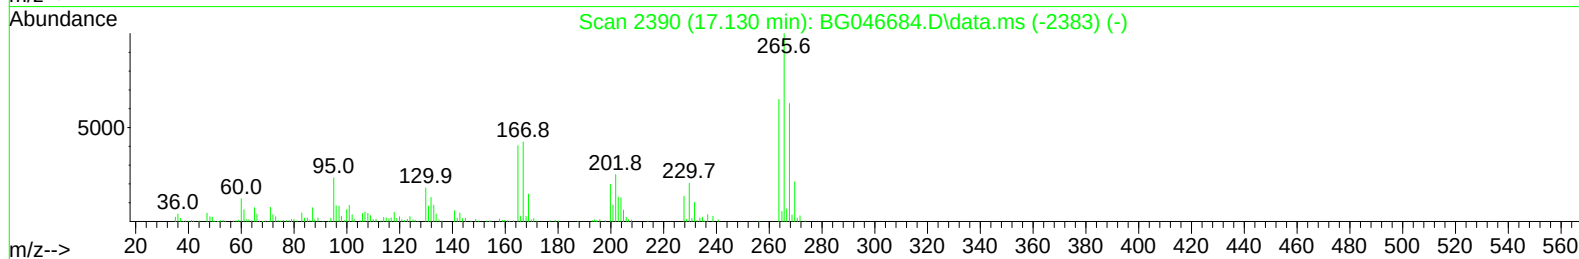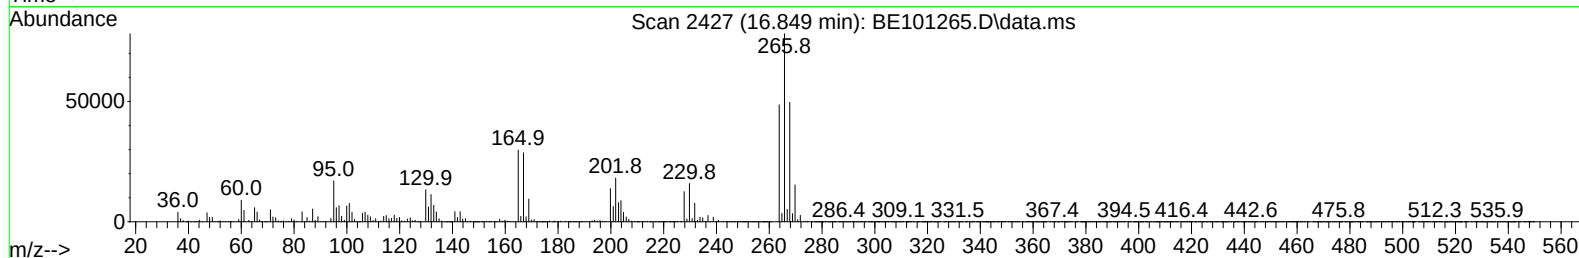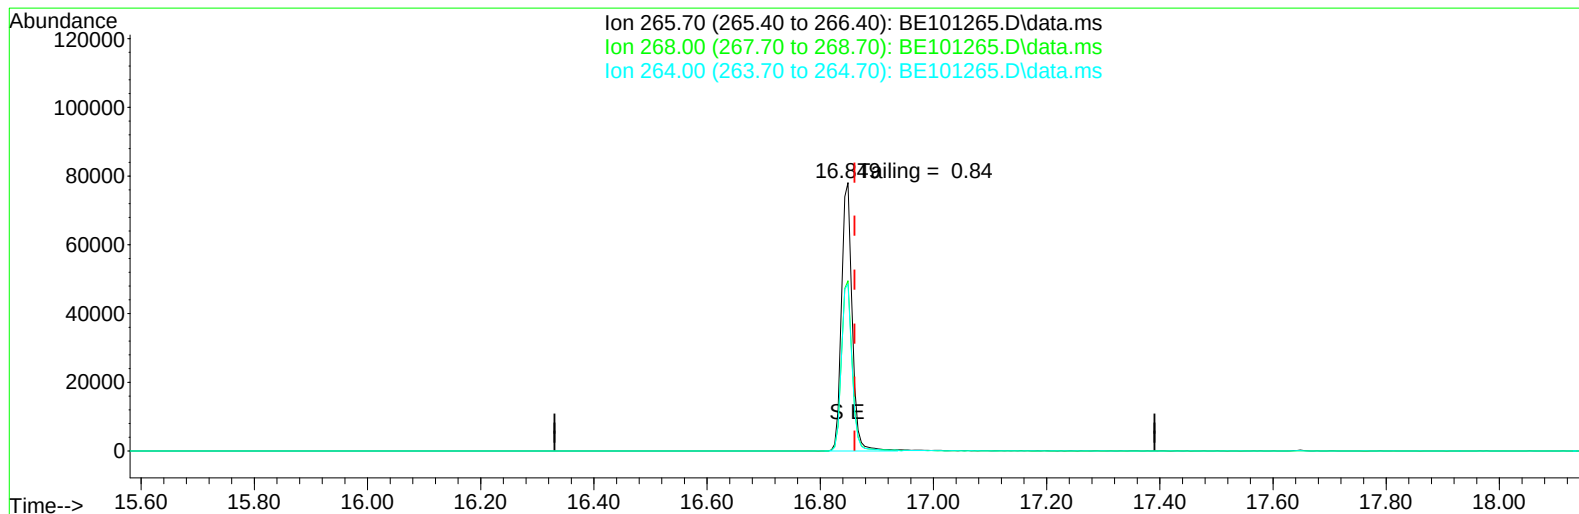

TIC: BE101265.D\data.ms

(70) Pentachlorophenol (C)

16.849min (-0.011) 620463.09 ng

response 102254

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.46
264.00	61.60	62.19
0.00	0.00	0.00