
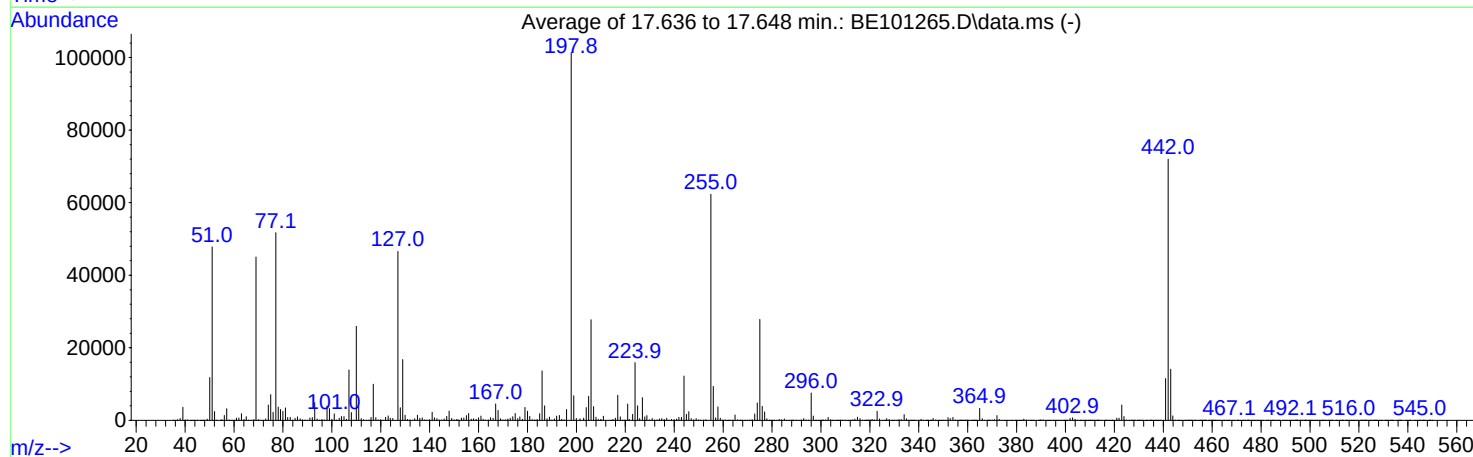


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040921\
 Data File : BE101265.D
 Acq On : 9 Apr 2021 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE040621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 07 10:22:45 2021

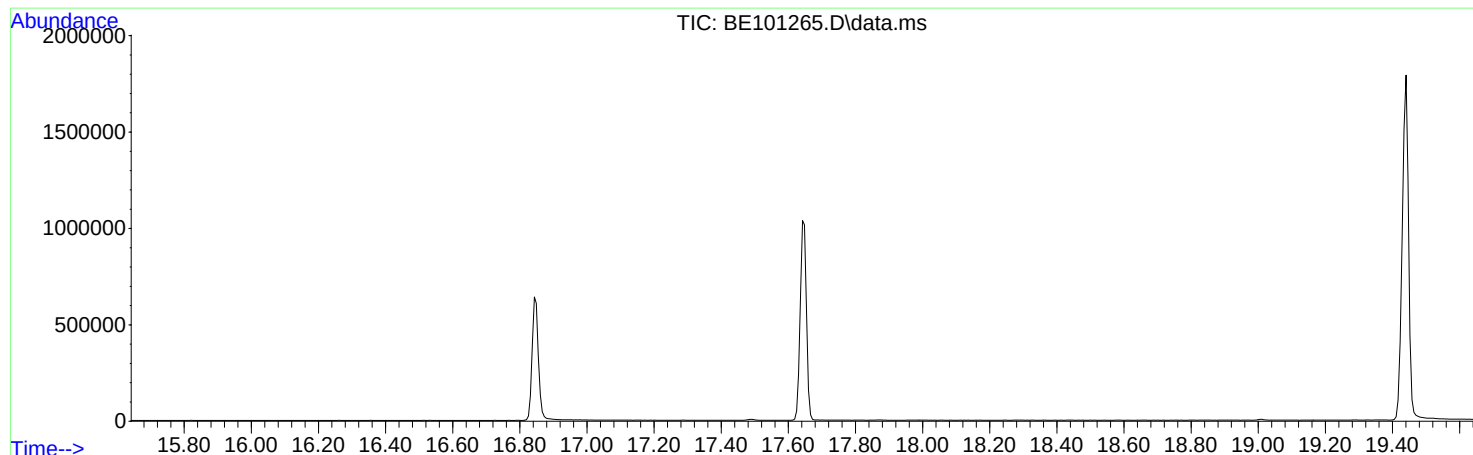




AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	47827	PASS
68	69	0.00	2	0.5	226	PASS
69	198	0.00	100	44.4	45014	PASS
70	69	0.00	2	0.4	181	PASS
127	198	10	80	46.0	46588	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101386	PASS
199	198	5	9	6.7	6792	PASS
275	198	10	60	27.5	27833	PASS
365	198	1	100	3.3	3325	PASS
441	198	0.01	100	11.4	11528	PASS
442	442	50	100	100.0	72027	PASS
443	442	15	24	19.6	14113	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040921\
Data File : BE101265.D
Acq On : 9 Apr 2021 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 09 11:05:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

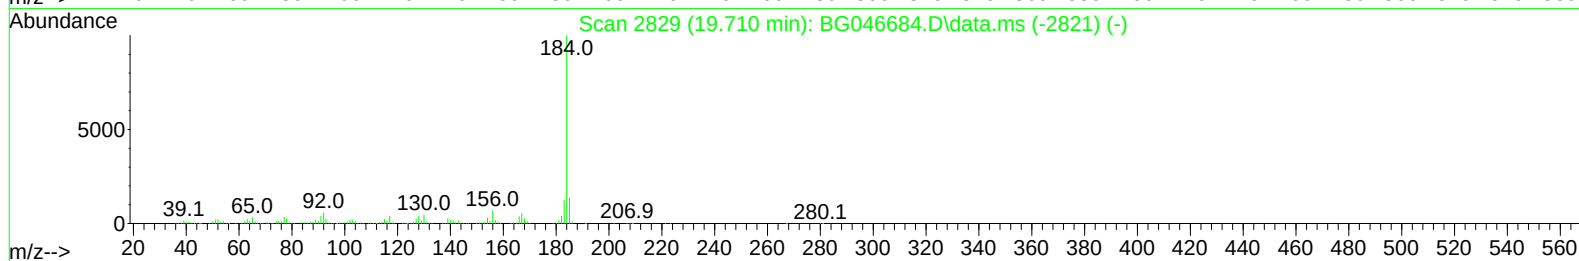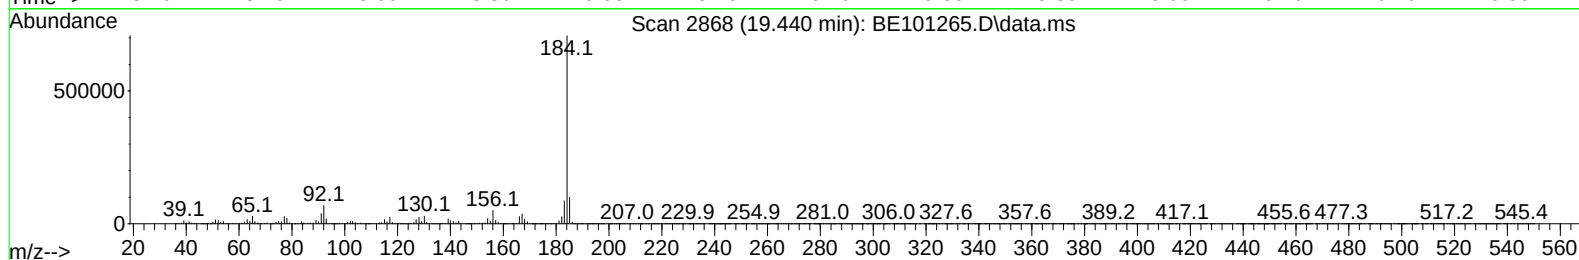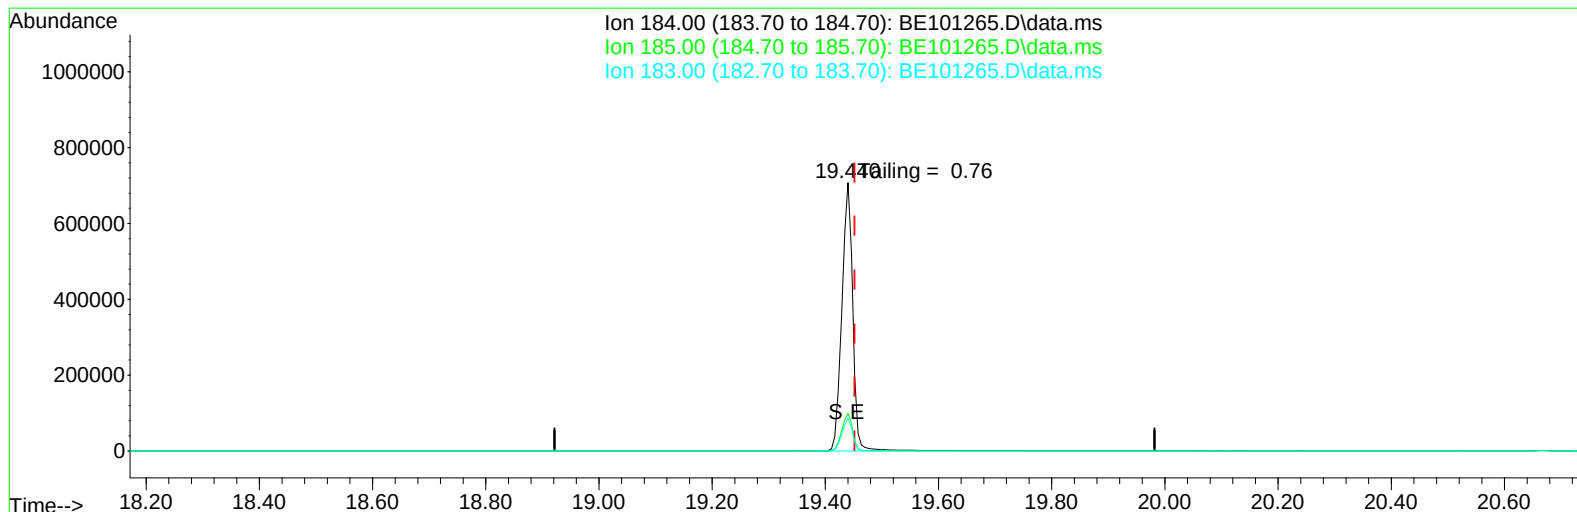

TIC: BE101265.D\data.ms

(77) Benzidine

19.440min (-0.011) 4343.87 ng




response 948423

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.01
183.00	13.20	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE040921\
 Data File : BE101265.D
 Acq On : 9 Apr 2021 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 09 11:05:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

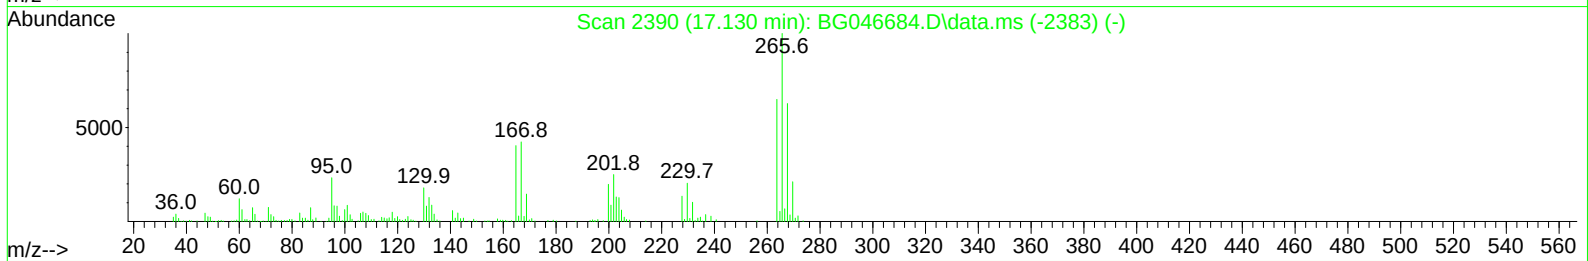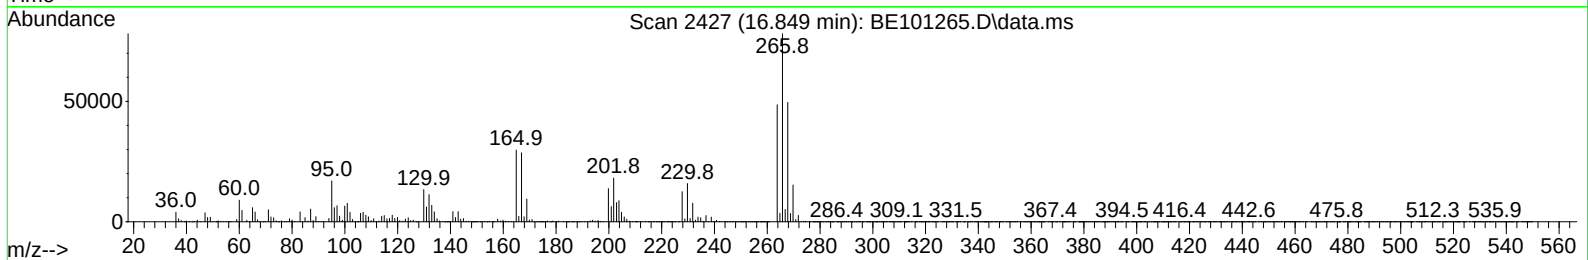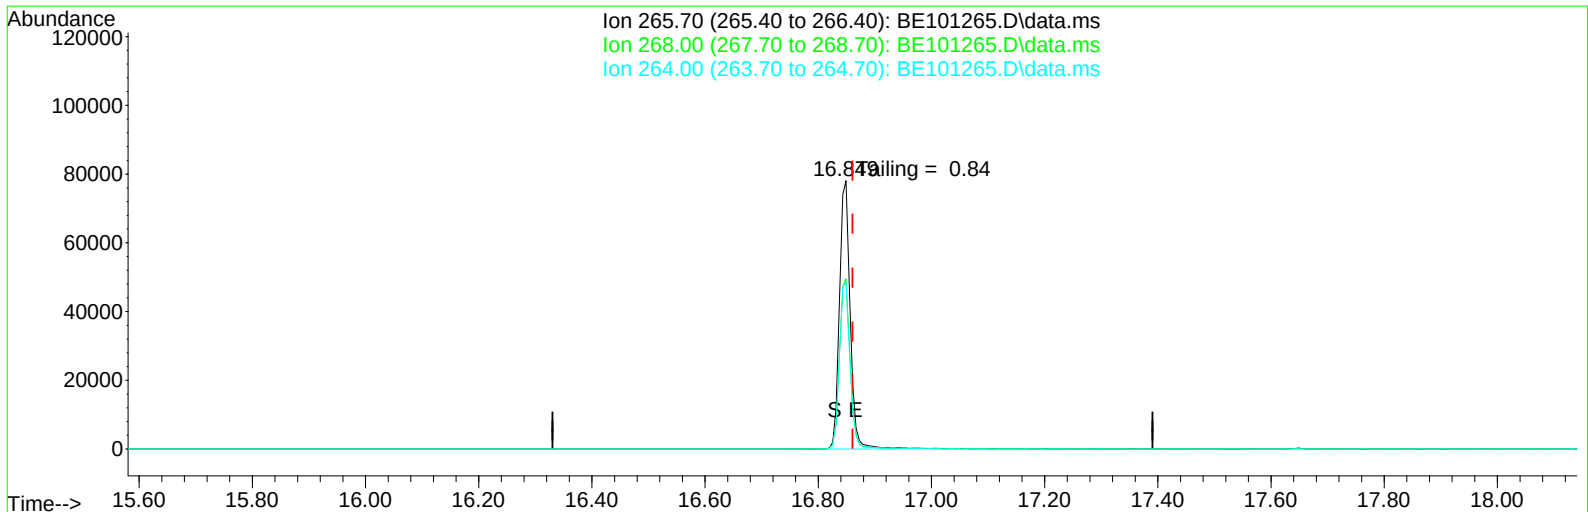

TIC: BE101265.D\data.ms

(70) Pentachlorophenol (C)

16.849min (-0.011) 620463.09 ng

response 102254

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.46
264.00	61.60	62.19
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/9/2021	BNA_E	BE101265.D
Compound Name	Response	Retention Time
DDT	474694	20.66
DDD	11431	20.22
DDE	1019	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12450	487144	2.56