
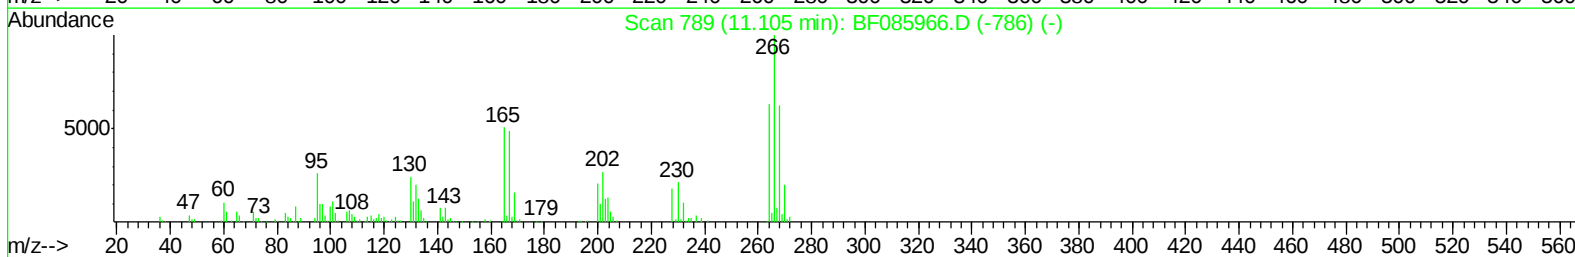
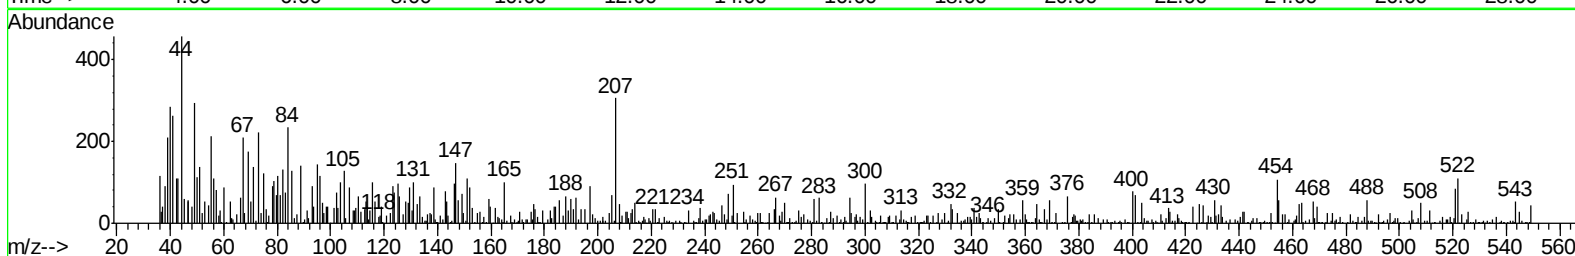


Data Path : Z:\HPCHEM1\BNA_E\Data\BE041116\
Data File : BE091619.D
Acq On : 11 Apr 2016 9:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

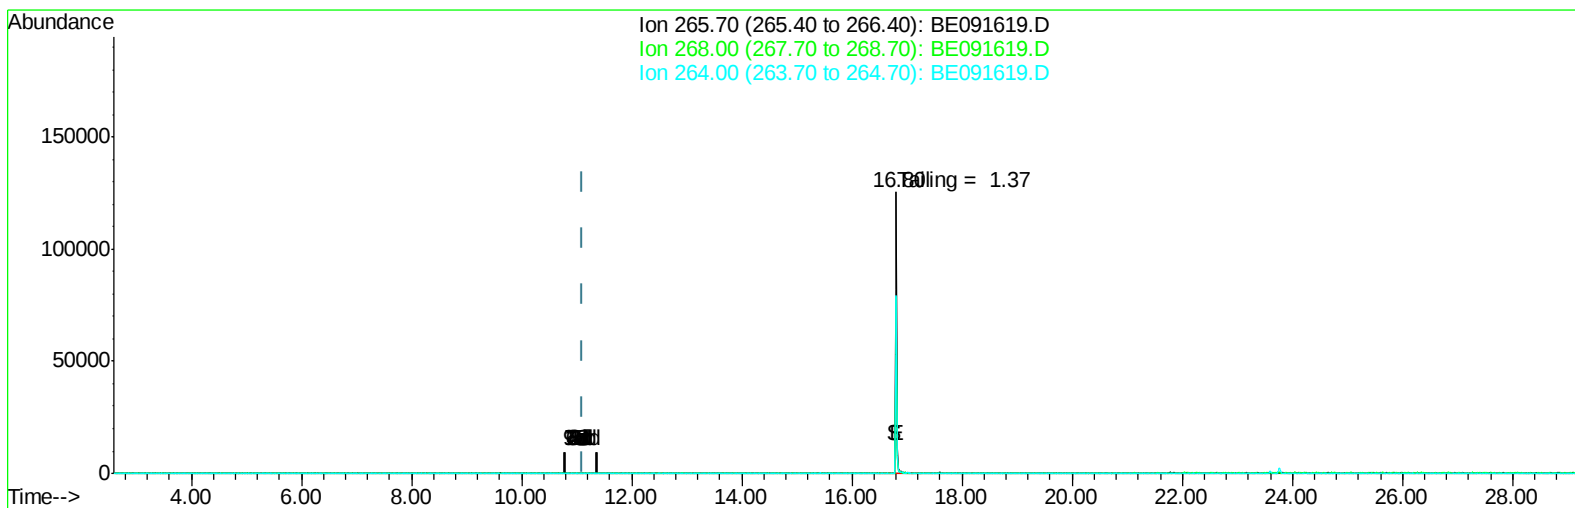

TIC: BE091619.D

(69) Pentachlorophenol (C)




10.896min (-0.209) 101.05ng

response 25

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	70.59
264.00	63.30	70.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE041116\
Data File : BE091619.D
Acq On : 11 Apr 2016 9:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:15:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

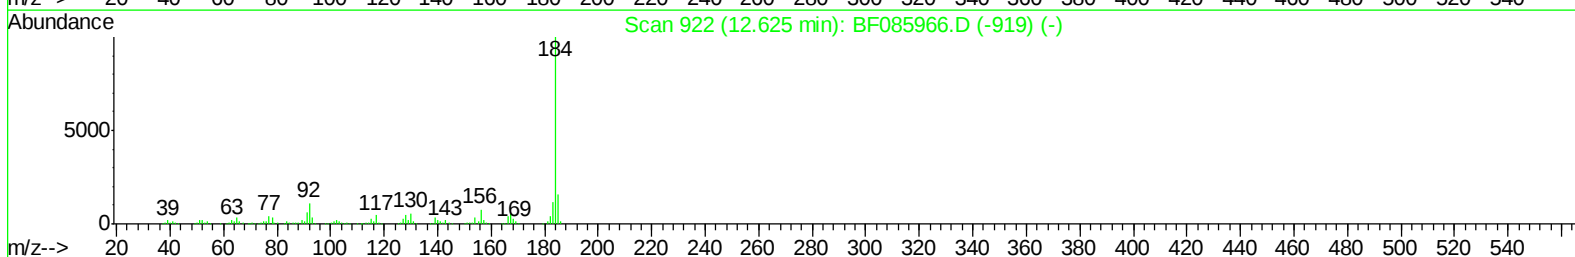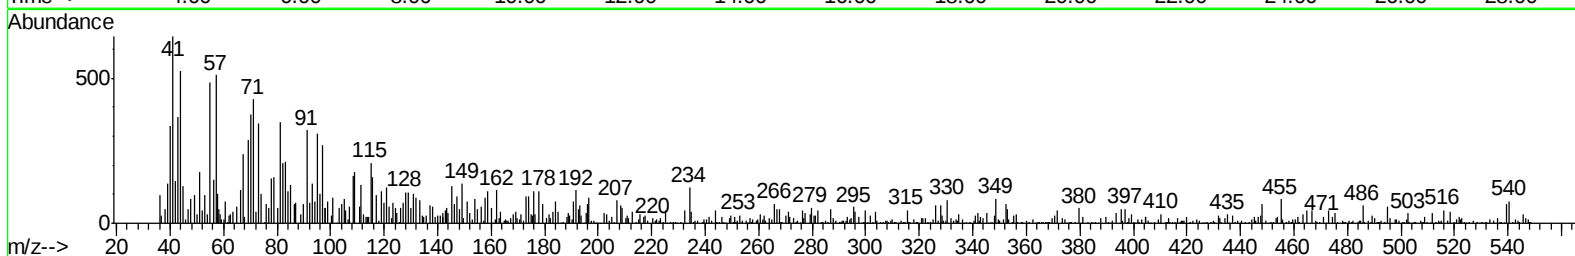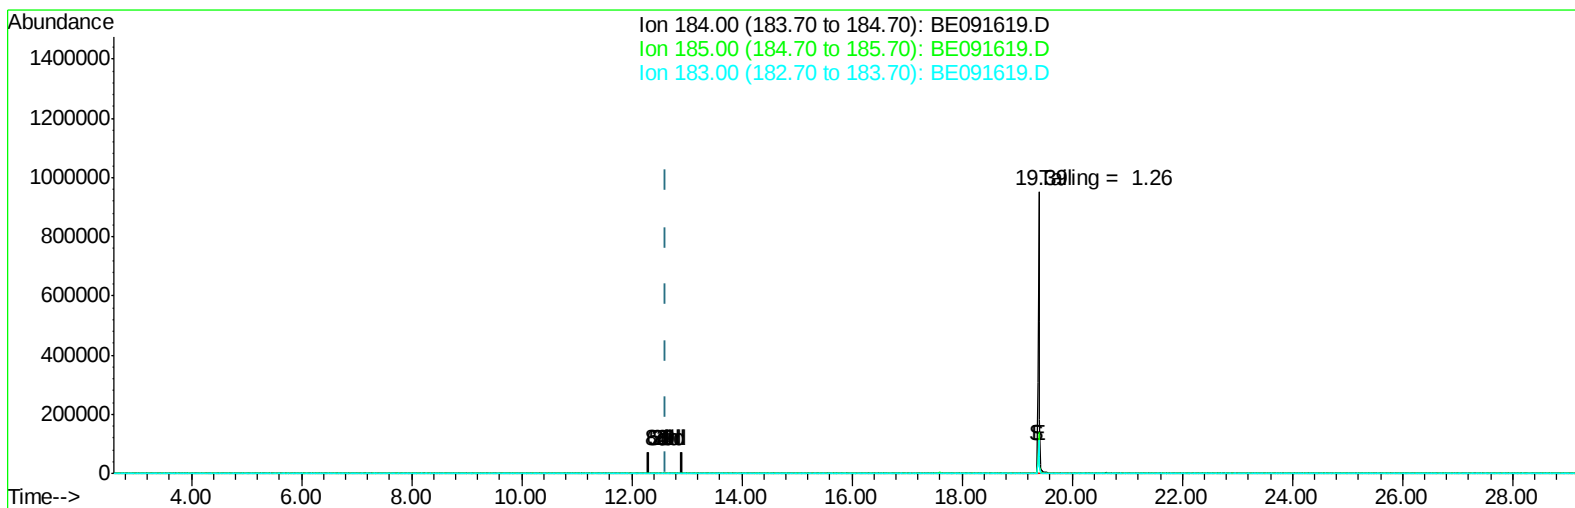

TIC: BE091619.D

(76) Benzidine

12.594min (-0.031) 52.33ng

response 72

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	55.41#
183.00	11.80	52.70#
0.00	0.00	0.00