
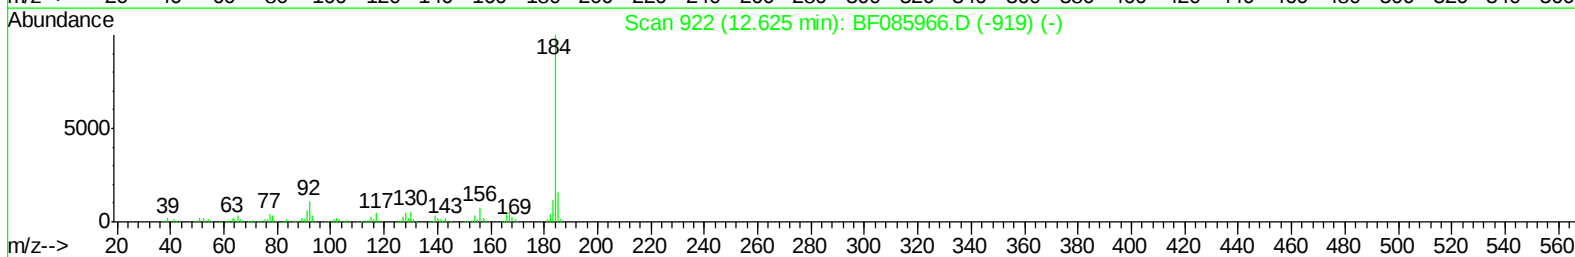
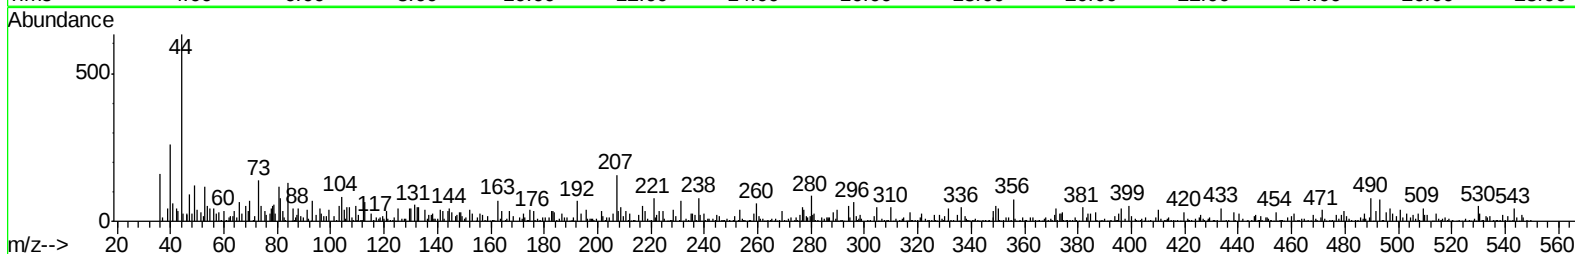


Data Path : Z:\HPCHEM1\BNA_E\Data\BE041116\
Data File : BE091632.D
Acq On : 11 Apr 2016 17:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:12:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

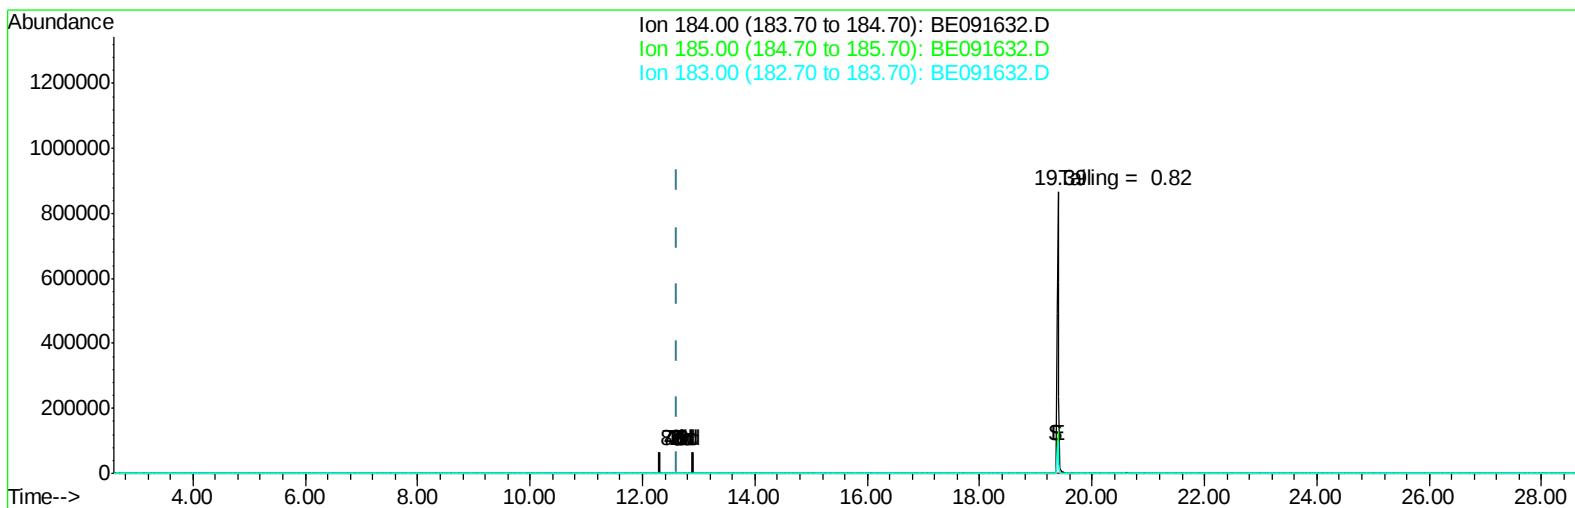

TIC: BE091632.D

(76) Benzidine




12.658min (+0.033) 68.02ng

response 24

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	22.22#
183.00	11.80	188.89#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE041116\
Data File : BE091632.D
Acq On : 11 Apr 2016 17:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 09:12:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

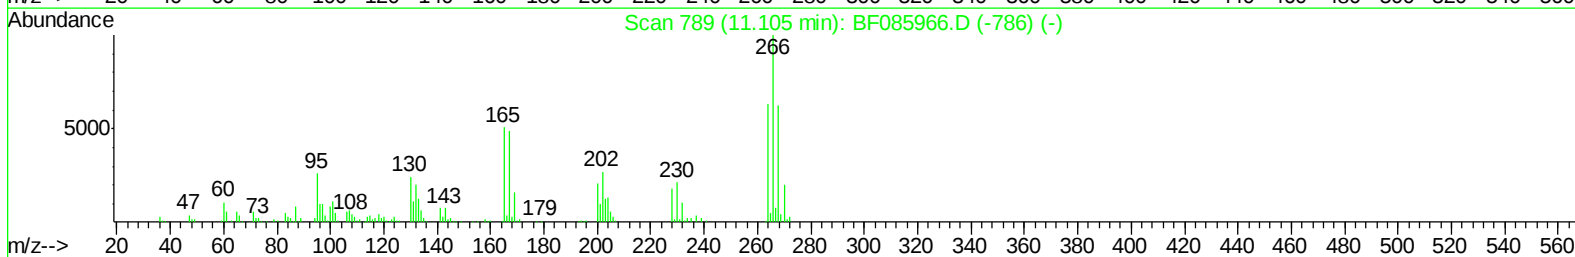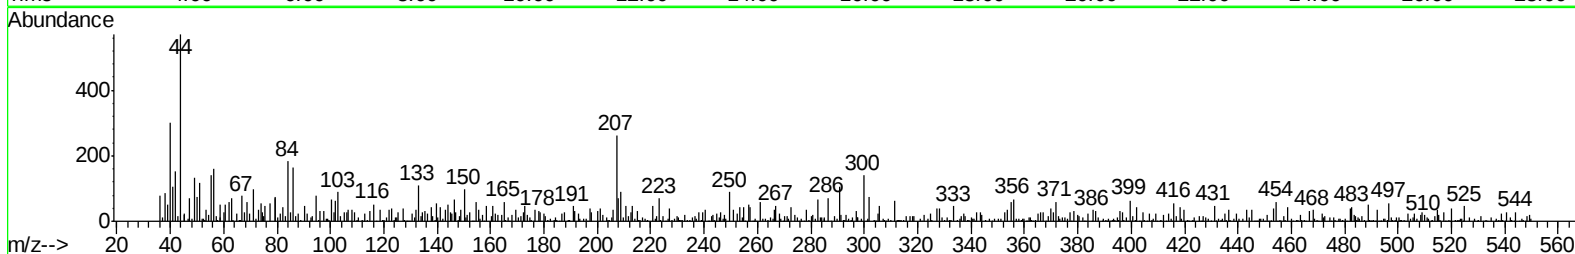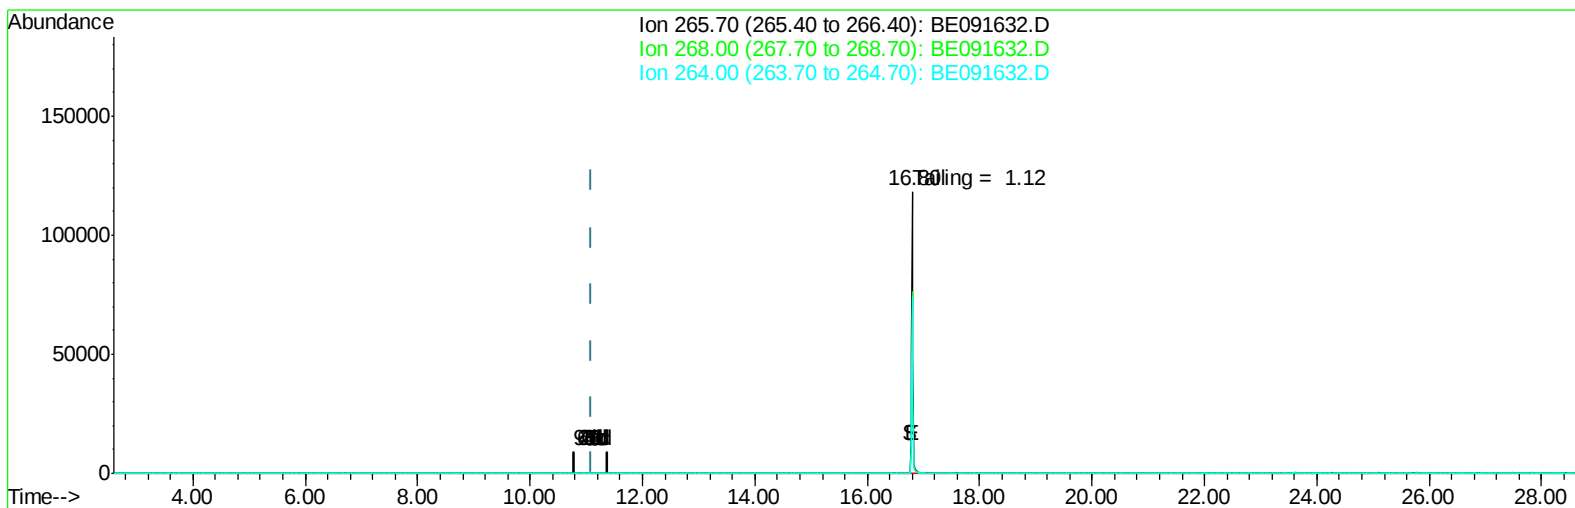

TIC: BE091632.D

(69) Pentachlorophenol (C)

11.153min (+0.049) 205.84ng

response 55

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	74.42
264.00	63.30	11.63#
0.00	0.00	0.00