


Data Path : Z:\HPCHEM1\BNA E\Data\BE041116\
Data File : BE091619.D
Acq On : 11 Apr 2016 9:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 08 16:48:14 2016

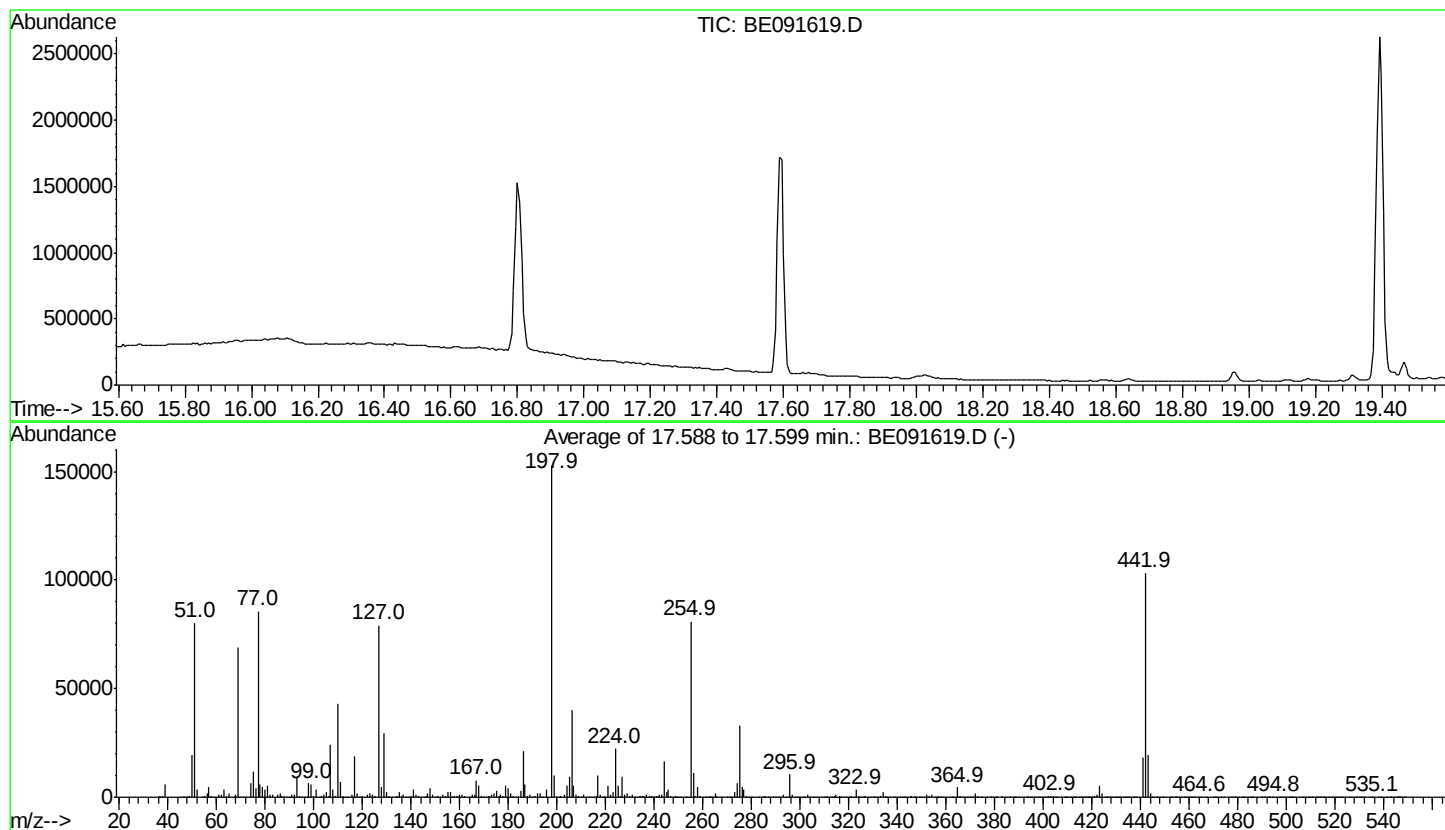

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	80318	PASS
68	69	0.00	2	1.7	1150	PASS
69	198	0.00	100	45.3	69146	PASS
70	69	0.00	2	0.5	318	PASS
127	198	10	80	51.7	78989	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	152687	PASS
199	198	5	9	6.7	10273	PASS
275	198	10	60	21.7	33072	PASS
365	198	1	100	3.0	4631	PASS
441	442	0.01	24	17.7	18279	PASS
442	198	50	100	67.7	103353	PASS
443	442	15	24	18.9	19506	PASS