


Data Path : Z:\HPCHEM1\BNA E\DATA\BE041116\
 Data File : BE091632.D
 Acq On : 11 Apr 2016 17:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 16:48:14 2016

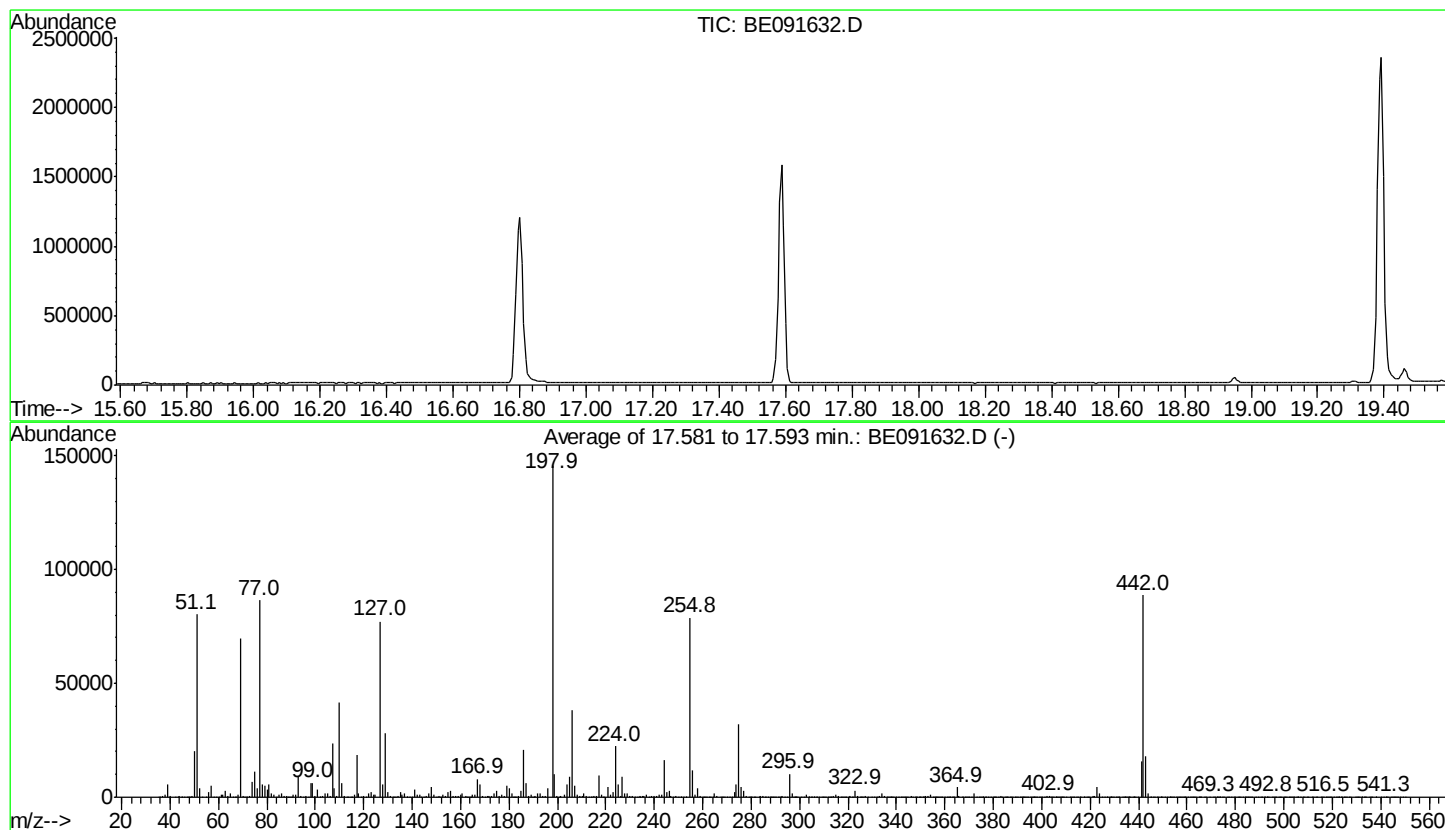

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	80094	PASS
68	69	0.00	2	1.8	1227	PASS
69	198	0.00	100	48.0	69848	PASS
70	69	0.00	2	0.5	358	PASS
127	198	10	80	53.1	77244	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145552	PASS
199	198	5	9	7.1	10278	PASS
275	198	10	60	21.8	31788	PASS
365	198	1	100	3.0	4416	PASS
441	442	0.01	24	17.8	15758	PASS
442	198	50	100	60.8	88528	PASS
443	442	15	24	20.4	18039	PASS