

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041118\
 Data File : BE095979.D
 Acq On : 11 Apr 2018 20:09
 Operator : SJ/JU
 Sample : J2215-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 12 04:16:42 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 11 17:26:43 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	1364	0.40	ng	0.00
7) Naphthalene-d8	11.22	136	5345	0.40	ng	0.00
13) Acenaphthene-d10	14.97	164	3002	0.40	ng	0.00
19) Phenanthrene-d10	17.68	188	6871	0.40	ng	0.00
27) Chrysene-d12	21.78	240	7453	0.40	ng	0.00
34) Perylene-d12	24.39	264	7125	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.88	112	711	0.17	ng	0.00
5) Phenol-d6	7.53	99	608	0.10	ng	0.00
8) Nitrobenzene-d5	9.57	82	3228	0.51	ng	0.00
11) 2-Methylnaphthalene-d10	12.76	152	3658	0.43	ng	0.00
14) 2,4,6-Tribromophenol	16.44	330	813	0.56	ng	0.00
15) 2-Fluorobiphenyl	13.61	172	9912	0.77	ng	0.00
25) Fluoranthene-d10	19.66	212	40106	0.43	ng	0.00
29) Terphenyl-d14	20.22	244	8898	0.54	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.61	88	22643	10.747	ng	# 88
6) bis(2-Chloroethyl)ether	7.78	93	464	0.091	ng	# 81
9) Naphthalene	11.27	128	1771	0.031	ng	# 88
12) 2-Methylnaphthalene	12.84	142	345	0.037	ng	# 84
22) Pentachlorophenol	17.33	266	397	0.347	ng	# 80
32) Bis(2-ethylhexyl)phthalate	21.62	149	5878	0.095	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041118\
Data File : BE095979.D
Acq On : 11 Apr 2018 20:09
Operator : SJ/JU
Sample : J2215-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 12 04:16:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 11 17:26:43 2018
Response via : Initial Calibration

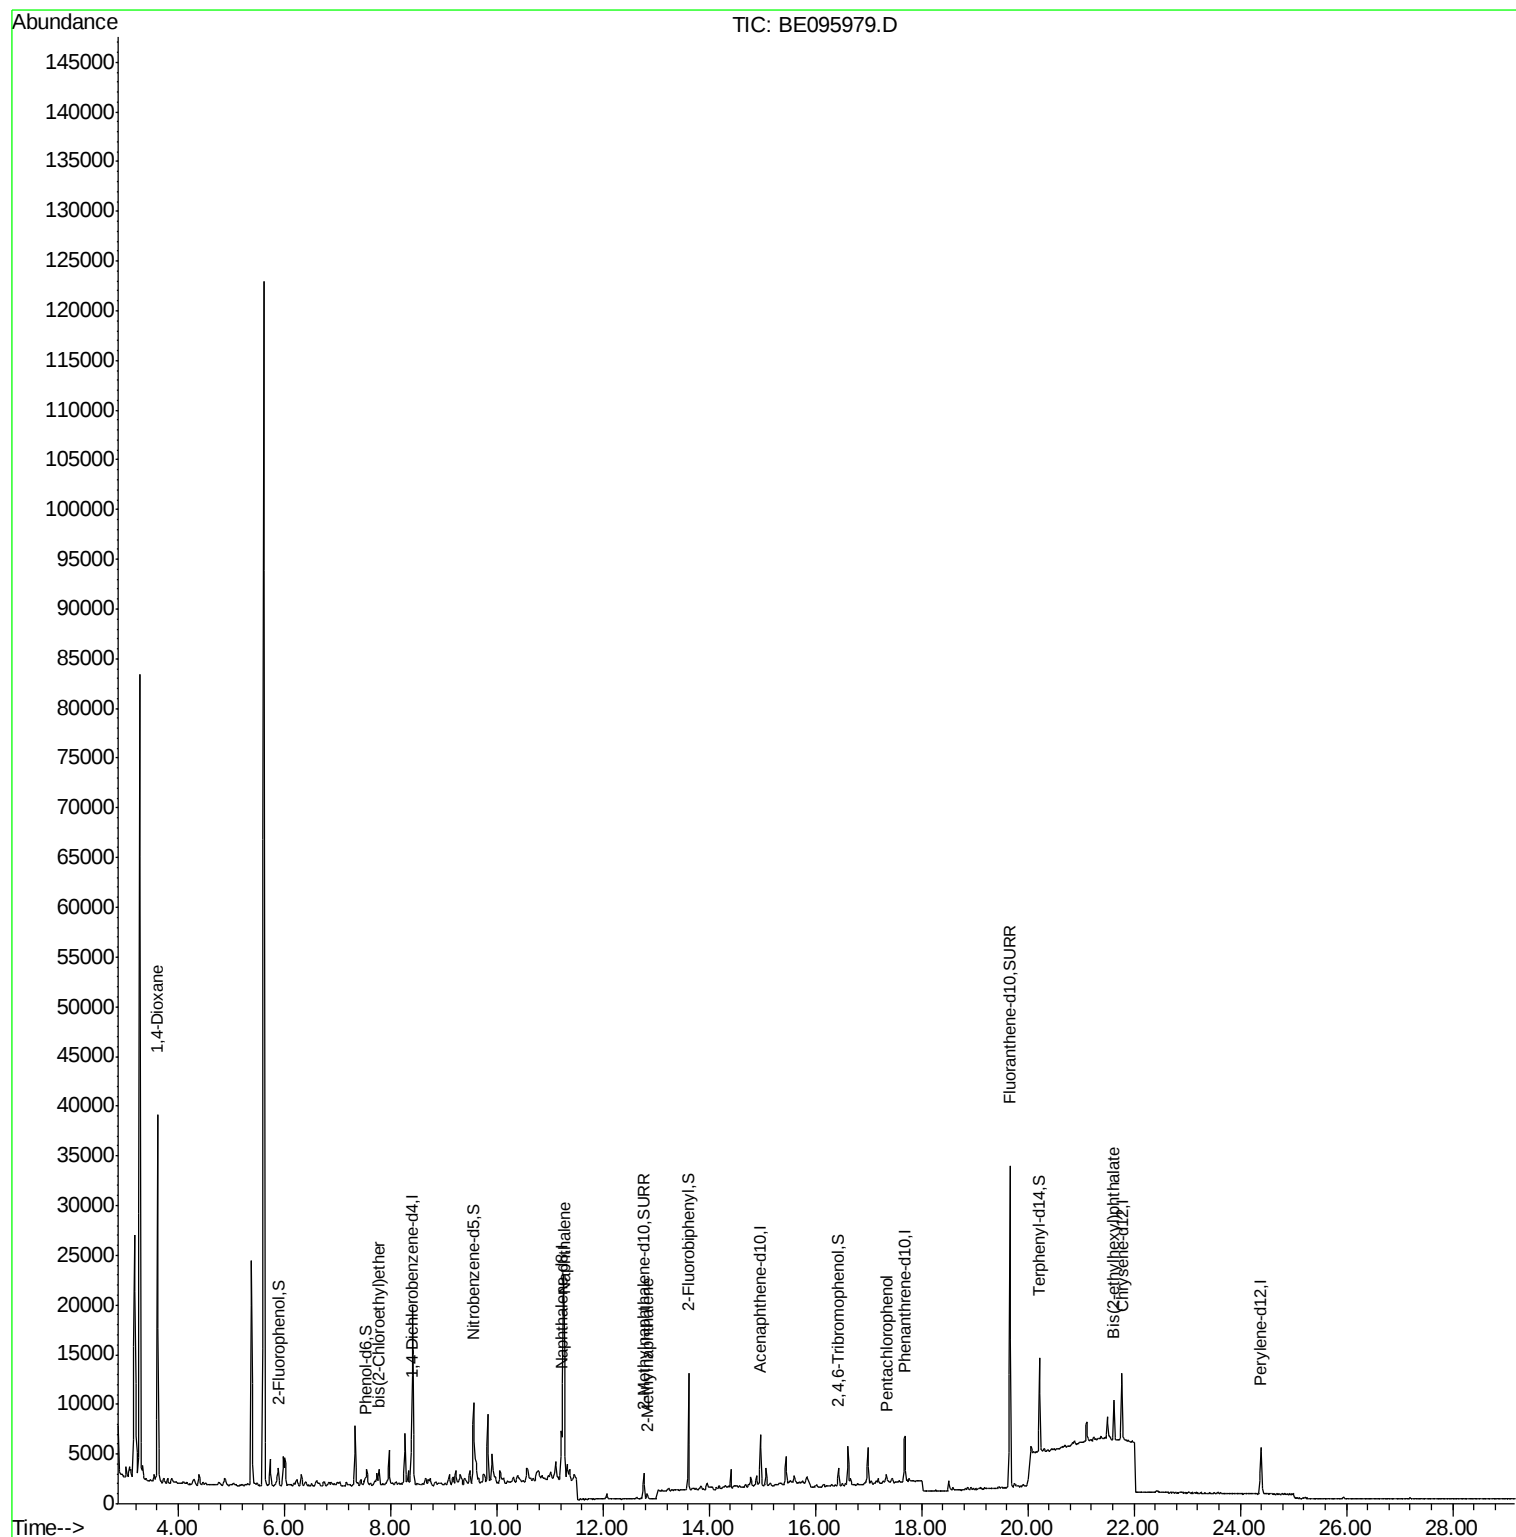




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.39 min Scan# 565
Delta R.T. 0.00 min
Lab File: BE095979.D
Acq: 11 Apr 2018 20:09

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 1364
Ion Ratio Lower Upper
152 100
150 149.5 117.2 175.8
115 71.2 57.0 85.6

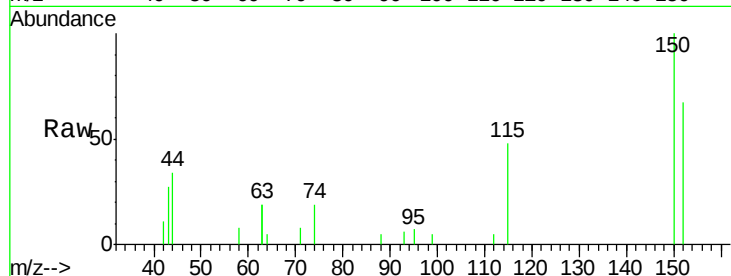


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

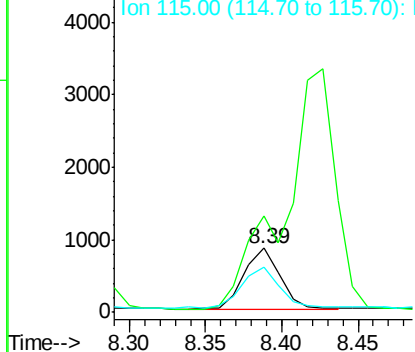



#2


1,4-Dioxane
Concen: 10.747 ng
RT: 3.61 min Scan# 77
Delta R.T. 0.00 min
Lab File: BE095979.D
Acq: 11 Apr 2018 20:09

Tgt Ion: 88 Resp: 22643
Ion Ratio Lower Upper
88 100
58 85.3 63.2 94.8
43 37.6 41.2 61.8#



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

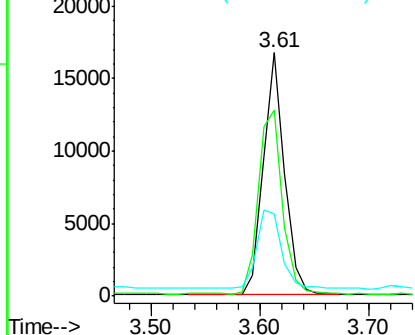

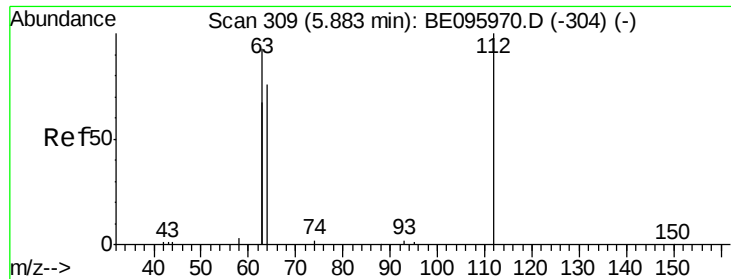

#4

2-Fluorophenol

Concen: 0.169 ng

RT: 5.88 min Scan# 309

Delta R.T. 0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 112 Resp: 711

Ion Ratio Lower Upper

112 100

64 76.9 60.1 90.1




63 167.2 116.8 175.2



Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

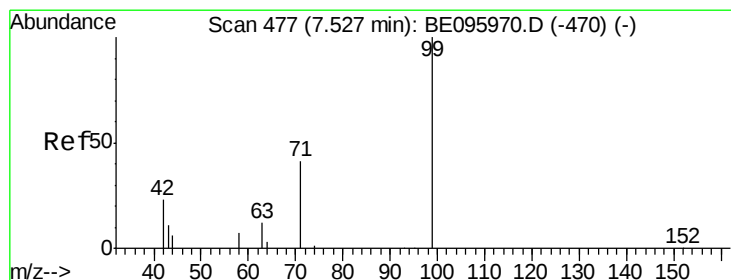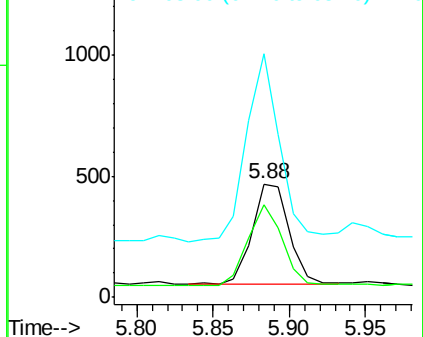

#5

Phenol-d6

Concen: 0.104 ng

RT: 7.53 min Scan# 477

Delta R.T. 0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09


Tgt Ion: 99 Resp: 608

Ion Ratio Lower Upper

99 100

42 59.2 20.2 30.2#



71 146.1 28.4 42.6#




Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

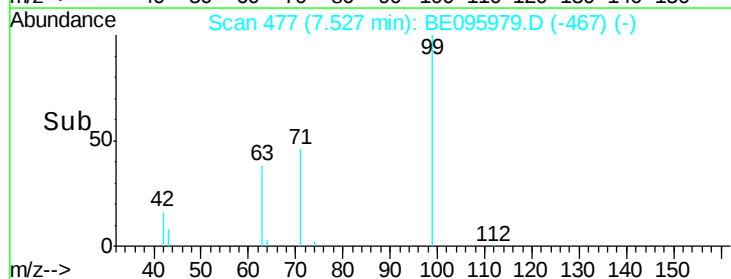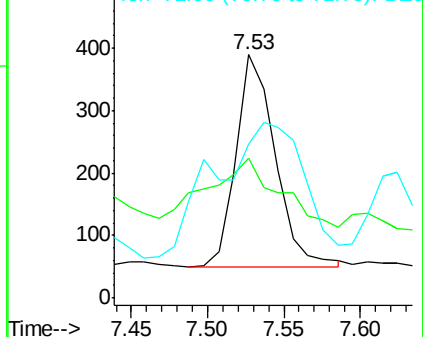

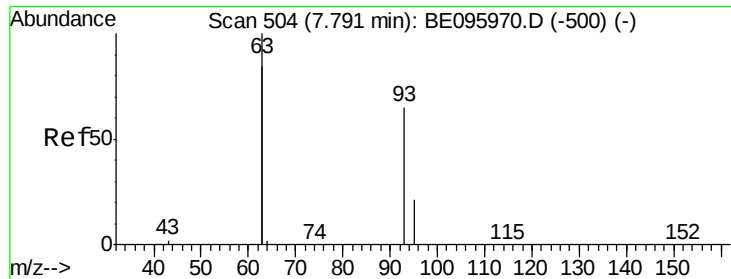

#6

bis(2-Chloroethyl)ether

Concen: 0.091 ng

RT: 7.78 min Scan# 503

Delta R.T. -0.01 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Instrument :

BNA_E

ClientSampled :





Tot Ion: 93 Resp: 464

Ion Ratio Lower Upper

93 100

63 303.9 275.3 412.9

95 41.2 25.2 37.8#

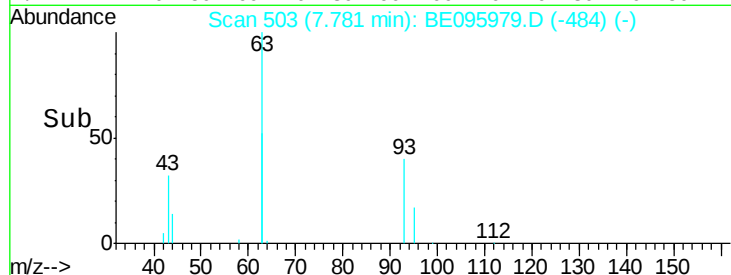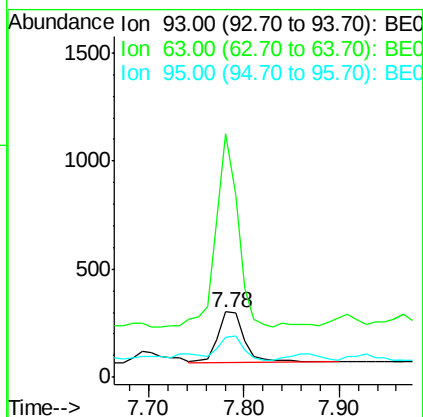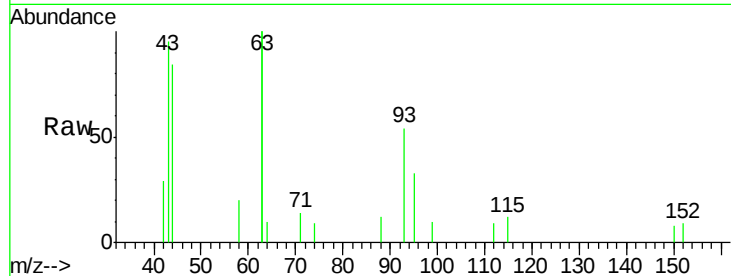

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.22 min Scan# 781

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Tgt Ion: 136 Resp: 5345




Ion Ratio Lower Upper


136 100

137 12.8 9.5 14.3

54 58.2 29.1 43.7#

68 13.6 6.2 9.2#

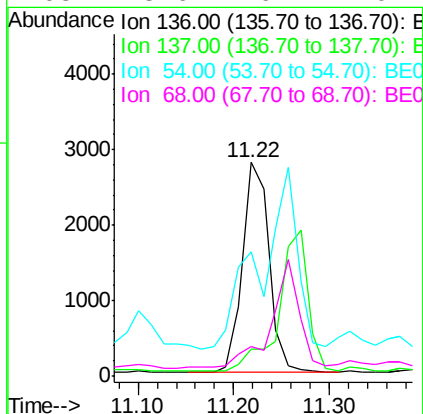

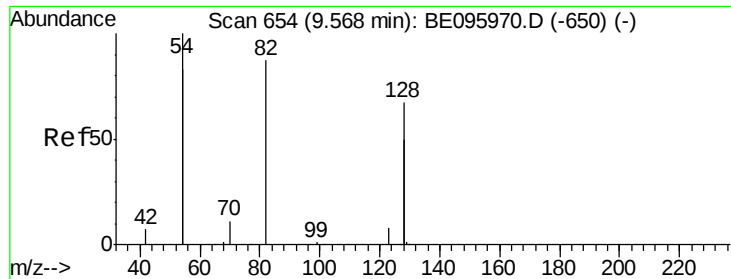

#8

Nitrobenzene-d5

Concen: 0.515 ng

RT: 9.57 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 3228

Ion Ratio Lower Upper

82 100

128 143.7 150.0 225.0#




54 213.0 154.2 231.4



Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

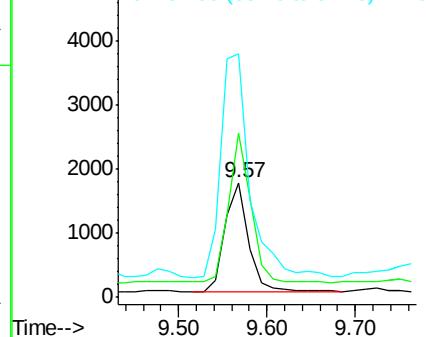

#9

Naphthalene

Concen: 0.031 ng

RT: 11.27 min Scan# 785

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09


Tgt Ion: 128 Resp: 1771

Ion Ratio Lower Upper

128 100

129 7.4 2.6 3.8#



127 7.2 2.8 4.2#




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E




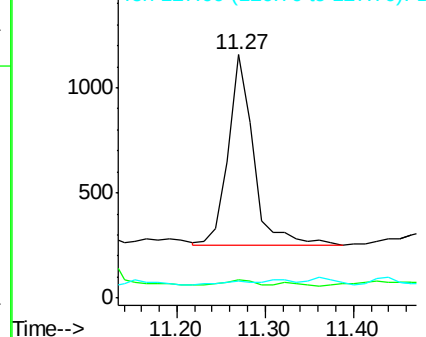


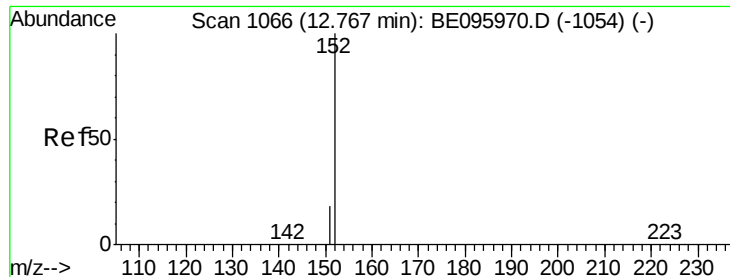

#11
 2-Methylnaphthalene-d10
 Concen: 0.432 ng
 RT: 12.76 min Scan# 1065
 Delta R.T. -0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:152 Resp: 3658
 Ion Ratio Lower Upper
 152 100
 151 19.2 15.4 23.0

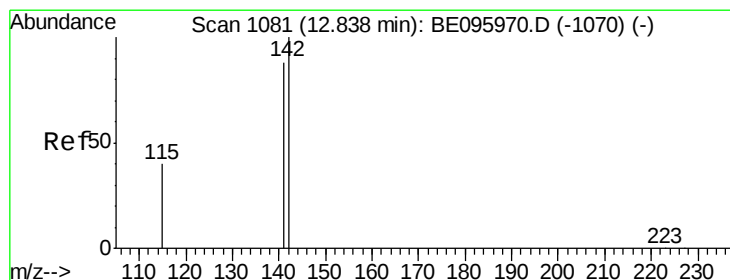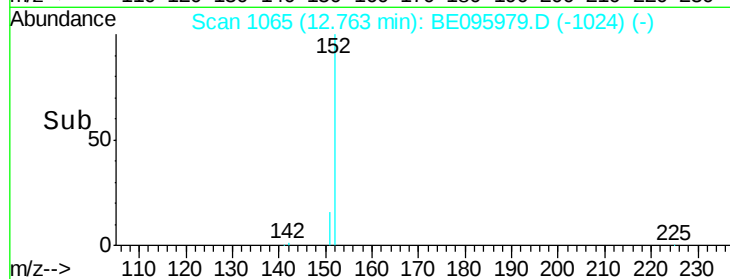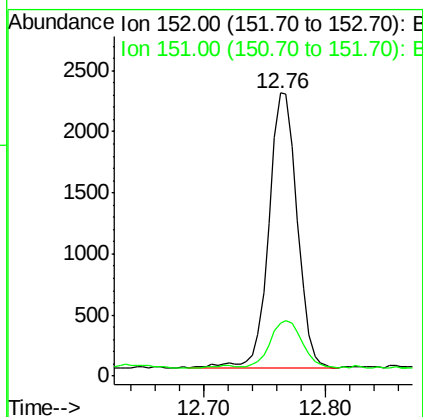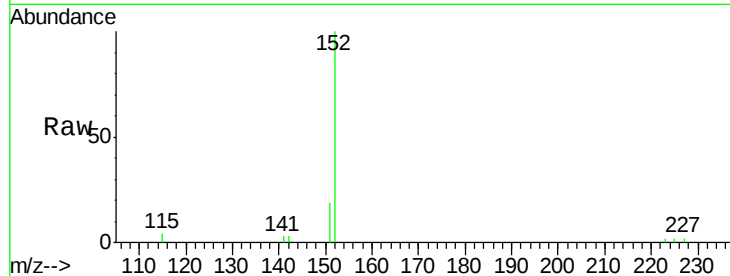

#12
 2-Methylnaphthalene
 Concen: 0.037 ng
 RT: 12.84 min Scan# 1081
 Delta R.T. 0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09

Tgt Ion:142 Resp: 345
 Ion Ratio Lower Upper
 142 100
 141 92.7 70.4 105.6
 115 65.0 31.7 47.5#


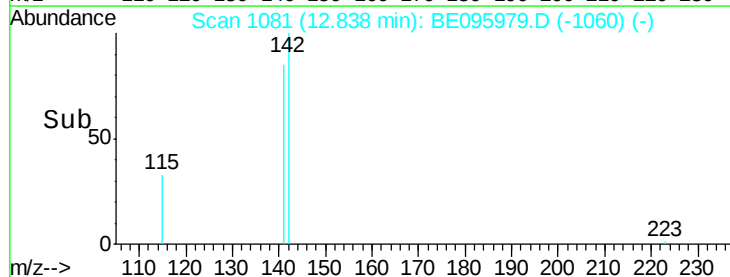
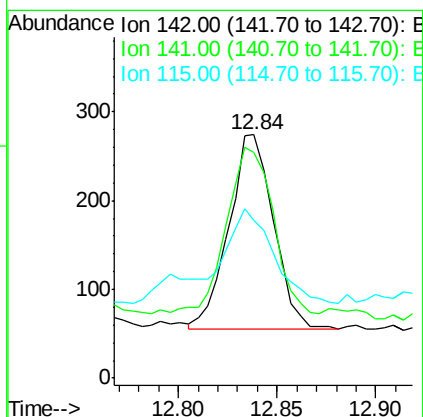
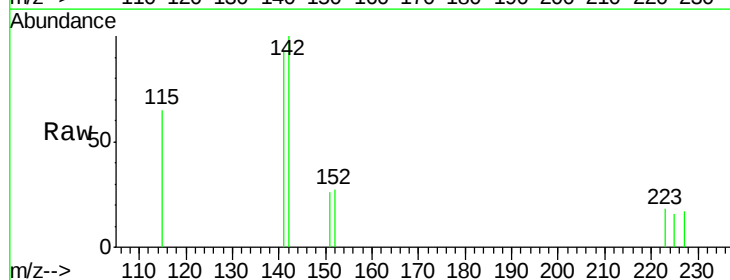


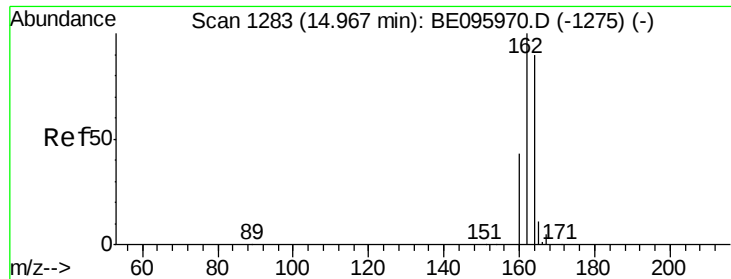

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.97 min Scan# 1283
 Delta R.T. -0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:164 Resp: 3002
 Ion Ratio Lower Upper
 164 100
 162 105.3 83.1 124.7
 160 47.4 37.1 55.7

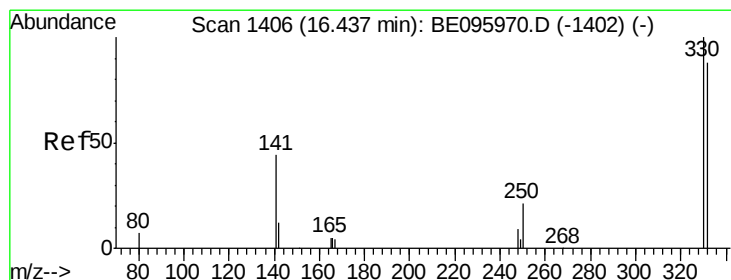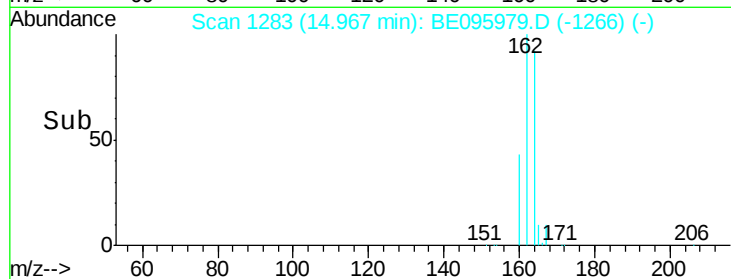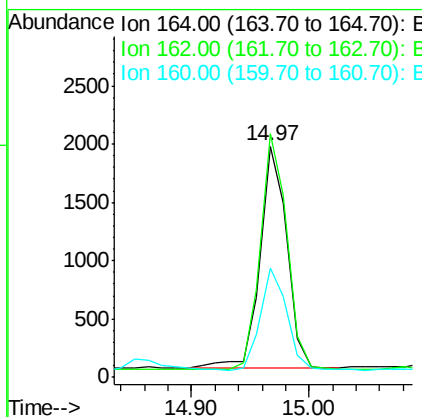

#14
 2,4,6-Tribromophenol
 Concen: 0.561 ng
 RT: 16.44 min Scan# 1406
 Delta R.T. -0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09

Tgt Ion:330 Resp: 813
 Ion Ratio Lower Upper
 330 100
 332 95.6 152.7 229.1#
 141 58.1 33.7 50.5#


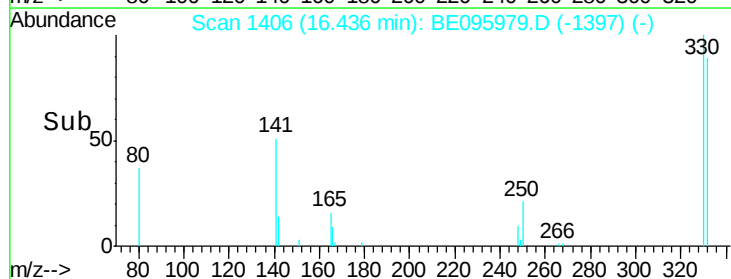
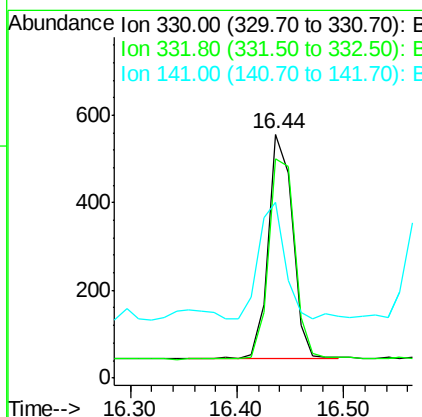
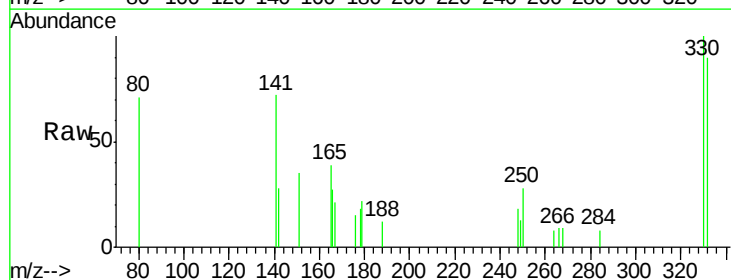


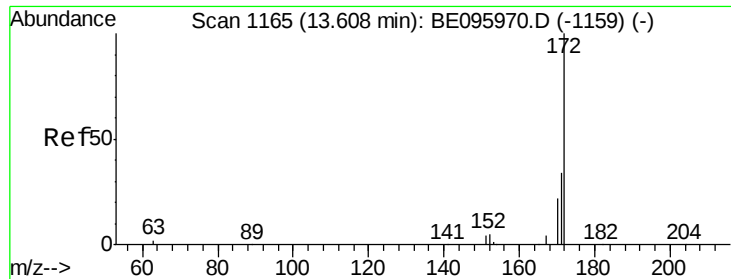

#15
2-Fluorobiphenyl
Concen: 0.772 ng
RT: 13.61 min Scan# 1165
Delta R.T. -0.00 min
Lab File: BE095979.D
Acq: 11 Apr 2018 20:09




Instrument :
BNA_E
ClientSampleId :


Tot Ion:172 Resp: 9912
Ion Ratio Lower Upper
172 100
171 35.5 29.9 44.9
170 22.5 21.8 32.8

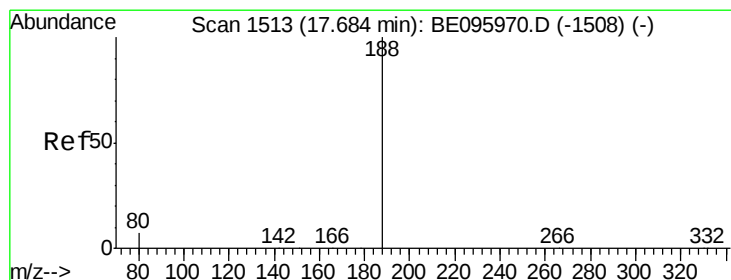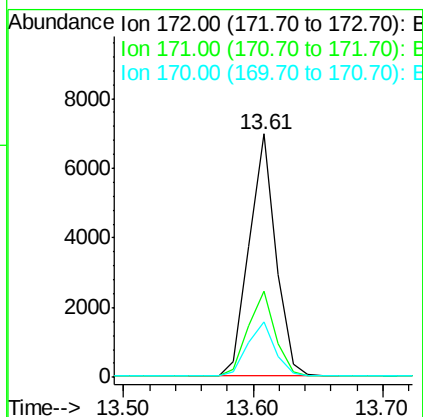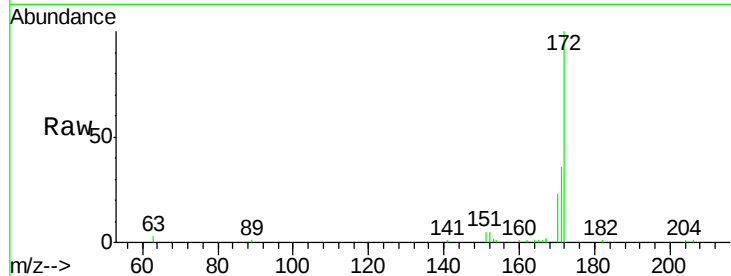

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.68 min Scan# 1513
Delta R.T. -0.00 min
Lab File: BE095979.D
Acq: 11 Apr 2018 20:09

Tgt Ion:188 Resp: 6871
Ion Ratio Lower Upper
188 100
94 0.0 3.9 5.9#
80 12.3 3.6 5.4#

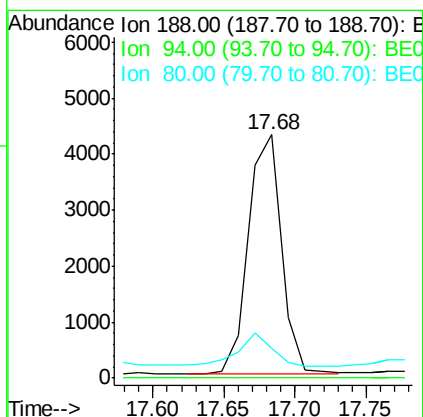







#22
 Pentachlorophenol
 Concen: 0.347 ng
 RT: 17.33 min Scan# 1483
 Delta R.T. -0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 397
 Ion Ratio Lower Upper
 266 100
 264 74.1 72.5 108.7
 268 71.3 73.8 110.6#

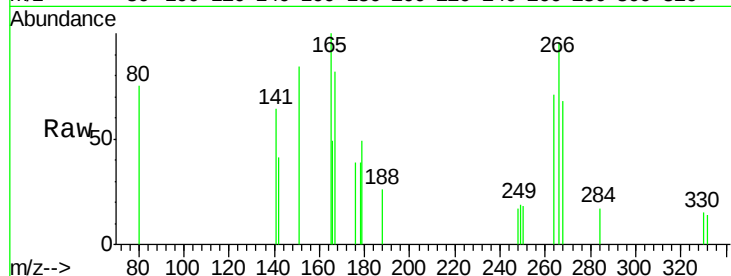


Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E


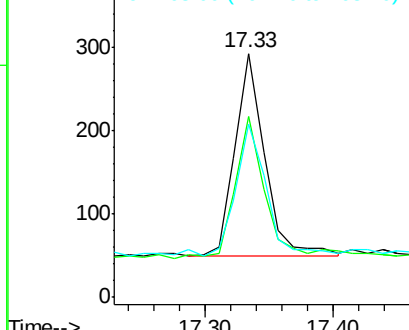



#25
 Fluoranthene-d10
 Concen: 0.430 ng
 RT: 19.66 min Scan# 1824
 Delta R.T. 0.00 min
 Lab File: BE095979.D
 Acq: 11 Apr 2018 20:09

Tgt Ion:212 Resp: 40106
 Ion Ratio Lower Upper
 212 100
 106 3.2 2.8 4.2
 104 1.8 1.6 2.4



Abundance Ion 212.00 (211.70 to 212.70): E
 Ion 106.00 (105.70 to 106.70): E
 Ion 104.00 (103.70 to 104.70): E

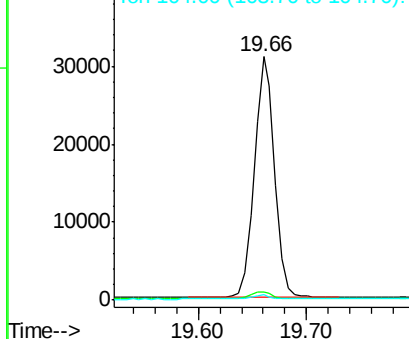



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.78 min Scan# 2027

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 7453

Ion Ratio Lower Upper

240 100

120 8.6 5.5 8.3#




236 27.5 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

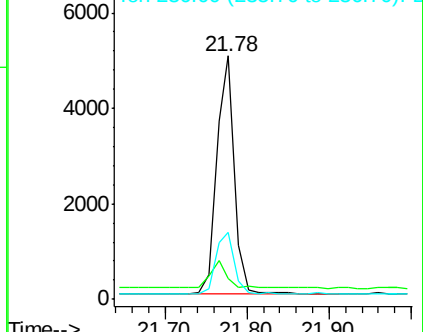

#29

Terphenyl-d14

Concen: 0.540 ng

RT: 20.22 min Scan# 1898

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09


Tgt Ion:244 Resp: 8898

Ion Ratio Lower Upper

244 100

212 11.8 25.4 38.0#



122 15.4 8.1 12.1#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

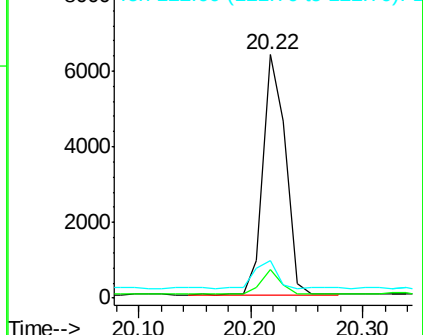



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.095 ng

RT: 21.62 min Scan# 2014

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09

Instrument :

BNA_E

ClientSampleId :


Tot Ion:149 Resp: 5878

Ion Ratio Lower Upper

149 100

167 7.0 5.4 8.0




279 1.7 0.7 1.1#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

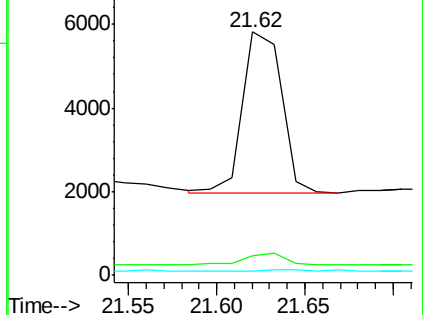

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.39 min Scan# 2709

Delta R.T. -0.00 min

Lab File: BE095979.D

Acq: 11 Apr 2018 20:09


Tgt Ion:264 Resp: 7125

Ion Ratio Lower Upper

264 100

260 26.9 20.5 30.7

265 30.0 22.8 34.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

