
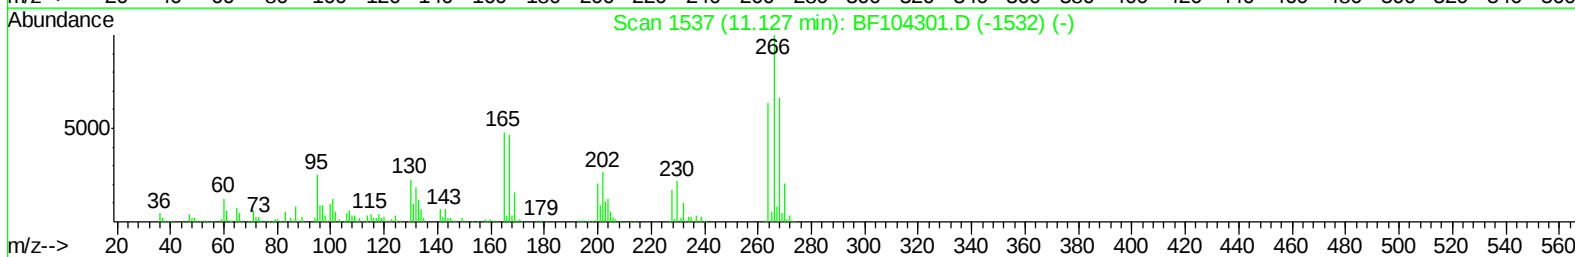
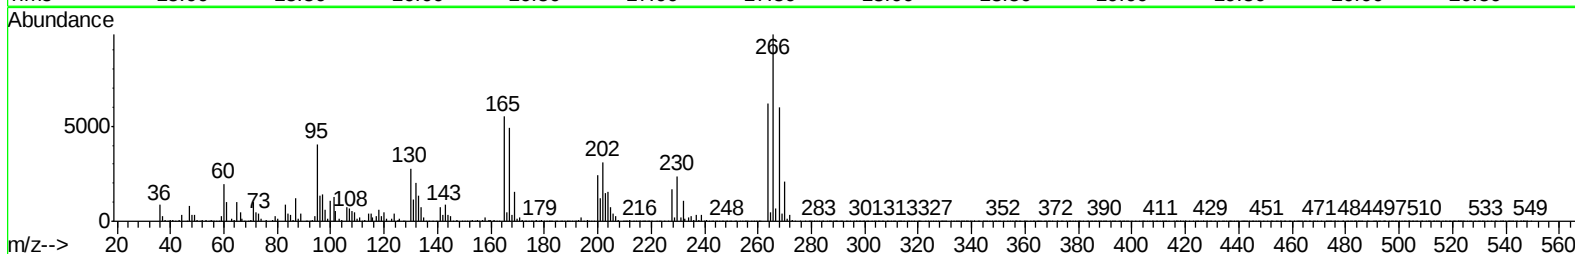


Data Path : Z:\HPCHEM1\BNA E\DATA\BE041118\
Data File : BE095967.D
Acq On : 11 Apr 2018 12:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 04:50:25 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 11 13:19:22 2018
Response via : Initial Calibration

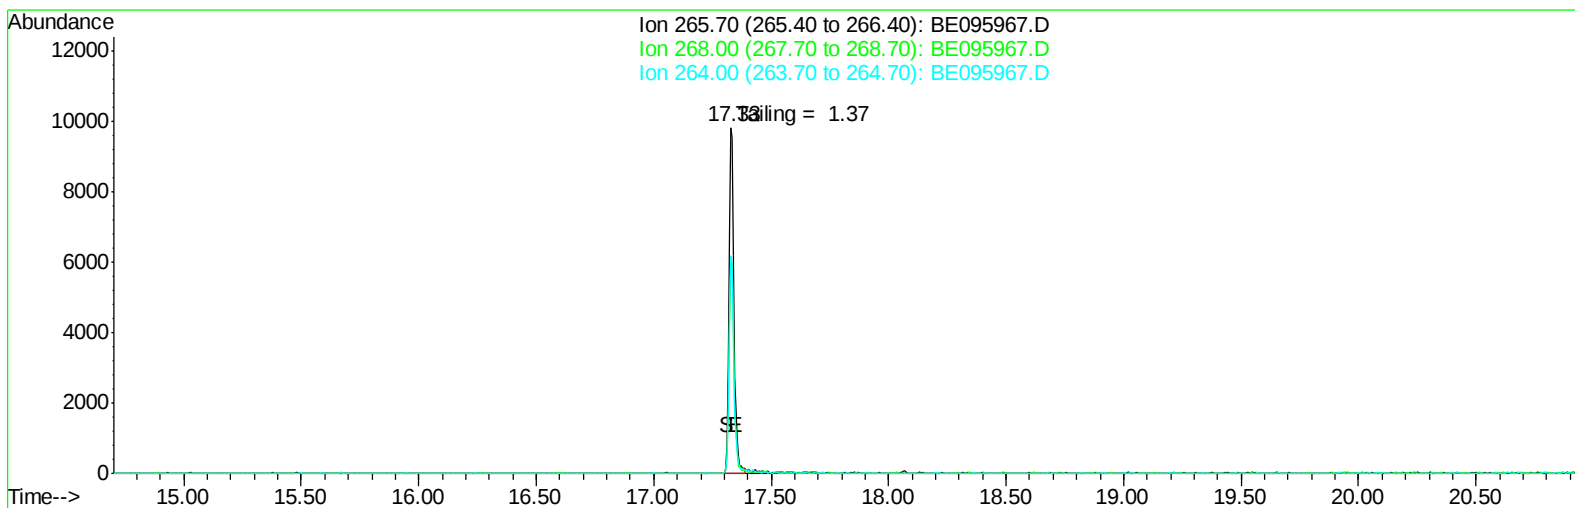

TIC: BE095967.D

(69) Pentachlorophenol (C)




17.329min (+6.190) 81679.94ng m

response 14515

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.06
264.00	61.90	63.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041118\
Data File : BE095967.D
Acq On : 11 Apr 2018 12:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 04:50:25 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 11 13:19:22 2018
Response via : Initial Calibration

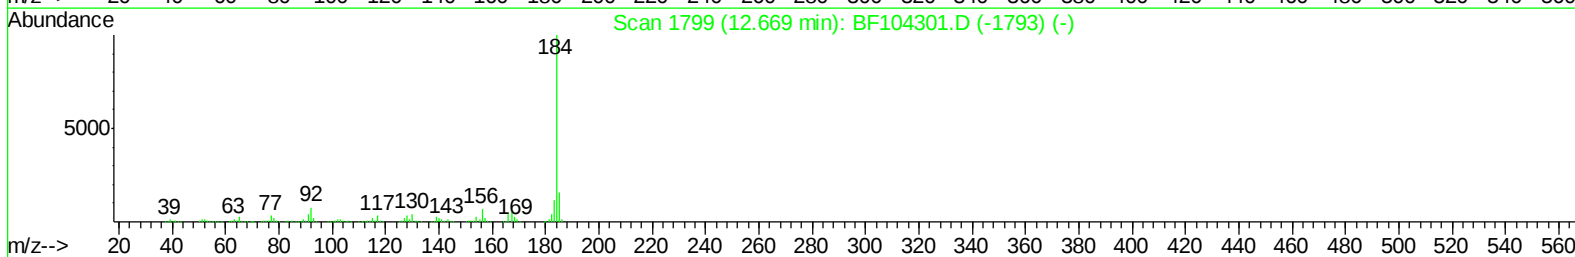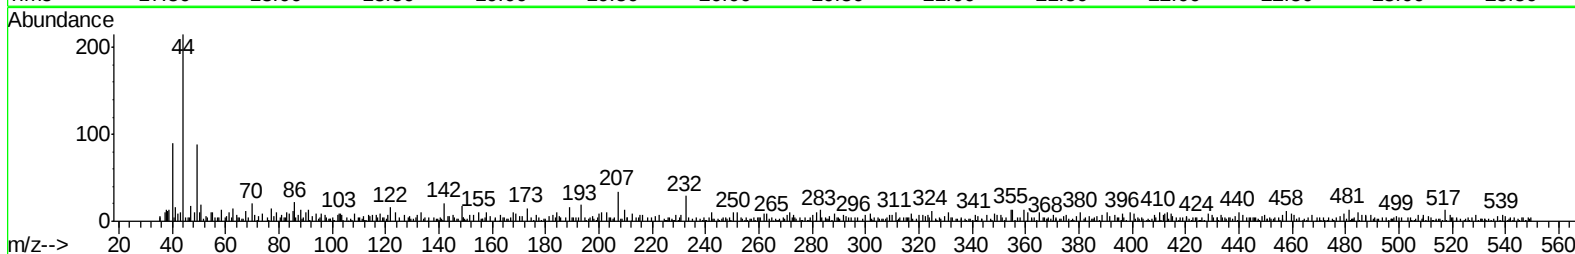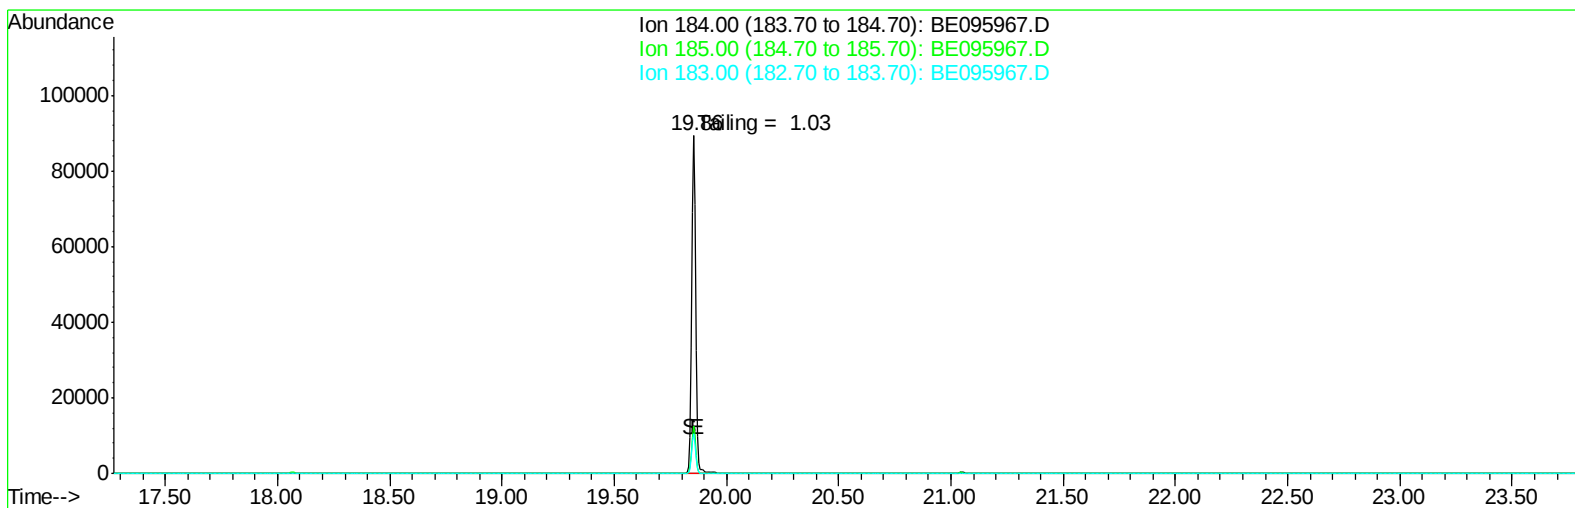

TIC: BE095967.D

(76) Benzidine

12.441min (-0.233) 8.42ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	66.67#
183.00	11.60	53.33#
0.00	0.00	0.00