


Data Path : Z:\HPCHEM1\BNA E\Data\BE041118\
 Data File : BE095967.D
 Acq On : 11 Apr 2018 12:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 12 13:55:20 2018

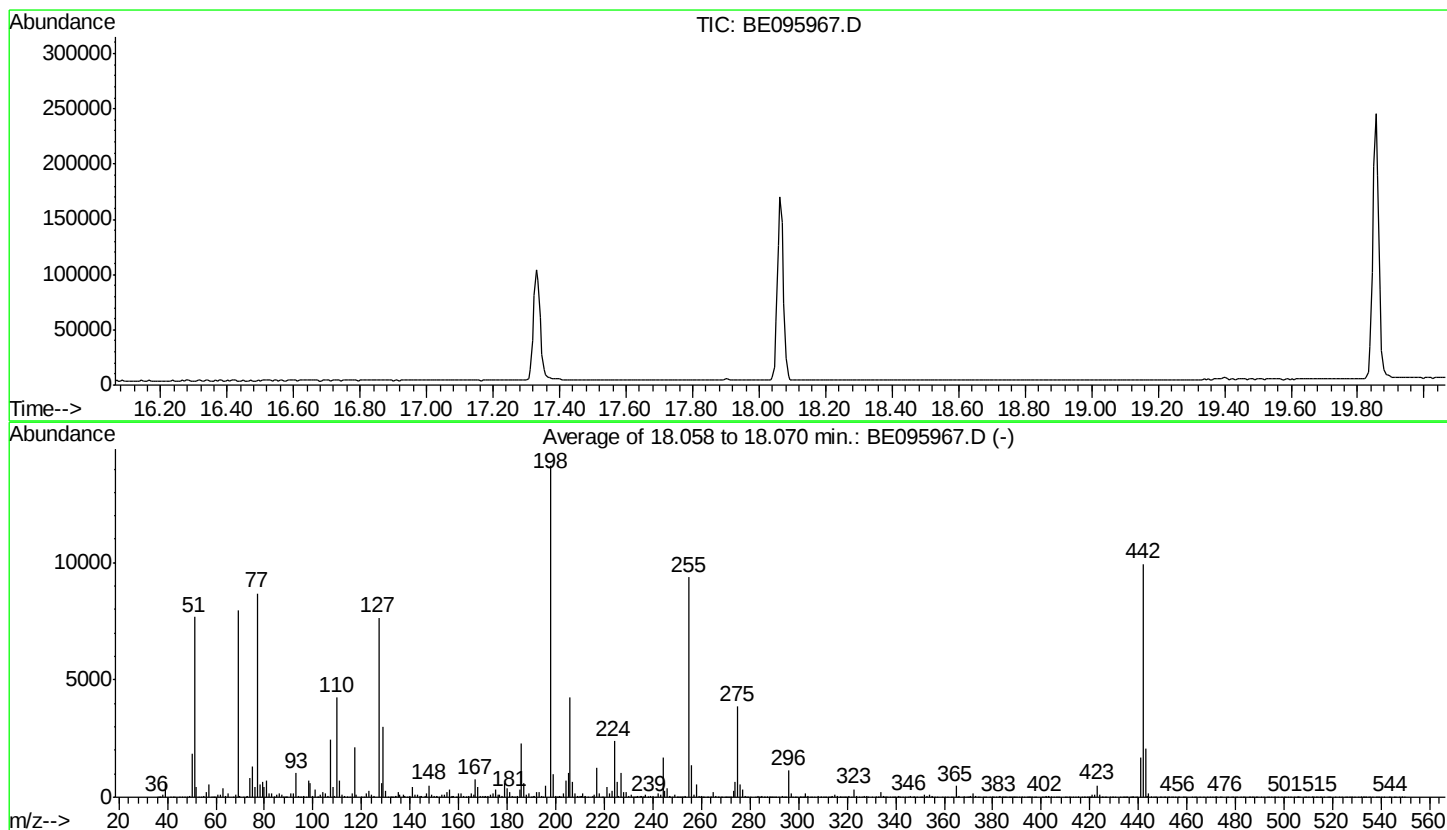

AutoFind: Scans 2633, 2634, 2635; Background Corrected with Scan 2626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	7682	PASS
68	69	0.00	2	1.7	132	PASS
69	198	0.00	100	56.3	7962	PASS
70	69	0.00	2	0.5	40	PASS
127	198	10	80	54.2	7657	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14139	PASS
199	198	5	9	6.8	966	PASS
275	198	10	60	27.3	3865	PASS
365	198	1	100	3.3	470	PASS
441	443	0.01	100	80.9	1674	PASS
442	198	50	100	70.4	9957	PASS
443	442	15	24	20.8	2068	PASS