


Data Path : Z:\HPCHEM1\BNA E\Data\BE041216\
Data File : BE091644.D
Acq On : 12 Apr 2016 9:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 08 16:48:14 2016

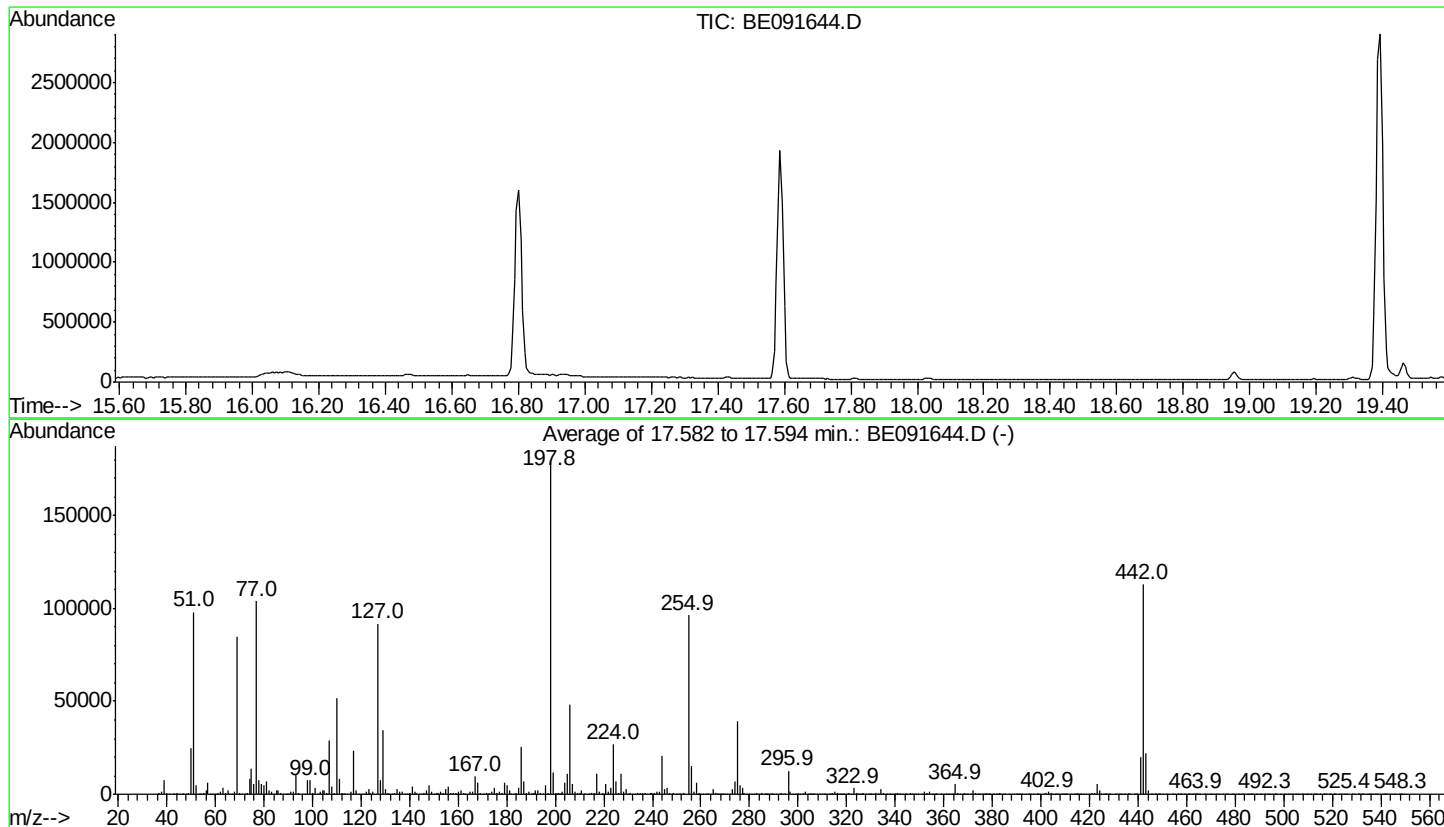

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	98208	PASS
68	69	0.00	2	1.9	1578	PASS
69	198	0.00	100	47.6	85006	PASS
70	69	0.00	2	0.5	459	PASS
127	198	10	80	51.4	91862	PASS
197	198	0.00	2	0.3	535	PASS
198	198	100	100	100.0	178568	PASS
199	198	5	9	6.7	11961	PASS
275	198	10	60	21.9	39040	PASS
365	198	1	100	2.9	5210	PASS
441	442	0.01	24	17.9	20163	PASS
442	198	50	100	63.2	112808	PASS
443	442	15	24	19.7	22205	PASS