
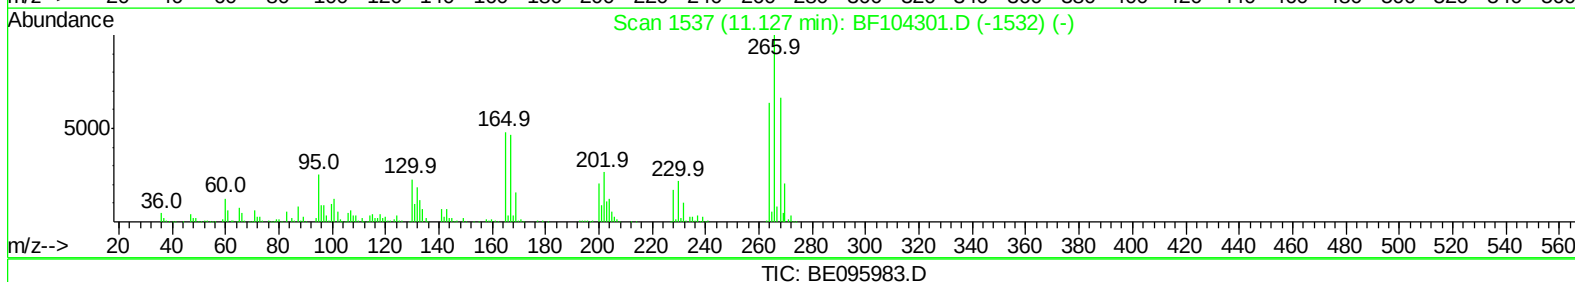
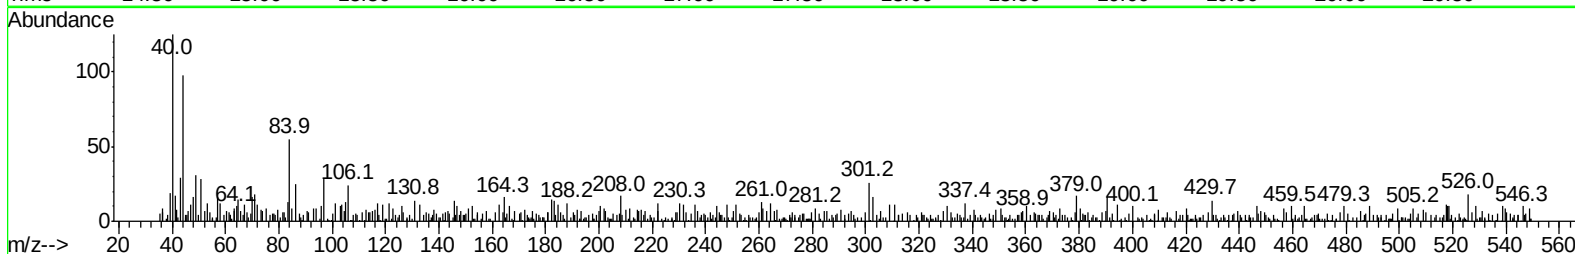


Data Path : Z:\HPCHEM1\BNA E\Data\BE041218\
Data File : BE095983.D
Acq On : 12 Apr 2018 8:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:04:37 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 12 17:07:03 2018
Response via : Initial Calibration

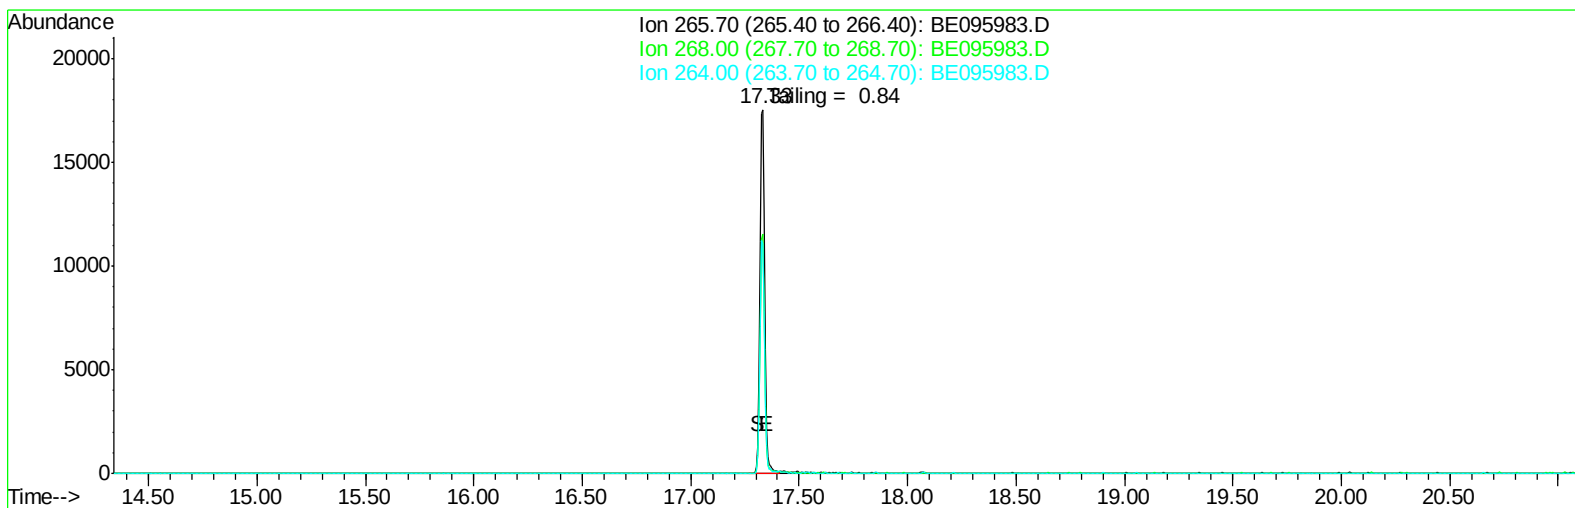

TIC: BE095983.D

(69) Pentachlorophenol (C)




11.130min (-0.015) 50.65ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	25.00#
264.00	61.90	150.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE041218\
Data File : BE095983.D
Acq On : 12 Apr 2018 8:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 05:04:37 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 12 17:07:03 2018
Response via : Initial Calibration

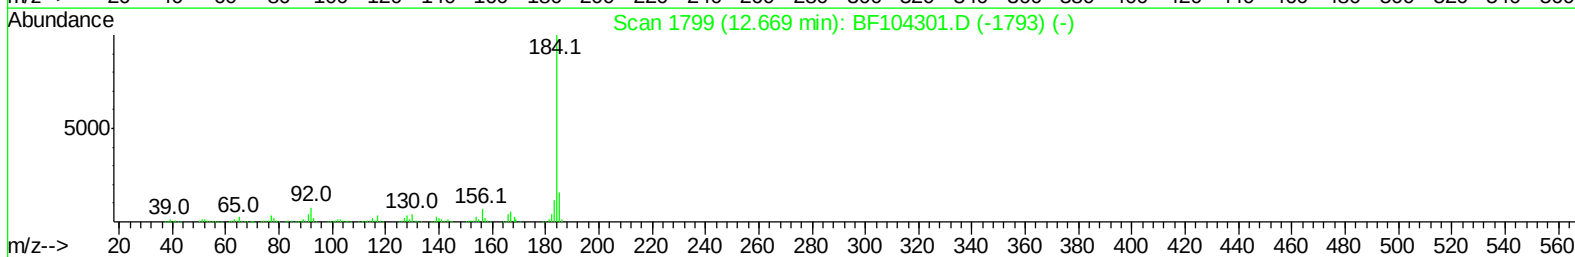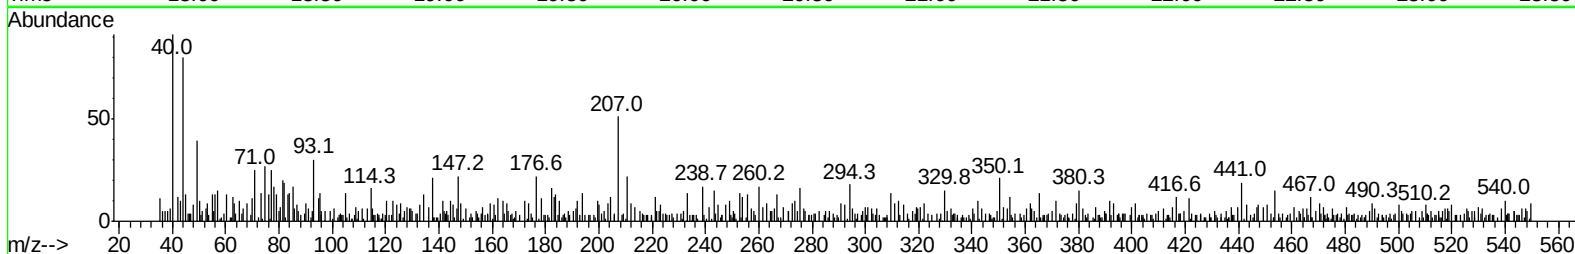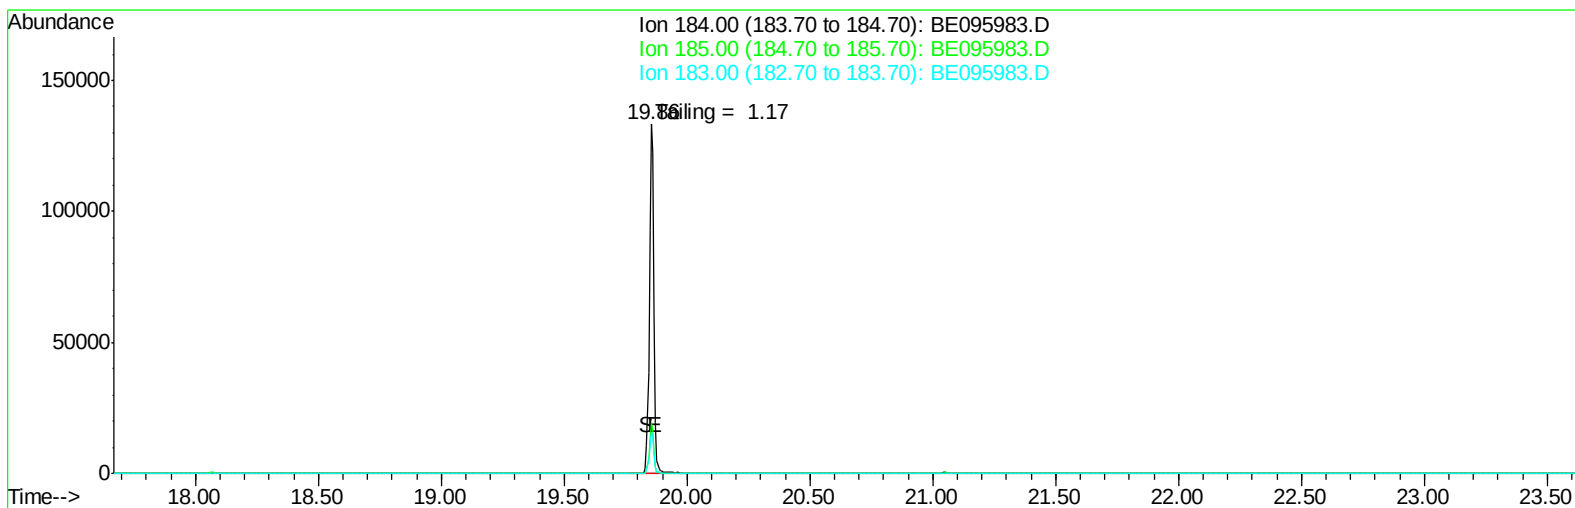

TIC: BE095983.D

(76) Benzidine

12.628min (-0.052) 48.69ng

response 14

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	62.50#
183.00	11.60	75.00#
0.00	0.00	0.00