


Data Path : Z:\HPCHEM1\BNA_E\Data\BE041218\
Data File : BE095983.D
Acq On : 12 Apr 2018 8:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 12 14:20:38 2018

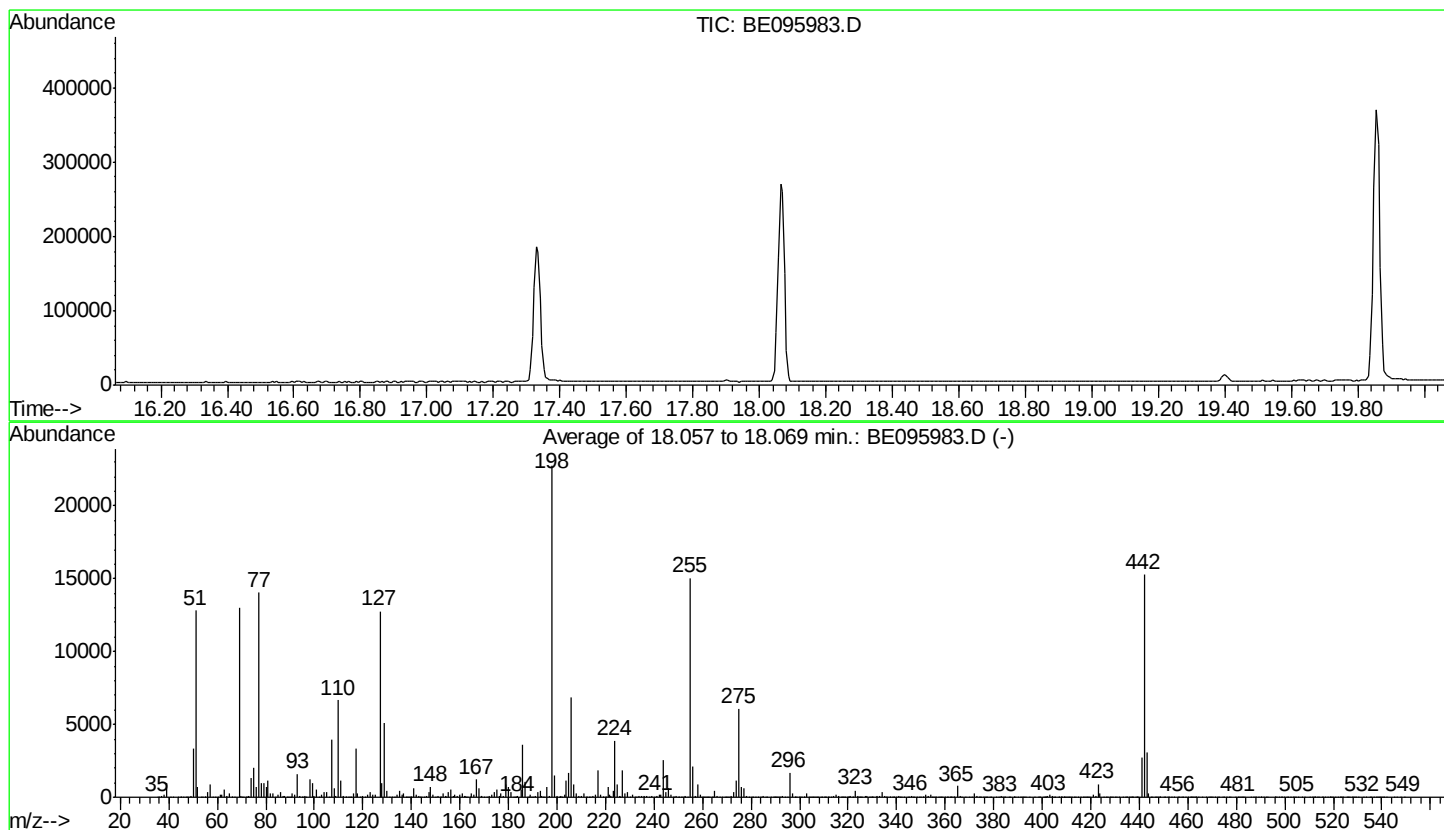

AutoFind: Scans 2633, 2634, 2635; Background Corrected with Scan 2627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.2	12794	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.0	12967	PASS
70	69	0.00	2	0.4	52	PASS
127	198	10	80	56.1	12780	PASS
197	198	0.00	2	0.3	61	PASS
198	198	100	100	100.0	22764	PASS
199	198	5	9	6.7	1530	PASS
275	198	10	60	26.8	6091	PASS
365	198	1	100	3.3	750	PASS
441	443	0.01	100	88.5	2752	PASS
442	198	50	100	67.1	15270	PASS
443	442	15	24	20.4	3108	PASS