
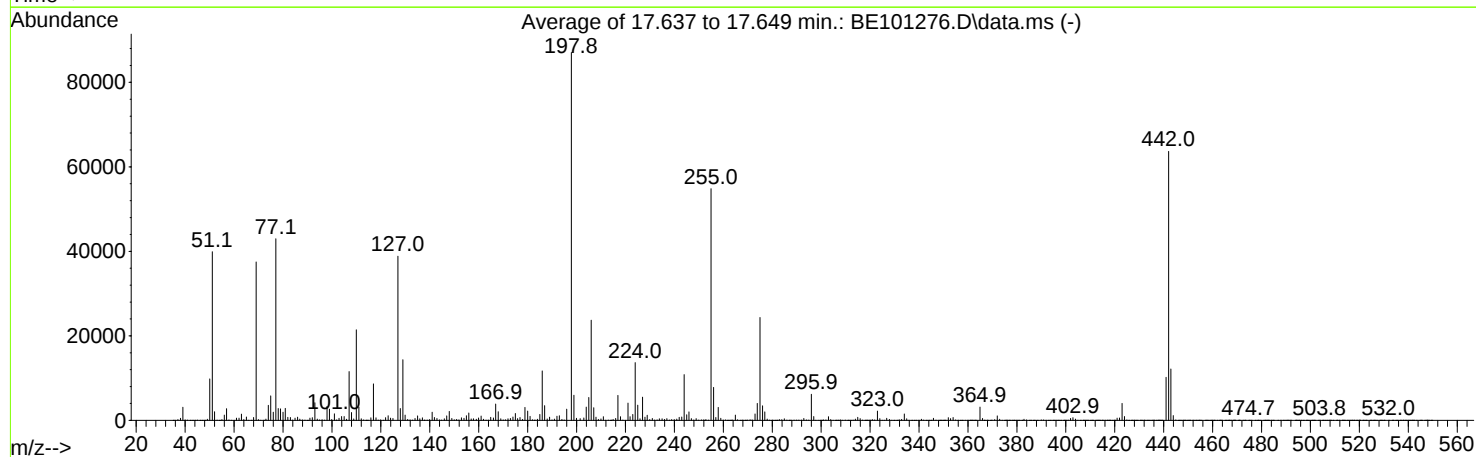


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041221\
 Data File : BE101276.D
 Acq On : 12 Apr 2021 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE041221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 12 18:02:55 2021

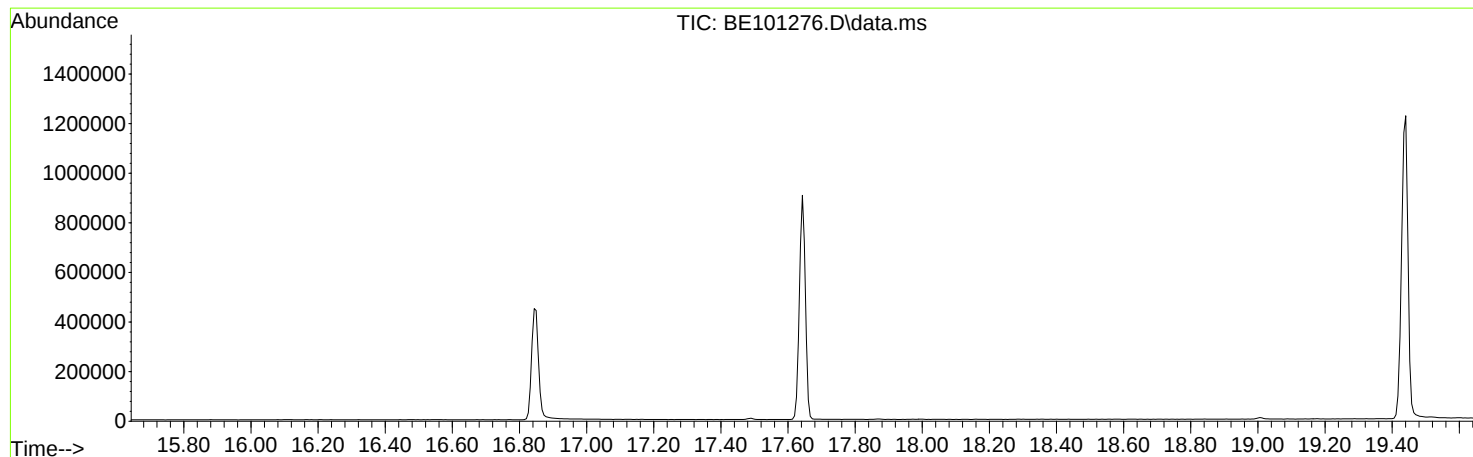

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	39923	PASS
68	69	0.00	2	1.9	702	PASS
69	198	0.00	100	43.1	37483	PASS
70	69	0.00	2	0.5	179	PASS
127	198	10	80	44.6	38841	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87066	PASS
199	198	5	9	6.8	5931	PASS
275	198	10	60	28.0	24357	PASS
365	198	1	100	3.6	3147	PASS
441	198	0.01	100	11.7	10180	PASS
442	442	50	100	100.0	63678	PASS
443	442	15	24	19.1	12175	PASS

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2021	BNA_E	<u>BE101276.D</u>
Compound Name	Response	Retention Time
DDT	374302	20.66
DDD	6326	20.22
DDE	1072	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7398	381700	1.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041221\
 Data File : BE101276.D
 Acq On : 12 Apr 2021 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 12 12:14:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

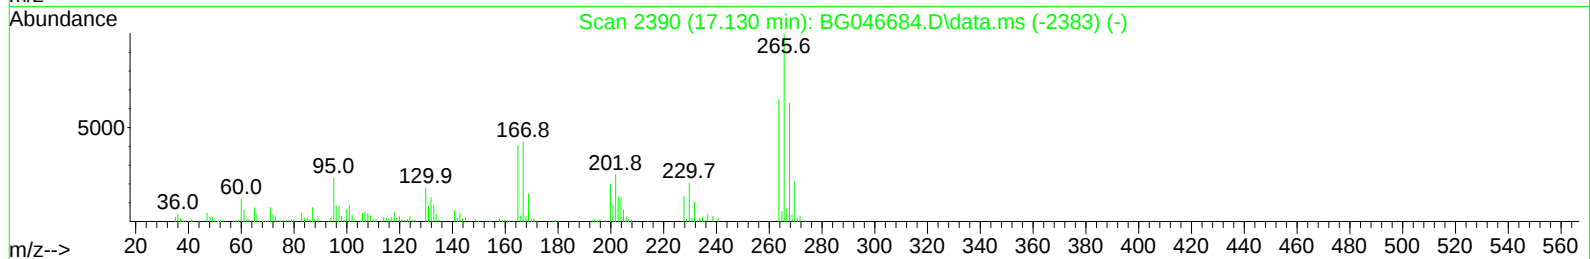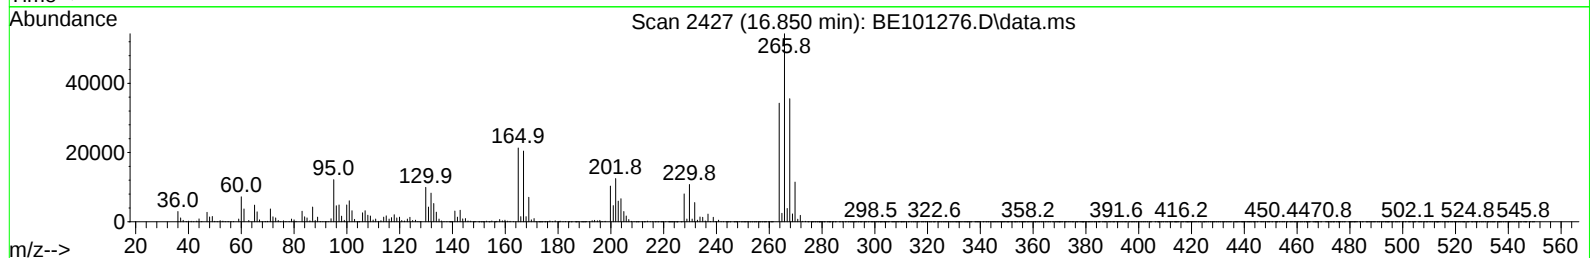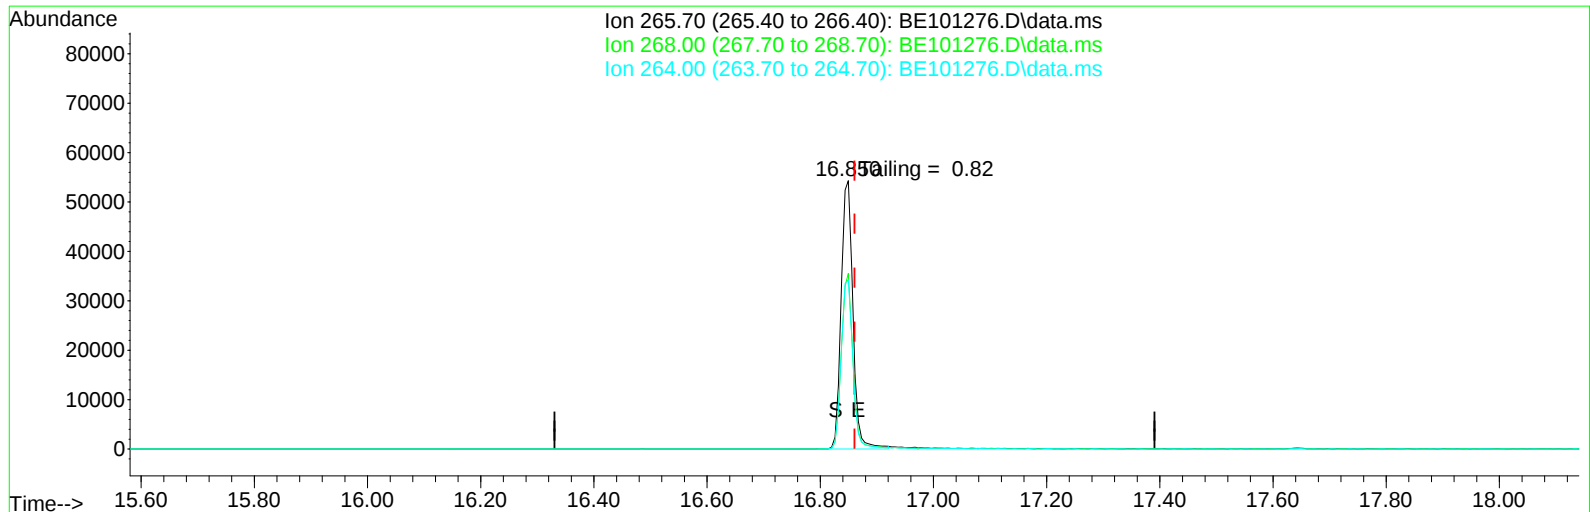

TIC: BE101276.D\data.ms

(70) Pentachlorophenol (C)

16.850min (-0.011) 777391.05 ng




response 79310

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.41
264.00	61.60	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041221\
 Data File : BE101276.D
 Acq On : 12 Apr 2021 11:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 12 12:14:05 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

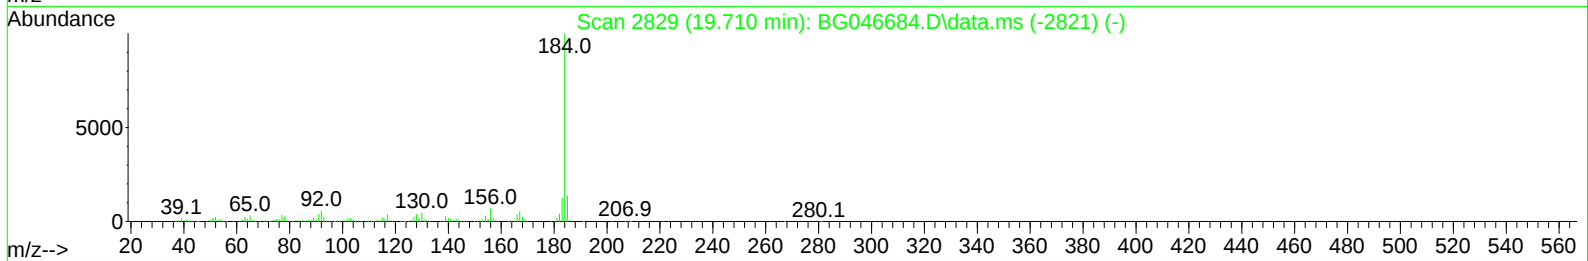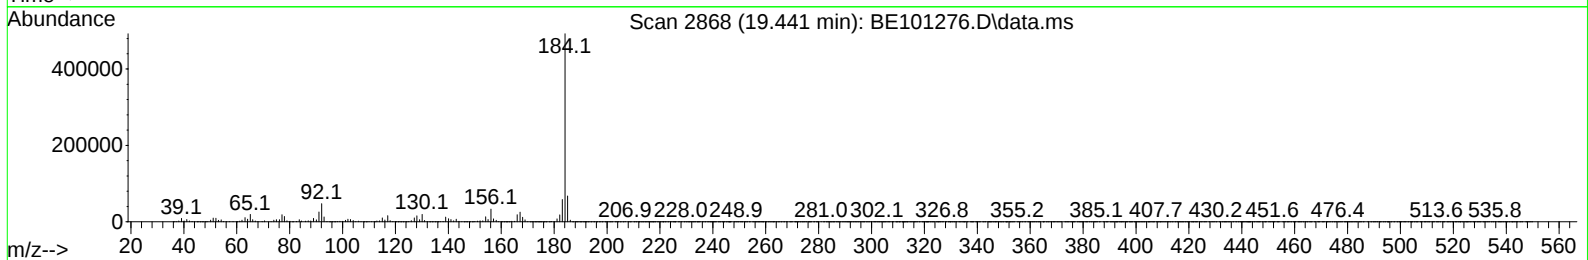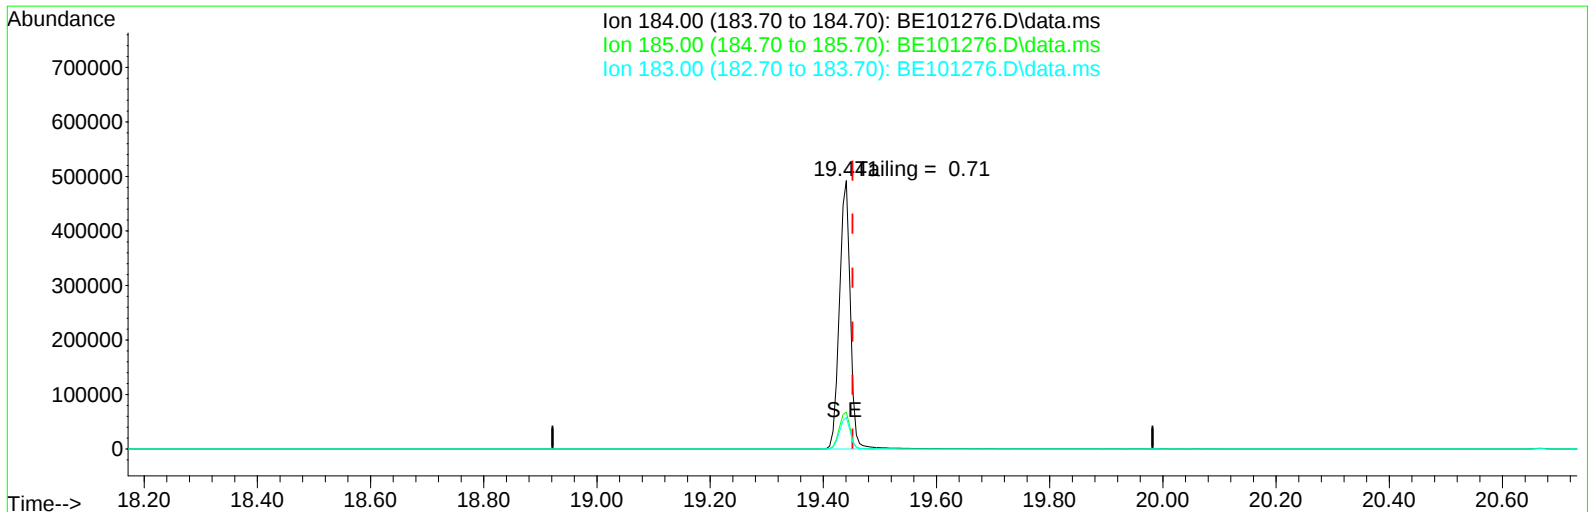

TIC: BE101276.D\data.ms

(77) Benzidine

19.441min (-0.011) 3924.54 ng

response 660284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.84
0.00	0.00	0.00