
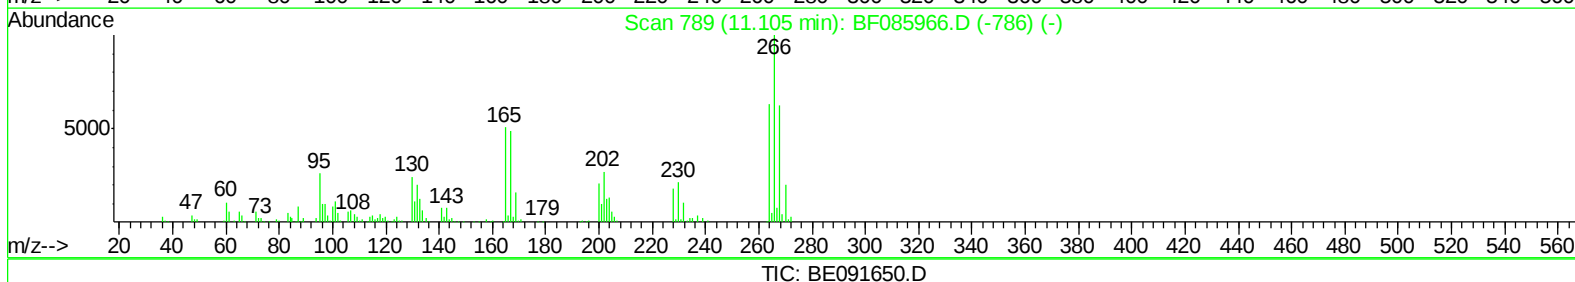
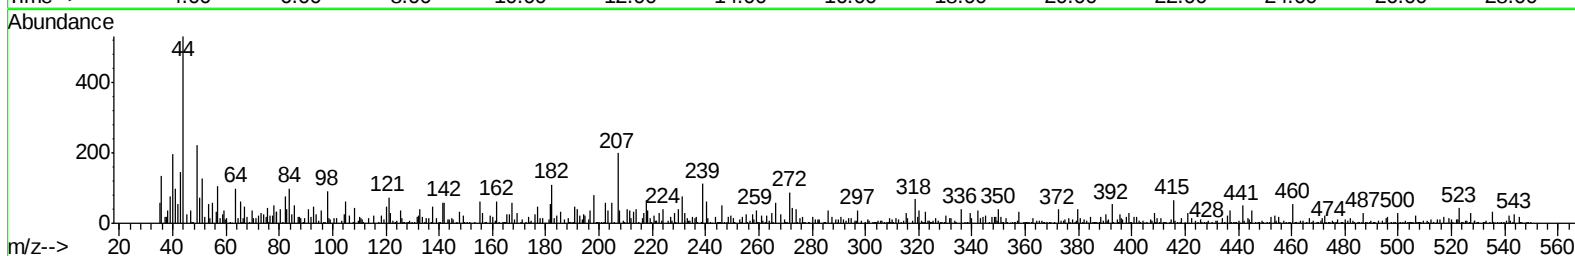


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE041316\  
Data File : BE091650.D  
Acq On : 13 Apr 2016 9:07  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 03:44:35 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040216.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 01 23:17:06 2016  
Response via : Initial Calibration



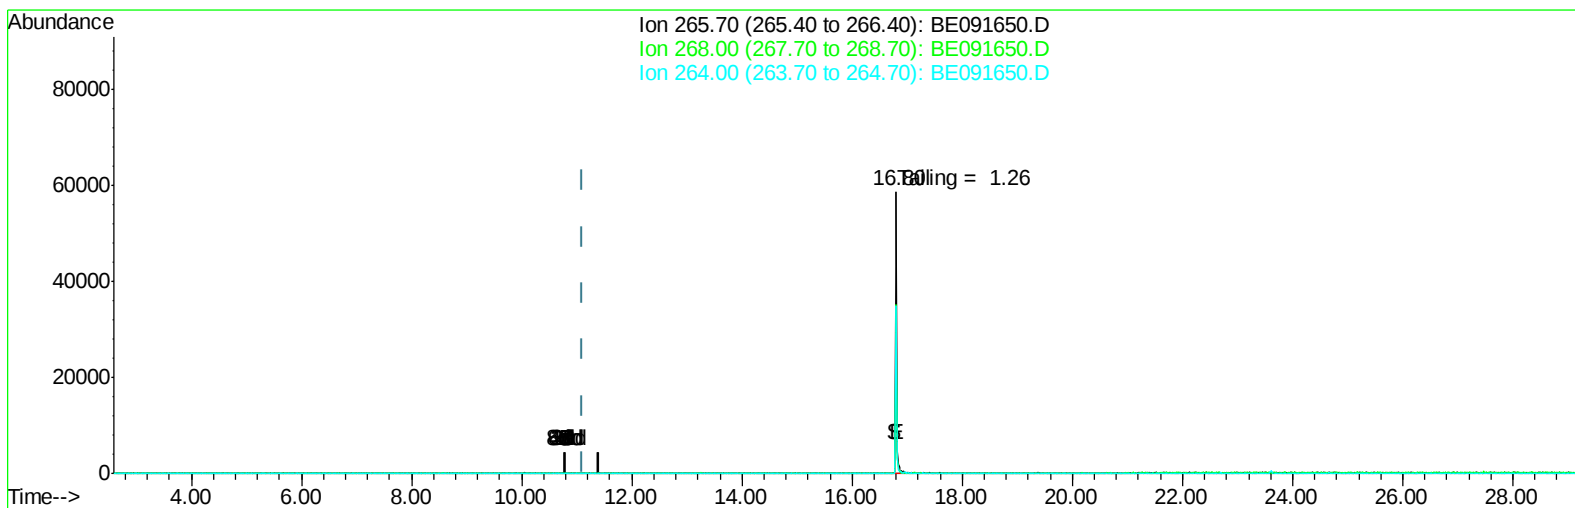


(69) Pentachlorophenol (C)  
10.814min (-0.291) 241.40ng  
response 43

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 265.70 | 100   | 100    |
| 268.00 | 64.40 | 39.34# |
| 264.00 | 63.30 | 57.38  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA\_E\Data\BE041316\  
Data File : BE091650.D  
Acq On : 13 Apr 2016 9:07  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 03:44:35 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040216.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Apr 01 23:17:06 2016  
Response via : Initial Calibration

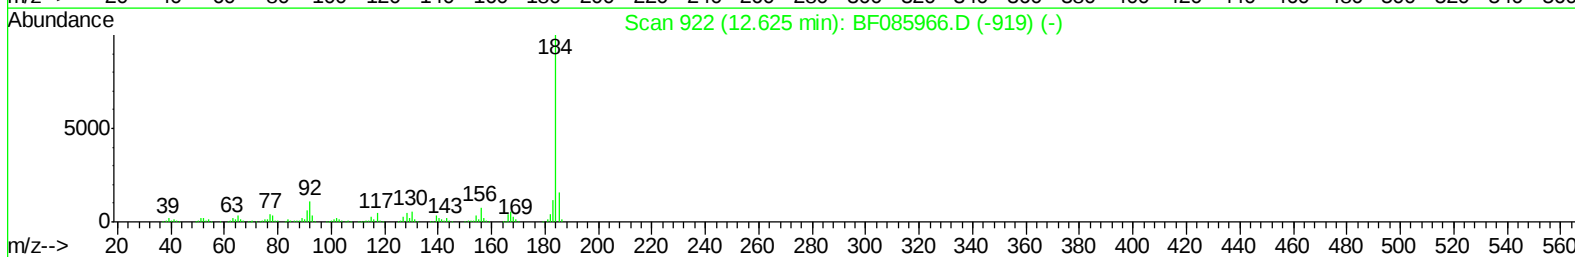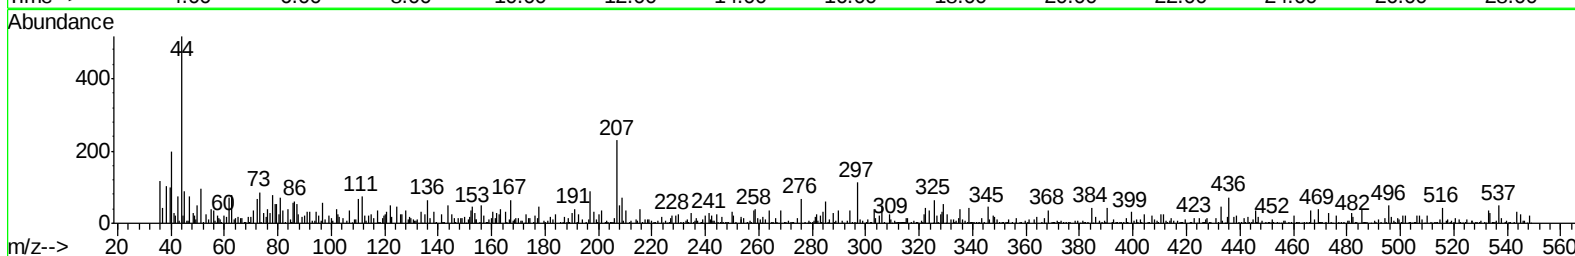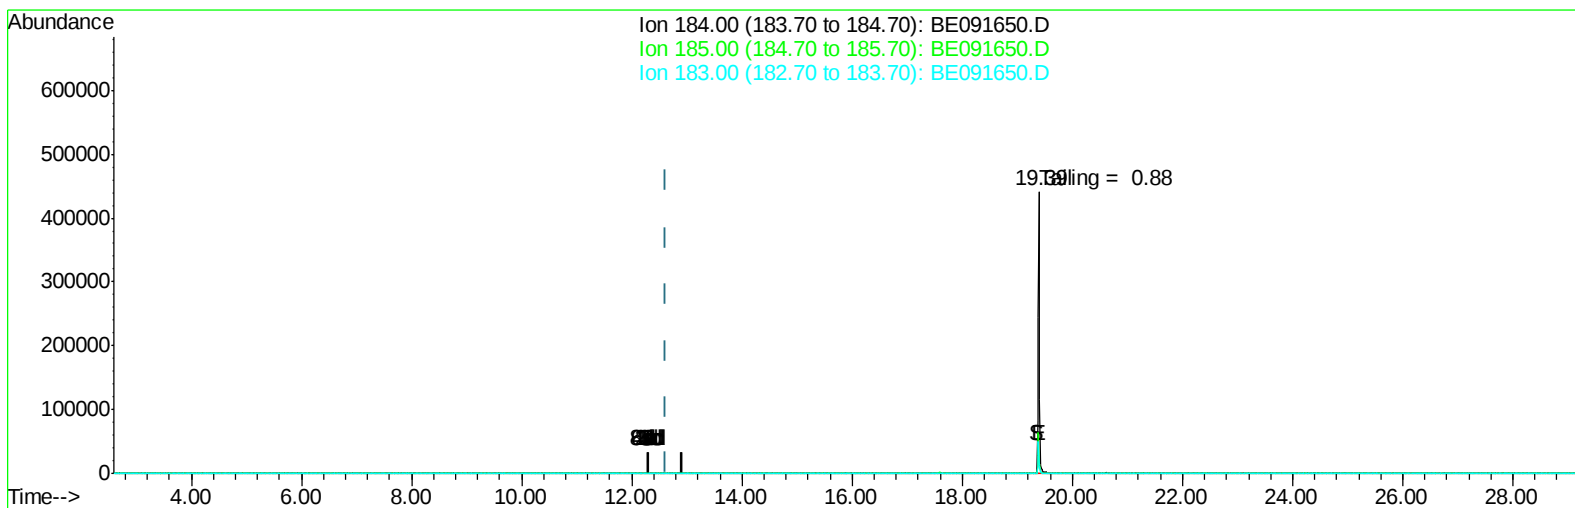

TIC: BE091650.D

(76) Benzidine

12.306min (-0.319) 23.03ng

response 13

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 15.50 | 0.00#  |
| 183.00 | 11.80 | 34.62# |
| 0.00   | 0.00  | 0.00   |