


Data Path : Z:\HPCHEM1\BNA_E\Data\BE041316\
 Data File : BE091650.D
 Acq On : 13 Apr 2016 9:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE040816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 08 16:48:14 2016

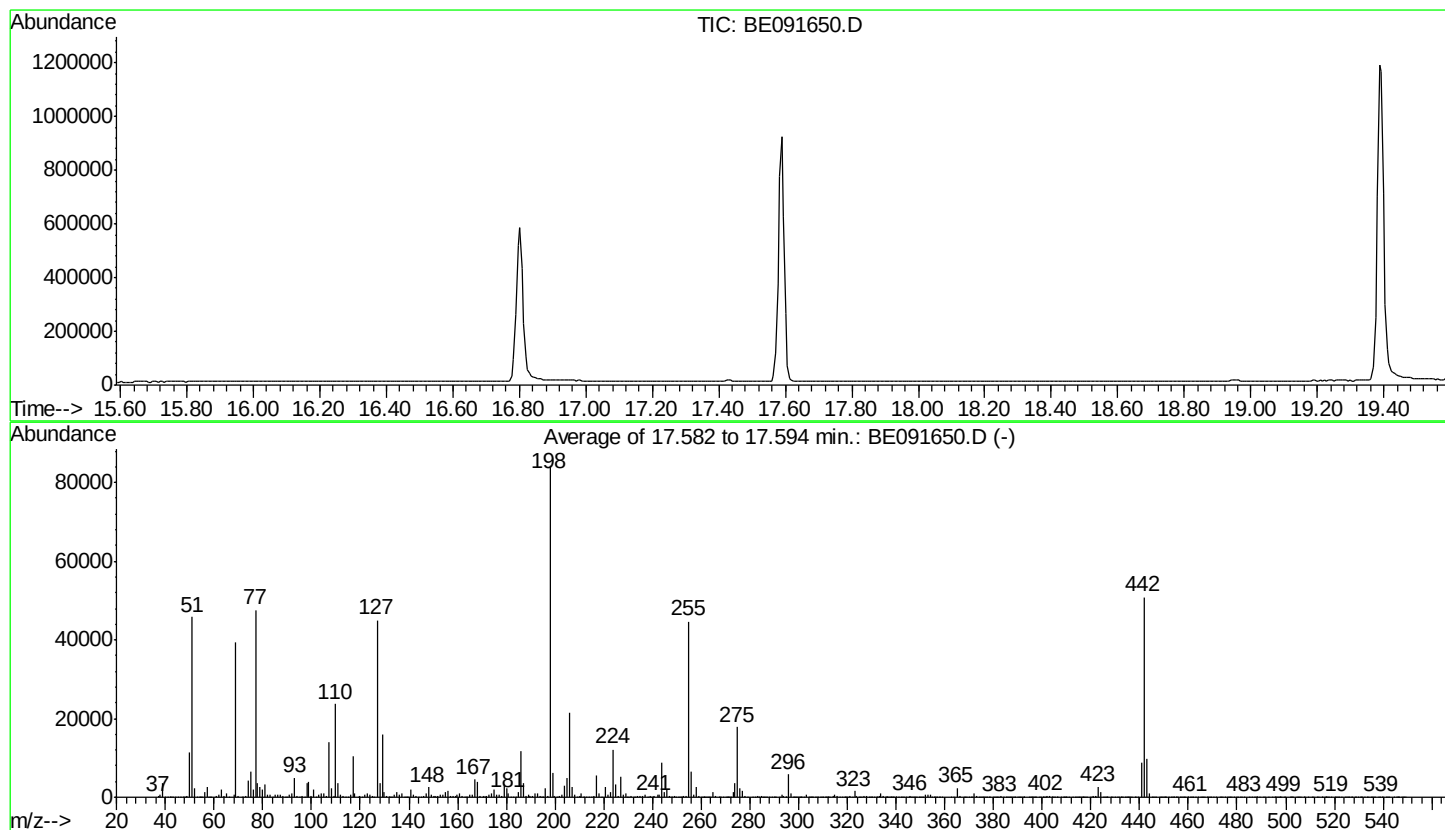

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	45741	PASS
68	69	0.00	2	1.6	620	PASS
69	198	0.00	100	46.7	39389	PASS
70	69	0.00	2	0.6	224	PASS
127	198	10	80	53.4	44976	PASS
197	198	0.00	2	0.2	181	PASS
198	198	100	100	100.0	84298	PASS
199	198	5	9	7.3	6156	PASS
275	198	10	60	21.1	17788	PASS
365	198	1	100	2.8	2367	PASS
441	442	0.01	24	17.4	8822	PASS
442	198	50	100	60.3	50821	PASS
443	442	15	24	19.4	9851	PASS