
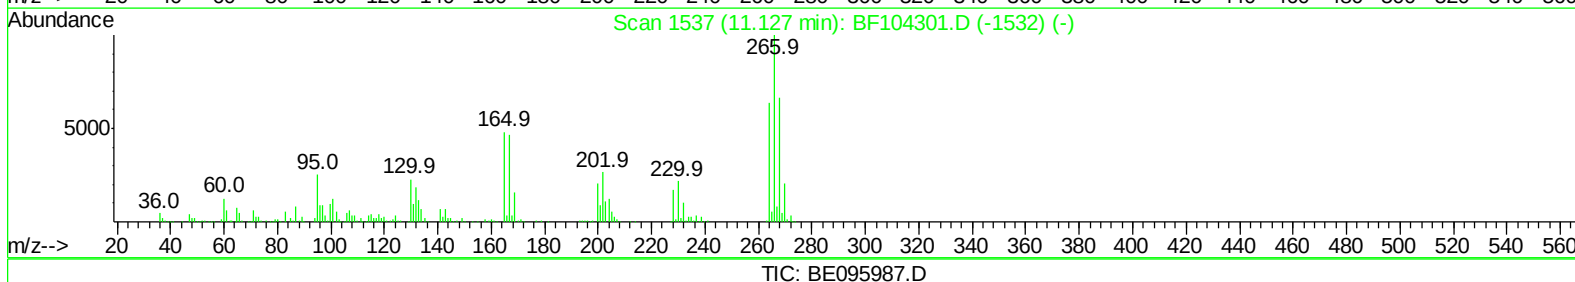
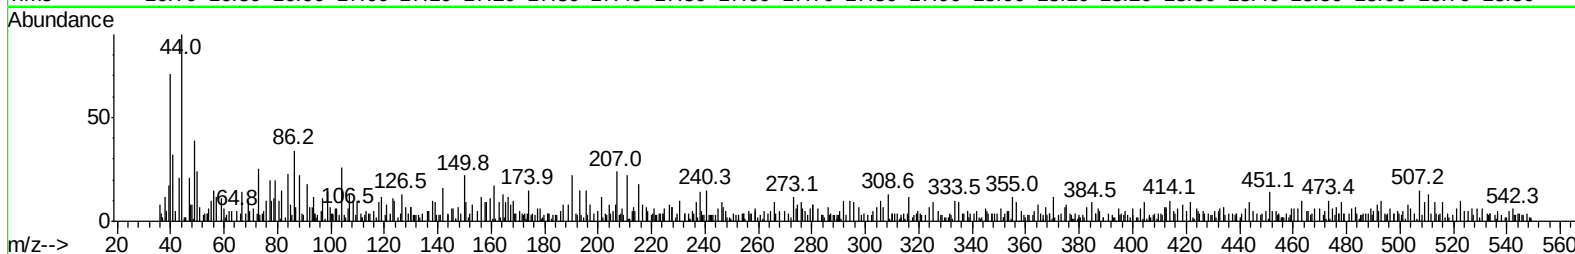


Data Path : Z:\HPCHEM1\BNA E\Data\BE041318\
Data File : BE095987.D
Acq On : 13 Apr 2018 8:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 02:06:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

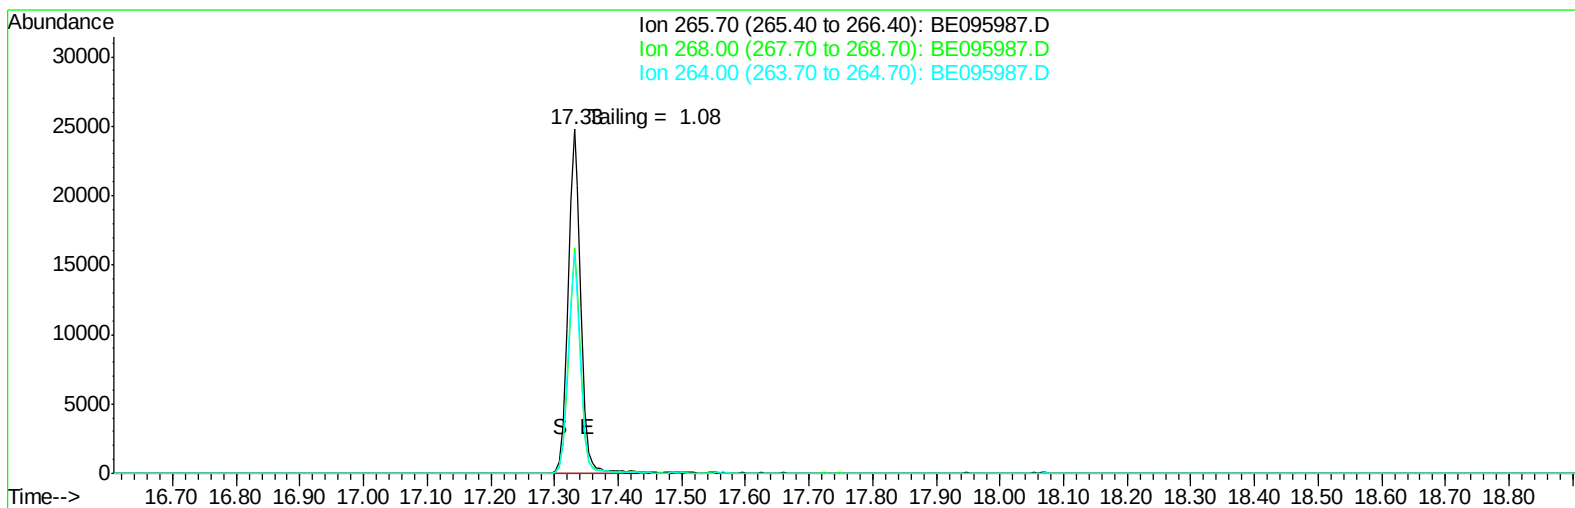

TIC: BE095987.D

(69) Pentachlorophenol (C)




11.214min (+0.069) 54.02ng

response 4

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.56
264.00	61.90	55.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE041318\
Data File : BE095987.D
Acq On : 13 Apr 2018 8:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 16 02:06:18 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 17:38:31 2018
Response via : Initial Calibration

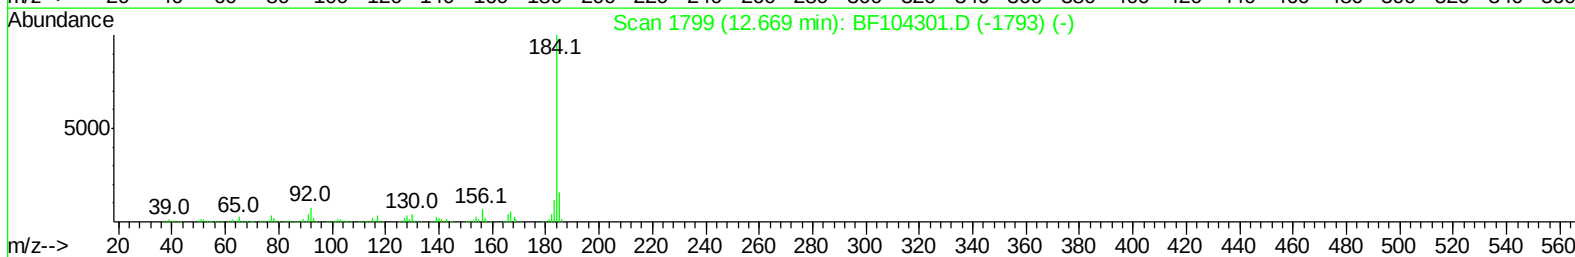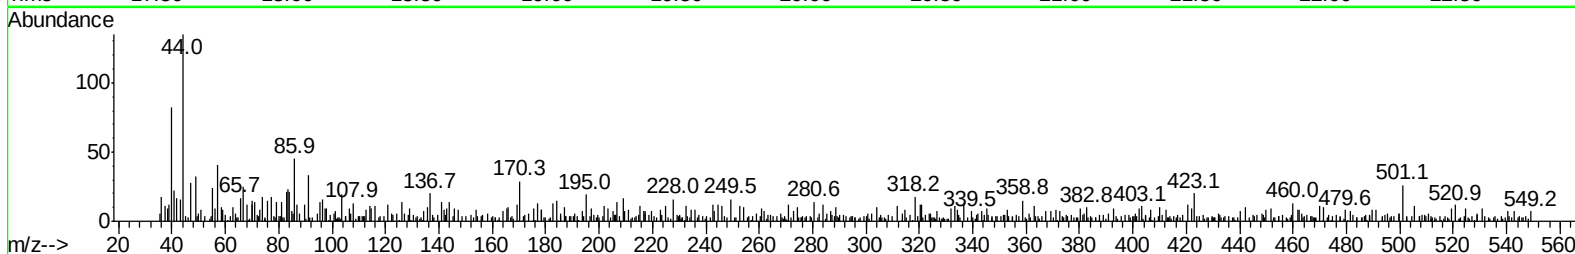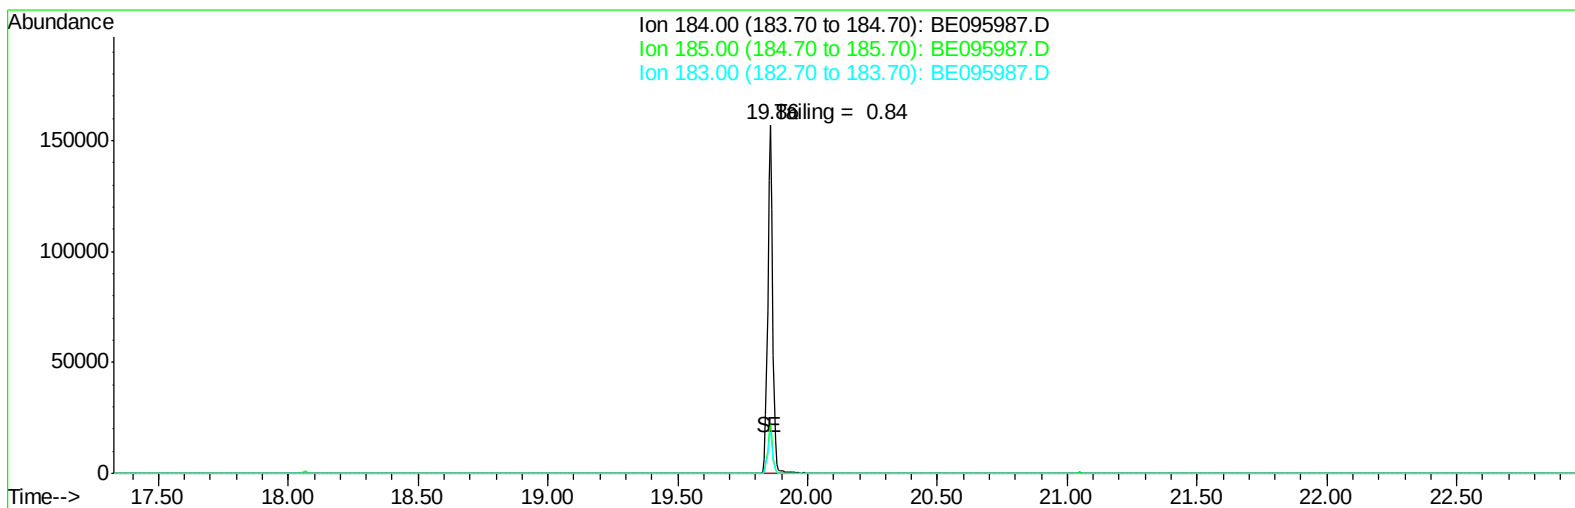

TIC: BE095987.D

(76) Benzidine

12.824min (+0.144) 65.49ng

response 15

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	40.00#
183.00	11.60	86.67#
0.00	0.00	0.00