

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE041318\
 Data File : BE095996.D
 Acq On : 13 Apr 2018 14:31
 Operator : SJ/JU
 Sample : J2308-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS034-180409

Quant Time: Apr 13 15:35:16 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 13 14:42:08 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1423	0.40	ng	0.00
7) Naphthalene-d8	11.22	136	5403	0.40	ng	0.00
13) Acenaphthene-d10	14.97	164	3004	0.40	ng	0.00
19) Phenanthrene-d10	17.67	188	7036	0.40	ng	0.00
27) Chrysene-d12	21.76	240	7374	0.40	ng	-0.01
34) Perylene-d12	24.38	264	7026	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.89	112	766	0.17	ng	0.00
5) Phenol-d6	7.53	99	634	0.10	ng	0.00
8) Nitrobenzene-d5	9.57	82	2761	0.44	ng	0.00
11) 2-Methylnaphthalene-d10	12.76	152	3827	0.45	ng	0.00
14) 2,4,6-Tribromophenol	16.44	330	644	0.44	ng	0.00
15) 2-Fluorobiphenyl	13.61	172	7560	0.59	ng	0.00
25) Fluoranthene-d10	19.66	212	40578	0.42	ng	0.00
29) Terphenyl-d14	20.22	244	9781	0.60	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.62	149	6276	0.103	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE041318\
Data File : BE095996.D
Acq On : 13 Apr 2018 14:31
Operator : SJ/JU
Sample : J2308-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
KY038PS034-180409

Quant Time: Apr 13 15:35:16 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 13 14:42:08 2018
Response via : Initial Calibration

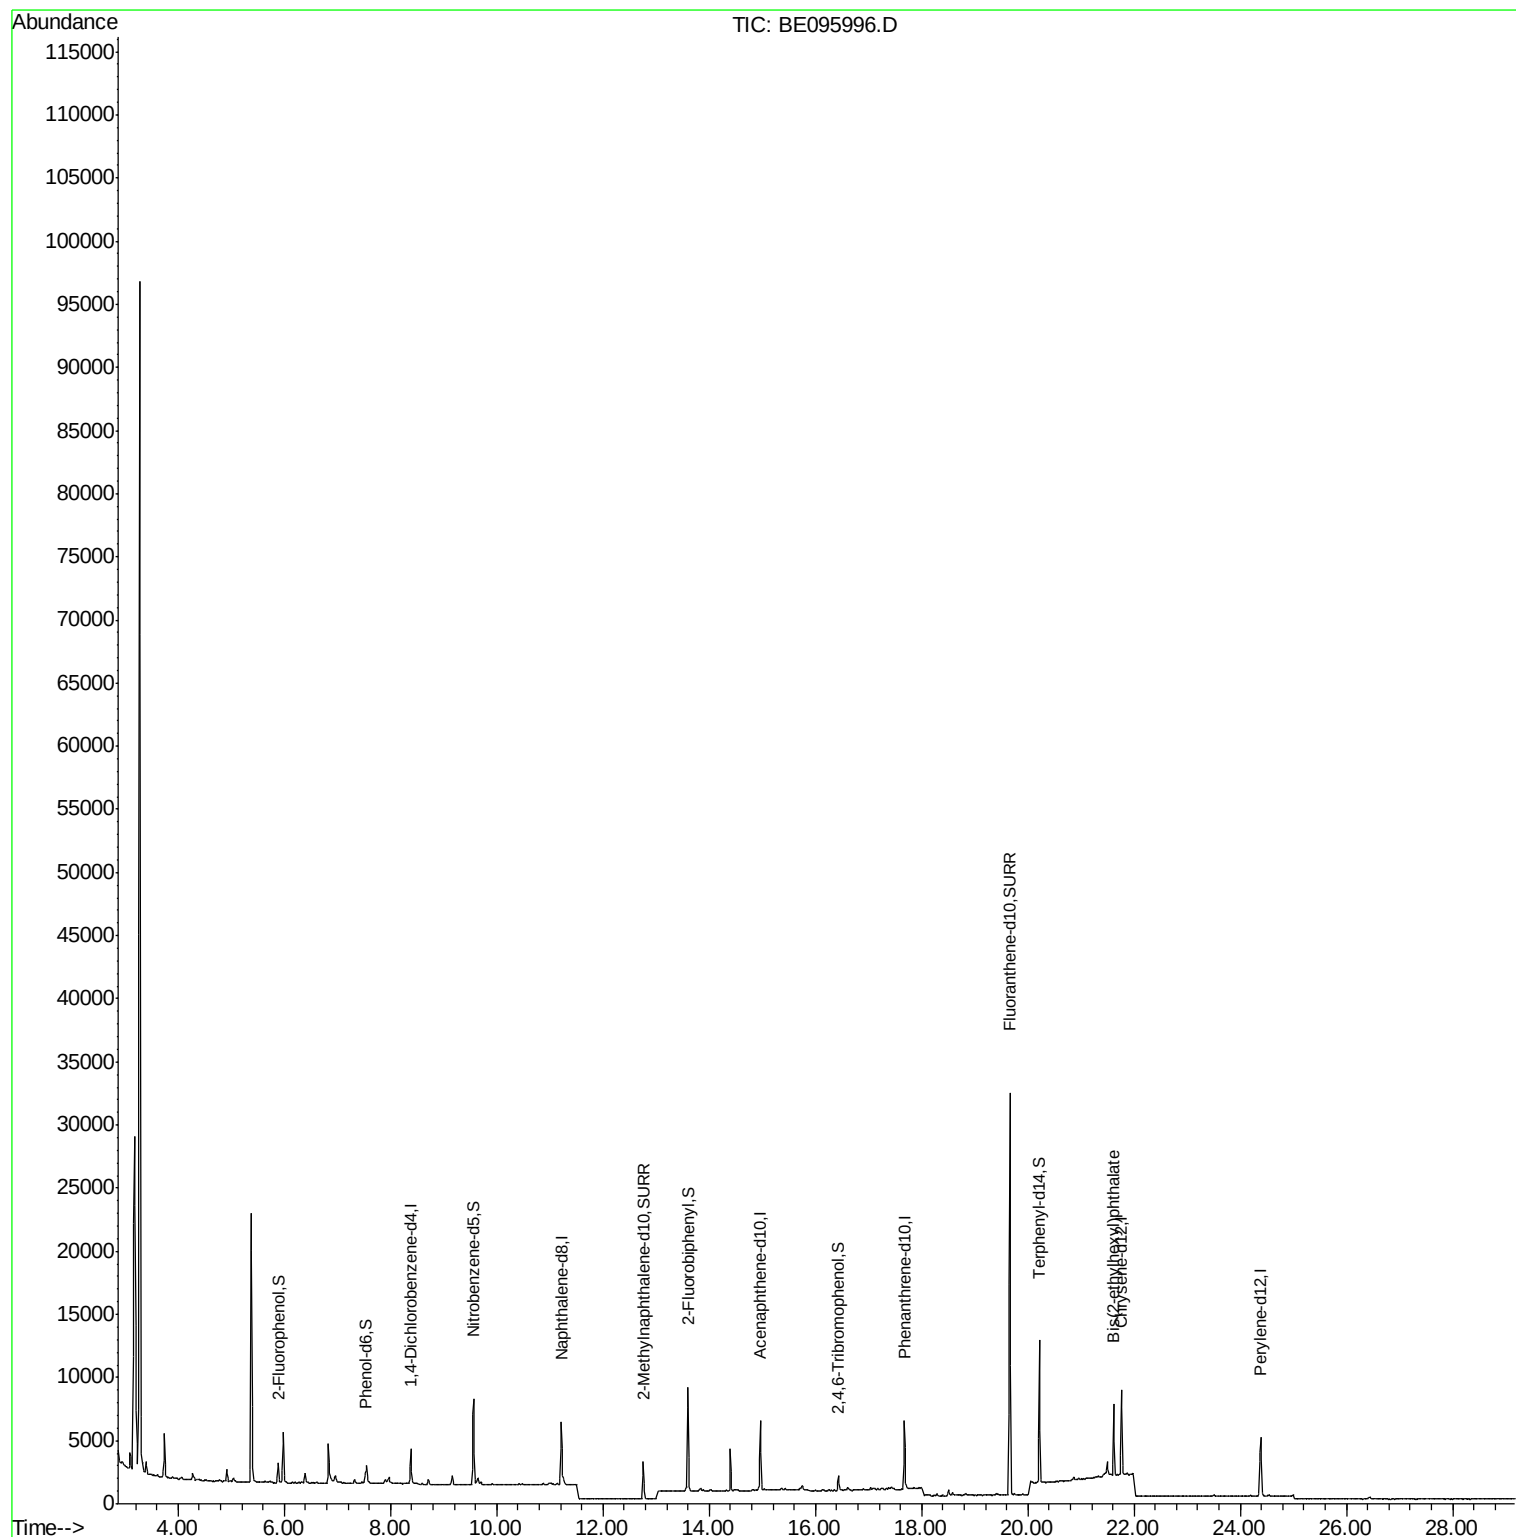

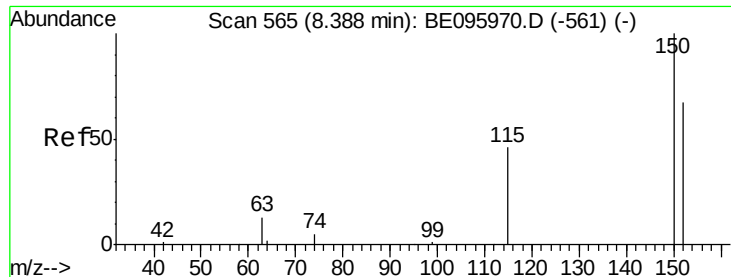

#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 8.38 min Scan# 564

Delta R.T. -0.01 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion:152 Resp: 1423

Ion Ratio Lower Upper

152 100

150 147.7 117.2 175.8




115 71.1 57.0 85.6

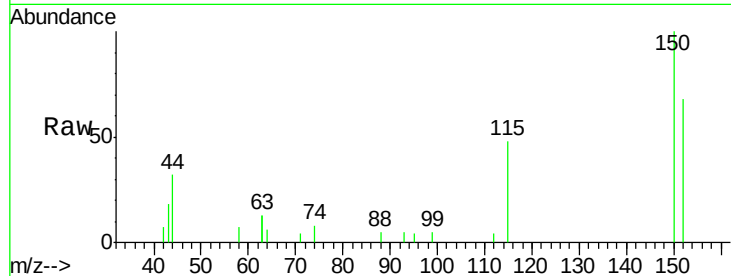

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

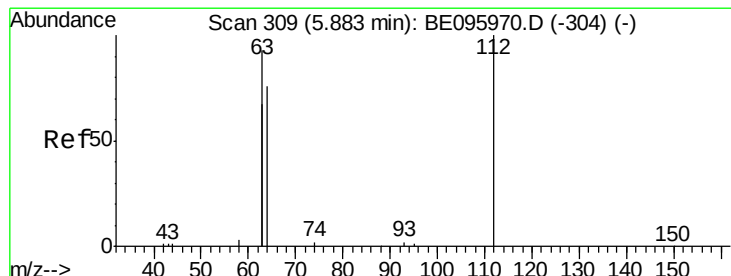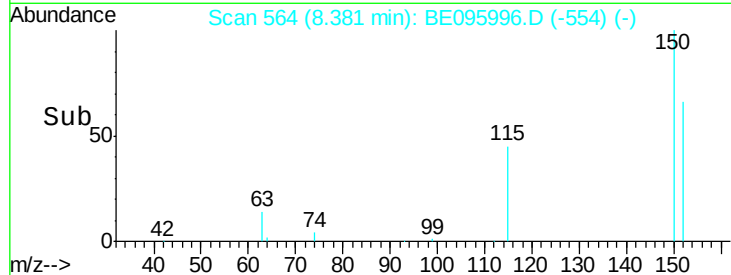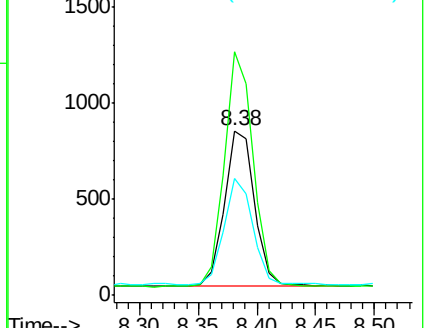

#4

2-Fluorophenol

Concen: 0.174 ng

RT: 5.89 min Scan# 309

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31


Tgt Ion:112 Resp: 766

Ion Ratio Lower Upper

112 100

64 75.1 60.1 90.1



63 177.7 116.8 175.2#

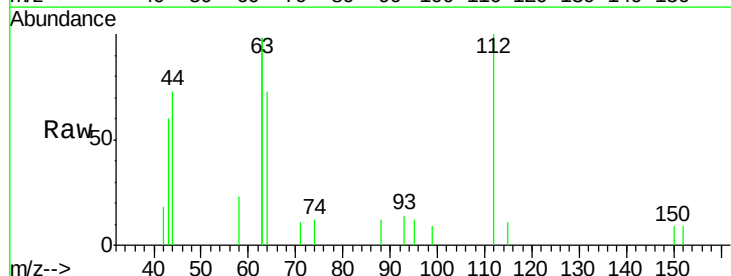


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

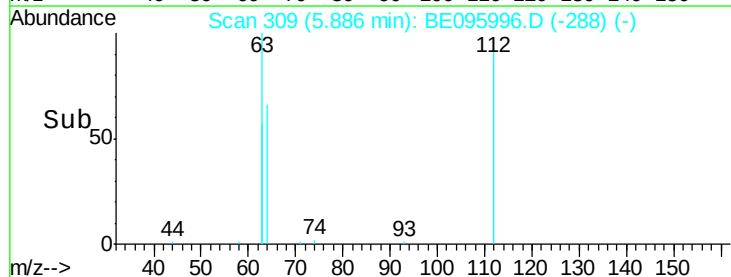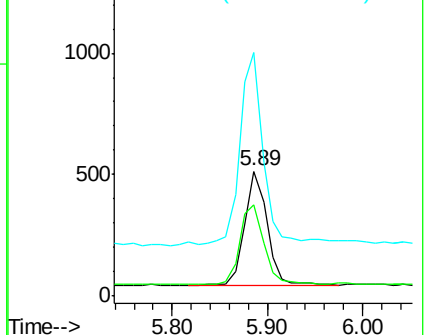

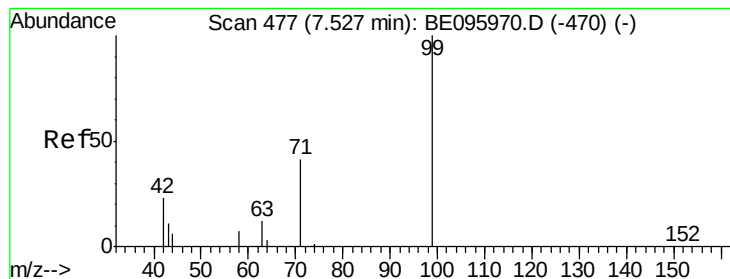

#5

Phenol-d6

Concen: 0.104 ng

RT: 7.53 min Scan# 477

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion: 99 Resp: 634

Ion Ratio Lower Upper

99 100

42 31.5 20.2 30.2#


71 47.0 28.4 42.6#

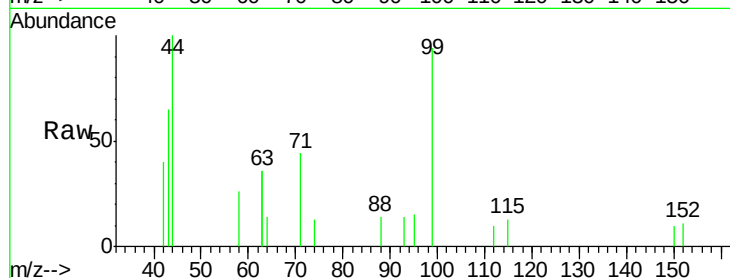



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

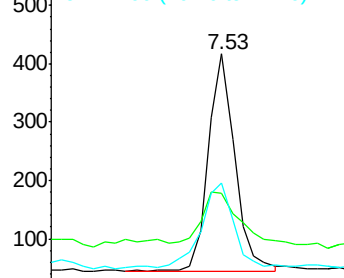

Time-->

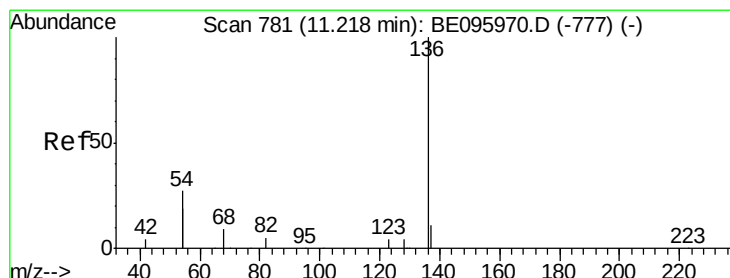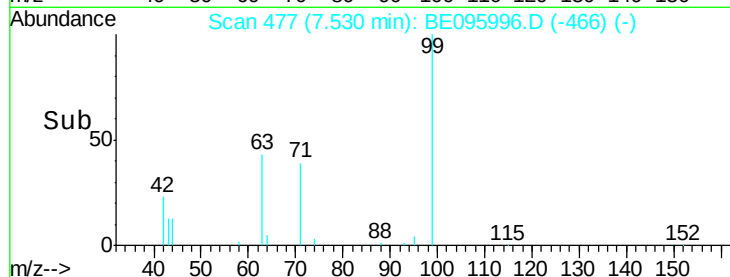

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.22 min Scan# 781

Delta R.T. -0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Tgt Ion: 136 Resp: 5403


Ion Ratio Lower Upper

136 100

137 11.9 9.5 14.3

54 46.9 29.1 43.7#

68 8.4 6.2 9.2

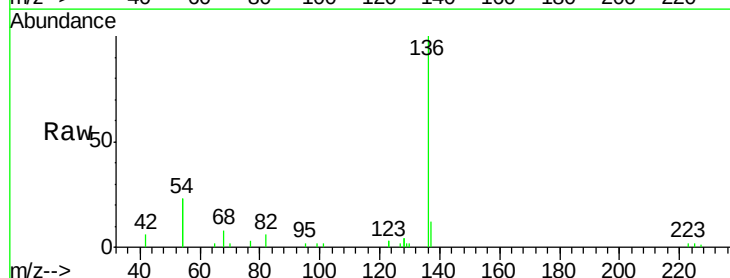


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

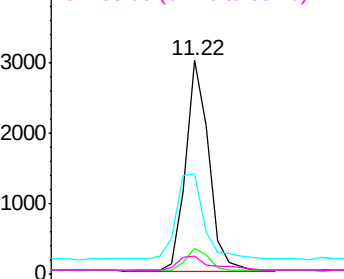

Time-->

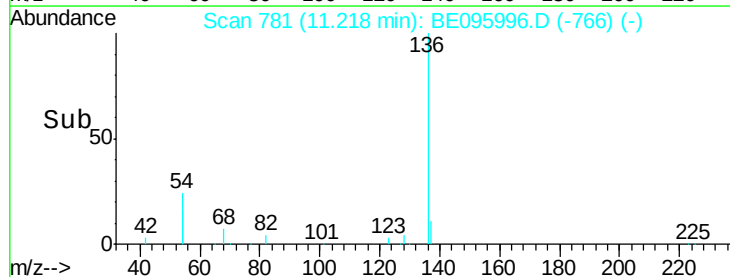

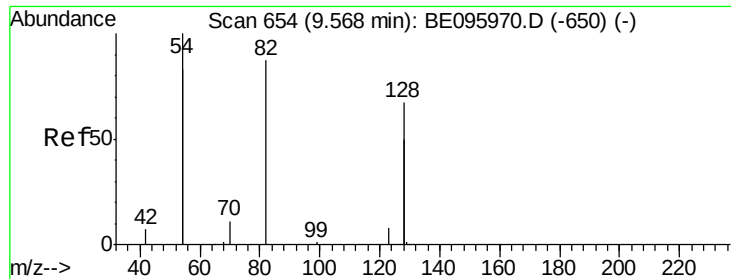

#8

Nitrobenzene-d5

Concen: 0.436 ng

RT: 9.57 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion: 82 Resp: 2761

Ion Ratio Lower Upper

82 100

128 148.3 150.0 225.0#




54 209.0 154.2 231.4

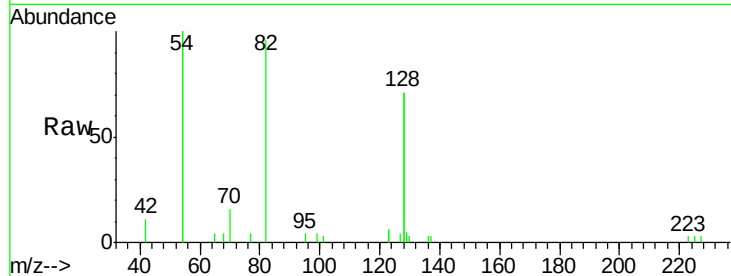

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

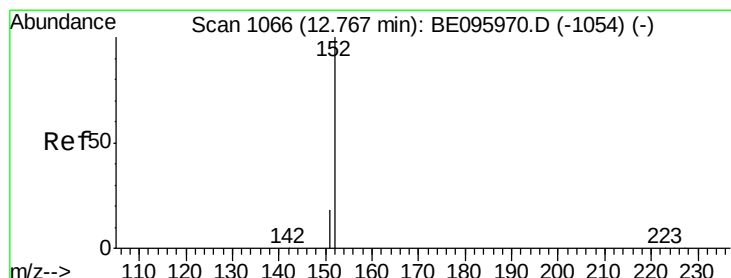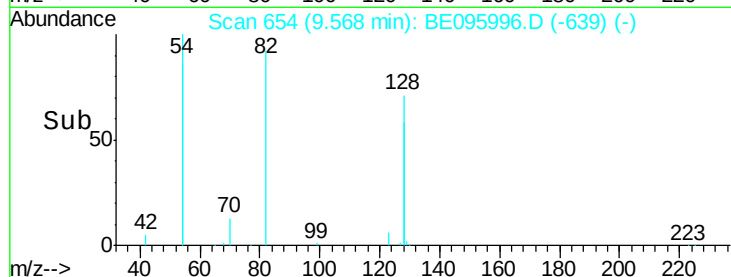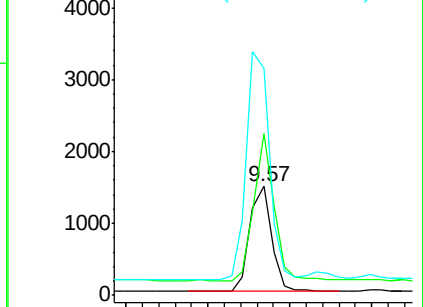

#11

2-Methylnaphthalene-d10

Concen: 0.447 ng

RT: 12.76 min Scan# 1065

Delta R.T. -0.00 min

Lab File: BE095996.D


Acq: 13 Apr 2018 14:31

Tgt Ion: 152 Resp: 3827

Ion Ratio Lower Upper



152 100


151 19.9 15.4 23.0

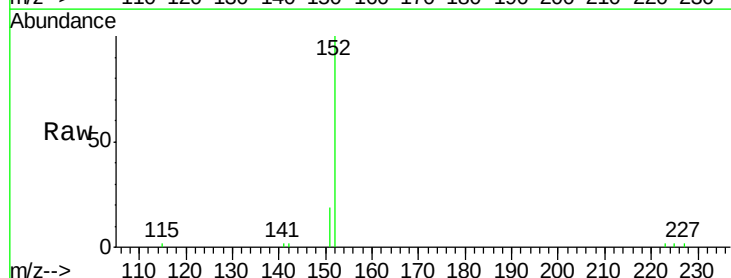

Abundance Ion 152.00 (151.70 to 152.70): BE0

Ion 151.00 (150.70 to 151.70): BE0

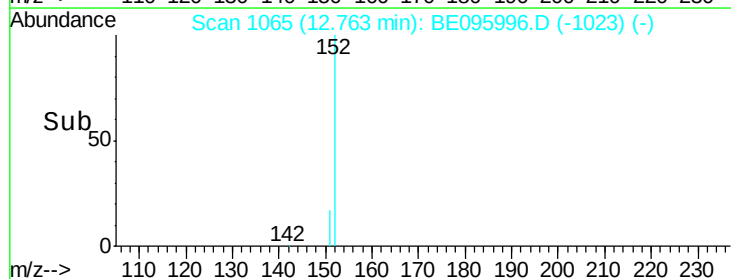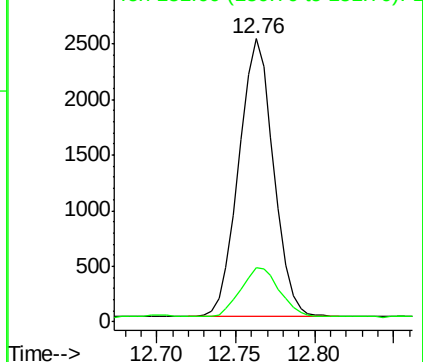

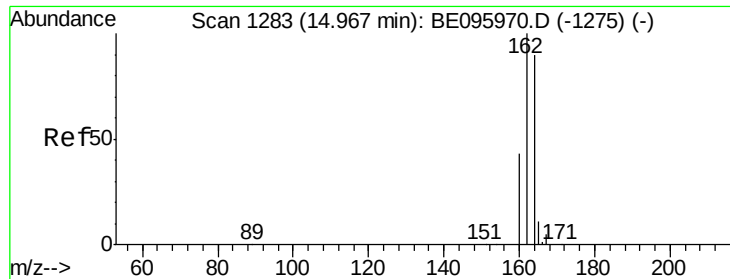

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.97 min Scan# 1283

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion:164 Resp: 3004

Ion Ratio Lower Upper

164 100

162 105.5 83.1 124.7




160 45.4 37.1 55.7

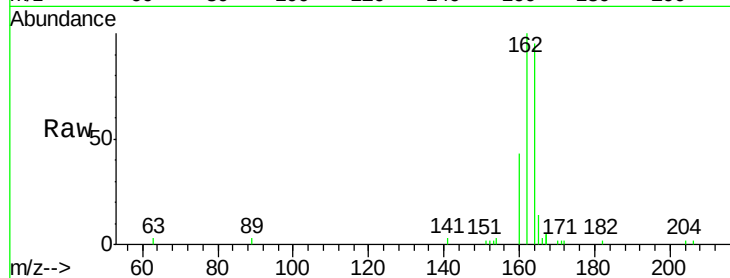

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

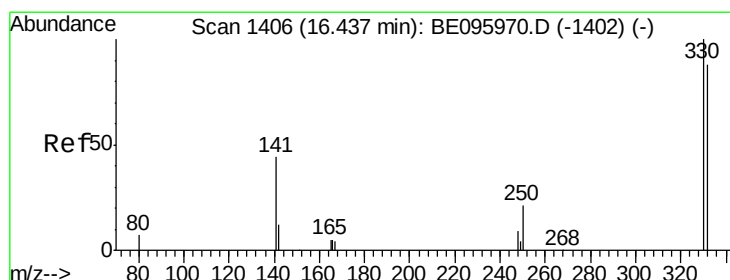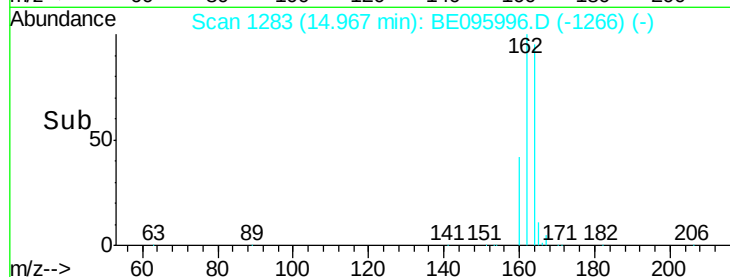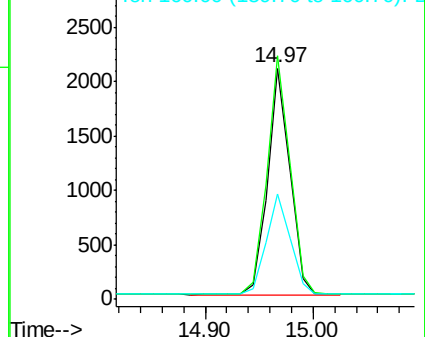

#14

2,4,6-Tribromophenol

Concen: 0.444 ng

RT: 16.44 min Scan# 1406

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31


Tgt Ion:330 Resp: 644

Ion Ratio Lower Upper

330 100

332 97.4 152.7 229.1#



141 43.5 33.7 50.5

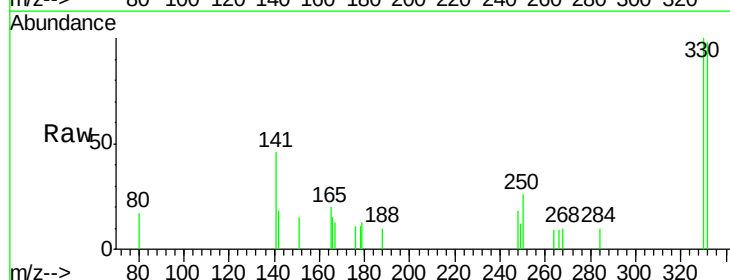


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

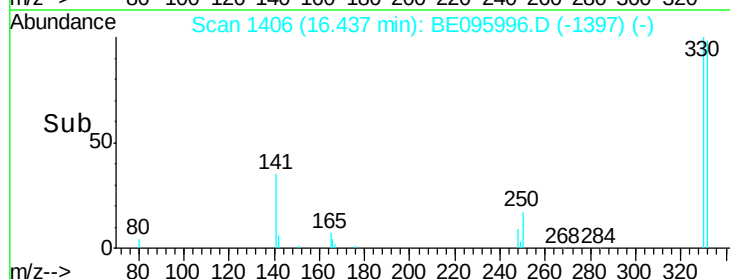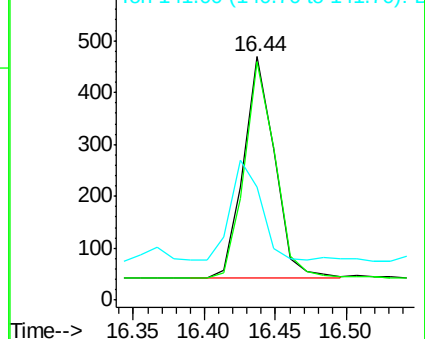

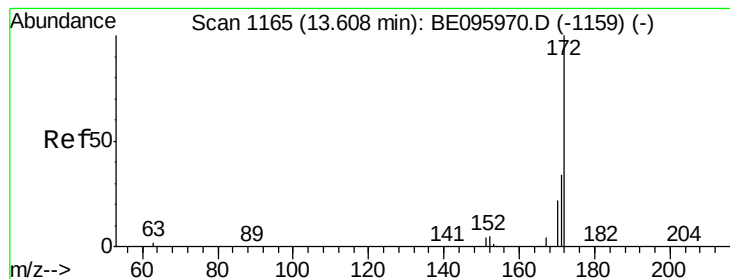

#15

2-Fluorobiphenyl

Concen: 0.588 ng

RT: 13.61 min Scan# 1165

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion:172 Resp: 7560

Ion Ratio Lower Upper

172 100

171 34.3 29.9 44.9




170 21.9 21.8 32.8

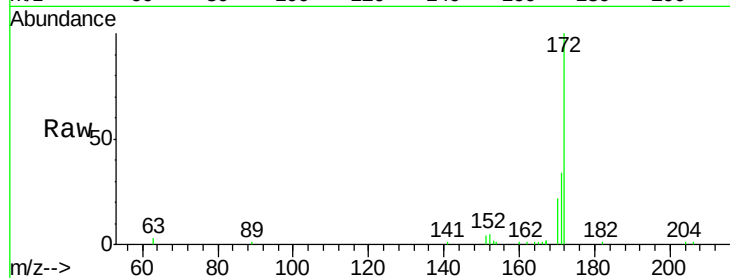

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

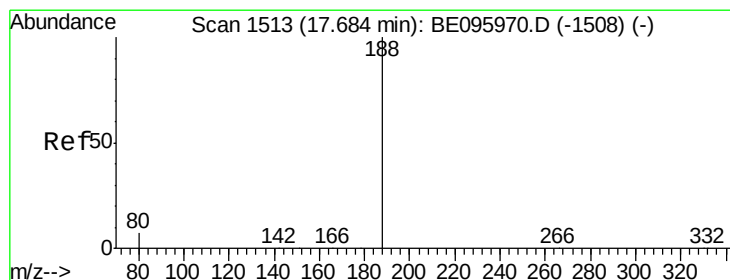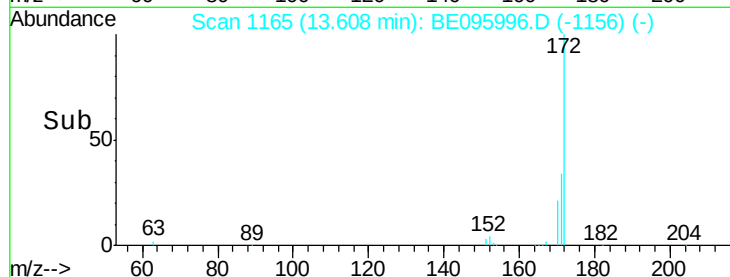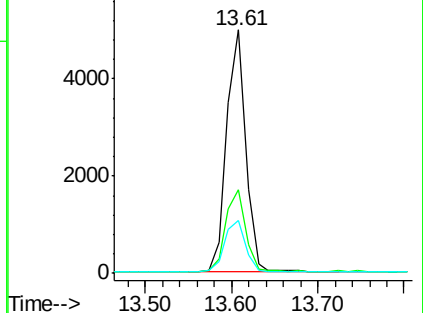

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.67 min Scan# 1512

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31


Tgt Ion:188 Resp: 7036

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#



80 13.9 3.6 5.4#

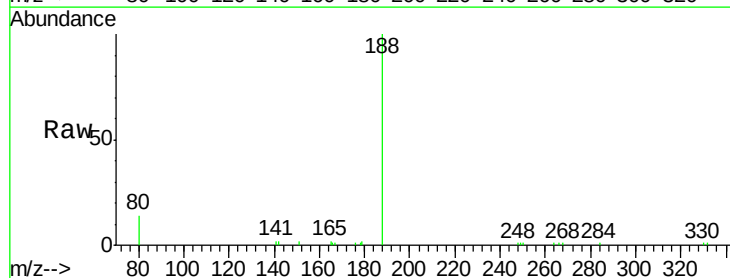


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

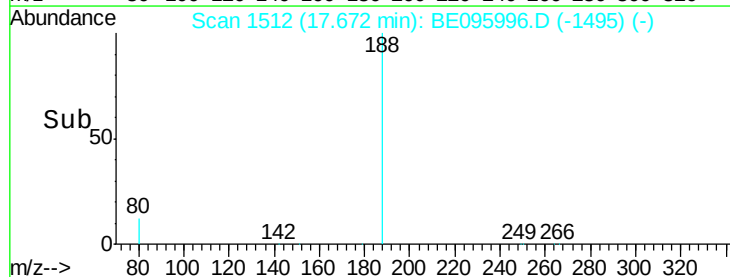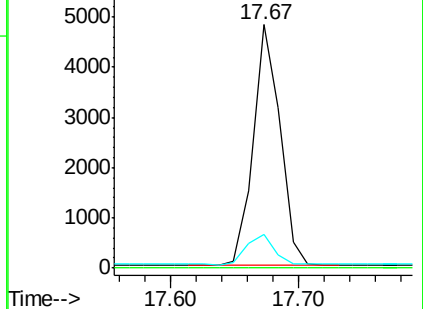

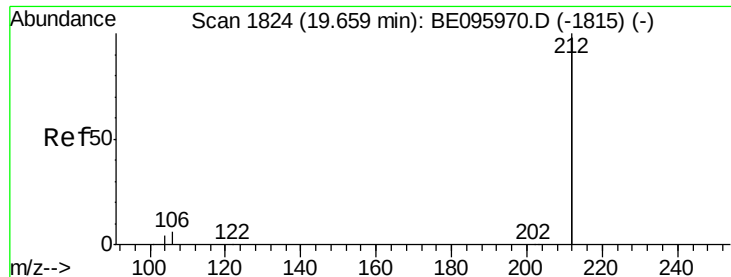

#25

Fluoranthene-d10

Concen: 0.425 ng

RT: 19.66 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion:212 Resp: 40578

Ion Ratio Lower Upper

212 100

106 2.9 2.8 4.2




104 1.7 1.6 2.4

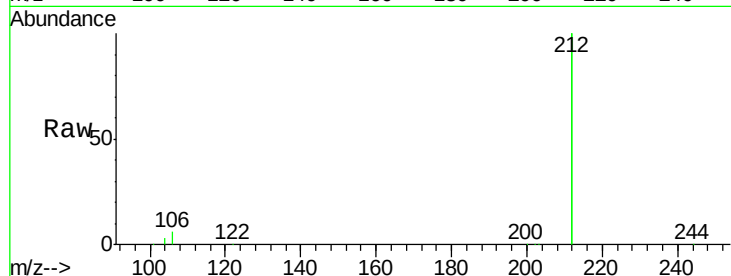

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

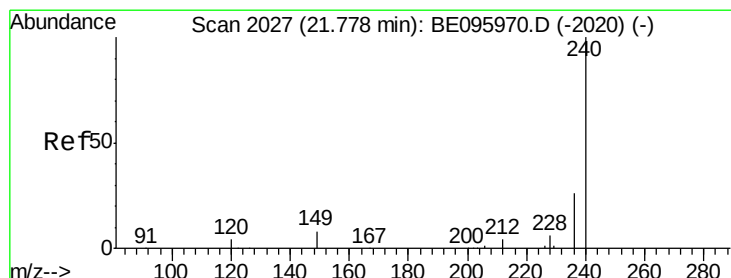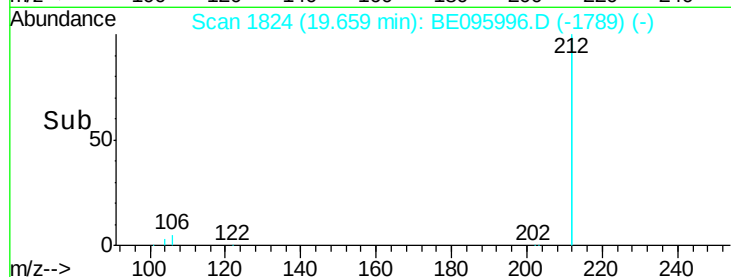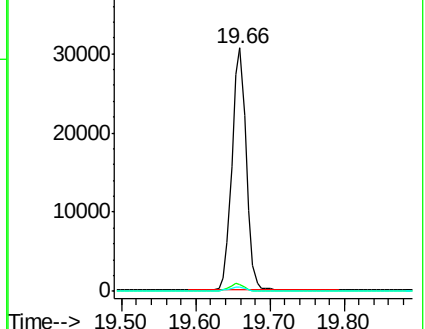

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.76 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31


Tgt Ion:240 Resp: 7374

Ion Ratio Lower Upper

240 100

120 14.0 5.5 8.3#



236 28.7 20.7 31.1

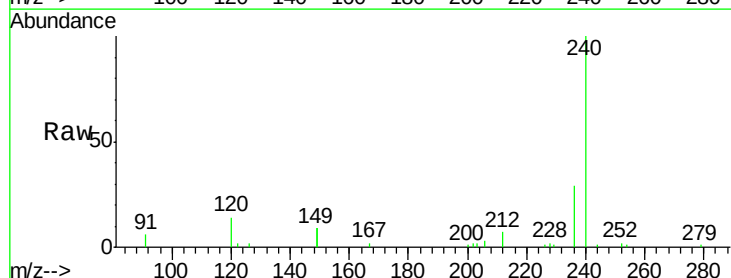


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

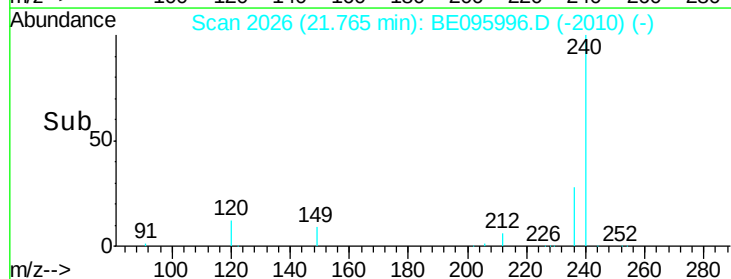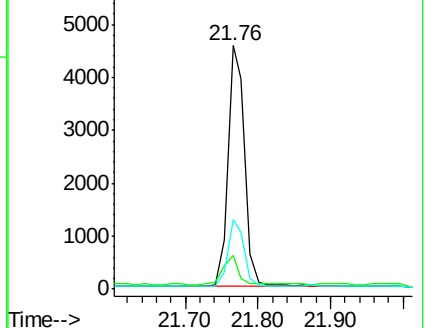

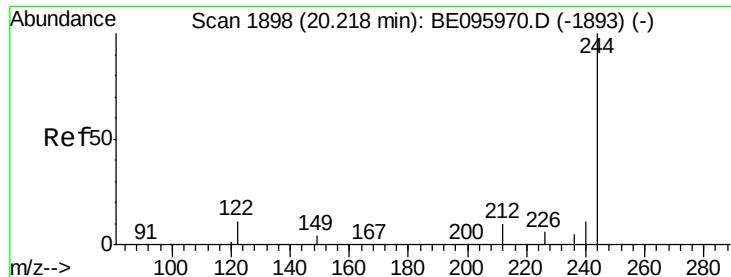

#29

Terphenyl-d14

Concen: 0.600 ng

RT: 20.22 min Scan# 1898

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409


Tgt Ion:244 Resp: 9781

Ion Ratio Lower Upper

244 100

212 9.1 25.4 38.0#

122 8.6 8.1 12.1

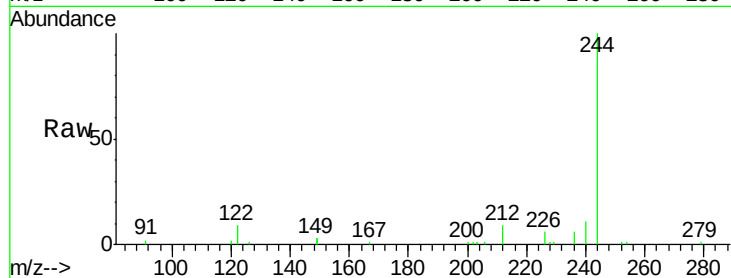


Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

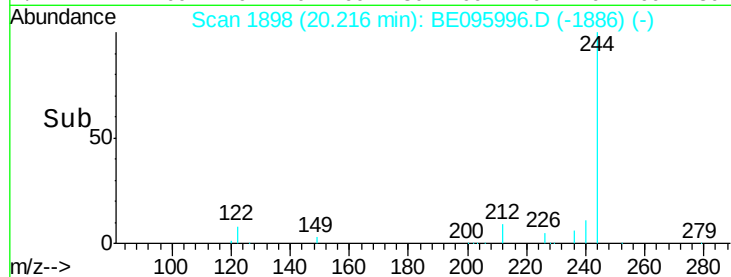

Time-->

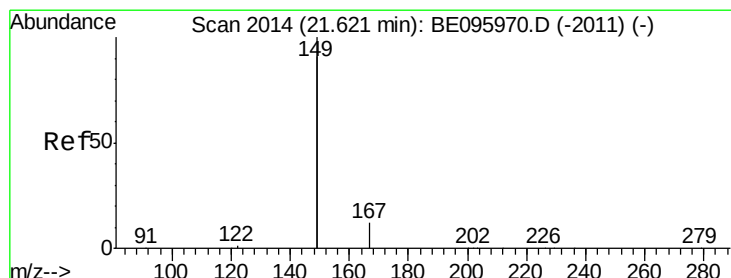

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.103 ng

RT: 21.62 min Scan# 2014

Delta R.T. 0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31


Tgt Ion:149 Resp: 6276

Ion Ratio Lower Upper

149 100

167 6.5 5.4 8.0

279 0.8 0.7 1.1

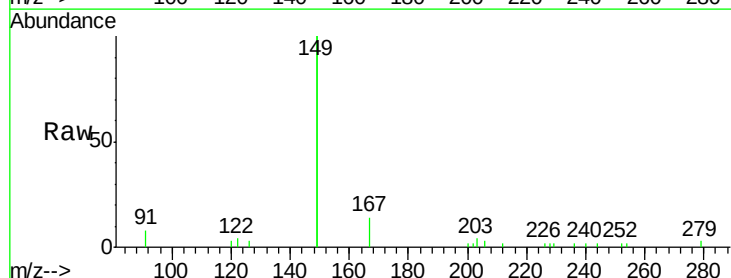


Abundance Ion 149.00 (148.70 to 149.70): E




Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

Time-->

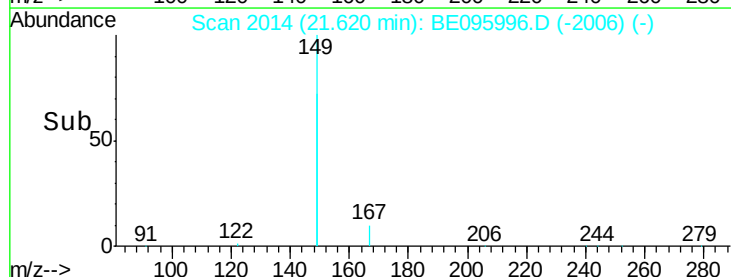

Time-->

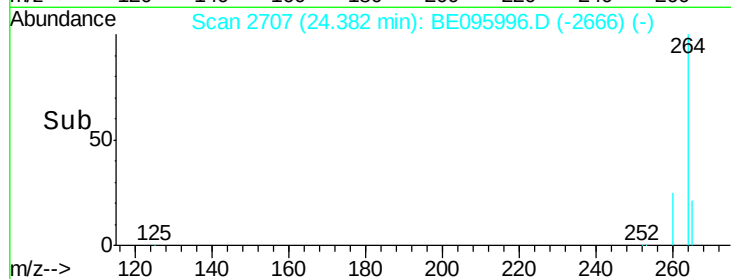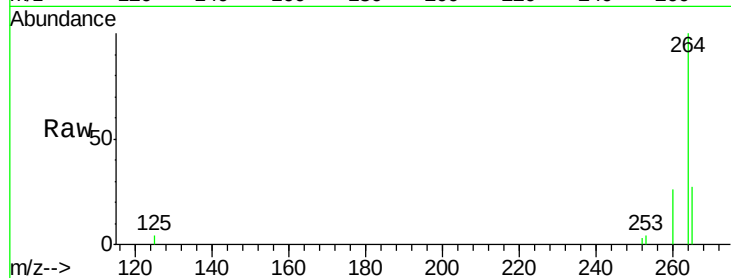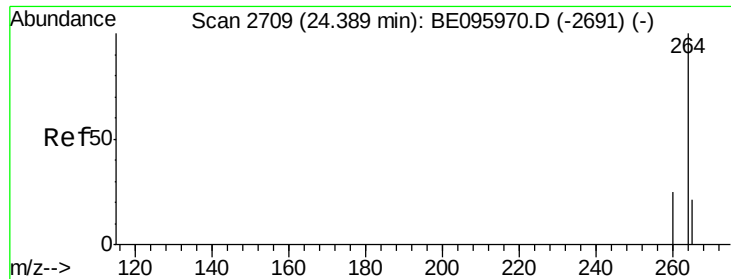

#34

Perylene-d12

Concen: 0.400 ng

RT: 24.38 min Scan# 2707

Delta R.T. -0.00 min

Lab File: BE095996.D

Acq: 13 Apr 2018 14:31

Instrument :

BNA_E

ClientSampleId :

KY038PS034-180409

Tgt Ion: 264 Resp: 7026

Ion Ratio Lower Upper

264 100

260 26.4 20.5 30.7

265 27.2 22.8 34.2

