


Data Path : Z:\HPCHEM1\BNA_E\Data\BE041318\
Data File : BE095987.D
Acq On : 13 Apr 2018 8:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 13 14:42:08 2018

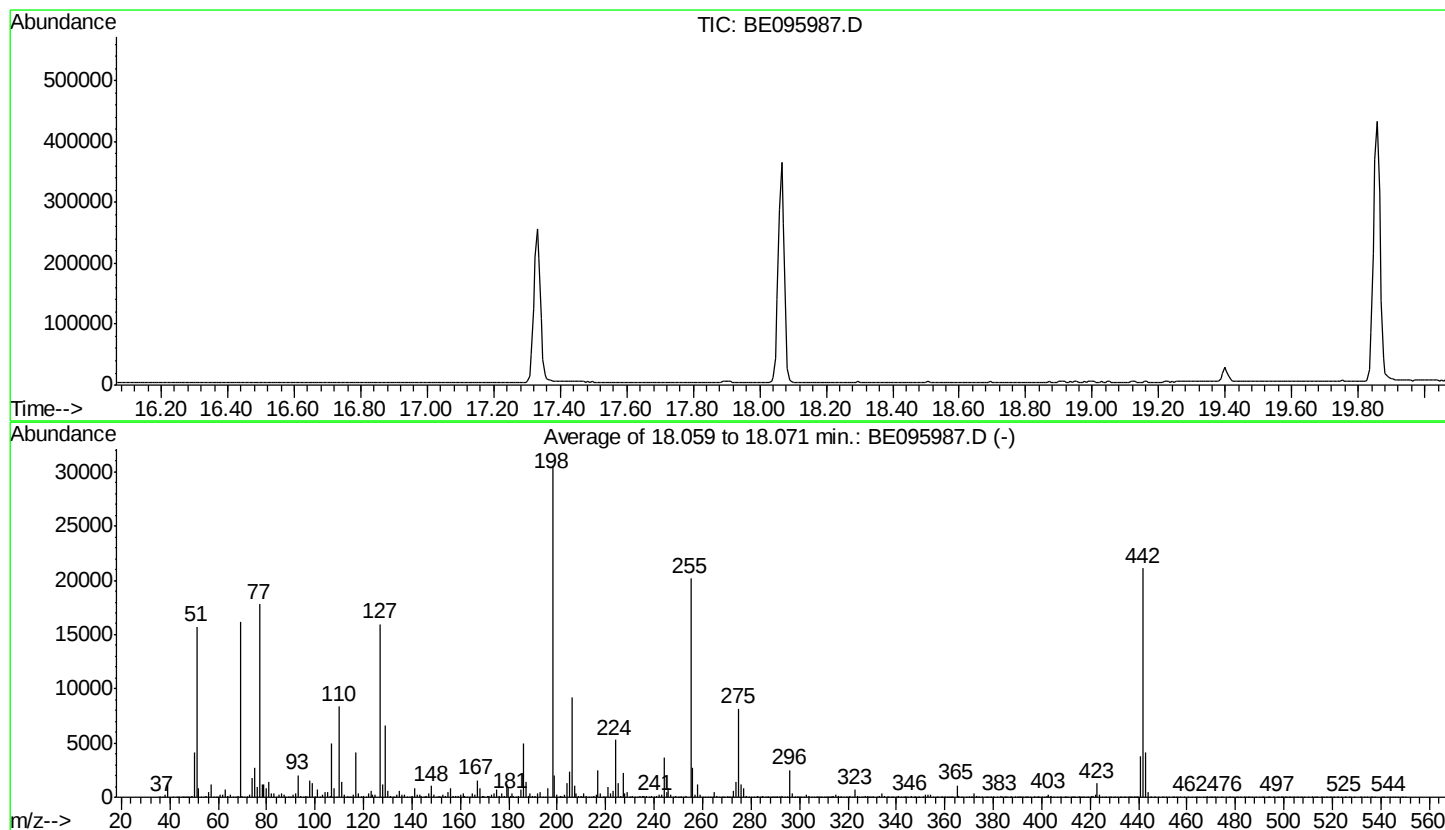

AutoFind: Scans 2633, 2634, 2635; Background Corrected with Scan 2626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	15732	PASS
68	69	0.00	2	0.6	105	PASS
69	198	0.00	100	53.1	16222	PASS
70	69	0.00	2	0.6	94	PASS
127	198	10	80	52.2	15948	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30578	PASS
199	198	5	9	6.7	2041	PASS
275	198	10	60	26.8	8180	PASS
365	198	1	100	3.5	1066	PASS
441	443	0.01	100	90.9	3793	PASS
442	198	50	100	69.1	21126	PASS
443	442	15	24	19.8	4173	PASS