
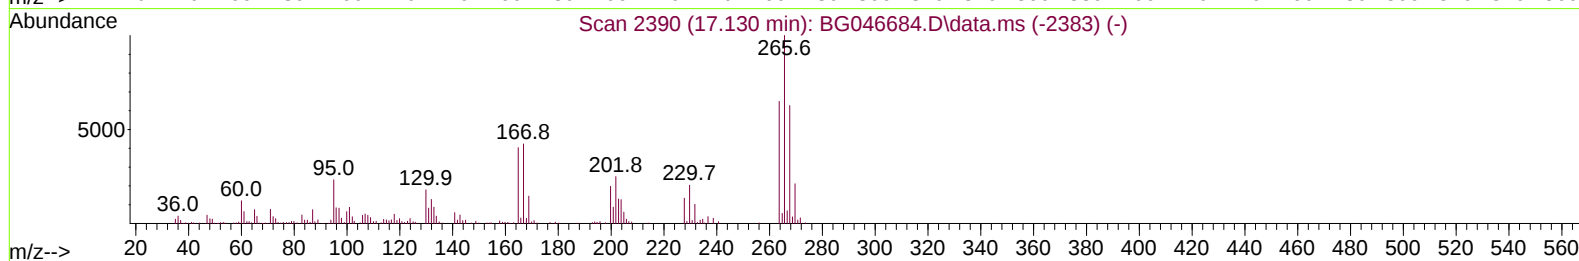
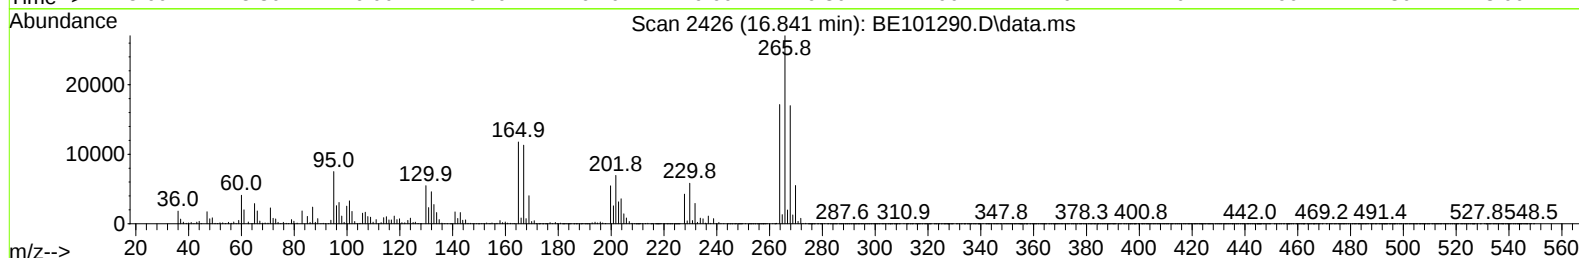


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041321\
 Data File : BE101290.D
 Acq On : 13 Apr 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 02:19:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

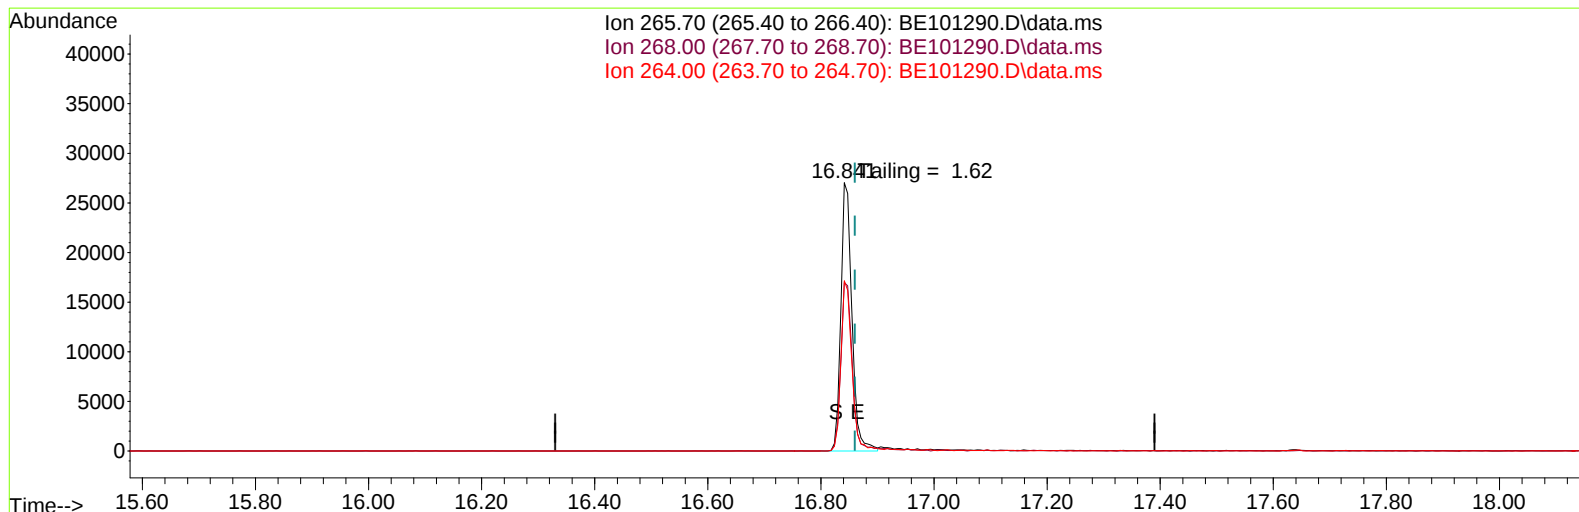

TIC: BE101290.D\data.ms

(70) Pentachlorophenol (C)




16.841min (-0.019) 311121.09 ng

response 36624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.79
264.00	61.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041321\
 Data File : BE101290.D
 Acq On : 13 Apr 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 02:19:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

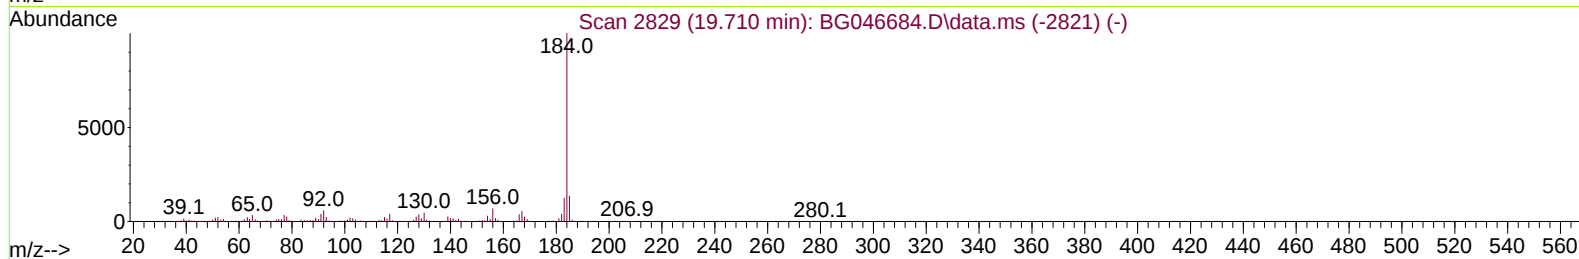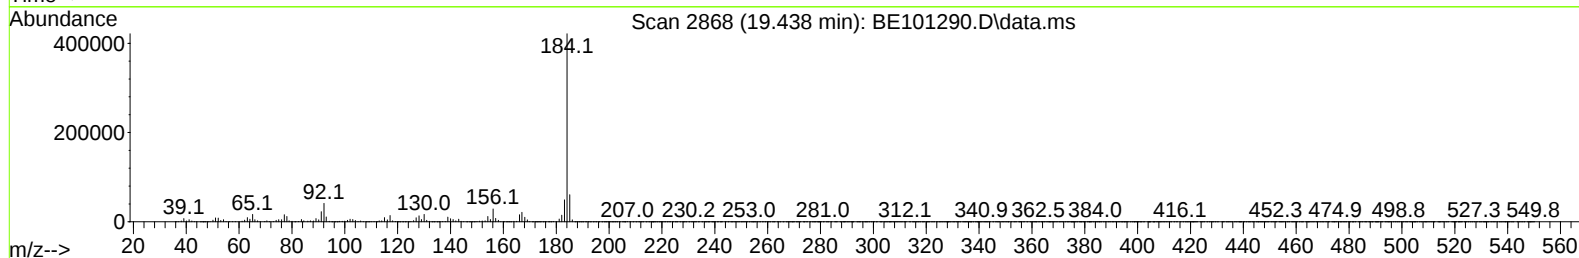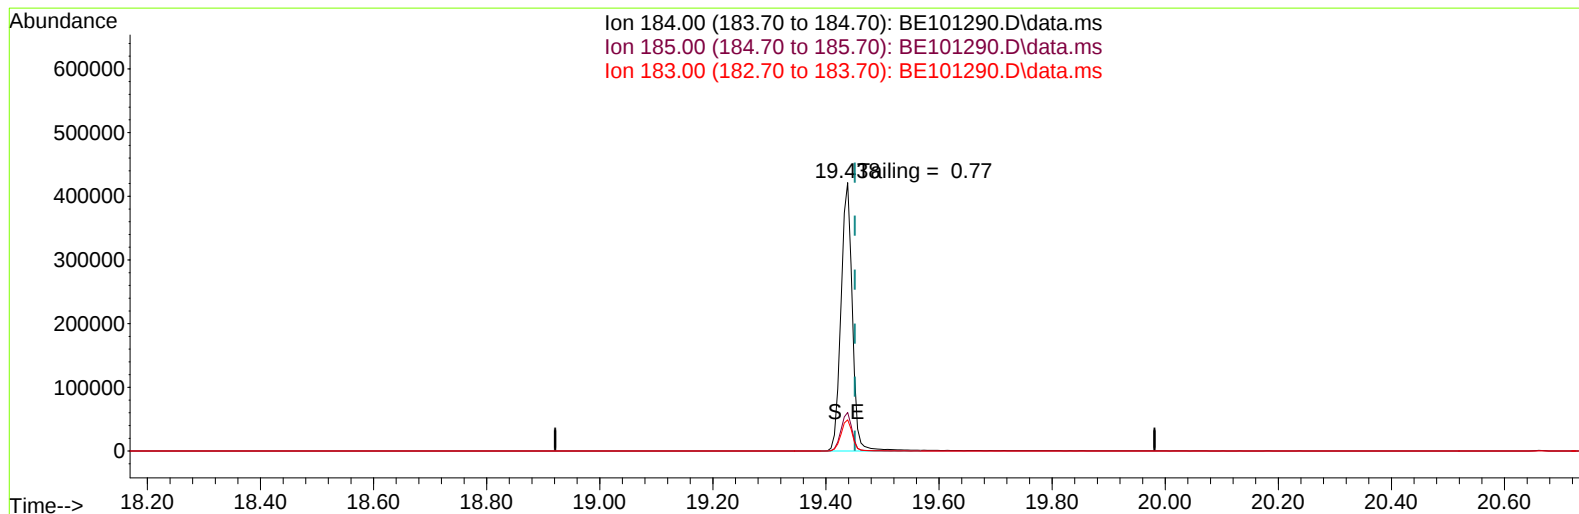

TIC: BE101290.D\data.ms

(77) Benzidine**19.438min (-0.013) 5011.04 ng****response 590683**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.64
0.00	0.00	0.00