
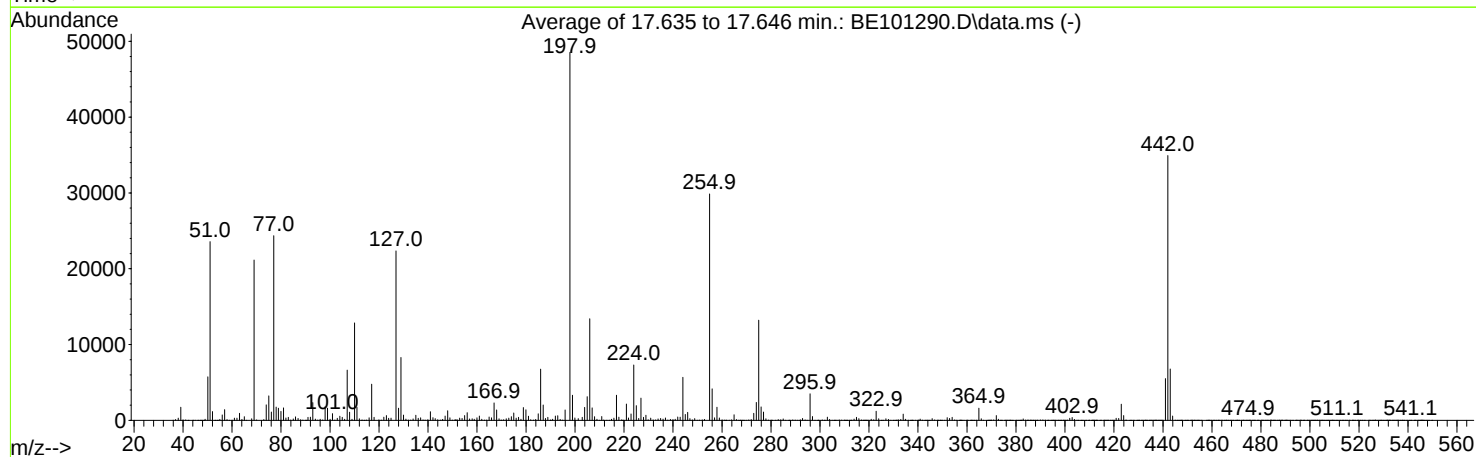


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041321\
 Data File : BE101290.D
 Acq On : 13 Apr 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE041221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 12 18:02:55 2021

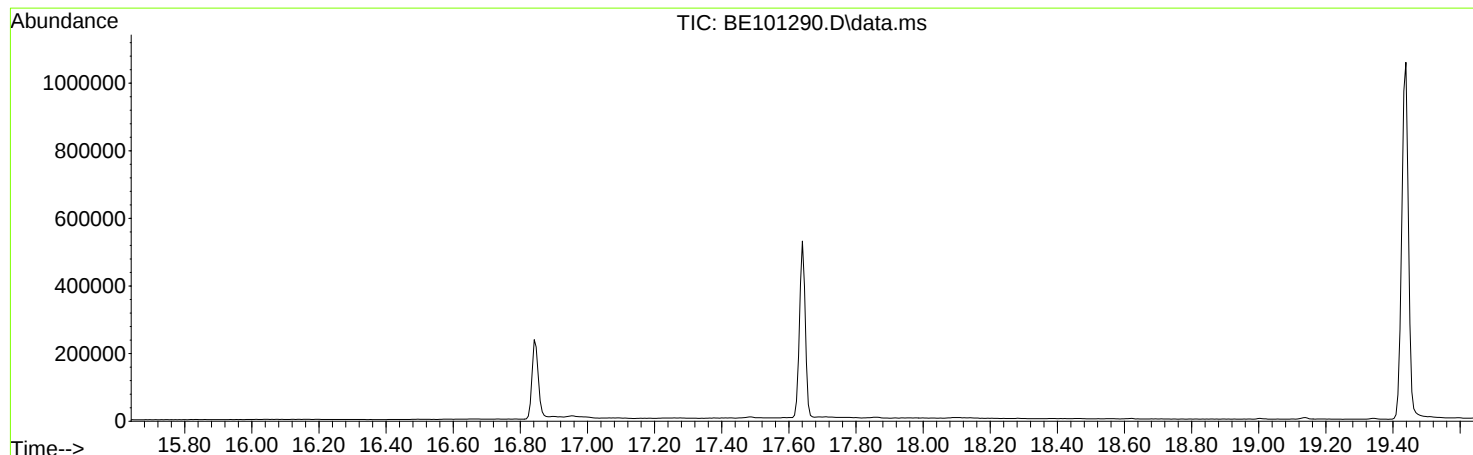

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	23568	PASS
68	69	0.00	2	1.0	218	PASS
69	198	0.00	100	43.6	21147	PASS
70	69	0.00	2	0.4	75	PASS
127	198	10	80	46.1	22358	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48520	PASS
199	198	5	9	6.8	3313	PASS
275	198	10	60	27.2	13213	PASS
365	198	1	100	3.3	1608	PASS
441	198	0.01	100	11.4	5518	PASS
442	442	50	100	100.0	34939	PASS
443	442	15	24	19.4	6776	PASS

Instrument :
BNA_E
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/13/2021	BNA_E	<u>BE101290.D</u>
Compound Name	Response	Retention Time
DDT	268775	20.66
DDD	2342	20.226
DDE	342	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2684	271459	0.99

Instrument :
BNA_E
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041321\
 Data File : BE101290.D
 Acq On : 13 Apr 2021 12:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 14 02:19:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 10:54:22 2021
 Response via : Initial Calibration

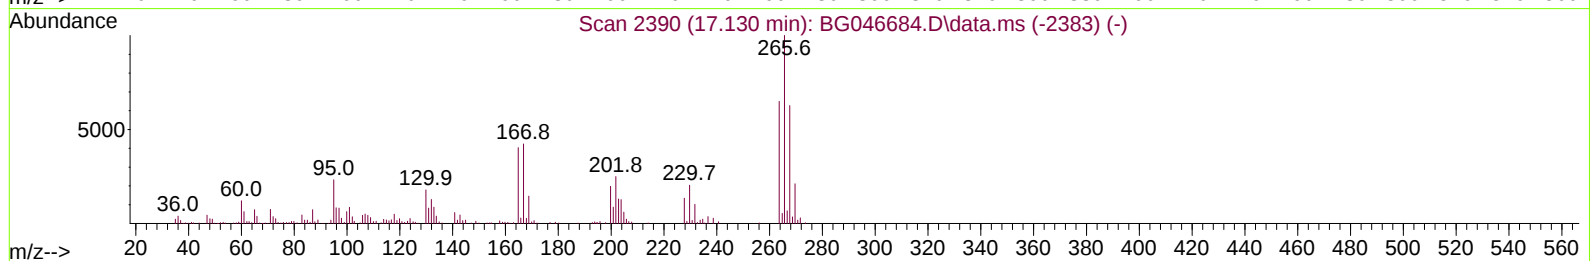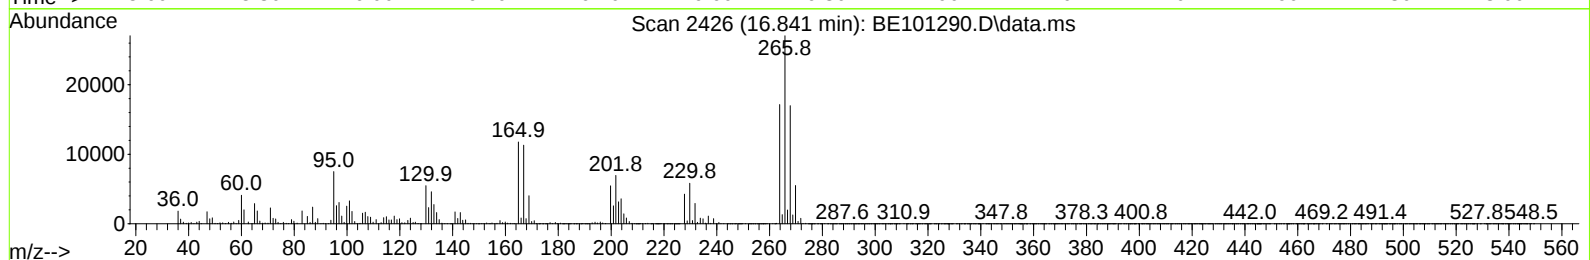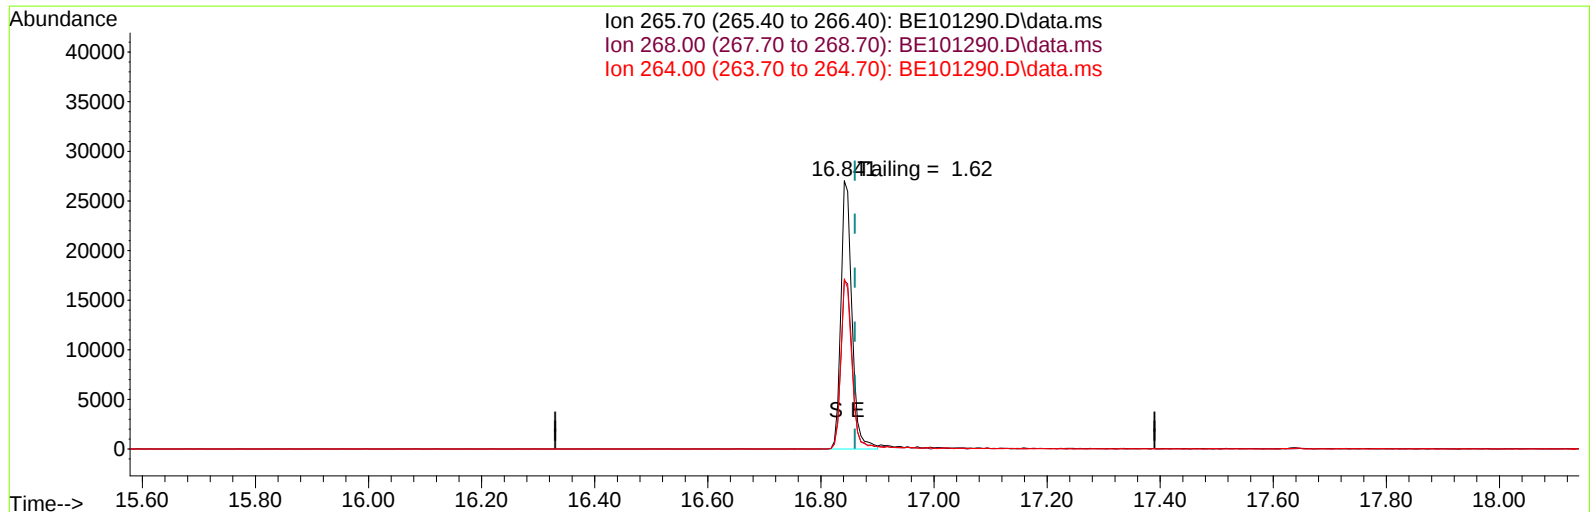

TIC: BE101290.D\data.ms

(70) Pentachlorophenol (C)

16.841min (-0.019) 311121.09 ng




response 36624

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.79
264.00	61.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041321\
Data File : BE101290.D
Acq On : 13 Apr 2021 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 14 02:19:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 10:54:22 2021
Response via : Initial Calibration

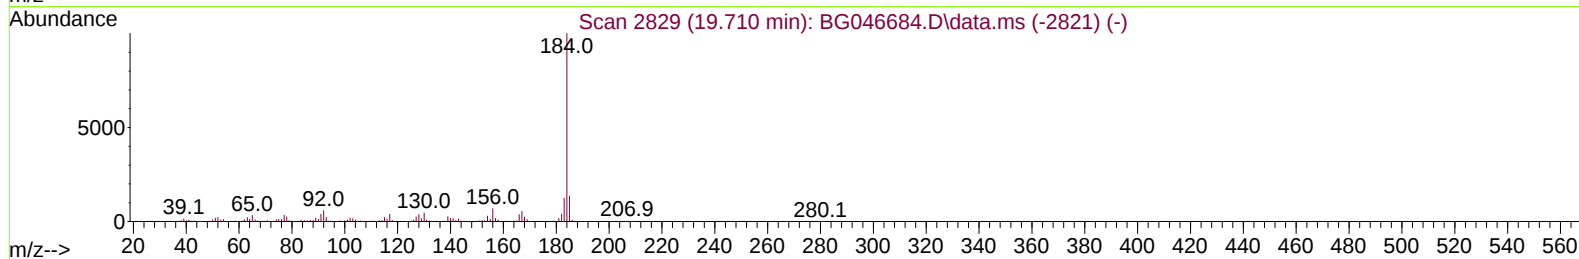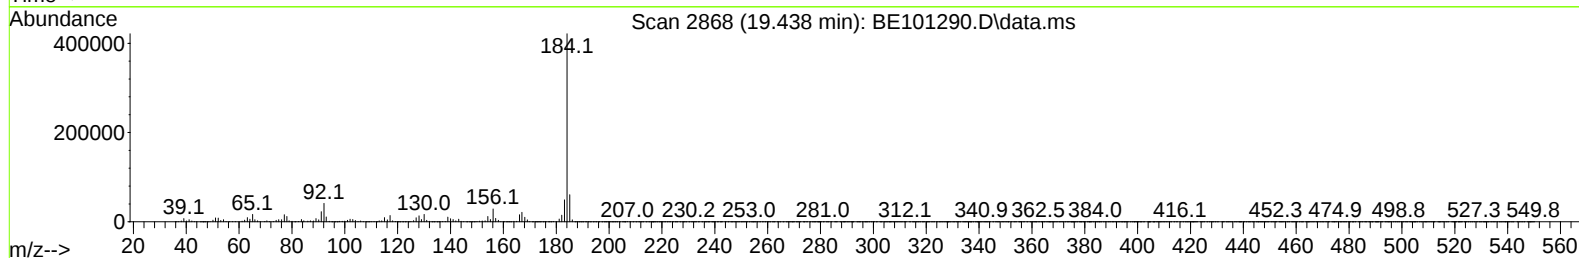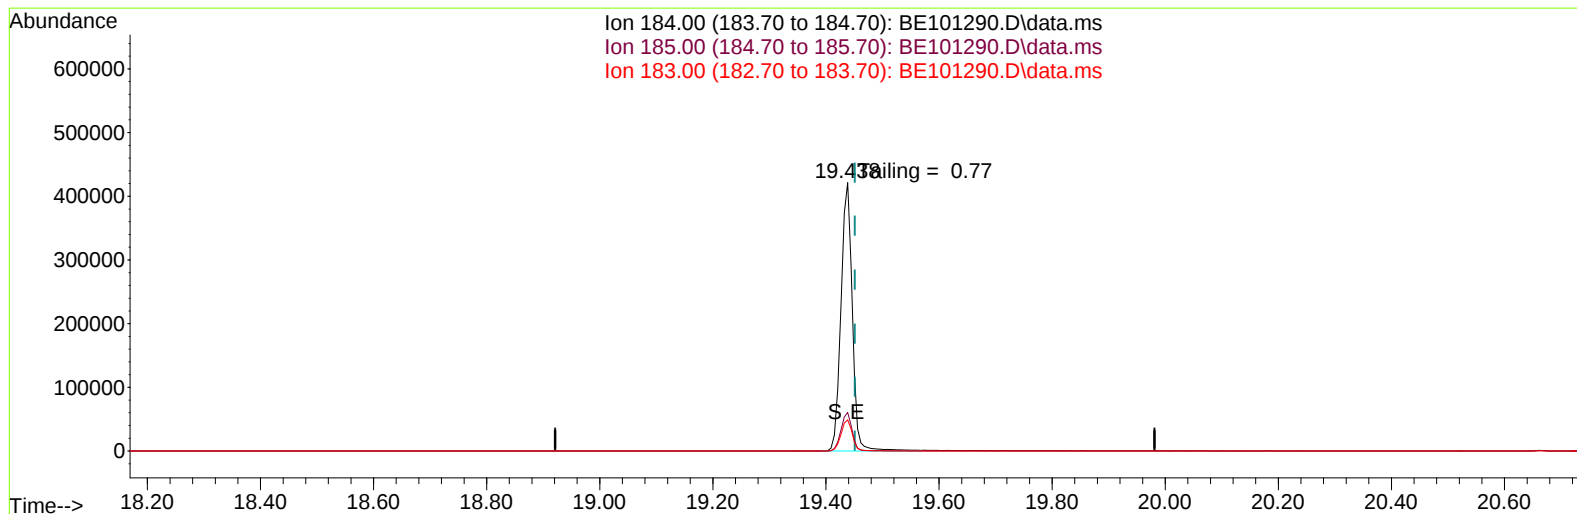

TIC: BE101290.D\data.ms

(77) Benzidine

19.438min (-0.013) 5011.04 ng

response 590683

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.64
0.00	0.00	0.00