
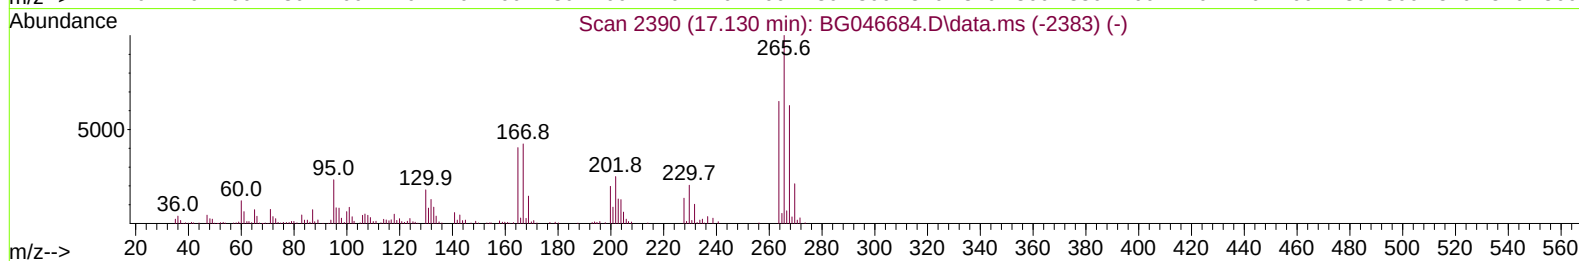
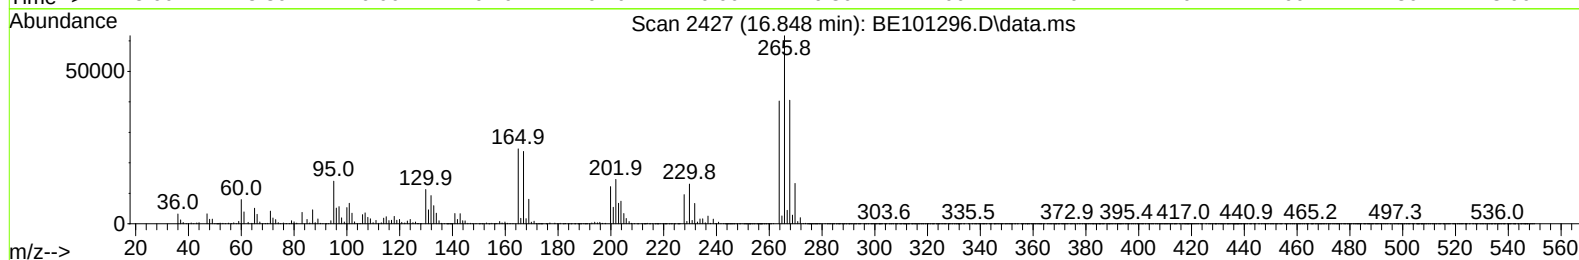


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041421\
 Data File : BE101296.D
 Acq On : 14 Apr 2021 9:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:44:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 04:44:12 2021
 Response via : Initial Calibration

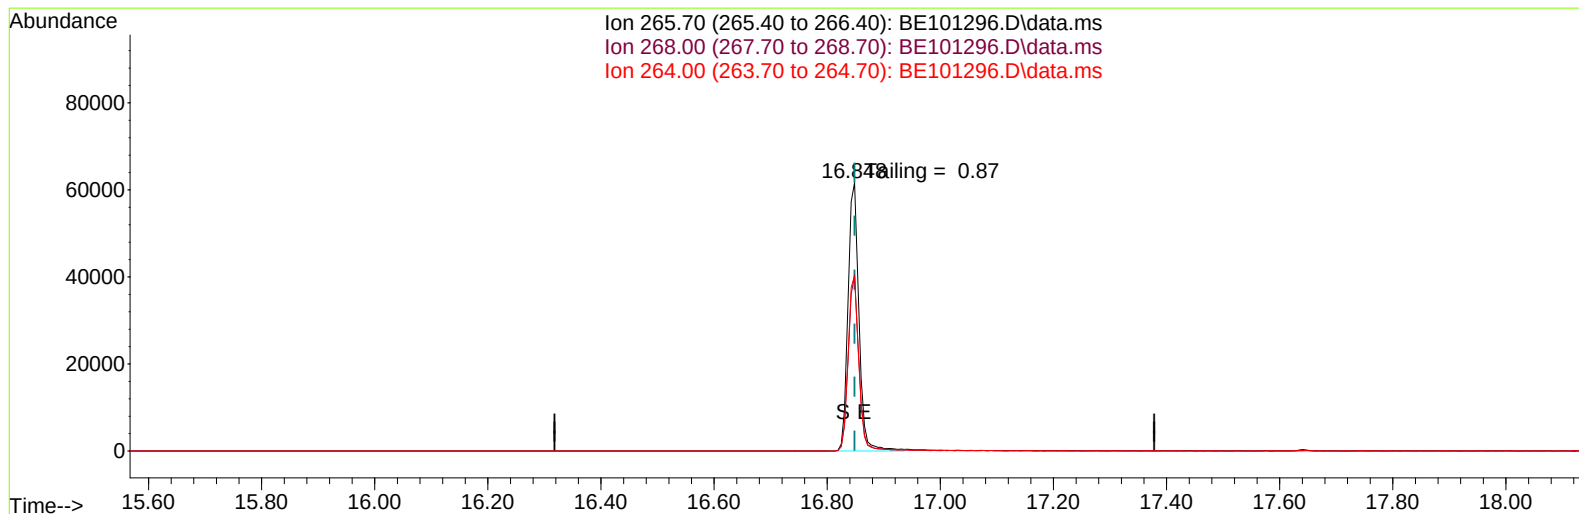

TIC: BE101296.D\data.ms

(70) Pentachlorophenol (C)




16.848min (0.000) 629240.07 ng

response 83948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.67
264.00	61.60	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041421\
 Data File : BE101296.D
 Acq On : 14 Apr 2021 9:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 04:44:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 04:44:12 2021
 Response via : Initial Calibration

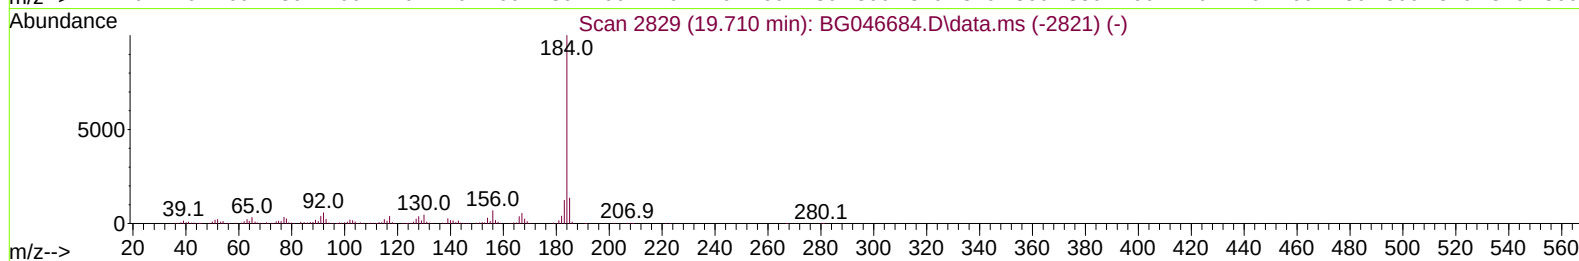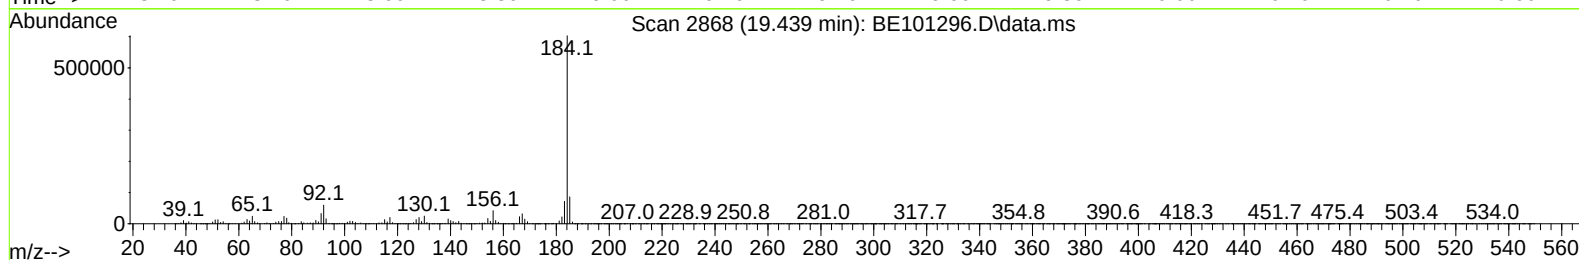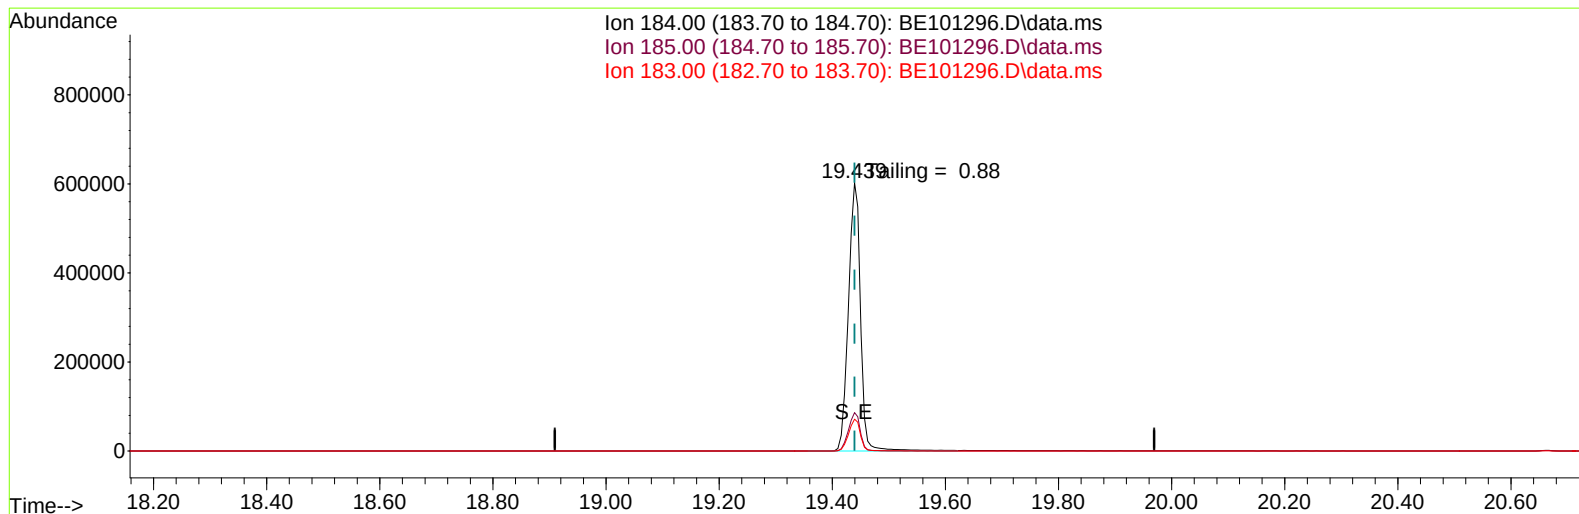

TIC: BE101296.D\data.ms

(77) Benzidine**19.439min (0.000) 4692.30 ng****response 897503**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	11.90
0.00	0.00	0.00