
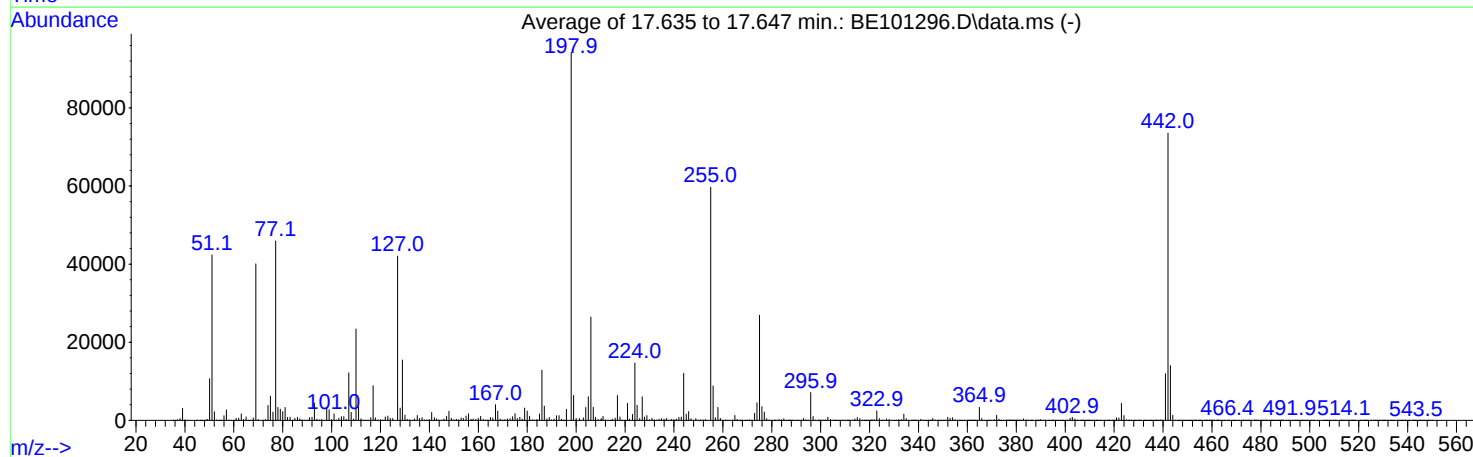


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041421\
 Data File : BE101296.D
 Acq On : 14 Apr 2021 9:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE041221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 12 18:02:55 2021

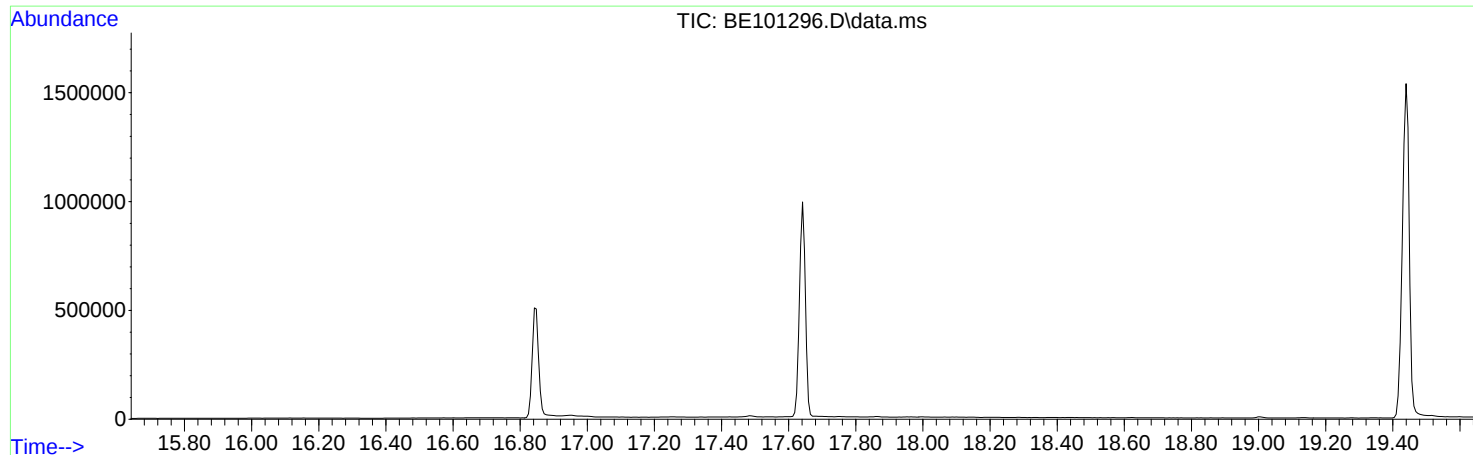

AutoFind: Scans 2561, 2562, 2563; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	42375	PASS
68	69	0.00	2	1.6	638	PASS
69	198	0.00	100	42.5	40069	PASS
70	69	0.00	2	0.5	208	PASS
127	198	10	80	44.7	42094	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94189	PASS
199	198	5	9	6.8	6379	PASS
275	198	10	60	28.6	26924	PASS
365	198	1	100	3.6	3359	PASS
441	198	0.01	100	12.7	11942	PASS
442	442	50	100	100.0	73531	PASS
443	442	15	24	19.1	14009	PASS

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2021	BNA_E	<u>BE101296.D</u>
Compound Name	Response	Retention Time
DDT	432768	20.661
DDD	3202	20.227
DDE	520	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3722	436490	0.85

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041421\
 Data File : BE101296.D
 Acq On : 14 Apr 2021 9:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Quant Time: Apr 22 04:44:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 04:44:12 2021
 Response via : Initial Calibration

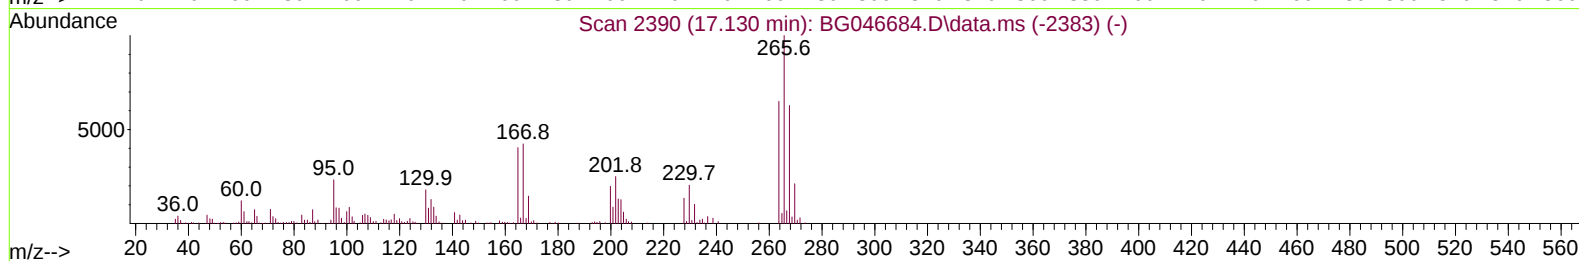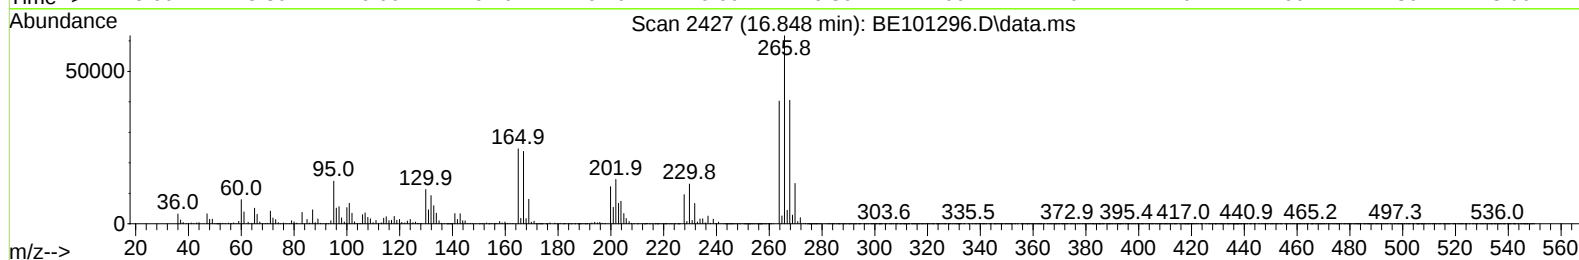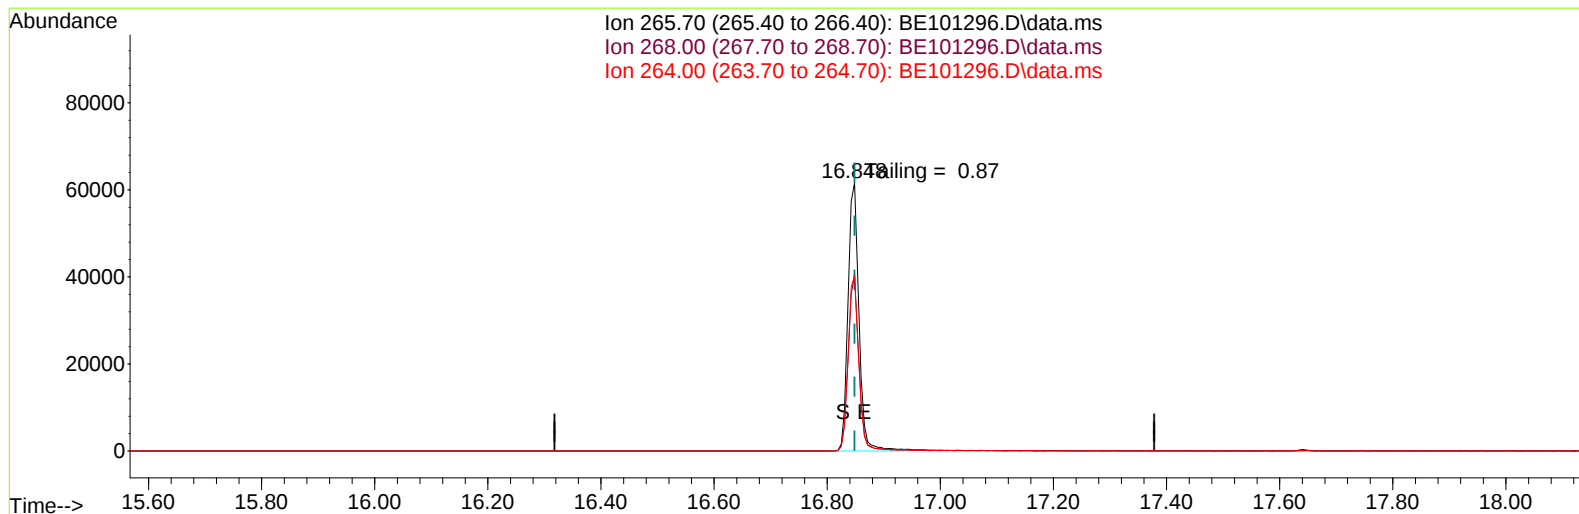

TIC: BE101296.D\data.ms

(70) Pentachlorophenol (C)

16.848min (0.000) 629240.07 ng




response 83948

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.67
264.00	61.60	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041421\
Data File : BE101296.D
Acq On : 14 Apr 2021 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 22 04:44:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 04:44:12 2021
Response via : Initial Calibration

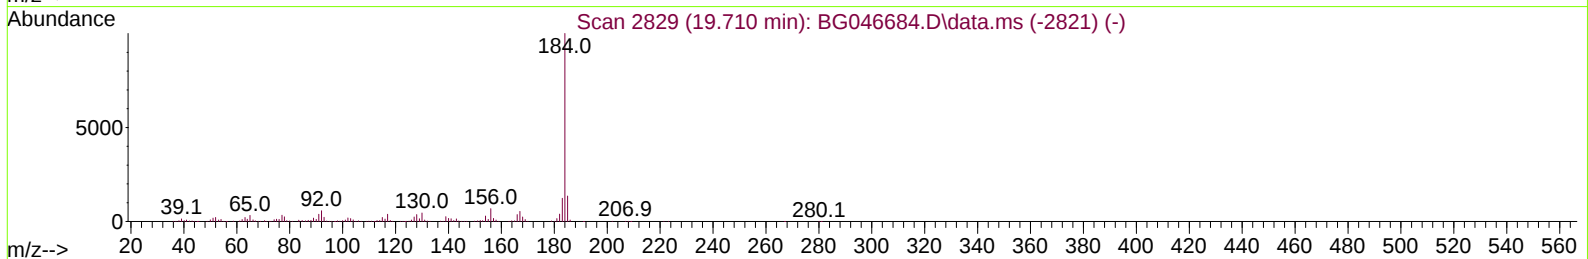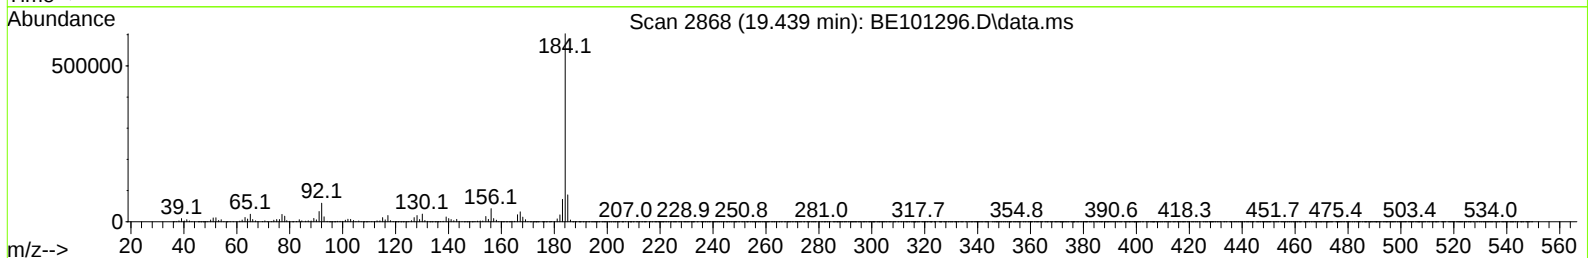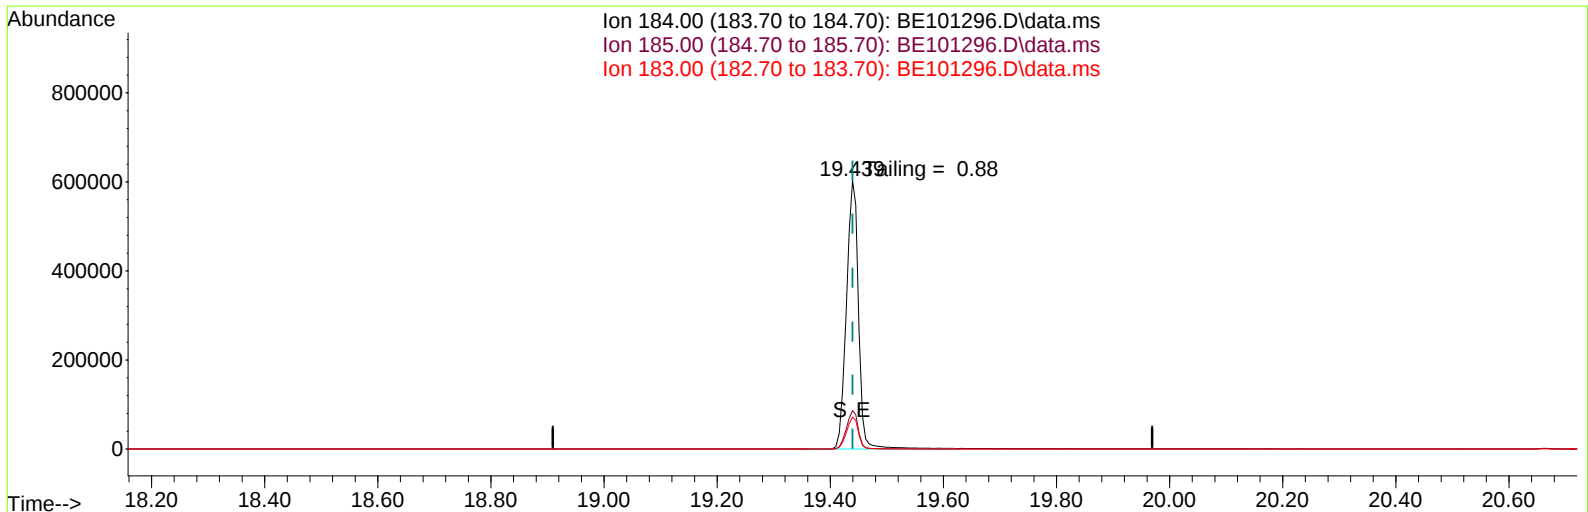

TIC: BE101296.D\data.ms

(77) Benzidine

19.439min (0.000) 4692.30 ng

response 897503

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	11.90
0.00	0.00	0.00