

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
 Data File : BE096002.D
 Acq On : 16 Apr 2018 10:37
 Operator : SJ/JU
 Sample : PB108199BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 16 13:04:14 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 16 13:04:01 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	1856	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	4882	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2925	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.78	188	525618	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.77
20) Perylene-d12	24.23	264	404246	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	2711	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.94	166	617	0.050	ng/ul#	Ovalue 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
Data File : BE096002.D
Acq On : 16 Apr 2018 10:37
Operator : SJ/JU
Sample : PB108199BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 16 13:04:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 16 13:04:01 2018
Response via : Initial Calibration

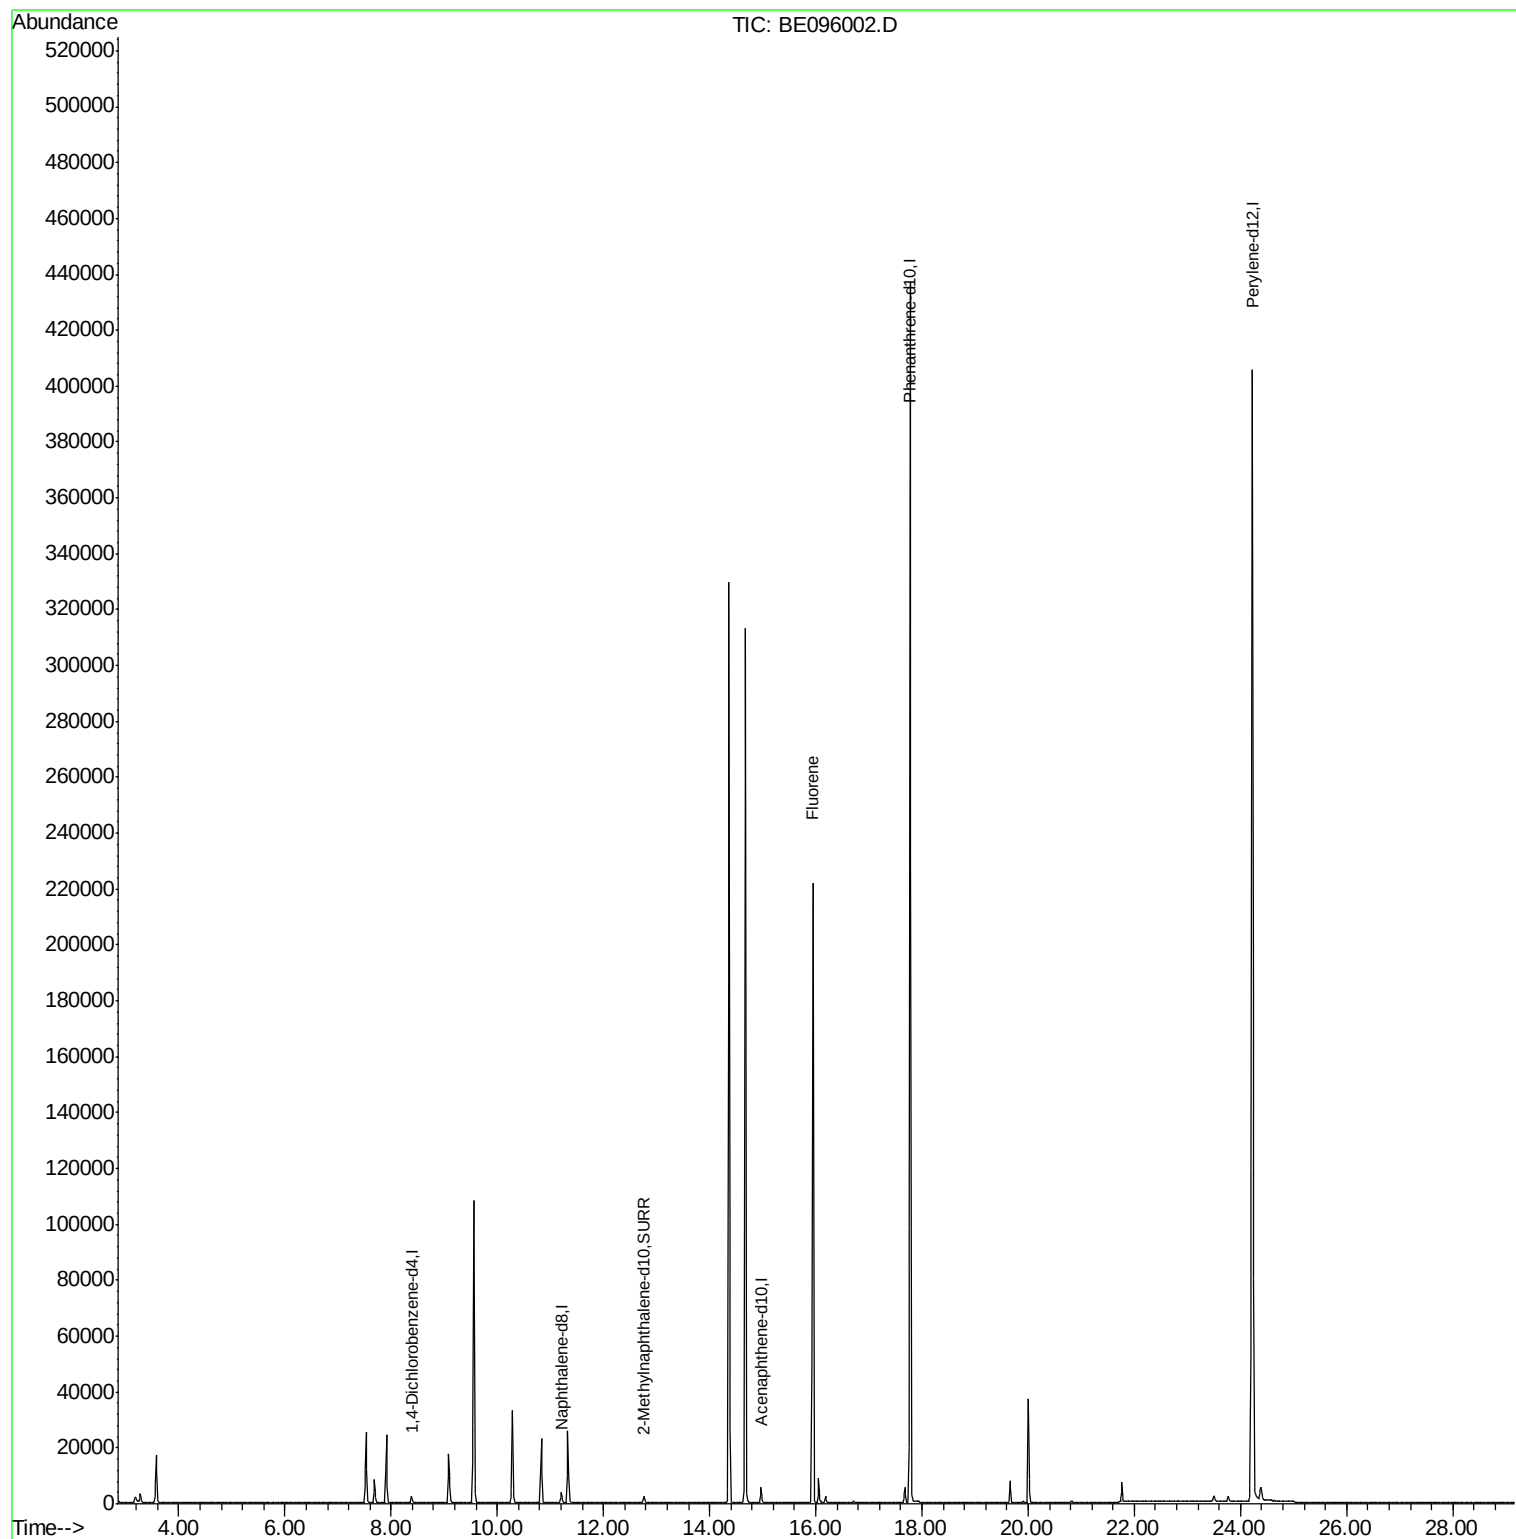

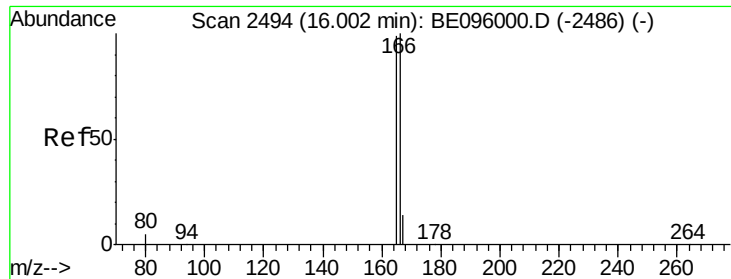

#9

Fluorene

Concen: 0.050 ng/ul

RT: 15.94 min Scan# 2484

Delta R.T. -0.06 min

Lab File: BE096002.D

Acq: 16 Apr 2018 10:37

Instrument :

BNA_E

ClientSampleId :

Tot Ion:166 Resp: 617

Ion Ratio Lower Upper

166 100

165 11.5 73.4 110.2#

167 37.2 14.6 22.0#

