

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
 Data File : BE096007.D
 Acq On : 16 Apr 2018 14:12
 Operator : SJ/JU
 Sample : J2313-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Apr 16 17:53:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 03:47:21 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1958	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5441	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3346	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.78	188	560649	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.77
20) Perylene-d12	24.22	264	472133	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3195	0.31	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	11.25	128	323	0.021	ng/ul#	46
8) Acenaphthene	15.02	153	1387	0.111	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
Data File : BE096007.D
Acq On : 16 Apr 2018 14:12
Operator : SJ/JU
Sample : J2313-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Apr 16 17:53:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 03:47:21 2018
Response via : Initial Calibration

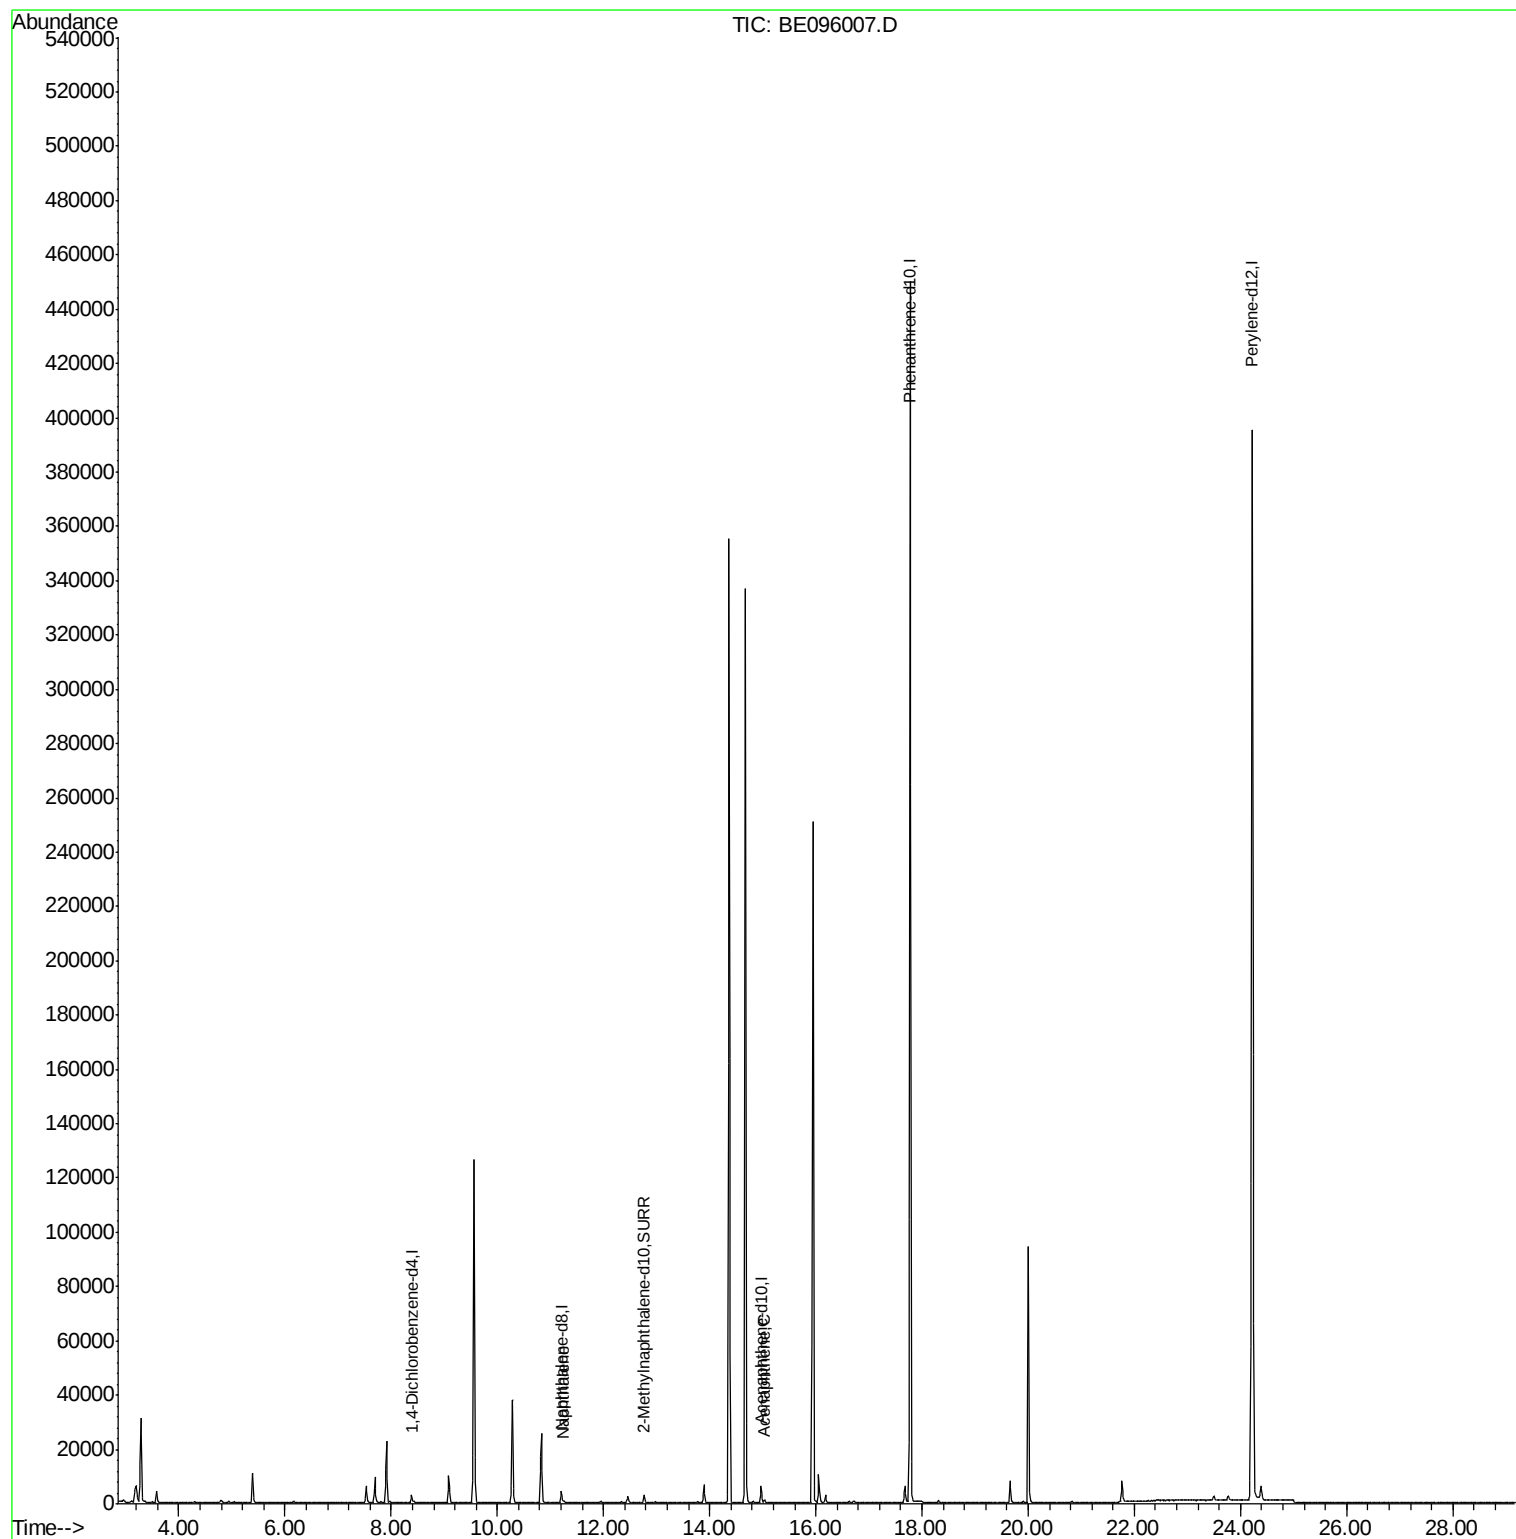

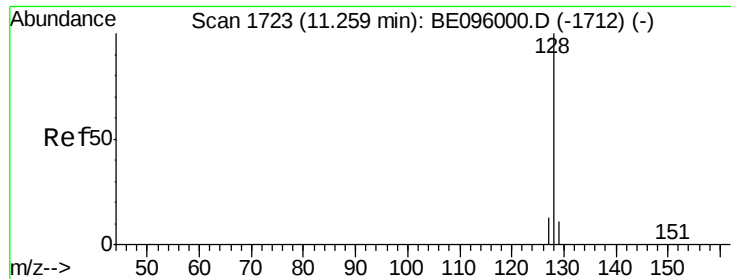

#3

Naphthalene

Concen: 0.021 ng/ul

RT: 11.25 min Scan# 1722

Delta R.T. -0.01 min


Lab File: BE096007.D

Acq: 16 Apr 2018 14:12

Instrument :

BNA_E

ClientSampleId :

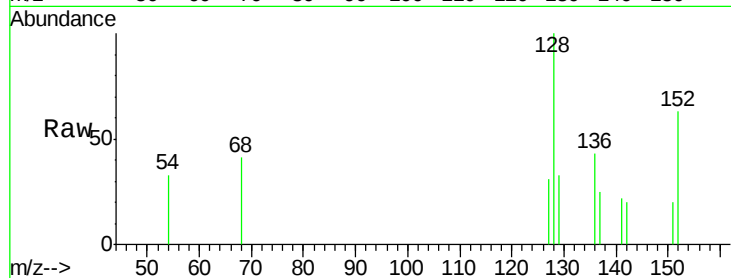




Tot Ion:128 Resp: 323

Ion Ratio Lower Upper

128 100

129 32.8 11.3 16.9#

127 30.6 4.0 6.0#

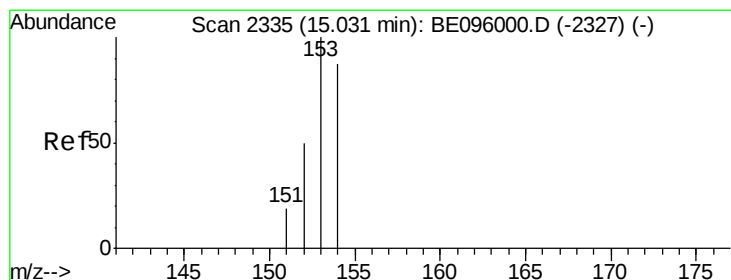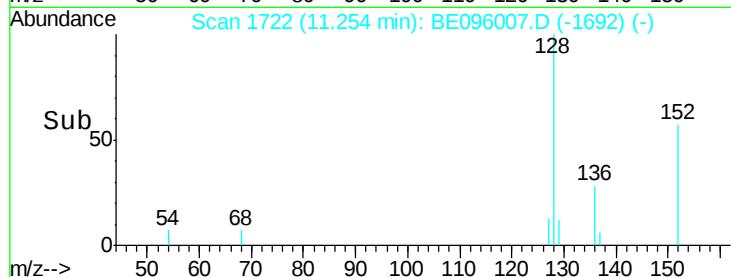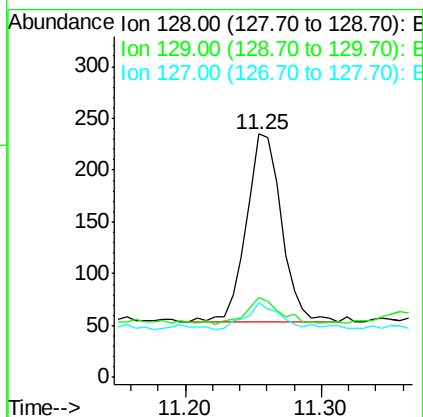

#8

Acenaphthene

Concen: 0.111 ng/ul

RT: 15.02 min Scan# 2333

Delta R.T. -0.01 min

Lab File: BE096007.D

Acq: 16 Apr 2018 14:12

Tgt Ion:153 Resp: 1387

Ion Ratio Lower Upper

153 100

152 6.6 36.0 54.0#

154 13.7 72.0 108.0#

