

Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
 Data File : BE096010.D
 Acq On : 16 Apr 2018 15:59
 Operator : SJ/JU
 Sample : J2313-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1A43

Manual Integrations
 APPROVED

Sohil
 4/17/2018 4:51:39 PM

Quant Time: Apr 16 18:48:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 10 03:47:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.39	152	1909	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5310	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3262	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6958m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	7122m	0.40	ng/ul	0.00
20) Perylene-d12	24.39	264	9117	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3262	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	8991m	0.31	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.26	128	357	0.024	ng/ul#	56
8) Acenaphthene	15.02	153	996	0.082	ng/ul#	29

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE041618\
Data File : BE096010.D
Acq On : 16 Apr 2018 15:59
Operator : SJ/JU
Sample : J2313-08
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F1A43

Manual Integrations
APPROVED

Sohil
4/17/2018 4:51:39 PM

Quant Time: Apr 16 18:48:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 10 03:47:21 2018
Response via : Initial Calibration

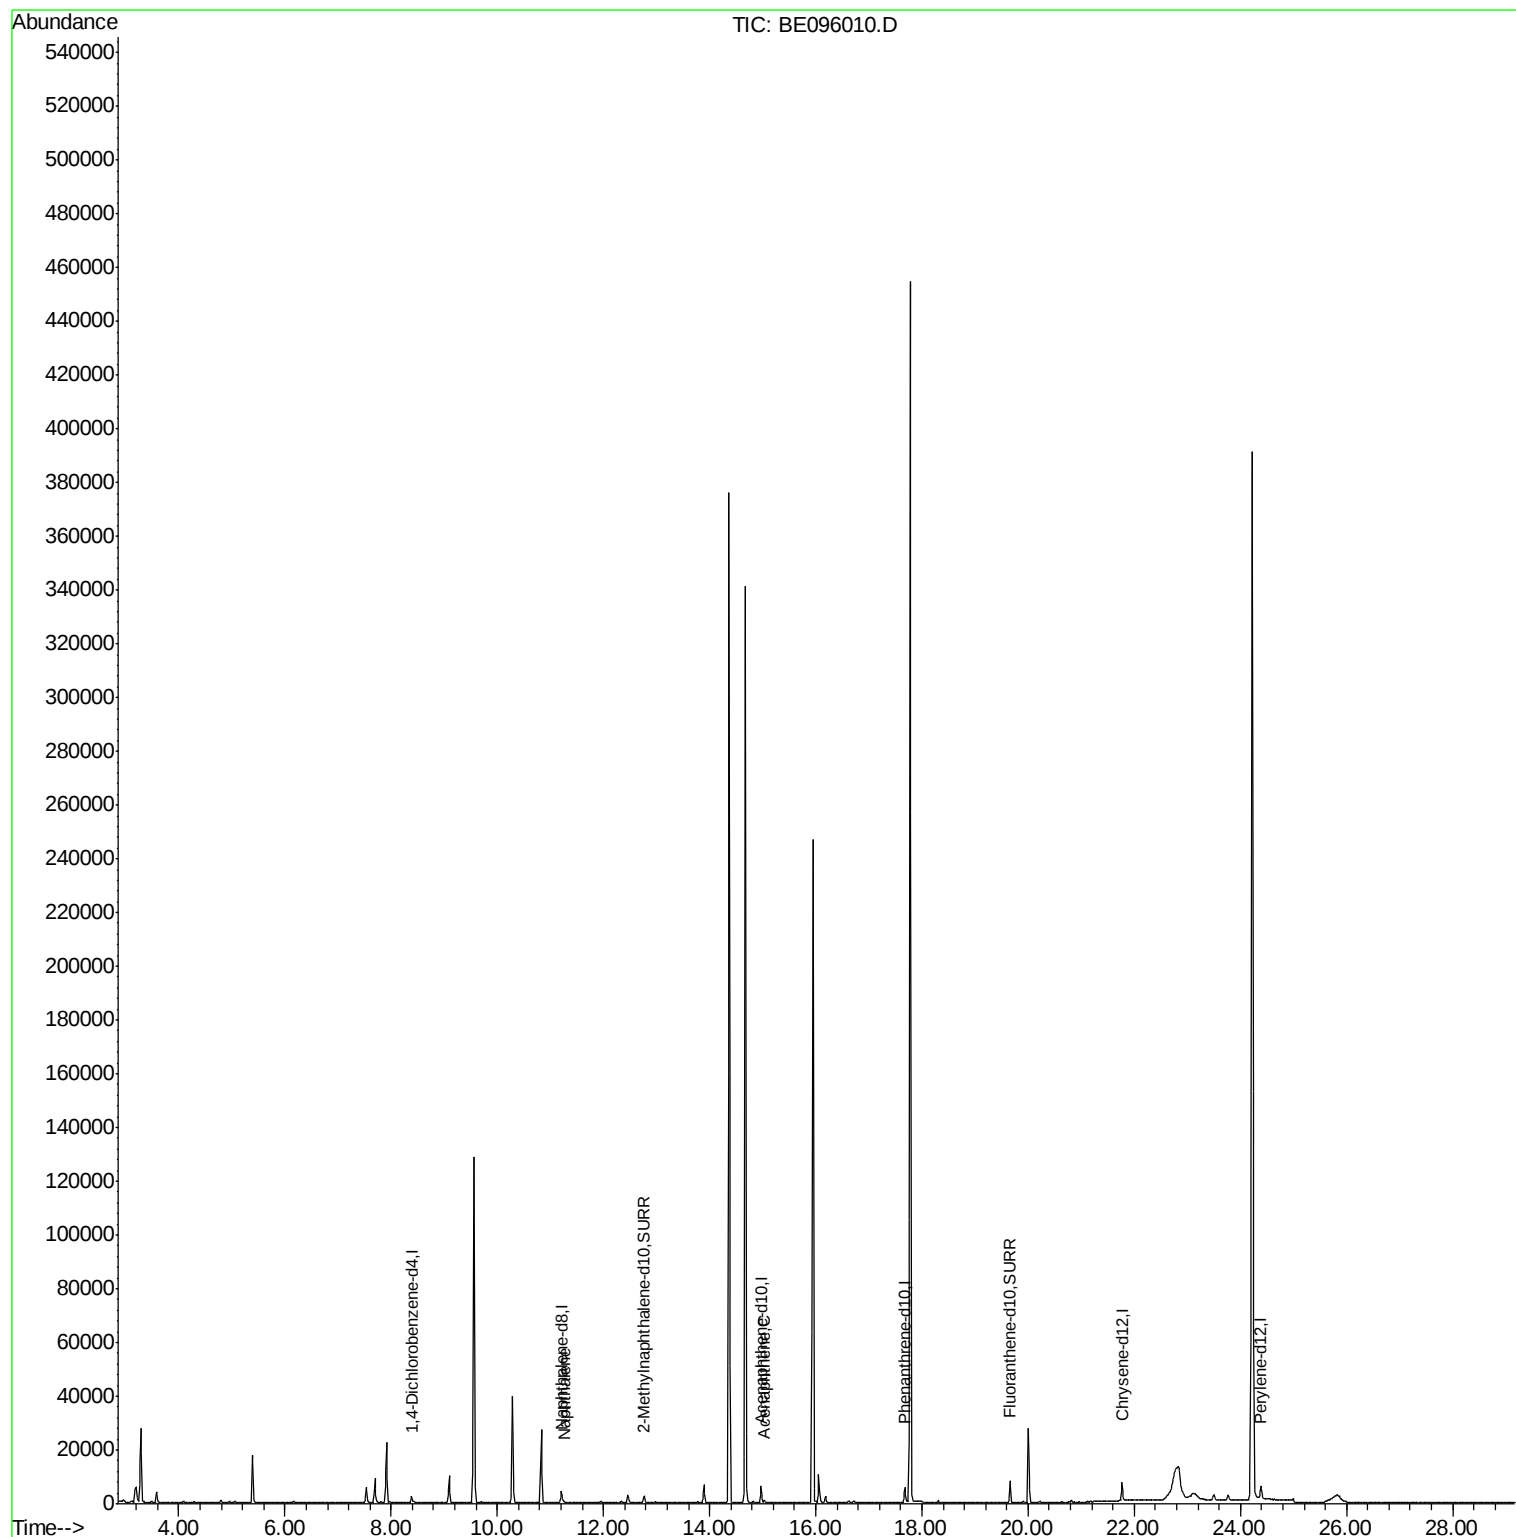

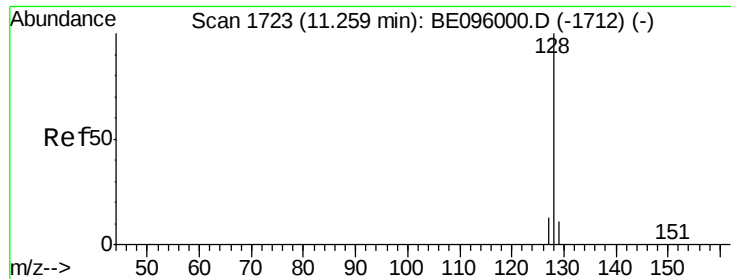

#3

Naphthalene

Concen: 0.024 ng/ul

RT: 11.26 min Scan# 1722

Delta R.T. -0.00 min

Lab File: BE096010.D

Acq: 16 Apr 2018 15:59

Instrument :

BNA_E





ClientSampleId :

F1A43

Tot Ion:	128	Resp:	357
Ion Ratio	Lower	Upper	
128	100		
129	27.8	11.3	16.9#
127	29.3	4.0	6.0#

Manual Integrations
APPROVED

Sohil
4/17/2018 4:51:39 PM

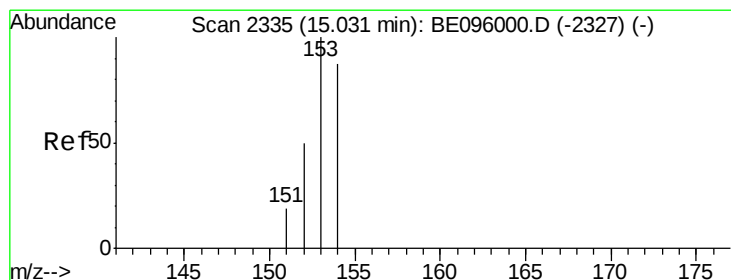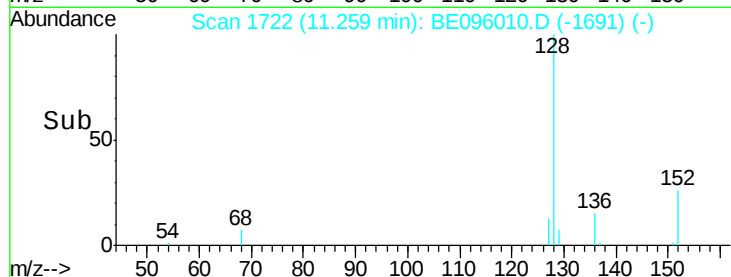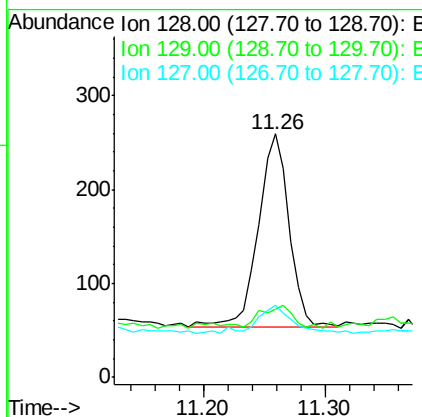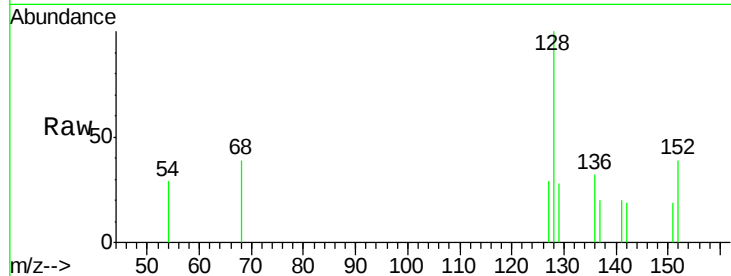

#8

Acenaphthene

Concen: 0.082 ng/ul

RT: 15.02 min Scan# 2333

Delta R.T. -0.01 min

Lab File: BE096010.D

Acq: 16 Apr 2018 15:59

Tgt Ion:	153	Resp:	996
Ion Ratio	Lower	Upper	
153	100		
152	8.8	36.0	54.0#
154	15.8	72.0	108.0#

