
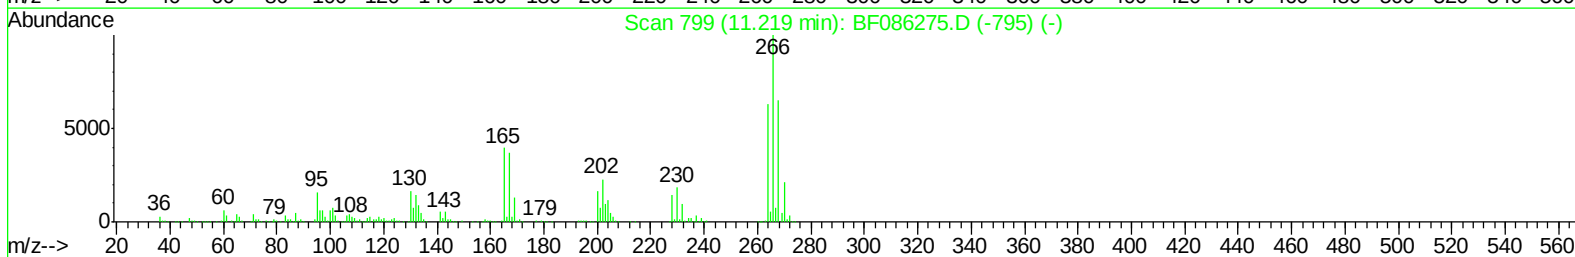
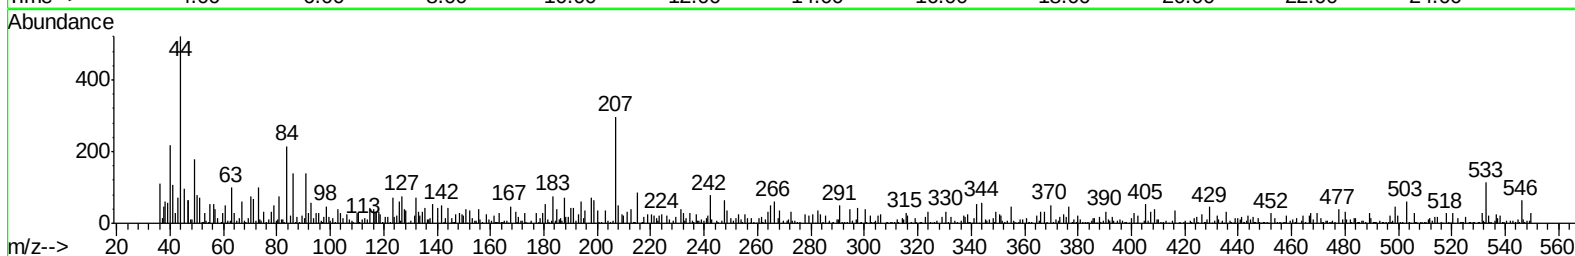


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE041816\
Data File : BE091668.D
Acq On : 18 Apr 2016 17:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 05:52:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 15 15:56:31 2016
Response via : Initial Calibration

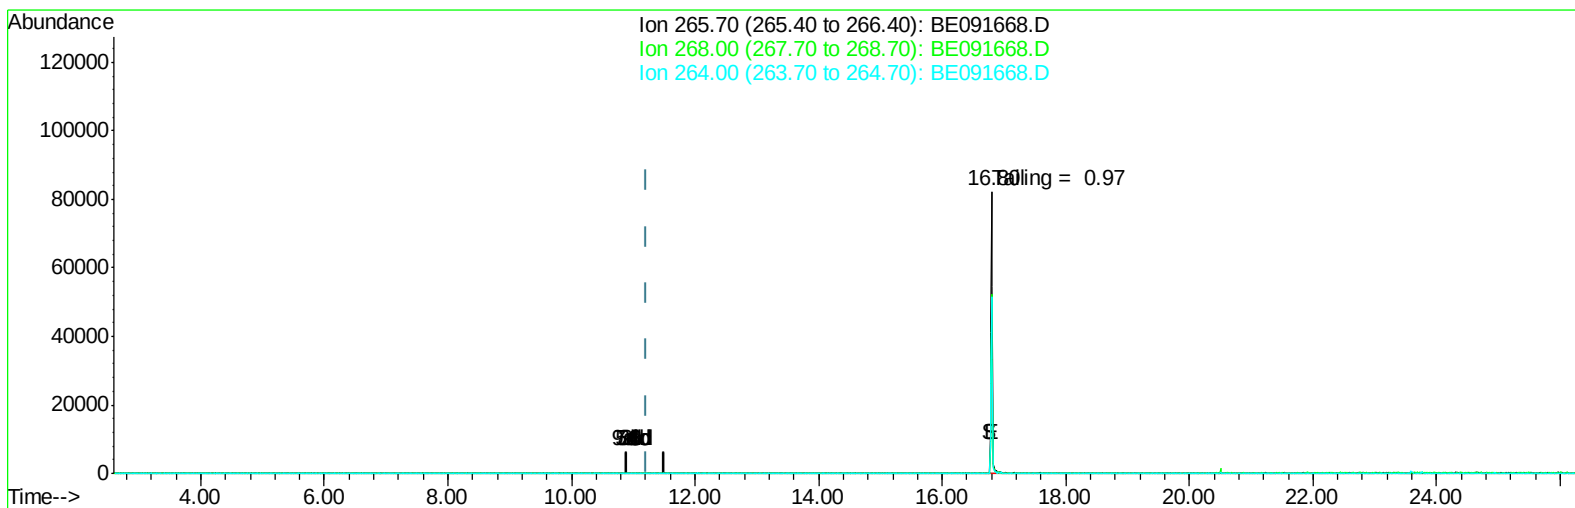

TIC: BE091668.D

(69) Pentachlorophenol (C)




11.043min (-0.176) 148.32ng

response 65

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	58.33
264.00	64.10	56.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE041816\
 Data File : BE091668.D
 Acq On : 18 Apr 2016 17:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 19 05:52:11 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 15 15:56:31 2016
 Response via : Initial Calibration

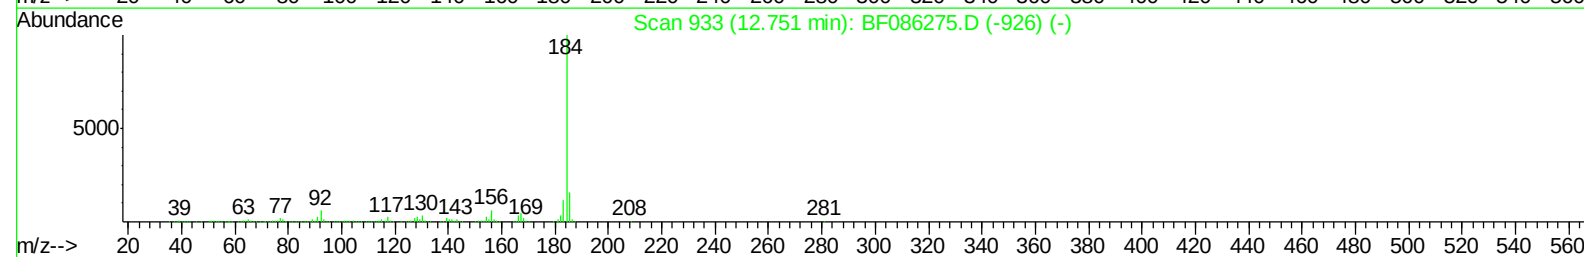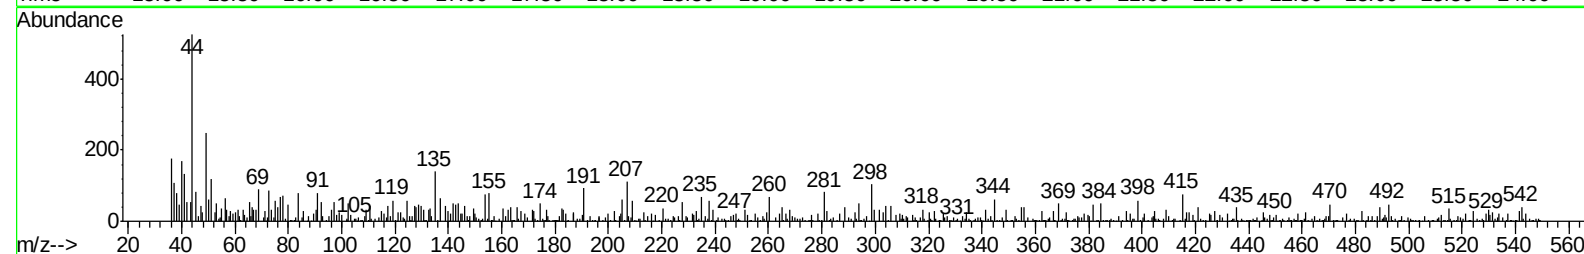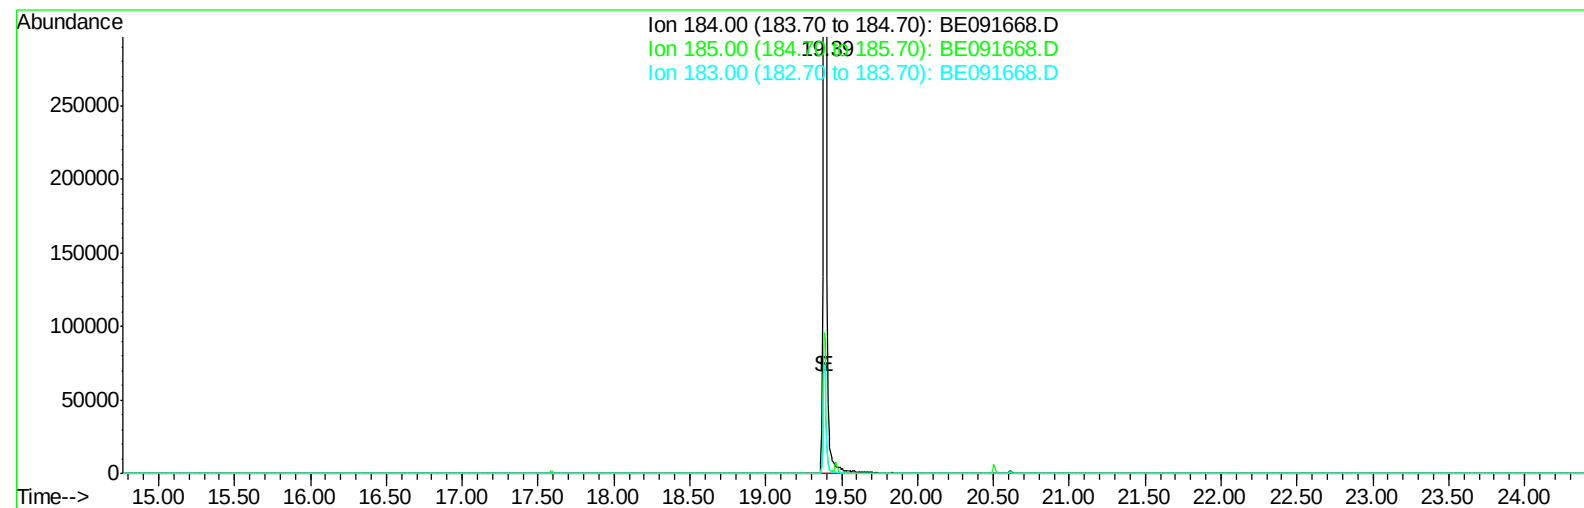

TIC: BE091668.D

(76) Benzidine

12.500min (-0.251) 12.89ng

response 13

Ion	Exp%	Act%
184.00	100	100
185.00	17.70	13.04#
183.00	12.20	143.48#
0.00	0.00	0.00