


Data Path : Z:\HPCHEM1\BNA E\Data\BE041816\
 Data File : BE091658.D
 Acq On : 18 Apr 2016 10:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 18 17:20:40 2016

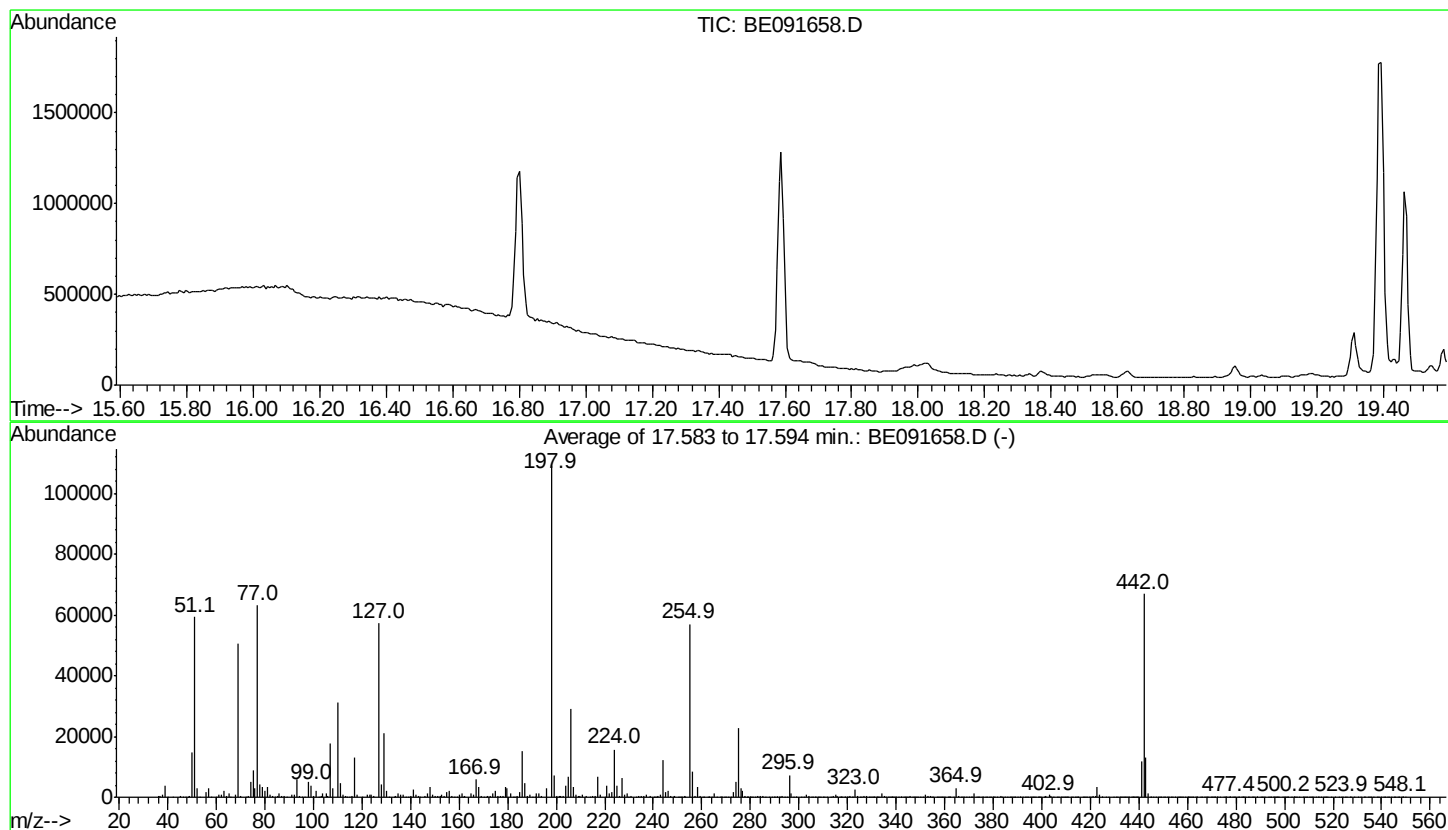

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.4	59371	PASS
68	69	0.00	2	1.8	931	PASS
69	198	0.00	100	46.4	50707	PASS
70	69	0.00	2	0.8	425	PASS
127	198	10	80	52.4	57232	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109215	PASS
199	198	5	9	6.5	7094	PASS
275	198	10	60	21.0	22981	PASS
365	198	1	100	2.9	3171	PASS
441	442	0.01	24	17.7	11882	PASS
442	198	50	100	61.4	67010	PASS
443	442	15	24	19.4	13015	PASS