


Data Path : Z:\HPCHEM1\BNA E\DATA\BE041816\
 Data File : BE091668.D
 Acq On : 18 Apr 2016 17:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE041816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 18 17:20:40 2016

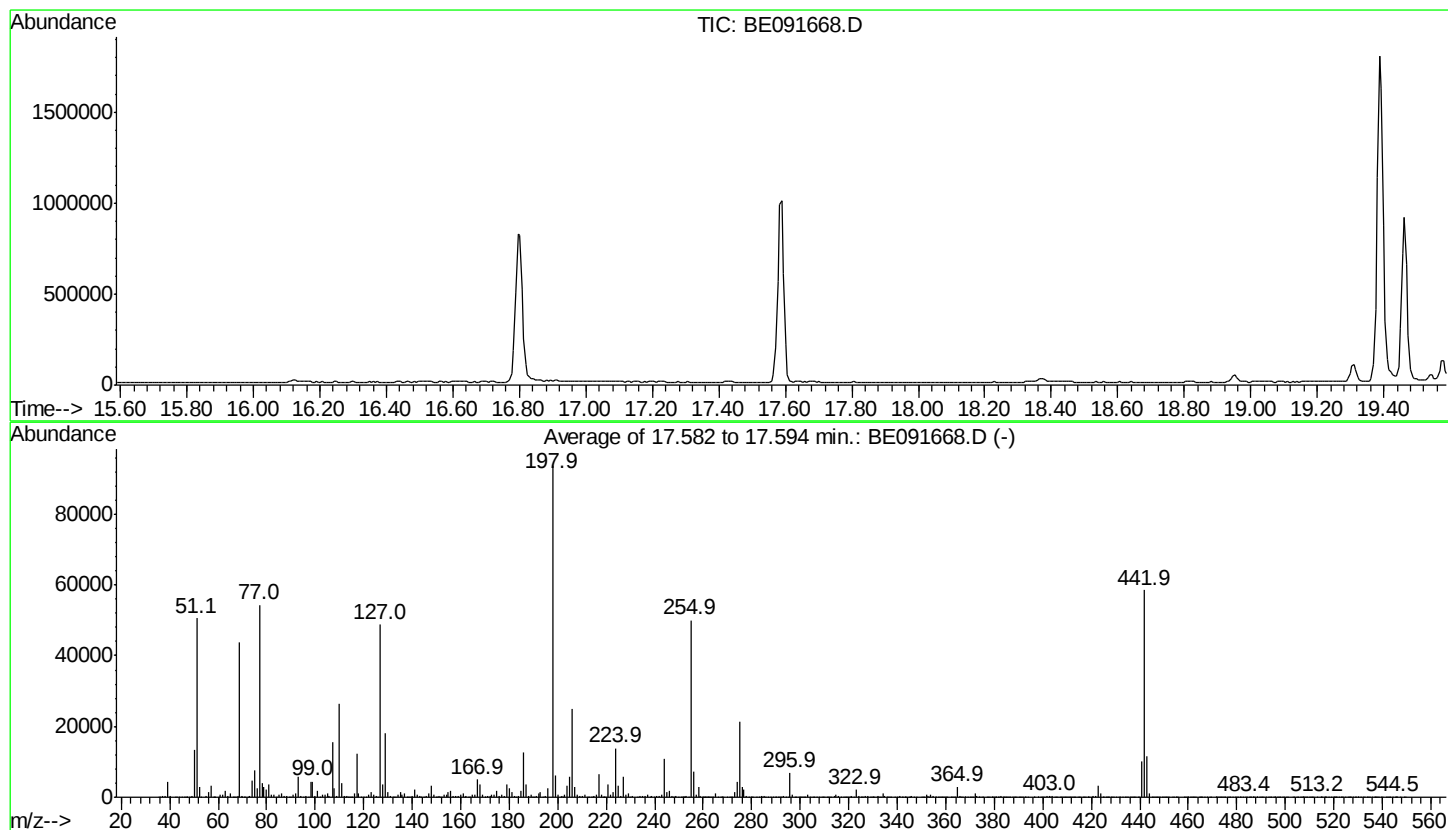

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.9	50550	PASS
68	69	0.00	2	1.0	436	PASS
69	198	0.00	100	46.6	43689	PASS
70	69	0.00	2	0.5	208	PASS
127	198	10	80	52.0	48684	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93707	PASS
199	198	5	9	6.6	6183	PASS
275	198	10	60	22.8	21350	PASS
365	198	1	100	3.1	2907	PASS
441	442	0.01	24	17.3	10137	PASS
442	198	50	100	62.4	58495	PASS
443	442	15	24	19.7	11513	PASS