
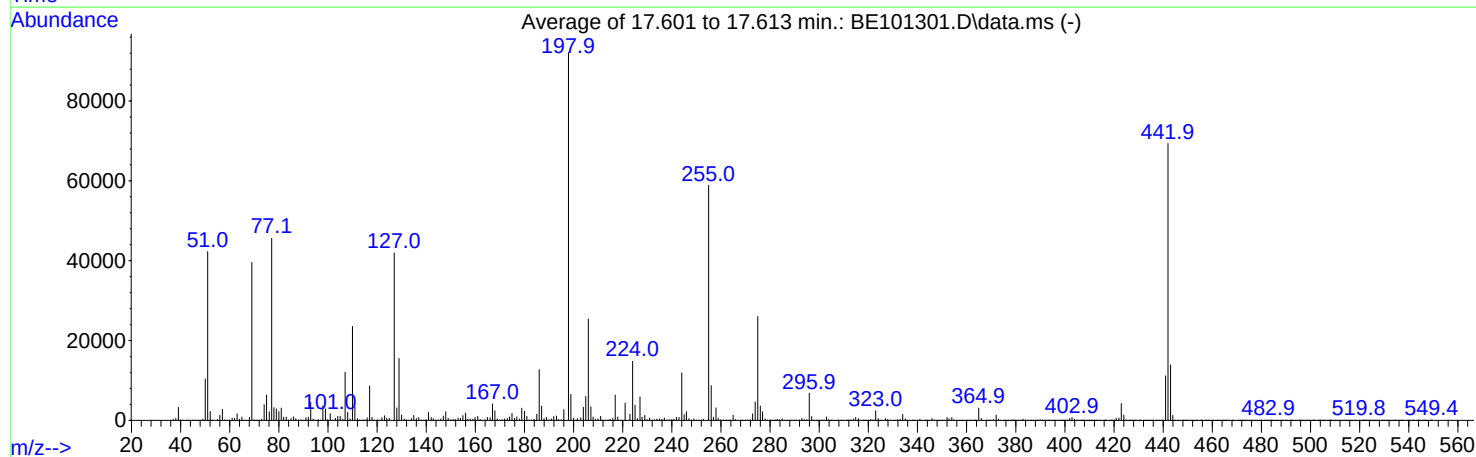


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041921\
 Data File : BE101301.D
 Acq On : 19 Apr 2021 13:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE041921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 19 18:59:35 2021

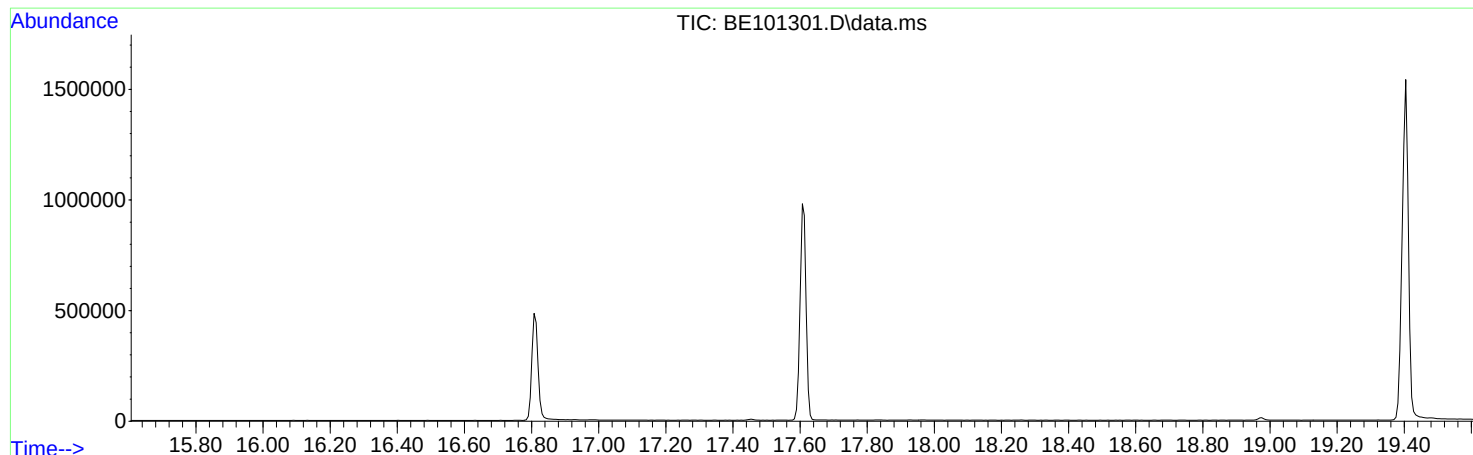

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	42309	PASS
68	69	0.00	2	1.8	706	PASS
69	198	0.00	100	42.9	39574	PASS
70	69	0.00	2	0.4	176	PASS
127	198	10	80	45.5	41920	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	92157	PASS
199	198	5	9	7.1	6527	PASS
275	198	10	60	28.2	26008	PASS
365	198	1	100	3.3	3066	PASS
441	198	0.01	100	12.1	11140	PASS
442	442	50	100	100.0	69379	PASS
443	442	15	24	20.0	13870	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/19/2021	BNA_E	<u>BE101301.D</u>
Compound Name	Response	Retention Time
DDT	432223	20.633
DDD	1514	20.245
DDE	425	19.687
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1939	434162	0.45

Instrument :
BNA_E
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041921\
Data File : BE101301.D
Acq On : 19 Apr 2021 13:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 21 06:37:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 06:36:00 2021
Response via : Initial Calibration

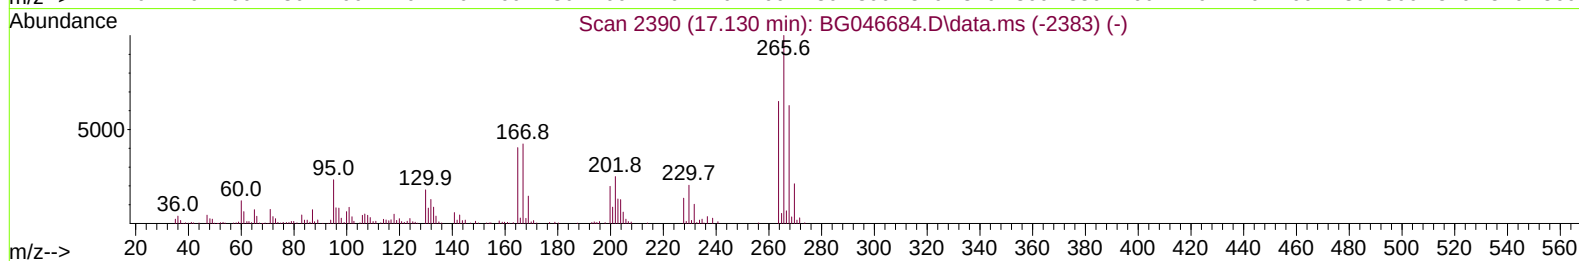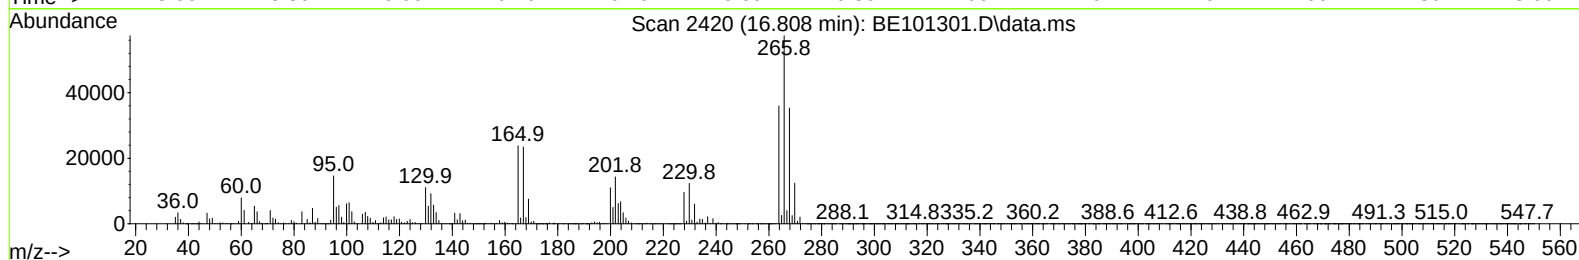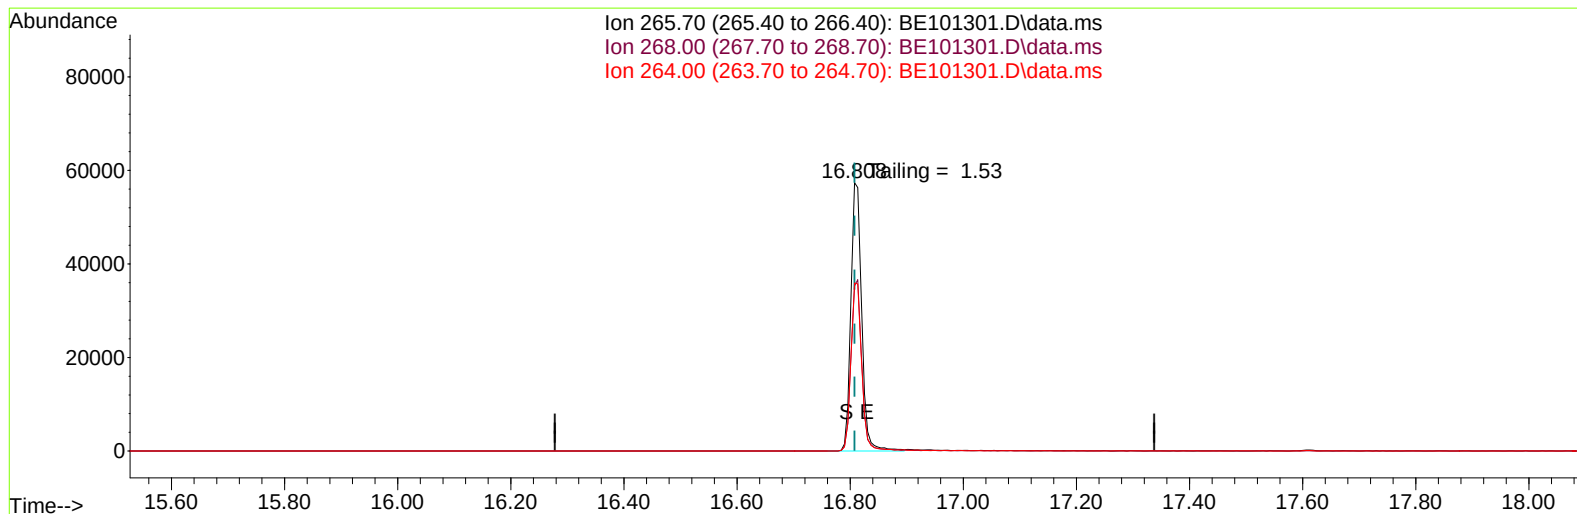

TIC: BE101301.D\data.ms

(70) Pentachlorophenol (C)

16.808min (0.000) 446358.49 ng




response 77064

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.51
264.00	61.60	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE041921\
Data File : BE101301.D
Acq On : 19 Apr 2021 13:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Apr 21 06:37:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 21 06:36:00 2021
Response via : Initial Calibration

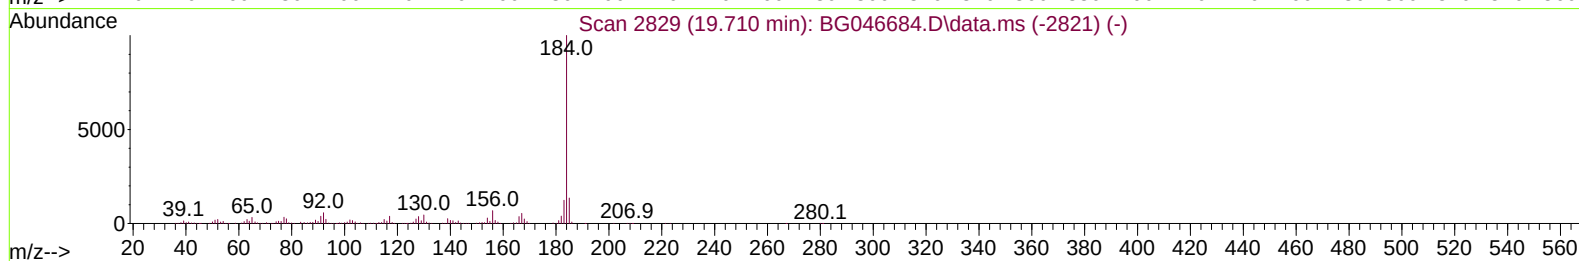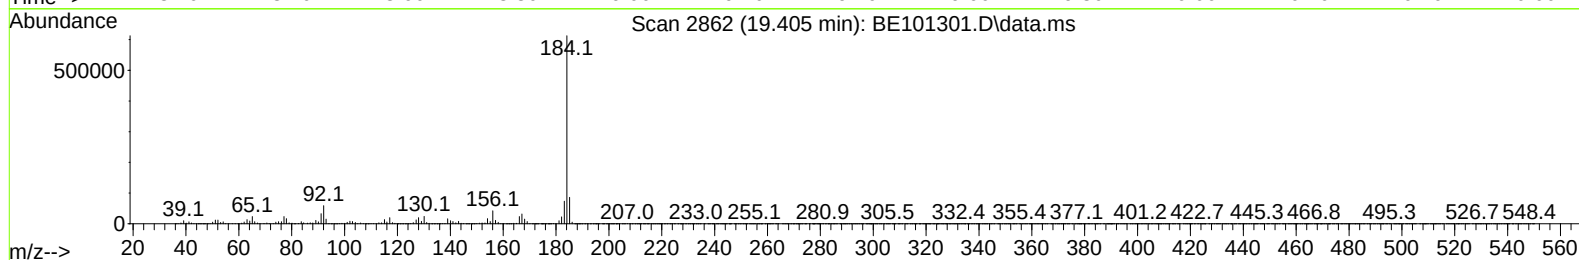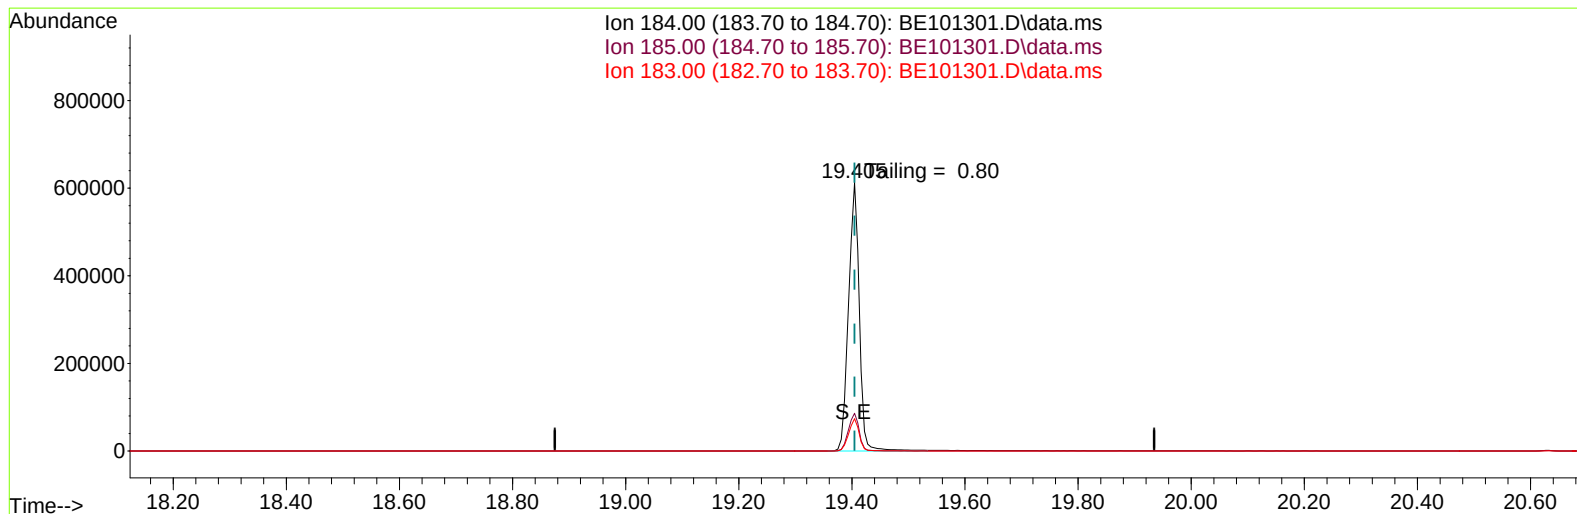

TIC: BE101301.D\data.ms

(77) Benzidine

19.405min (0.000) 4179.94 ng

response 812774

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.07
183.00	13.20	12.04
0.00	0.00	0.00