


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042016\
 Data File : BE091680.D
 Acq On : 20 Apr 2016 10:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 20 18:55:38 2016

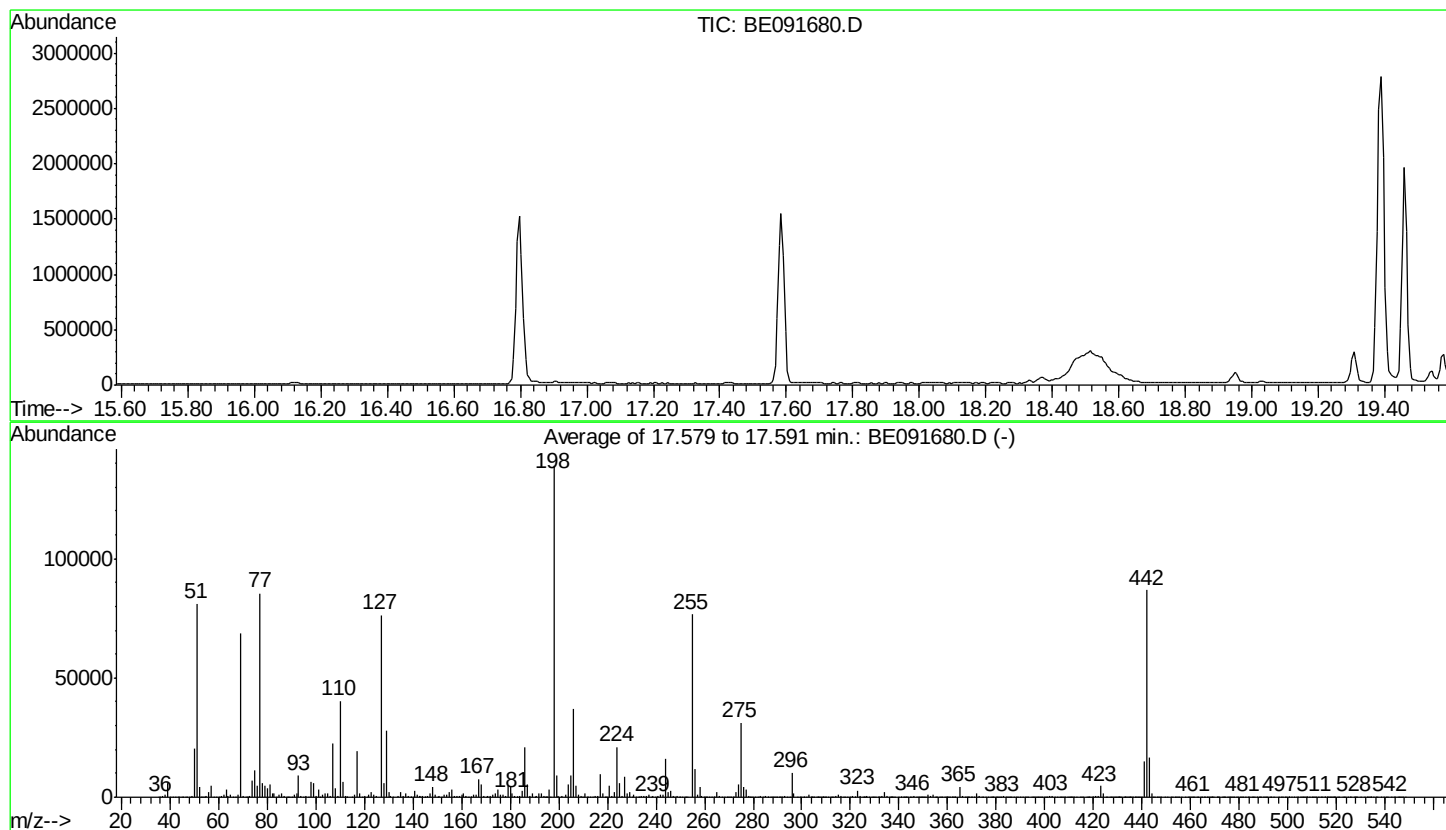

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.5	81231	PASS
68	69	0.00	2	1.3	896	PASS
69	198	0.00	100	49.3	68438	PASS
70	69	0.00	2	0.6	395	PASS
127	198	10	80	54.9	76224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	138931	PASS
199	198	5	9	6.6	9153	PASS
275	198	10	60	22.6	31388	PASS
365	198	1	100	3.1	4318	PASS
441	442	0.01	24	17.1	14861	PASS
442	198	50	100	62.4	86753	PASS
443	442	15	24	19.1	16599	PASS