


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042017\
Data File : BE092897.D
Acq On : 20 Apr 2017 13:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 20 17:35:10 2017

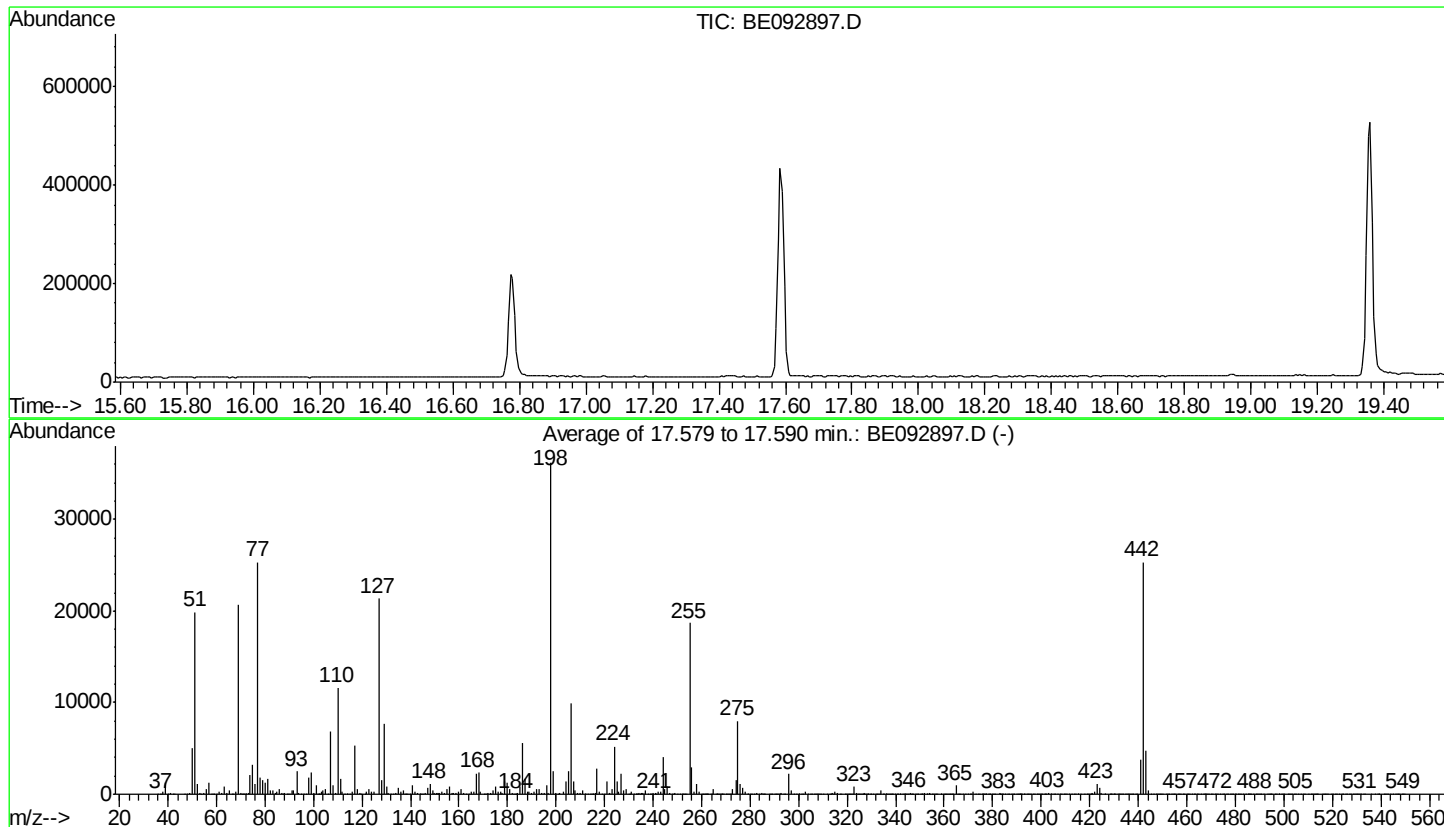

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	19883	PASS
68	69	0.00	2	1.3	276	PASS
69	198	0.00	100	57.2	20708	PASS
70	69	0.00	2	0.7	149	PASS
127	198	10	80	58.9	21314	PASS
197	198	0.00	2	0.5	180	PASS
198	198	100	100	100.0	36181	PASS
199	198	5	9	6.8	2475	PASS
275	198	10	60	22.0	7964	PASS
365	198	1	100	2.6	951	PASS
441	442	0.01	24	15.2	3832	PASS
442	198	50	100	69.9	25284	PASS
443	442	15	24	19.0	4811	PASS