

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096044.D
 Acq On : 20 Apr 2018 17:01
 Operator : SJ/JU
 Sample : SSTDC00.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTD0.444

Quant Time: Apr 21 01:00:17 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 00:59:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1872	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	4920	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2907	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6882	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	8426	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	6635	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3518	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	9776	0.34	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	11.25	128	5056	0.368	ng/ul#	89
5) 2-Methylnaphthalene	12.83	142	3525	0.378	ng/ul	99
7) Acenaphthylene	14.70	152	5408	0.359	ng/ul	98
8) Acenaphthene	15.03	153	3968	0.367	ng/ul	95
9) Fluorene	15.99	166	4509	0.369	ng/ul#	89
11) Pentachlorophenol	17.33	266	498	0.342	ng/ul	91
12) Phenanthrene	17.72	178	7406	0.365	ng/ul#	88
13) Anthracene	17.81	178	7379	0.366	ng/ul#	92
15) Fluoranthene	19.69	202	9434	0.342	ng/ul	83
17) Pyrene	20.04	202	11055	0.386	ng/ul#	80
18) Benzo(a)anthracene	21.75	228	11026	0.324	ng/ul#	86
19) Chrysene	21.81	228	8191	0.334	ng/ul	97
21) Benzo(b)fluoranthene	23.57	252	7876	0.367	ng/ul	90
22) Benzo(k)fluoranthene	23.62	252	7867	0.368	ng/ul	92
23) Benzo(a)pyrene	24.26	252	7573	0.366	ng/ul#	85
24) Indeno(1,2,3-cd)pyrene	27.17	276	8489	0.369	ng/ul#	77
25) Dibenzo(a,h)anthracene	27.19	278	6808	0.367	ng/ul	95
26) Benzo(g,h,i)perylene	28.04	276	7115	0.370	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096044.D
Acq On : 20 Apr 2018 17:01
Operator : SJ/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleID :
SSTD0.444

Quant Time: Apr 21 01:00:17 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 00:59:26 2018
Response via : Initial Calibration

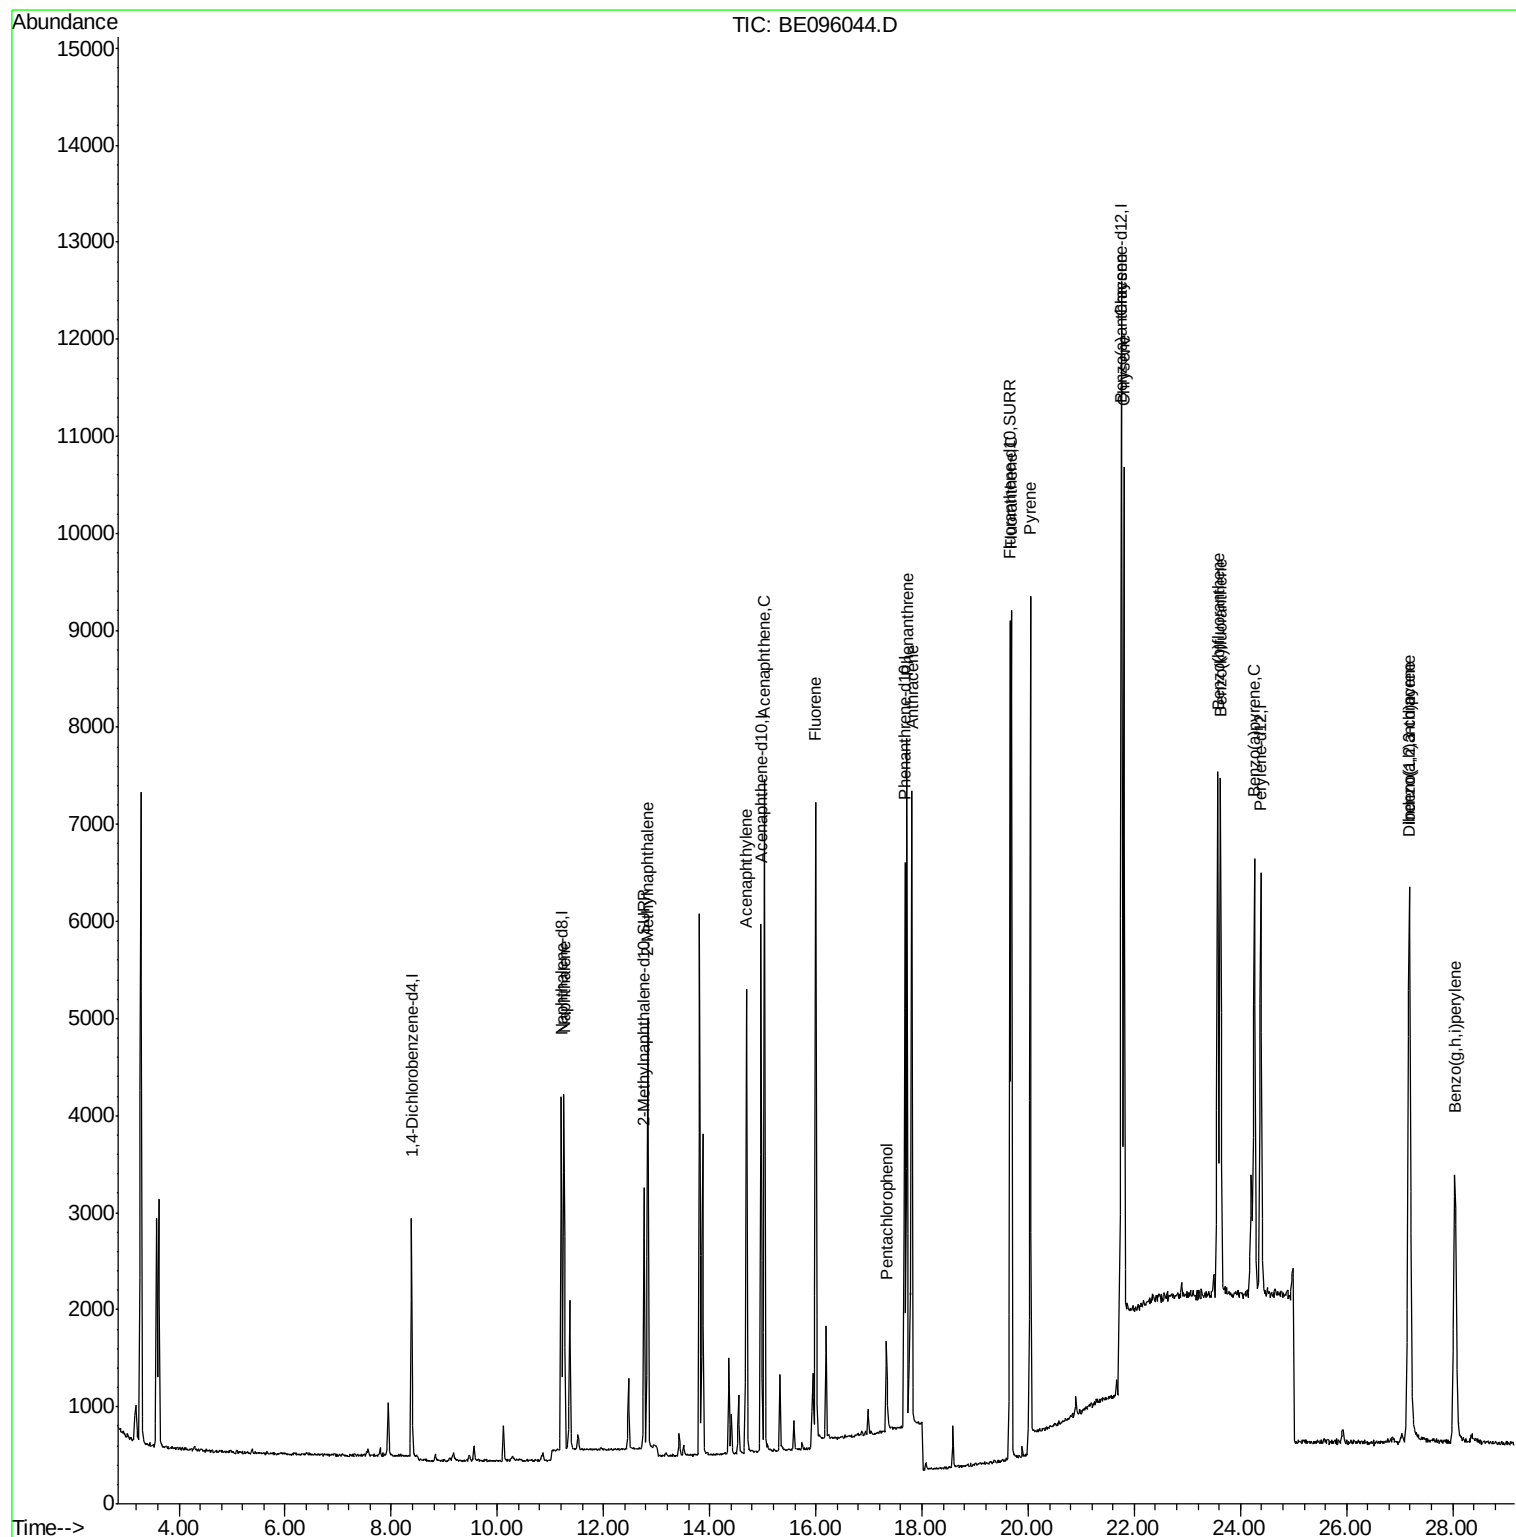

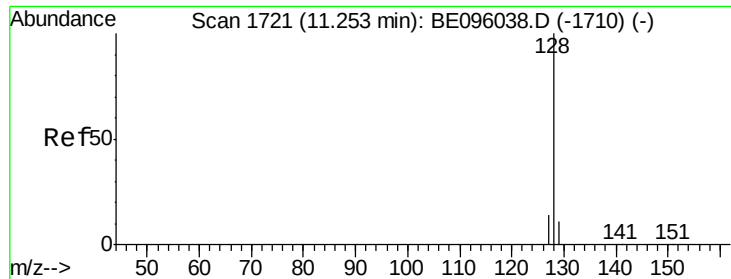

#3

Naphthalene

Concen: 0.368 ng/ul

RT: 11.25 min Scan# 1722

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:128 Resp: 5056

Ion Ratio Lower Upper

128 100

129 12.0 11.3 16.9




127 14.1 4.0 6.0#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

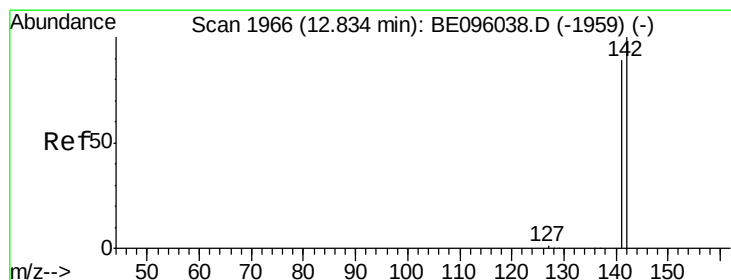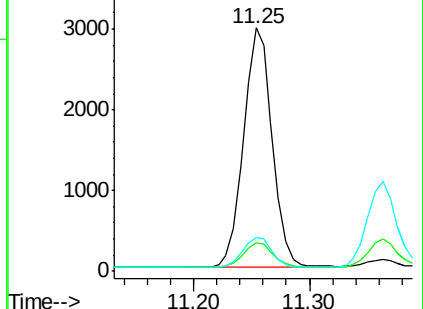

#5

2-Methylnaphthalene

Concen: 0.378 ng/ul

RT: 12.83 min Scan# 1967

Delta R.T. 0.00 min

Lab File: BE096044.D


Acq: 20 Apr 2018 17:01

Tgt Ion:142 Resp: 3525

Ion Ratio Lower Upper



142 100


141 91.5 72.6 108.8

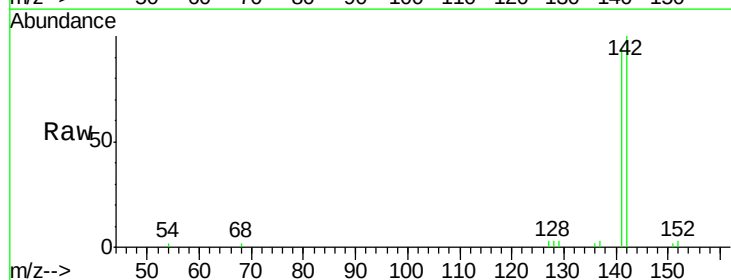

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

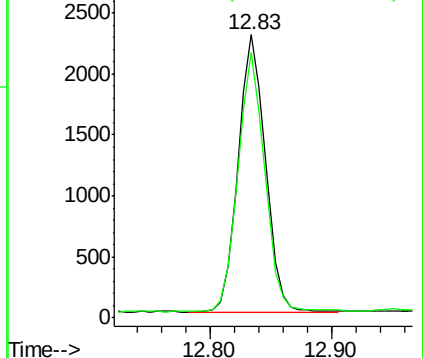



#7

Acenaphthylene

Concen: 0.359 ng/ul

RT: 14.70 min Scan# 2277

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:152 Resp: 5408

Ion Ratio Lower Upper

152 100

151 21.1 17.1 25.7




153 14.3 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

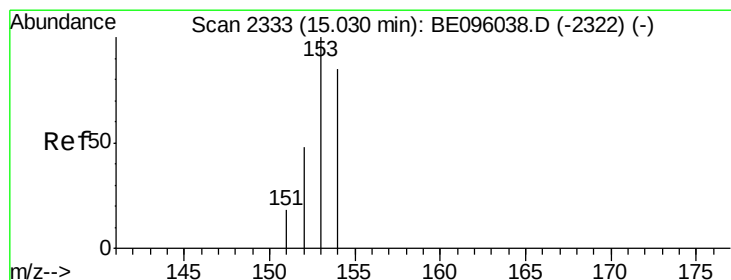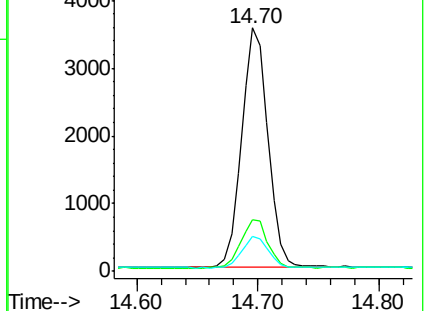

#8

Acenaphthene

Concen: 0.367 ng/ul

RT: 15.03 min Scan# 2334

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:153 Resp: 3968

Ion Ratio Lower Upper

153 100

152 48.6 36.0 54.0



154 86.1 72.0 108.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

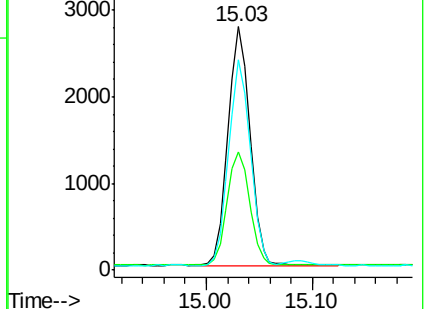

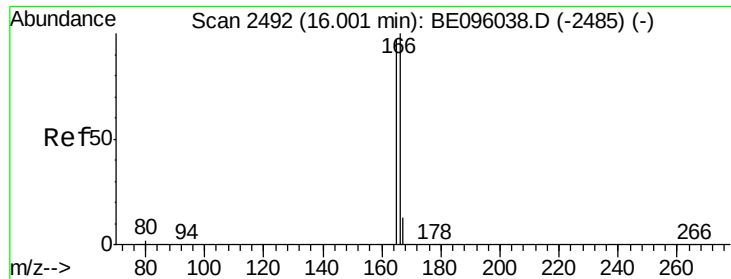

#9

Fluorene

Concen: 0.369 ng/ul

RT: 15.99 min Scan# 2492

Delta R.T. -0.01 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:166 Resp: 4509

Ion Ratio Lower Upper

166 100

165 103.2 73.4 110.2




167 14.4 14.6 22.0#

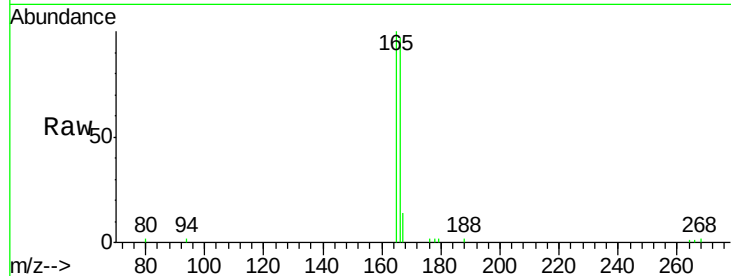

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

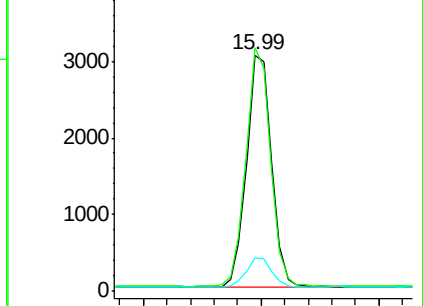

#11

Pentachlorophenol

Concen: 0.342 ng/ul

RT: 17.33 min Scan# 2682

Delta R.T. -0.01 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:266 Resp: 498

Ion Ratio Lower Upper

266 100

264 63.5 47.9 71.9



268 72.7 49.8 74.8




Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

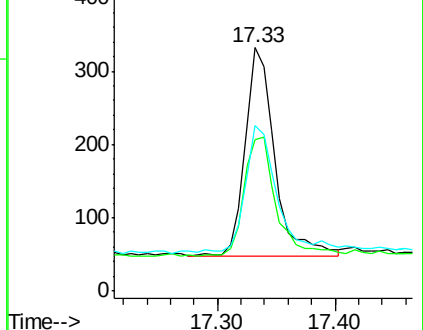



#12

Phenanthrene

Concen: 0.365 ng/ul

RT: 17.72 min Scan# 2737

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:178 Resp: 7406

Ion Ratio Lower Upper




178 100

179 15.9 18.4 27.6#

176 20.7 13.6 20.4#



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

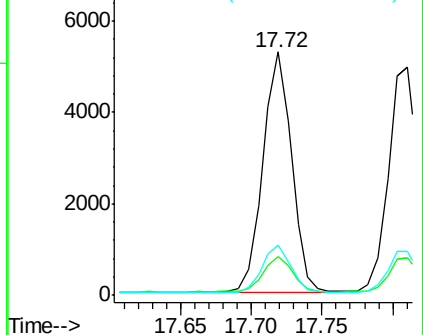

#13

Anthracene

Concen: 0.366 ng/ul

RT: 17.81 min Scan# 2750

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:178 Resp: 7379

Ion Ratio Lower Upper



178 100


179 16.3 18.1 27.1#

176 19.1 14.7 22.1



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

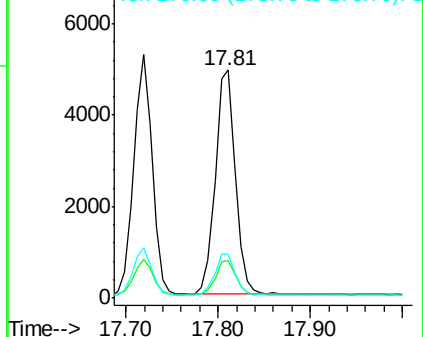

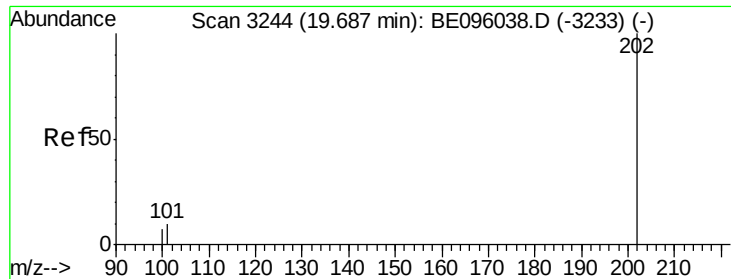

#15

Fluoranthene

Concen: 0.342 ng/ul

RT: 19.69 min Scan# 3245

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:202 Resp: 9434

Ion Ratio Lower Upper

202 100

101 9.9 0.0 30.3




100 8.1 0.0 39.5



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

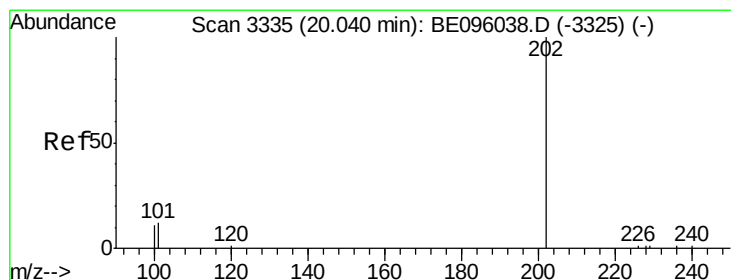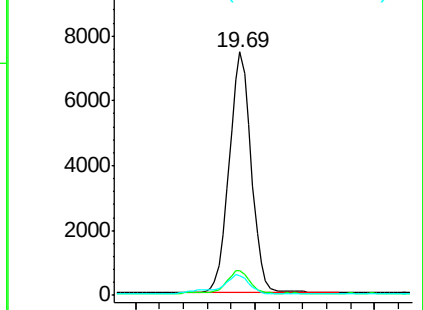

#17

Pyrene

Concen: 0.386 ng/ul

RT: 20.04 min Scan# 3336

Delta R.T. -0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:202 Resp: 11055

Ion Ratio Lower Upper

202 100

101 12.3 18.2 27.4#



100 11.0 15.6 23.4#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

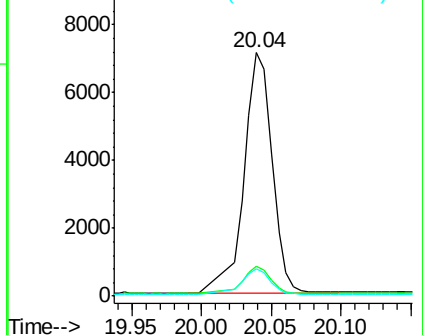

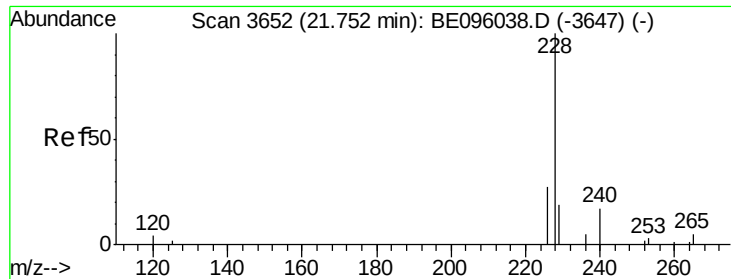

#18

Benzo(a)anthracene

Concen: 0.324 ng/ul

RT: 21.75 min Scan# 3653

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:228 Resp: 11026

Ion Ratio Lower Upper

228 100

229 20.7 22.8 34.2#




226 28.0 17.0 25.6#

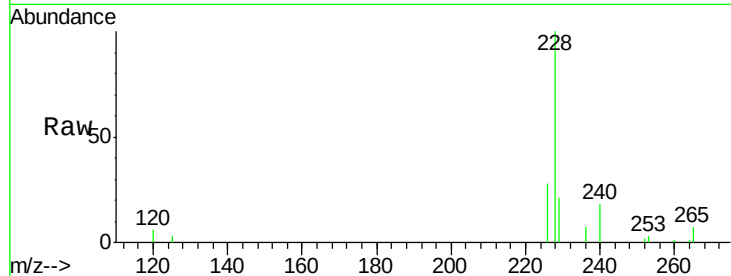

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

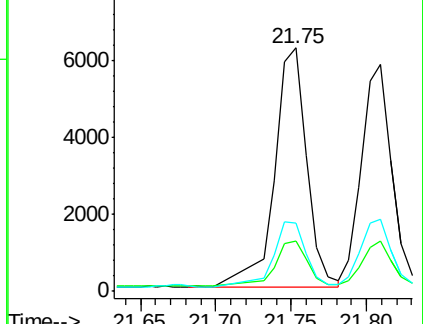

#19

Chrysene

Concen: 0.334 ng/ul

RT: 21.81 min Scan# 3661

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:228 Resp: 8191

Ion Ratio Lower Upper

228 100

226 31.7 23.4 35.0



229 22.3 17.7 26.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E




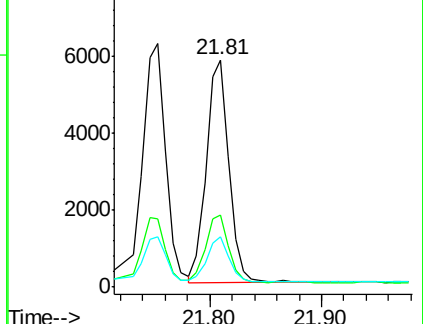


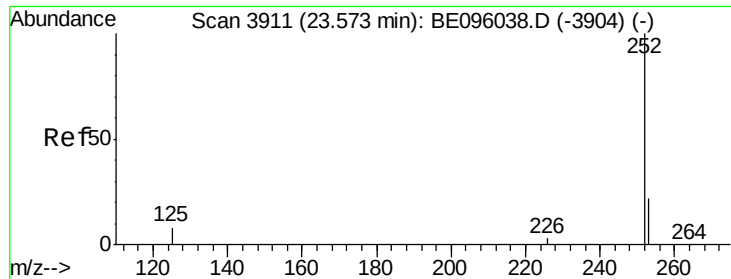

#21
Benzo(b)fluoranthene
Concen: 0.367 ng/ul
RT: 23.57 min Scan# 3912
Delta R.T. 0.00 min
Lab File: BE096044.D
Acq: 20 Apr 2018 17:01




Instrument :
BNA_E
ClientSampleId :
SSTD0.444


Tot Ion:252 Resp: 7876
Ion Ratio Lower Upper
252 100
253 26.3 0.0 64.2
125 13.2 0.0 35.0

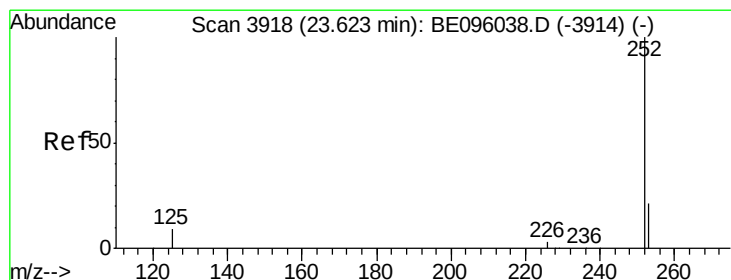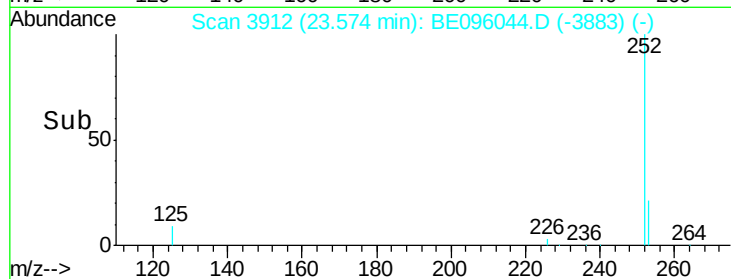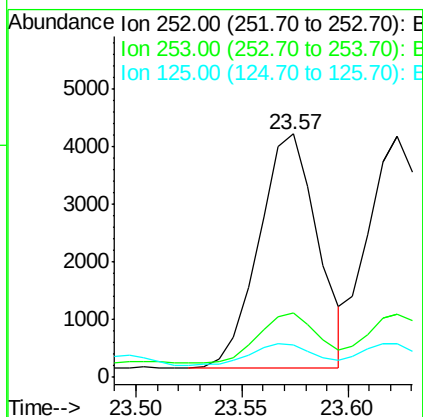

#22
Benzo(k)fluoranthene
Concen: 0.368 ng/ul
RT: 23.62 min Scan# 3919
Delta R.T. 0.00 min
Lab File: BE096044.D
Acq: 20 Apr 2018 17:01

Tgt Ion:252 Resp: 7867
Ion Ratio Lower Upper
252 100
253 26.1 24.5 36.7
125 13.7 13.7 20.5

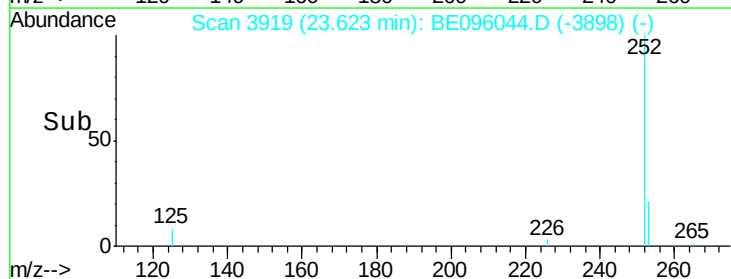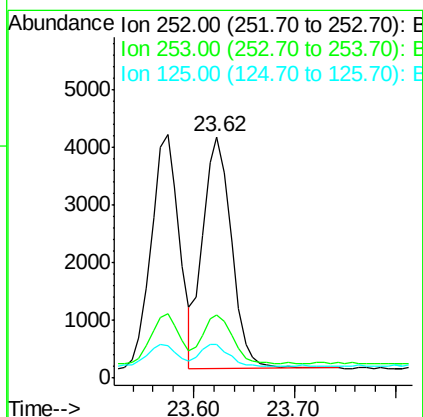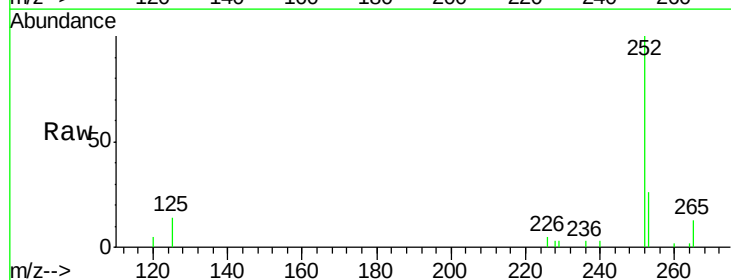

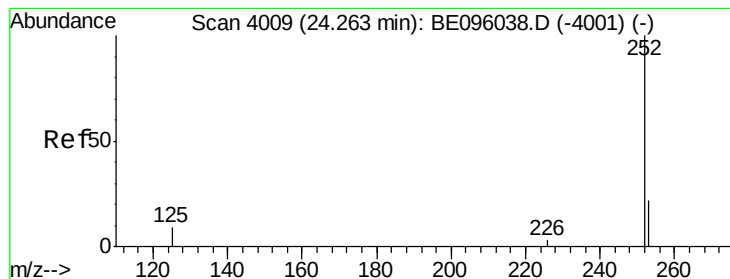

#23

Benzo(a)pyrene

Concen: 0.366 ng/ul

RT: 24.26 min Scan# 4010

Delta R.T. 0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01

Instrument :

BNA_E

ClientSampleId :

SSTD0.444


Tot Ion:252 Resp: 7573

Ion Ratio Lower Upper

252 100

253 27.3 28.5 42.7#




125 15.3 18.1 27.1#

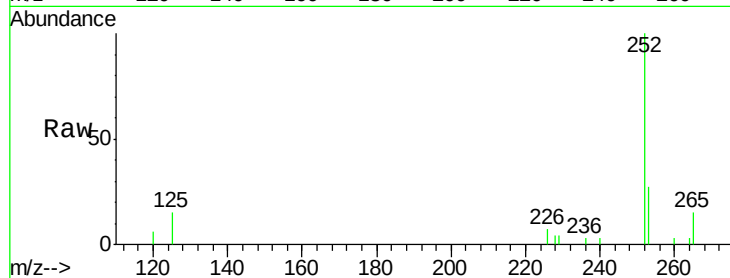

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

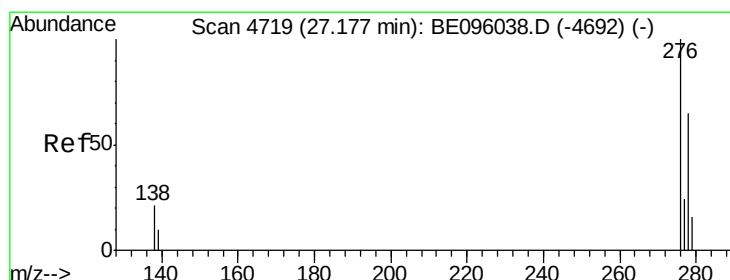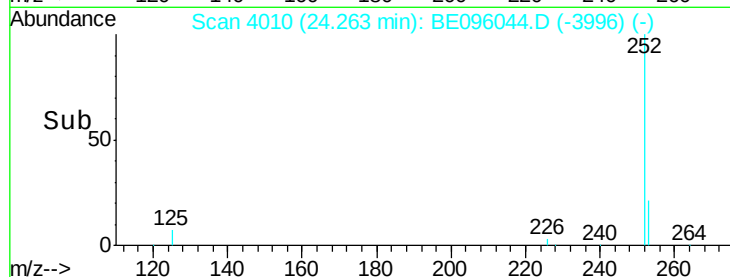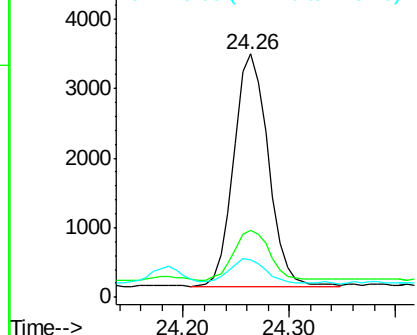

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.369 ng/ul

RT: 27.17 min Scan# 4719

Delta R.T. -0.00 min

Lab File: BE096044.D

Acq: 20 Apr 2018 17:01


Tgt Ion:276 Resp: 8489

Ion Ratio Lower Upper

276 100

138 22.4 28.0 42.0#



227 0.0 8.0 12.0#

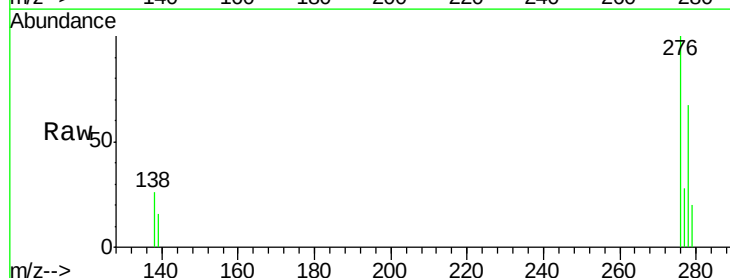


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

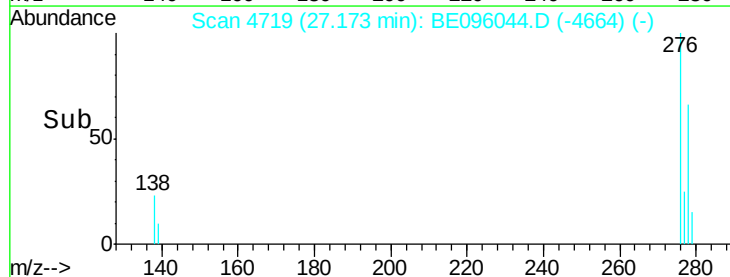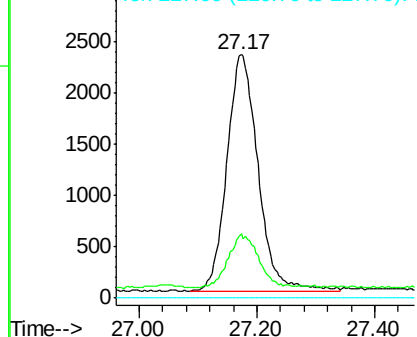




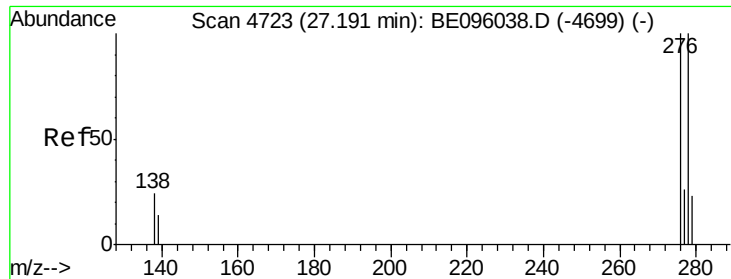


#25
Dibenzo(a,h)anthracene
Concen: 0.367 ng/ul
RT: 27.19 min Scan# 4724
Delta R.T. 0.00 min
Lab File: BE096044.D
Acq: 20 Apr 2018 17:01

Instrument :
BNA_E
ClientSampleId :
SSTD0.444

Tot Ion:278 Resp: 6808

Ion	Ratio	Lower	Upper
278	100		
139	23.1	17.4	26.0
279	28.7	25.9	38.9

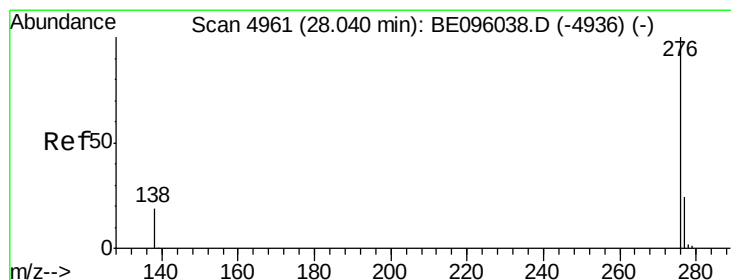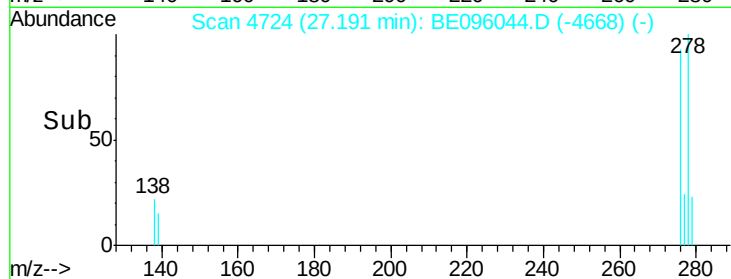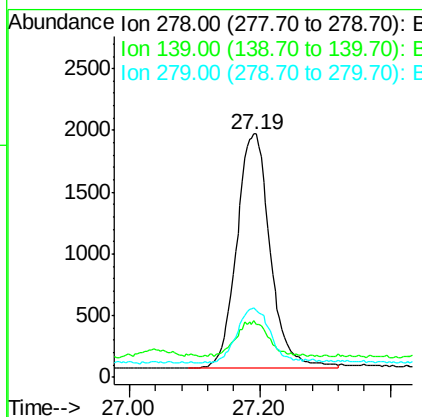

#26
Benzo(g,h,i)perylene
Concen: 0.370 ng/ul
RT: 28.04 min Scan# 4962
Delta R.T. 0.00 min
Lab File: BE096044.D
Acq: 20 Apr 2018 17:01

Tgt Ion:276 Resp: 7115

Ion	Ratio	Lower	Upper
276	100		
138	24.0	21.8	32.8
277	26.6	20.5	30.7

