

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096046.D
 Acq On : 20 Apr 2018 18:17
 Operator : SJ/JU
 Sample : PB108446BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK46

Quant Time: Apr 21 01:28:57 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 01:28:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1924	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5025	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3161	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.78	188	542104	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.77
20) Perylene-d12	24.22	264	451512	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3096	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.95	166	780	0.059	ng/ul#	Ovalue 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096046.D
Acq On : 20 Apr 2018 18:17
Operator : SJ/JU
Sample : PB108446BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK46

Quant Time: Apr 21 01:28:57 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 01:28:31 2018
Response via : Initial Calibration

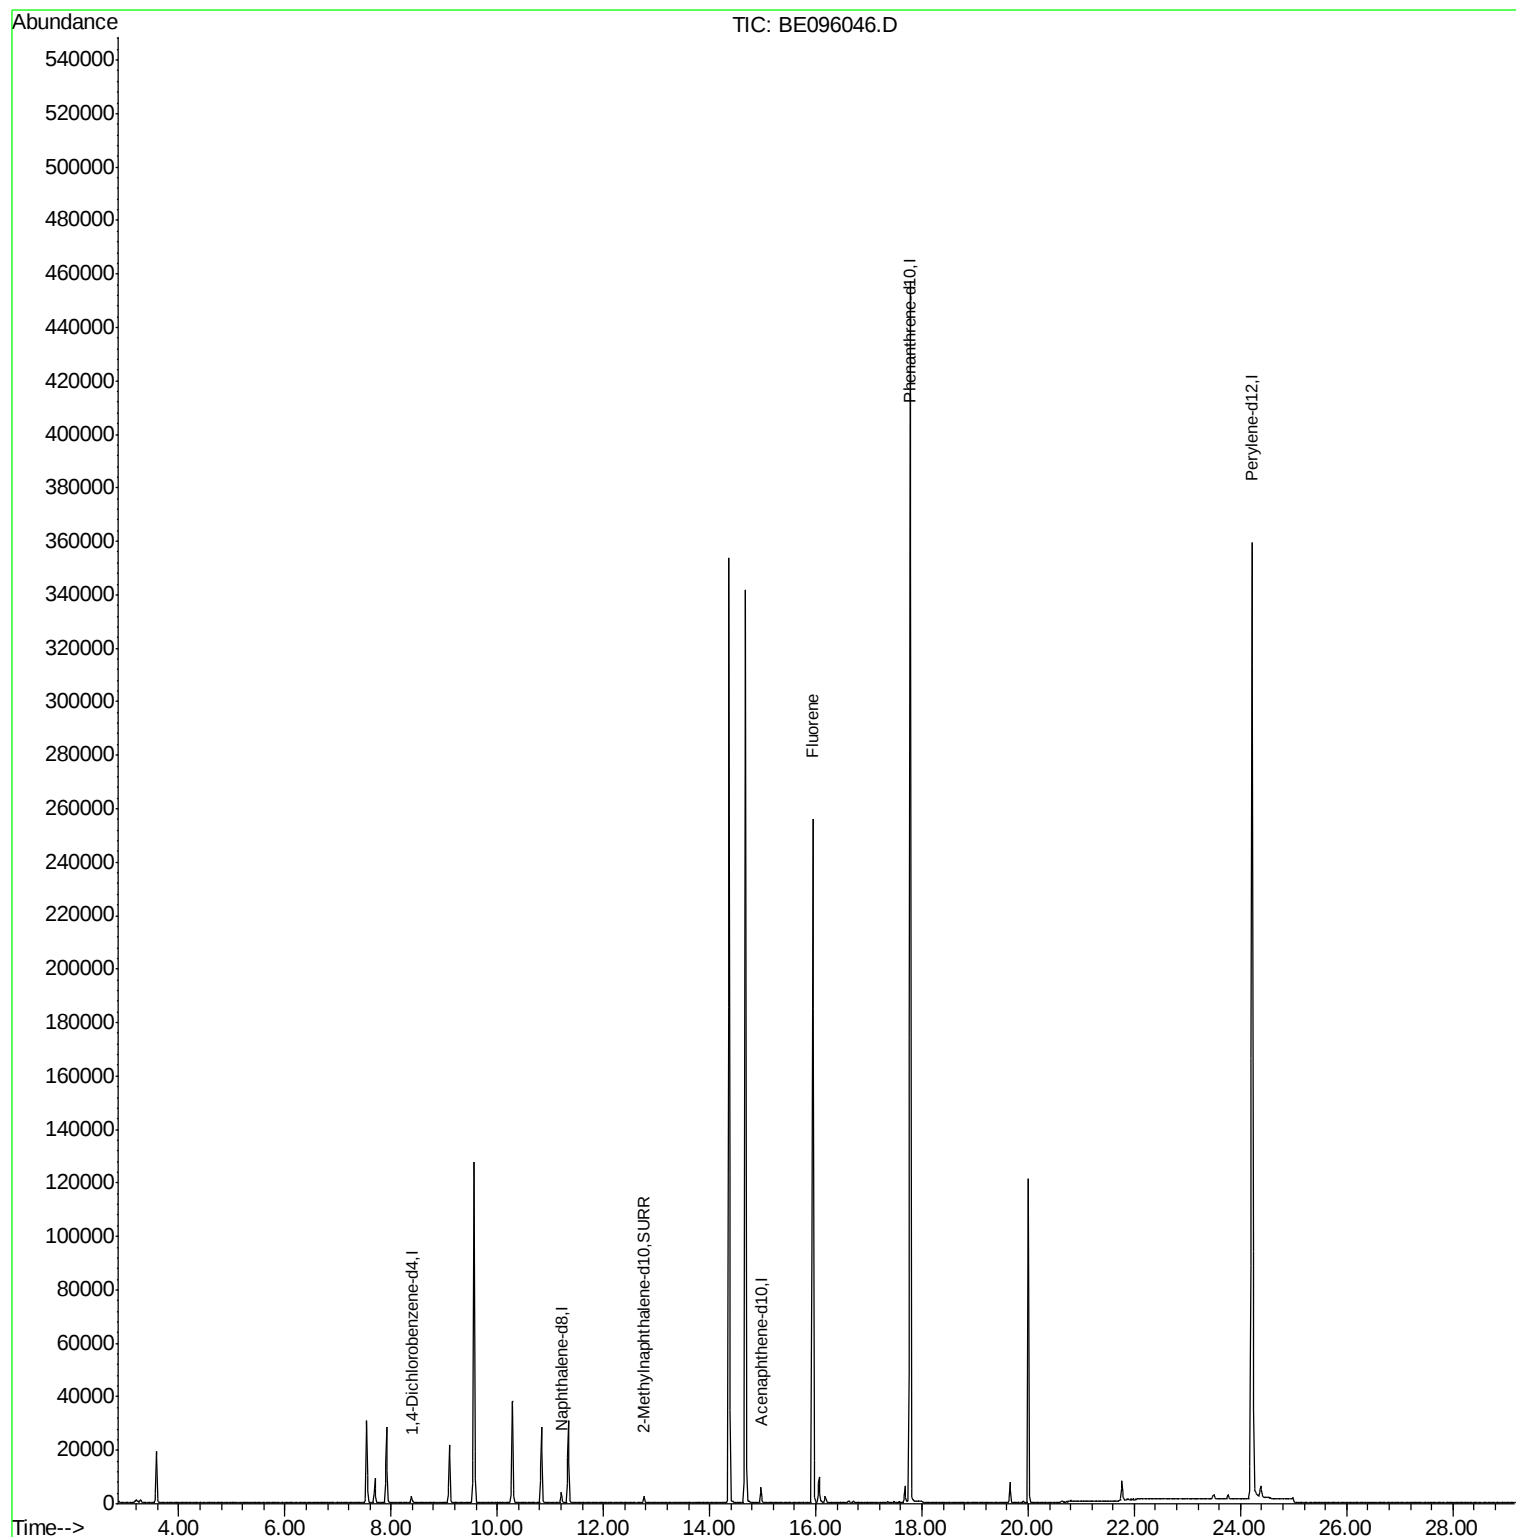

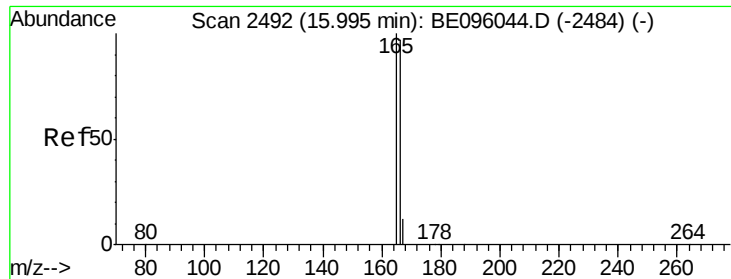

#9

Fluorene

Concen: 0.059 ng/ul

RT: 15.95 min Scan# 2485

Delta R.T. -0.05 min

Lab File: BE096046.D

Acq: 20 Apr 2018 18:17

Instrument :

BNA_E

ClientSampleId :

SBLK46



Tot Ion:166 Resp: 780

Ion Ratio Lower Upper

166 100

165 13.4 73.4 110.2#

167 39.9 14.6 22.0#

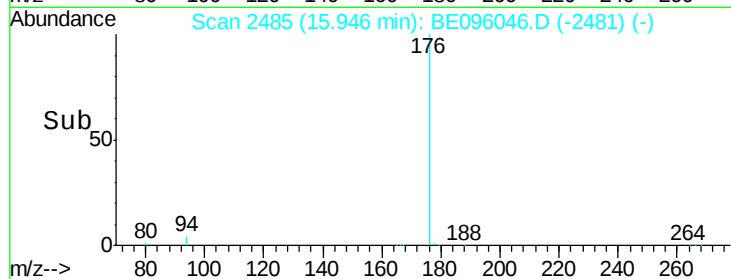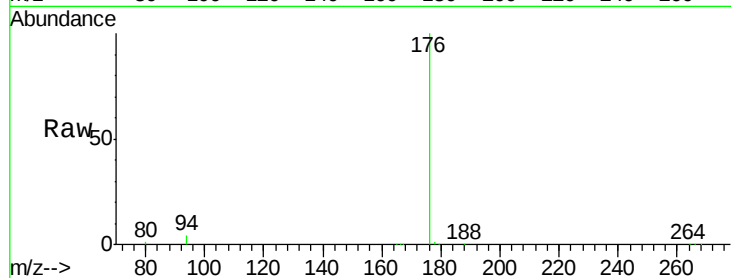

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

