

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096055.D
 Acq On : 20 Apr 2018 23:39
 Operator : SJ/JU
 Sample : J2356-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3XT7

Quant Time: Apr 21 01:29:52 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 01:28:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1952	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5332	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3263	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.78	188	530245	0.40	ng/ul	0.10
16) Chrysene-d12	21.88	240	14	0.40	ng/ul	0.11
20) Perylene-d12	24.38	264	9808	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3148	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
17) Pyrene	20.04	202	1264	26.570	ng/ul#	89
18) Benzo(a)anthracene	21.80	228	643	11.369	ng/ul#	73
19) Chrysene	21.80	228	640	15.722	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096055.D
Acq On : 20 Apr 2018 23:39
Operator : SJ/JU
Sample : J2356-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3XT7

Quant Time: Apr 21 01:29:52 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 01:28:31 2018
Response via : Initial Calibration




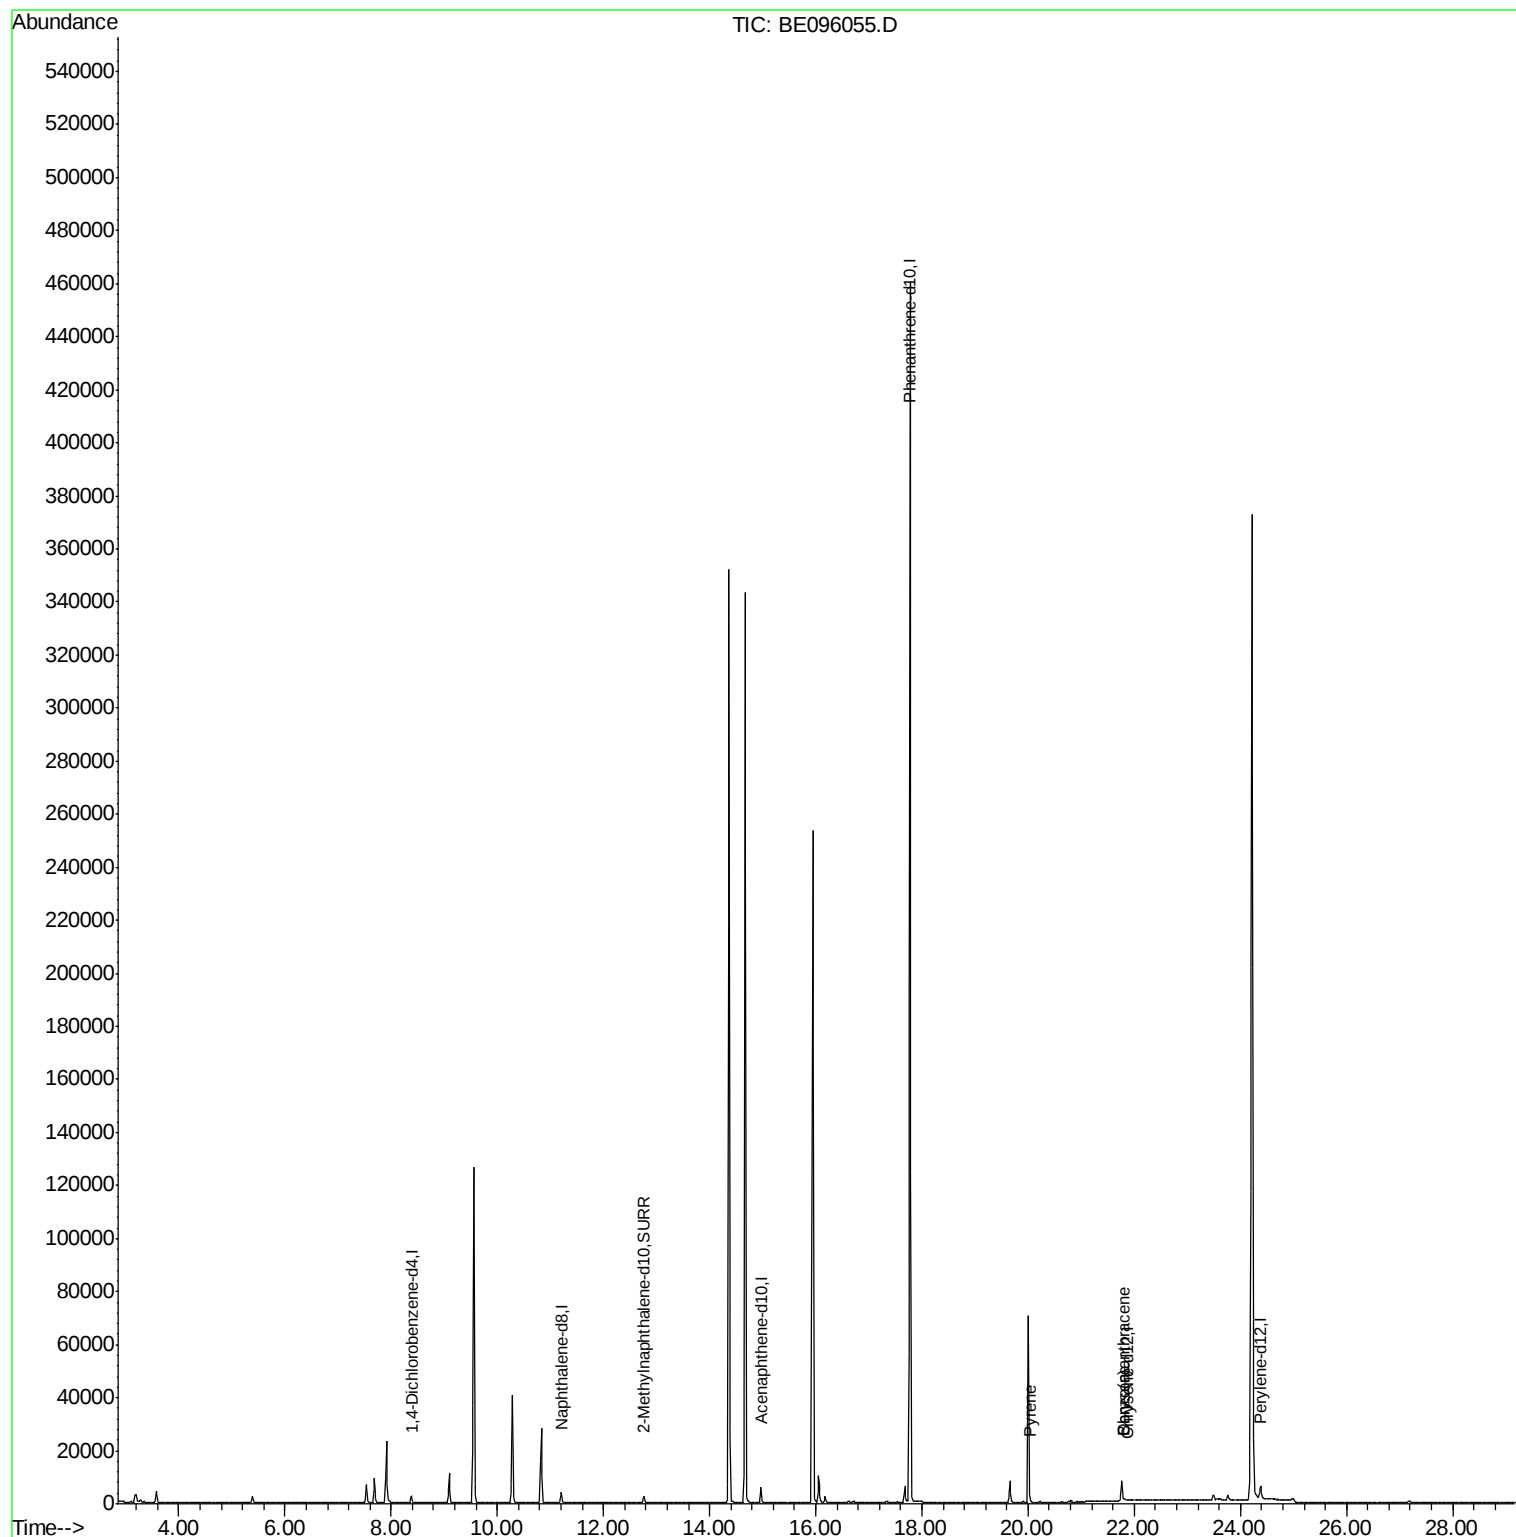


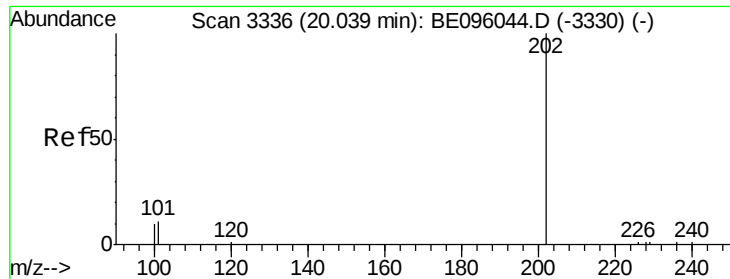

#17
Pvrene
Concen: 26.570 ng/ul
RT: 20.04 min Scan# 3336
Delta R.T. 0.00 min
Lab File: BE096055.D
Acq: 20 Apr 2018 23:39




Instrument :
BNA_E
ClientSampleId :
A3XT7




Tot Ion:202 Resp: 1264
Ion Ratio Lower Upper
202 100
101 21.7 18.2 27.4
100 29.2 15.6 23.4#

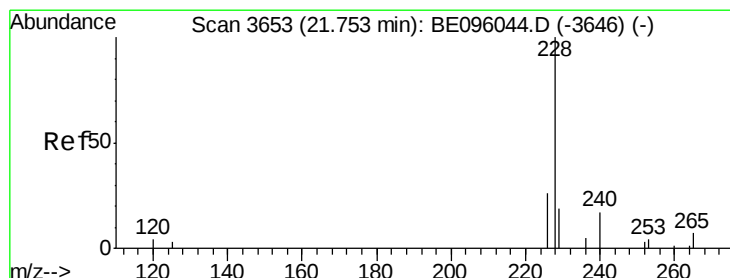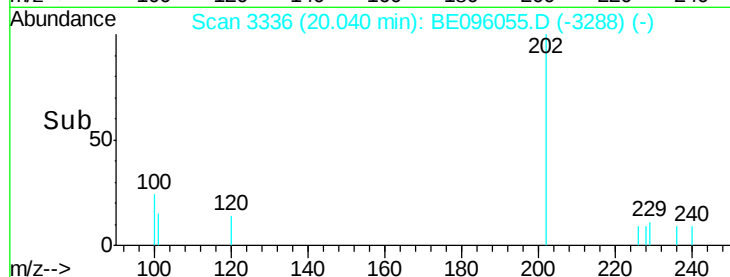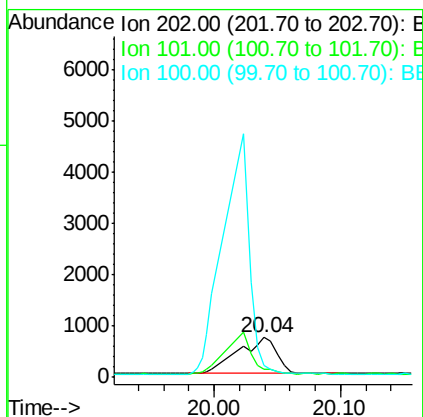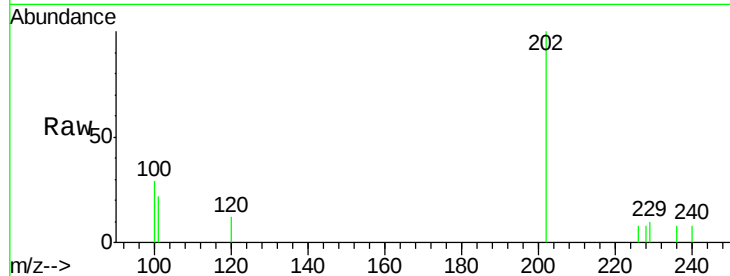

#18
Benzo(a)anthracene
Concen: 11.369 ng/ul
RT: 21.80 min Scan# 3660
Delta R.T. 0.05 min
Lab File: BE096055.D
Acq: 20 Apr 2018 23:39

Tgt Ion:228 Resp: 643
Ion Ratio Lower Upper
228 100
229 36.5 22.8 34.2#
226 41.0 17.0 25.6#

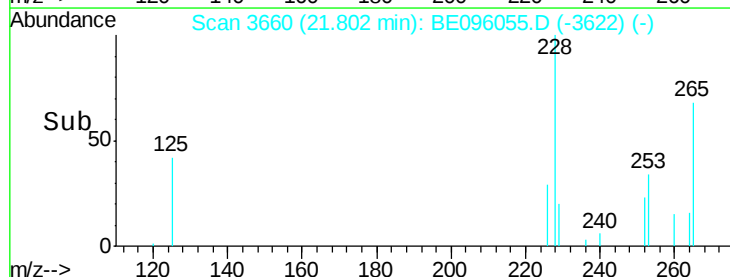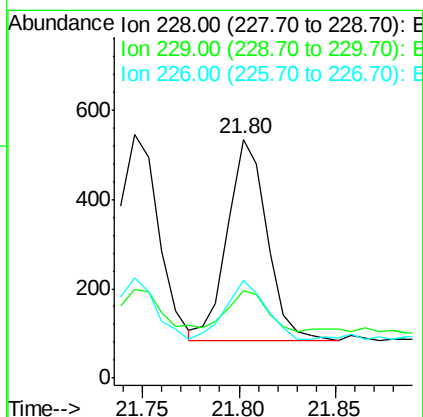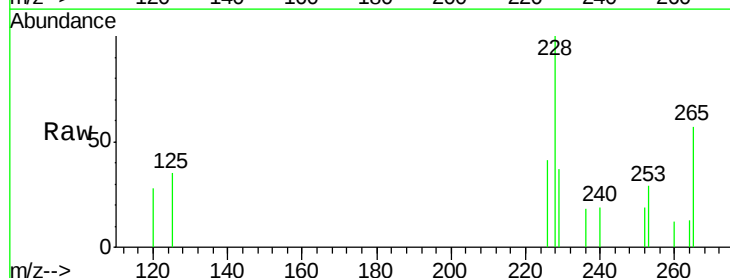

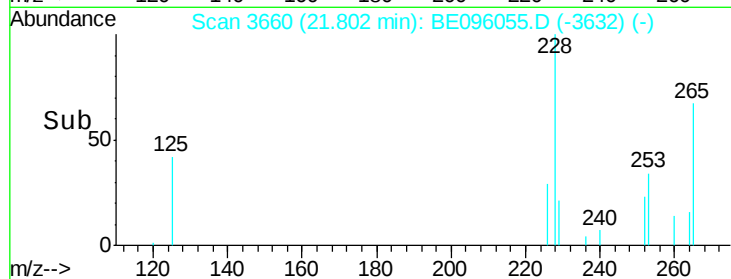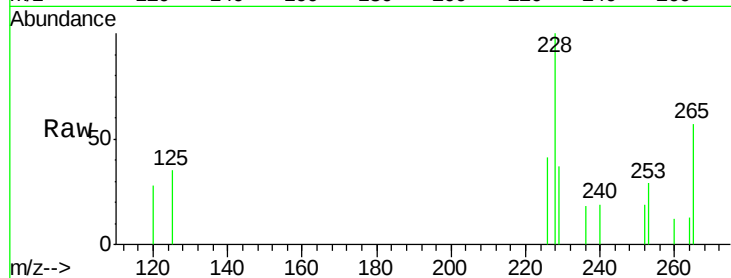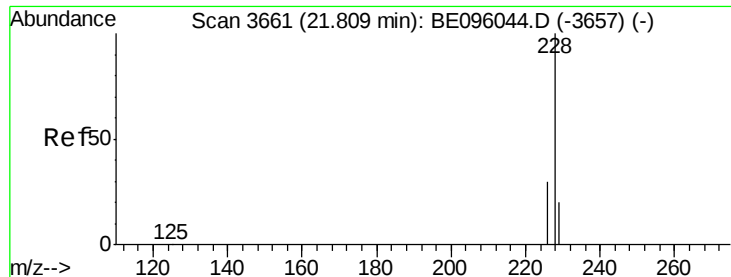

#19

Chrysene

Concen: 15.722 ng/ul

RT: 21.80 min Scan# 3660

Delta R.T. -0.01 min

Lab File: BE096055.D

Acq: 20 Apr 2018 23:39

Instrument :

BNA_E

ClientSampleId :

A3XT7

Tot Ion: 228 Resp: 640

Ion Ratio Lower Upper

228 100

226 41.0 23.4 35.0#

229 36.5 17.7 26.5#

