

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096058.D
 Acq On : 21 Apr 2018 1:27
 Operator : SJ/JU
 Sample : J2356-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3XS0

Quant Time: Apr 21 02:24:14 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 01:28:31 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	2072	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	6106	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3634	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.77	188	577109	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.77
20) Perylene-d12	24.22	264	474627	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3420	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	11.25	128	1009	0.059	ng/ul#	83
5) 2-Methylnaphthalene	12.83	142	493	0.043	ng/ul	94
8) Acenaphthene	15.02	153	2053	0.152	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096058.D
Acq On : 21 Apr 2018 1:27
Operator : SJ/JU
Sample : J2356-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3XS0

Quant Time: Apr 21 02:24:14 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 01:28:31 2018
Response via : Initial Calibration

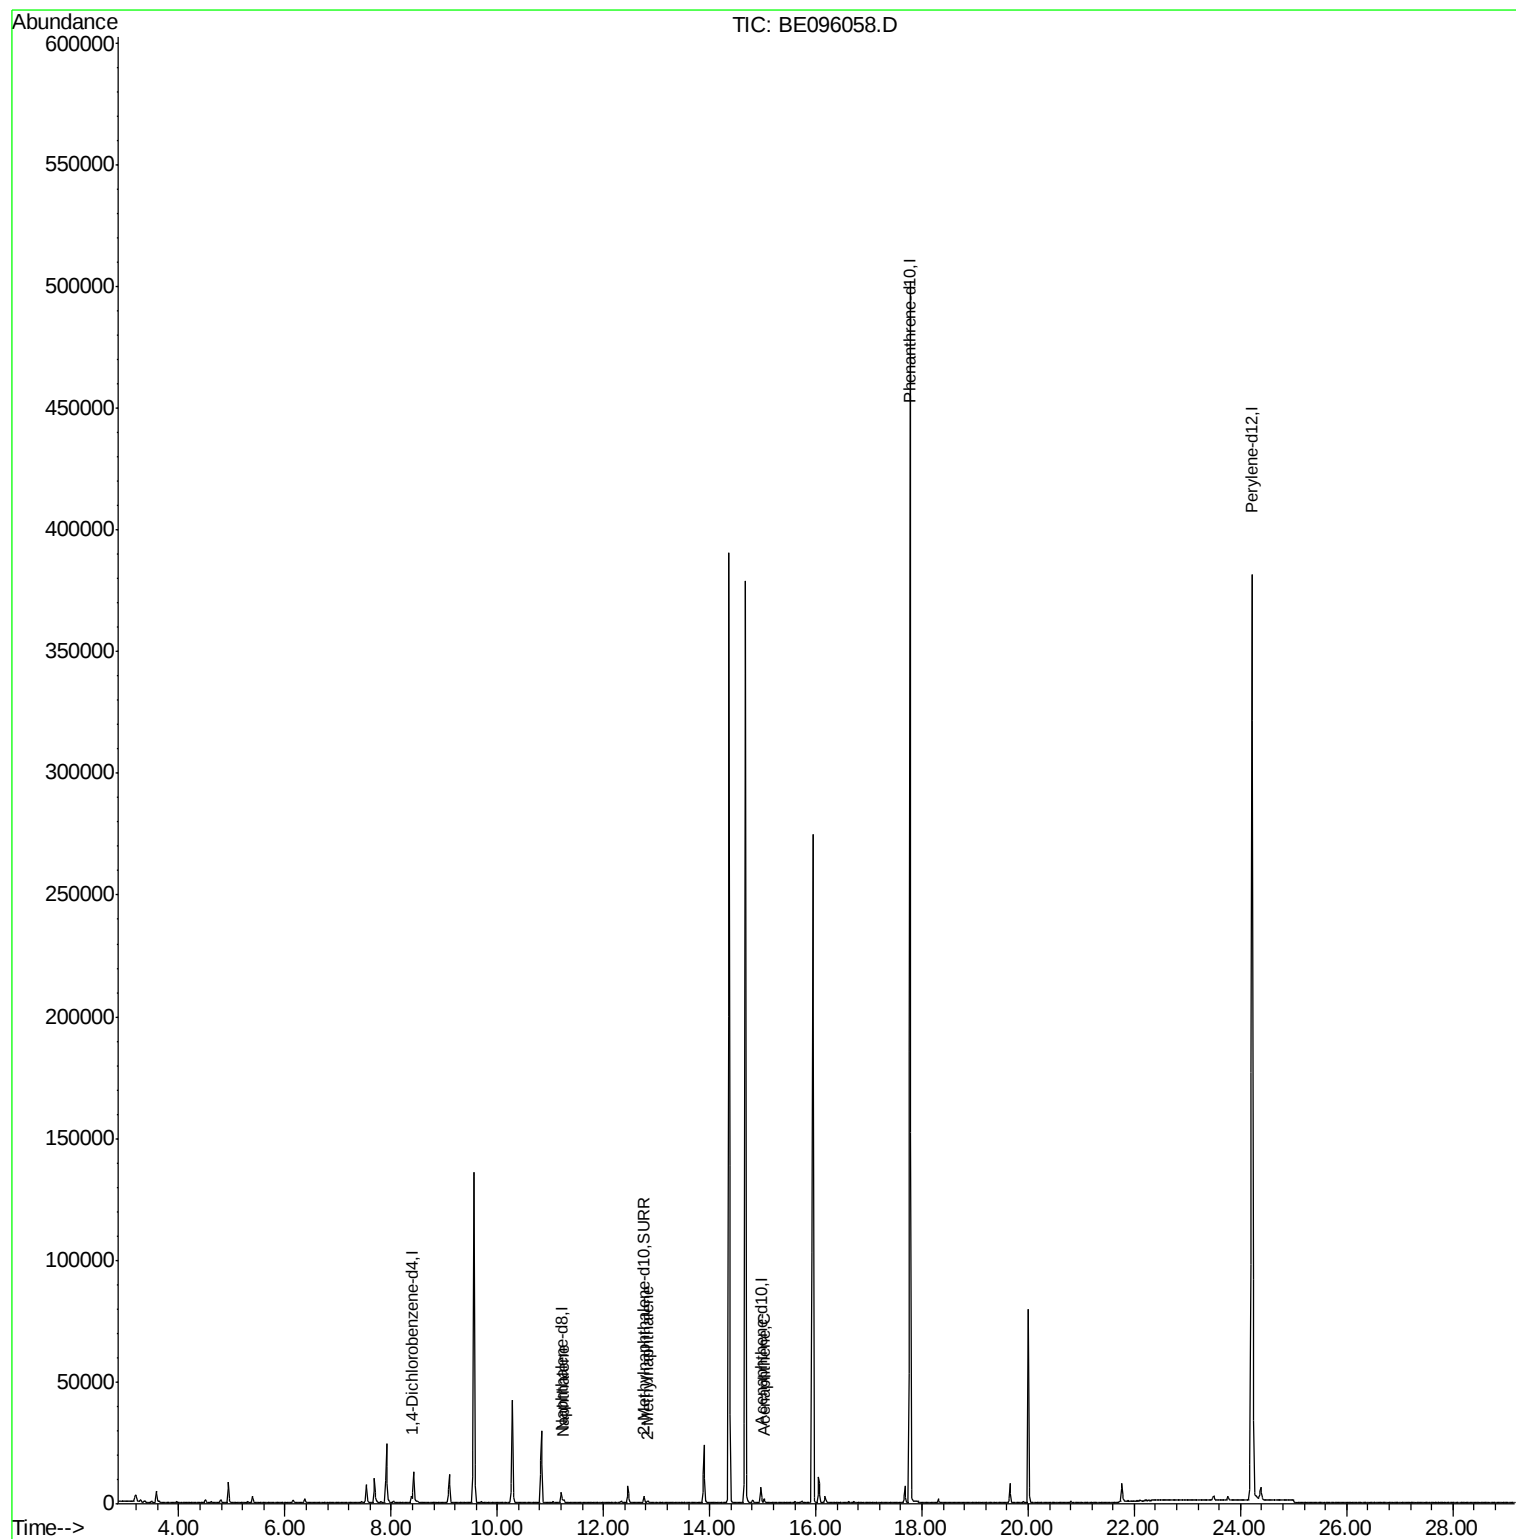

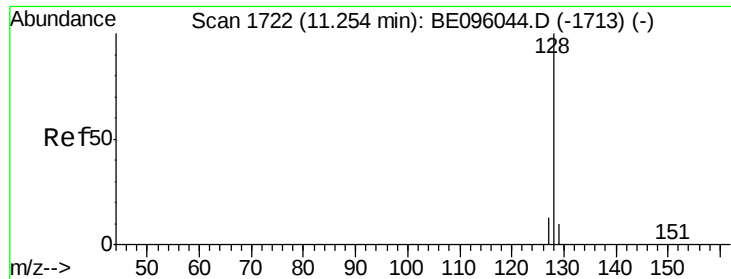

#3

Naphthalene

Concen: 0.059 ng/ul

RT: 11.25 min Scan# 1721

Delta R.T. -0.00 min

Lab File: BE096058.D

Acq: 21 Apr 2018 1:27

Instrument :

BNA_E

ClientSampleId :

A3XS0





Tot Ion:128 Resp: 1009

Ion Ratio Lower Upper

128 100

129 17.3 11.3 16.9#

127 19.6 4.0 6.0#

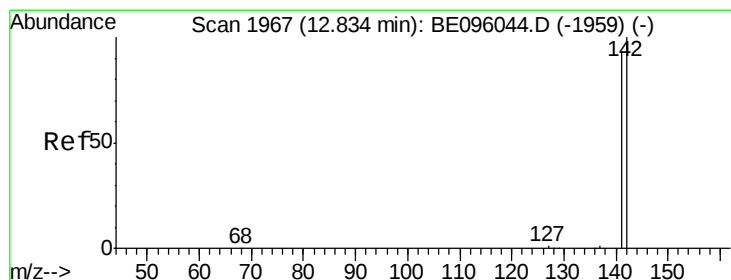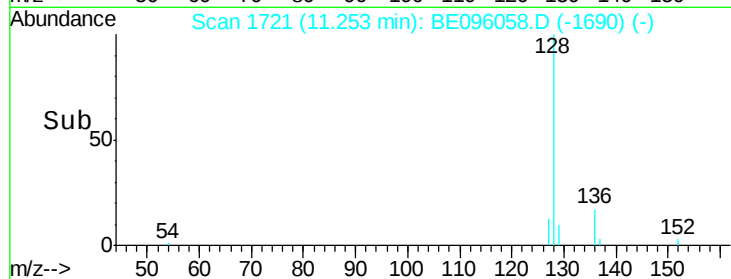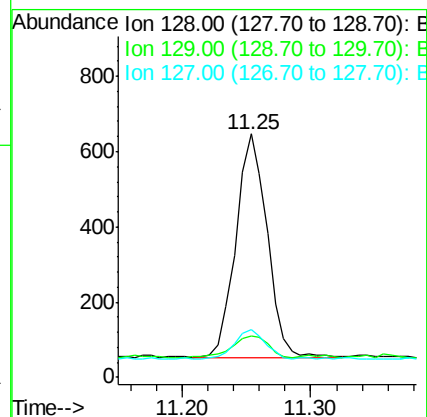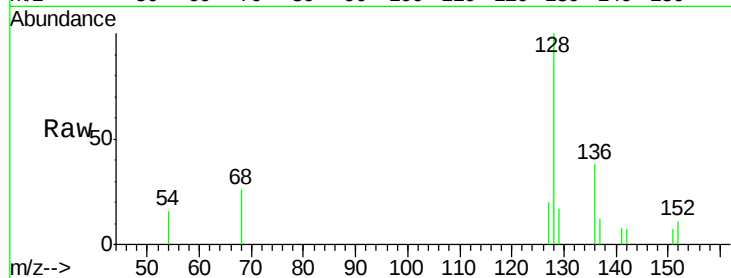

#5

2-Methylnaphthalene

Concen: 0.043 ng/ul

RT: 12.83 min Scan# 1966

Delta R.T. -0.00 min

Lab File: BE096058.D




Acq: 21 Apr 2018 1:27




Tgt Ion:142 Resp: 493

Ion Ratio Lower Upper

142 100

141 96.8 72.6 108.8

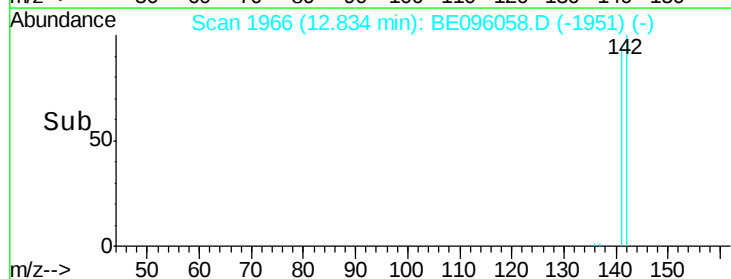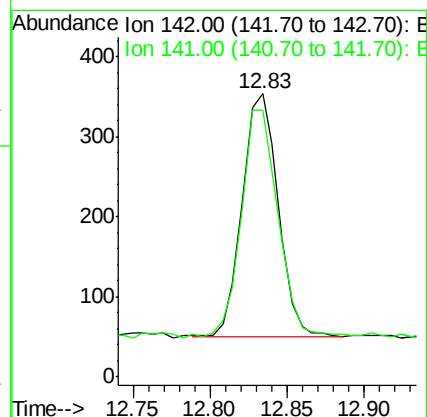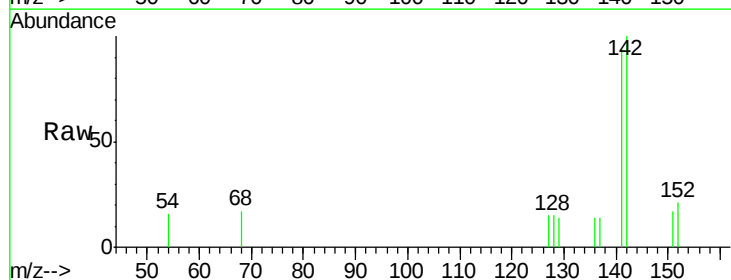

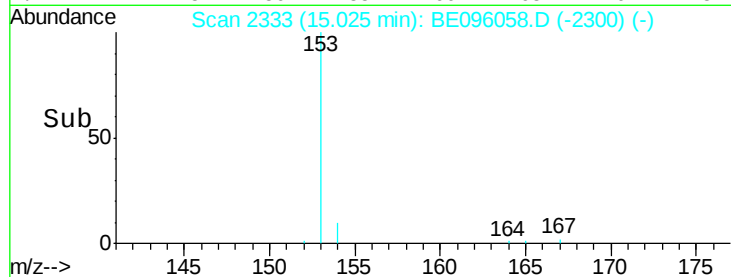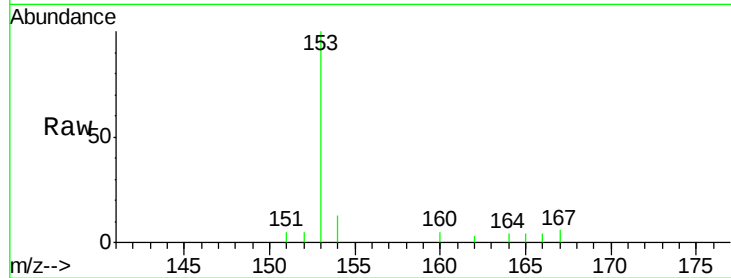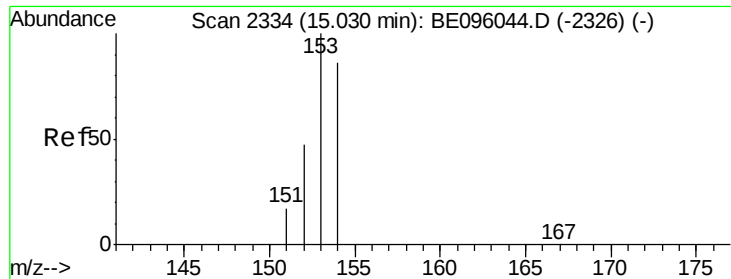

#8

Acenaphthene

Concen: 0.152 ng/ul

RT: 15.02 min Scan# 2333

Delta R.T. -0.01 min

Lab File: BE096058.D

Acq: 21 Apr 2018 1:27

Instrument :

BNA_E

ClientSampleId :

A3XS0

Tot Ion:153 Resp: 2053

Ion Ratio Lower Upper

153 100

152 4.8 36.0 54.0#

154 12.5 72.0 108.0#

