

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096061.D
 Acq On : 21 Apr 2018 3:38
 Operator : SJ/JU
 Sample : J2356-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3XZ8

Quant Time: Apr 23 01:08:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.37	152	2072	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5775	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3581	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.77	188	574322	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.77
20) Perylene-d12	24.21	264	514299	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	3455	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.95	166	781	0.052	ng/ul#	21




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096061.D
Acq On : 21 Apr 2018 3:38
Operator : SJ/JU
Sample : J2356-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3XZ8

Quant Time: Apr 23 01:08:47 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

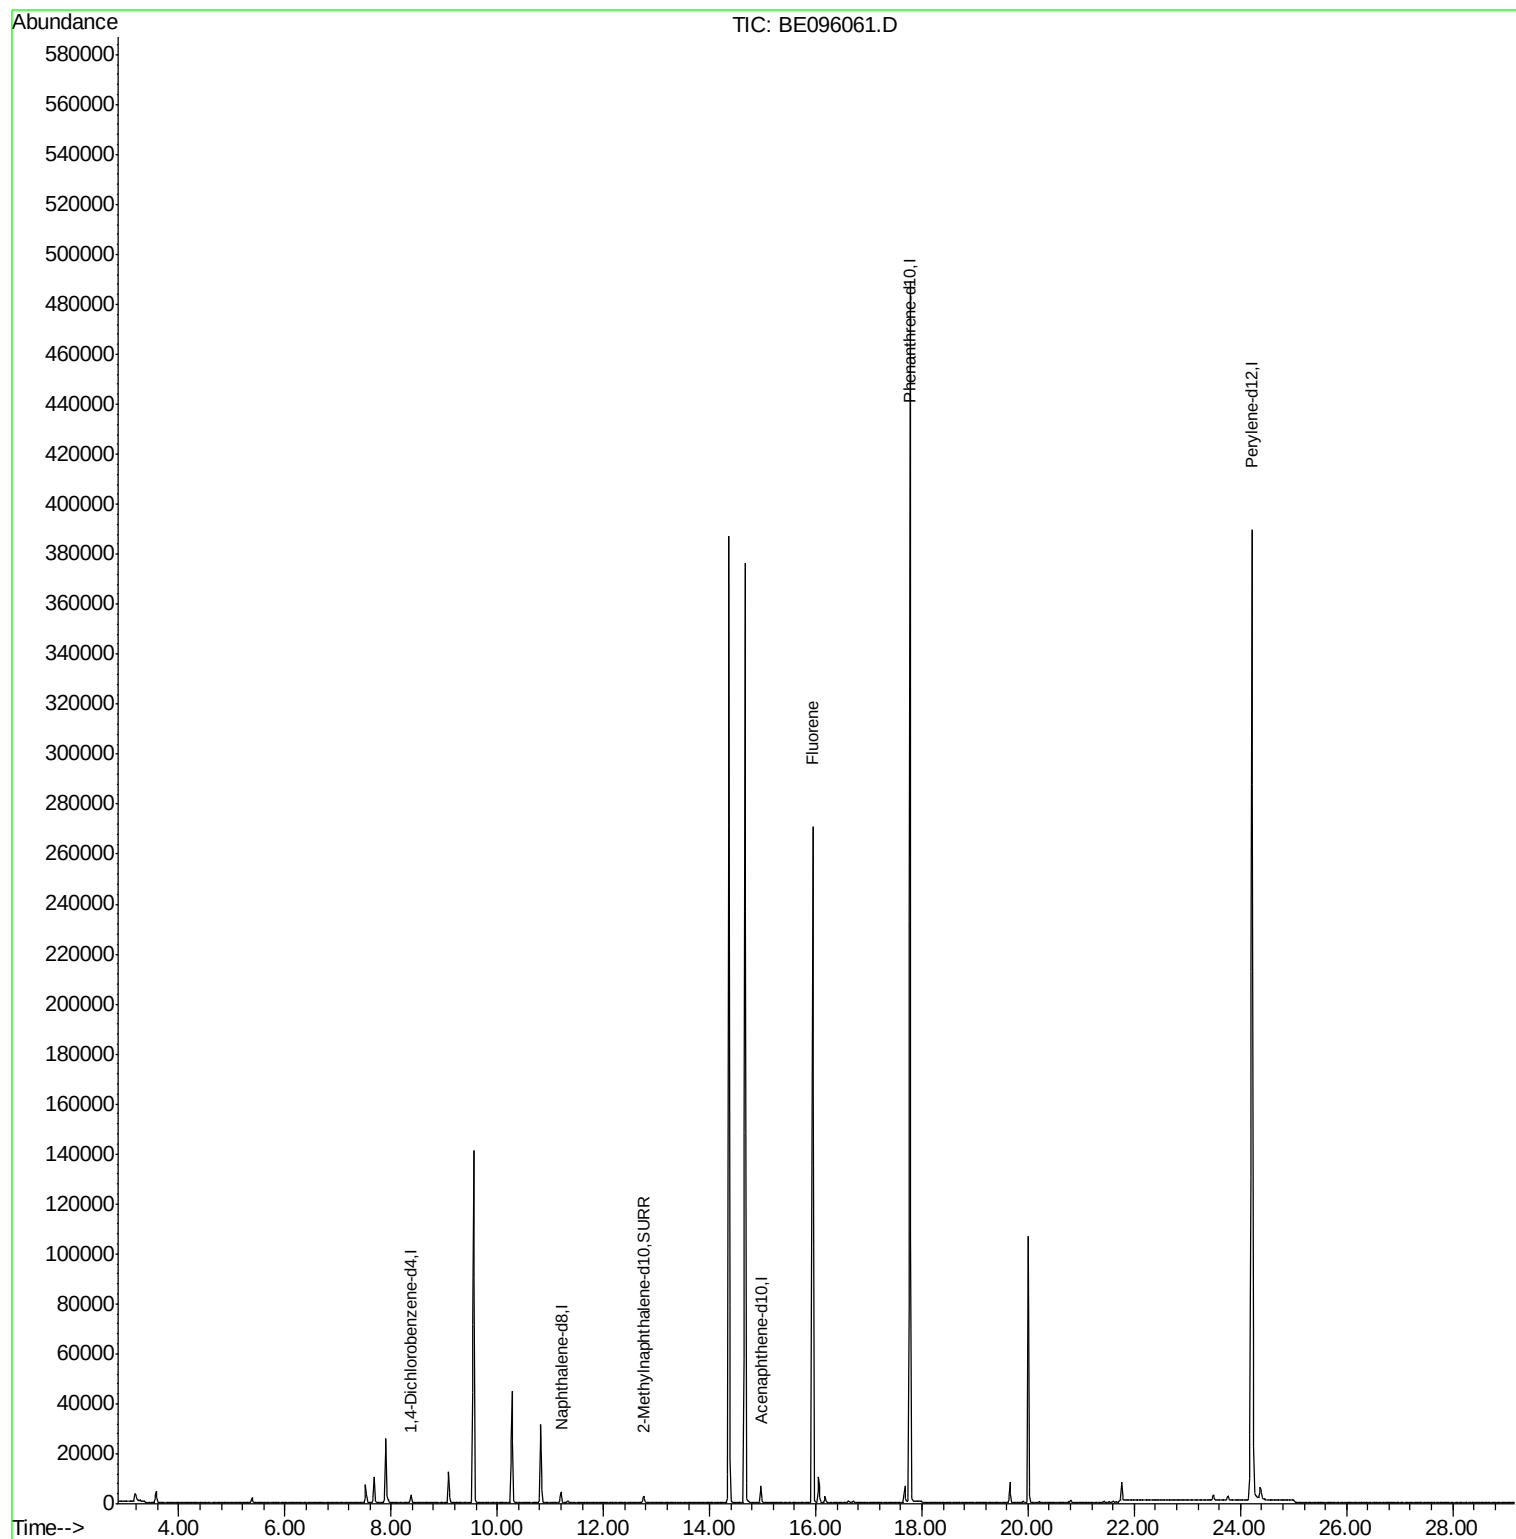

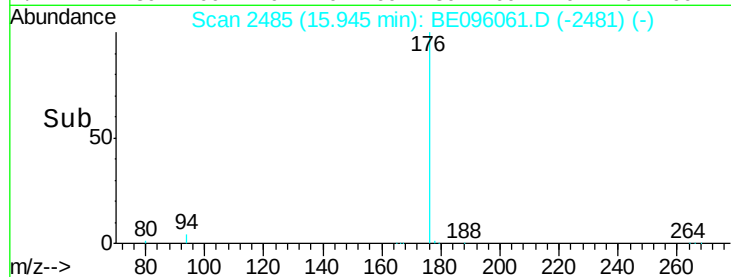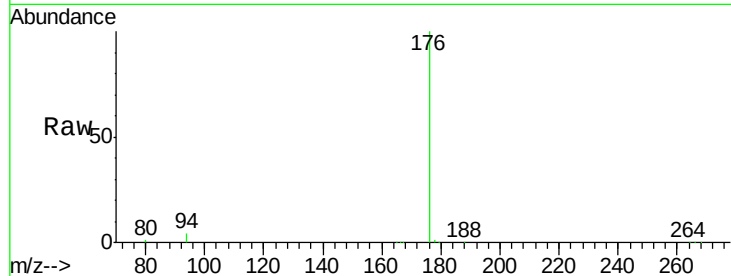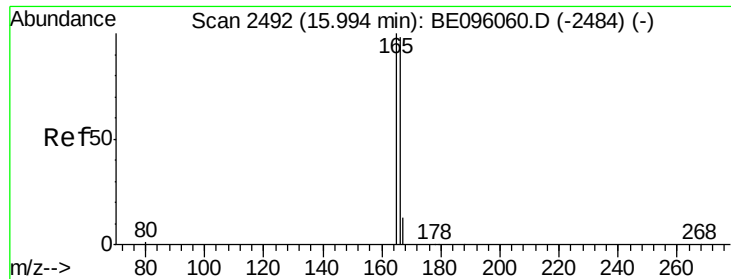

#9

Fluorene

Concen: 0.052 ng/ul

RT: 15.95 min Scan# 2485

Delta R.T. -0.05 min

Lab File: BE096061.D

Acq: 21 Apr 2018 3:38

Instrument :

BNA_E

ClientSampleId :

A3XZ8

Tot Ion:166 Resp: 781

Ion Ratio Lower Upper

166 100

165 11.6 73.4 110.2#

167 42.1 14.6 22.0#

