

Quantitation Report (QT Reviewed)


Instrument :
BNA_E
Client Sampled :
C0AC9

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:36:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

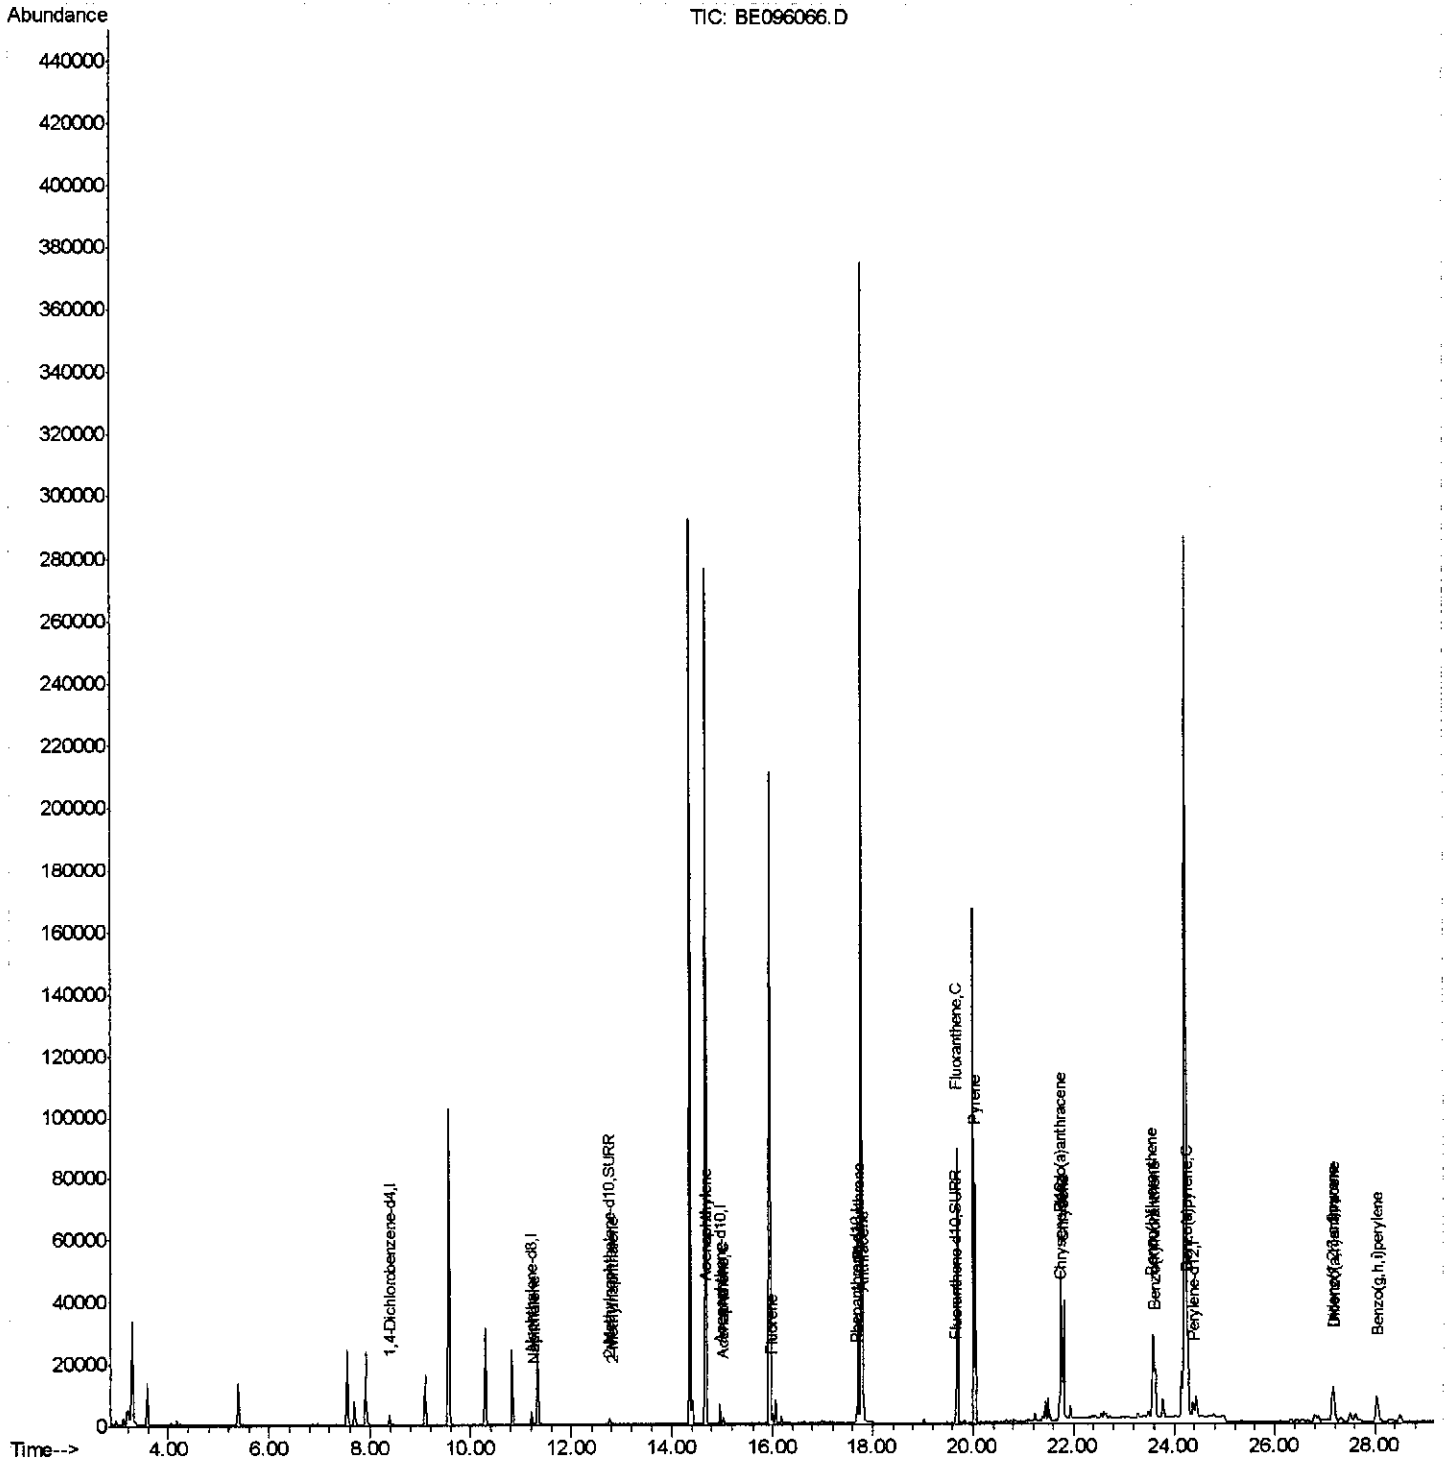




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
APPROVED
 Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 01:09:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

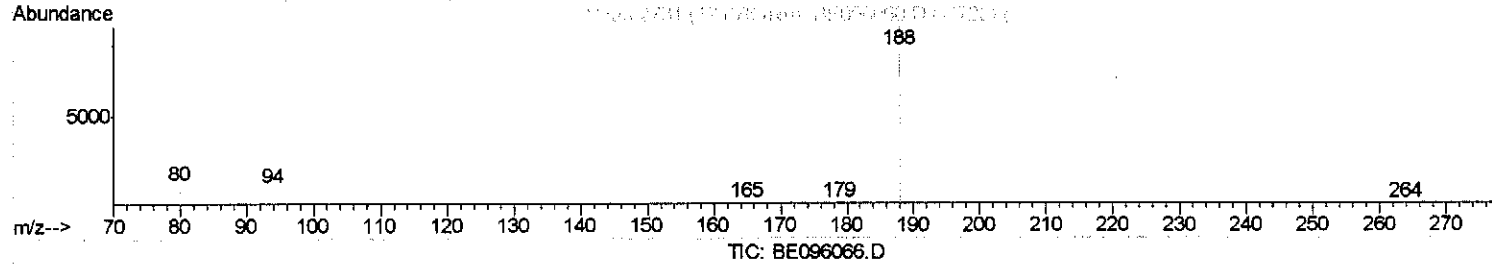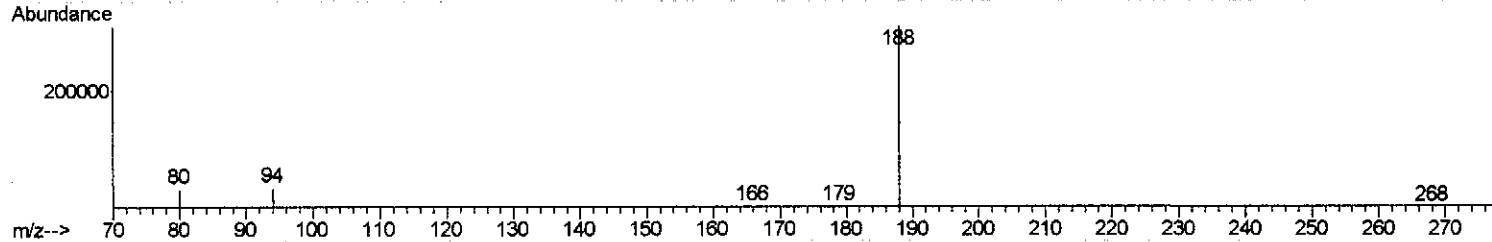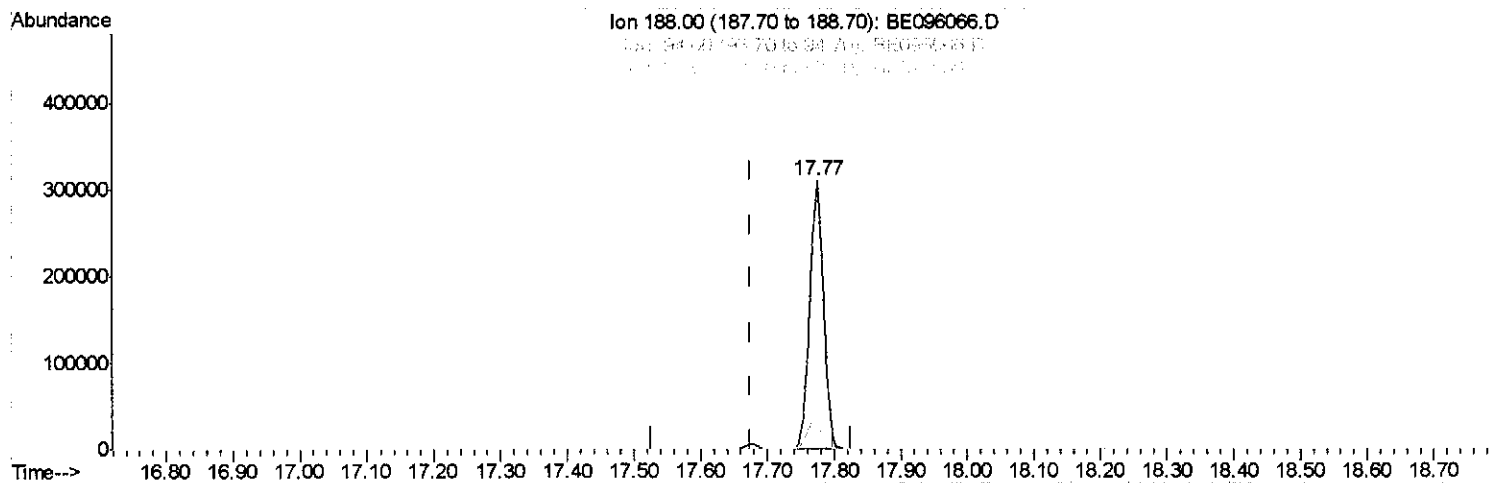

(10) Phenanthrene-d10 (I)
 17.774min (+0.098) 0.40ng/ul
 response 432732

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.59
80.00	11.80	9.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 01:09:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

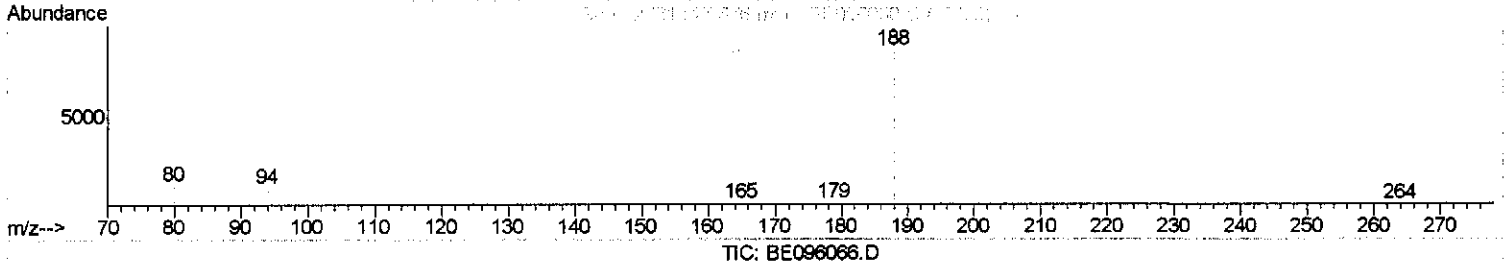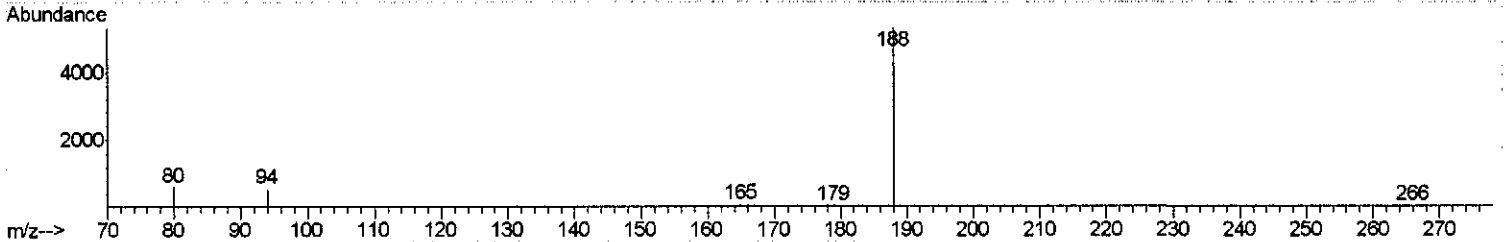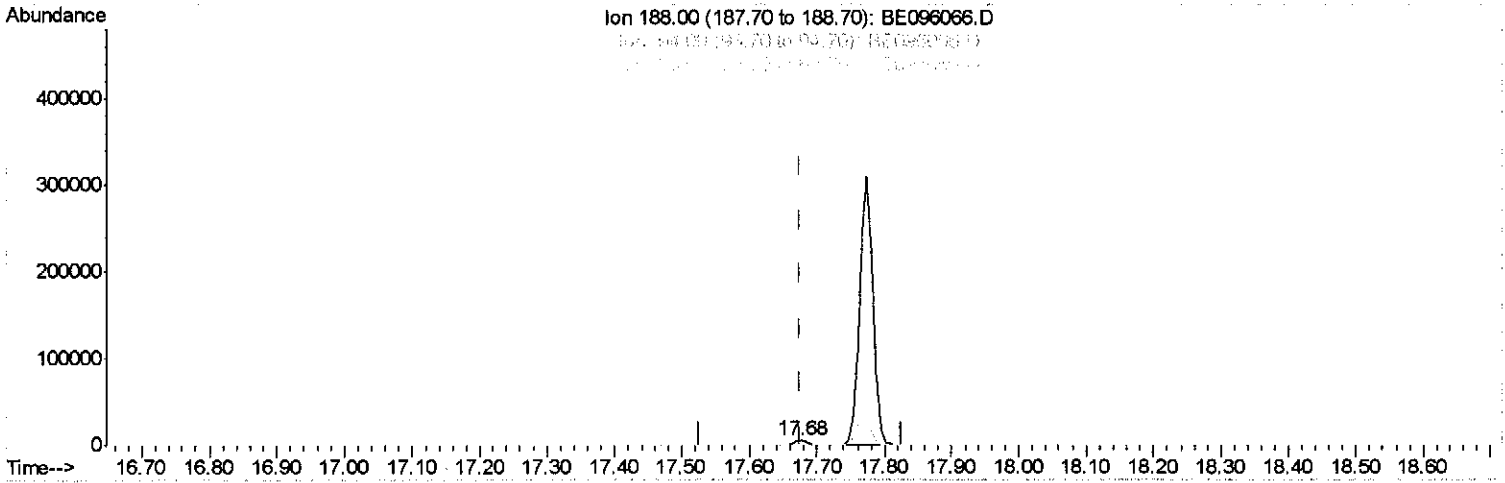

(10) Phenanthrene-d10 (I)

17.676min (-0.000) 0.40ng/ul m) SJ 4/24/18

response 7404

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.54
80.00	11.80	11.58
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
 APPROVED
 Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

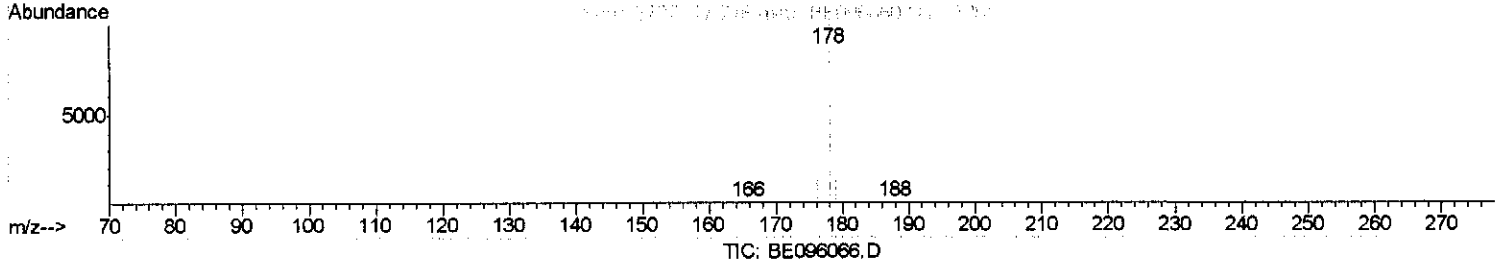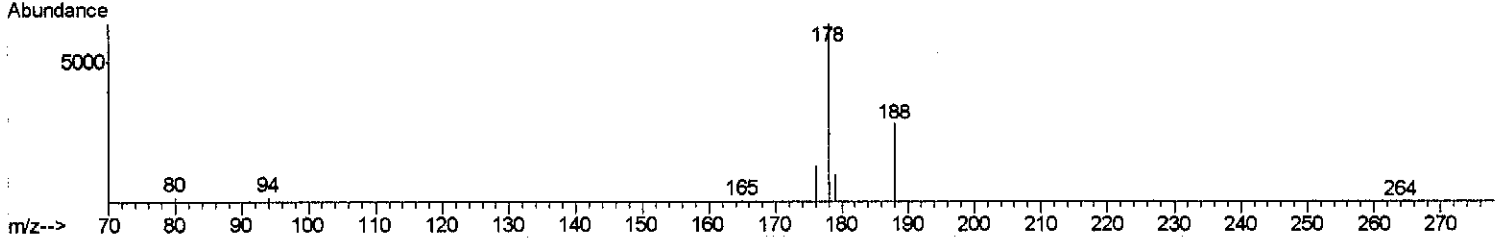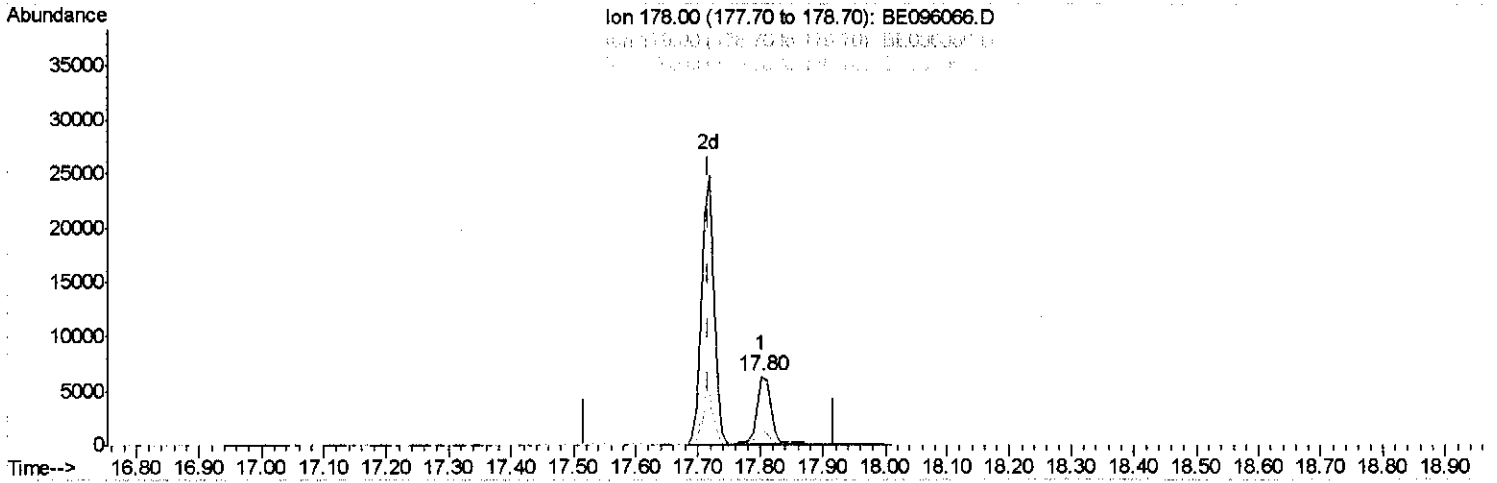

(12) Phenanthrene

17.802min (+0.084) 0.45ng/ul

response 9766

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.80#
176.00	17.00	20.46#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
 APPROVED
 Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

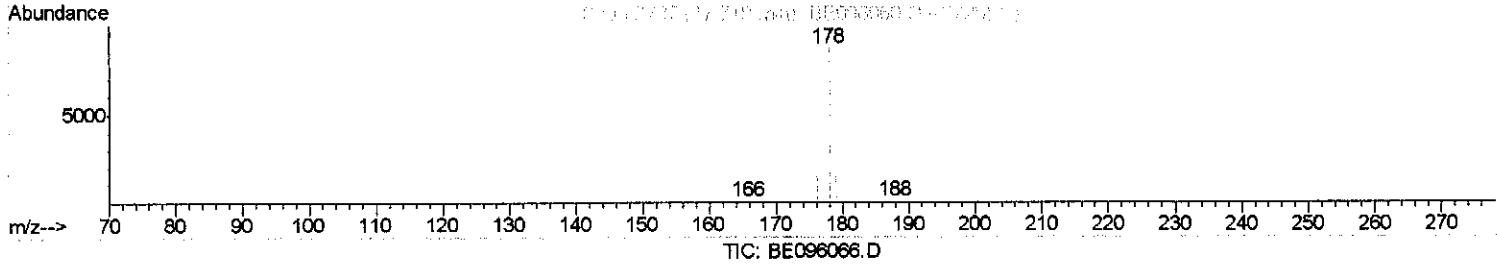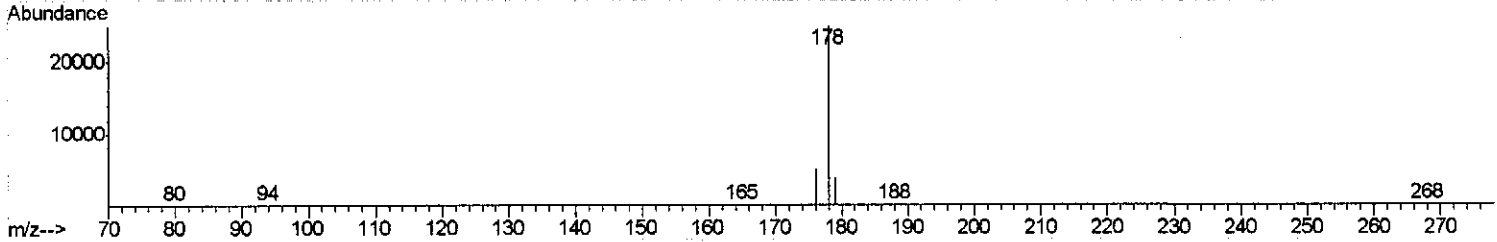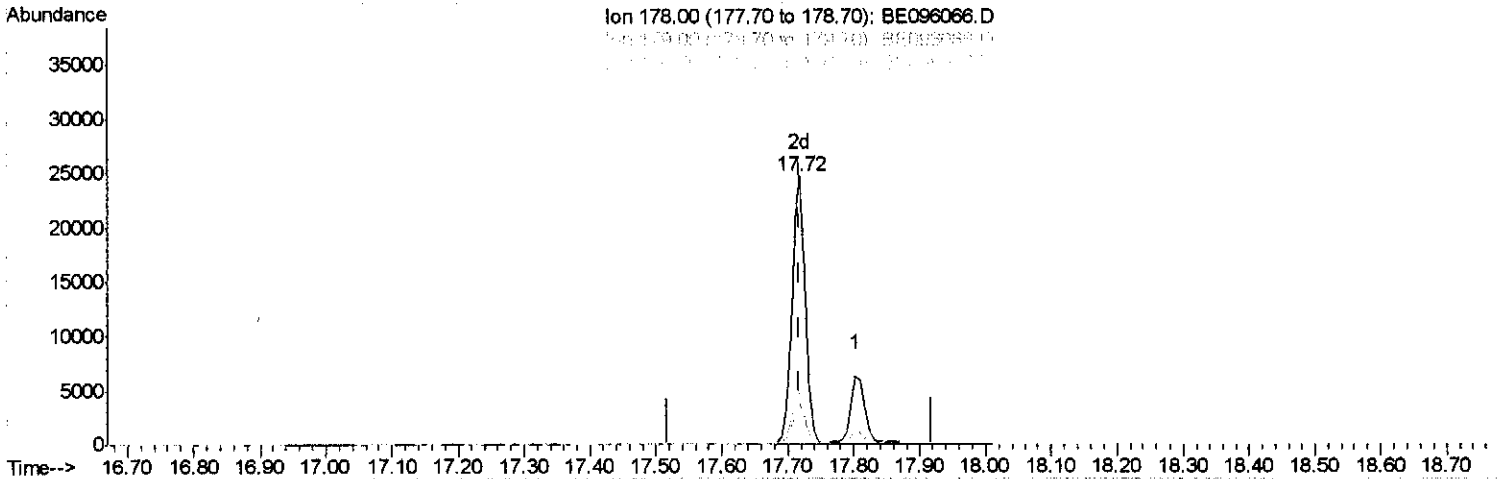

(12) Phenanthrene

17.718min (-0.000) 1.61ng/ul m

SJ 4/24/18

response 35064

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.55#
176.00	17.00	19.71
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument :
BNA_E
ClientSampled :
C0AC9

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

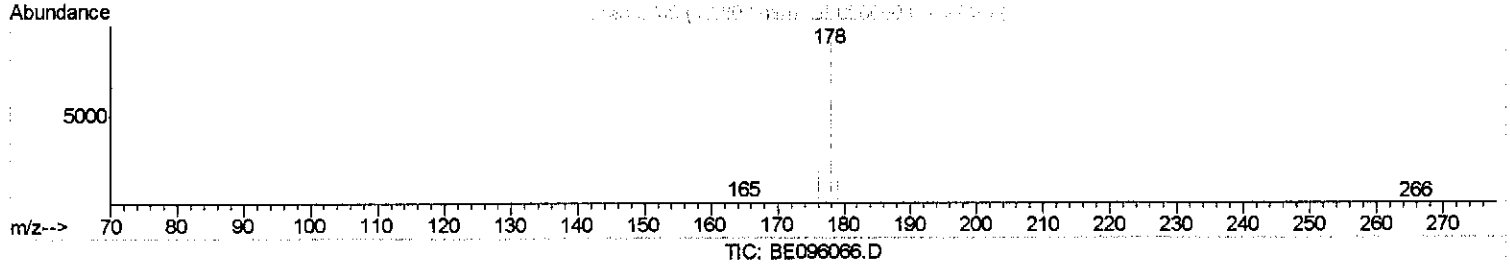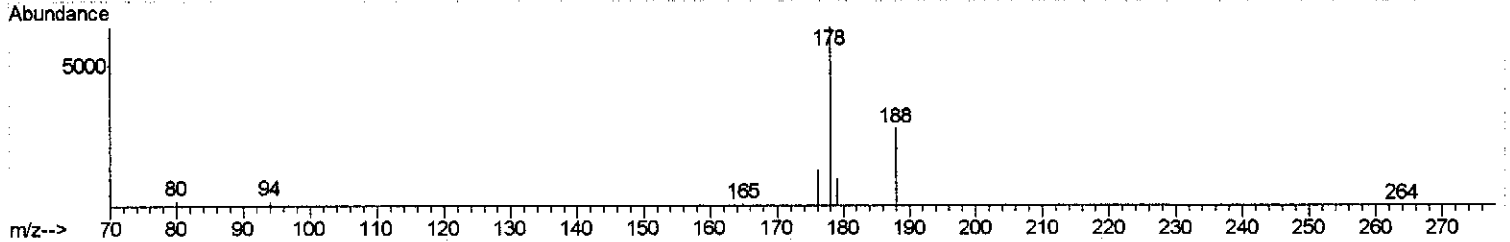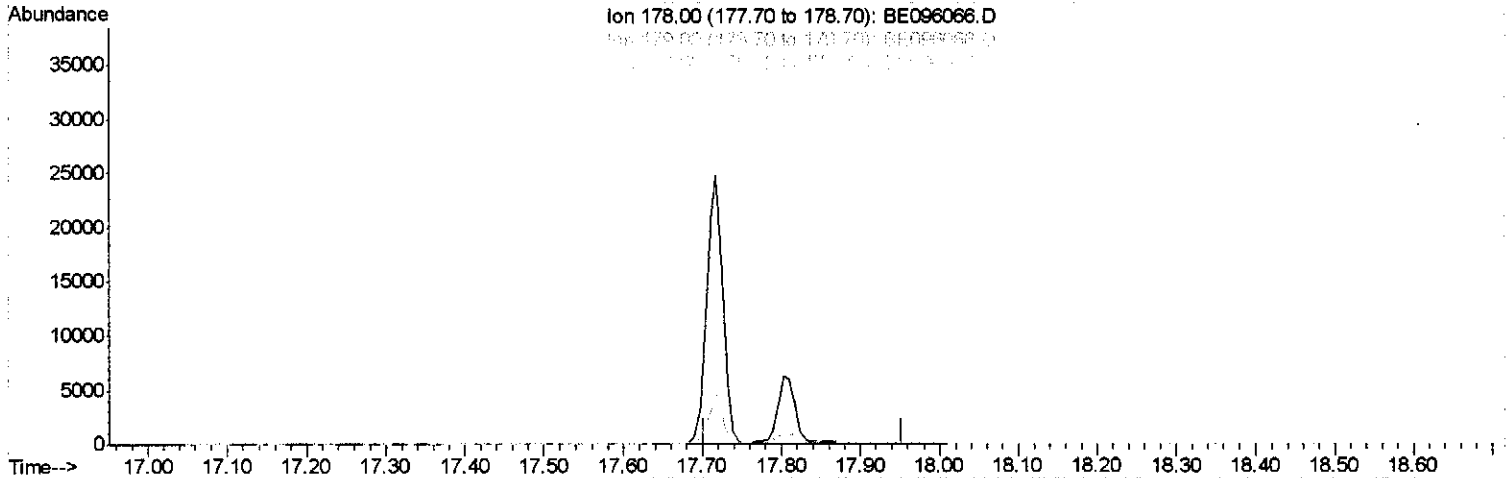

(13) Anthracene

17.803min (-17.803) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	22.60	0.00#
176.00	18.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 Client Sampled :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

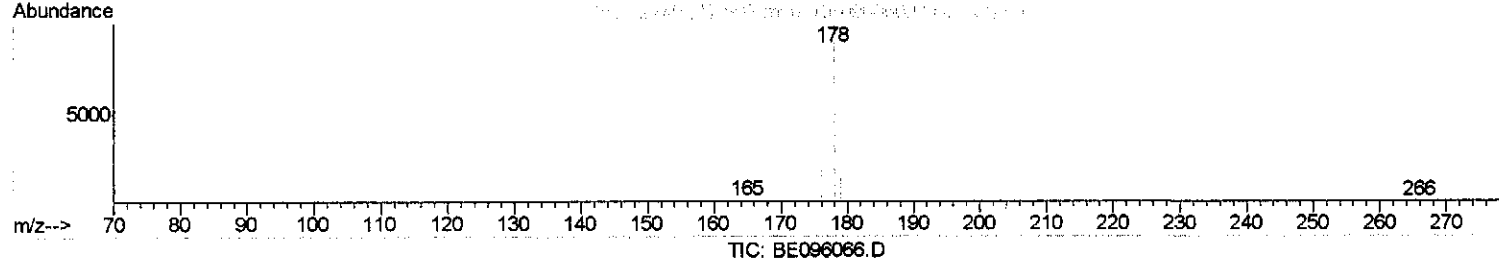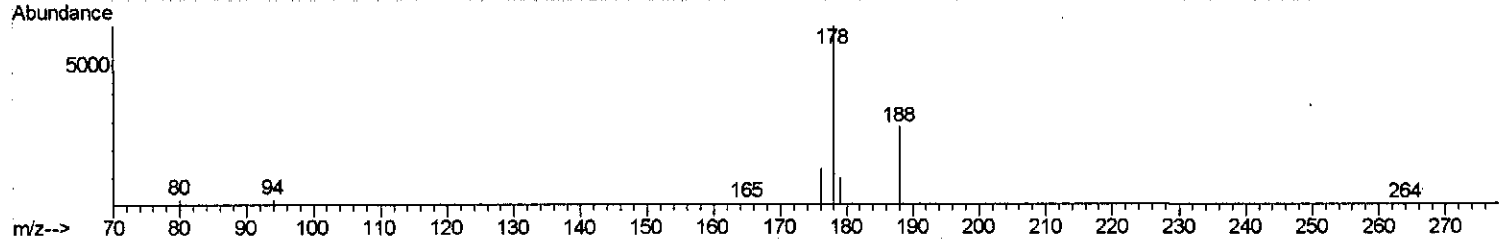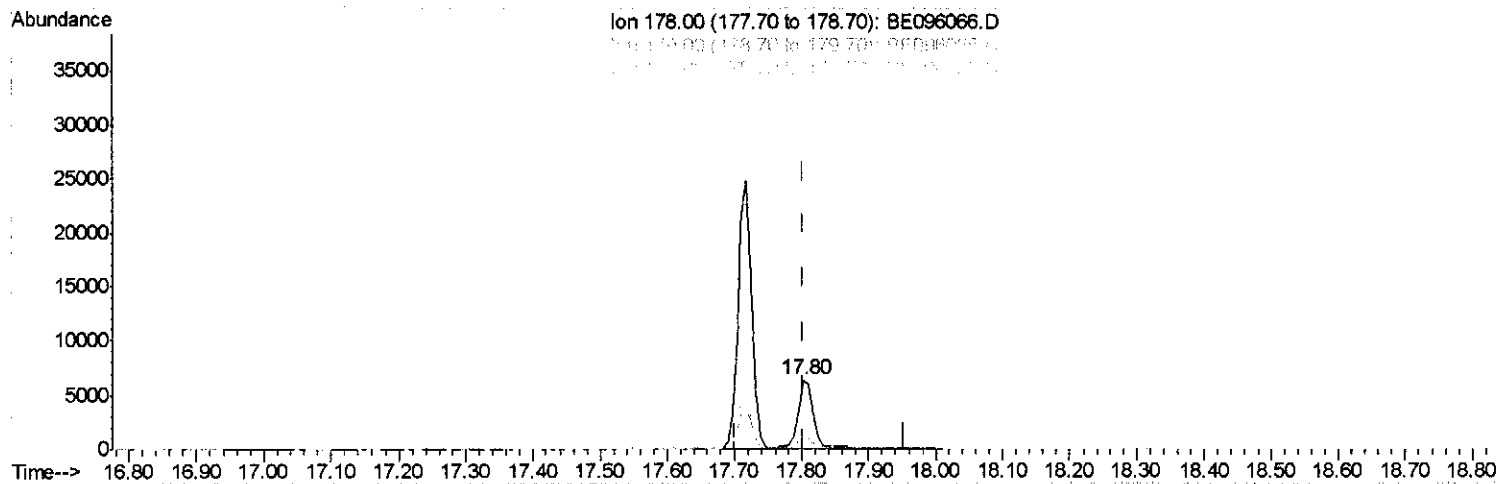

(13) Anthracene
 17.802min (-0.000) 0.43ng/ul m) SJ 4/24/18
 response 9386

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	15.80#
176.00	18.40	20.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC9

Manual Integrations
APPROVED

Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

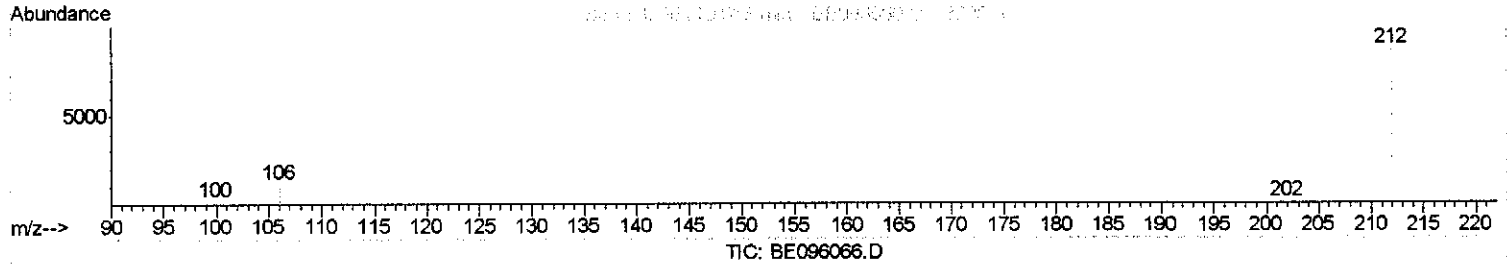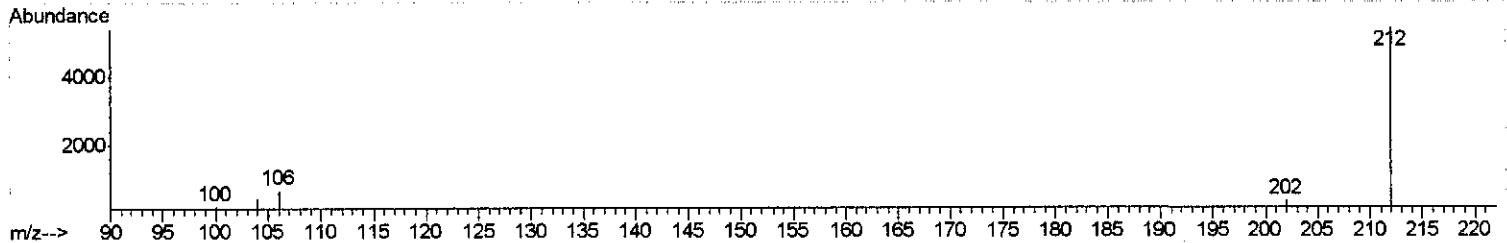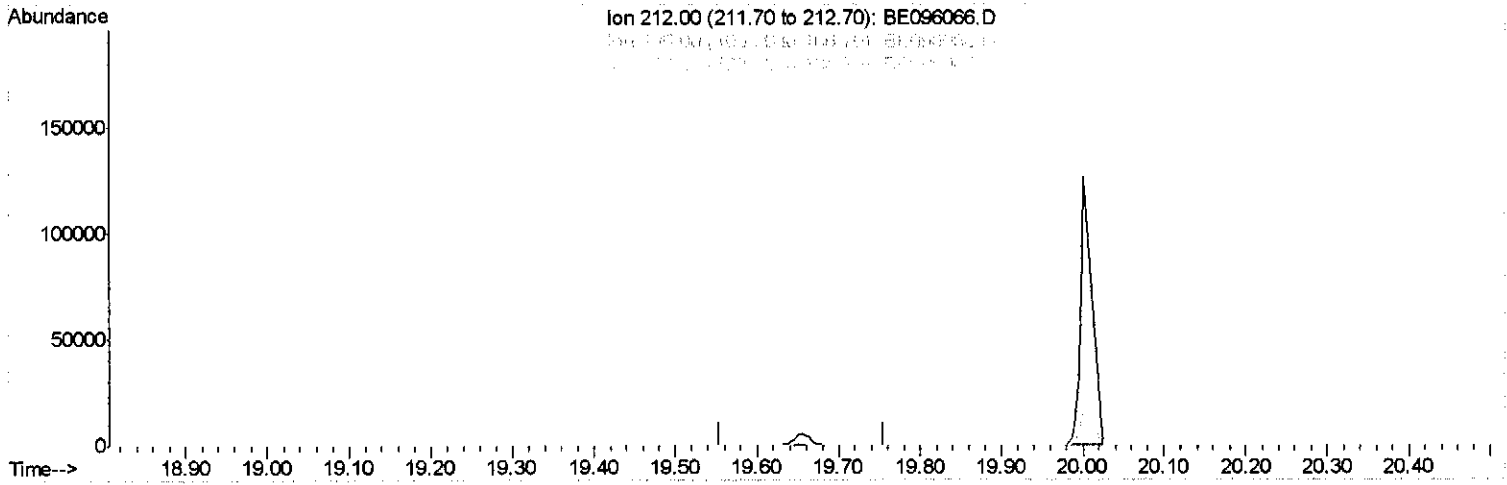

(14) Fluoranthene-d10 (SURR)

19.656min (-19.656) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC9

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

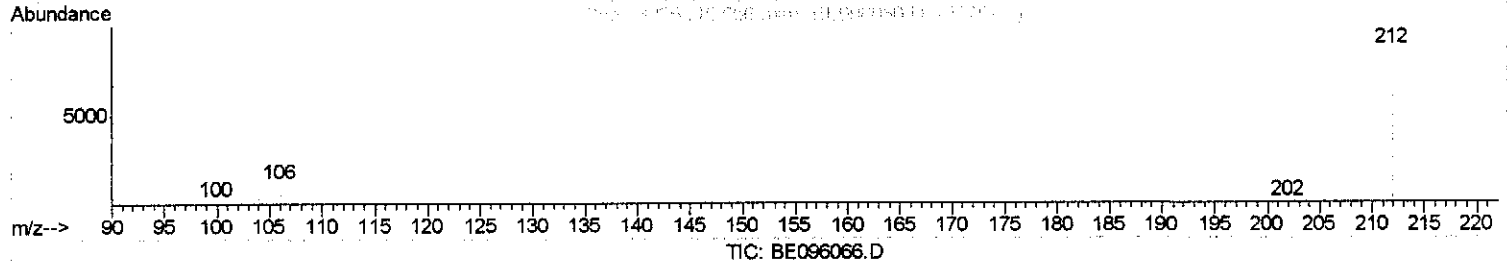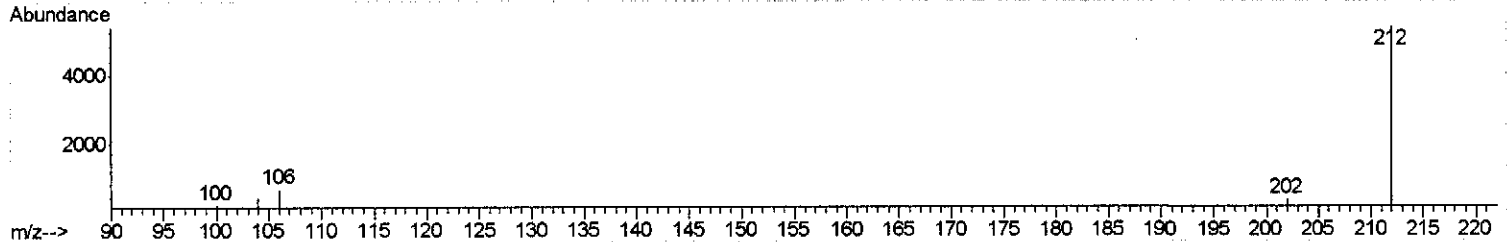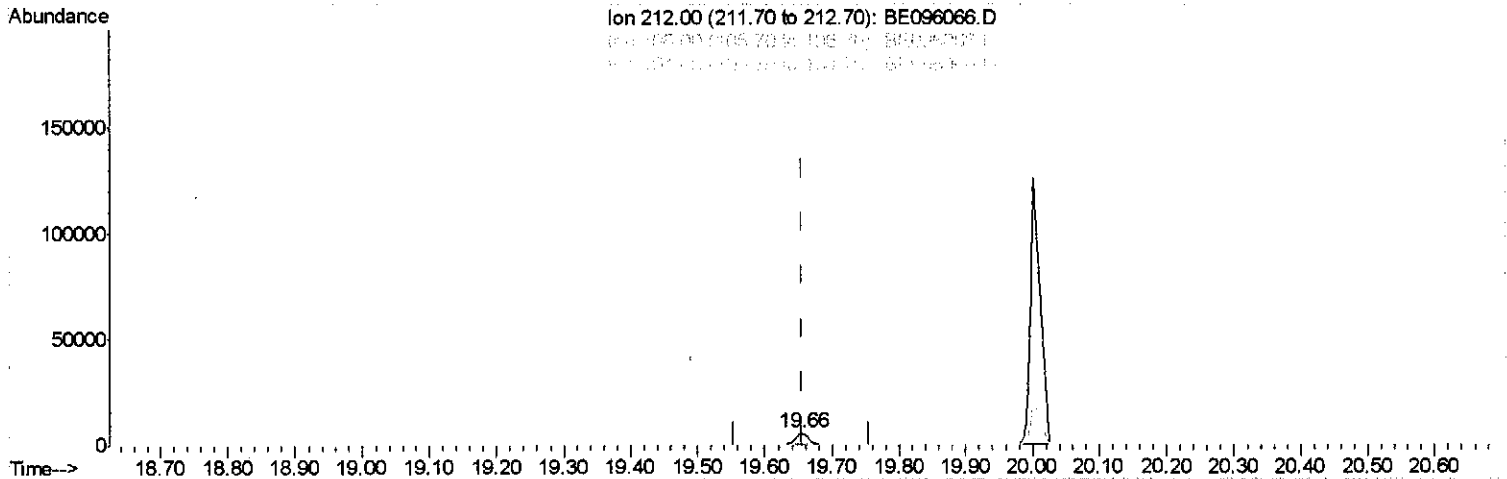

(14) Fluoranthene-d10 (SURR)

19.655min (-0.000) 0.23ng/ul m> SJ 4/24/18

response 7004

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC9

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

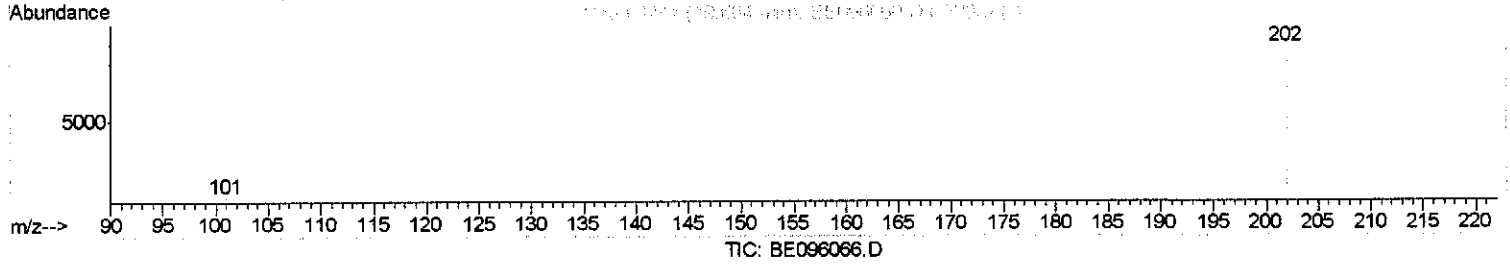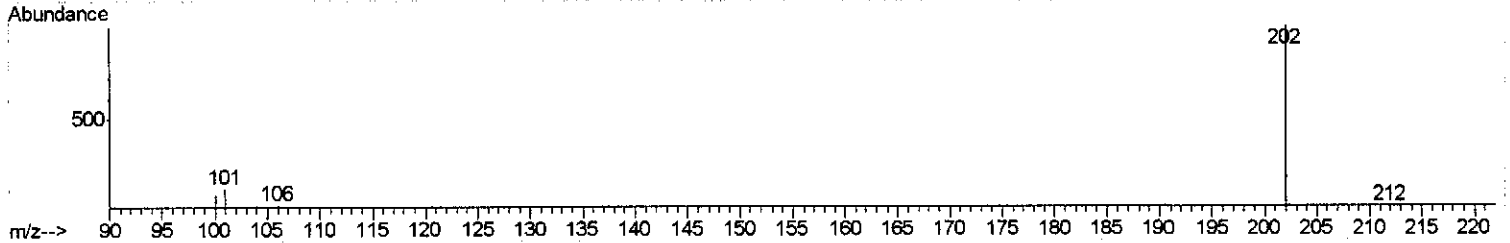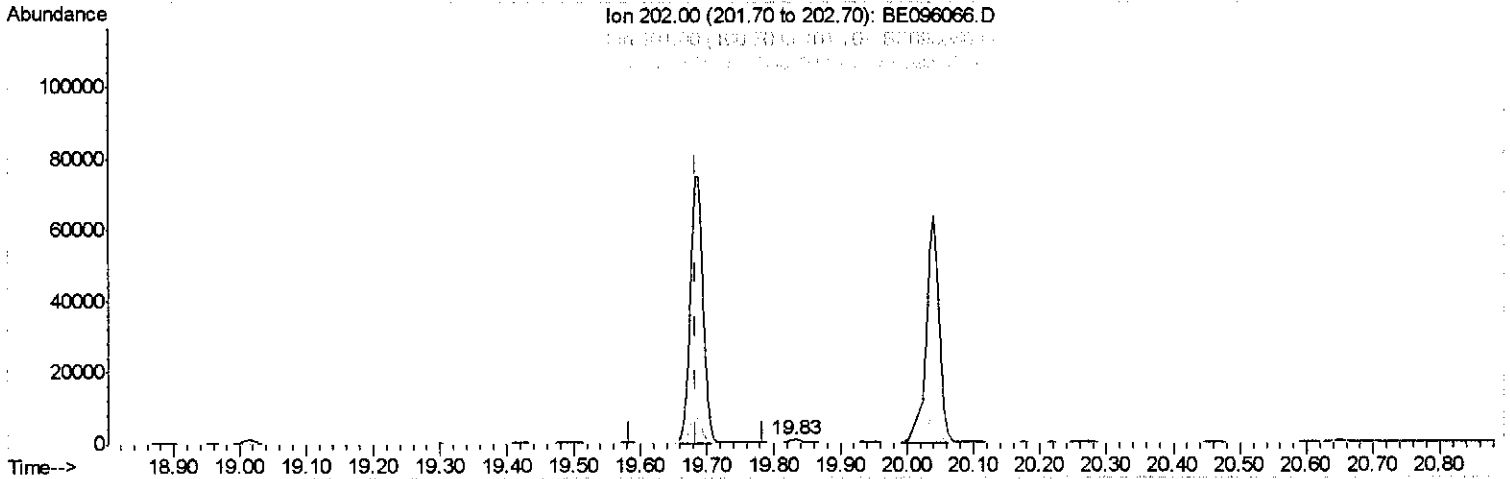

(15) Fluoranthene (C)

19.830min (+0.146) 0.04ng/ul

response 1180

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	16.46
100.00	19.50	13.82
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC9

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

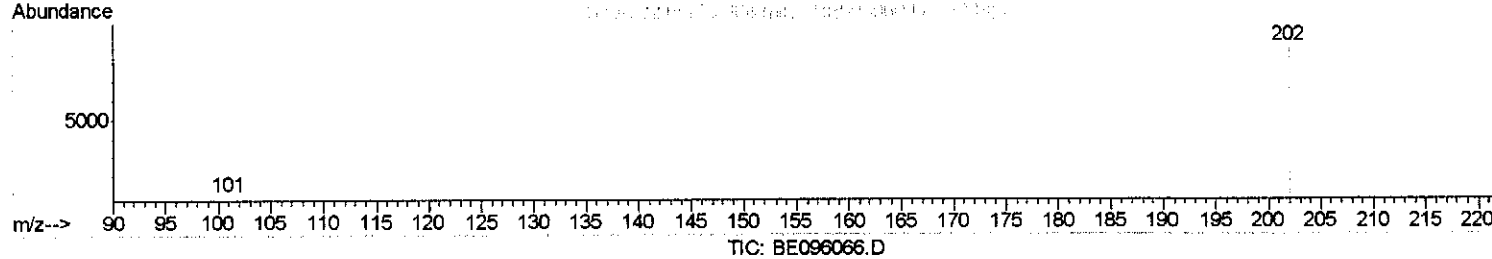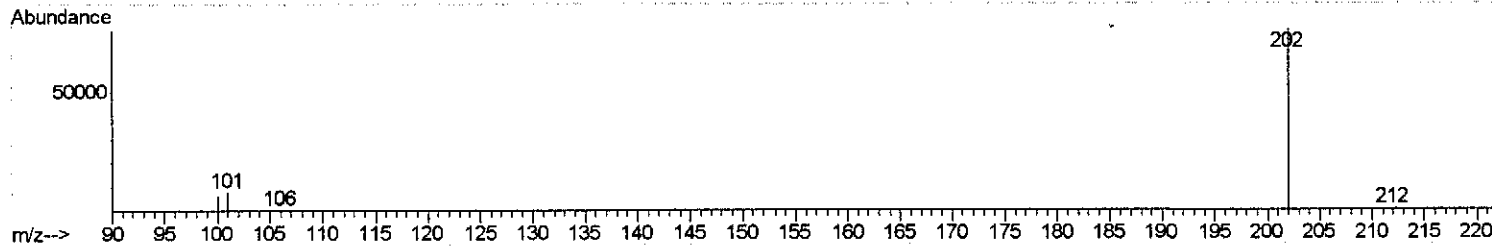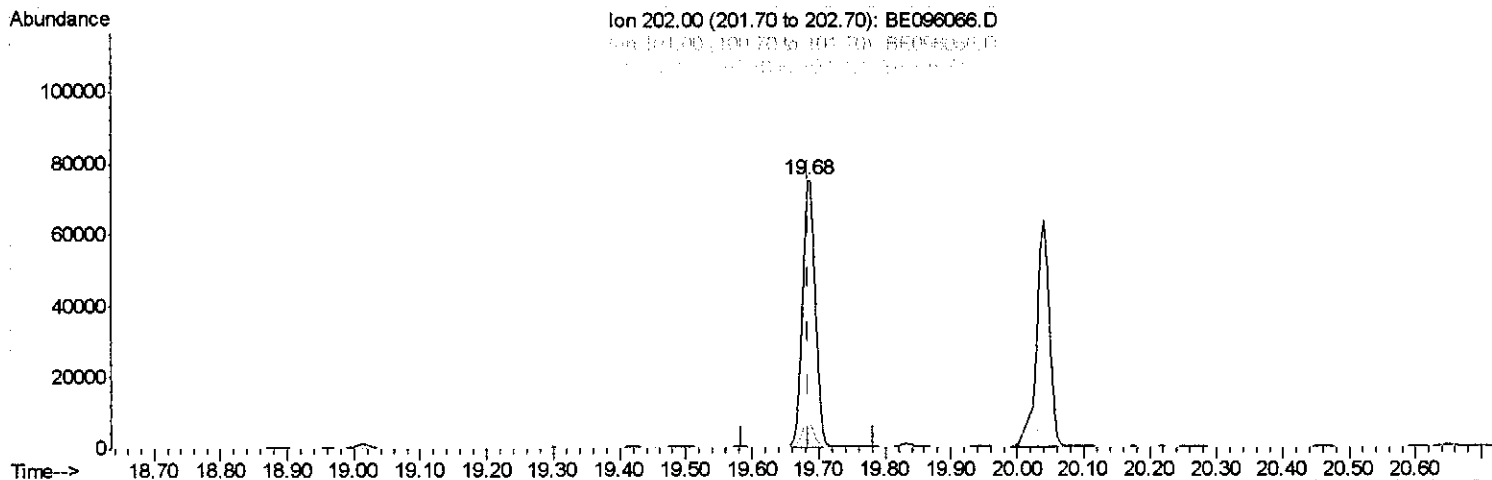

(15) Fluoranthene (C)

19.684min (-0.000) 3.28ng/ul m) SJ 4/24/18

response 97357

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.18
100.00	19.50	8.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

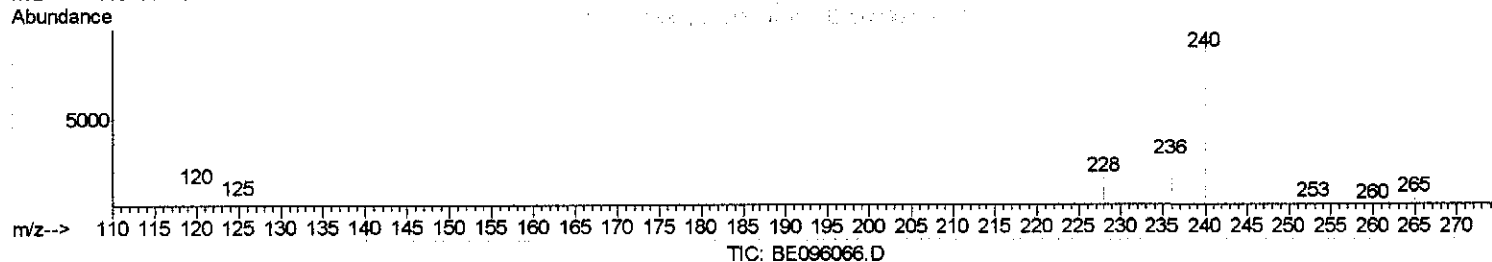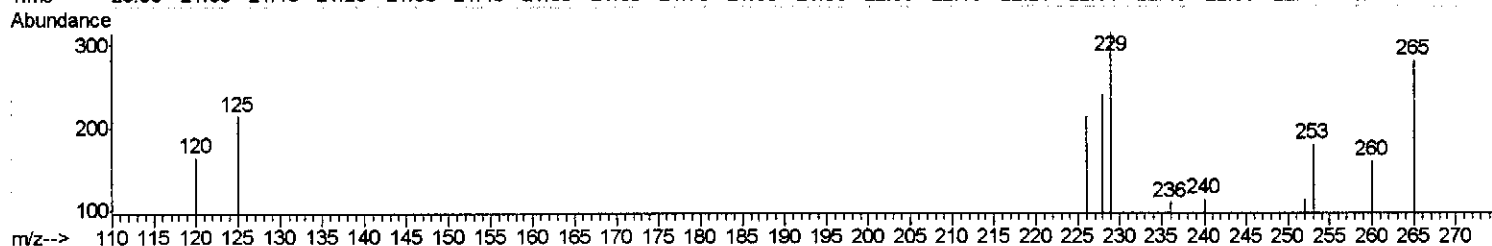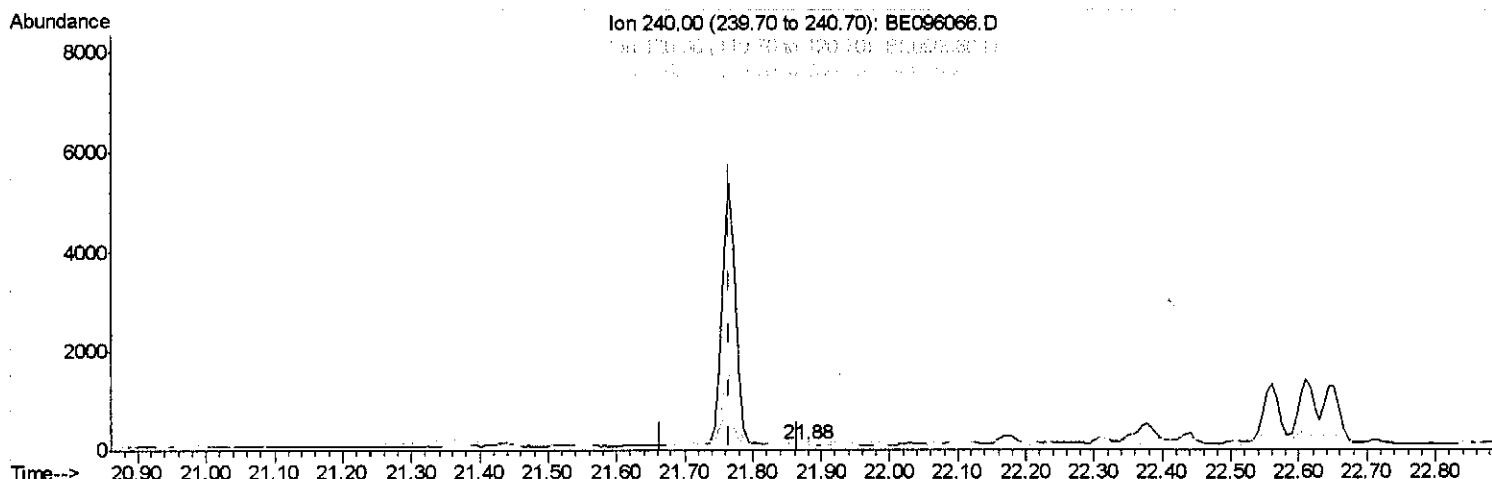

(16) Chrysene-d12 (I)
 21.878min (+0.113) 0.40ng/ul
 response 14

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	146.43#
236.00	34.90	96.43#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC9

Manual Integrations
APPROVED
 Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

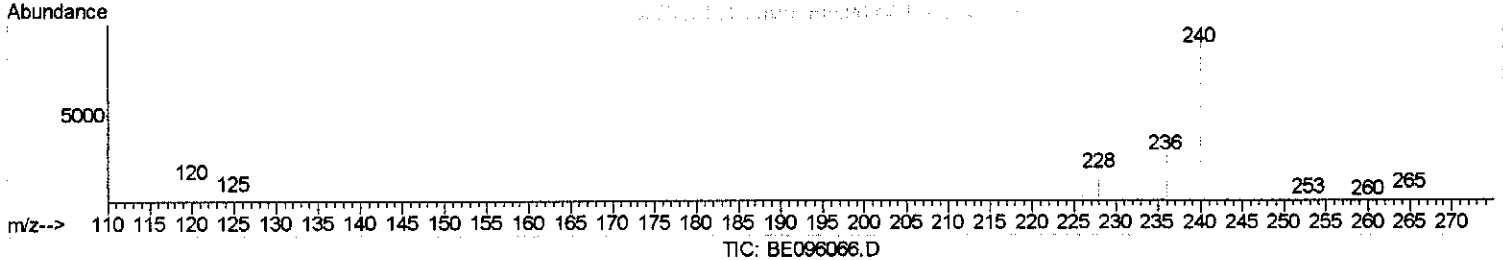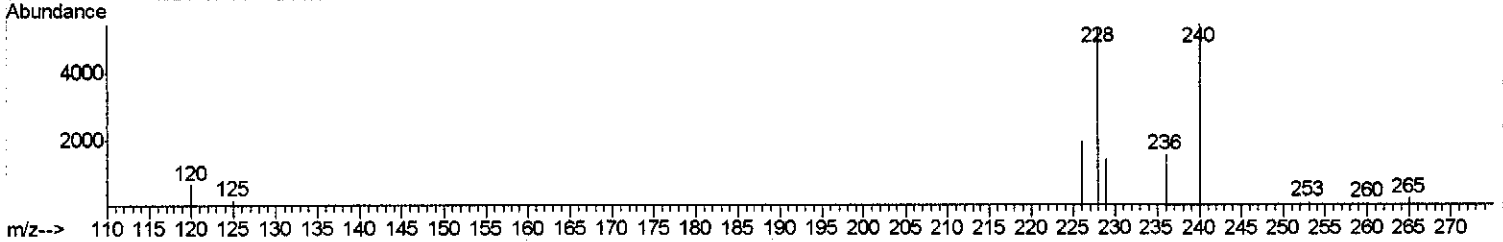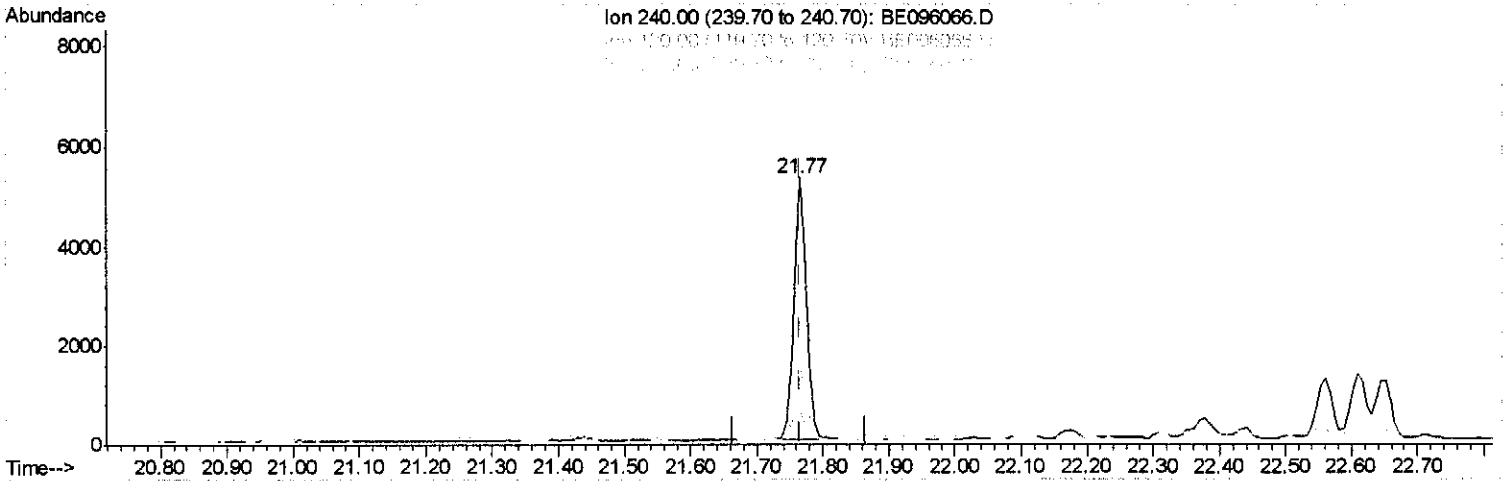

(16) Chrysene-d12 (I)

21.765min (+0.000) 0.40ng/ul m > SJ 4/24/18

response 7135

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.95#
236.00	34.90	28.95
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC9

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

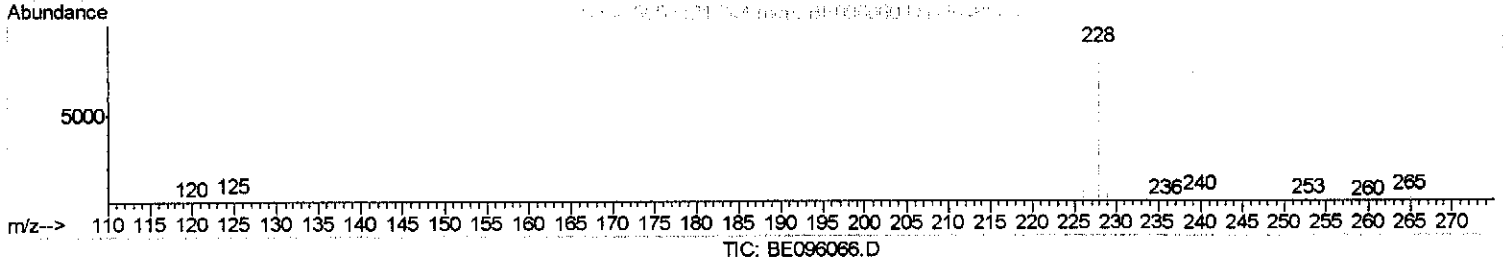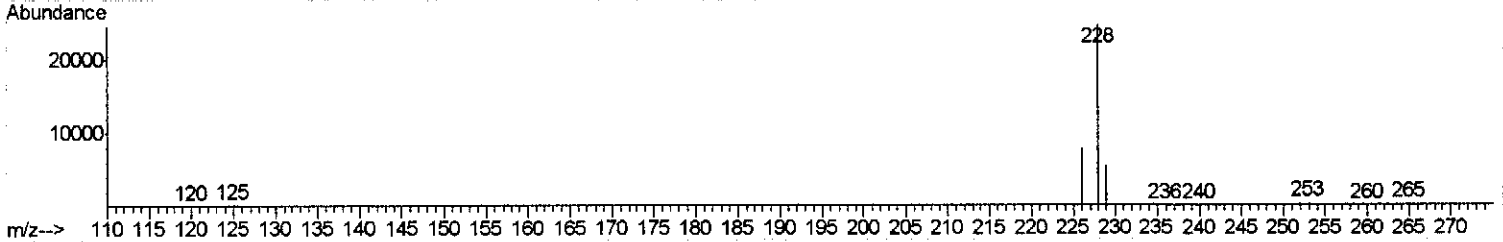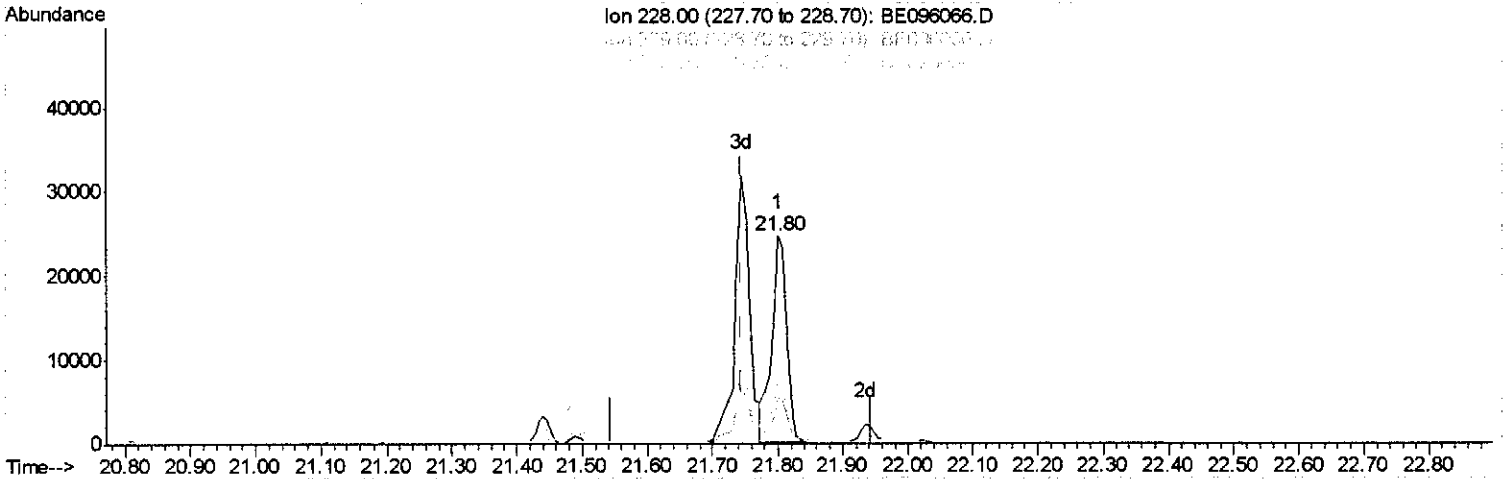

(18) Benzo(a)anthracene

21.800min (+0.056) 1.37ng/ul

response 39493

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	21.96#
226.00	21.30	31.56#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
C0AC9

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

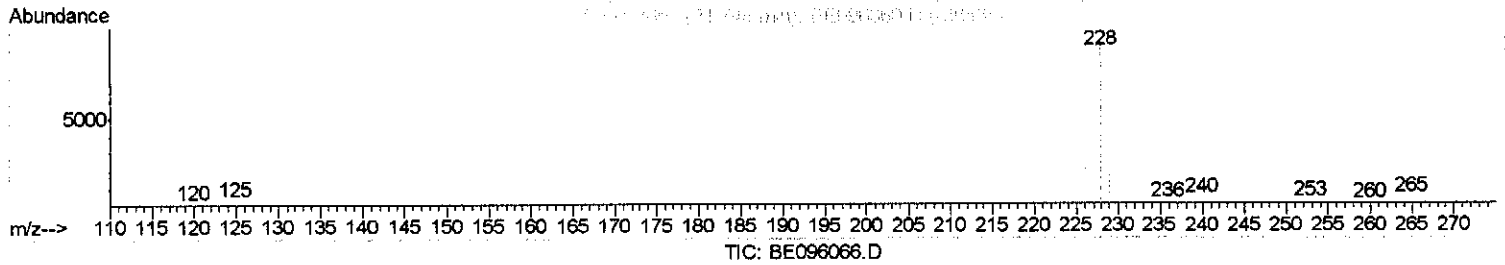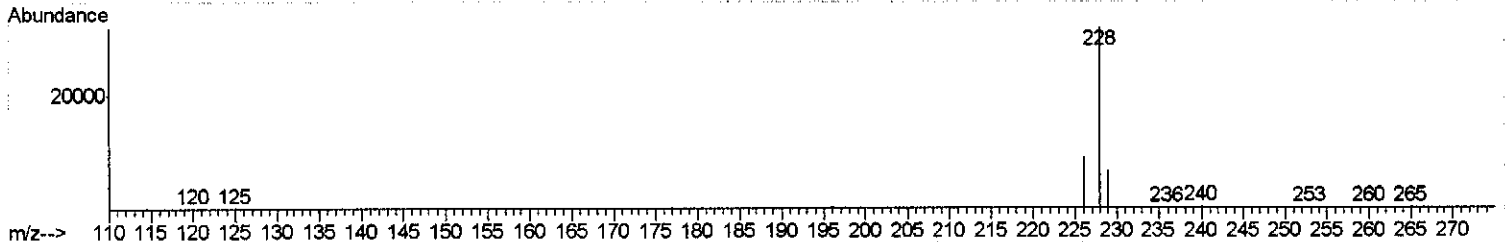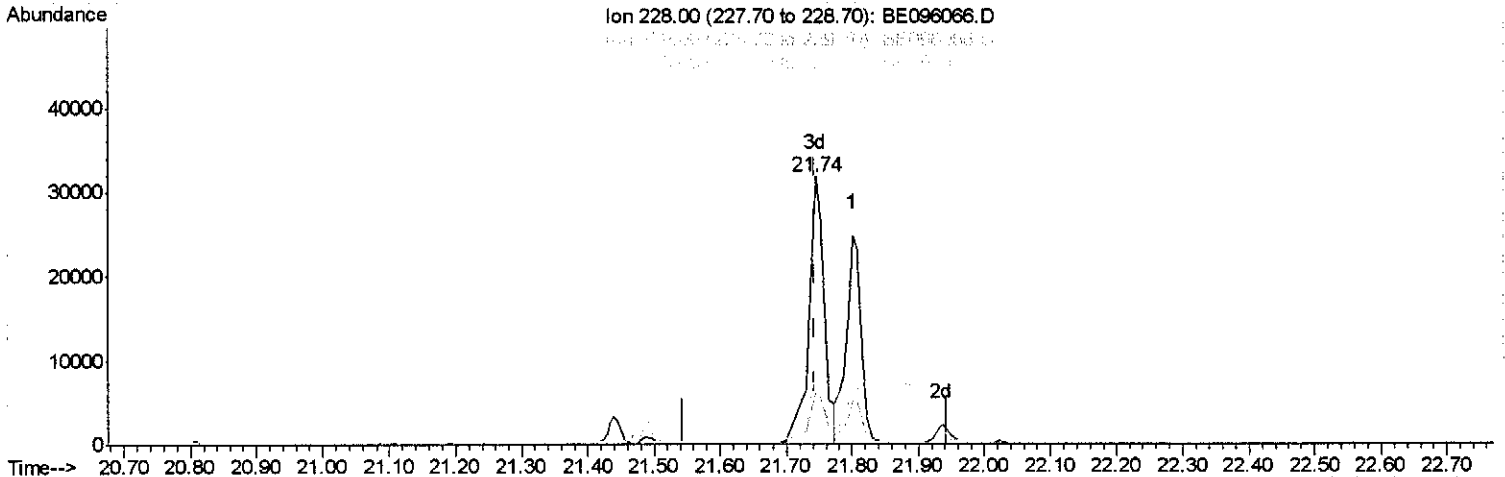

(18) Benzo(a)anthracene

21.744min (+0.000) 1.96ng/ul m) SJ 4/20/18

response 56623

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.58#
226.00	21.30	28.14#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

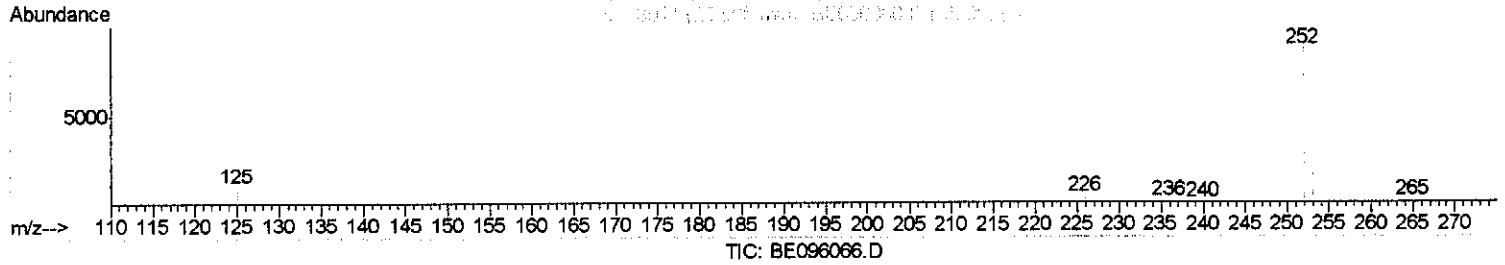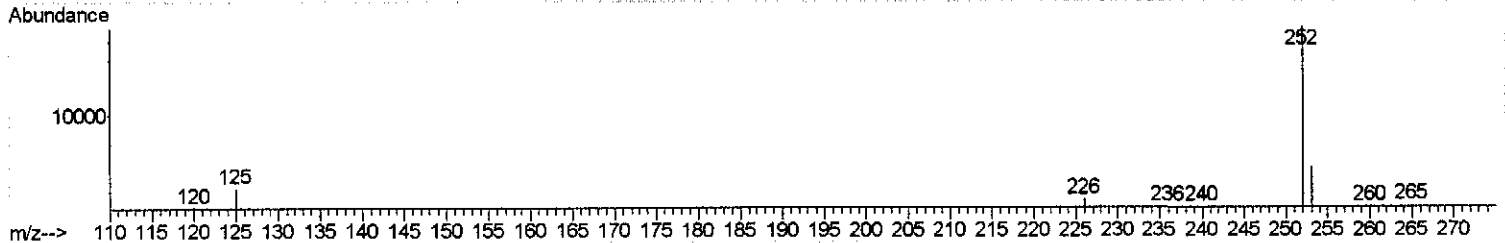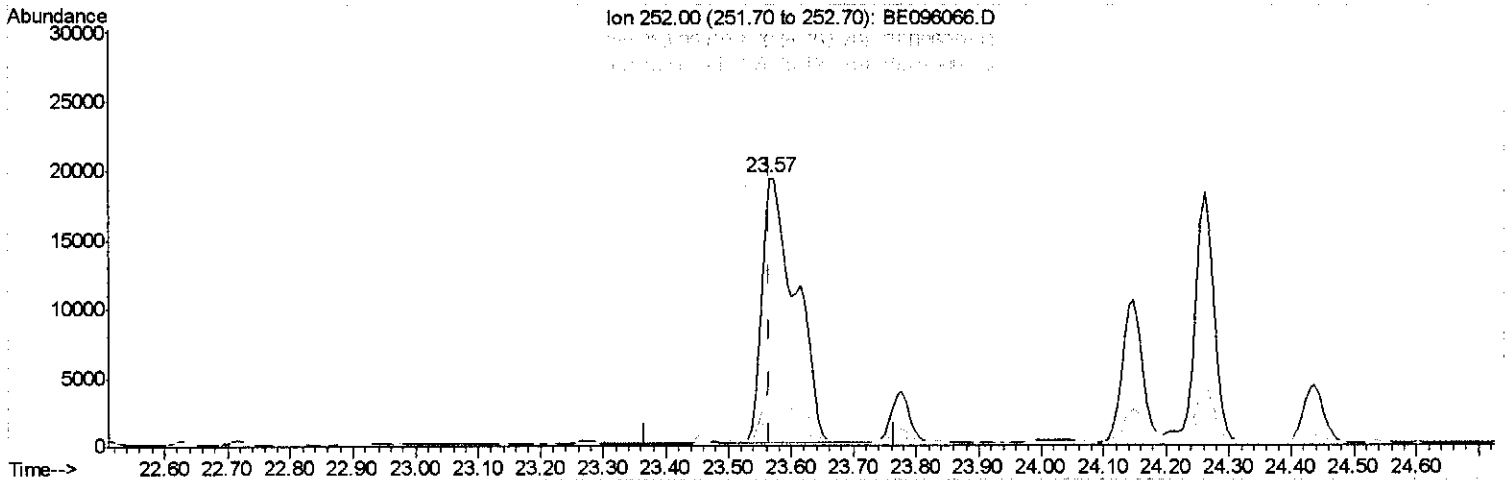

(21) Benzo(b)fluoranthene

23.565min (+0.000) 2.48ng/ul

response 71205

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.25
125.00	17.50	11.59
0.00	0.00	0.00



Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleID :
 C0AC9

Manual Integrations
 APPROVED
 Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

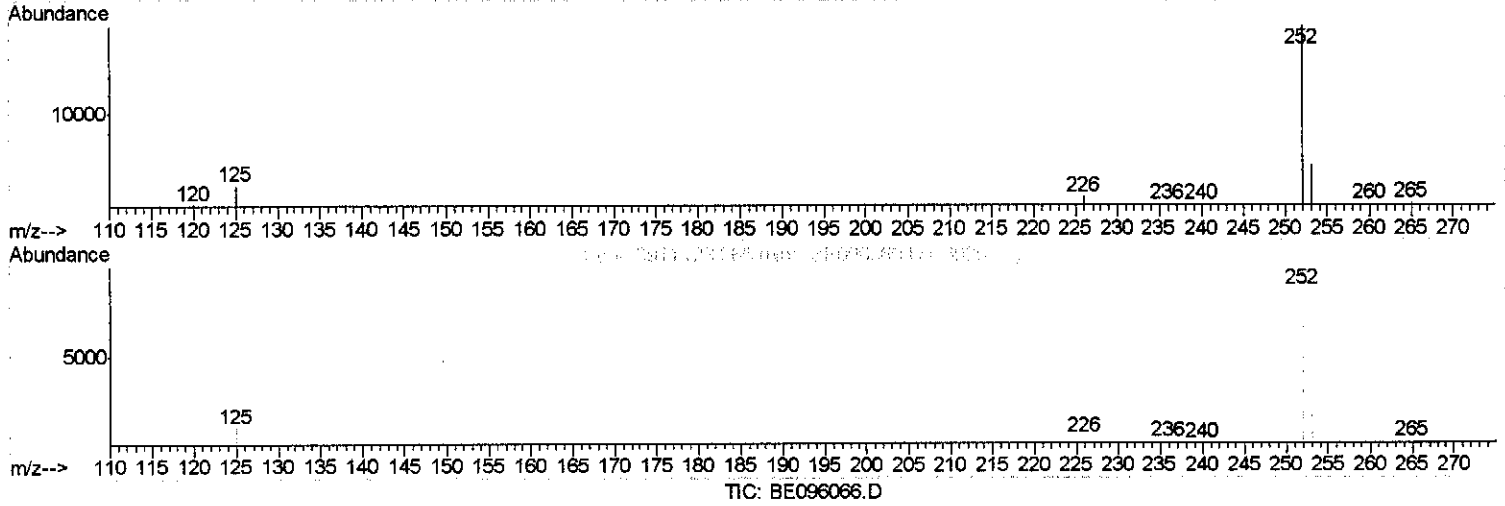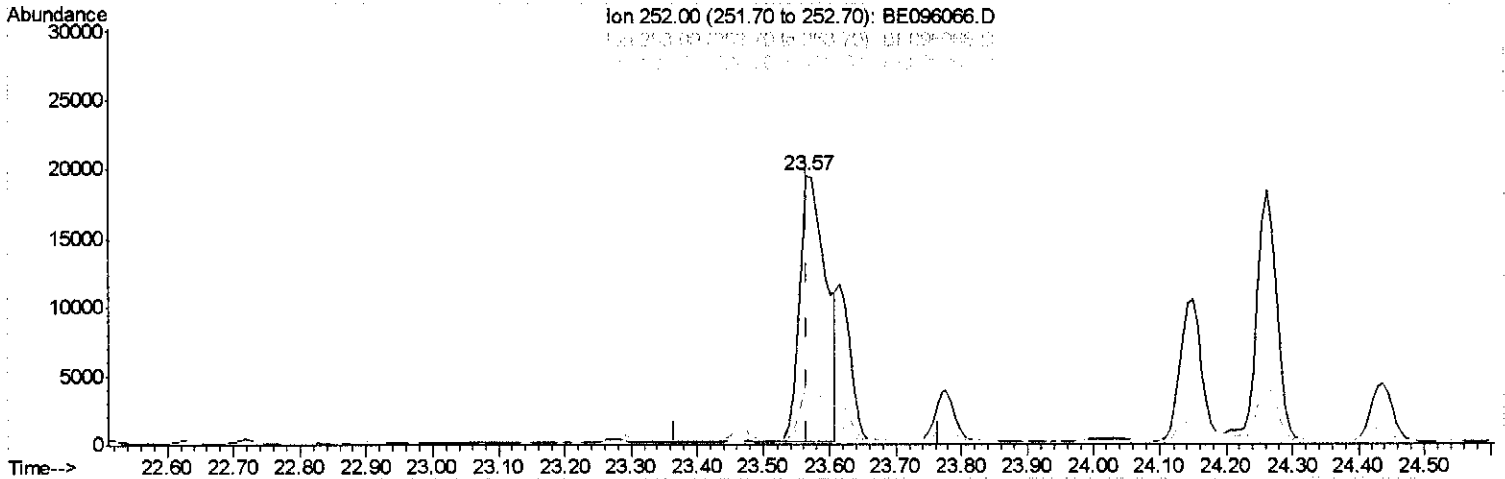

(21) Benzo(b)fluoranthene

23.565min (+0.000) 1.93ng/ul m > SJ 4/24/18

response 55476

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.25
125.00	17.50	11.59
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096066.D
 Acq On : 21 Apr 2018 6:37
 Operator : SJ/JU
 Sample : J2434-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC9

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 23 01:07:45 2018
 Response via : Initial Calibration

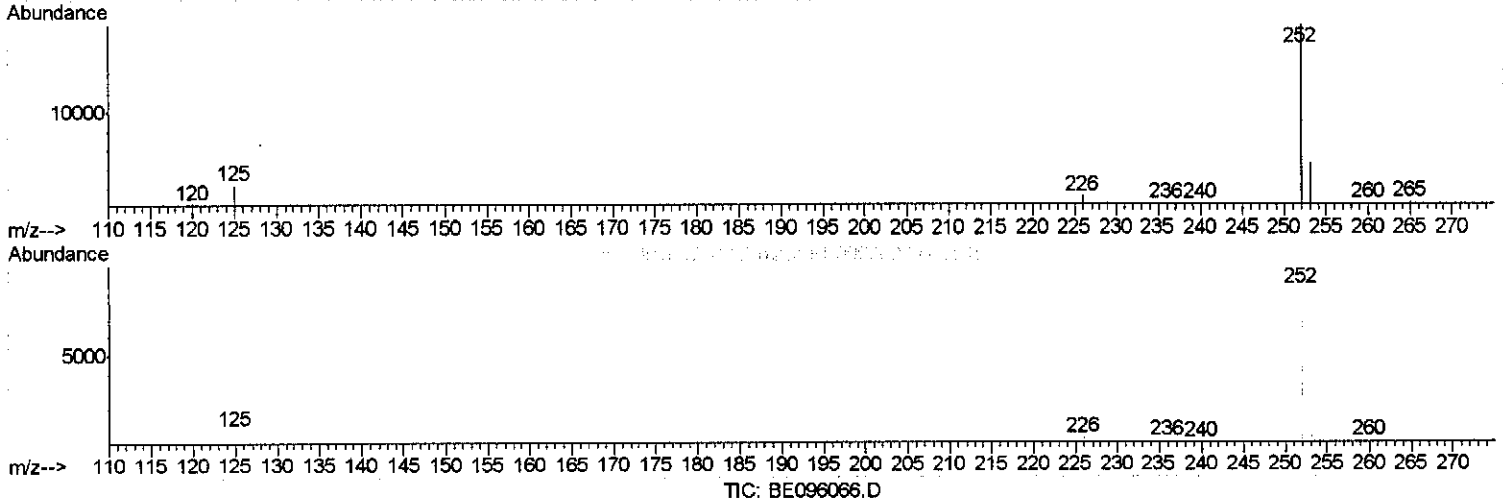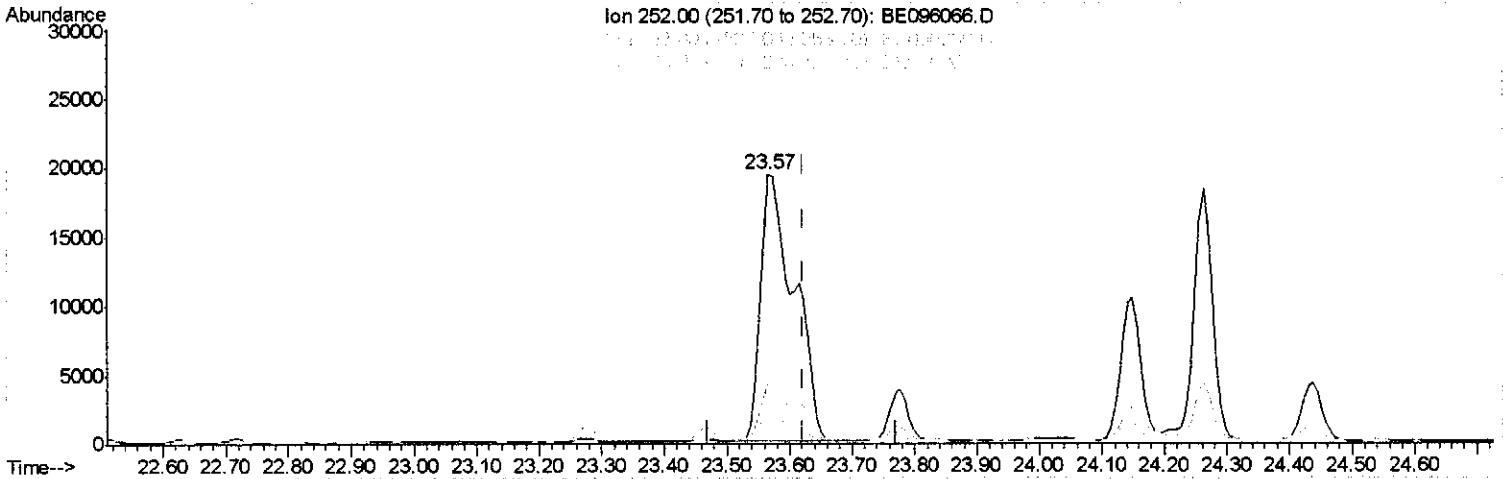

(22) Benzo(k)fluoranthene

23.565min (-0.056) 2.49ng/ul

response 71205

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.25#
125.00	17.10	11.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Instrument : BNA_E
Client Sampled : C0AC9

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:33:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

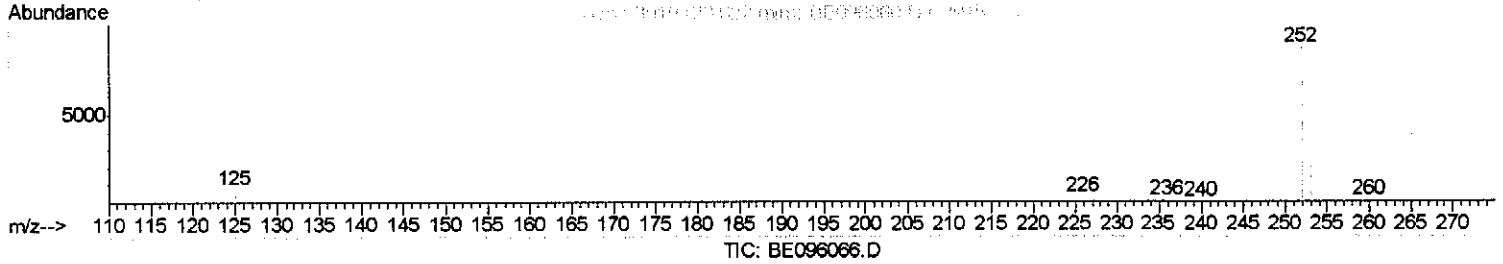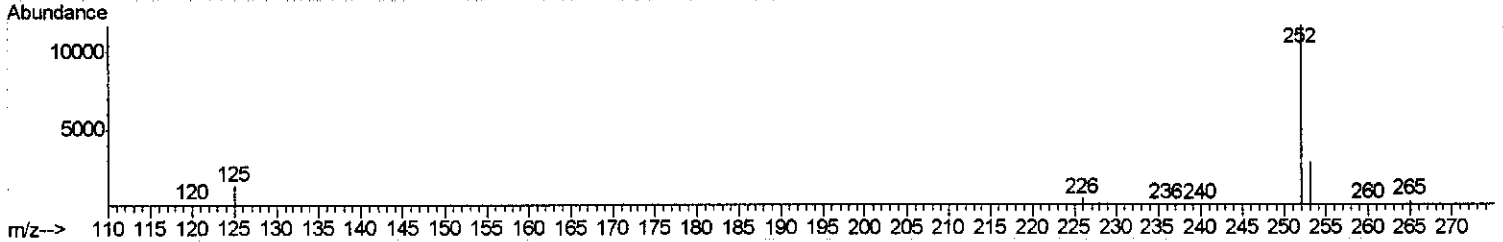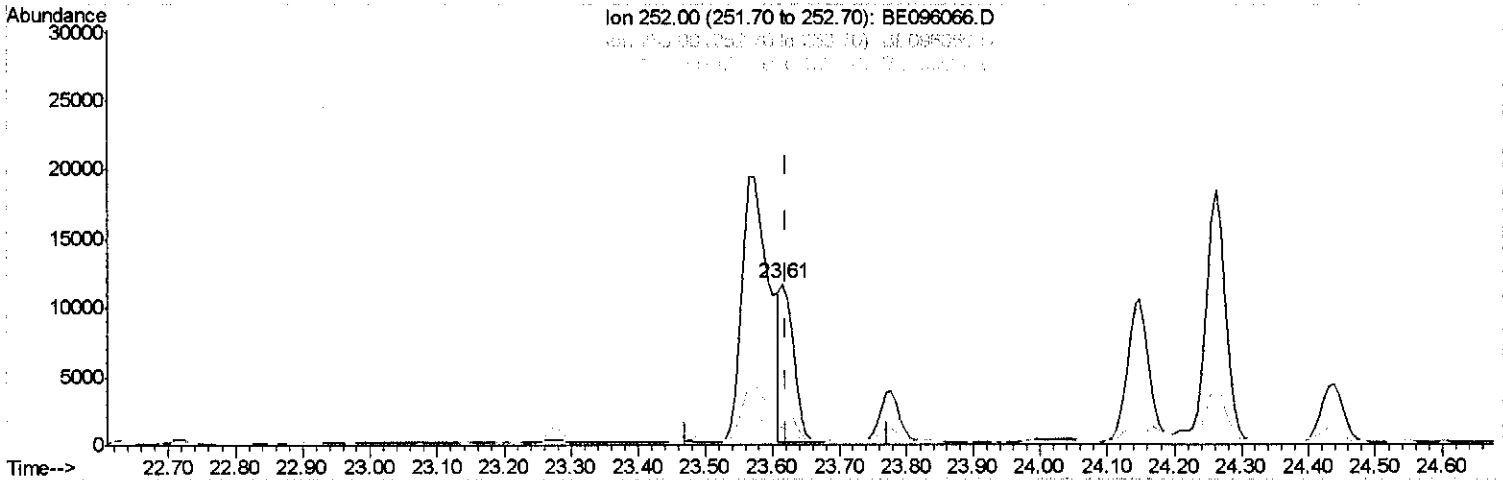

(22) Benzo(k)fluoranthene

23.615min (-0.007) 0.55ng/ul m > SD 4/24/18

response	15641	
Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.07#
125.00	17.10	11.49#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
Client Sampled :
C0AC9

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096066.D
Acq On : 21 Apr 2018 6:37
Operator : SJ/JU
Sample : J2434-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Manual Integrations
APPROVED
Sohil
4/23/2018 6:44:24 PM

Quant Time: Apr 23 02:36:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 01:07:45 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	2039	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5717	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3387	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	7404m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	7135m	0.40	ng/ul	0.00
20) Perylene-di2	24.37	264	8867	0.40	ng/ul	0.00

SJ 4/24/18

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methvl naphthalene-d10	12.76	152	2616	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	7004m)	0.23	ng/ul	0.00

SJ 4/24/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	11.25	128	768	0.048	ng/ul#	72
5) 2-Methvinaphthalene	12.83	142	352	0.033	ng/ul	98
7) Acenaphthvlene	14.70	152	2293	0.131	ng/ul	94
8) Acenaphthene	15.03	153	1087	0.086	ng/ul	96
9) Fluorene	15.99	166	1760	0.124	ng/ul	90
12) Phenanthrene	17.72	178	35064m	1.607	ng/ul	
13) Anthracene	17.80	178	9386m	0.432	ng/ul	
15) Fluoranthene	19.68	202	97357m	3.279	ng/ul	
17) Pyrene	20.04	202	84501	3.485	ng/ul#	78
18) Benzo(a)anthracene	21.74	228	56623m	1.964	ng/ul	
19) Chrysene	21.80	228	39402	1.899	ng/ul	97
21) Benzo(b)fluoranthene	23.57	252	55476m	1.933	ng/ul	
22) Benzo(k)fluoranthene	23.61	252	15641m	0.547	ng/ul	
23) Benzo(a)pyrene	24.26	252	38537	1.392	ng/ul#	79
24) Indeno(1,2,3-cd)pyrene	27.16	276	22660	0.736	ng/ul#	73
25) Dibenzo(a,h)anthracene	27.18	278	5938	0.240	ng/ul	98
26) Benzo(a,h,i)perylene	28.04	276	21202	0.825	ng/ul#	94

SJ 4/24/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed