

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096041.D
 Acq On : 20 Apr 2018 15:14
 Operator : SJ/JU
 Sample : J2313-17RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F1A54RE

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:43:10 PM

Quant Time: Apr 21 01:10:38 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 00:59:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1948	0.40	ng/ul	0.00
2) Naphthalene-d8	11.21	136	5129	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	6607	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	7244m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6129m	0.40	ng/ul	0.00
20) Perylene-d12	24.39	264	7250	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	2863	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	6766m	0.23	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.25	128	1155	0.081	ng/ul#	1
11) Pentachlorophenol	17.34	266	173m	0.113	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096041.D
Acq On : 20 Apr 2018 15:14
Operator : SJ/JU
Sample : J2313-17RE
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F1A54RE

Manual Integrations
APPROVED

Sohil
4/23/2018 6:43:10 PM

Quant Time: Apr 21 01:10:38 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 00:59:26 2018
Response via : Initial Calibration

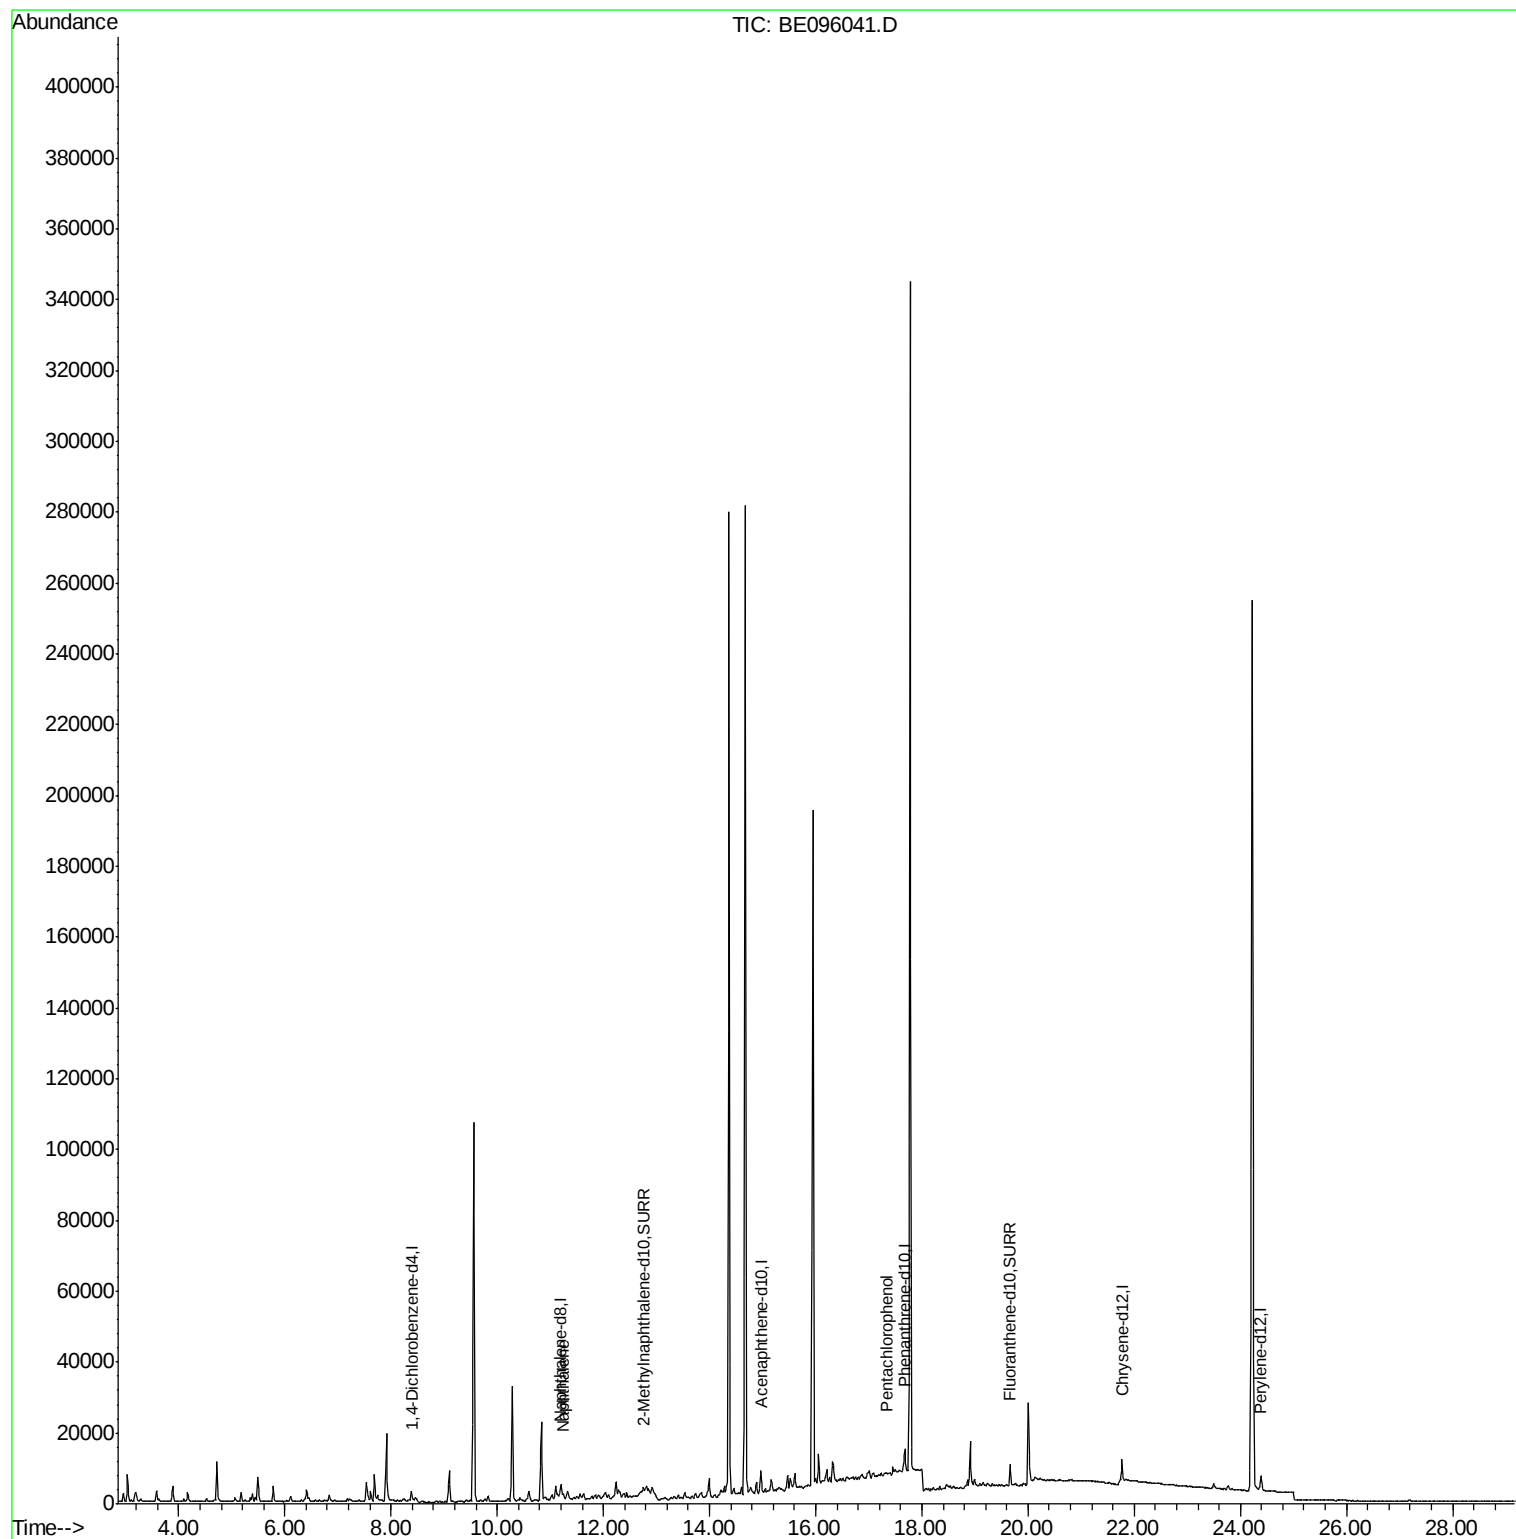

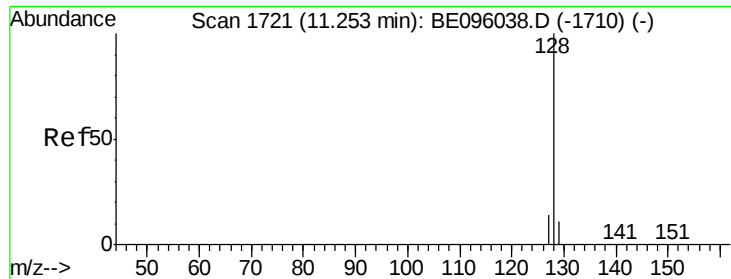

#3

Naphthalene

Concen: 0.081 ng/ul

RT: 11.25 min Scan# 1720

Delta R.T. -0.01 min

Lab File: BE096041.D

Acq: 20 Apr 2018 15:14

Instrument :

BNA_E





ClientSampled :

F1A54RE

Tot Ion:	128	Resp:	1155
Ion Ratio	Lower	Upper	
128	100		
129	74.6	11.3	16.9#
127	44.6	4.0	6.0#

Manual Integrations
APPROVED

Sohil
4/23/2018 6:43:10 PM

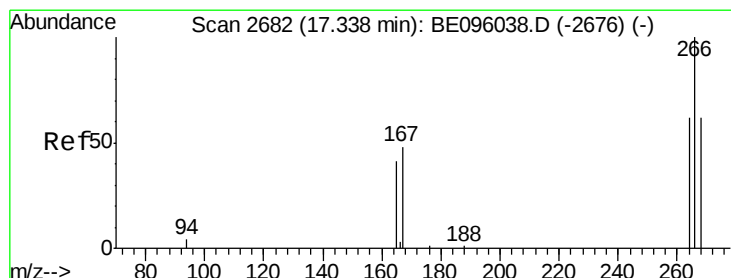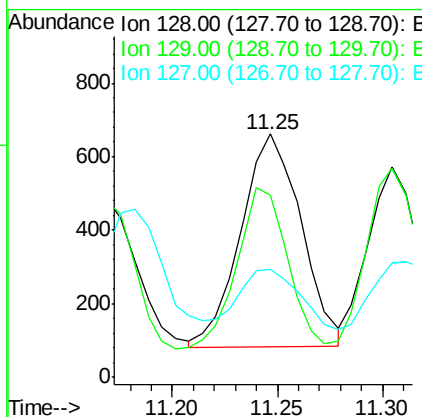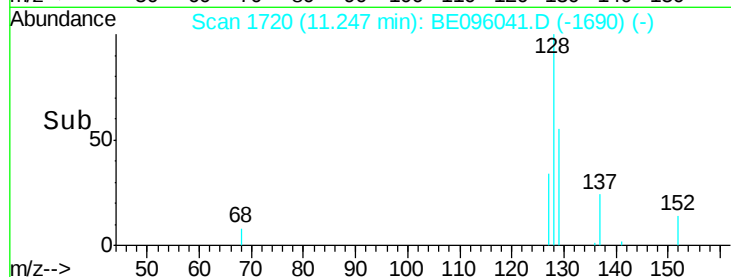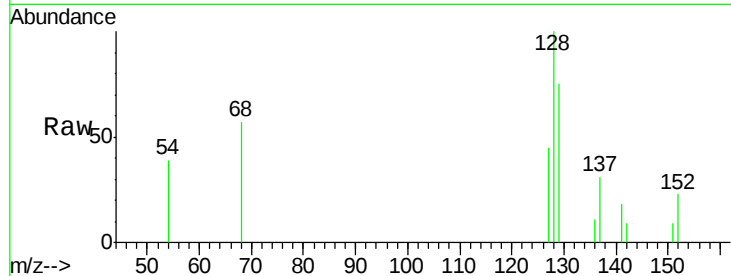

#11

Pentachlorophenol

Concen: 0.113 ng/ul m

RT: 17.34 min Scan# 2682

Delta R.T. 0.00 min

Lab File: BE096041.D

Acq: 20 Apr 2018 15:14

Tgt Ion:	266	Resp:	173
Ion Ratio	Lower	Upper	
266	100		
264	1.2	47.9	71.9#
268	0.0	49.8	74.8#

