

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
 Data File : BE096050.D
 Acq On : 20 Apr 2018 20:40
 Operator : SJ/JU
 Sample : J2356-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3XX2

Manual Integrations
 APPROVED

Sohil
 4/23/2018 6:43:25 PM

Quant Time: Apr 21 01:53:10 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 21 01:28:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1902	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5363	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3257	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	7307m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6979m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	7998	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	2003	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	5577m	0.19	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.72	178	539m	0.025	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042018\
Data File : BE096050.D
Acq On : 20 Apr 2018 20:40
Operator : SJ/JU
Sample : J2356-09
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
A3XX2

Manual Integrations
APPROVED

Sohil
4/23/2018 6:43:25 PM

Quant Time: Apr 21 01:53:10 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 21 01:28:31 2018
Response via : Initial Calibration

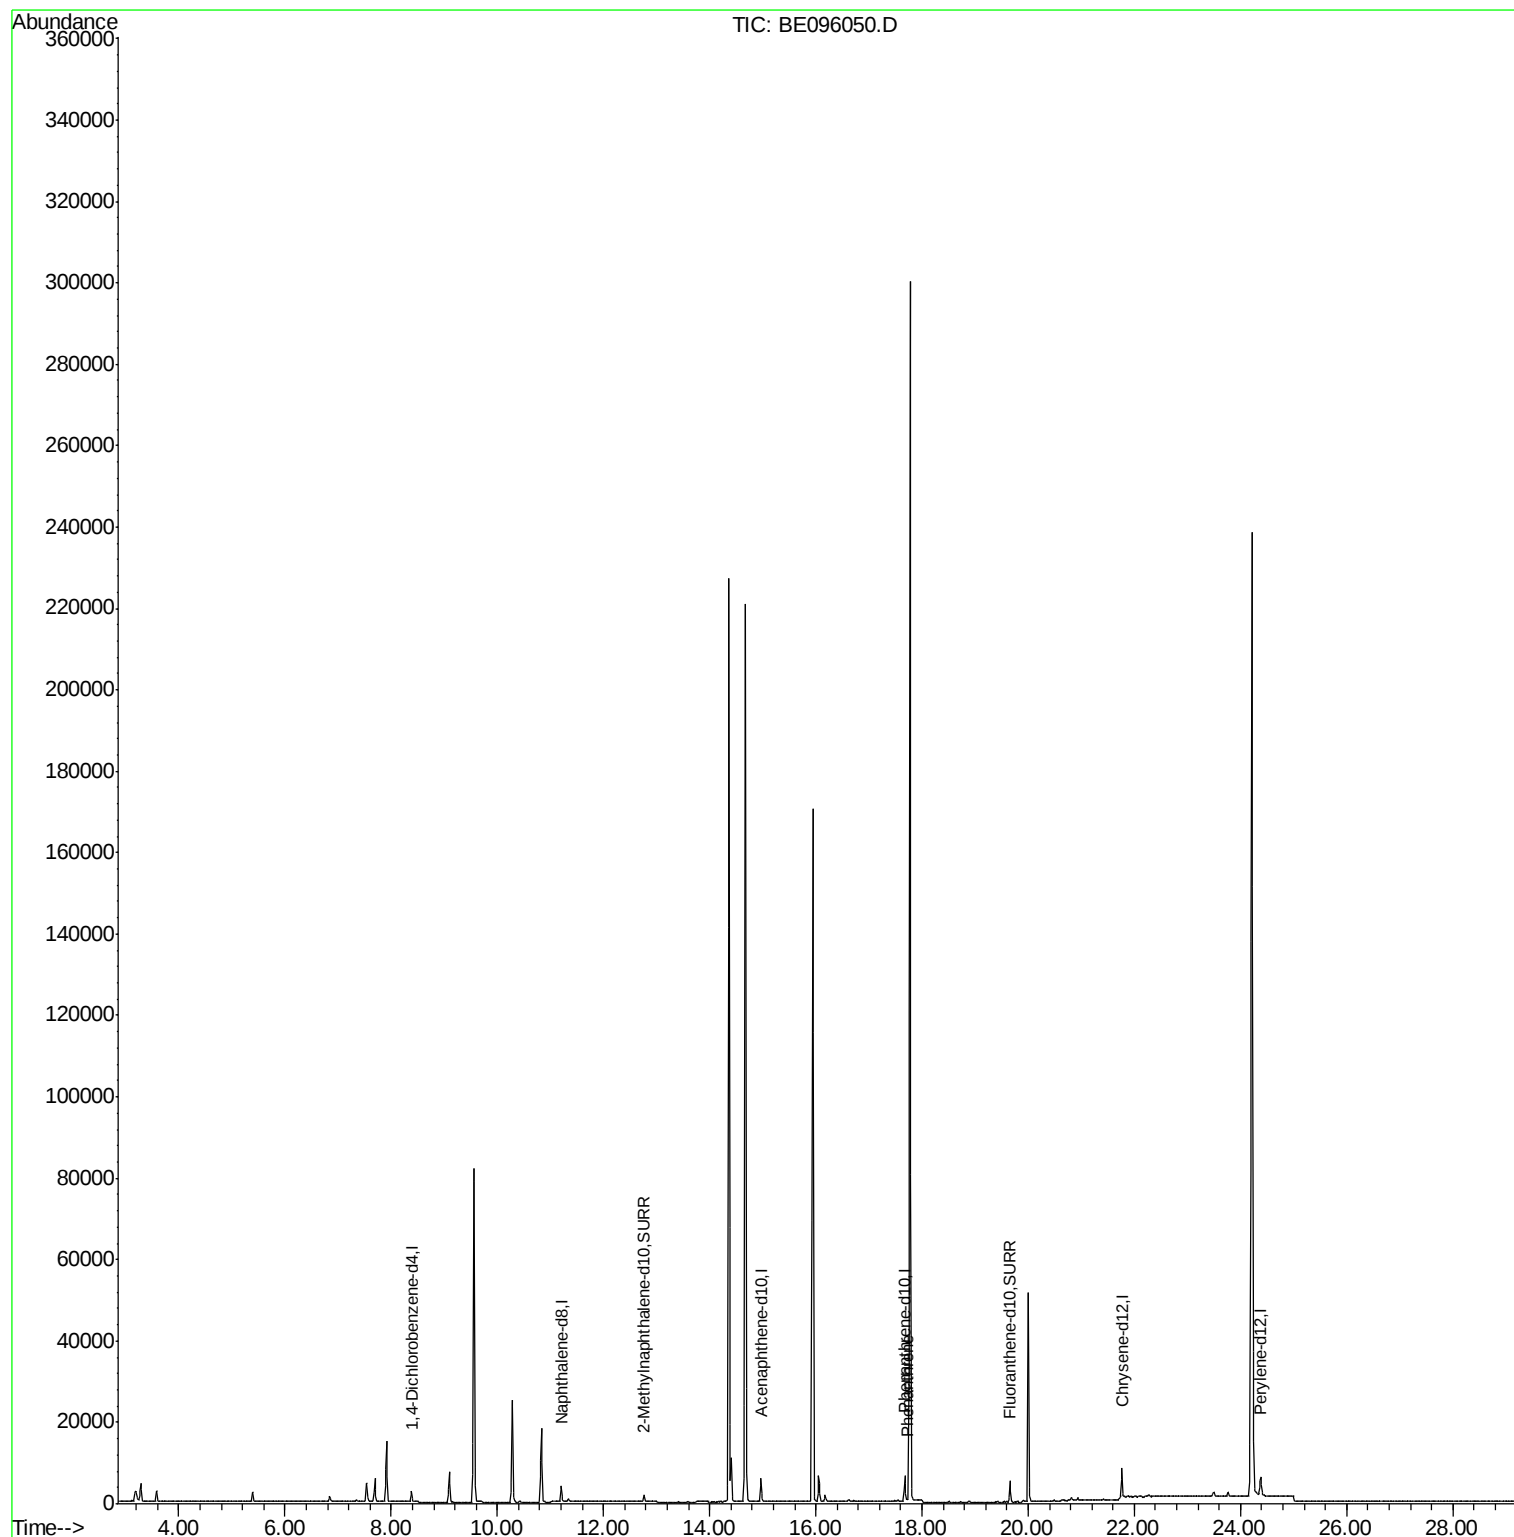

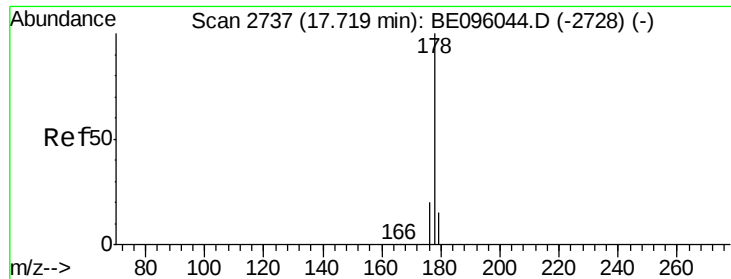

#12

Phenanthrene

Concen: 0.025 ng/ul m

RT: 17.72 min Scan# 2737

Delta R.T. -0.00 min

Lab File: BE096050.D

Acq: 20 Apr 2018 20:40

Instrument :

BNA_E

ClientSampleId :

A3XX2

Tot Ion:178 Resp: 539

Ion Ratio Lower Upper

178 100

179 29.8 18.4 27.6#

176 35.1 13.6 20.4#

Manual Integrations
APPROVED

Sohil

4/23/2018 6:43:25 PM

