
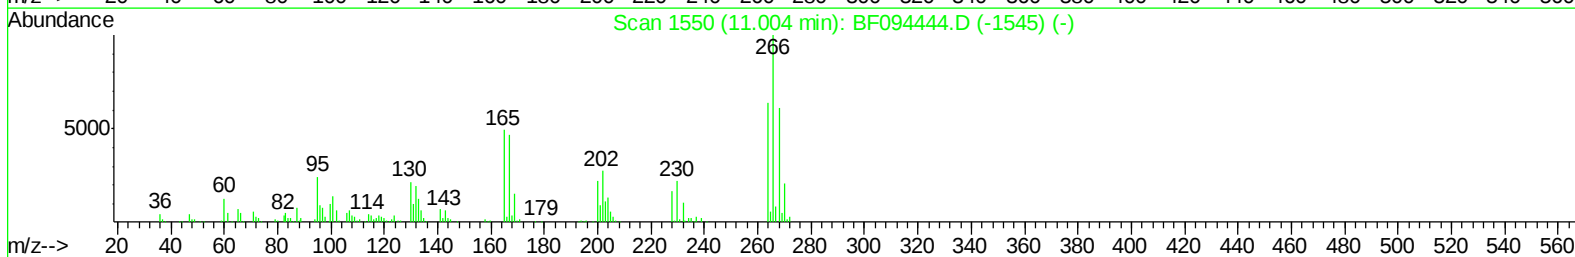
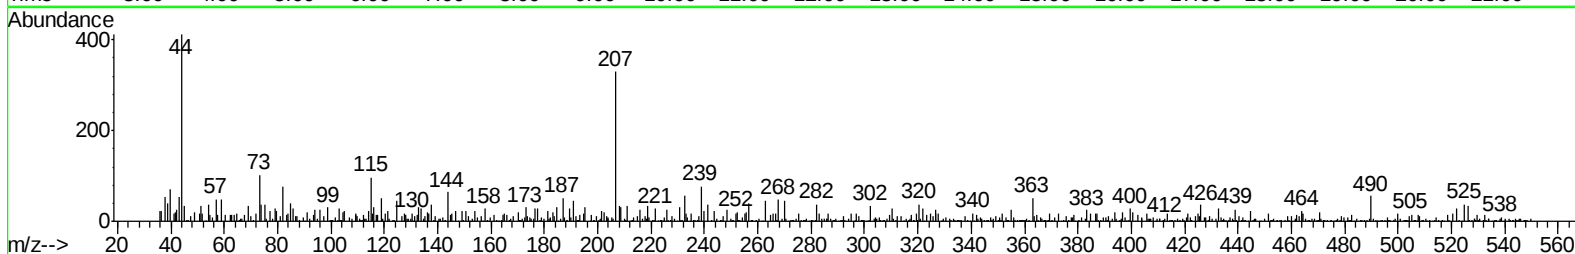


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042117\
Data File : BE092905.D
Acq On : 21 Apr 2017 12:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 06:44:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

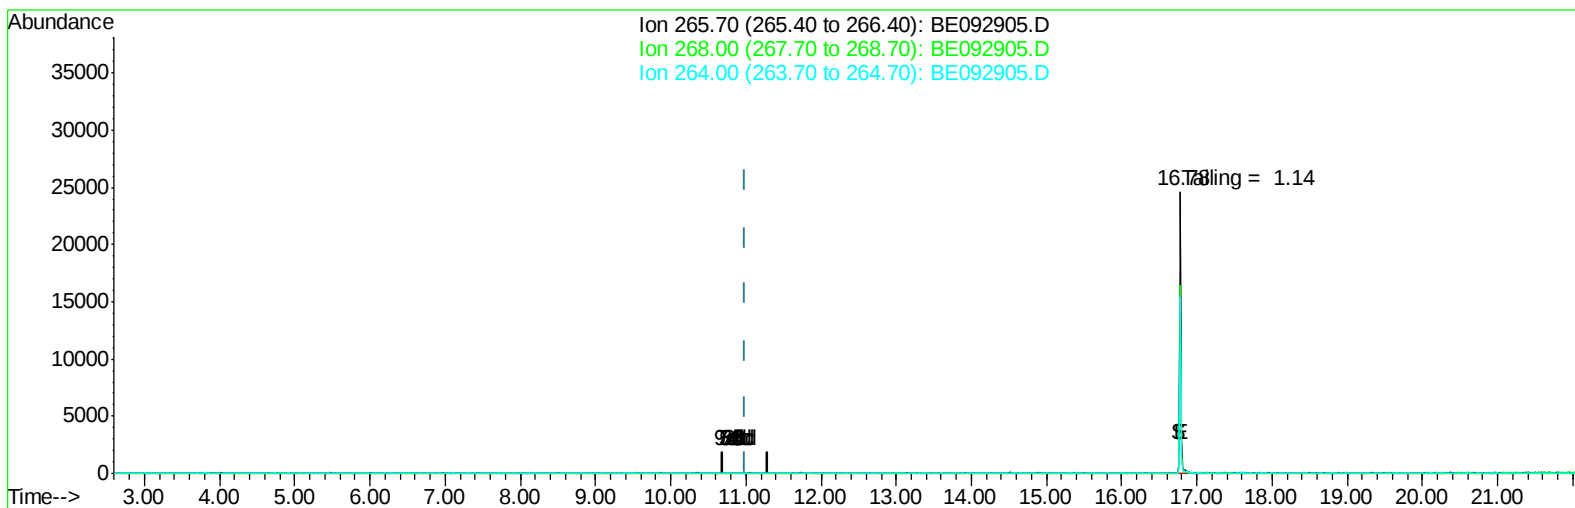

TIC: BE092905.D

(69) Pentachlorophenol (C)




10.890min (-0.114) 96.80ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	261.11#
264.00	64.60	77.78#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042117\
Data File : BE092905.D
Acq On : 21 Apr 2017 12:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 06:44:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

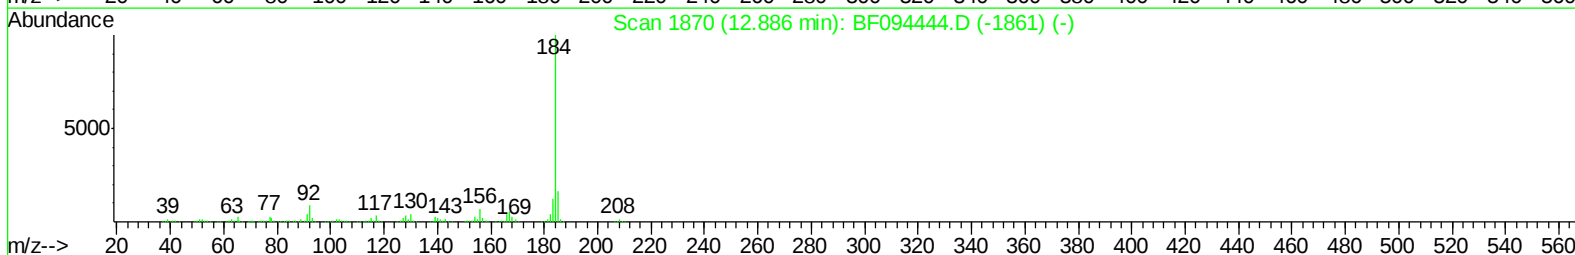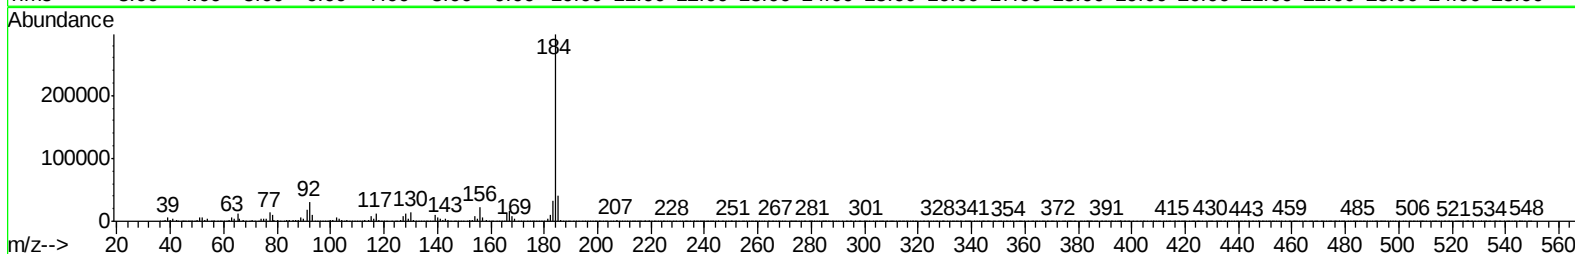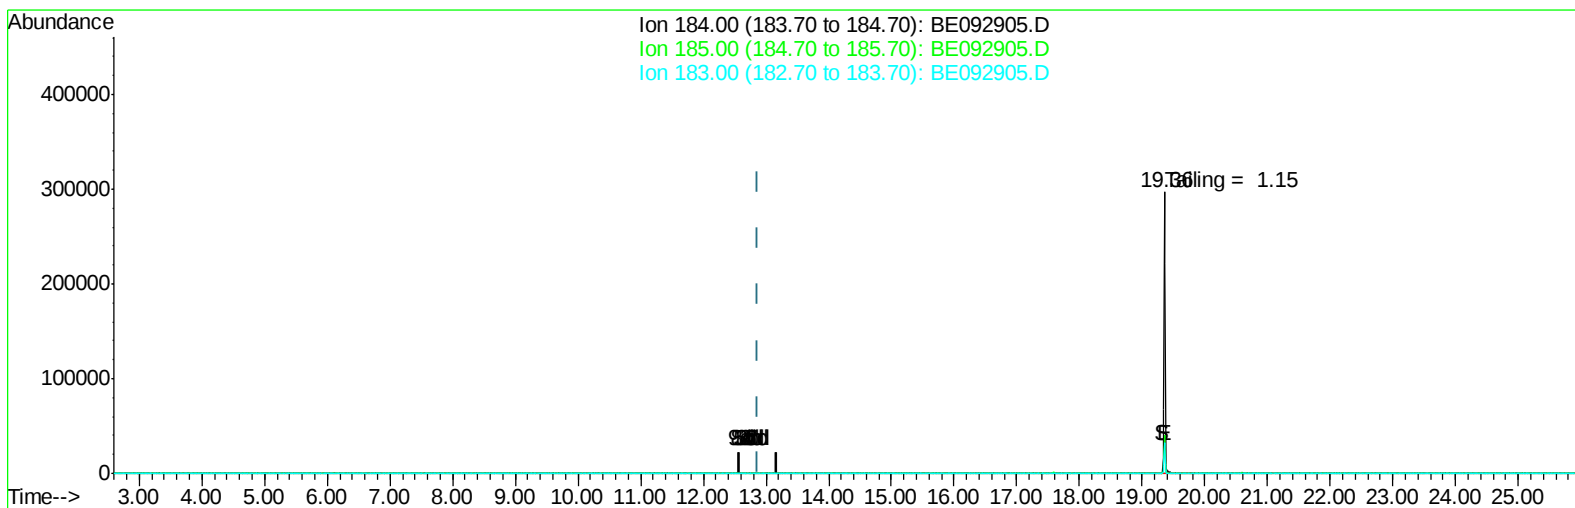

TIC: BE092905.D

(76) Benzidine

19.356min (+6.470) 1224442.10ng m

response 347042

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.85#
183.00	12.20	11.14
0.00	0.00	0.00