


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE042117\
Data File : BE092905.D
Acq On : 21 Apr 2017 12:20
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042017.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 20 17:35:10 2017

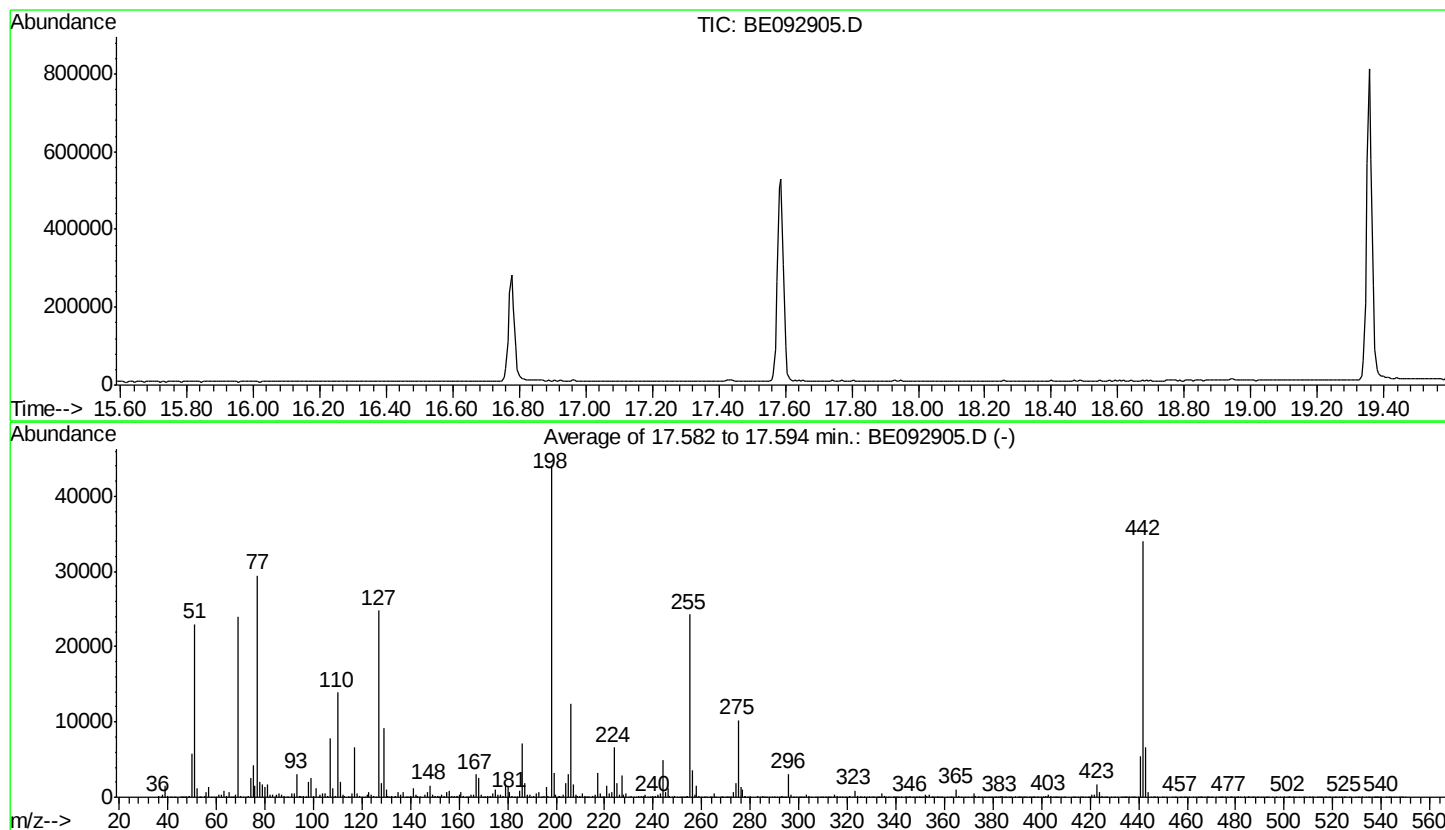

AutoFind: Scans 2552, 2553, 2554; Background Corrected with Scan 2543

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	23044	PASS
68	69	0.00	2	1.4	340	PASS
69	198	0.00	100	54.3	23910	PASS
70	69	0.00	2	0.6	149	PASS
127	198	10	80	56.4	24826	PASS
197	198	0.00	2	0.3	128	PASS
198	198	100	100	100.0	44051	PASS
199	198	5	9	7.2	3190	PASS
275	198	10	60	23.4	10286	PASS
365	198	1	100	2.5	1080	PASS
441	442	0.01	24	16.1	5502	PASS
442	198	50	100	77.4	34088	PASS
443	442	15	24	19.5	6663	PASS