


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096079.D
Acq On : 23 Apr 2018 11:36
Operator : SJ/JU
Sample : PB108290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK90

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:48:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

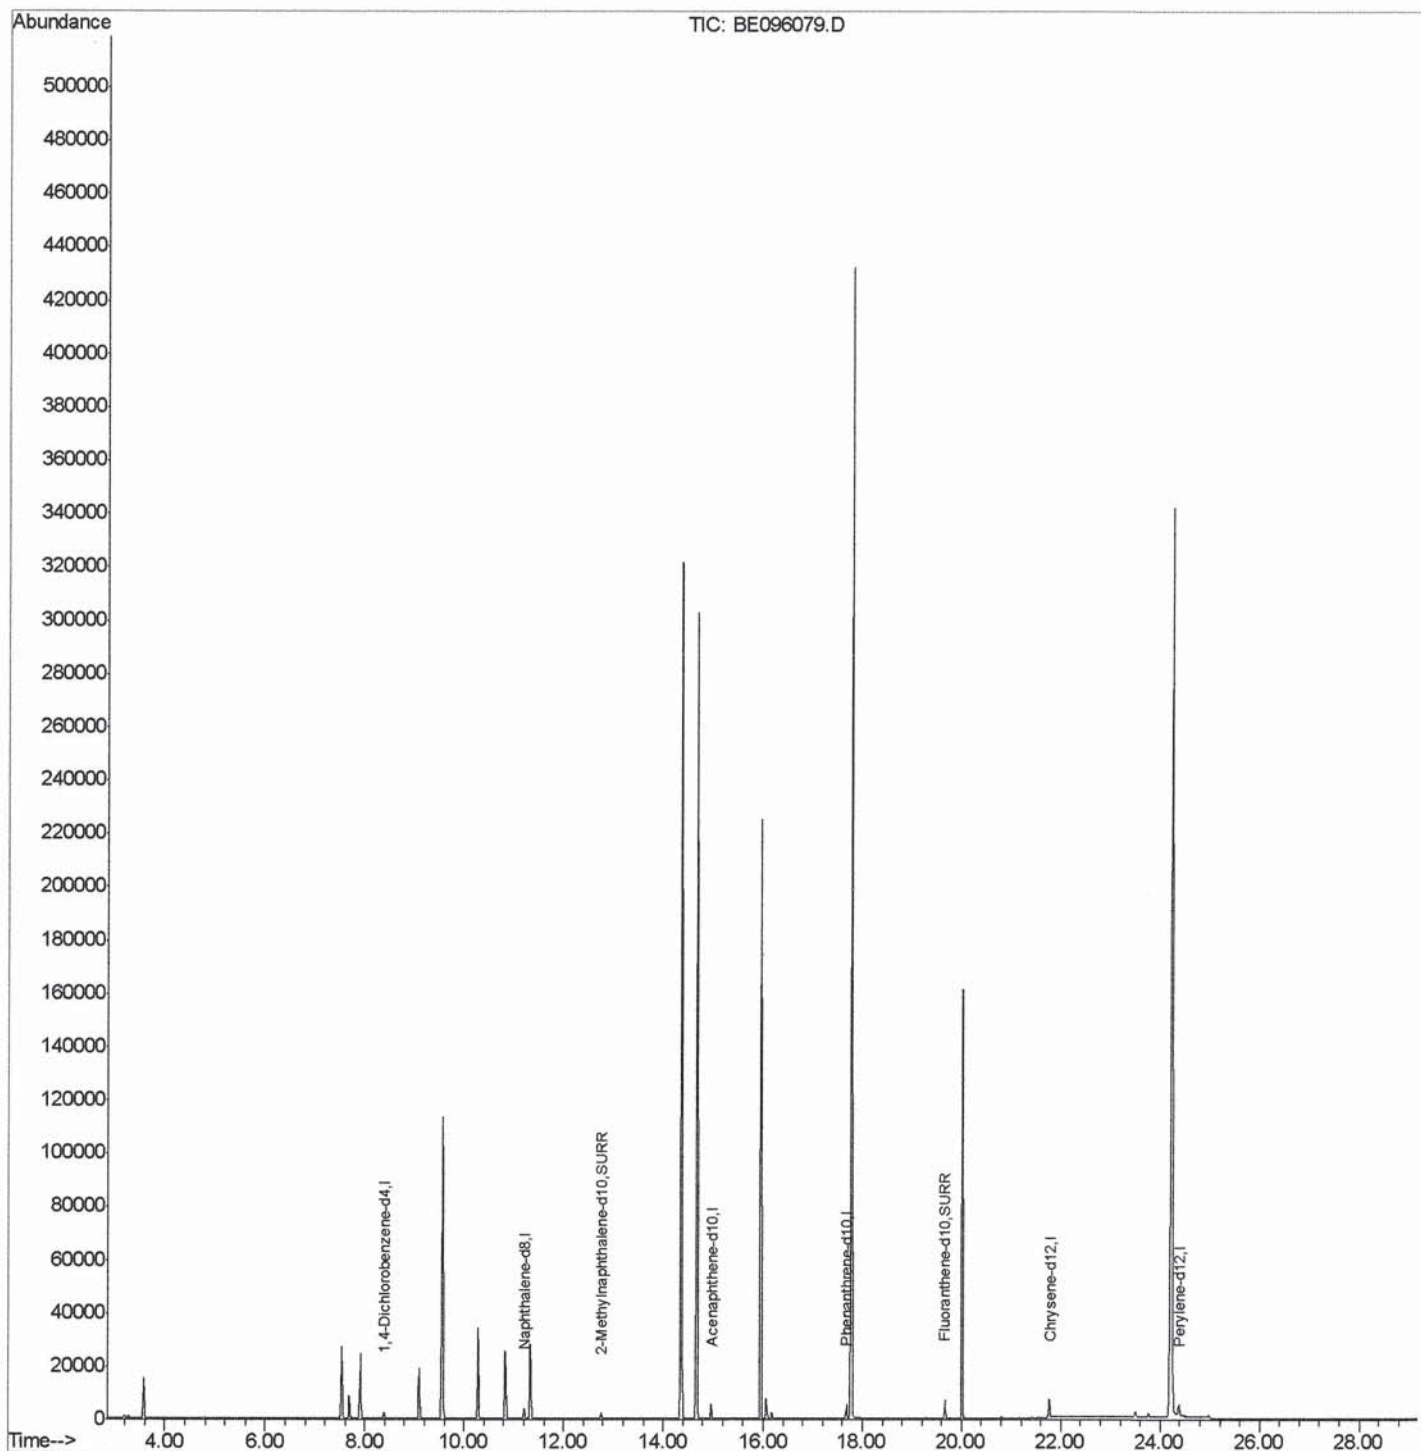

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096079.D
 Acq On : 23 Apr 2018 11:36
 Operator : SJ/JU
 Sample : PB108290BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK90

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:21:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

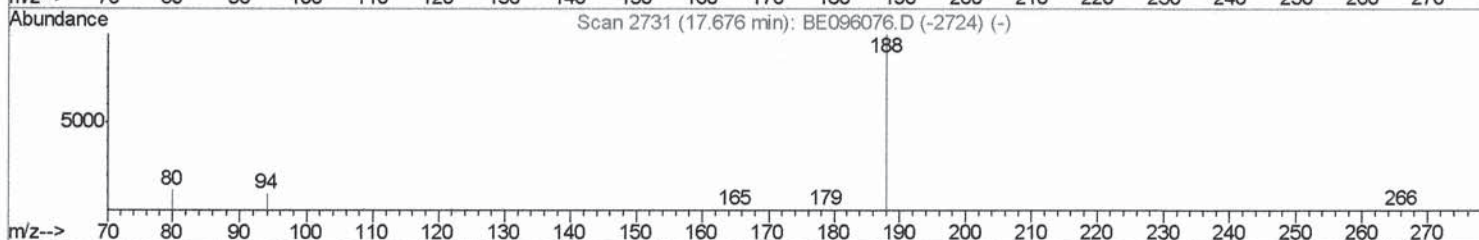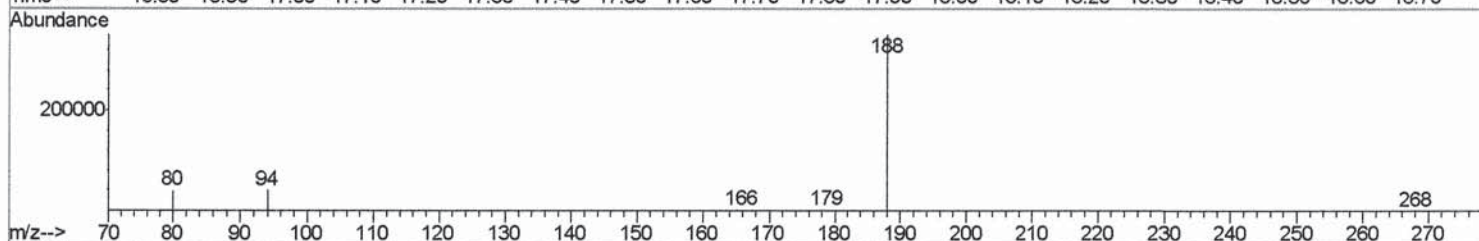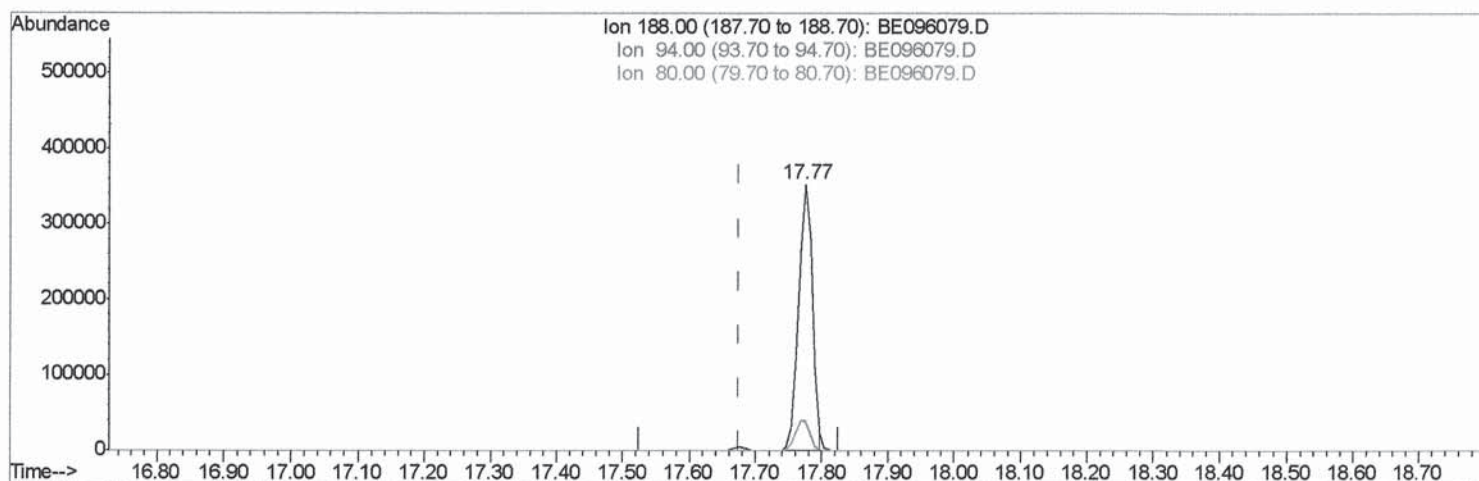

TIC: BE096079.D

(10) Phenanthrene-d10 (I)

17.775min (+0.098) 0.40ng/ul

response 501416

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.42
80.00	11.80	11.11
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096079.D
Acq On : 23 Apr 2018 11:36
Operator : SJ/JU
Sample : PB108290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK90

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:21:47 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

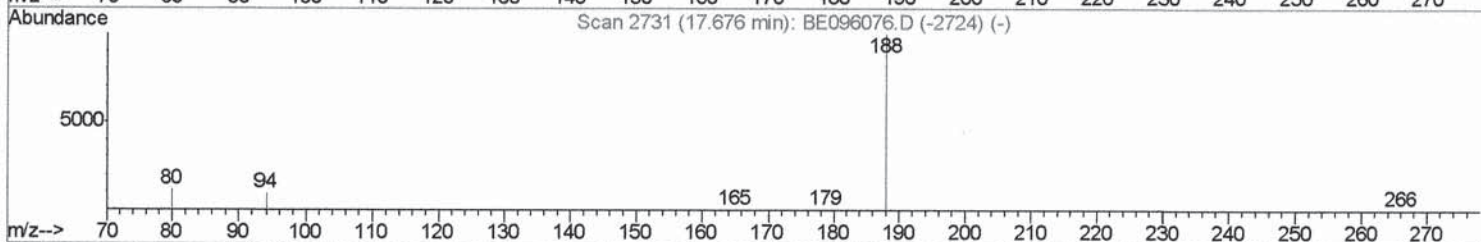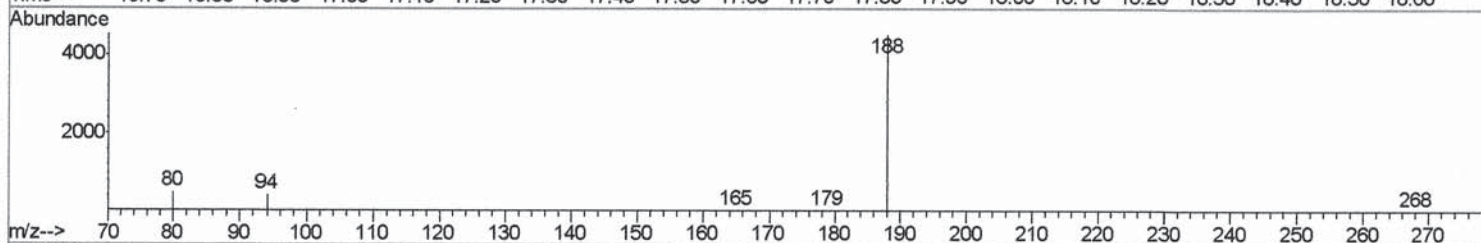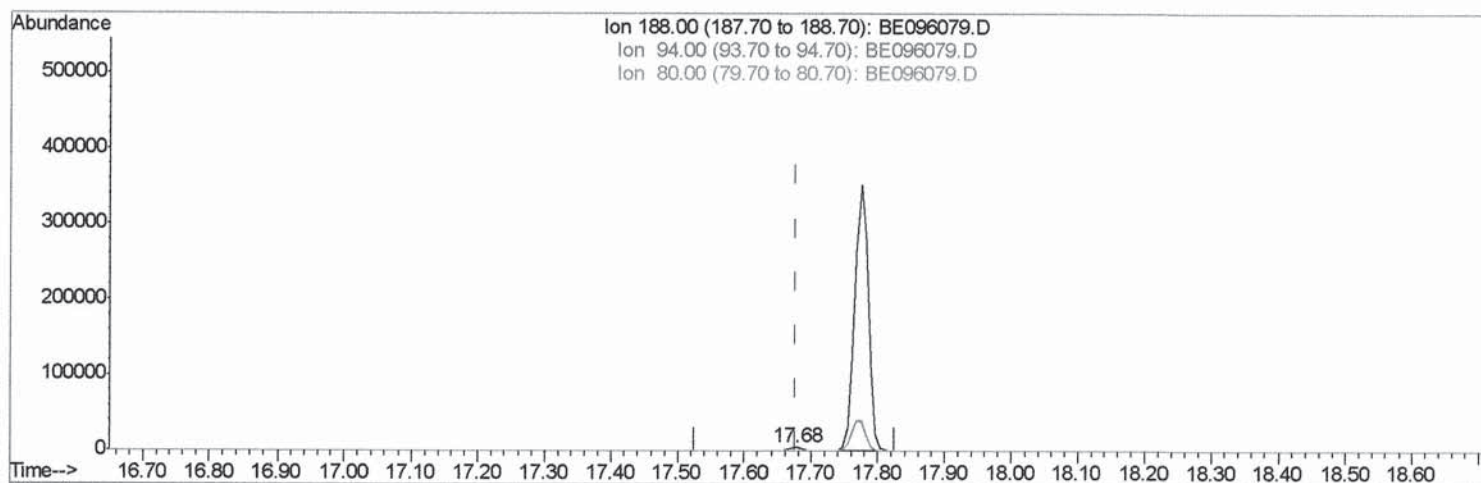

TIC: BE096079.D

(10) Phenanthrene-d10 (I)

17.676min (-0.000) 0.40ng/ul m> SJ 4/24/18

response 6365

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.96
80.00	11.80	11.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096079.D
Acq On : 23 Apr 2018 11:36
Operator : SJ/JU
Sample : PB108290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK90

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:46:09 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

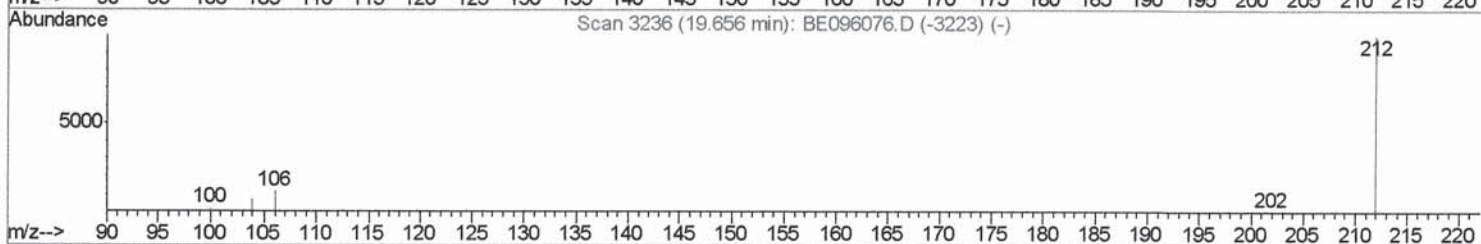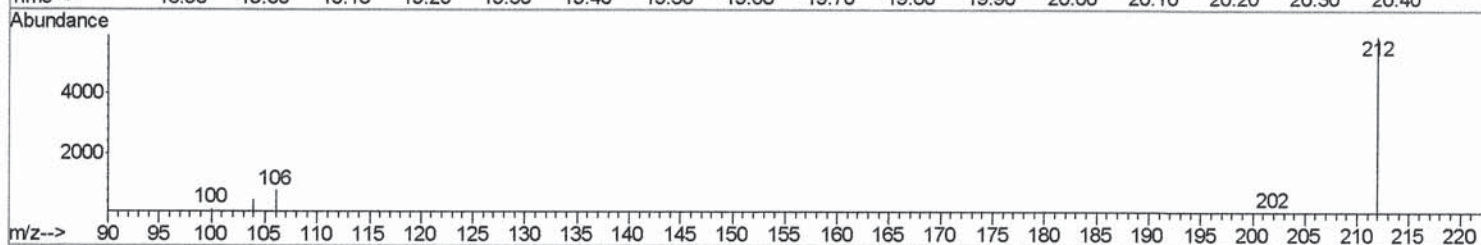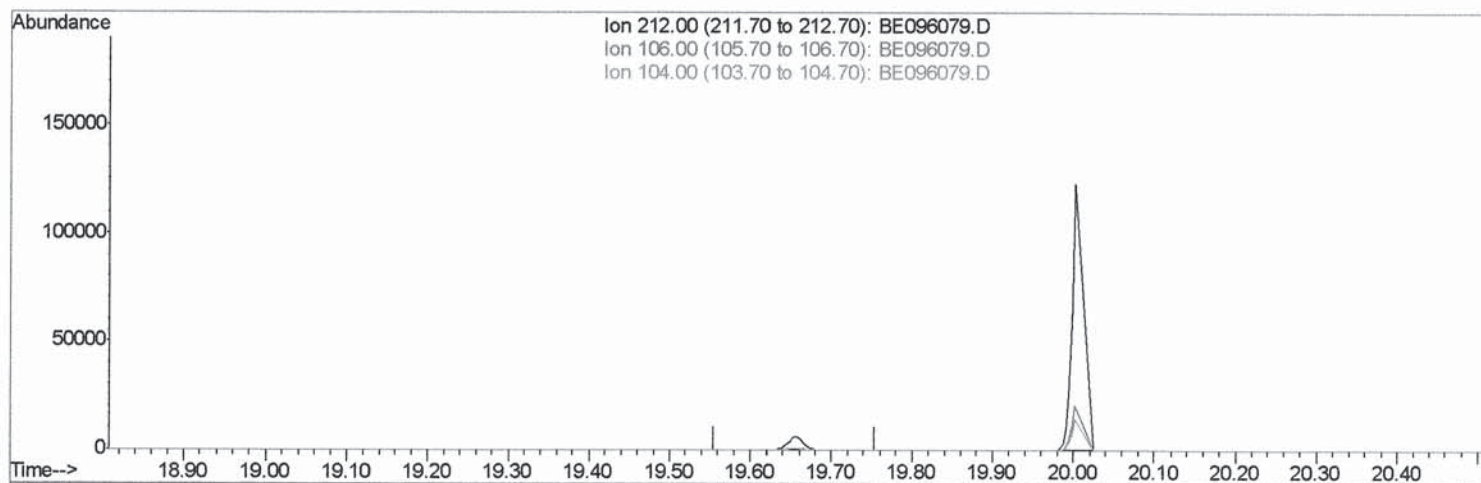

TIC: BE096079.D

(14) Fluoranthene-d10 (SURR)

19.656min (-19.656) 0.00ng/ui

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096079.D
Acq On : 23 Apr 2018 11:36
Operator : SJ/JU
Sample : PB108290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK90

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:46:09 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

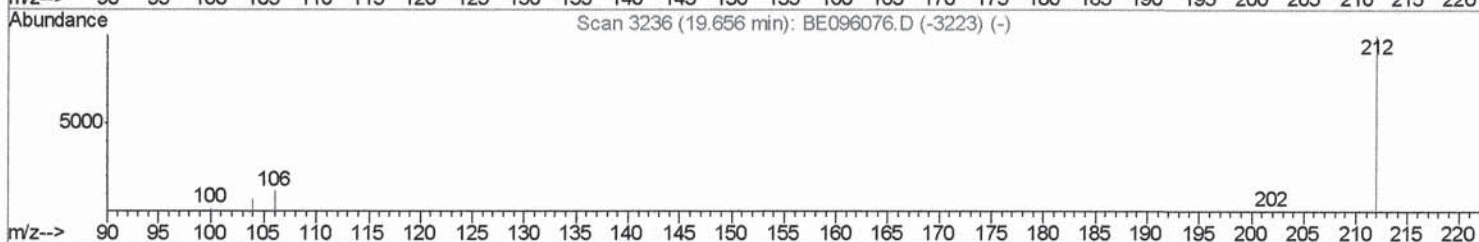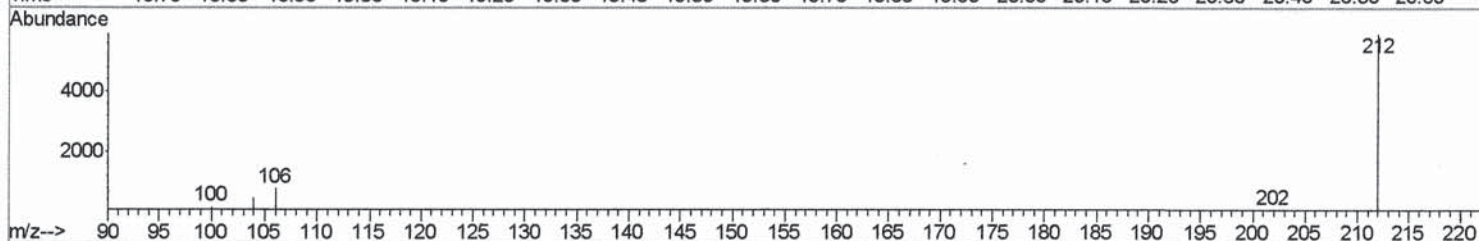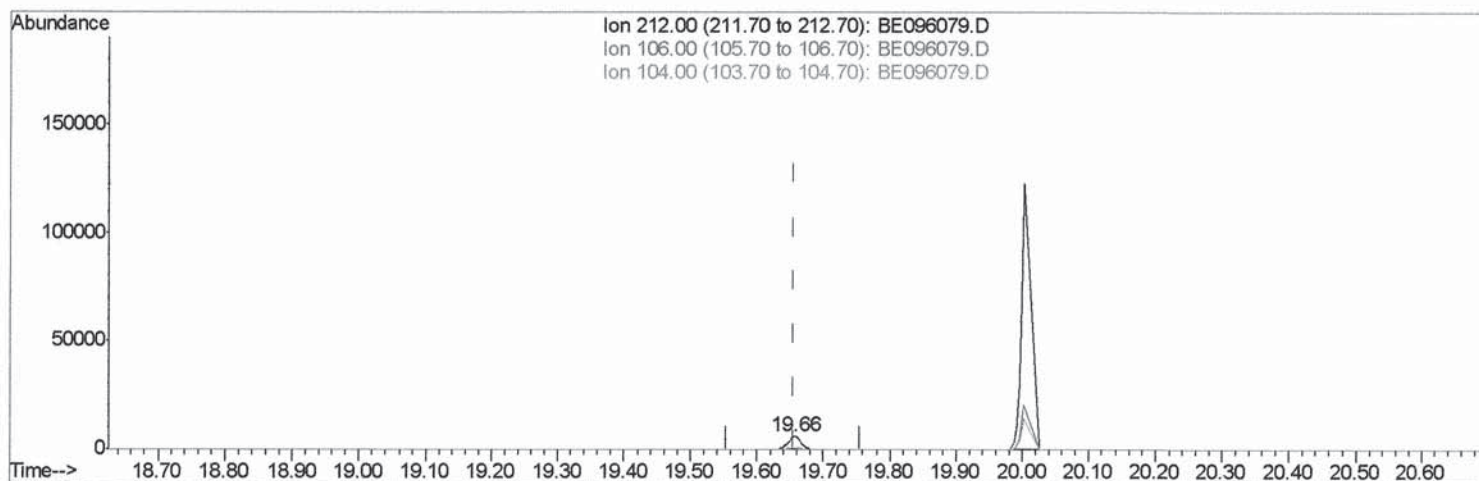

TIC: BE096079.D

(14) Fluoranthene-d10 (SURR)

19.656min (-0.000) 0.30ng/ul m > SJ 4/24/18

response 7828

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096079.D
 Acq On : 23 Apr 2018 11:36
 Operator : SJ/JU
 Sample : PB108290BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK90

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:46:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

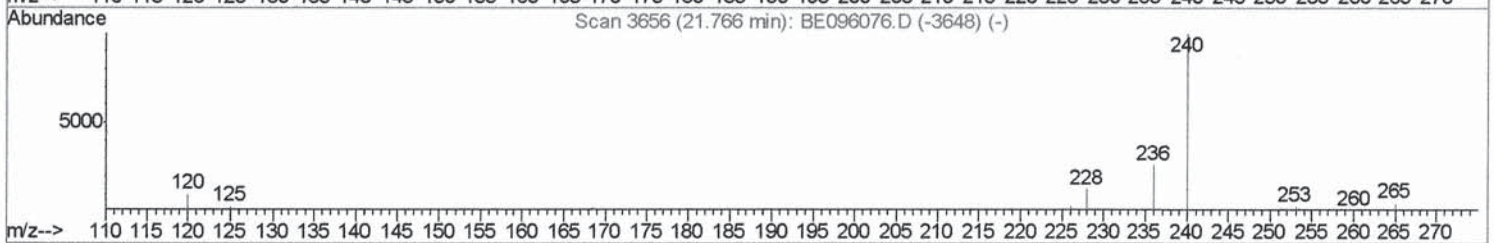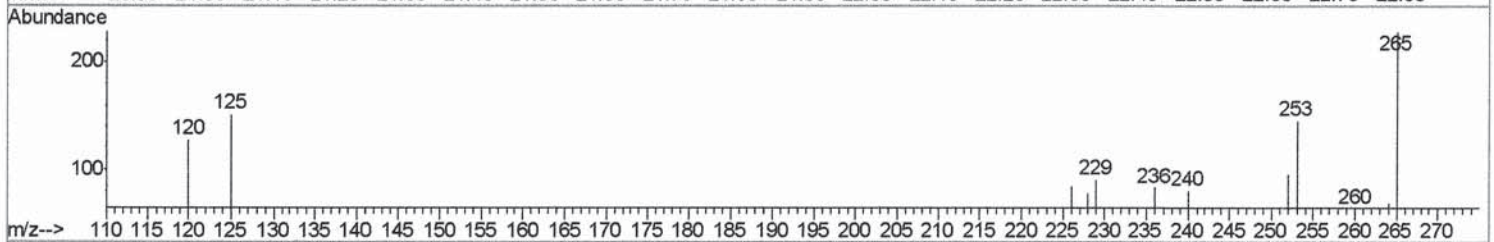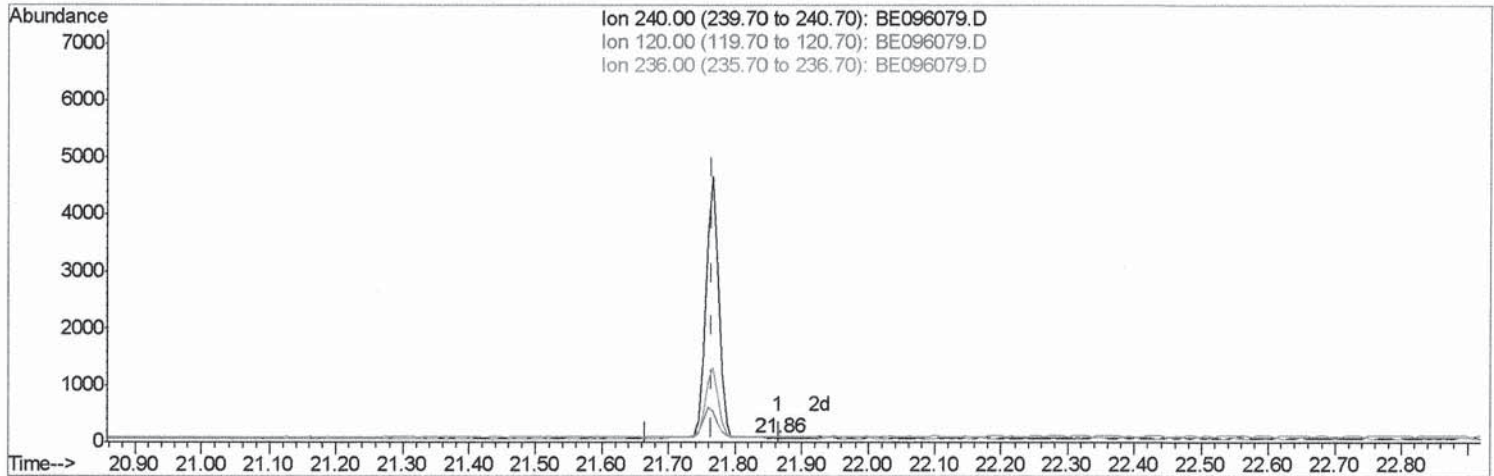

TIC: BE096079.D

(16) Chrysene-d12 (I)

21.864min (+0.098) 0.40ng/ul

response 21

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	158.75#
236.00	34.90	103.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096079.D
 Acq On : 23 Apr 2018 11:36
 Operator : SJ/JU
 Sample : PB108290BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK90

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:46:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

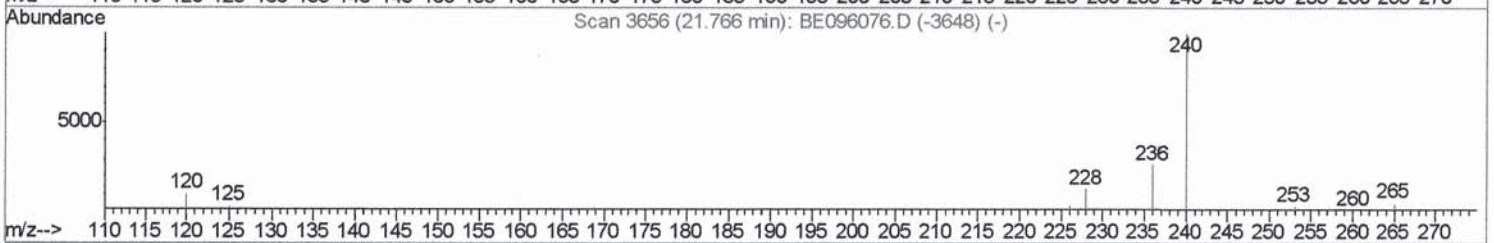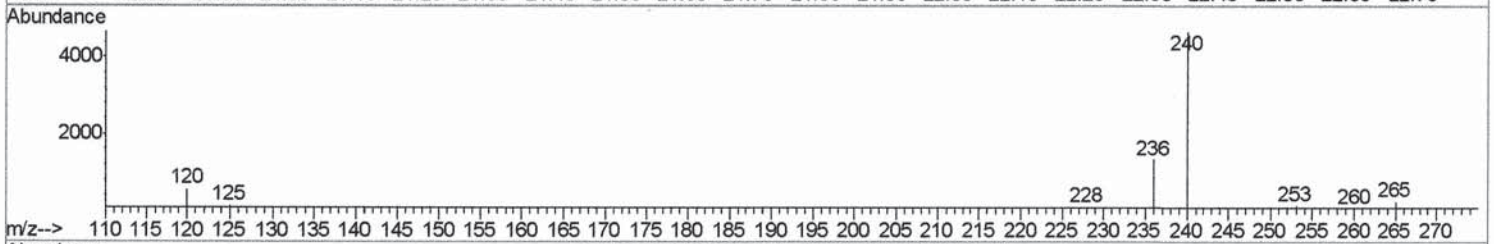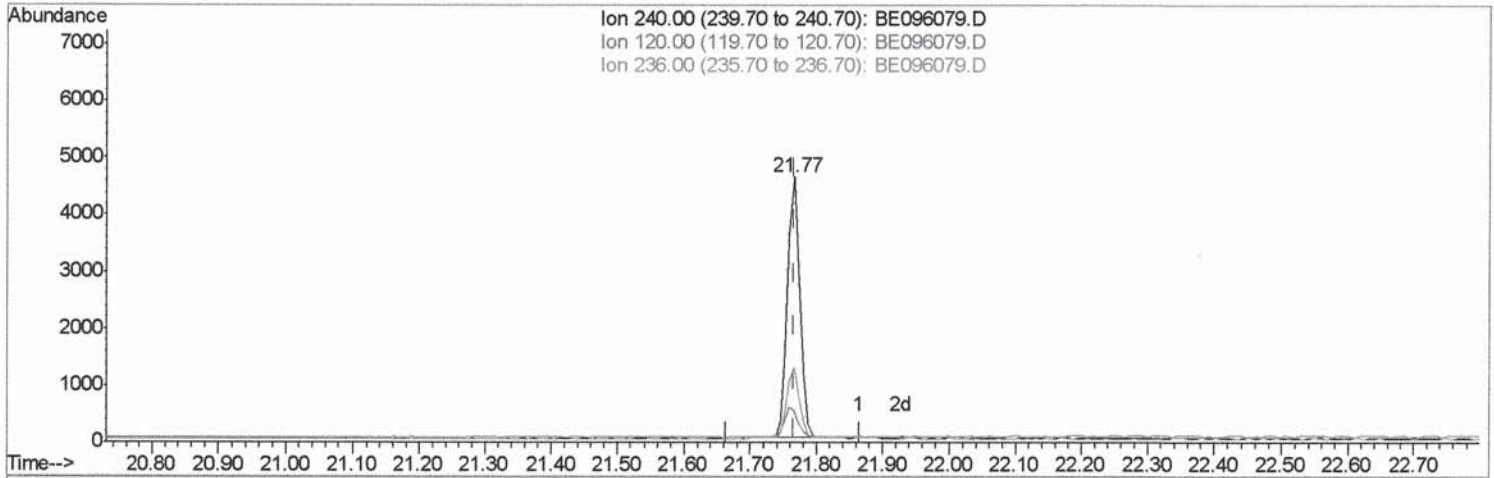

TIC: BE096079.D

(16) Chrysene-d12 (I)

21.766min (-0.000) 0.40ng/ul m> SJ 4/24/18

response 6019

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.81#
236.00	34.90	28.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096079.D
Acq On : 23 Apr 2018 11:36
Operator : SJ/JU
Sample : PB108290BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK90

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:45 PM

Quant Time: Apr 24 05:48:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1834	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	4891	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2967	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6365m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6019m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	7925	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.76	152	2781	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	7828m	0.30	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed