


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 06:17:27 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

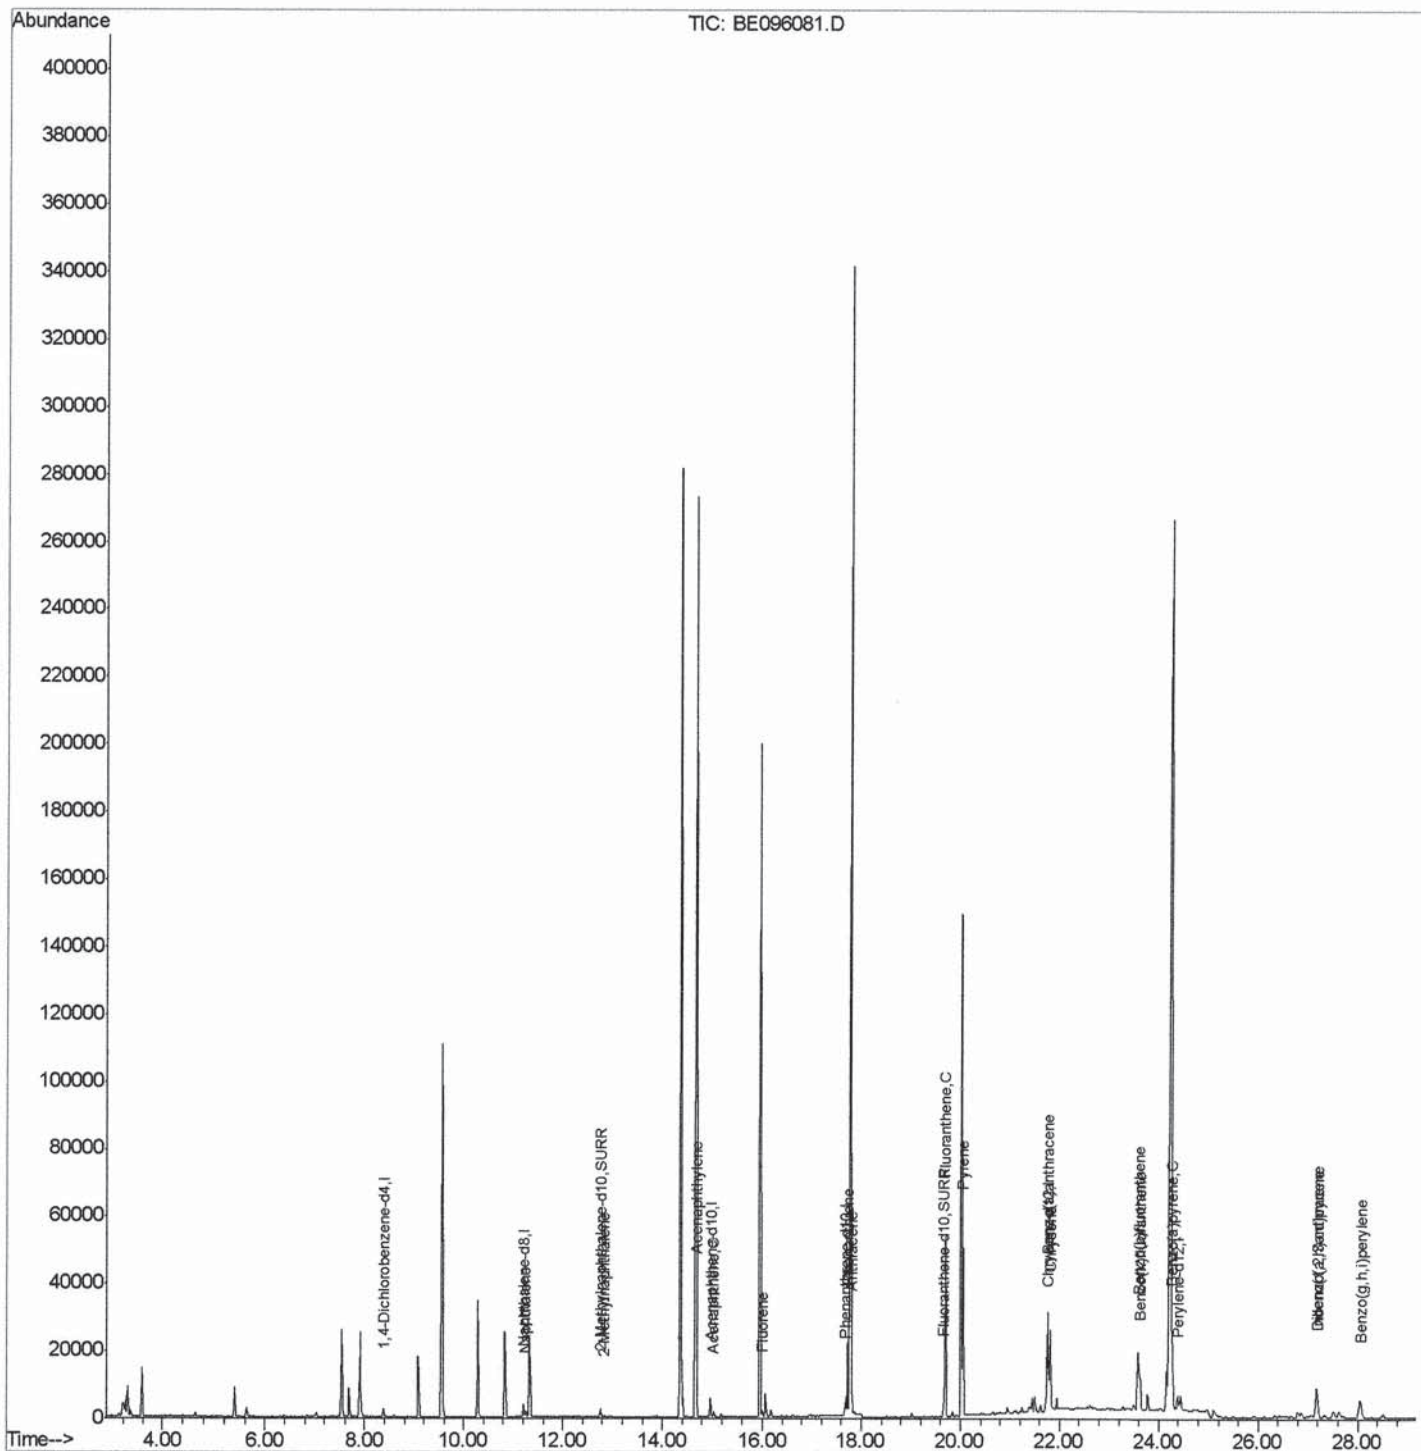

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:22:11 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

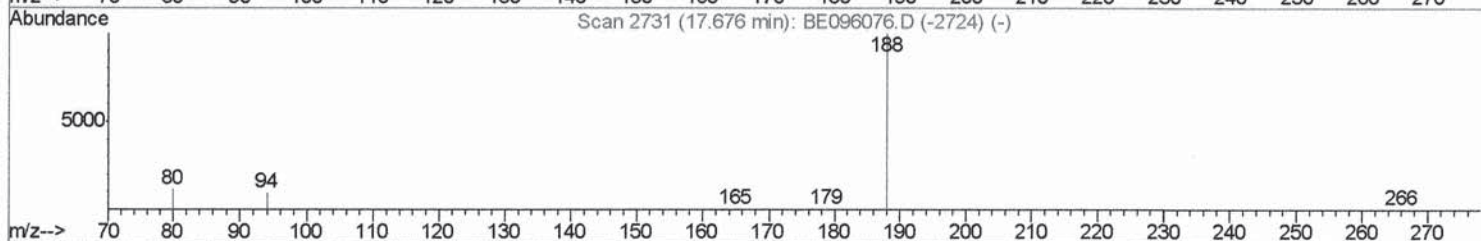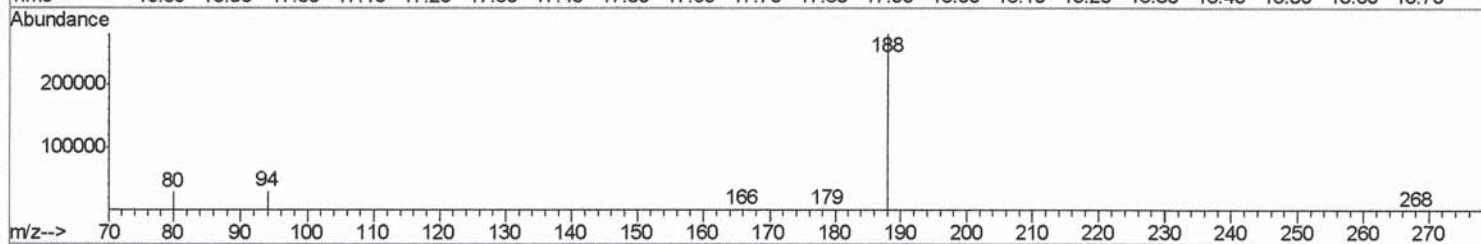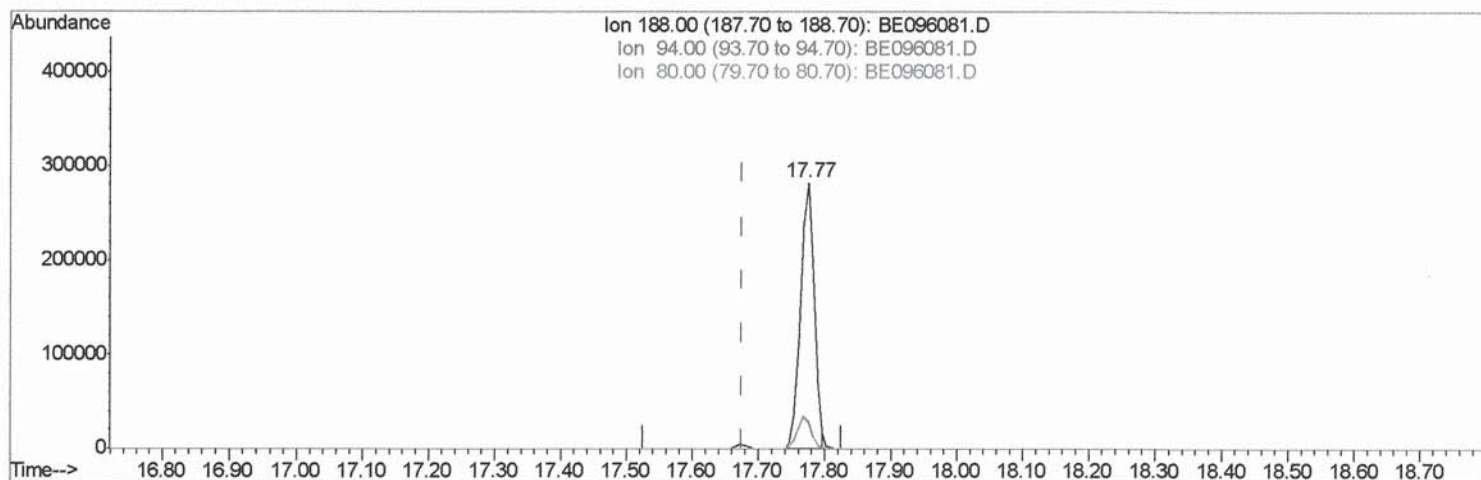

TIC: BE096081.D

(10) Phenanthrene-d10 (I)

17.775min (+0.098) 0.40ng/ul

response 401037

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.62
80.00	11.80	10.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:22:11 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

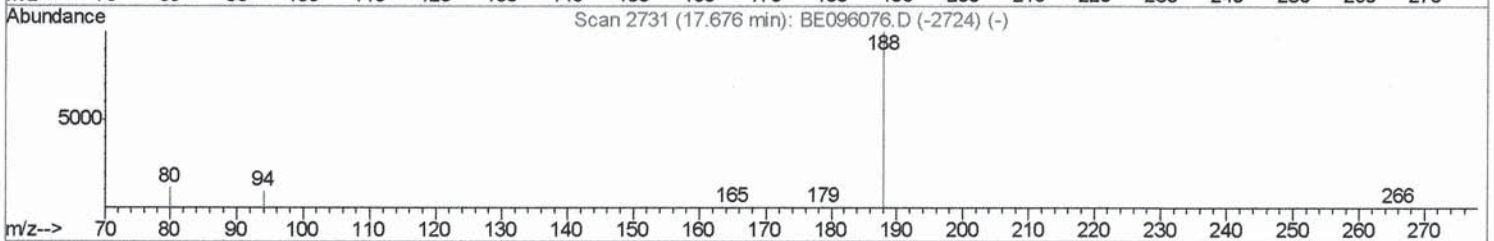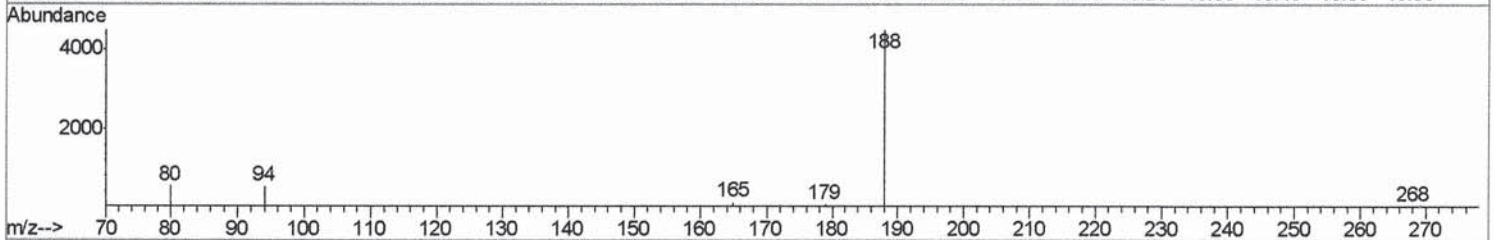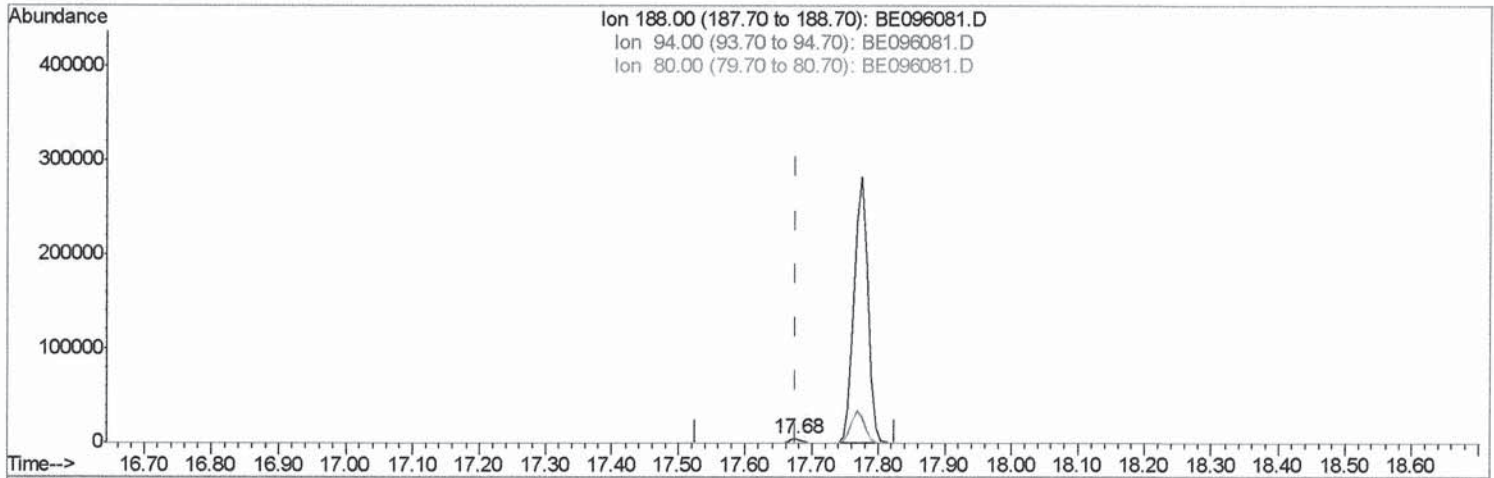

TIC: BE096081.D

(10) Phenanthrene-d10 (I)

17.676min (-0.000) 0.40ng/ul m> SJ 4/27/18

response 6545

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.06
80.00	11.80	12.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

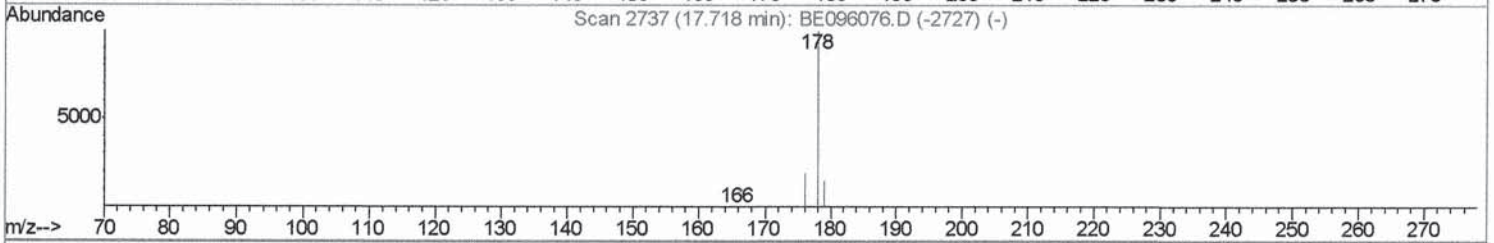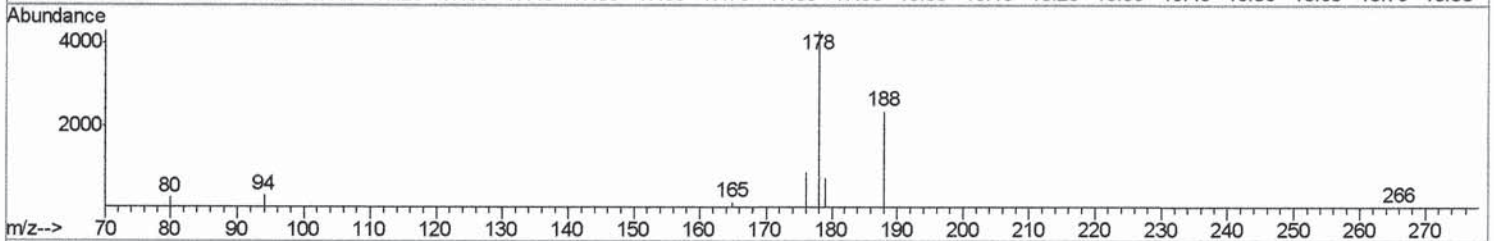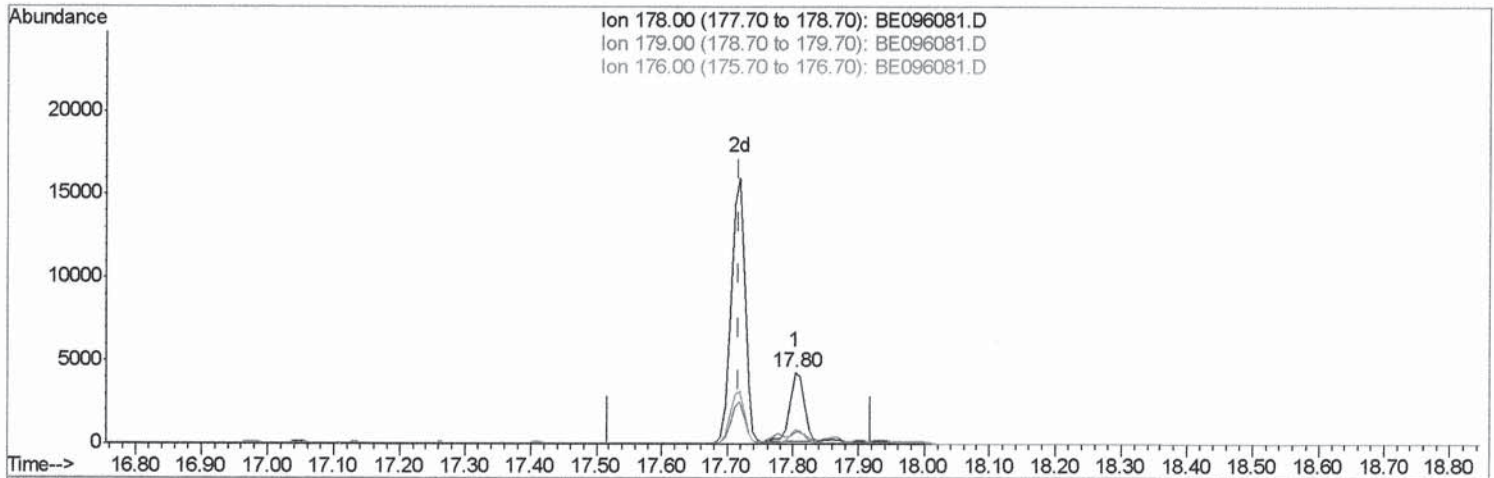

TIC: BE096081.D

(12) Phenanthrene

17.803min (+0.084) 0.32ng/ul

response 6224

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	17.38#
176.00	17.00	20.46#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

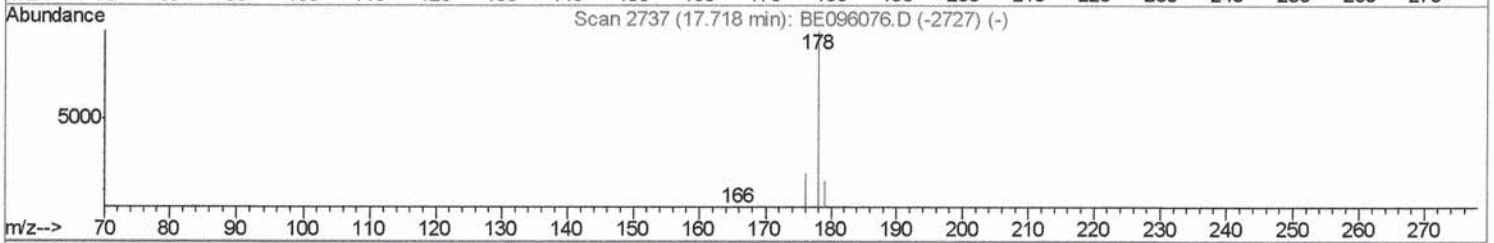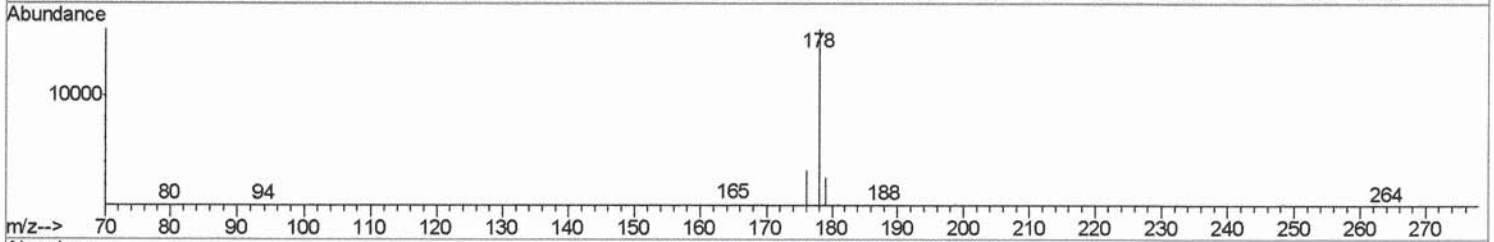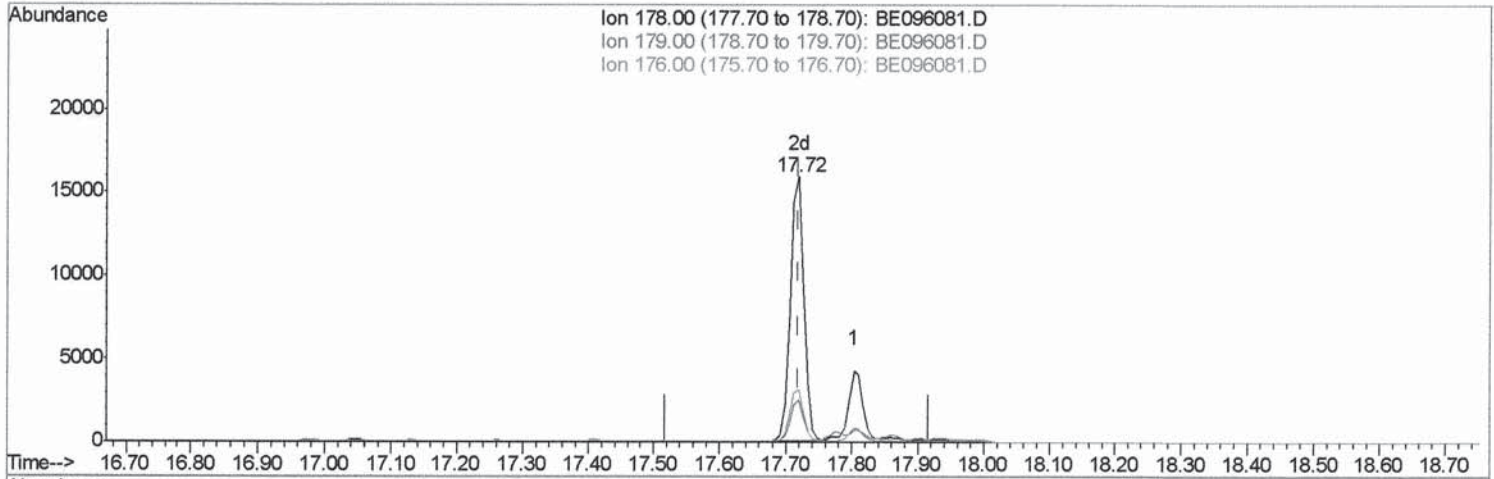

TIC: BE096081.D

(12) Phenanthrene

17.718min (-0.000) 1.18ng/ul m

SJ 4/27/18

response 22840

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.03#
176.00	17.00	19.85
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

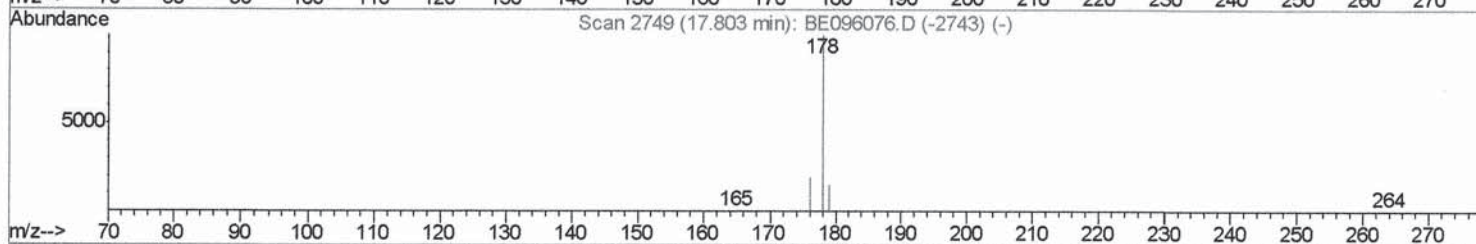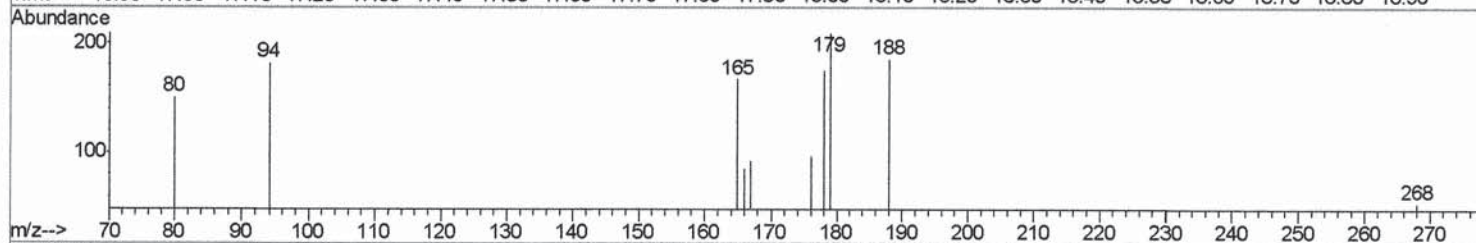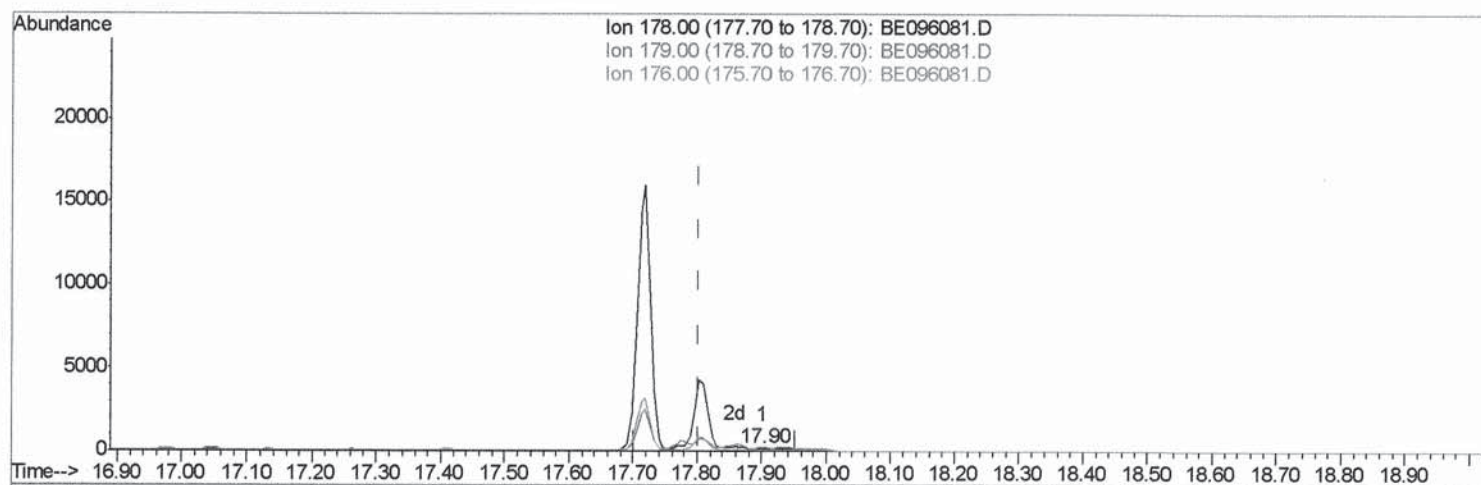

TIC: BE096081.D

(13) Anthracene

17.901min (+0.099) 0.05ng/ul

response 1047

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	119.43#
176.00	18.40	55.43#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

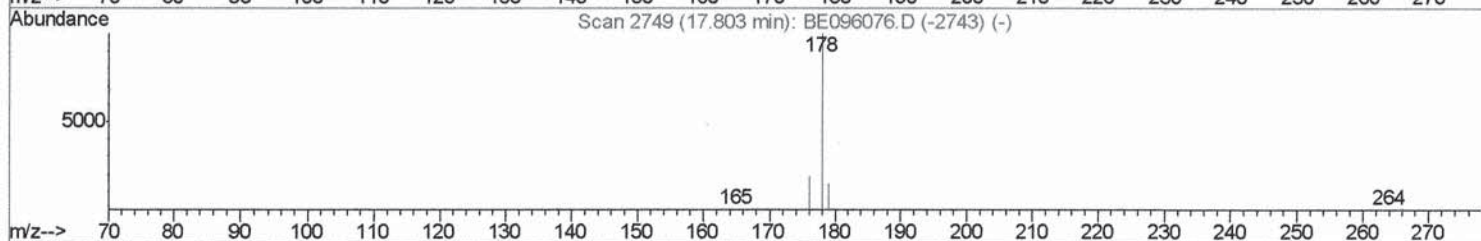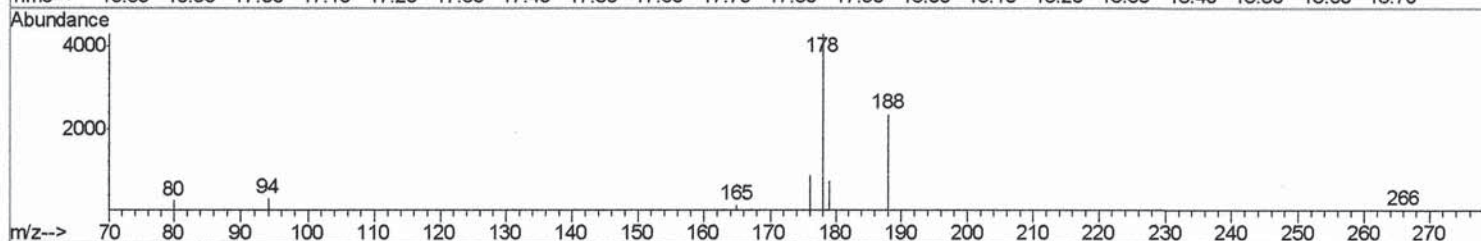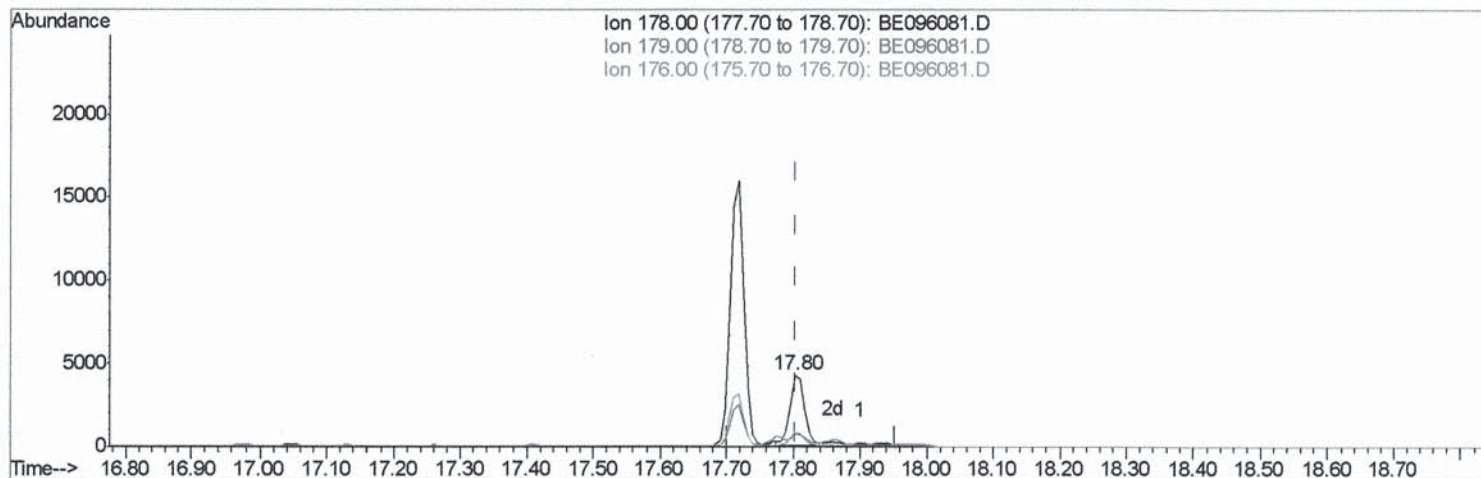

TIC: BE096081.D

(13) Anthracene

17.803min (-0.000) 0.33ng/ul m> SJ 4/23/18

response 6321

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	17.38#
176.00	18.40	20.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

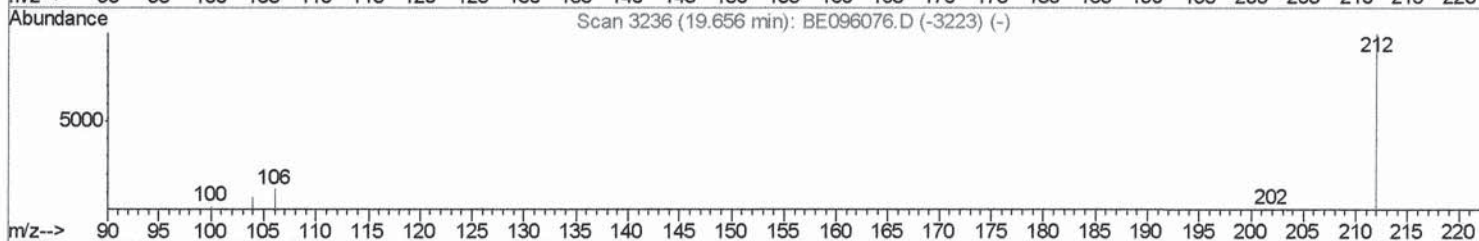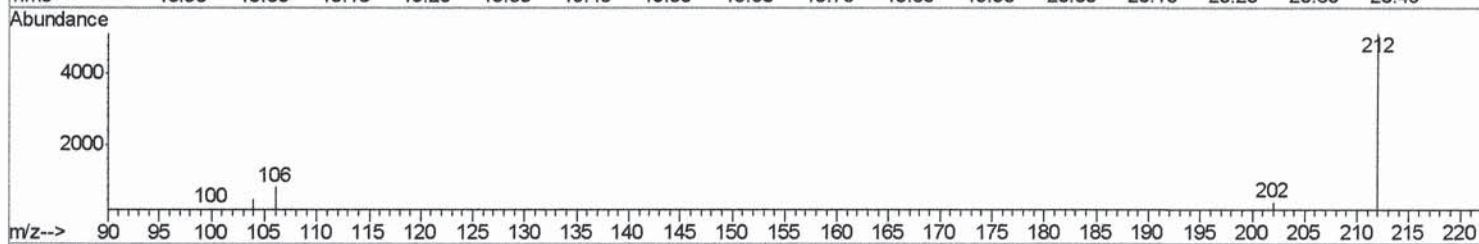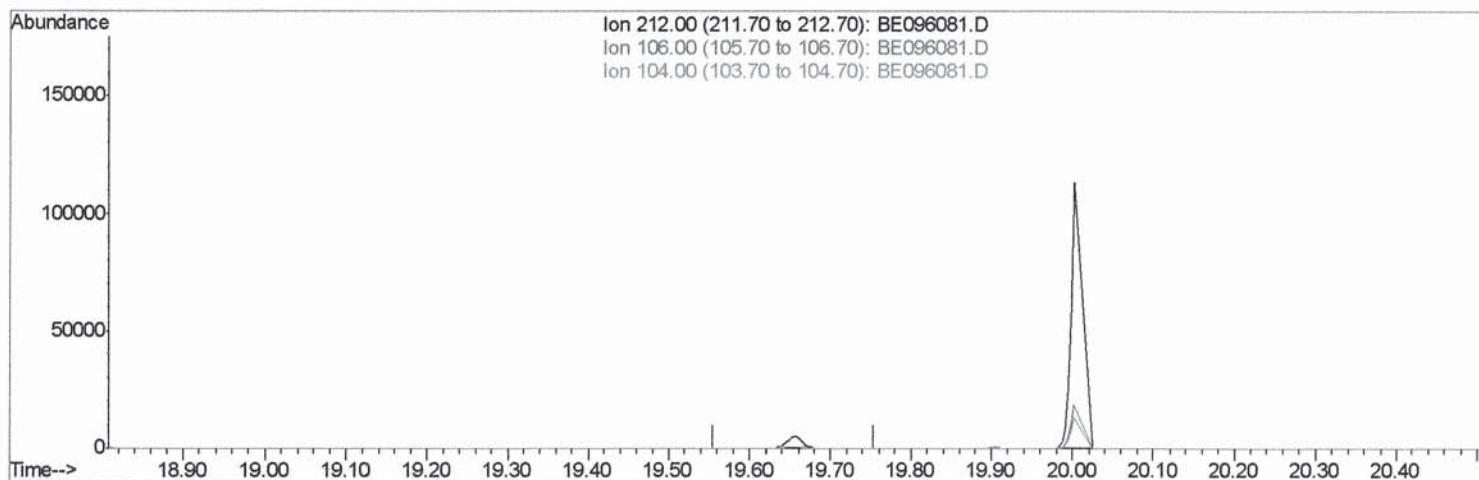

(14) Fluoranthene-d10 (SURR)

19.656min (-19.656) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

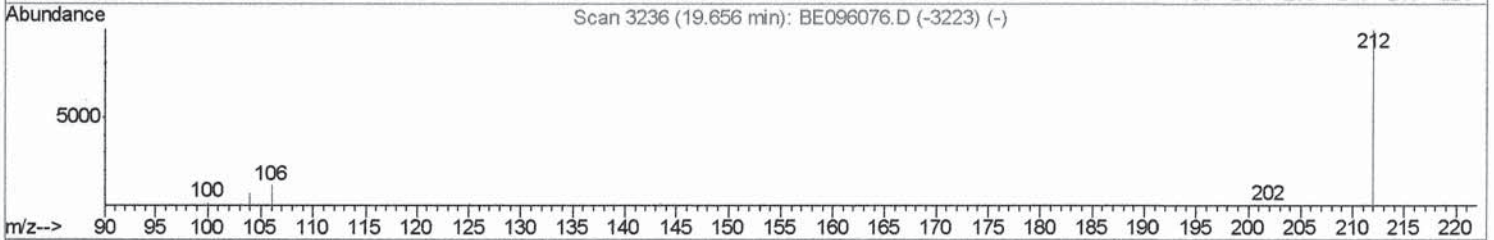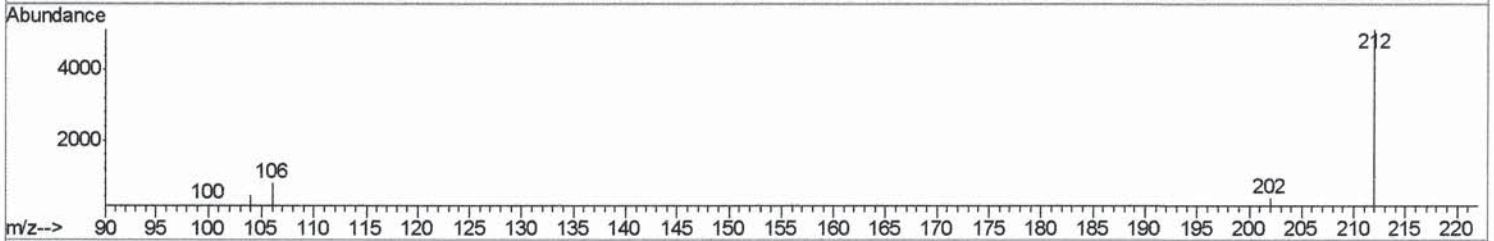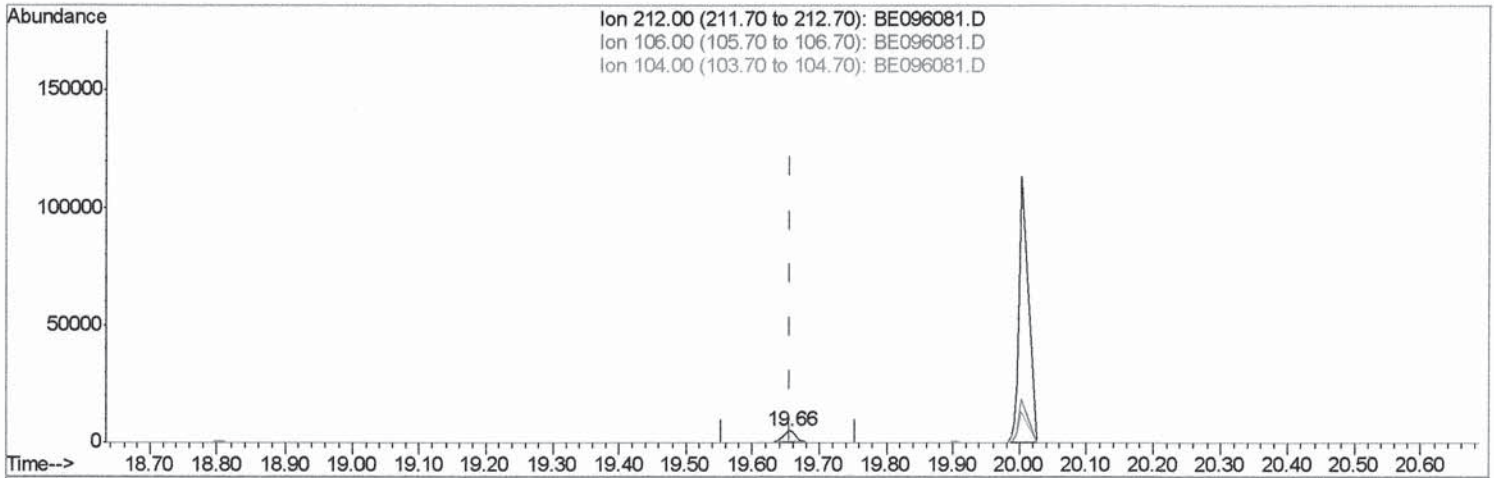

TIC: BE096081.D

(14) Fluoranthene-d10 (SURR)

19.656min (0.000) 0.24ng/ul m > 52 4/24/18

response 6579

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

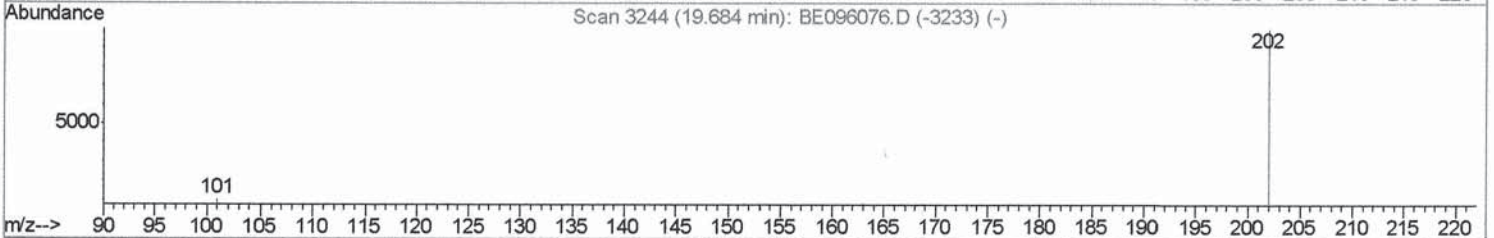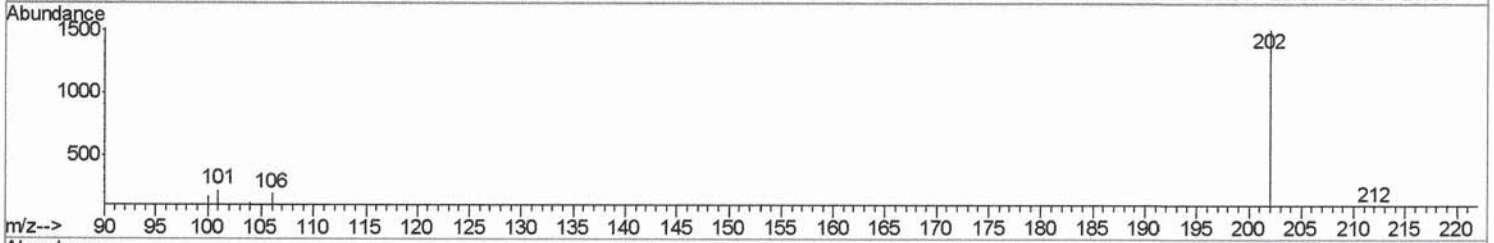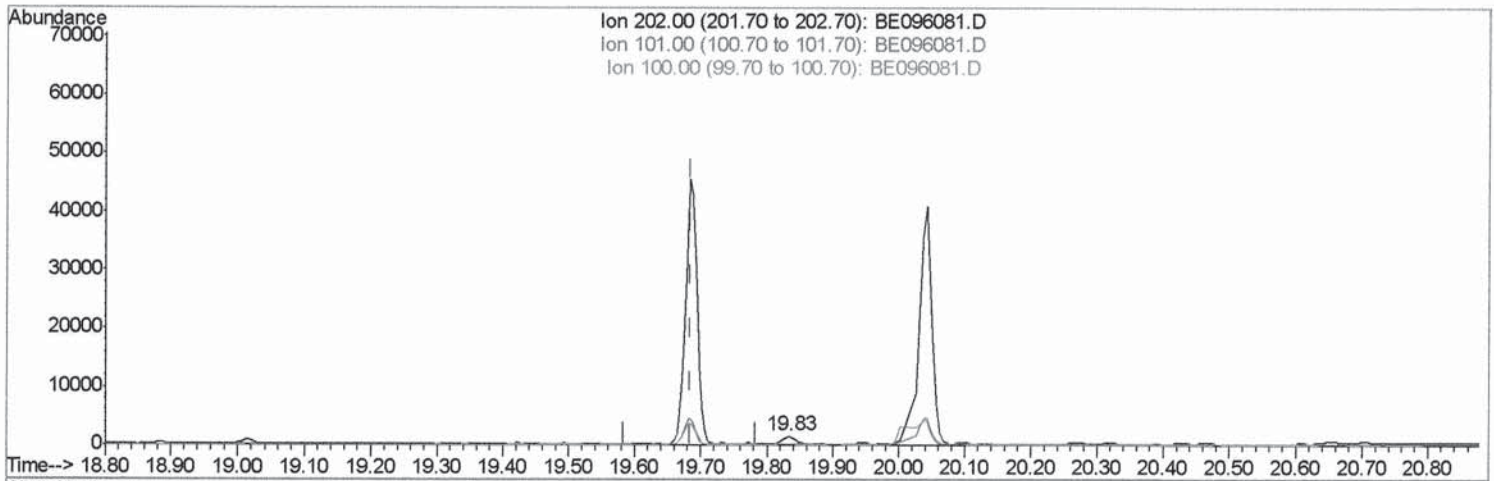

TIC: BE096081.D

(15) Fluoranthene (C)
 19.834min (+0.150) 0.07ng/ul
 response 1855

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	14.70
100.00	19.50	11.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

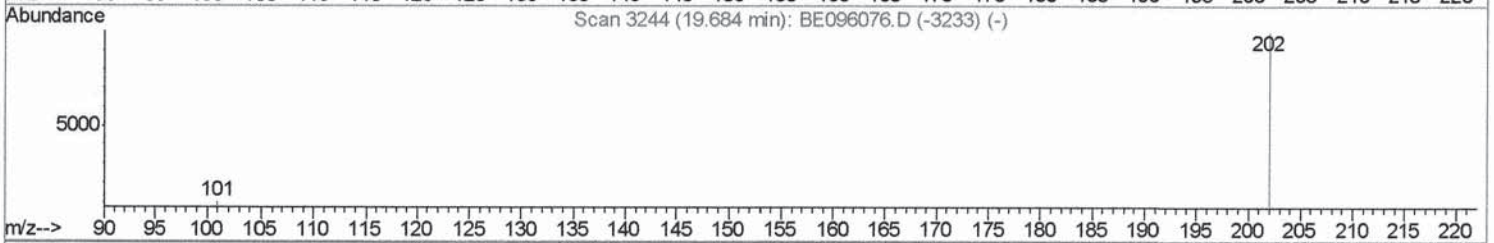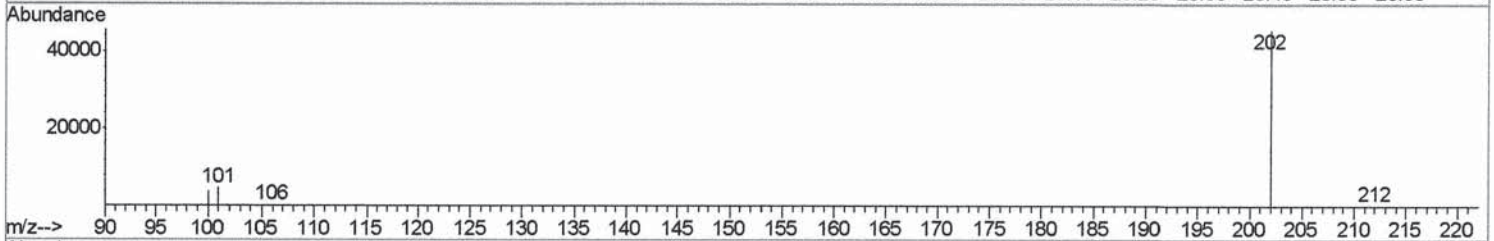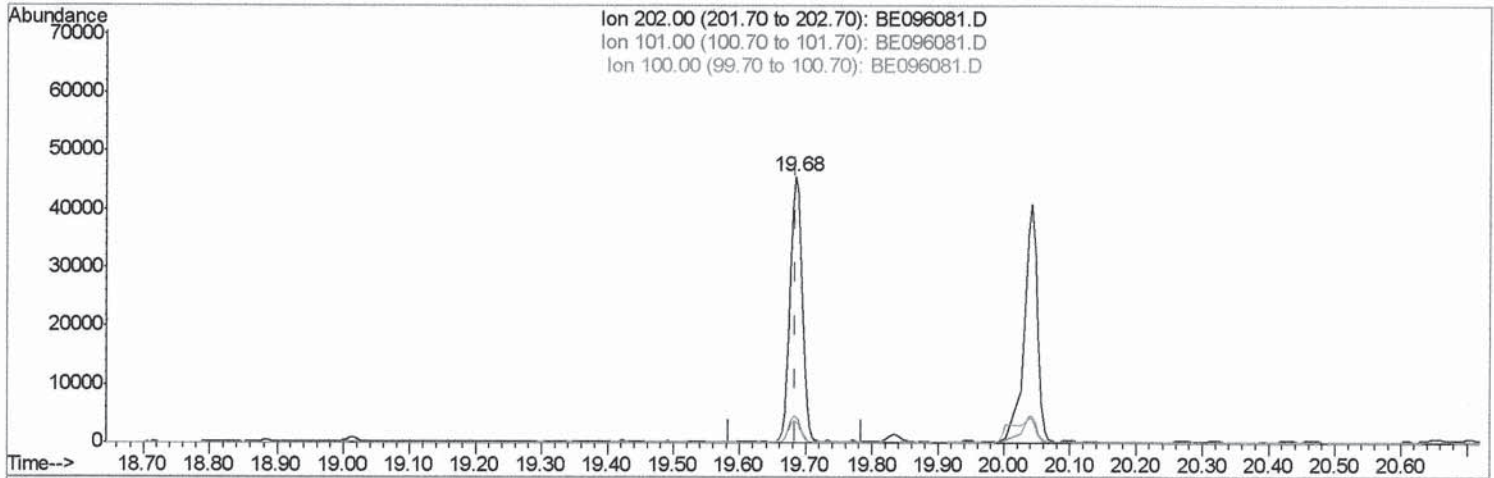

TIC: BE096081.D

(15) Fluoranthene (C)

19.684min (-0.000) 2.25ng/ul m > 5] 4/17/18

response 59042

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.24
100.00	19.50	8.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

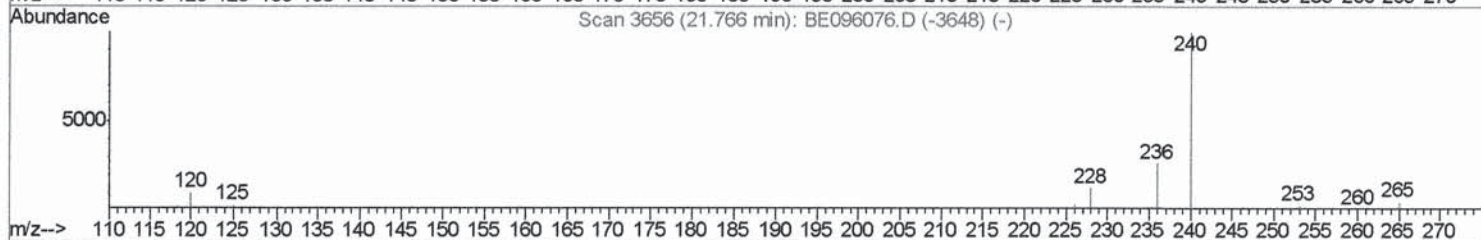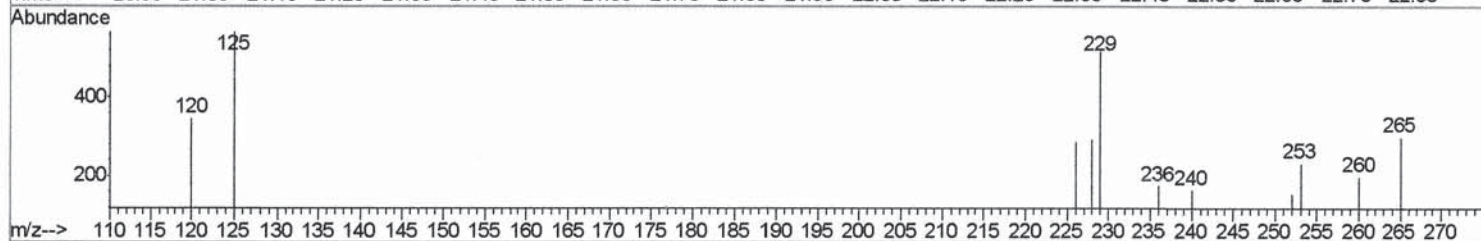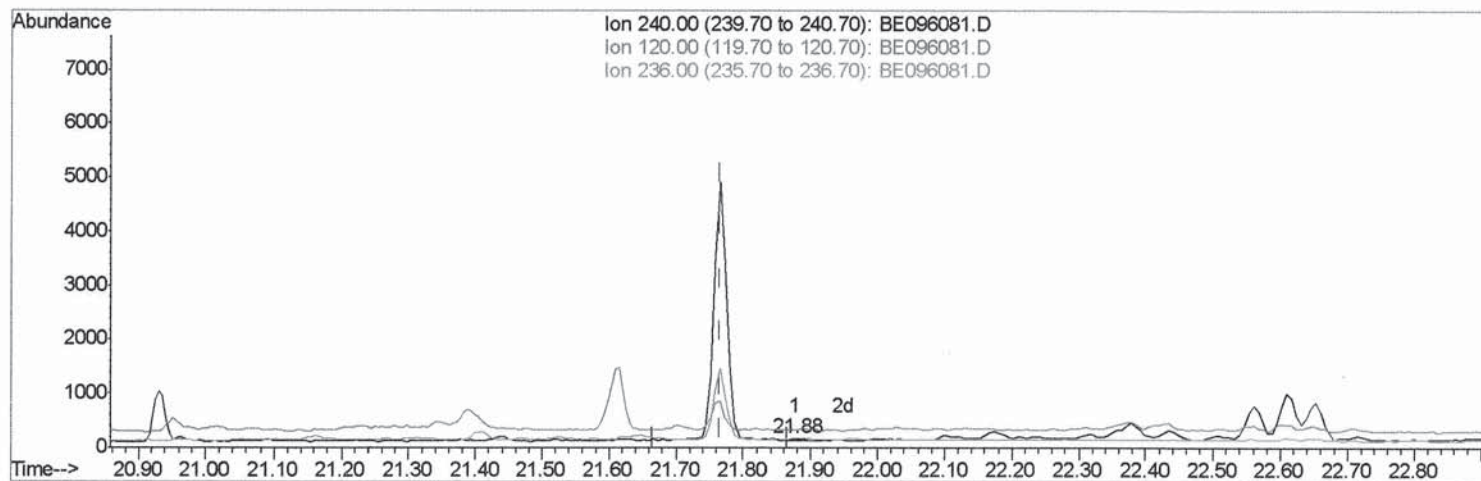

TIC: BE096081.D

(16) Chrysene-d12 (I)

21.878min (+0.112) 0.40ng/ul

response 39

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	209.70#
236.00	34.90	106.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:53:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

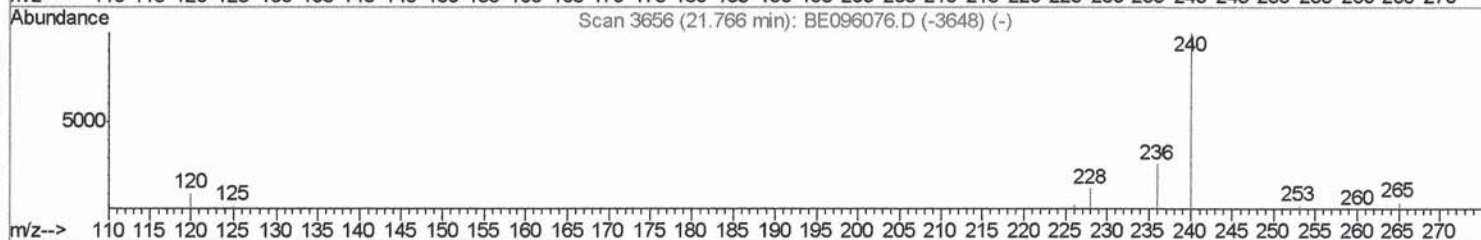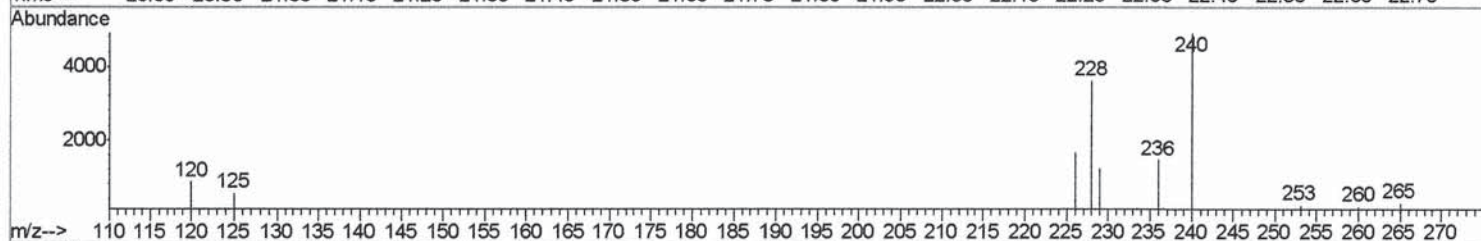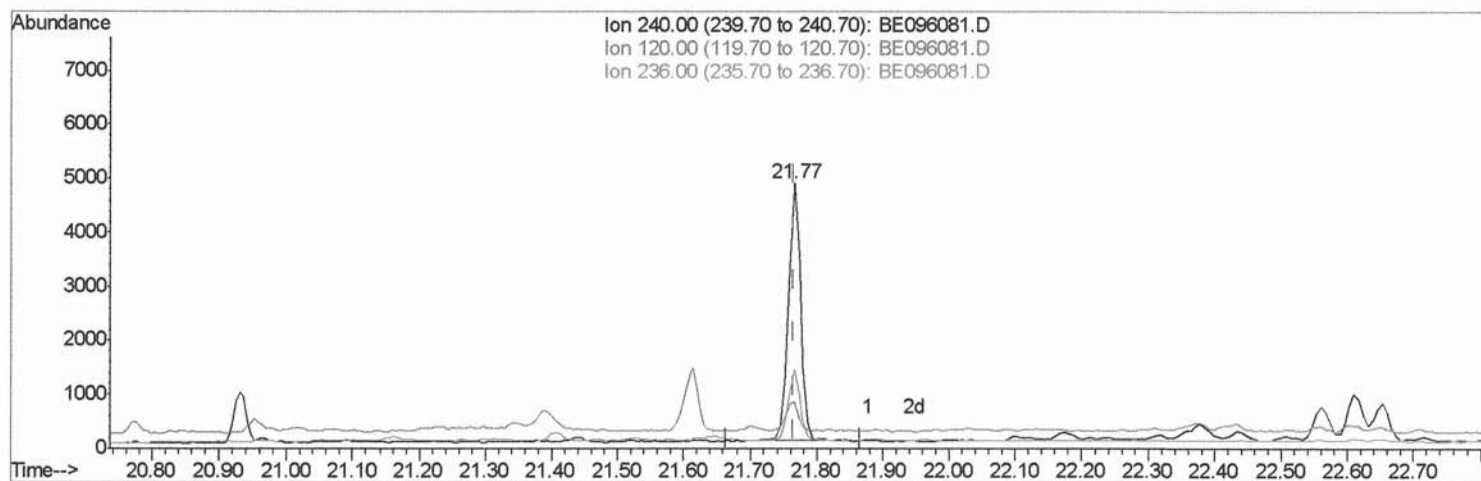

TIC: BE096081.D

(16) Chrysene-d12 (I)

21.766min (-0.000) 0.40ng/ul m > SJ 4/23/18

response 6185

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	17.73
236.00	34.90	29.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

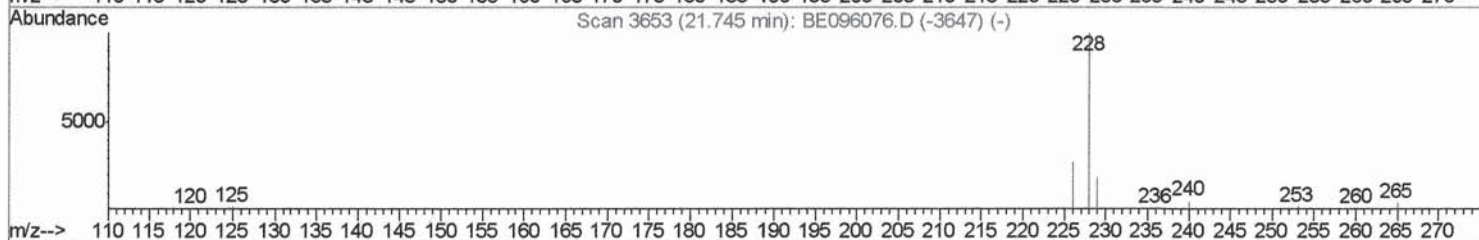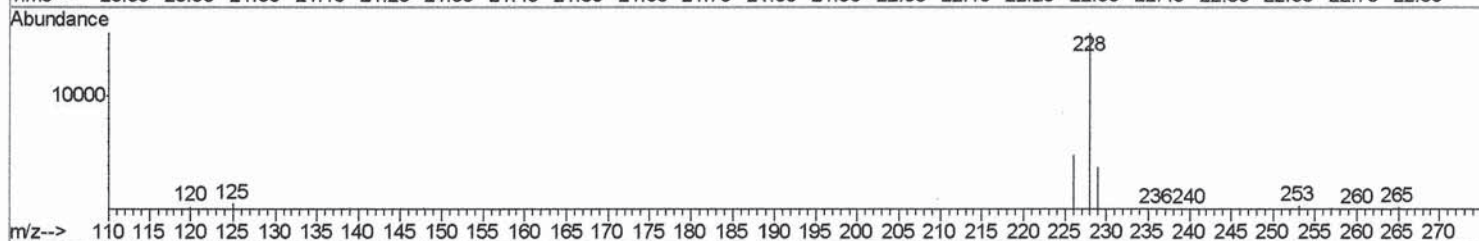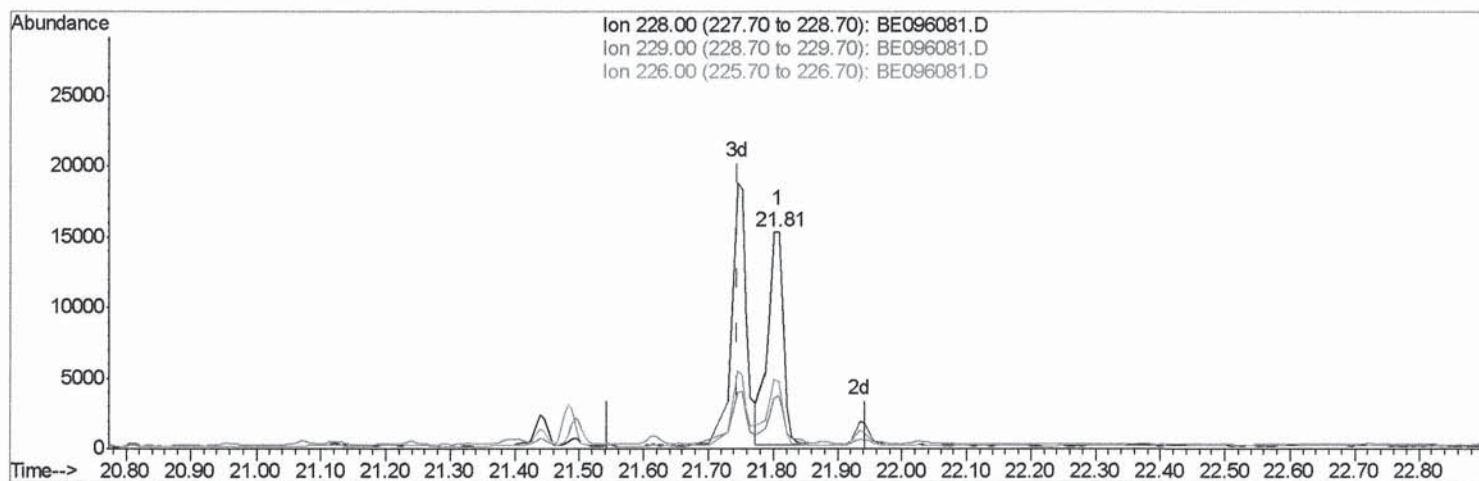

TIC: BE096081.D

(18) Benzo(a)anthracene

21.808min (+0.063) 1.04ng/ul

response 25938

Ion	Exp%	Act%
-----	------	------

228.00	100	100
--------	-----	-----

229.00	28.50	24.56
--------	-------	-------

226.00	21.30	31.28#
--------	-------	--------

0.00	0.00	0.00
------	------	------

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

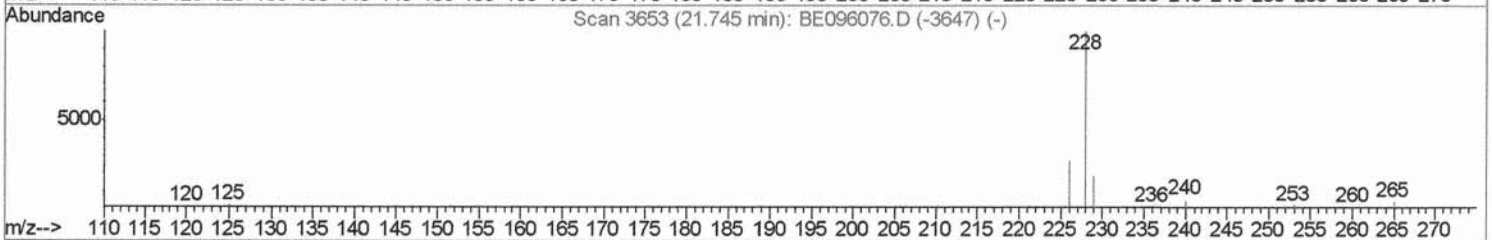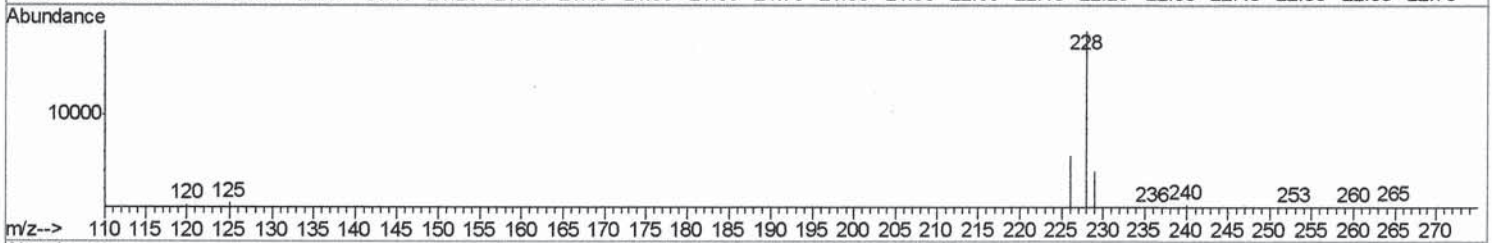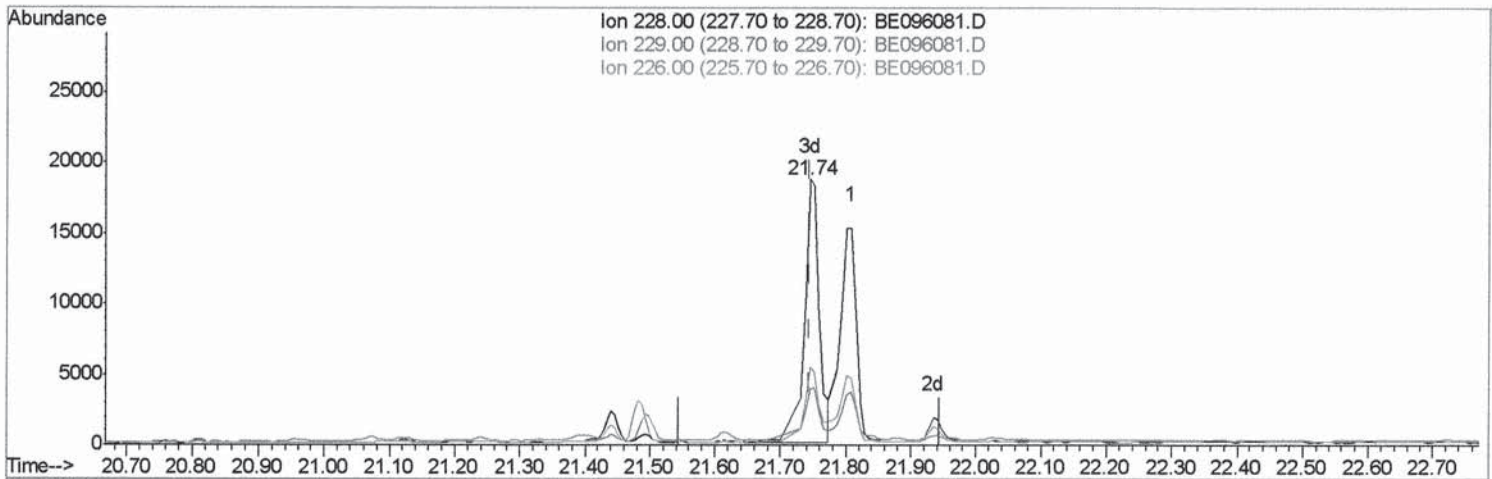

TIC: BE096081.D

(18) Benzo(a)anthracene

21.744min (-0.000) 1.30ng/ul m > SJ 4/27/18

response 32359

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	21.21#
226.00	21.30	29.61#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

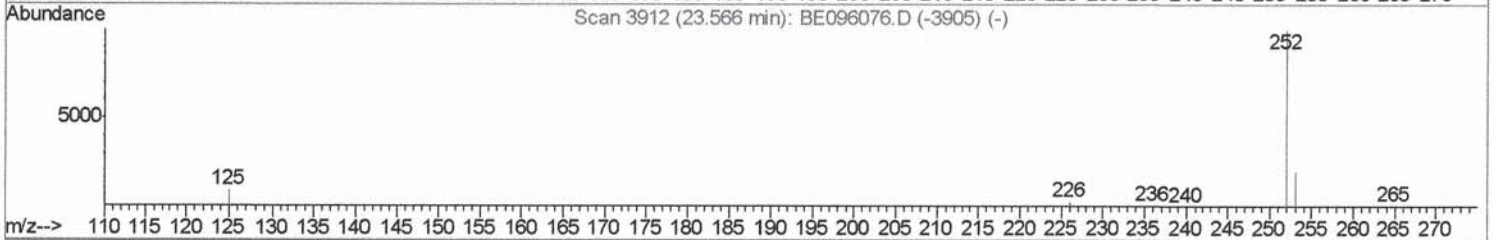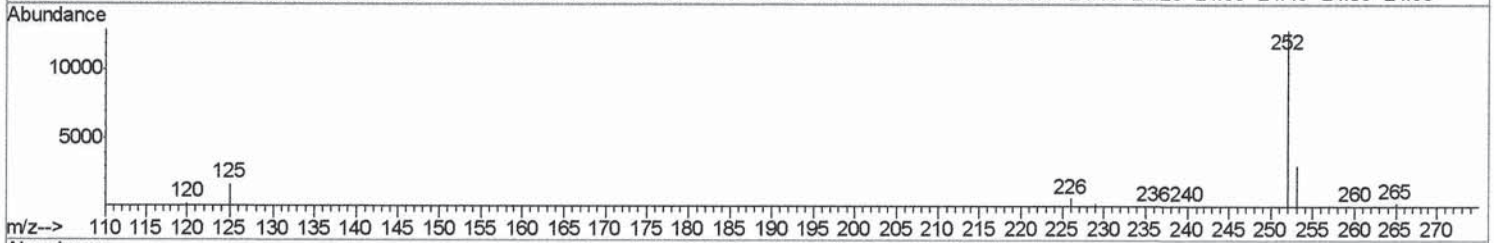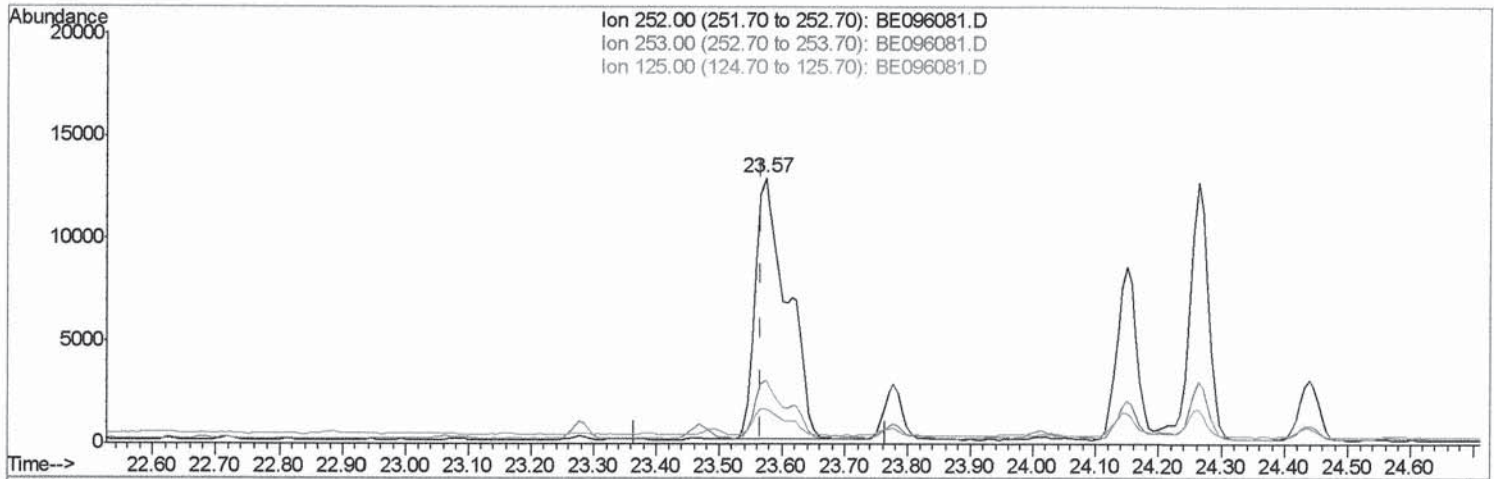

TIC: BE096081.D

(21) Benzo(b)fluoranthene

23.573min (+0.007) 1.78ng/ul

response 44922

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.99
125.00	17.50	13.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

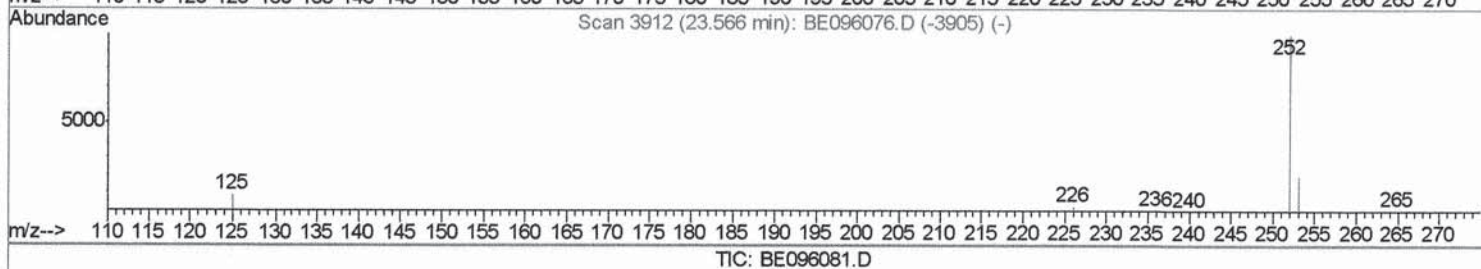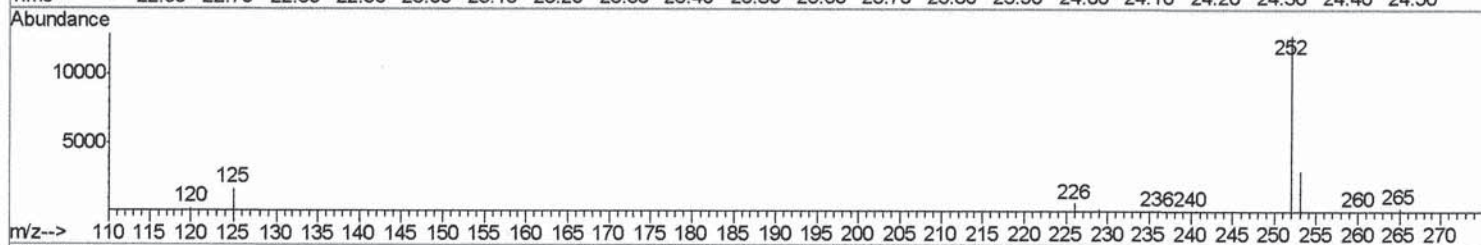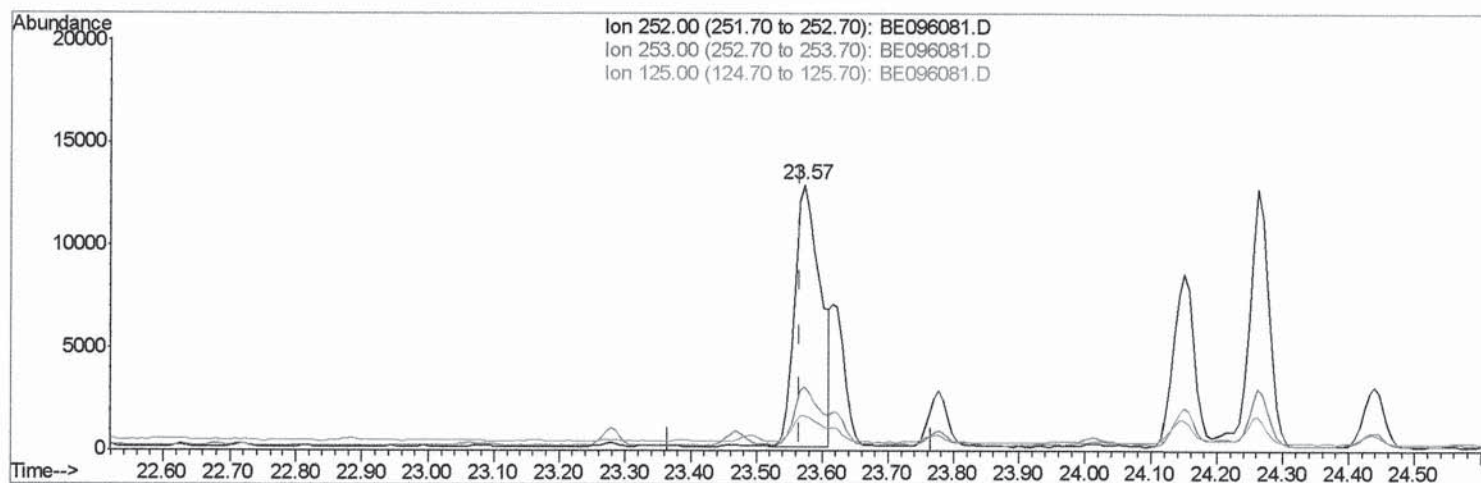

(21) Benzo(b)fluoranthene

23.573min (+0.007) 1.38ng/ul m> SJ 4/27/18

response 34876

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.99
125.00	17.50	13.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

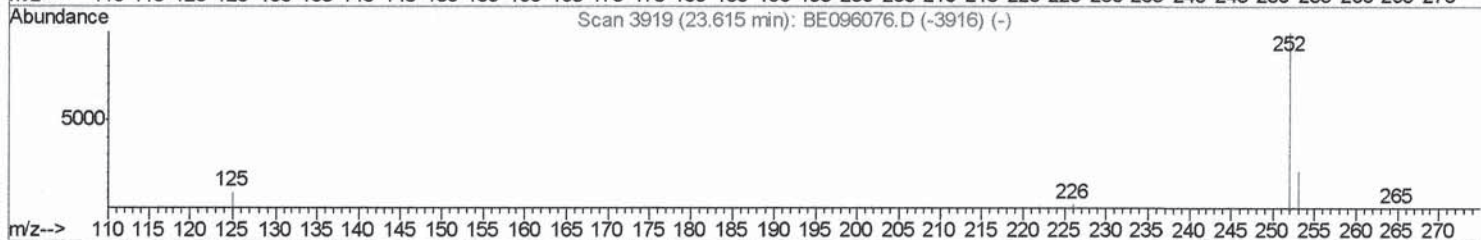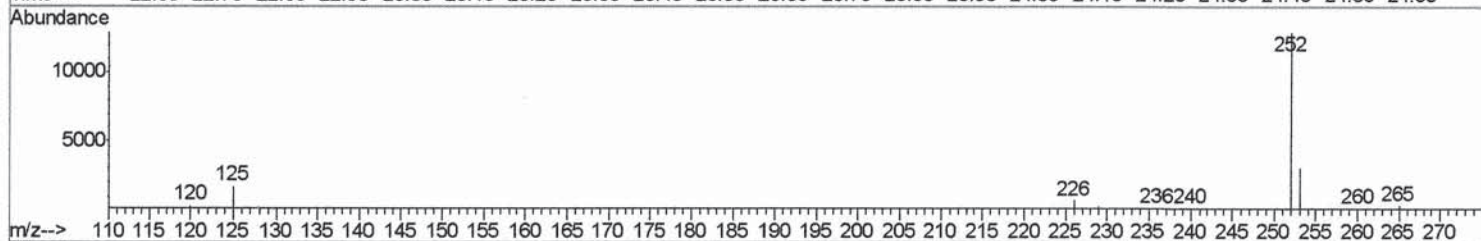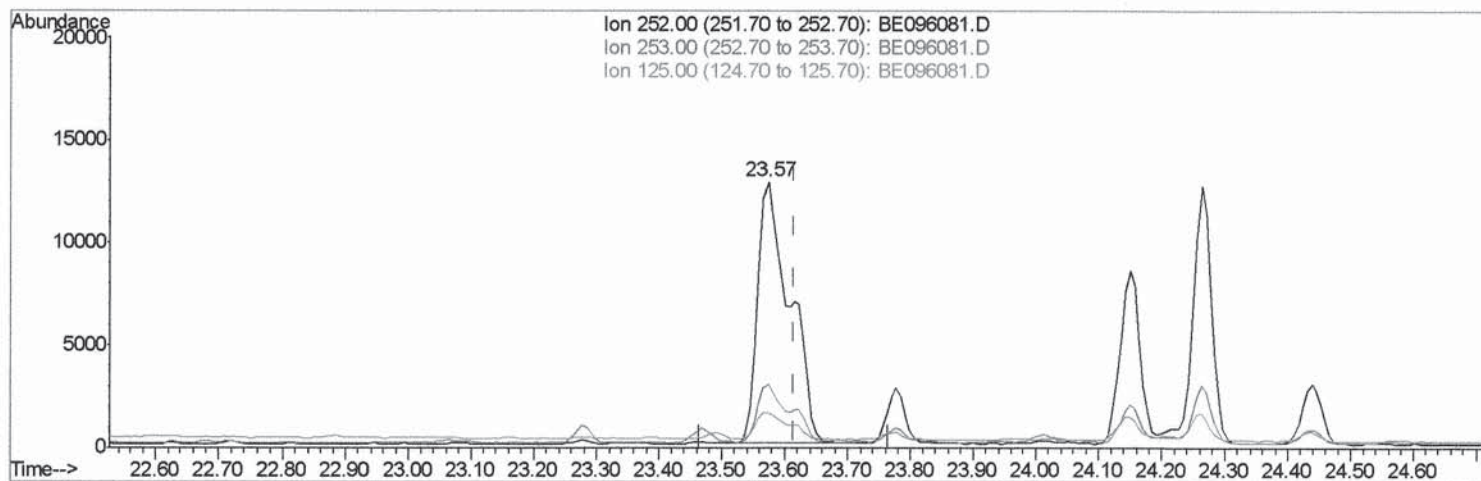

TIC: BE096081.D

(22) Benzo(k)fluoranthene

23.573min (-0.043) 1.79ng/ul

response 44922

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.99#
125.00	17.10	13.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096081.D
Acq On : 23 Apr 2018 12:48
Operator : SJ/JU
Sample : J2355-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y33

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:48 PM

Quant Time: Apr 24 05:57:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

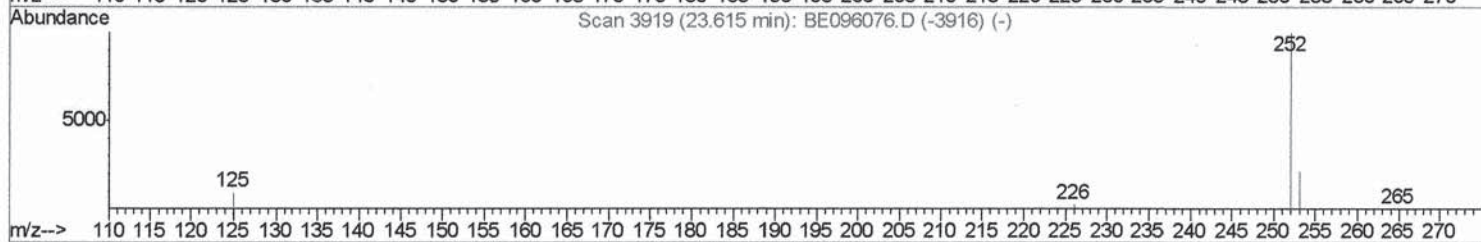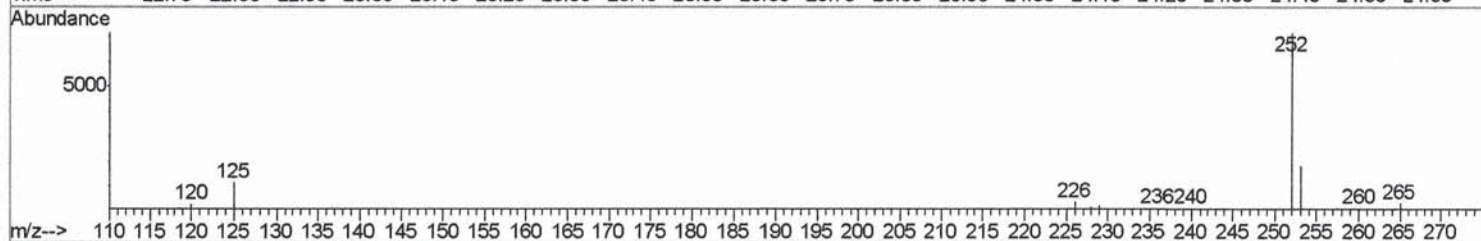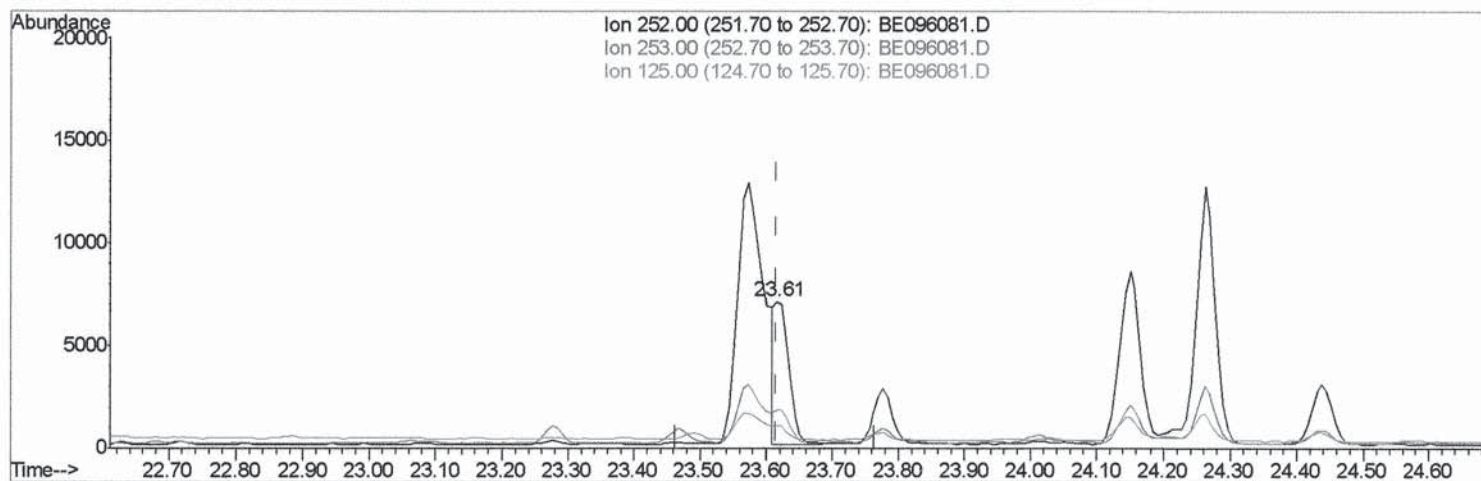

TIC: BE096081.D

(22) Benzo(k)fluoranthene

23.615min (-0.000) 0.40ng/ul m > SJ 4/27/18

response 10092

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.01
125.00	17.10	16.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096081.D
 Acq On : 23 Apr 2018 12:48
 Operator : SJ/JU
 Sample : J2355-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y33

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:48 PM

Quant Time: Apr 24 06:17:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1852	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5346	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3039	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6545m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6185m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	7794	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.76	152	2651	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	6579m	0.24	ng/ul	0.00

Target Compounds

Ovalue

3) Naphthalene	11.25	128	1702	0.114	ng/ul#	89
5) 2-Methylnaphthalene	12.83	142	424	0.042	ng/ul	99
7) Acenaphthylene	14.70	152	2452	0.156	ng/ul	95
8) Acenaphthene	15.03	153	859	0.076	ng/ul#	94
9) Fluorene	15.99	166	1153	0.090	ng/ul	91
12) Phenanthrene	17.72	178	22840m	1.184	ng/ul	
13) Anthracene	17.80	178	6321m	0.329	ng/ul	
15) Fluoranthene	19.68	202	59042m	2.249	ng/ul	
17) Pyrene	20.04	202	58409	2.779	ng/ul#	79
18) Benzo(a)anthracene	21.74	228	32359m	1.295	ng/ul	
19) Chrysene	21.81	228	25915	1.441	ng/ul	96
21) Benzo(b)fluoranthene	23.57	252	34876m	1.383	ng/ul	
22) Benzo(k)fluoranthene	23.61	252	10092m	0.402	ng/ul	
23) Benzo(a)pyrene	24.26	252	26316	1.081	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	27.17	276	16879	0.624	ng/ul#	74
25) Dibenzo(a,h)anthracene	27.17	278	4297	0.197	ng/ul	95
26) Benzo(a,h,i)perylene	28.04	276	13056	0.578	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed