


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:44:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

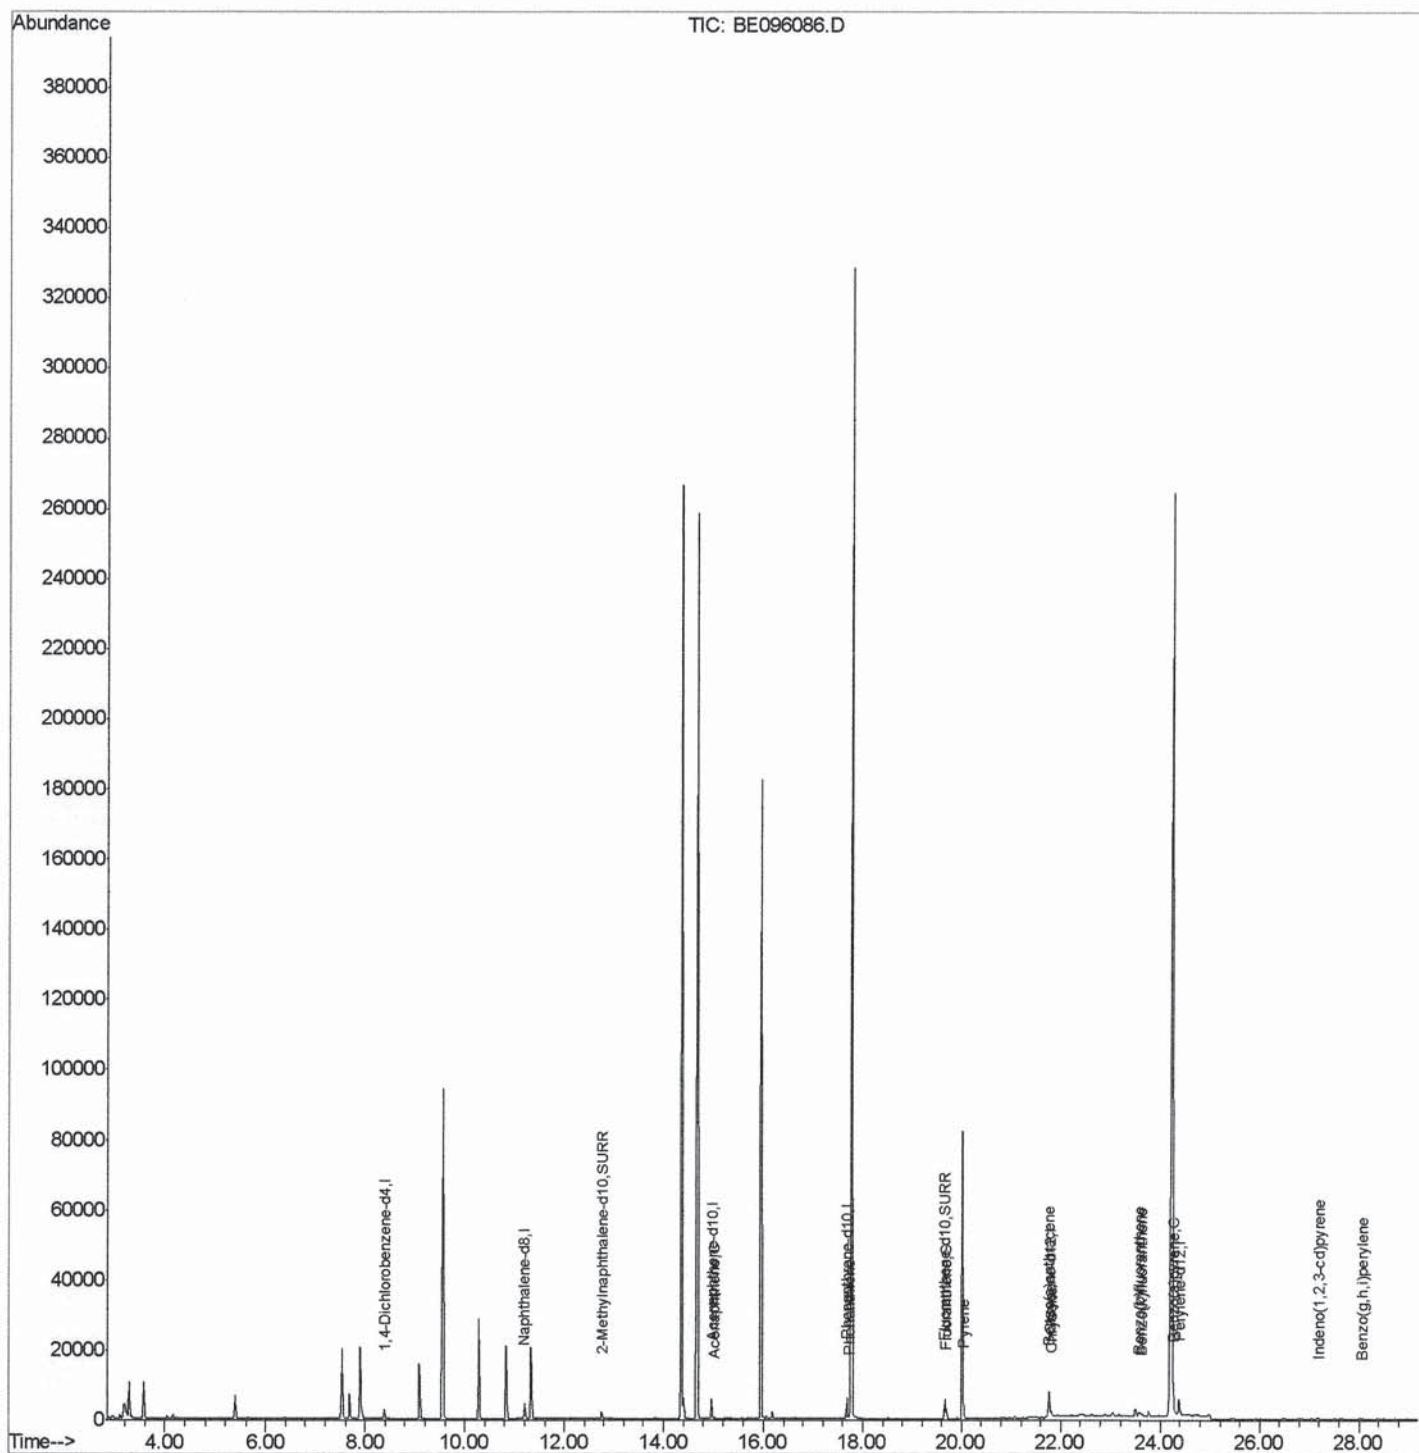

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 05:23:13 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

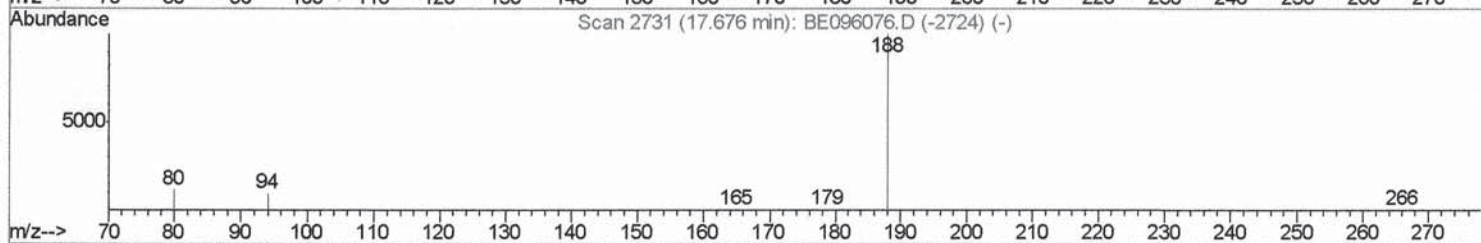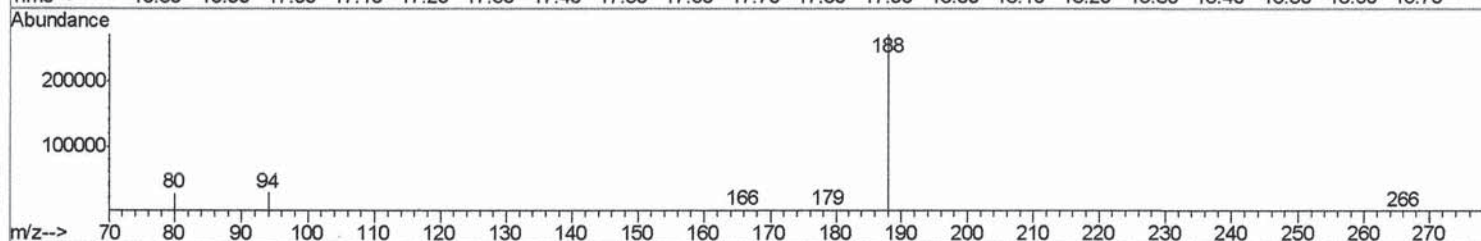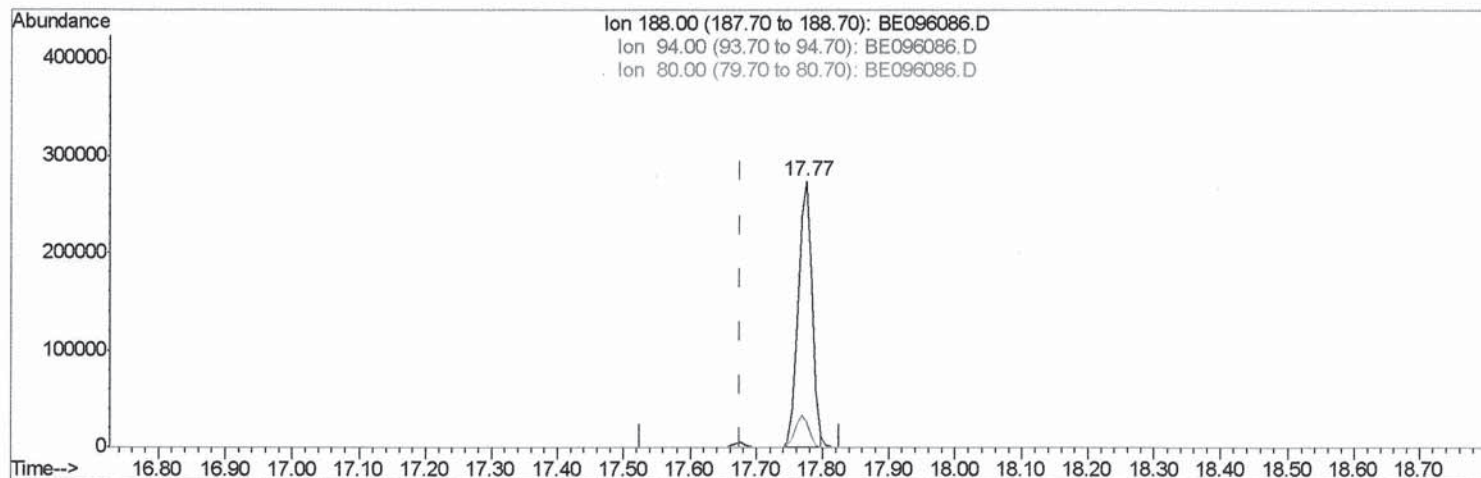

TIC: BE096086.D

(10) Phenanthrene-d10 (I)

17.775min (+0.098) 0.40ng/ul

response 389127

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.18
80.00	11.80	9.63
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 05:23:13 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

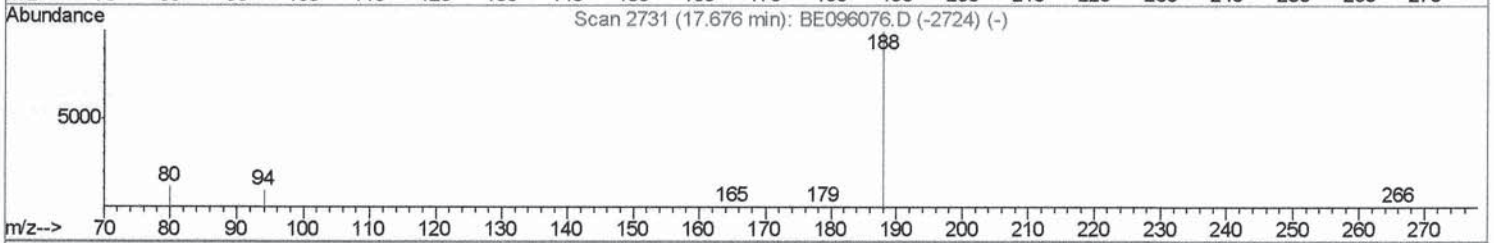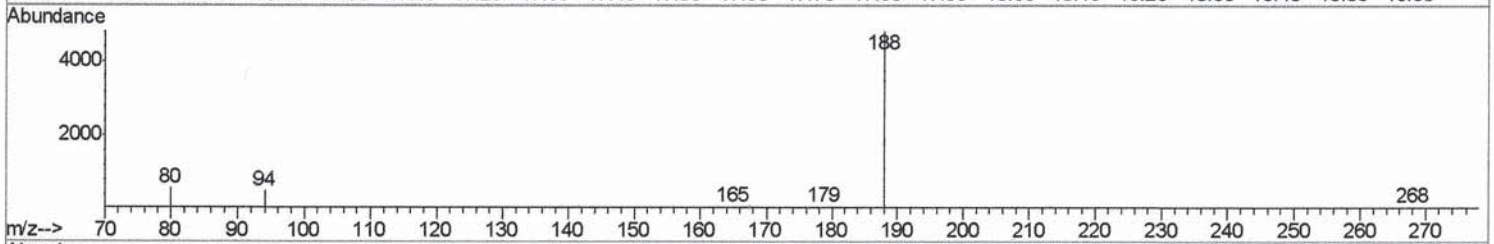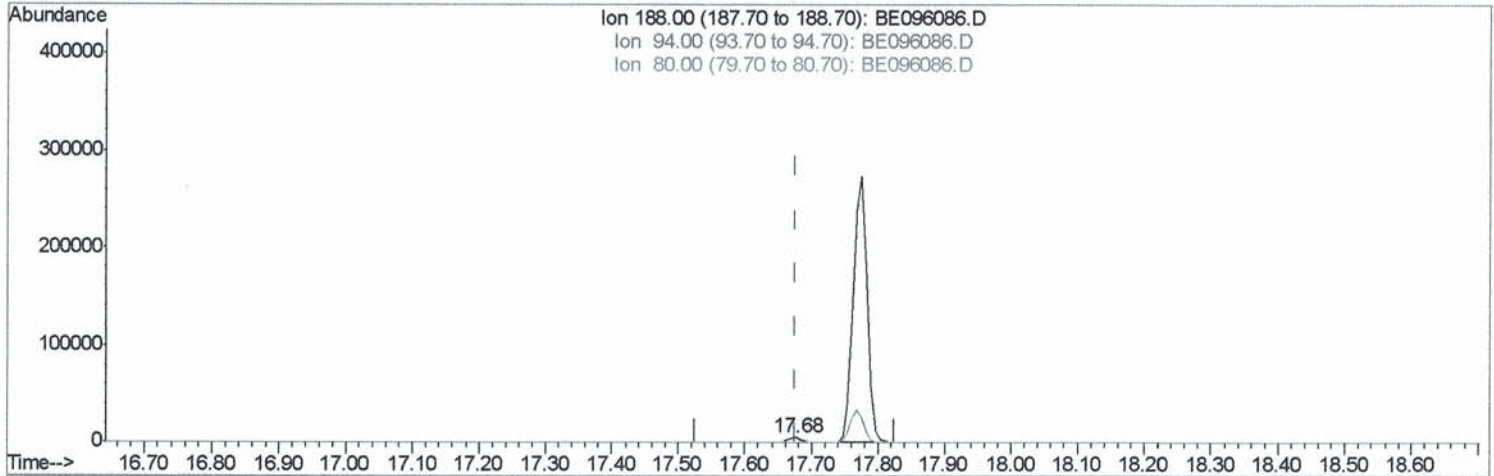

TIC: BE096086.D

(10) Phenanthrene-d10 (I)

17.676min (-0.000) 0.40ng/ul m> SJ 4/23/18

response 6818

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.21
80.00	11.80	11.62
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

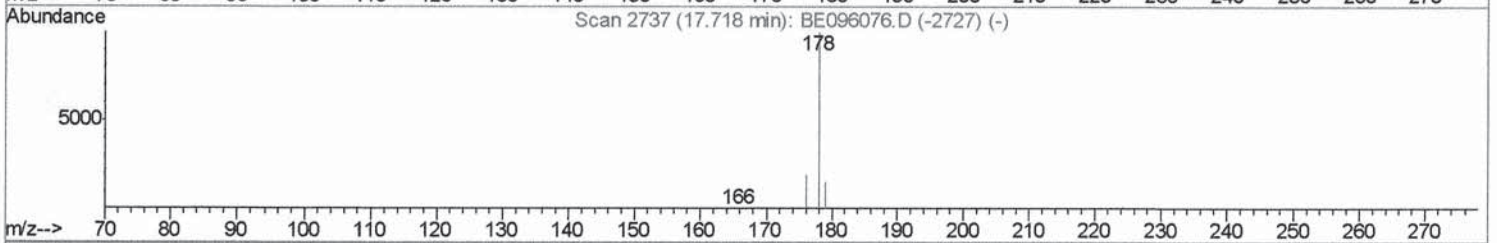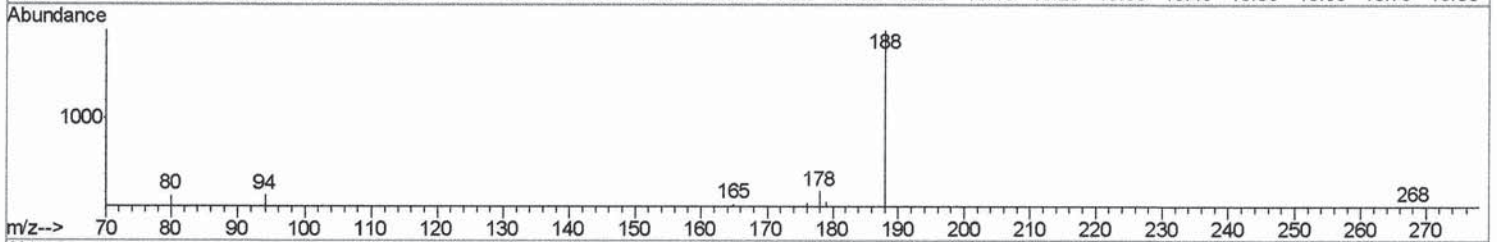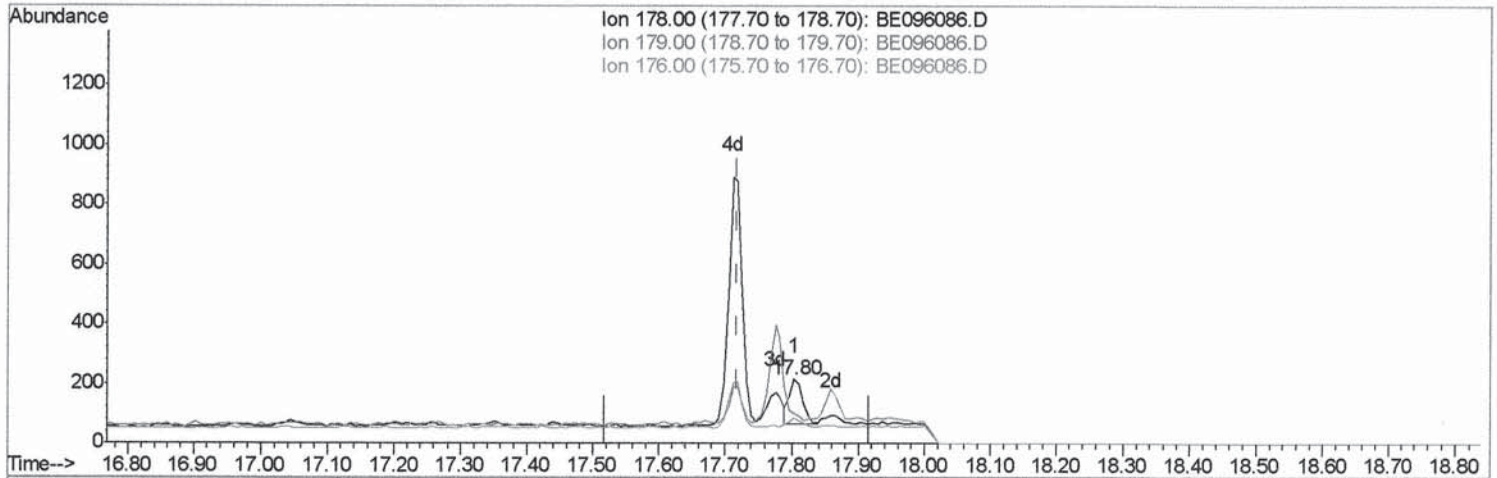

TIC: BE096086.D

(12) Phenanthrene

17.803min (+0.084) 0.01ng/ul

response 207

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	46.95#
176.00	17.00	40.85#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

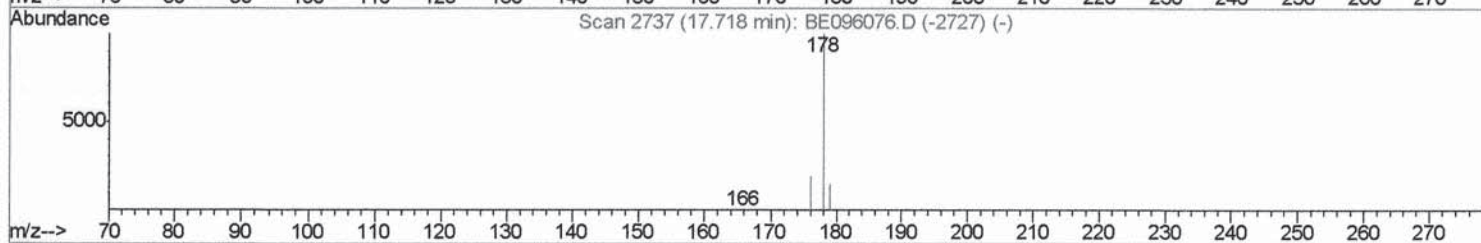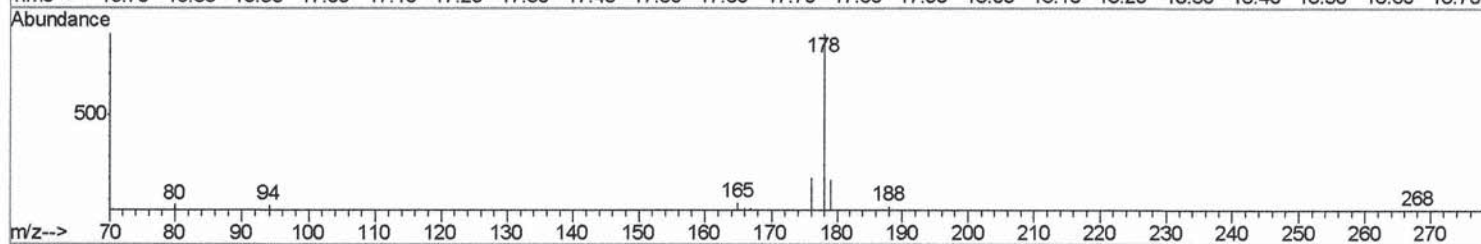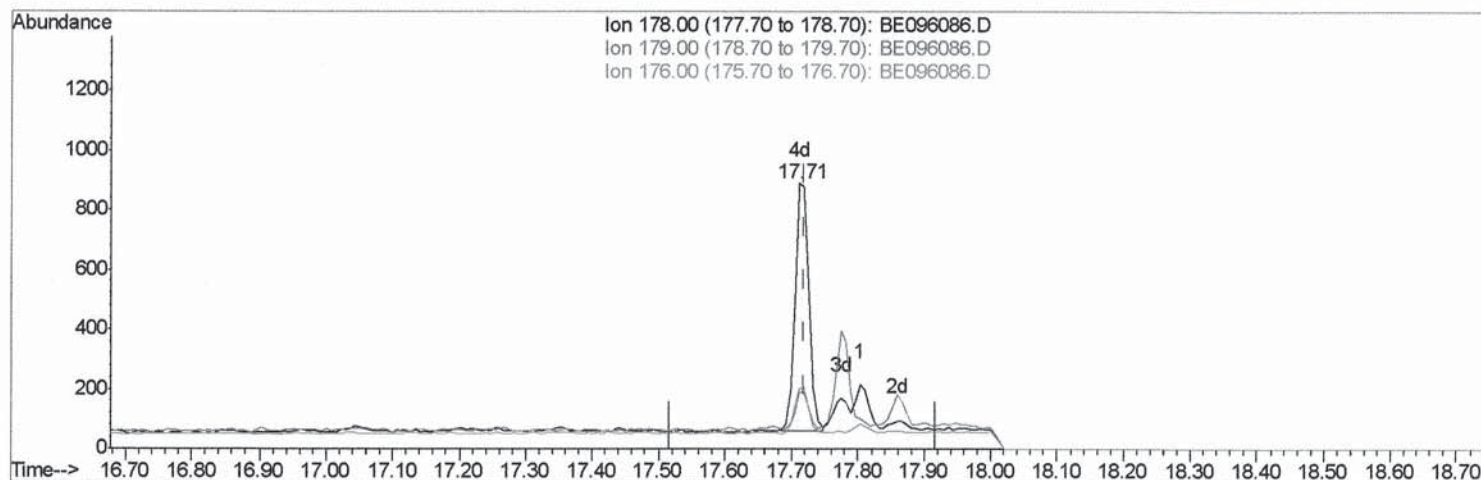

TIC: BE096086.D

(12) Phenanthrene

17.711min (-0.007) 0.06ng/ul m > 52 4/27/18

response 1235

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	21.60
176.00	17.00	22.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

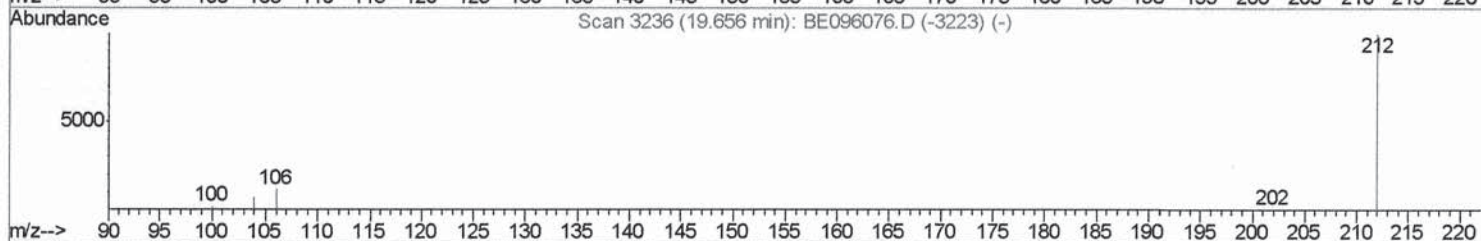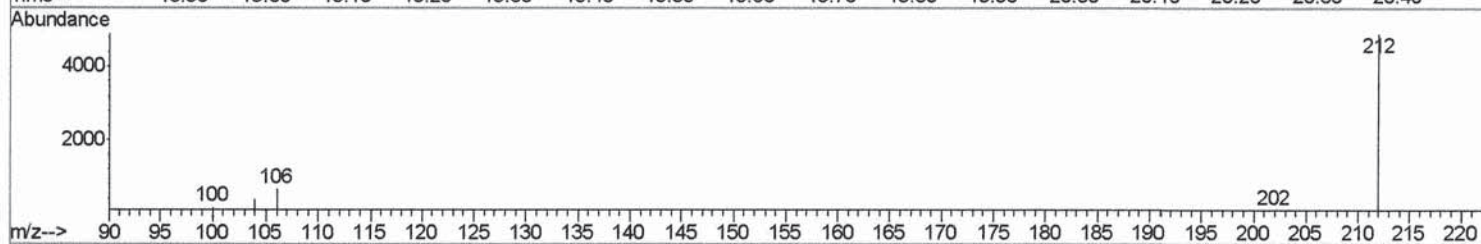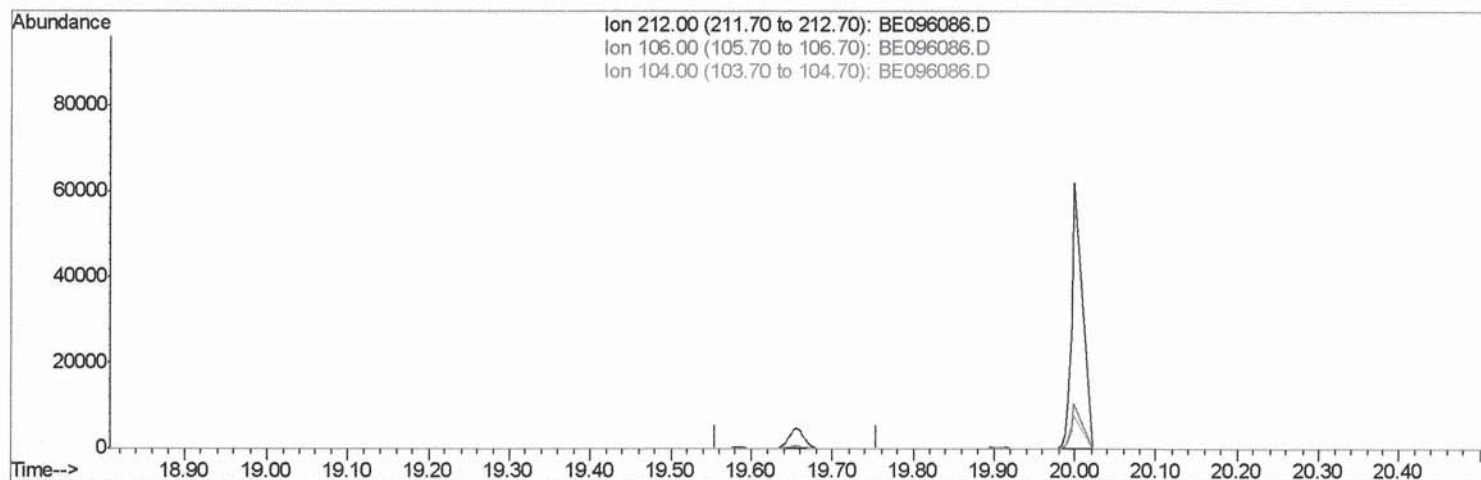

TIC: BE096086.D

(14) Fluoranthene-d10 (SURR)

19.656min (-19.656) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

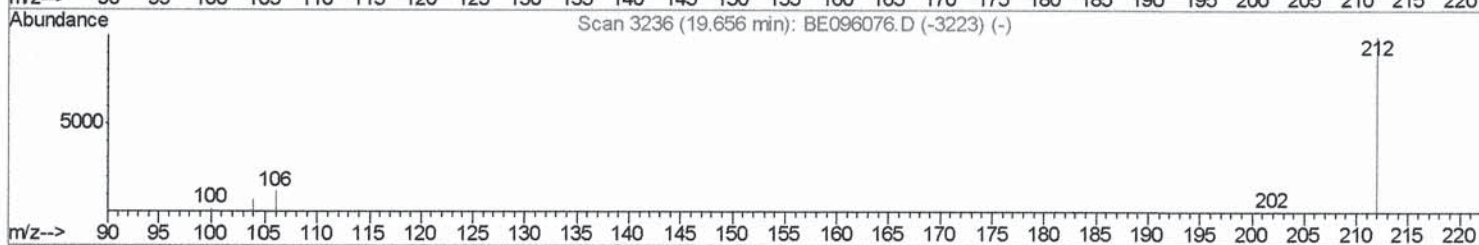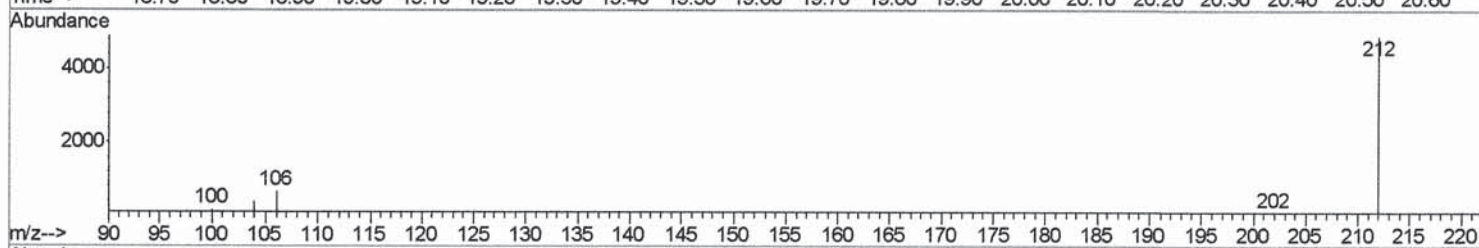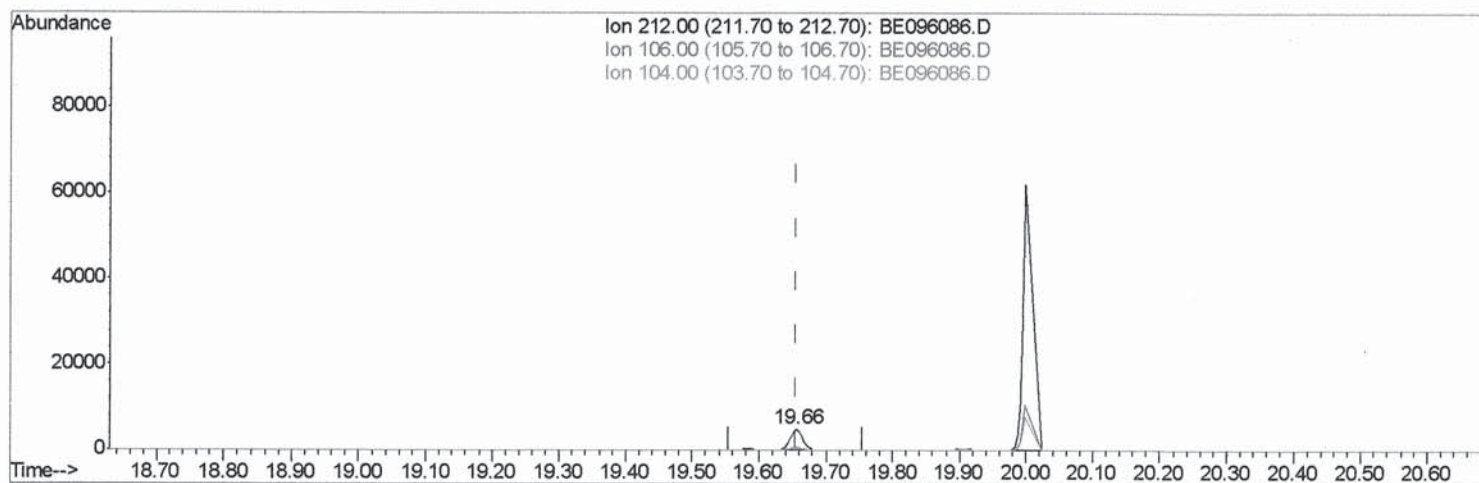

TIC: BE096086.D

(14) Fluoranthene-d10 (SURR)

19.656min (-0.000) 0.22ng/ul m > SJ 4/27/18

response 6108

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

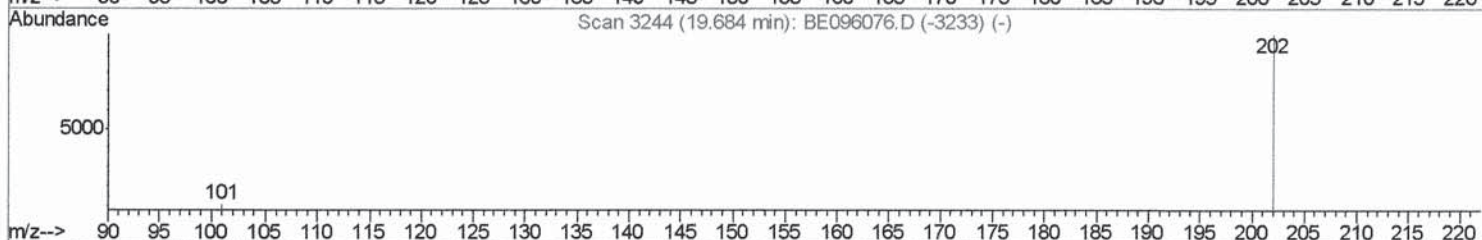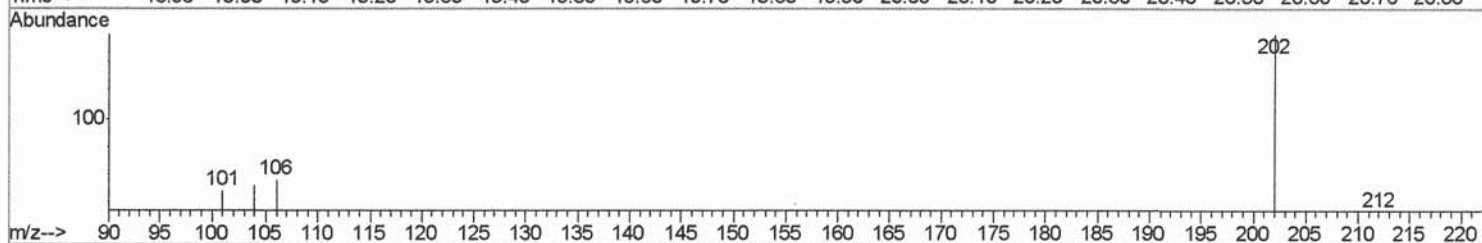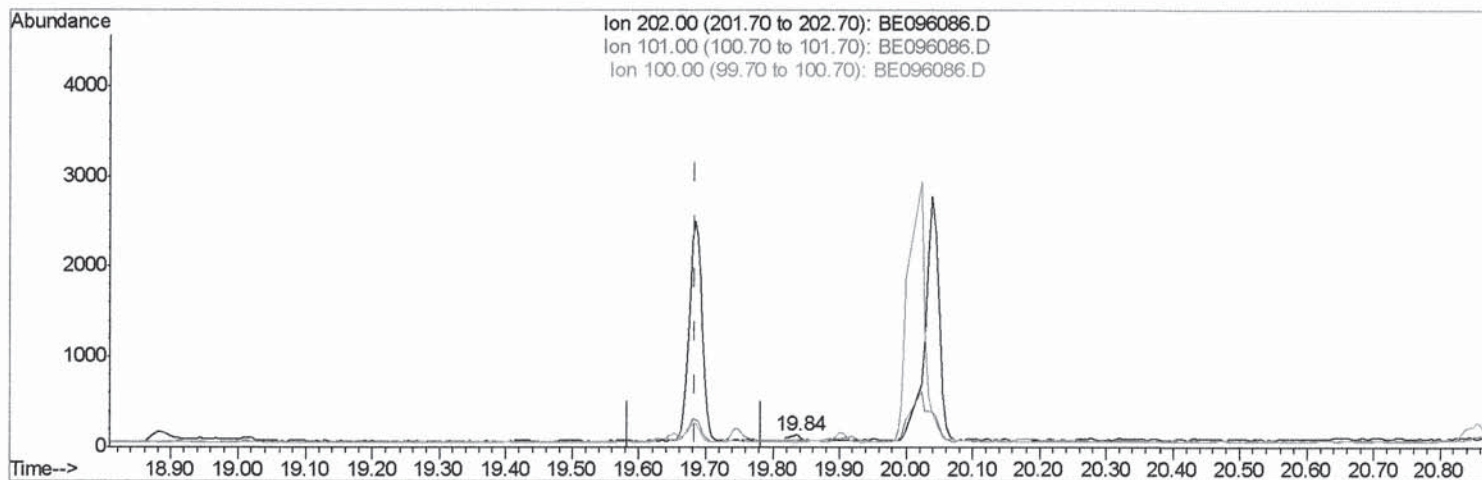

TIC: BE096086.D

(15) Fluoranthene (C)

19.838min (+0.153) 0.00ng/ul

response 70

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	56.92#
100.00	19.50	51.54#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

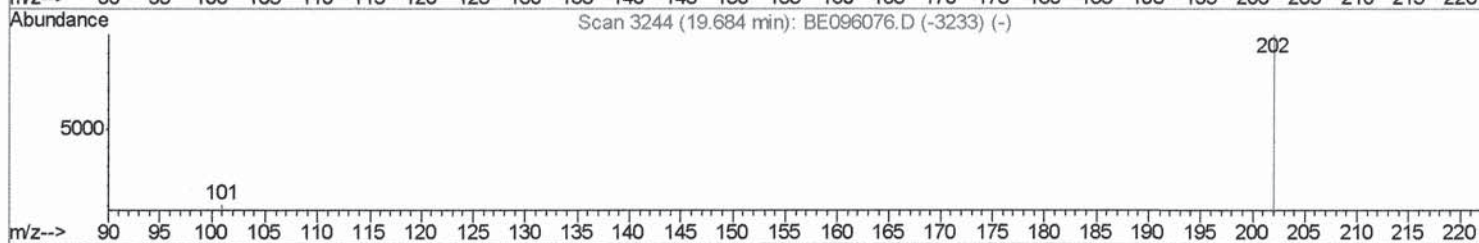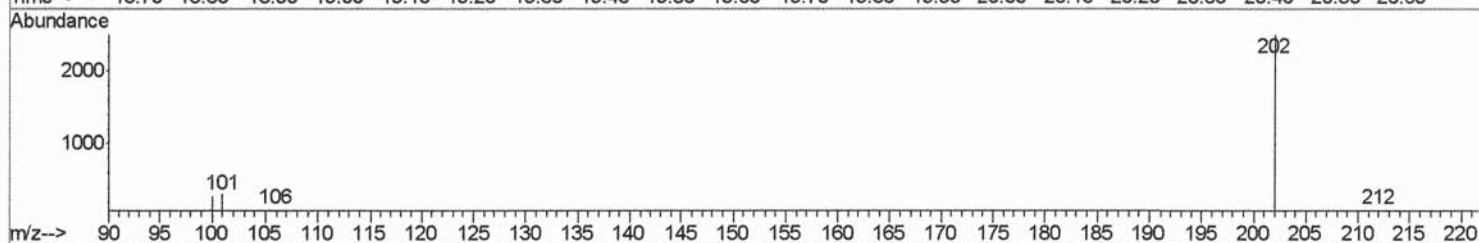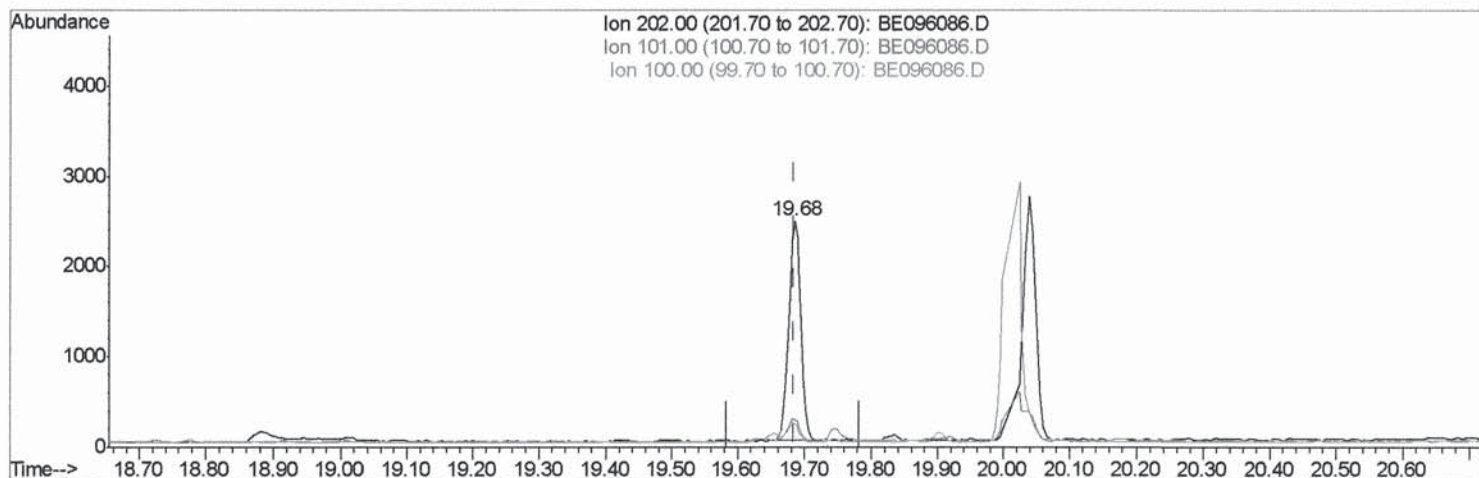

TIC: BE096086.D

(15) Fluoranthene (C)

19.684min (-0.000) 0.12ng/ul m *SS 4/22/18*

response 3225

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.17
100.00	19.50	10.77
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

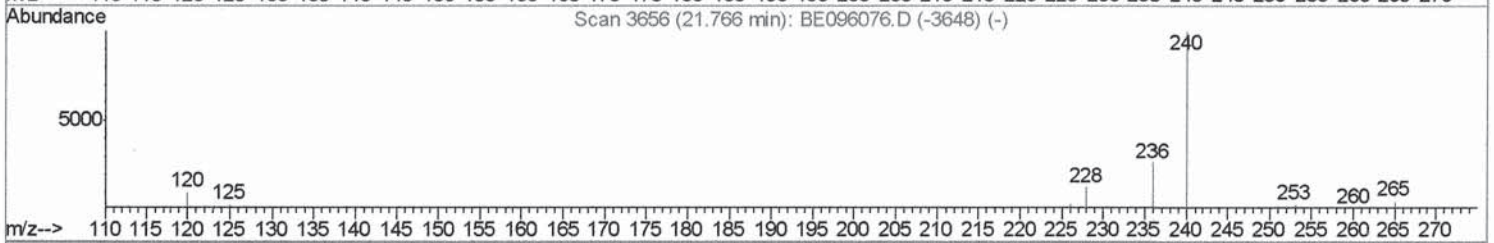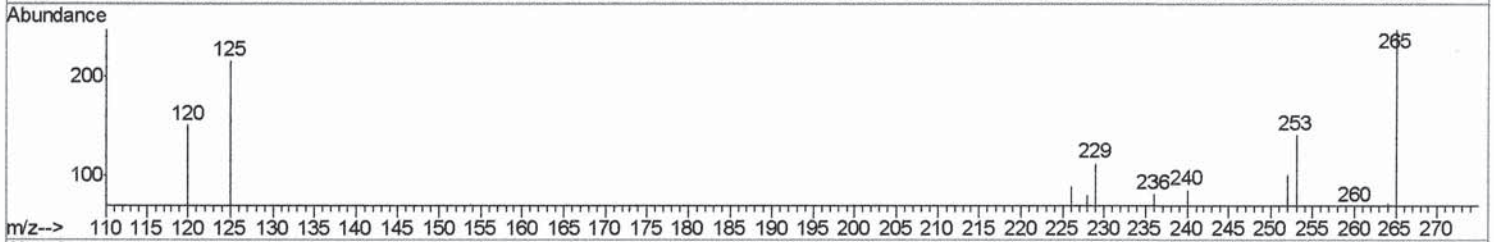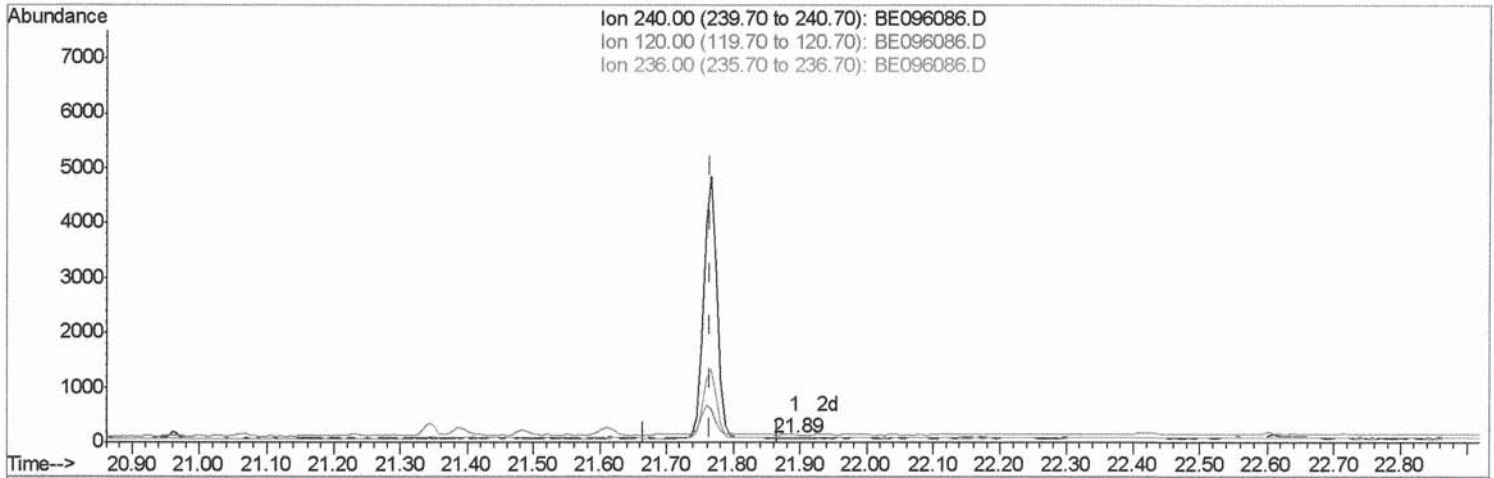

TIC: BE096086.D

(16) Chrysene-d12 (I)

21.893min (+0.127) 0.40ng/ul

response 28

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	175.58#
236.00	34.90	95.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:40:39 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

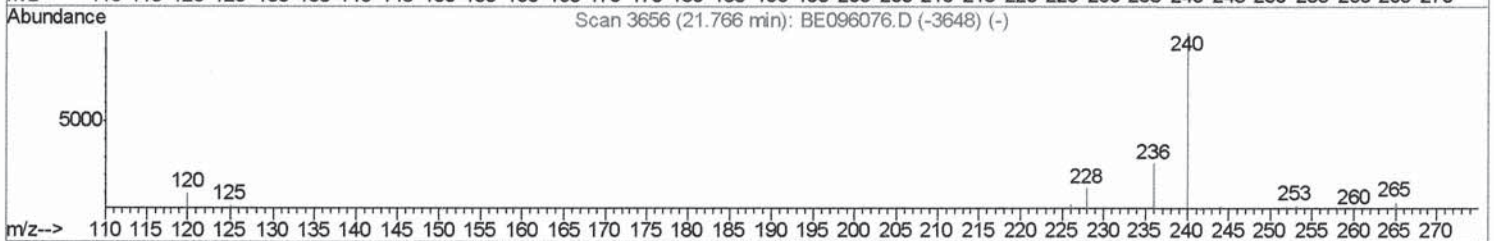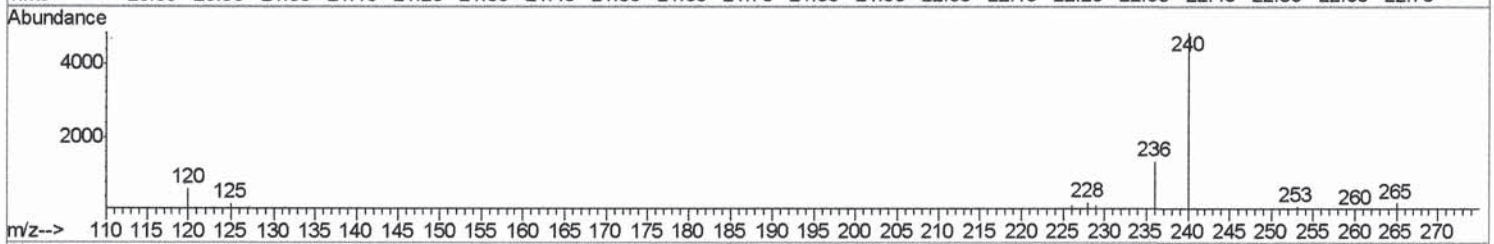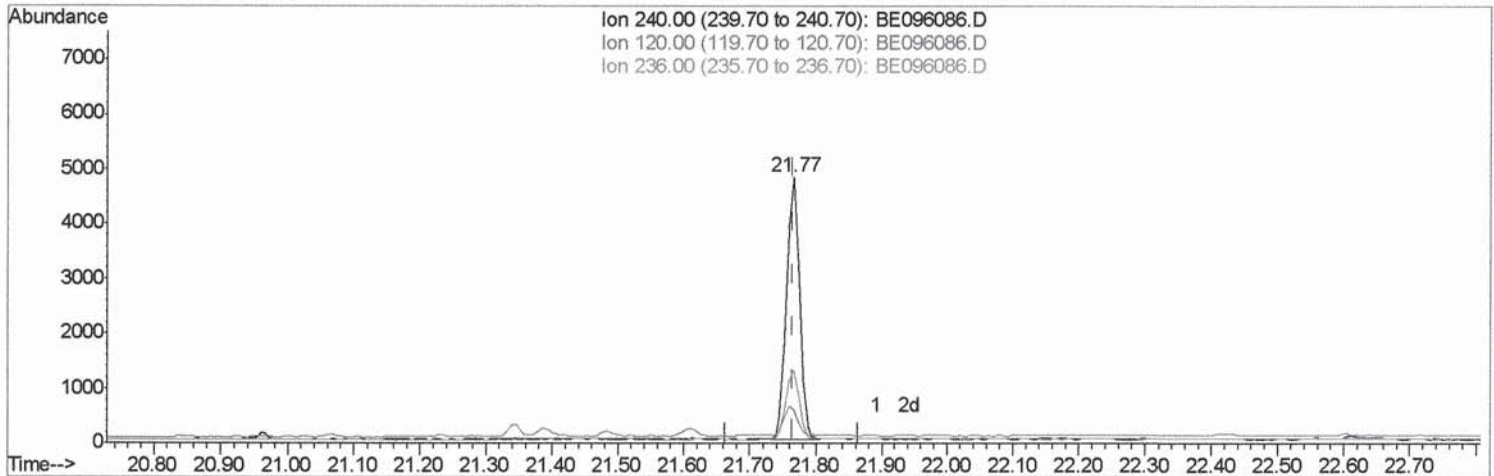

TIC: BE096086.D

(16) Chrysene-d12 (I)

21.766min (+0.000) 0.40ng/ul m > 52 4/24/18

response 6442

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.53#
236.00	34.90	27.87#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

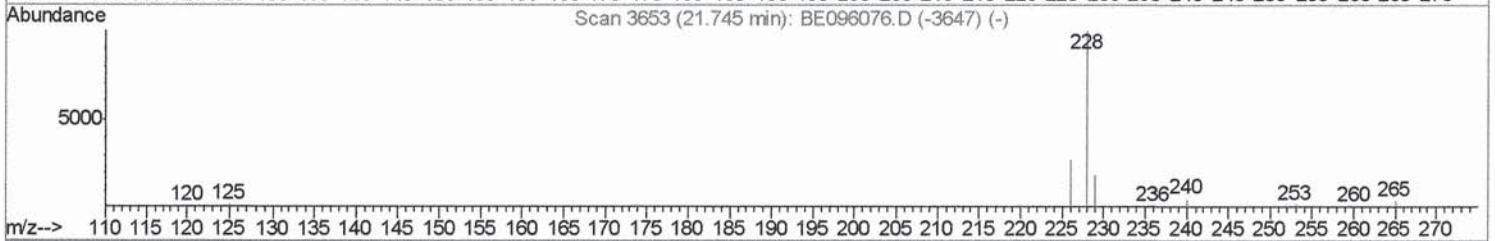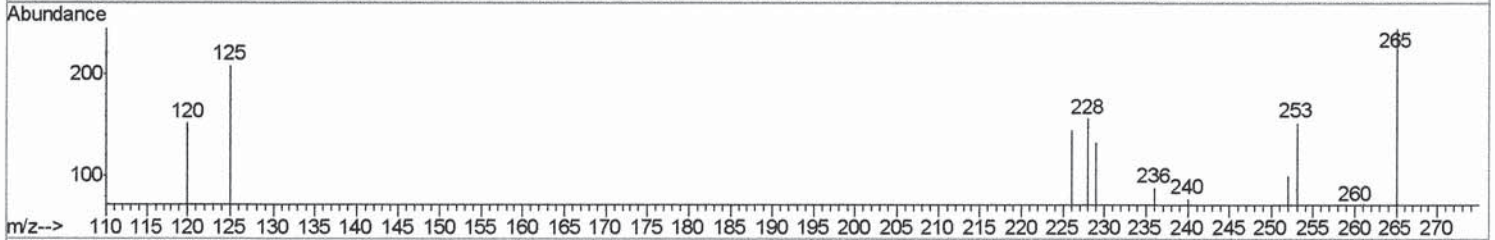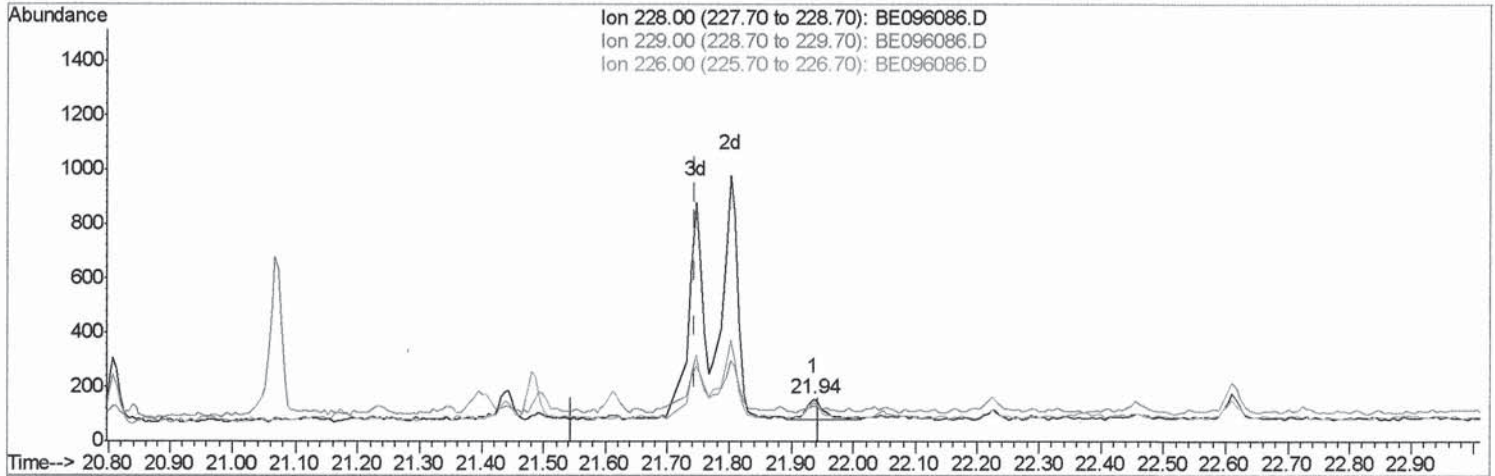

TIC: BE096086.D

(18) Benzo(a)anthracene
 21.935min (+0.190) 0.01ng/ul
 response 157

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	84.71#
226.00	21.30	92.36#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

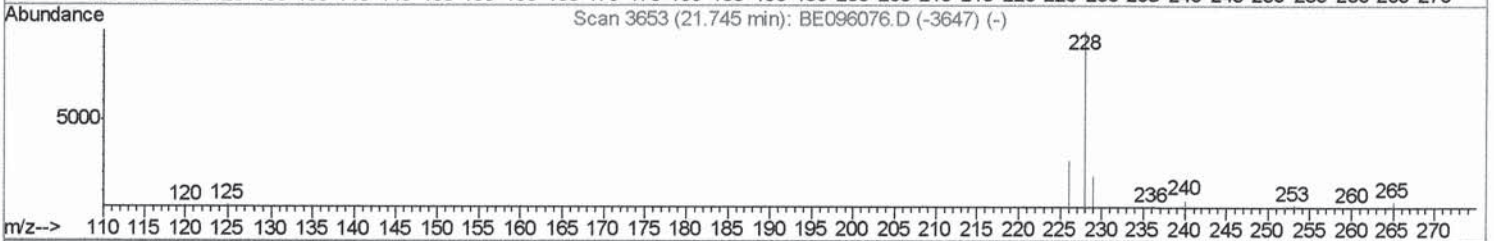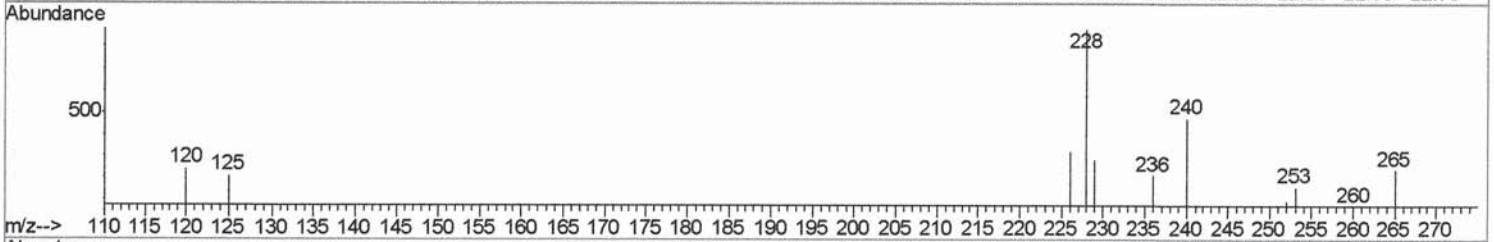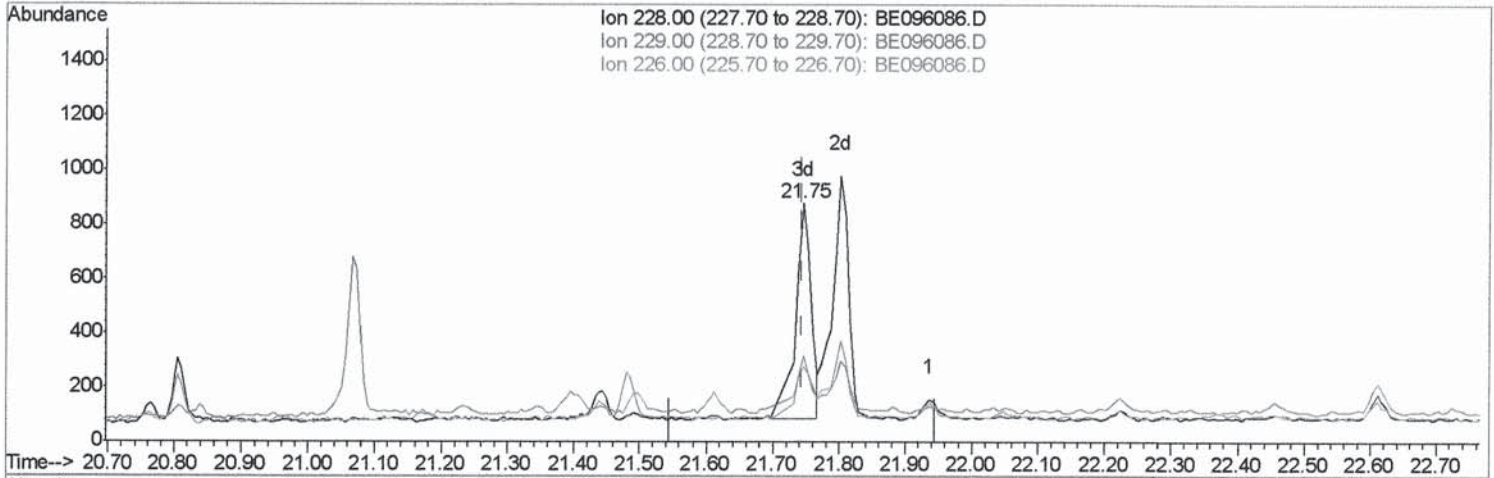

TIC: BE096086.D

(18) Benzo(a)anthracene

21.745min (+0.000) 0.07ng/ul m> SJ 4/27/18

response 1833

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	32.05
226.00	21.30	36.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

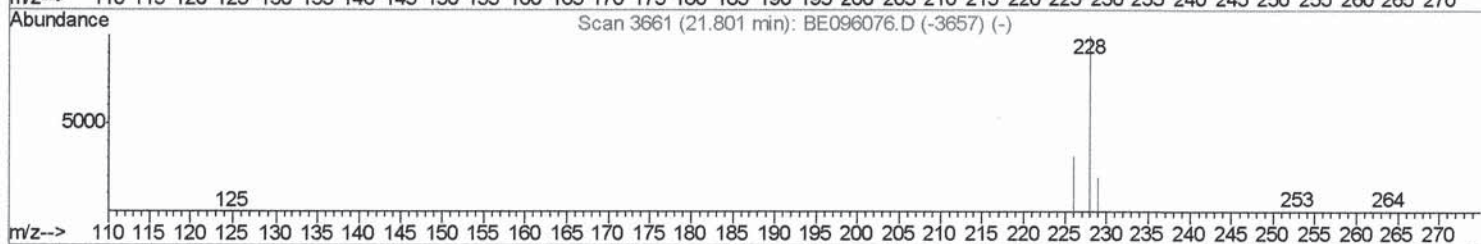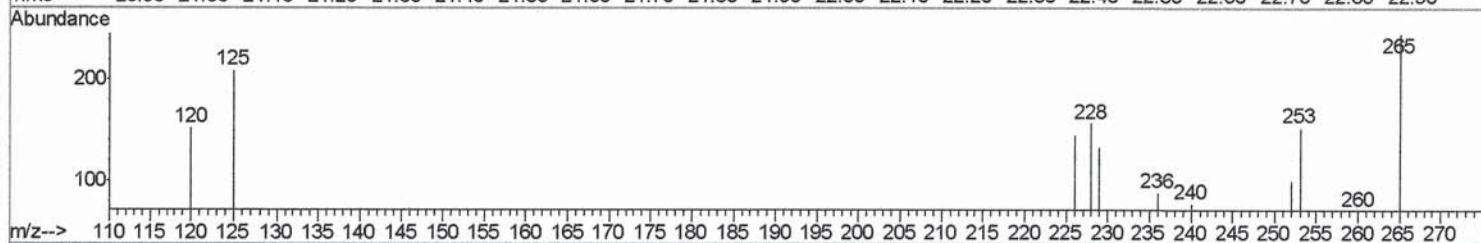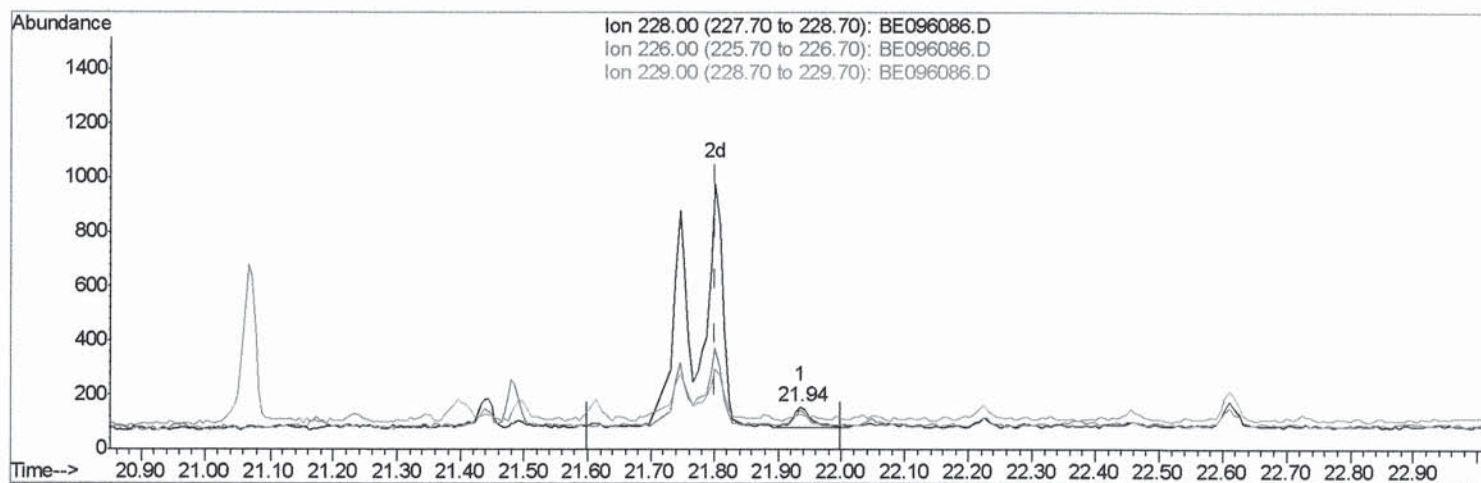

TIC: BE096086.D

(19) Chrysene

21.935min (+0.134) 0.01ng/ul

response 157

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	92.36#
229.00	22.10	84.71#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

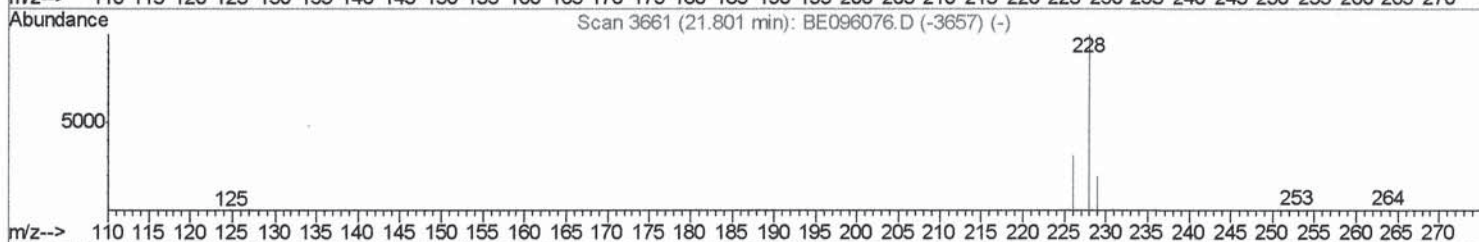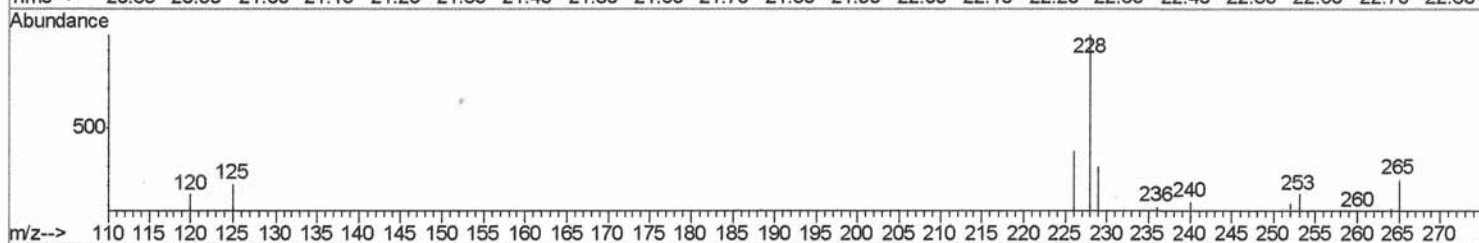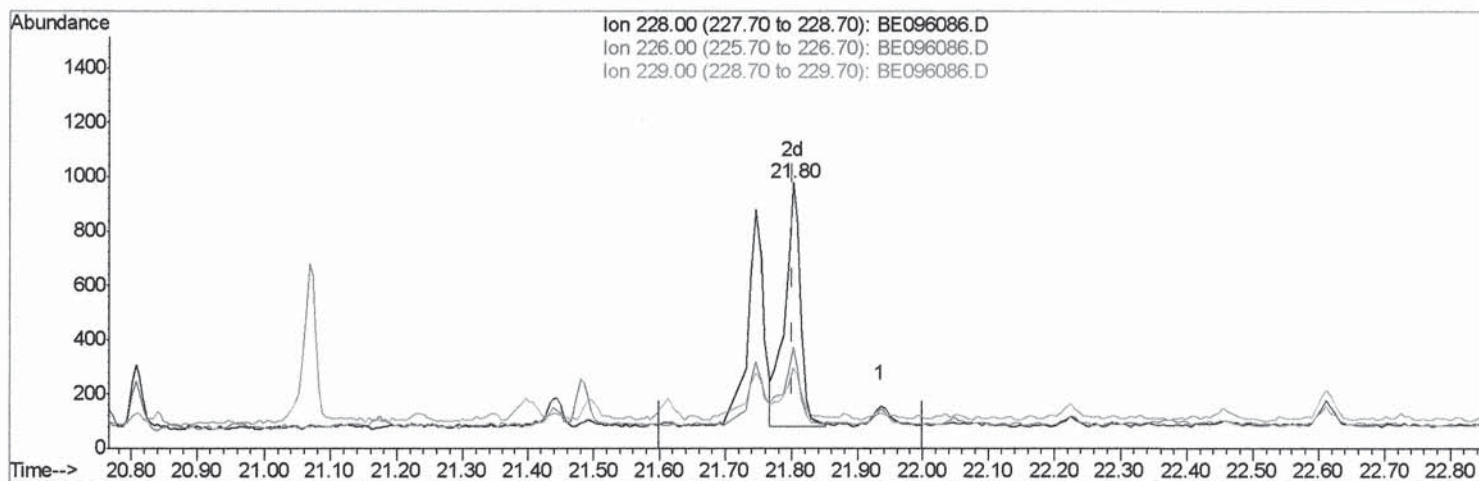

TIC: BE096086.D

(19) Chrysene

21.801min (+0.000) 0.08ng/ul m> 4/22/18

response 1526

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	38.04#
229.00	22.10	30.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

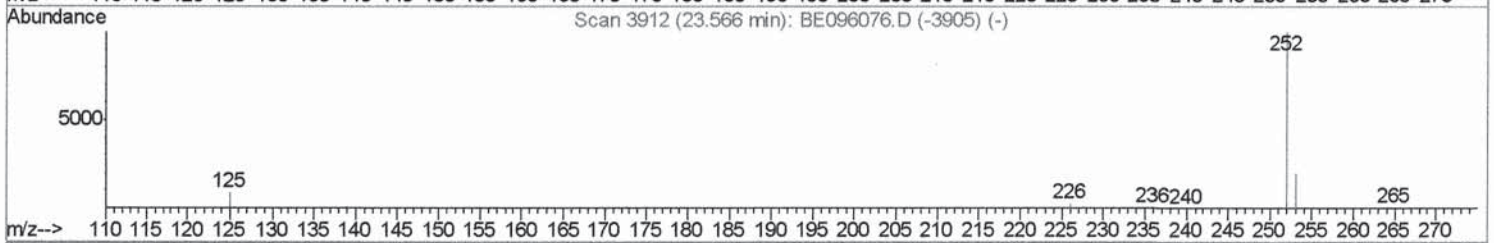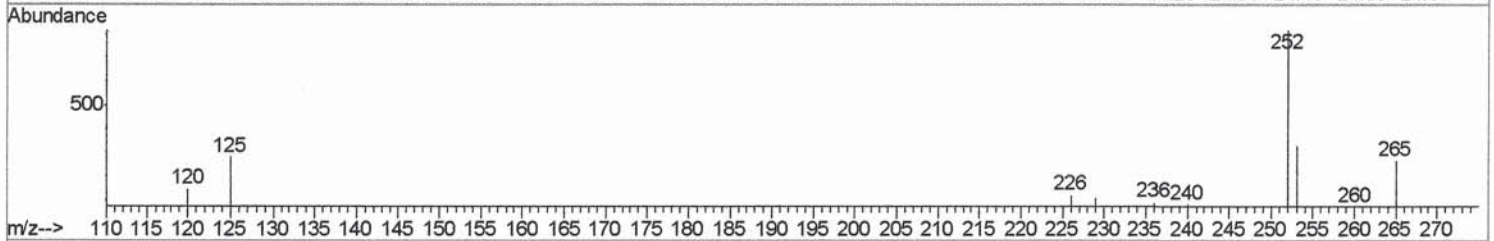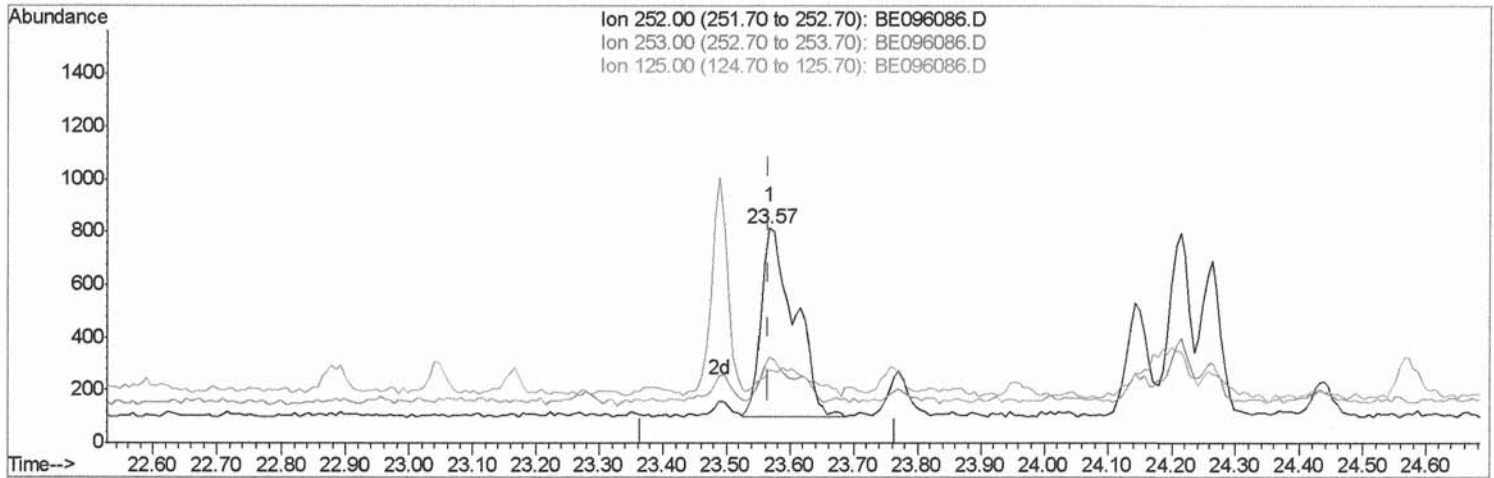

TIC: BE096086.D

(21) Benzo(b)fluoranthene

23.566min (+0.000) 0.11ng/ul

response 2577

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	40.17
125.00	17.50	34.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

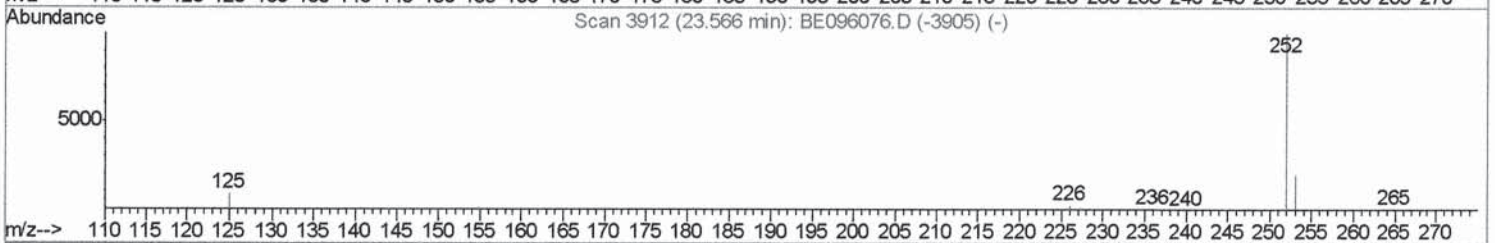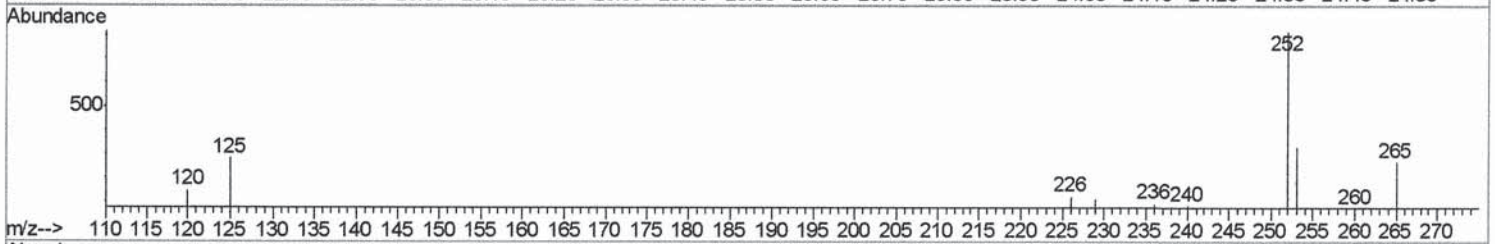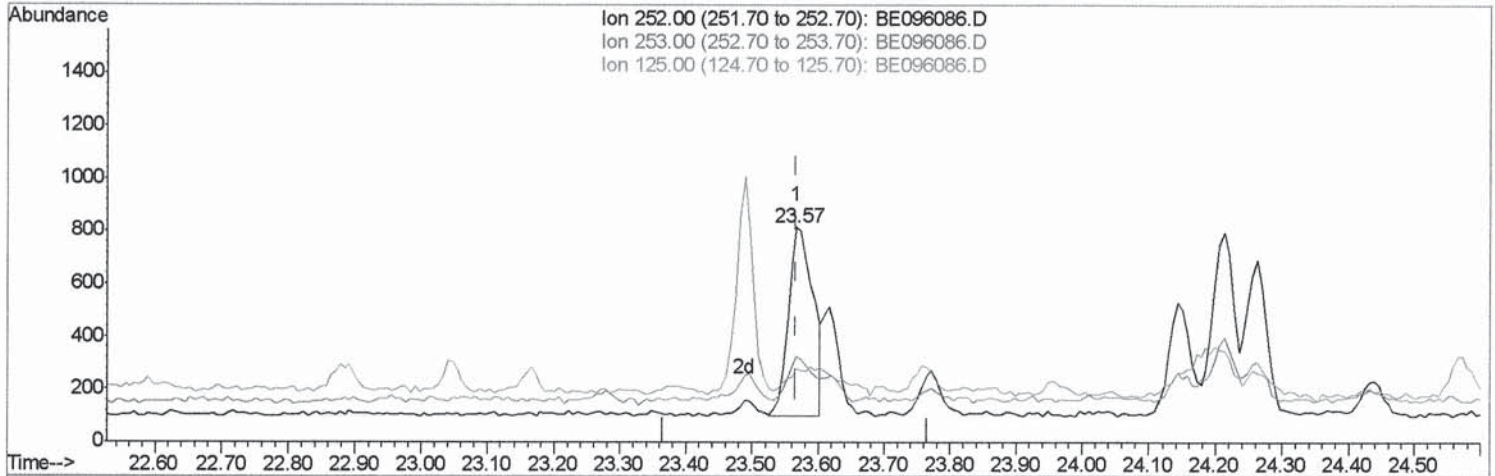

TIC: BE096086.D

(21) Benzo(b)fluoranthene

23.566min (+0.000) 0.08ng/ul m > SJ 4/23/18

response 1896

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	40.17
125.00	17.50	34.52
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

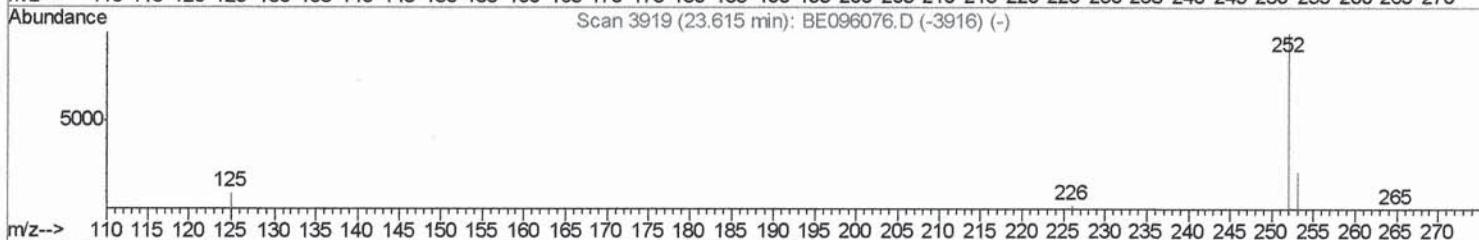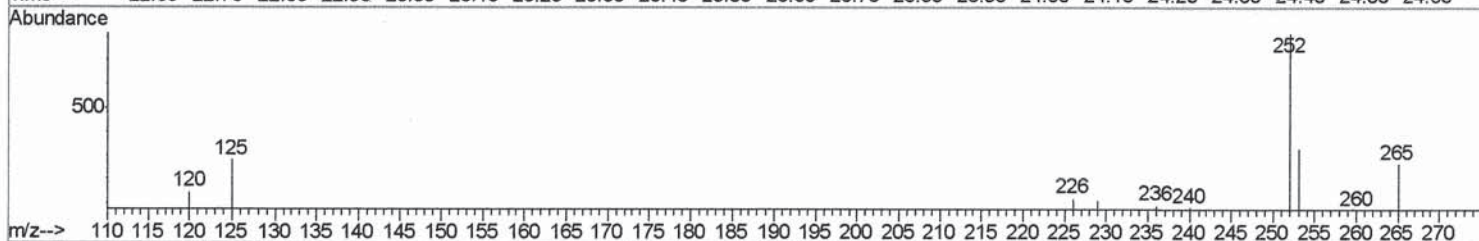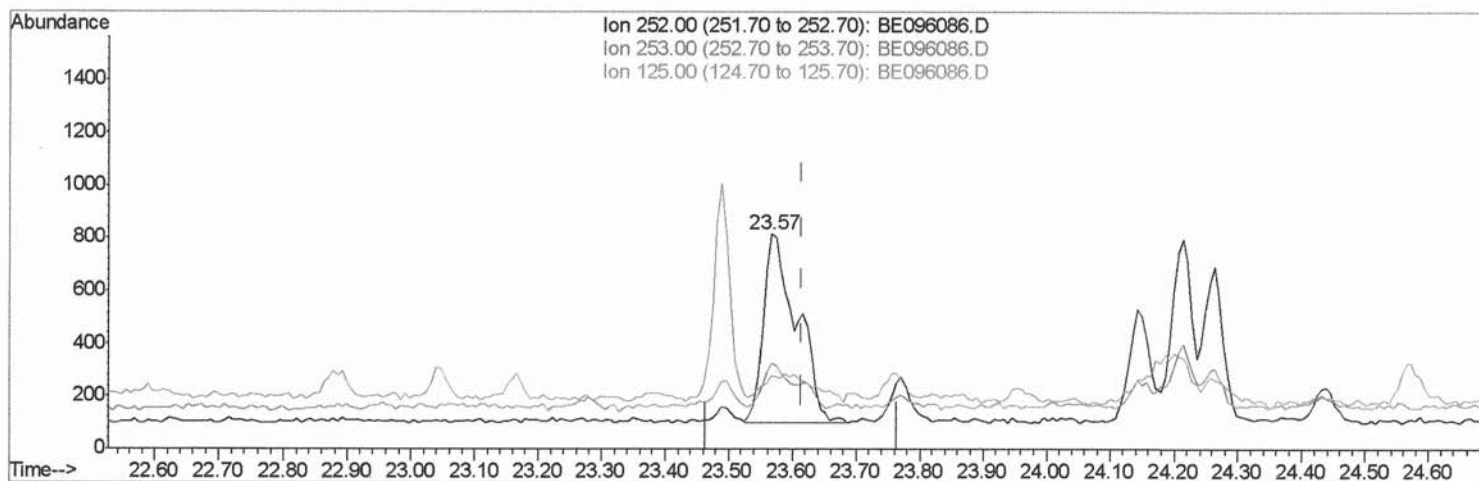

TIC: BE096086.D

(22) Benzo(k)fluoranthene

23.566min (-0.049) 0.11ng/ui

response 2577

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	40.17#
125.00	17.10	34.52#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096086.D
Acq On : 23 Apr 2018 15:47
Operator : SJ/JU
Sample : J2355-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y32

Manual Integrations
APPROVED

Sohil
4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:42:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

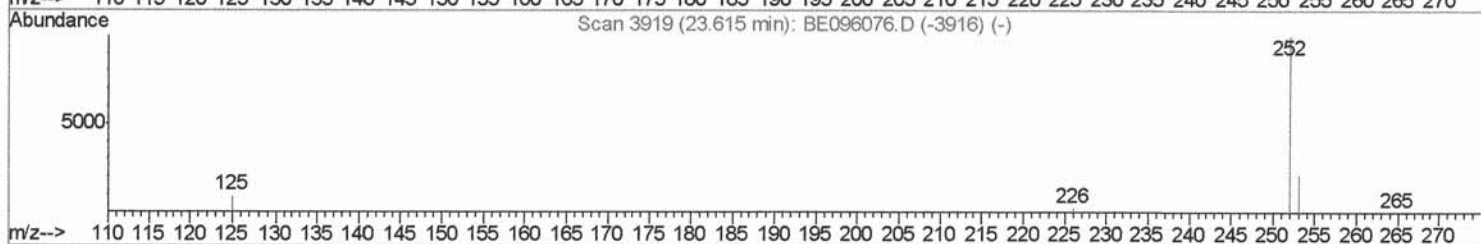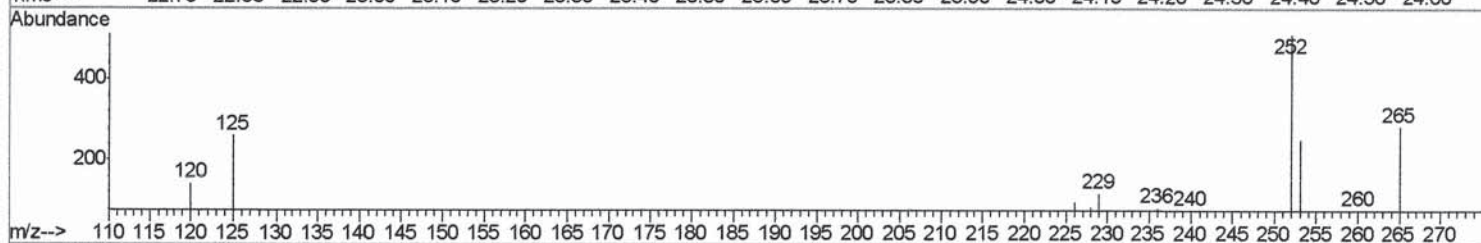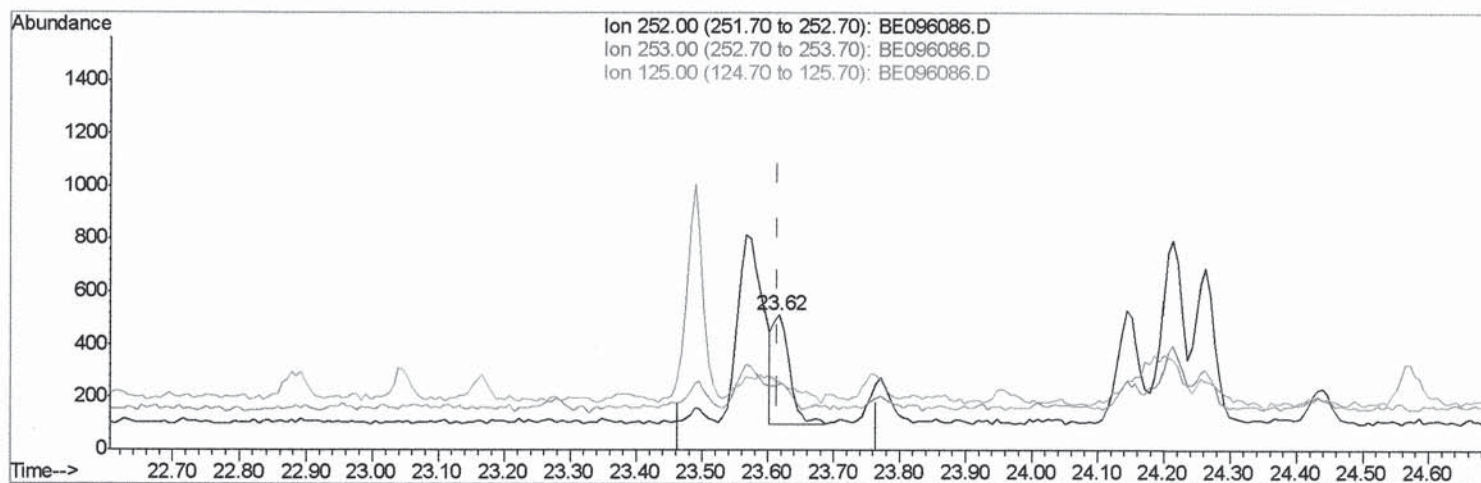

TIC: BE096086.D

(22) Benzo(k)fluoranthene

23.616min (+0.000) 0.03ng/ul m> SJ 4/24/18

response 719

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	49.12#
125.00	17.10	50.88#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096086.D
 Acq On : 23 Apr 2018 15:47
 Operator : SJ/JU
 Sample : J2355-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y32

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:09:57 PM

Quant Time: Apr 24 06:44:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1950	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5282	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3136	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6818m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6442m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	7456	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.76	152	2327	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	6108m	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
8) Acenaphthene	15.02	153	248	0.021	ng/ul#	86
12) Phenanthrene	17.71	178	1235m	0.061	ng/ul	
15) Fluoranthene	19.68	202	3225m	0.118	ng/ul	
17) Pyrene	20.04	202	3802	0.174	ng/ul#	86
18) Benzo(a)anthracene	21.75	228	1833m	0.070	ng/ul	
19) Chrysene	21.80	228	1526m	0.081	ng/ul	
21) Benzo(b)fluoranthene	23.57	252	1896m	0.079	ng/ul	
22) Benzo(k)fluoranthene	23.62	252	719m	0.030	ng/ul	
23) Benzo(a)pyrene	24.26	252	1210	0.052	ng/ul#	78
24) Indeno(1,2,3-cd)pyrene	27.17	276	893	0.035	ng/ul#	78
26) Benzo(a,h,i)perylene	28.04	276	676	0.031	ng/ul#	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed