


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096088.D
Acq On : 23 Apr 2018 17:01
Operator : SJ/JU
Sample : J2355-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y30

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:53:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

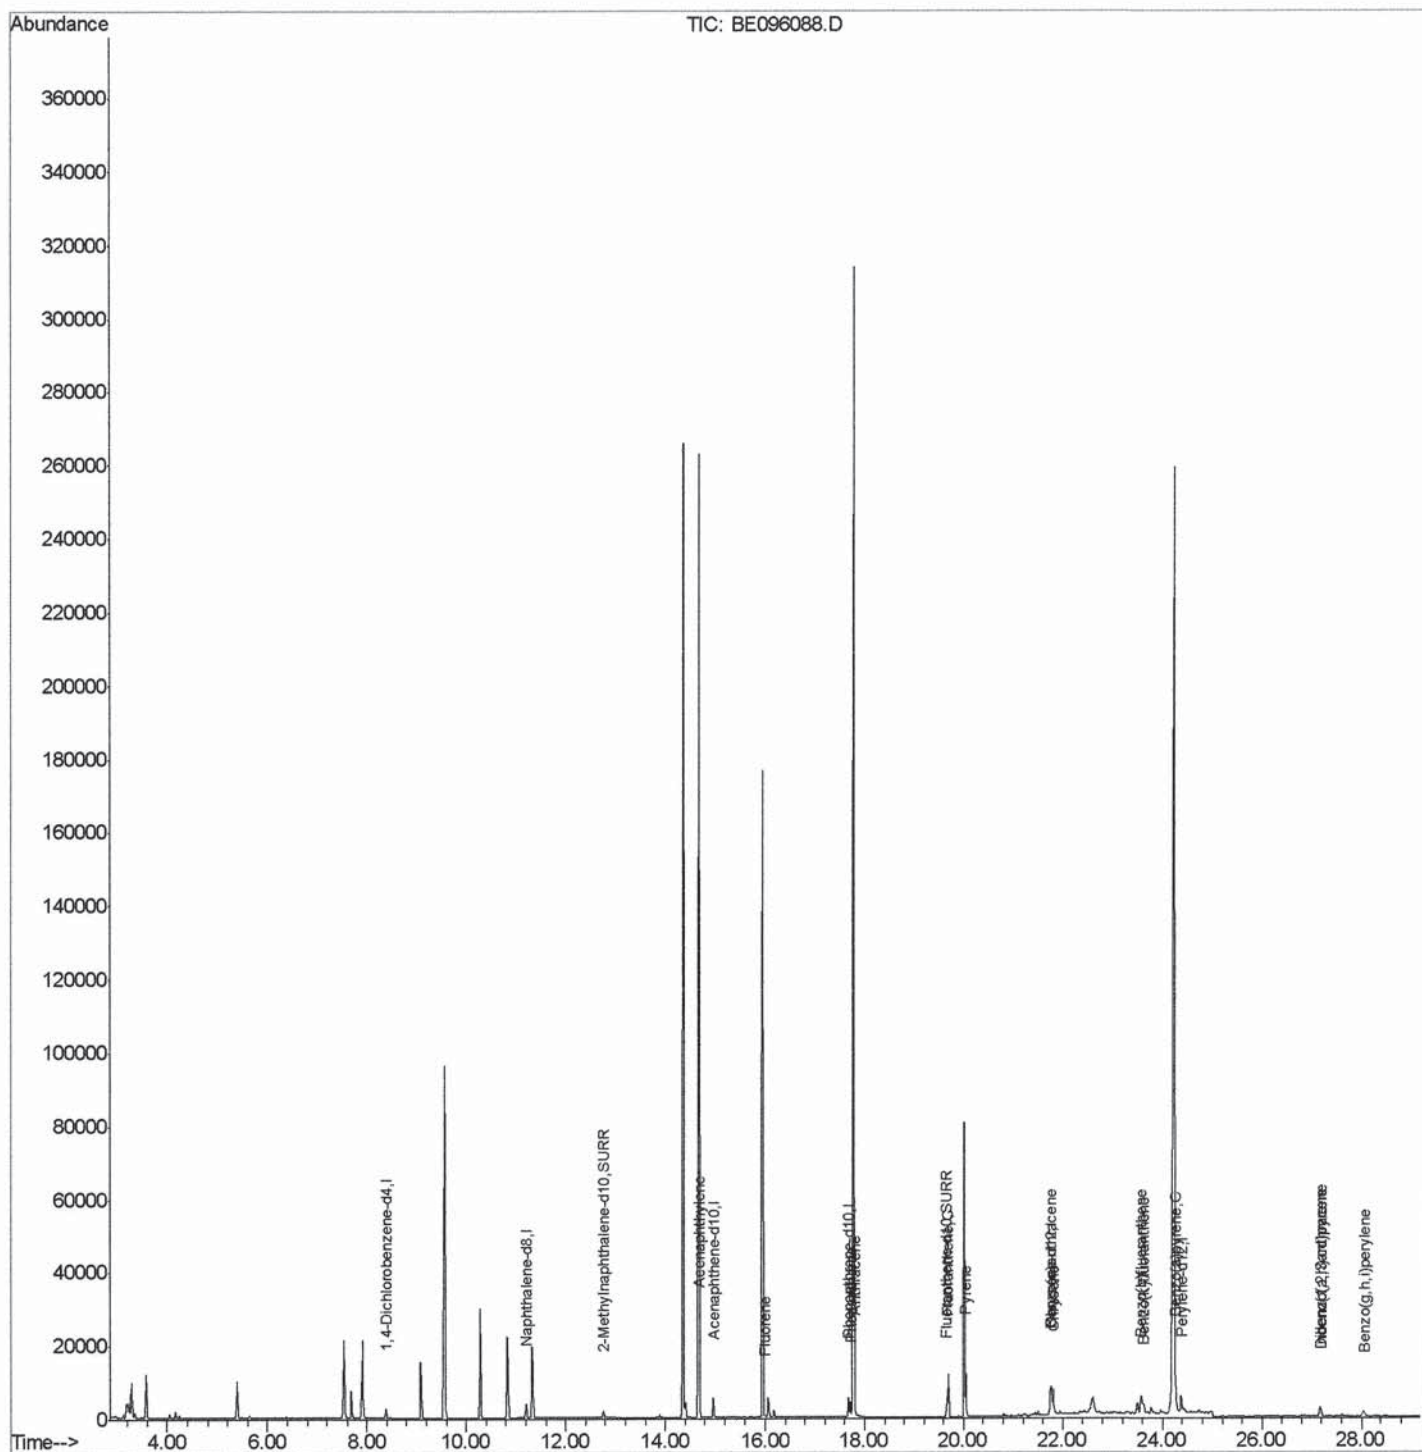

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 05:23:35 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

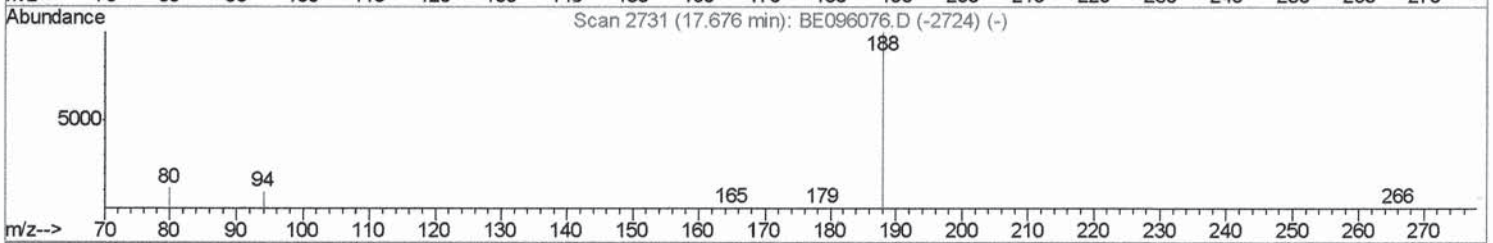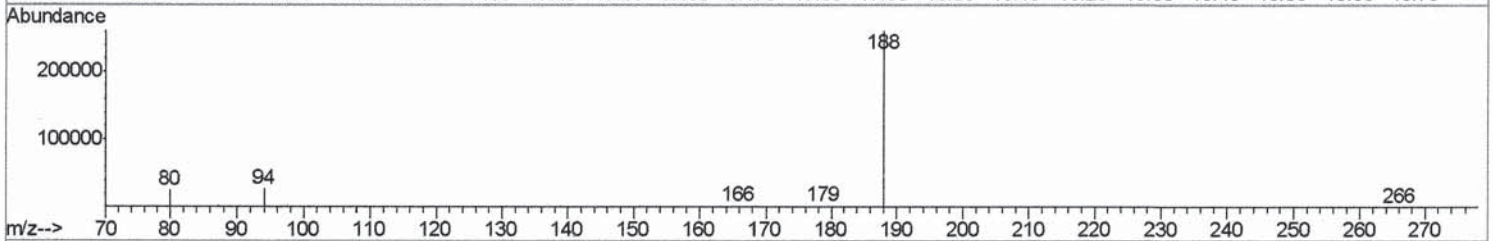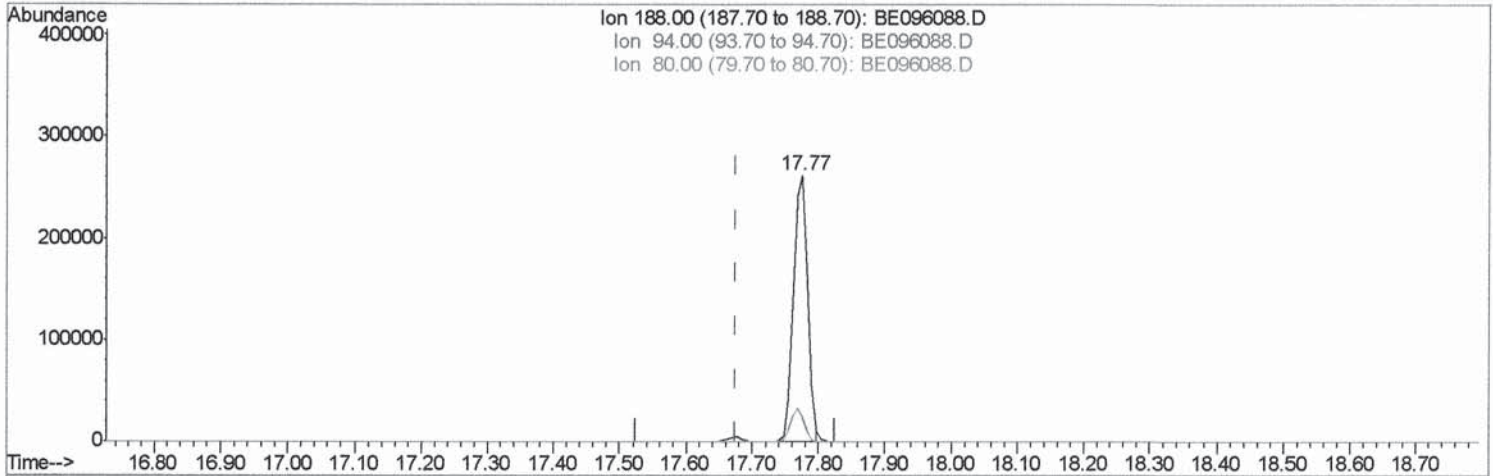

TIC: BE096088.D

(10) Phenanthrene-d10 (I)

17.775min (+0.099) 0.40ng/ul

response 383424

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.16
80.00	11.80	9.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 05:23:35 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

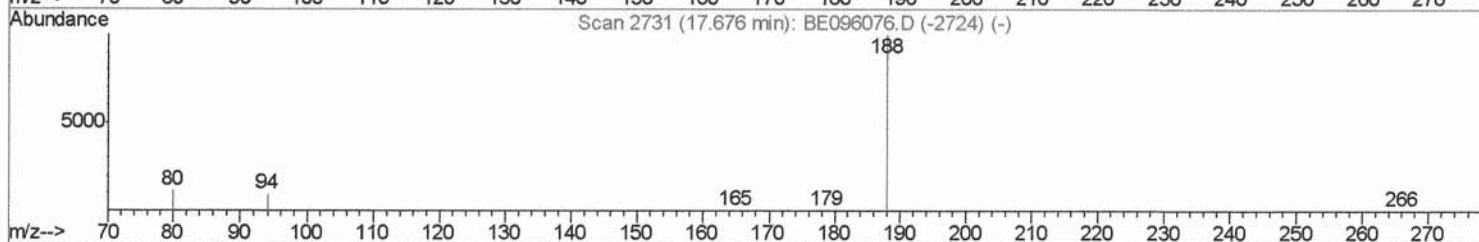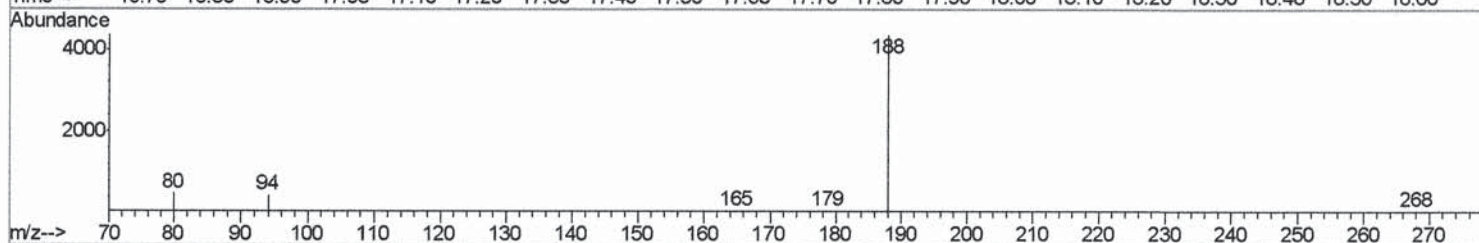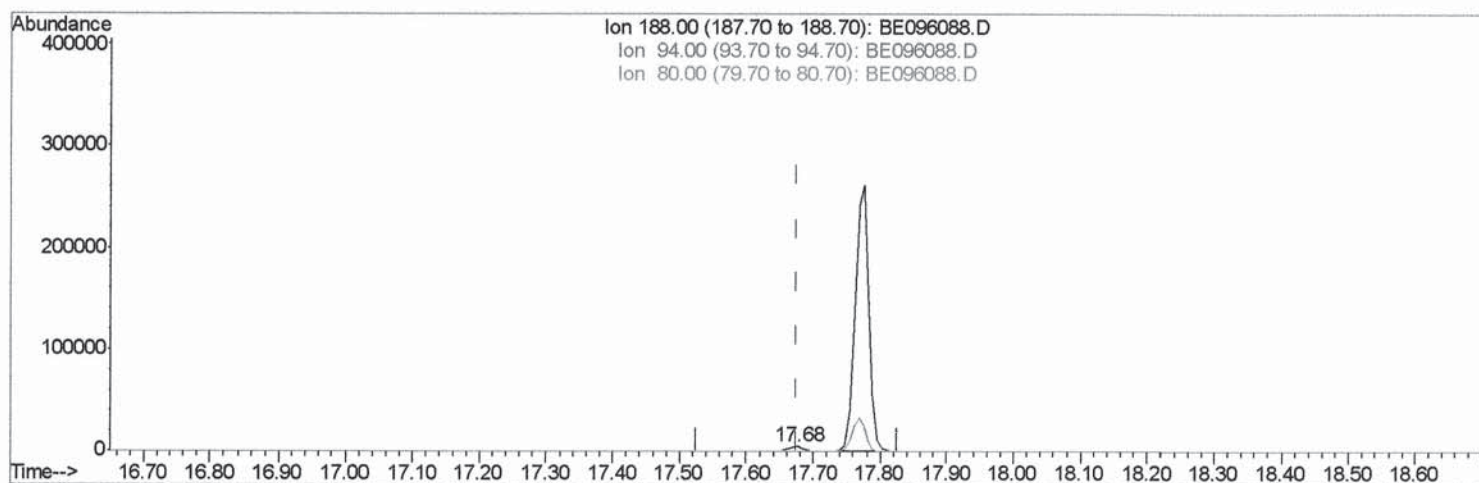

TIC: BE096088.D

(10) Phenanthrene-d10 (I)

17.676min (0.000) 0.40ng/ul m> S2 4/27/18

response 6491

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.01
80.00	11.80	11.13
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:07 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

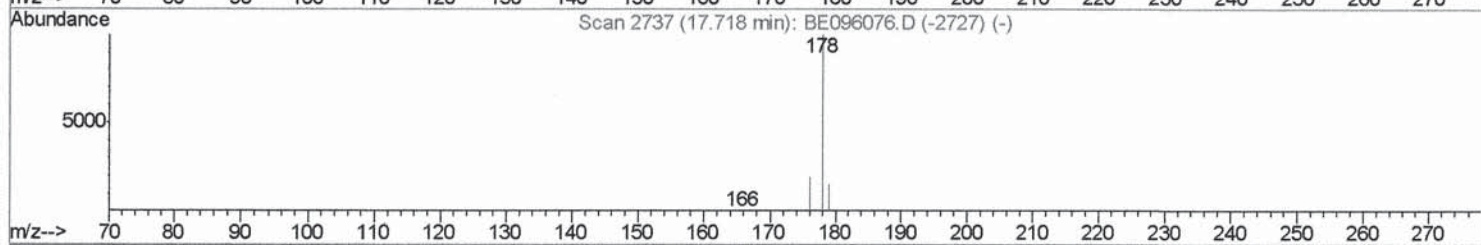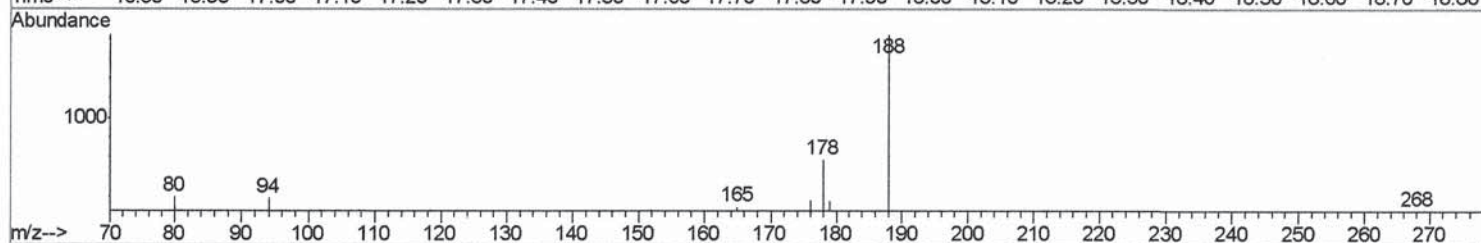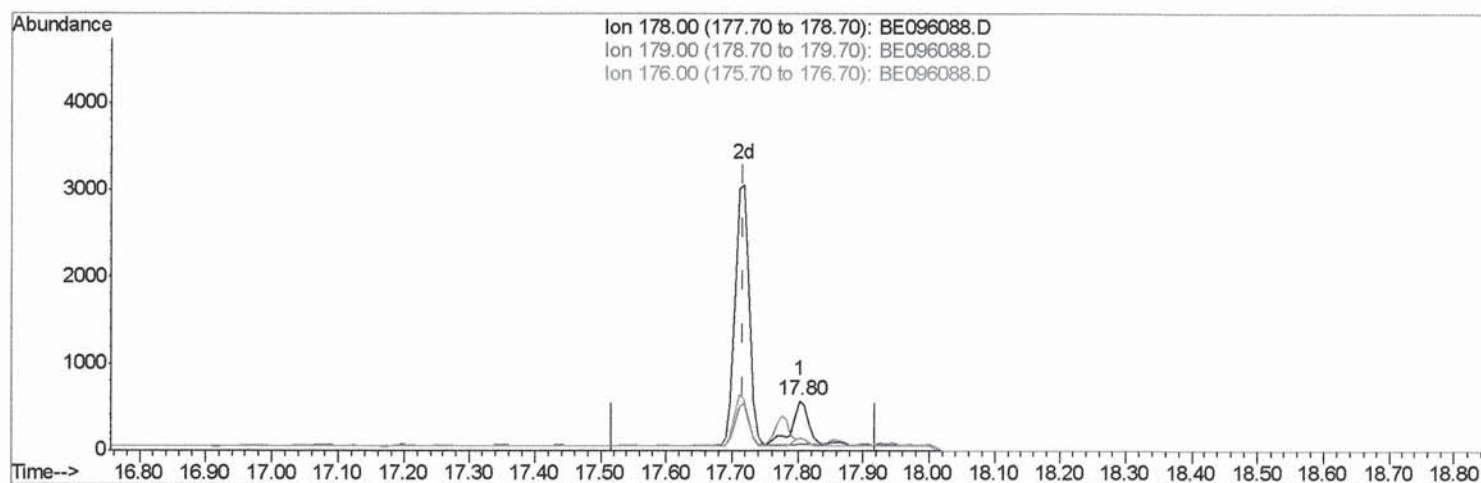

TIC: BE096088.D

(12) Phenanthrene

17.803min (+0.084) 0.04ng/ul

response 848

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.52
176.00	17.00	26.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096088.D
Acq On : 23 Apr 2018 17:01
Operator : SJ/JU
Sample : J2355-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y30

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

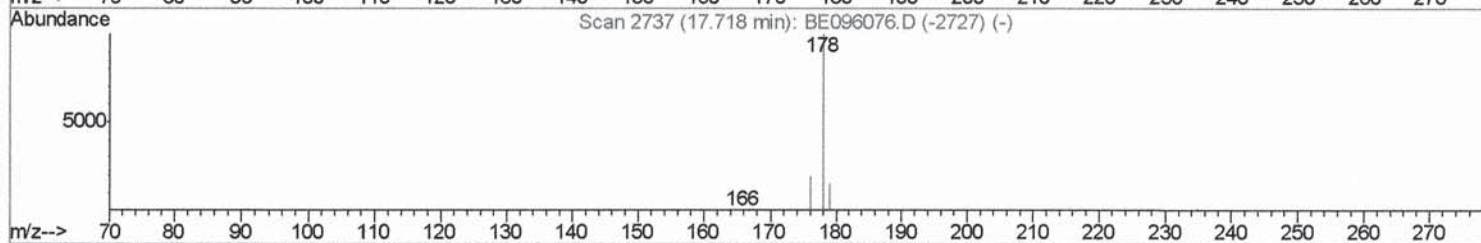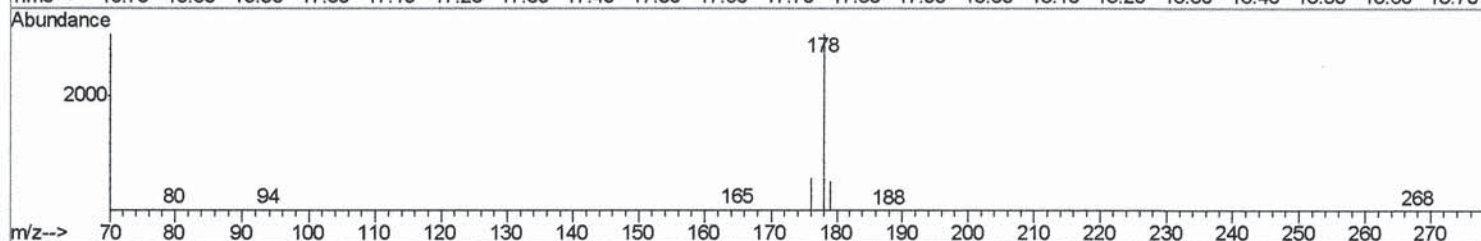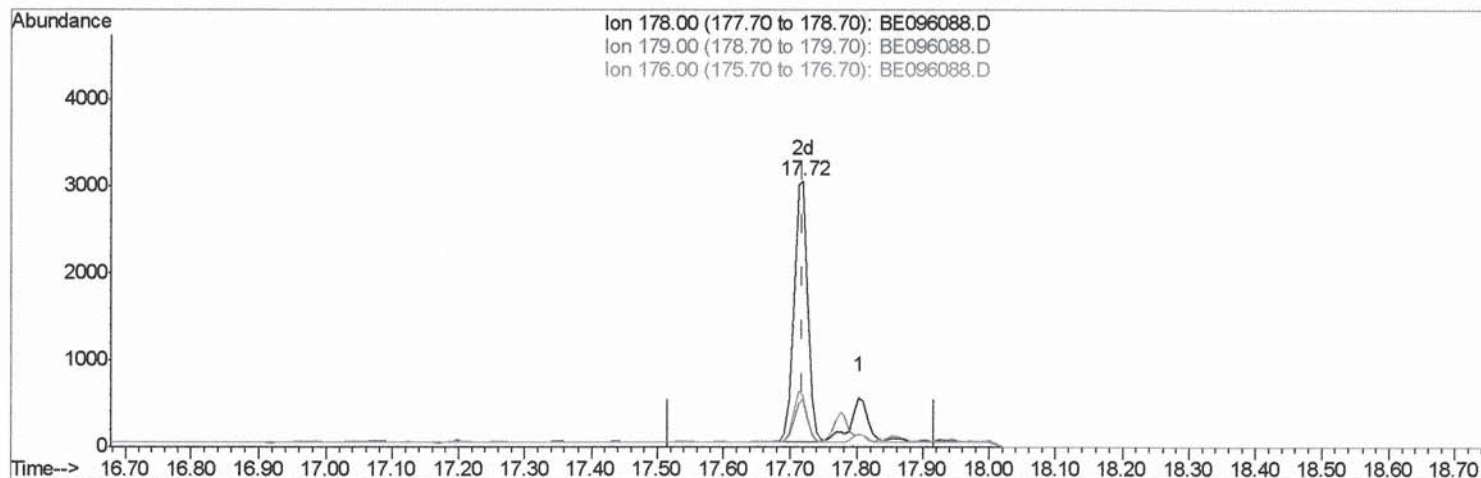

TIC: BE096088.D

(12) Phenanthrene

17.718min (0.000) 0.23ng/ul m > SJ 4/27/18

response 4415

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	17.97#
176.00	17.00	19.64
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

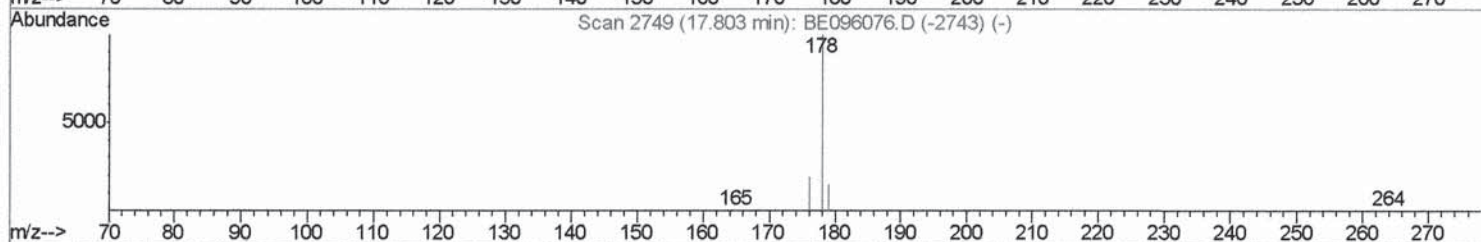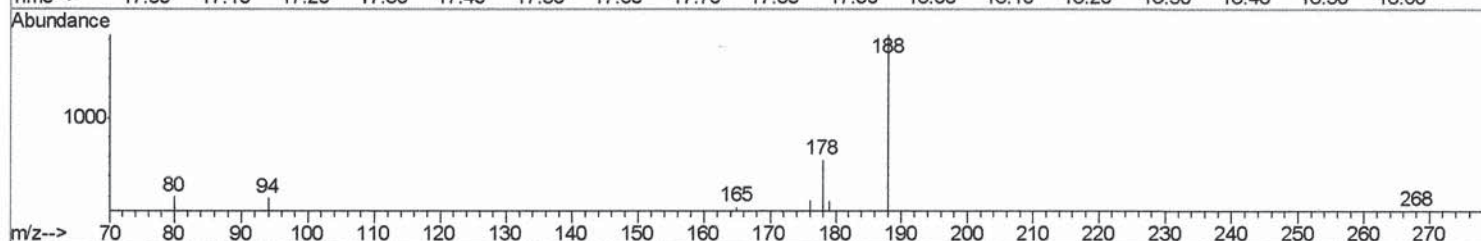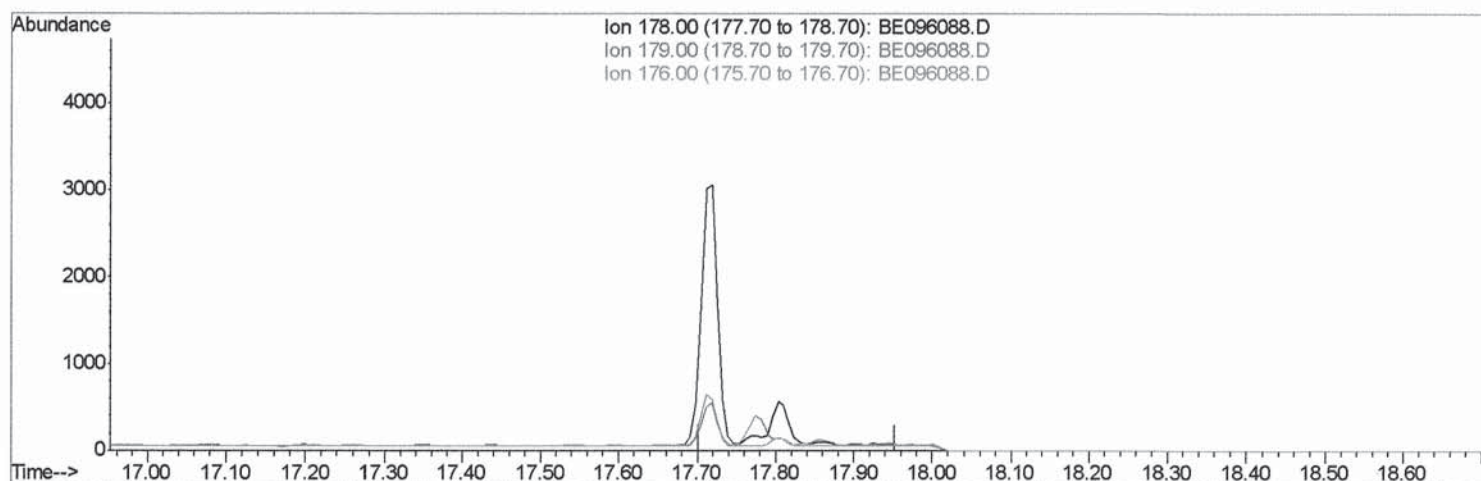

TIC: BE096088.D

(13) Anthracene

17.803min (-17.803) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	22.60	0.00#
176.00	18.40	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096088.D
Acq On : 23 Apr 2018 17:01
Operator : SJ/JU
Sample : J2355-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y30

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

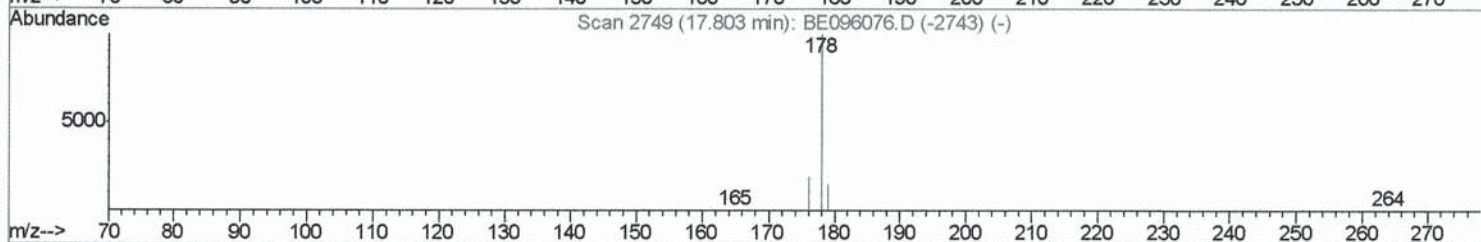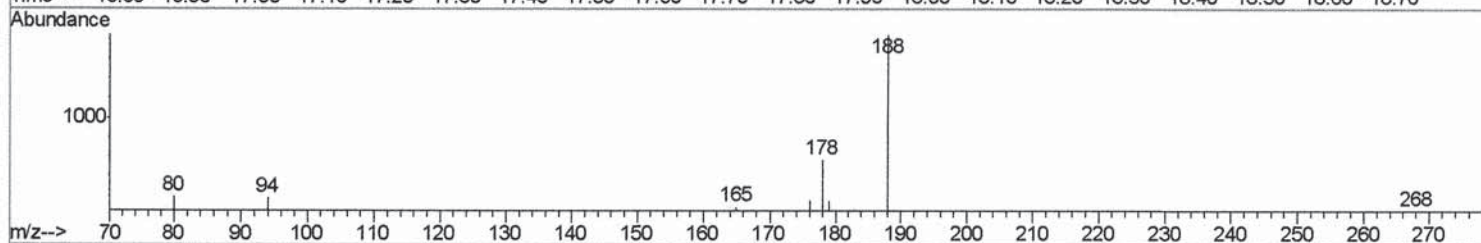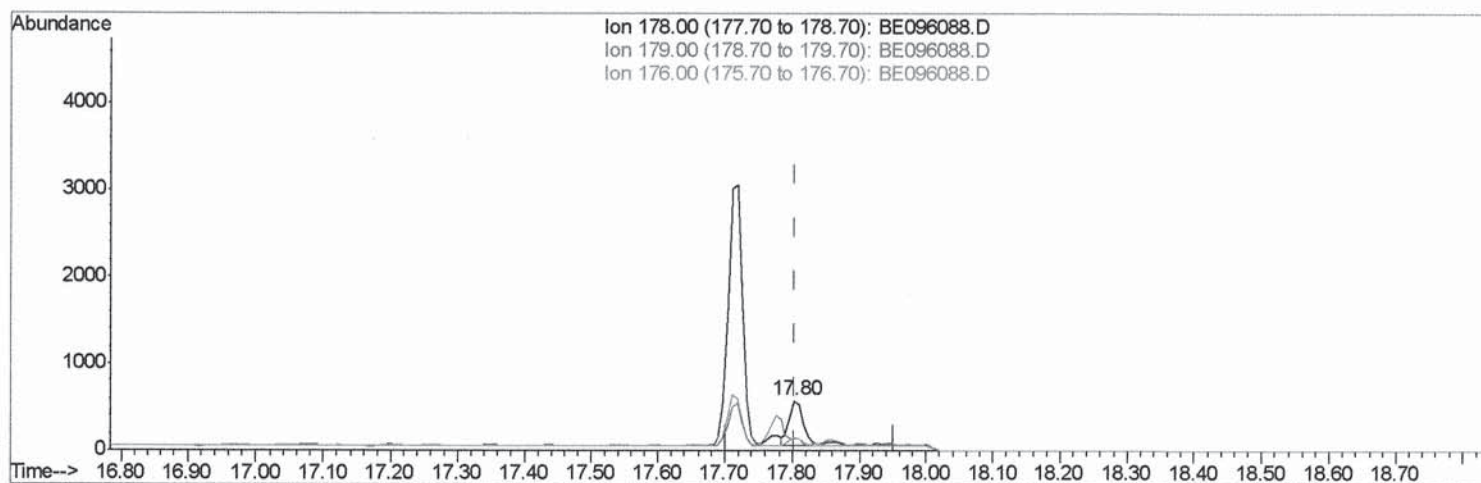

TIC: BE096088.D

(13) Anthracene

17.803min (0.000) 0.04ng/ul m > SJ 4/24/18

response 749

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	24.52
176.00	18.40	26.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

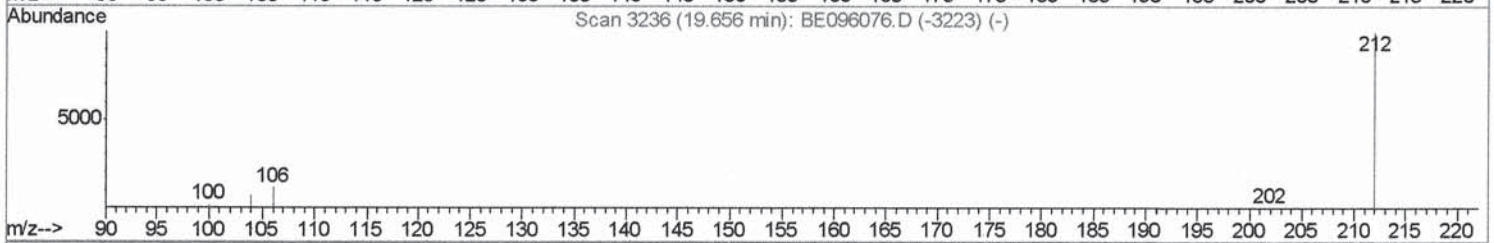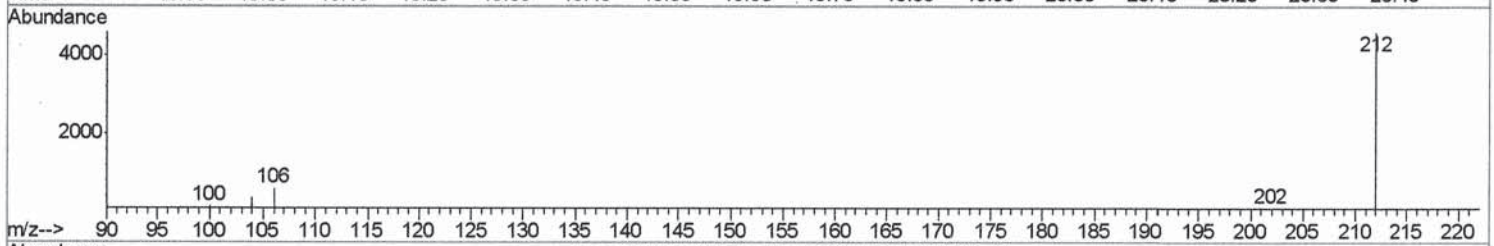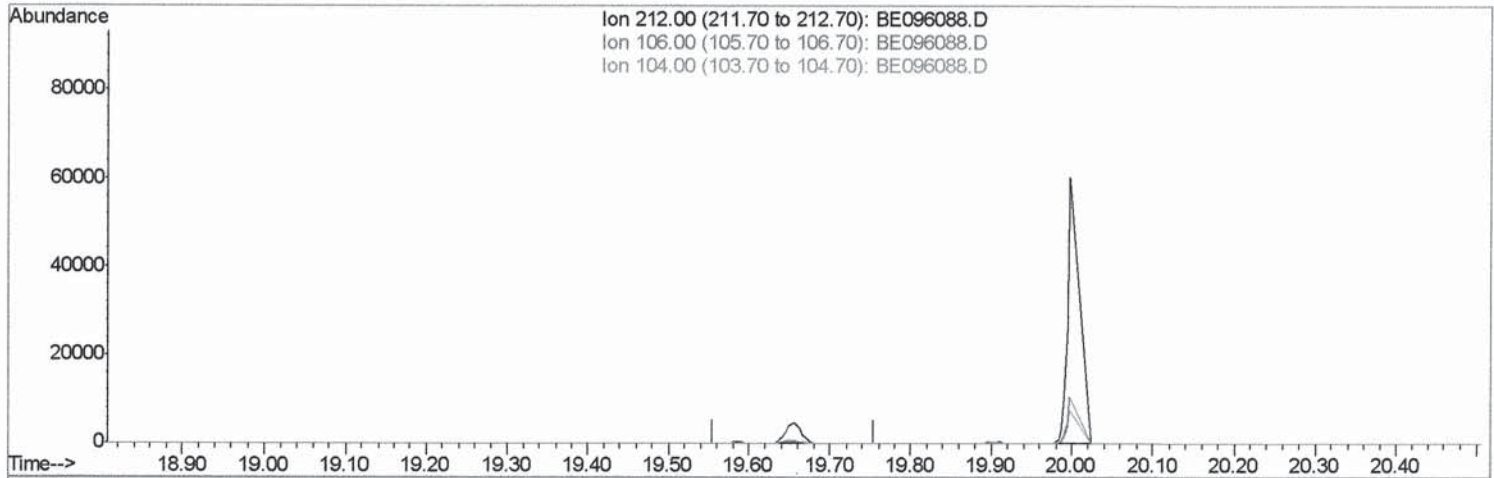

TIC: BE096088.D

(14) Fluoranthene-d10 (SURR)

19.656min (-19.656) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

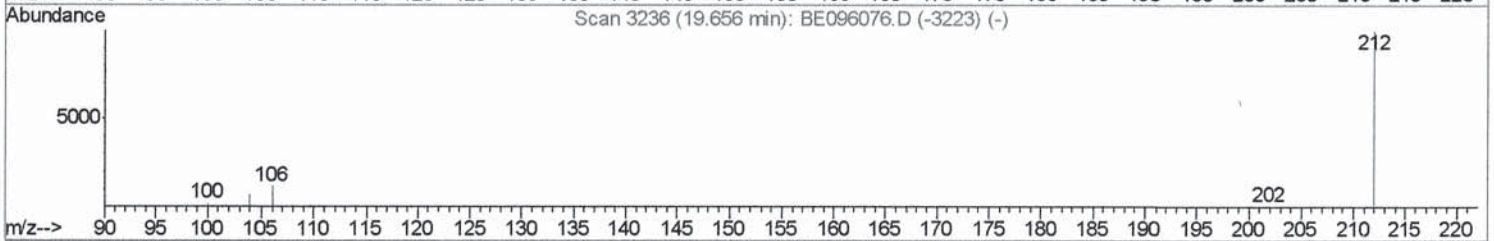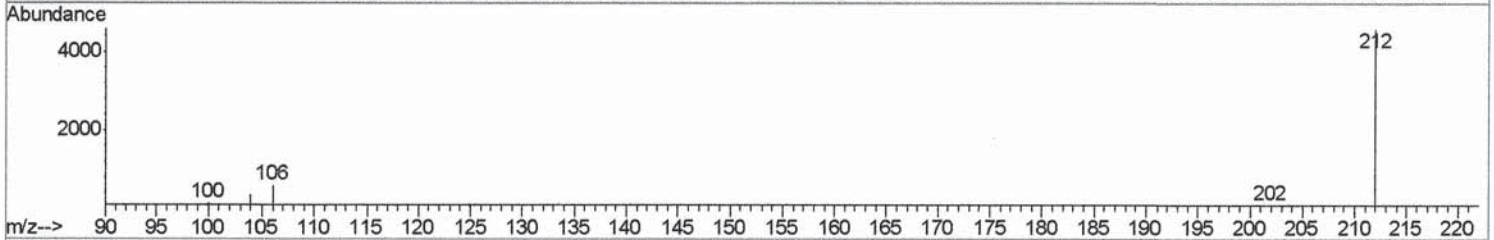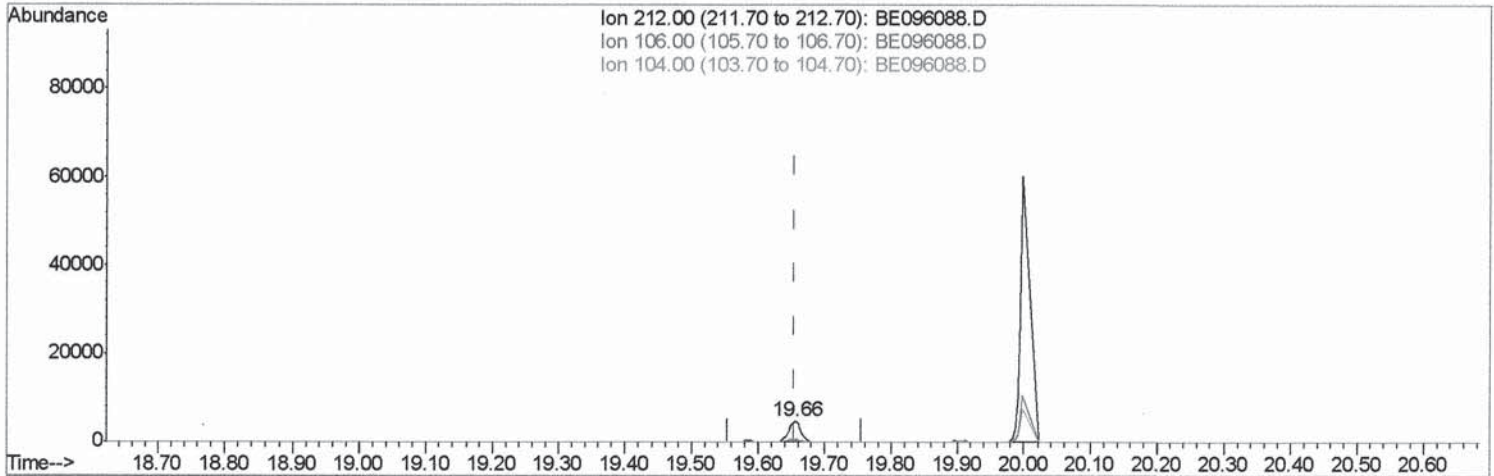

TIC: BE096088.D

(14) Fluoranthene-d10 (SURR)

19.655min (-0.001) 0.23ng/ul m > SJ 4/24/18

response 6147

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

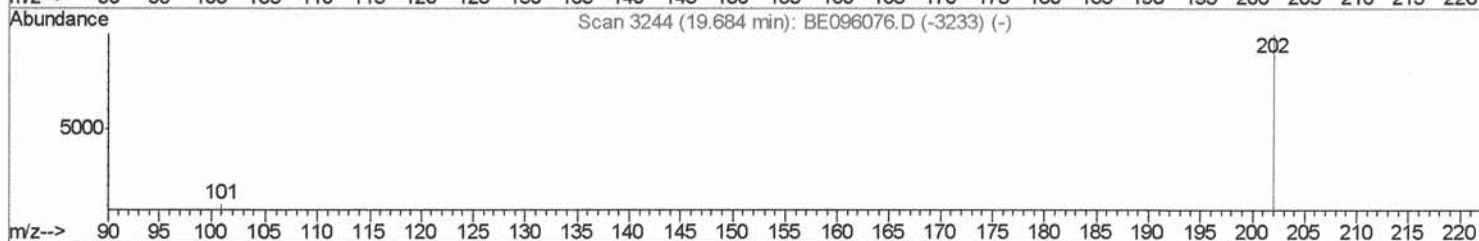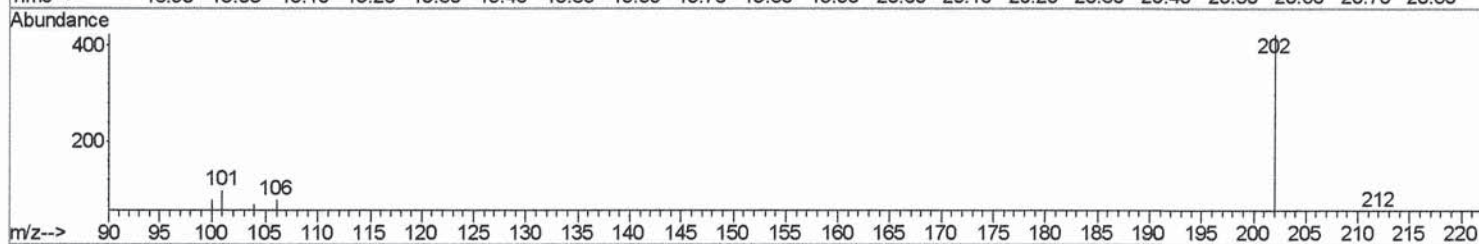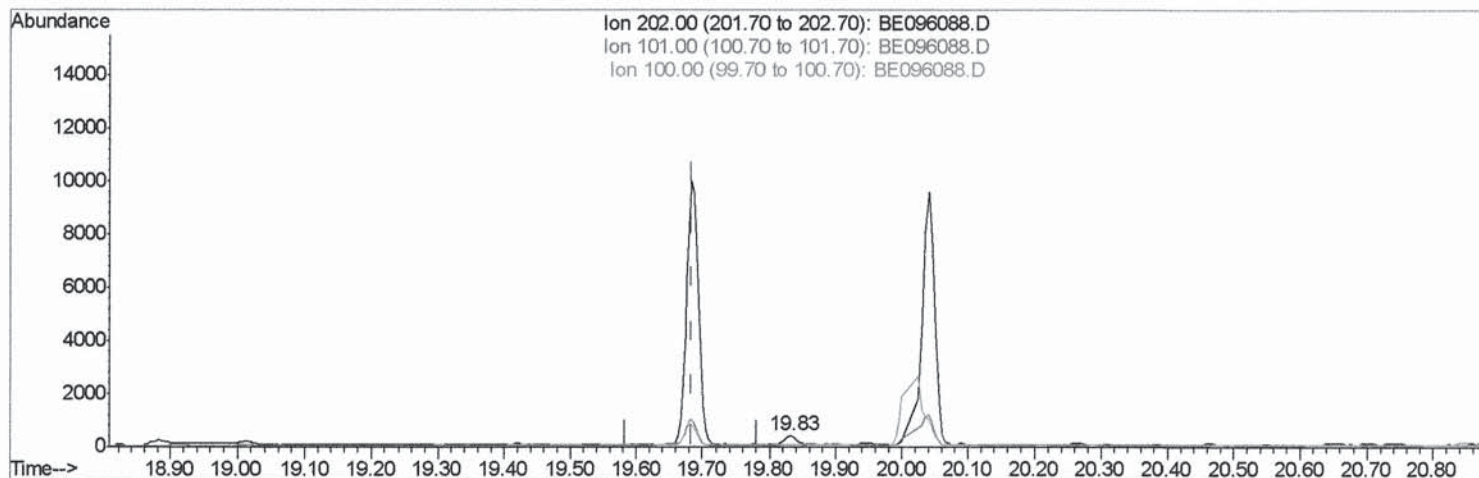

TIC: BE096088.D

(15) Fluoranthene (C)

19.833min (+0.149) 0.02ng/ul

response 465

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	23.40
100.00	19.50	19.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

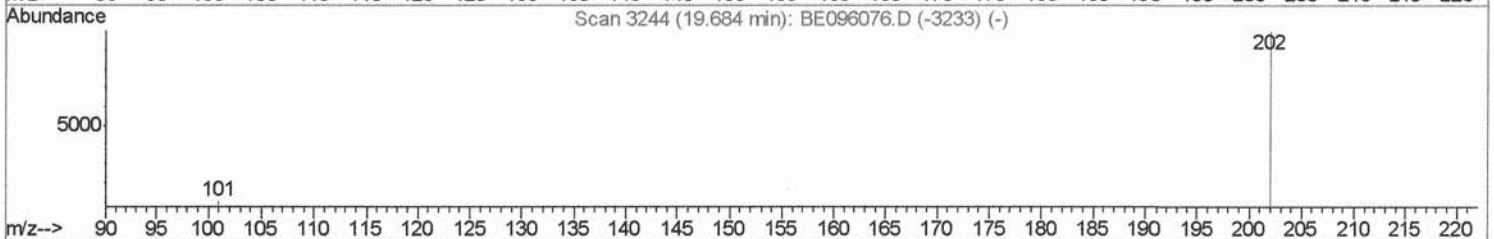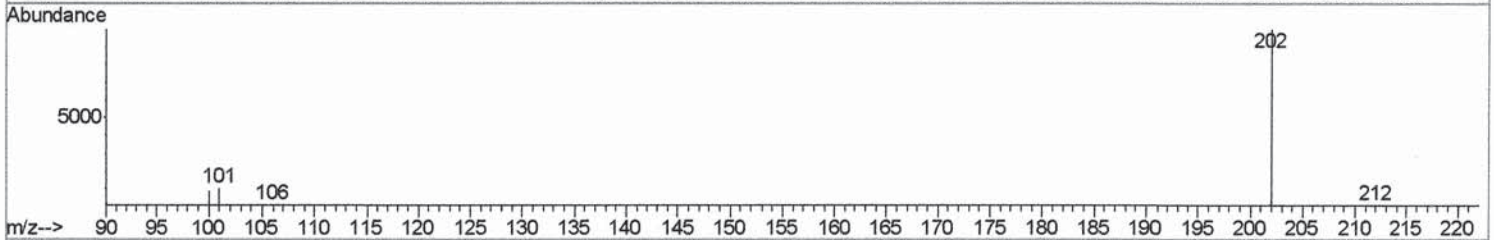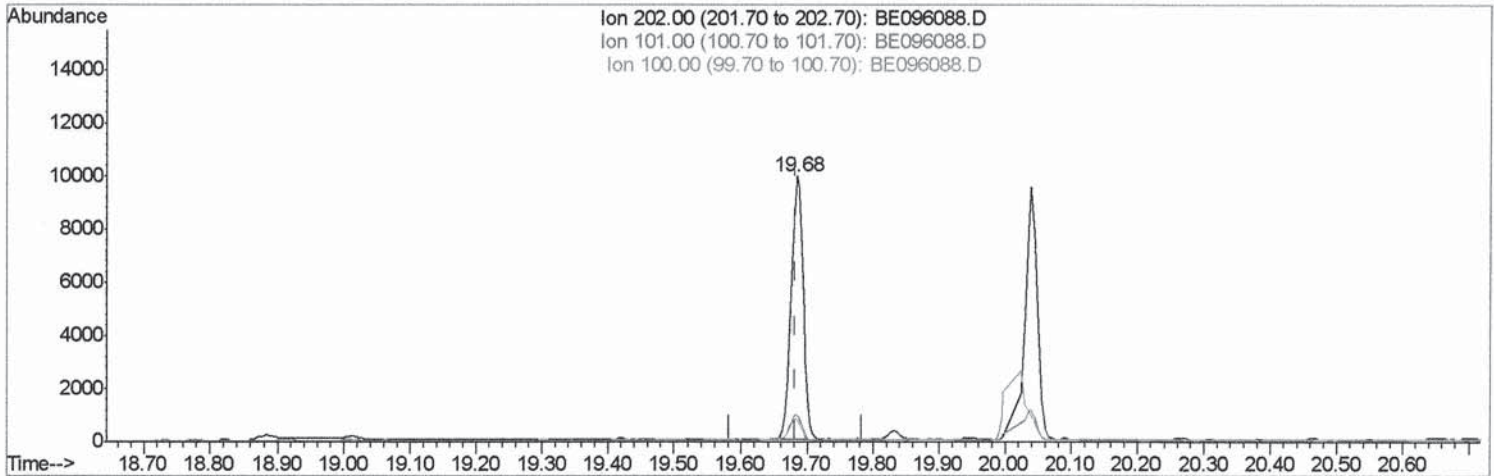

TIC: BE096088.D

(15) Fluoranthene (C)

19.684min (-0.001) 0.49ng/ul m> s> 4/23/18

response 12808

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.34
100.00	19.50	8.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

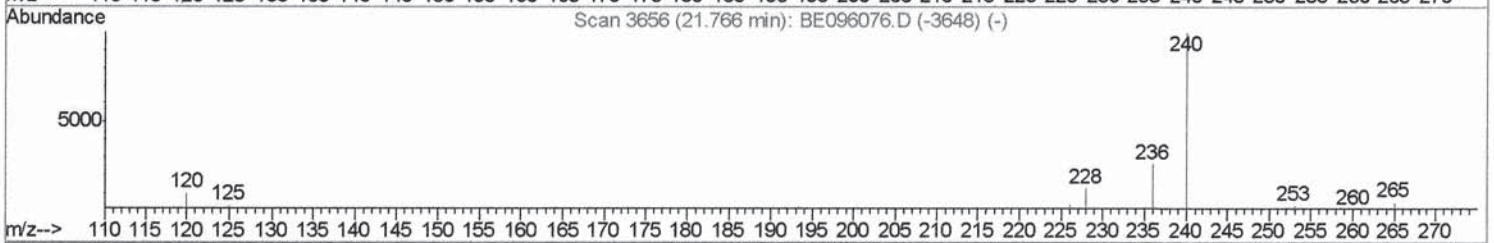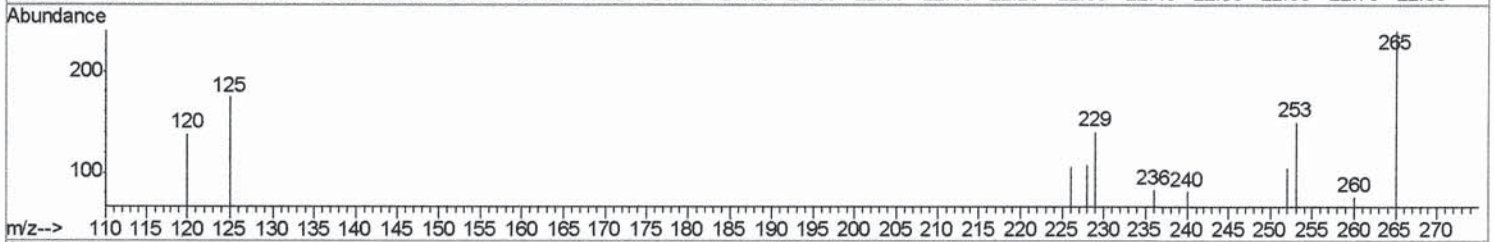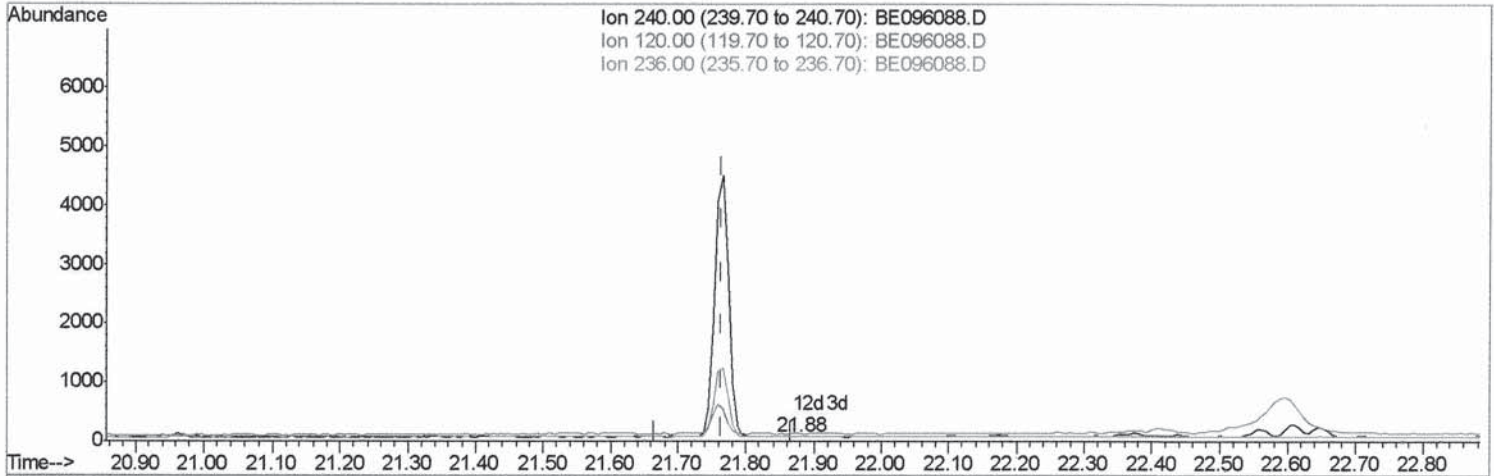

TIC: BE096088.D

(16) Chrysene-d12 (I)

21.879min (+0.113) 0.40ng/ul

response 7

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	170.37#
236.00	34.90	102.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:50:45 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

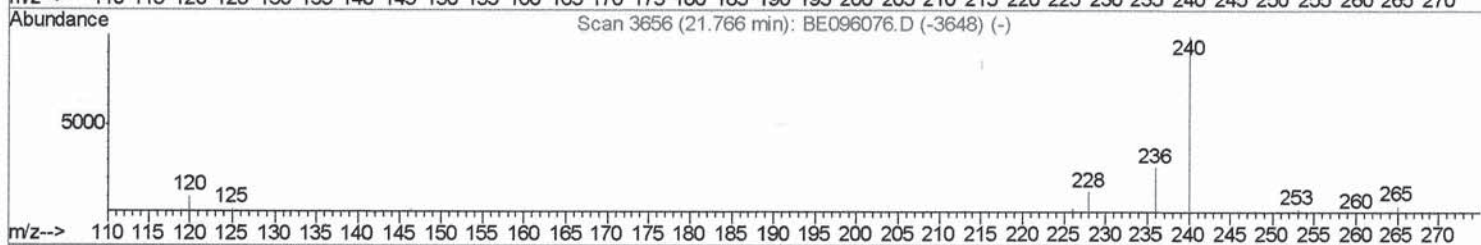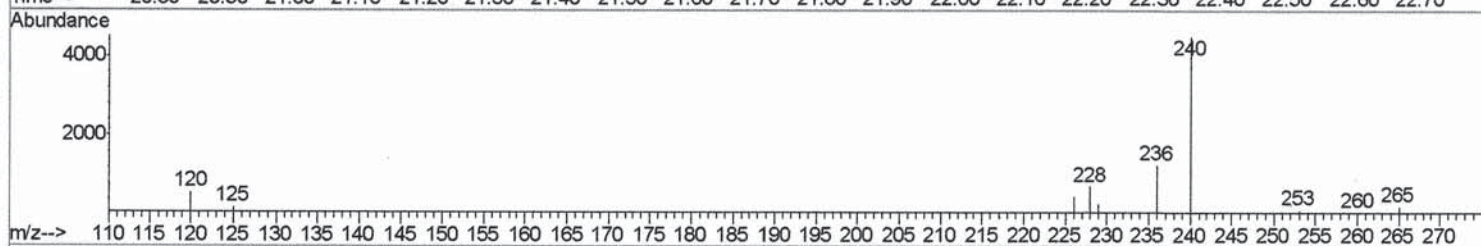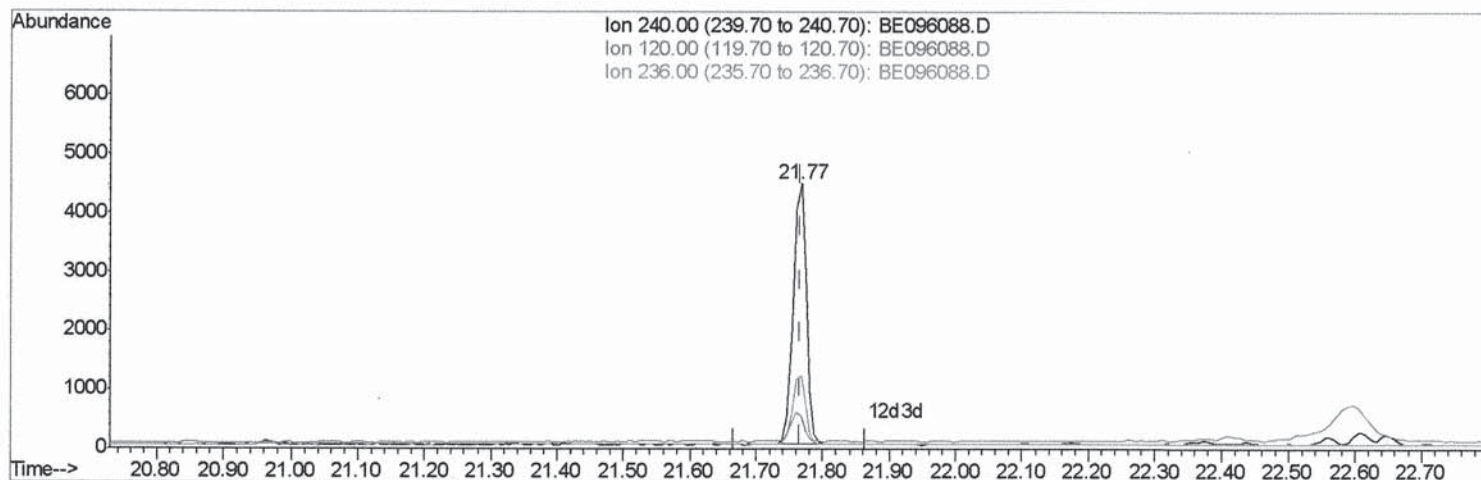

TIC: BE096088.D

(16) Chrysene-d12 (I)

21.766min (+0.000) 0.40ng/ul m > 52 4/22/18

response 6210

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.34#
236.00	34.90	27.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

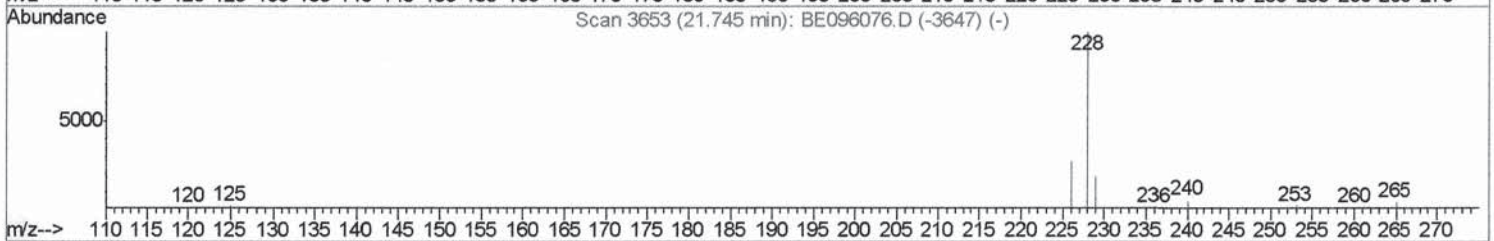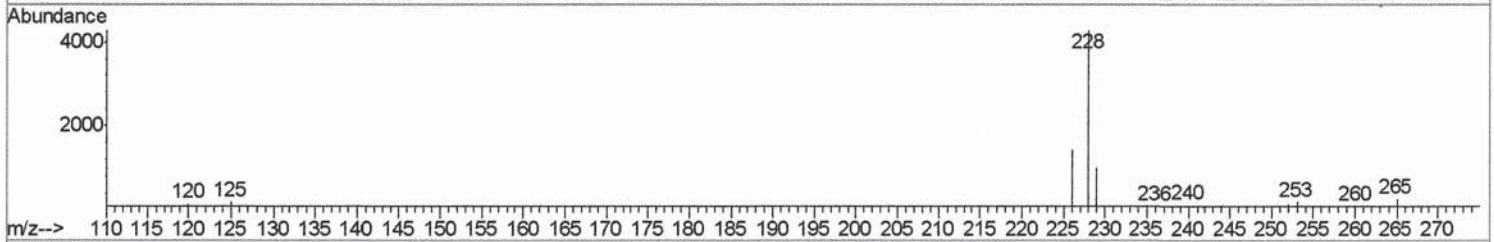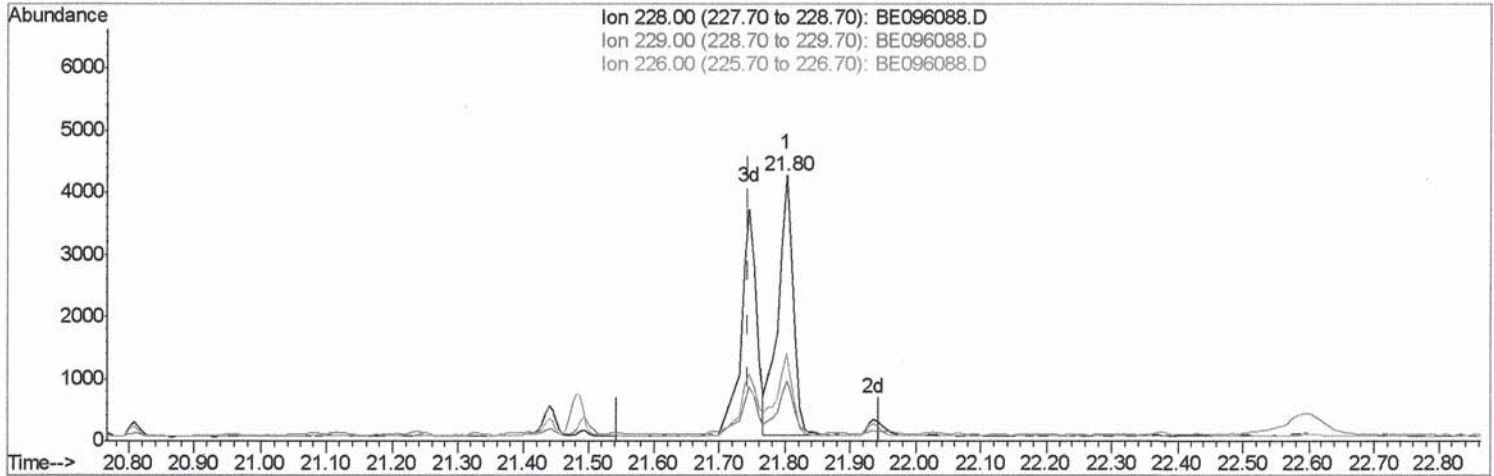

TIC: BE096088.D

(18) Benzo(a)anthracene

21.801min (+0.057) 0.28ng/ul

response 6945

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	22.91
226.00	21.30	33.19#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

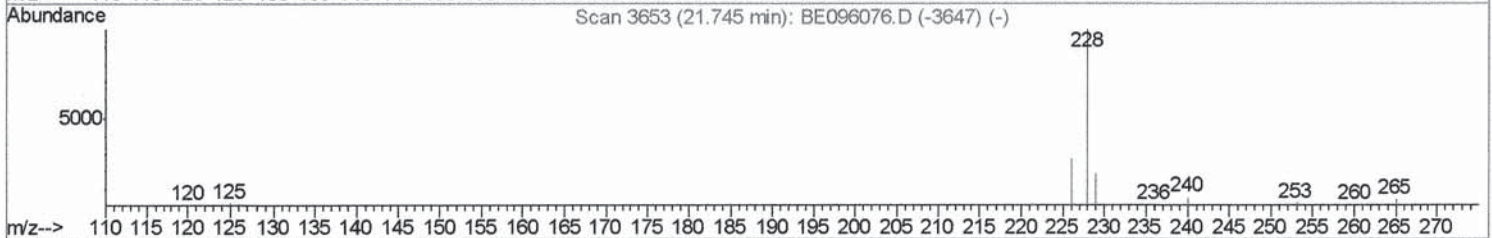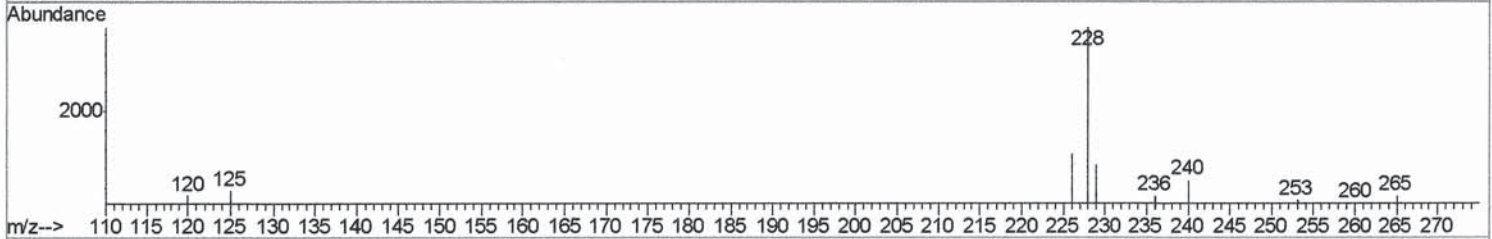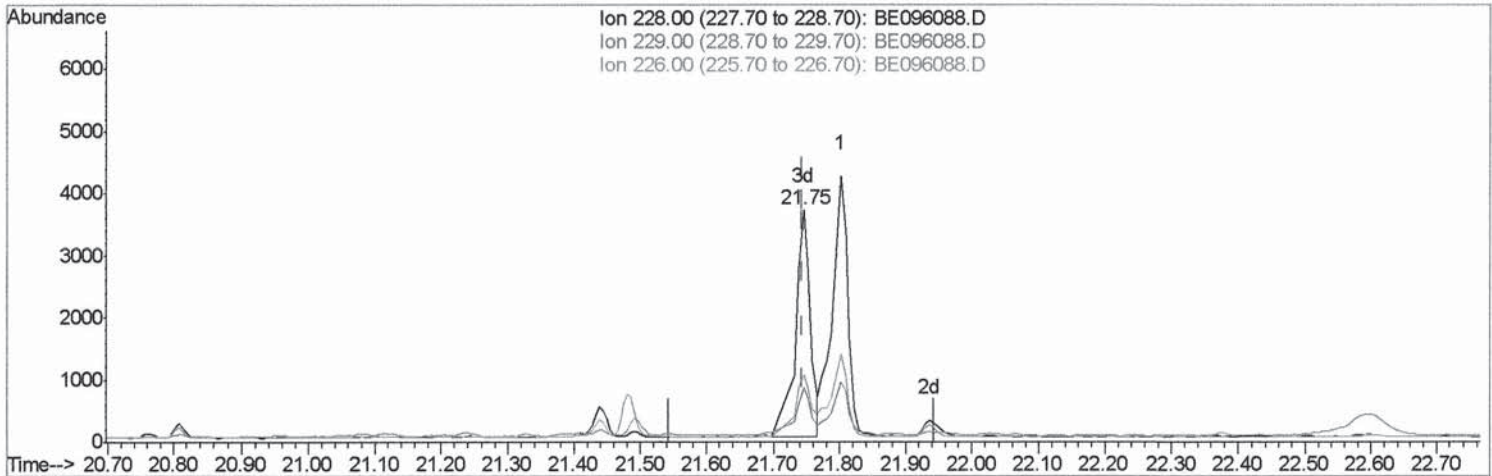

TIC: BE096088.D

(18) Benzo(a)anthracene

21.745min (+0.000) 0.33ng/ul m > 50 4/24/18

response 8194

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	23.27
226.00	21.30	29.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

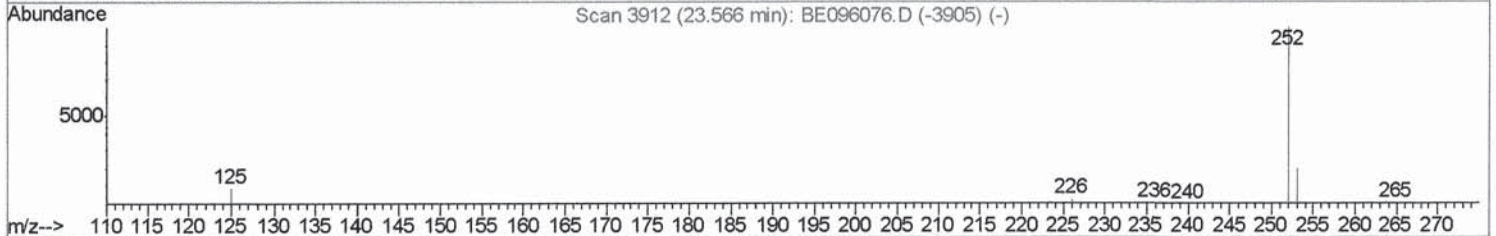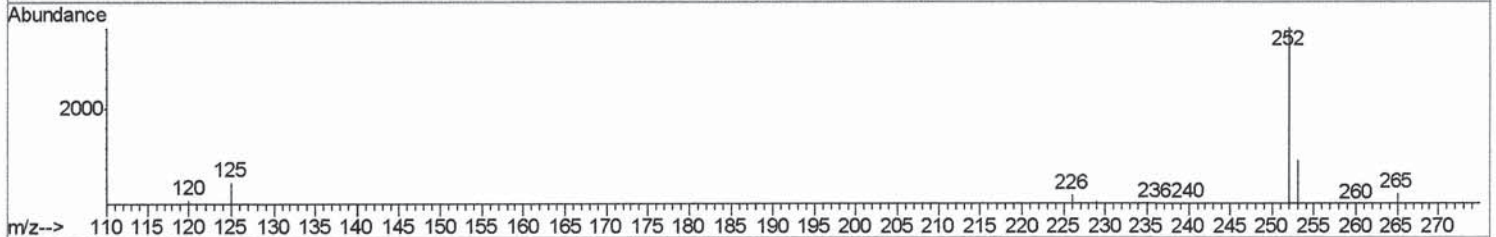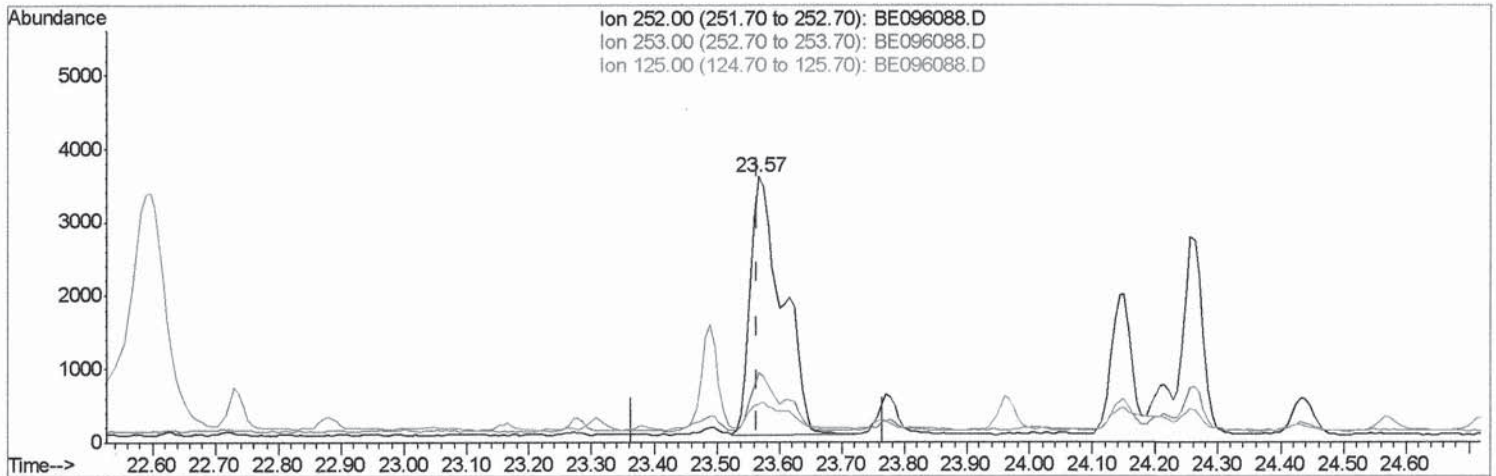

TIC: BE096088.D

(21) Benzo(b)fluoranthene
 23.566min (+0.000) 0.50ng/ul
 response 12315

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.47
125.00	17.50	14.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

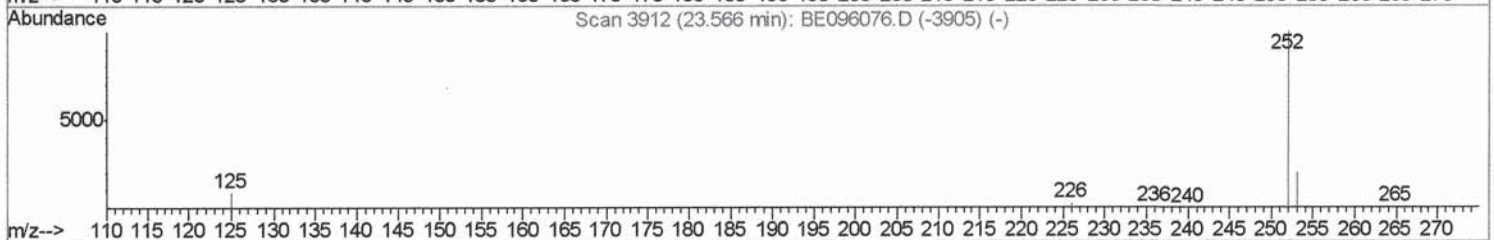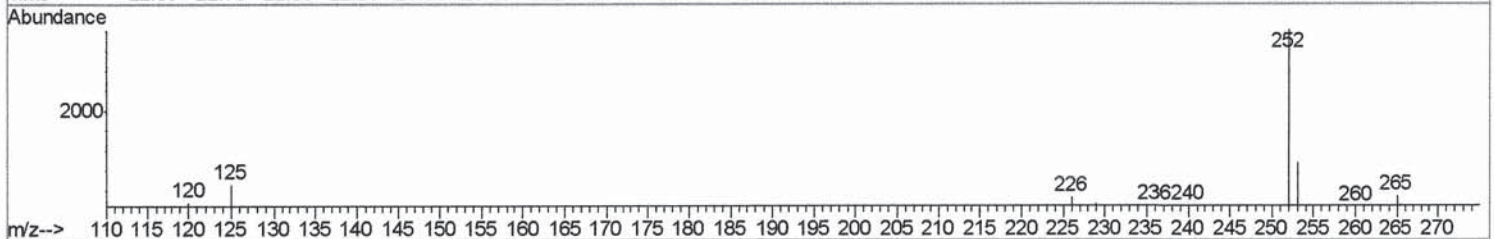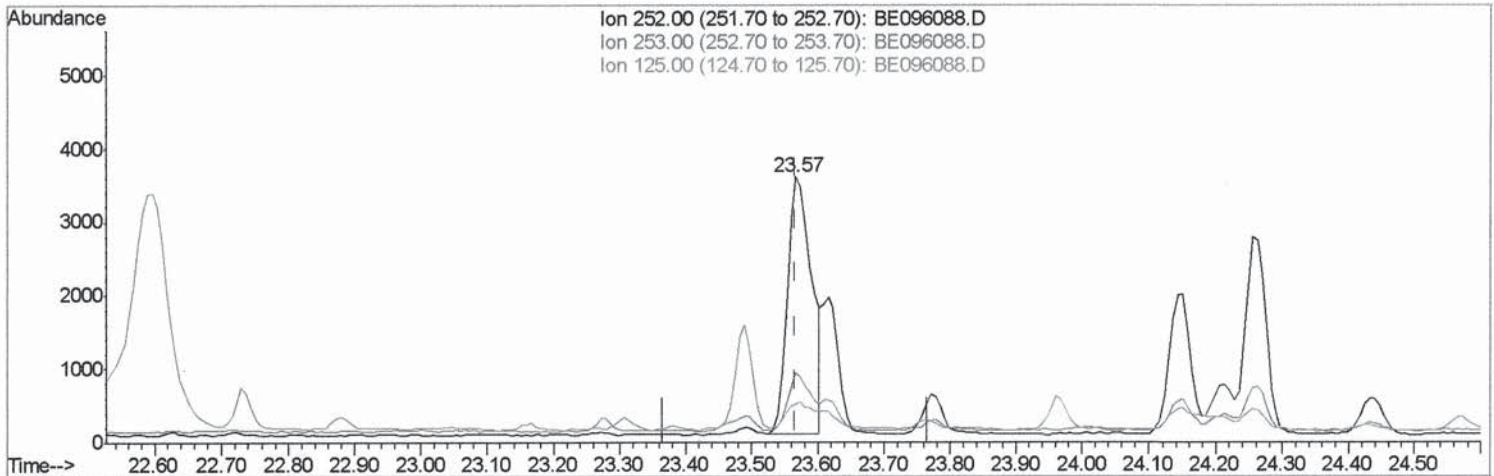

TIC: BE096088.D

(21) Benzo(b)fluoranthene

23.566min (+0.000) 0.37ng/ul m > SJ 4/22/18

response 9117

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	26.47
125.00	17.50	14.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096088.D
Acq On : 23 Apr 2018 17:01
Operator : SJ/JU
Sample : J2355-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y30

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 05:21:12 2018
Response via : Initial Calibration

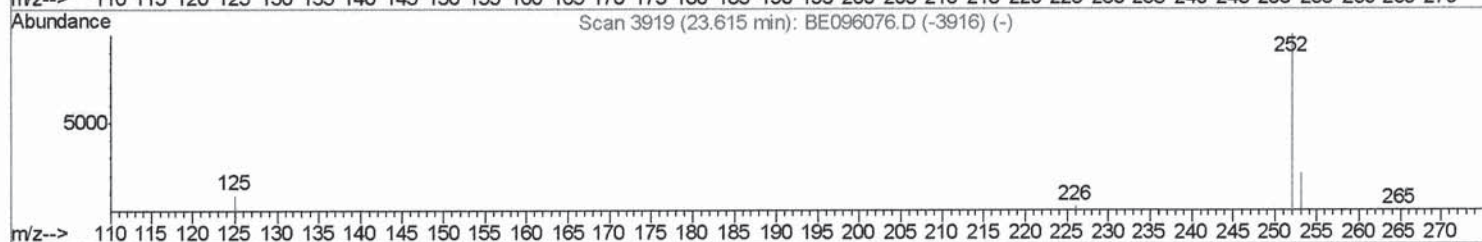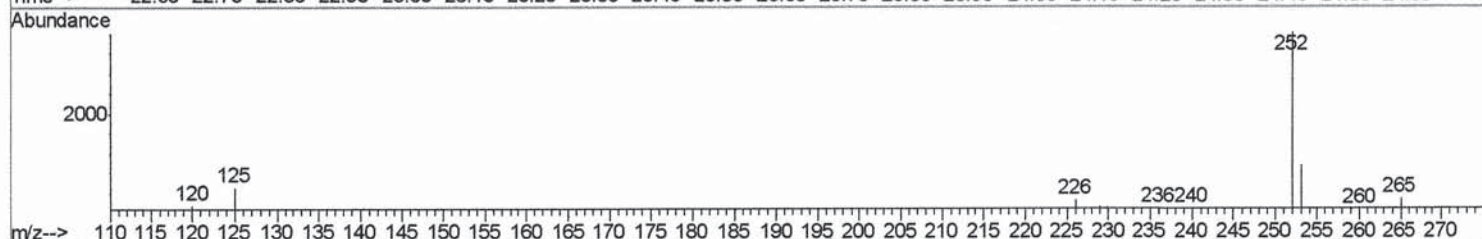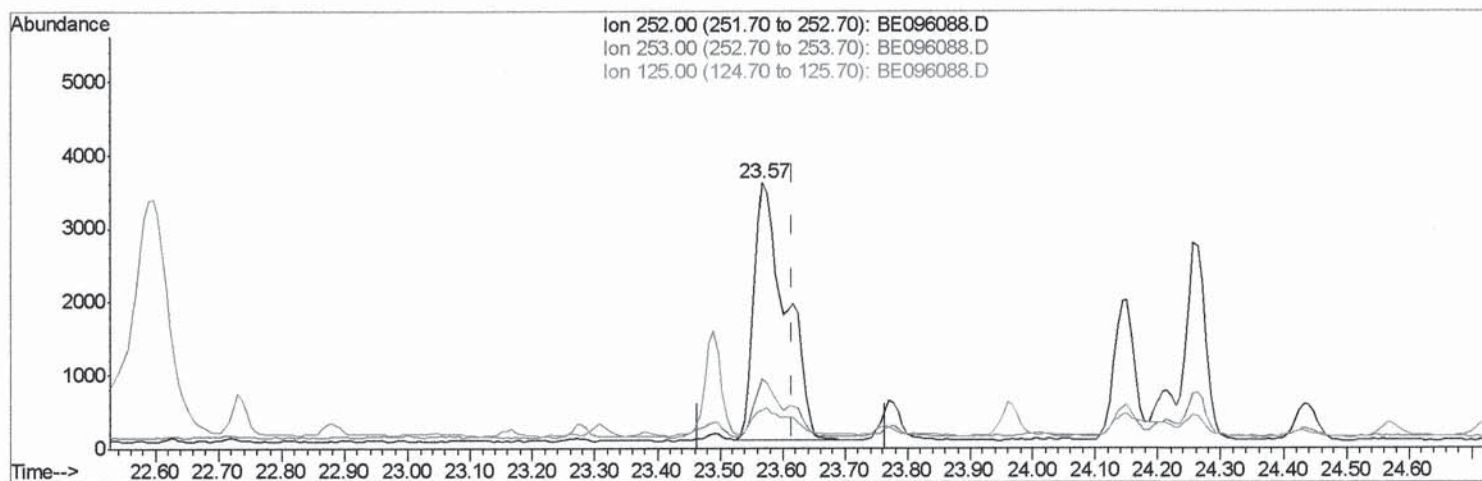

TIC: BE096088.D

(22) Benzo(k)fluoranthene

23.566min (-0.049) 0.50ng/ul

response 12273

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.47
125.00	17.10	14.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:52:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

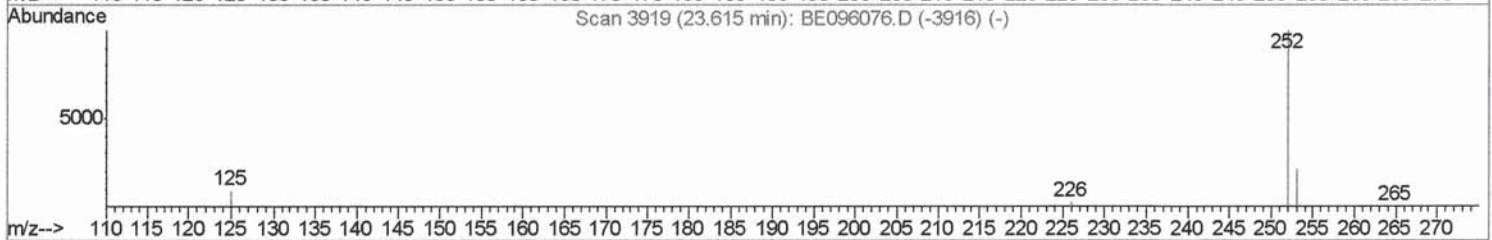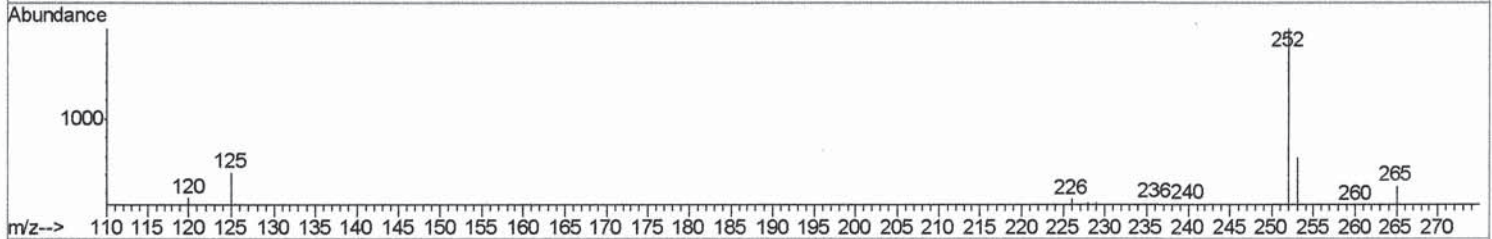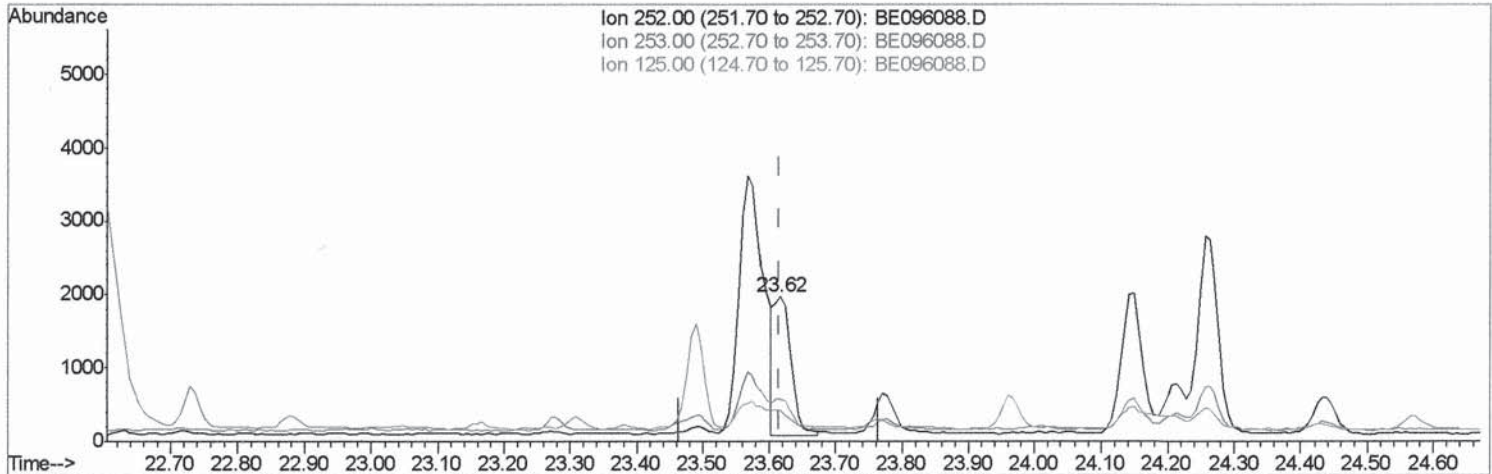

TIC: BE096088.D

(22) Benzo(k)fluoranthene

23.616min (+0.000) 0.13ng/ul m > SJ 4/22/18

response 3281

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	29.54
125.00	17.10	21.32#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096088.D
 Acq On : 23 Apr 2018 17:01
 Operator : SJ/JU
 Sample : J2355-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y30

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:01 PM

Quant Time: Apr 24 06:53:55 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 05:21:12 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	1860	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5036	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	2987	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	6491m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	6210m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	7627	0.40	ng/ul	0.00

SJ 4/23/18

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.76	152	2396	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	6147m	0.23	ng/ul	0.00

SJ 4/23/18

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	14.70	152	668	0.043	ng/ul#	87
9) Fluorene	15.99	166	269	0.021	ng/ul#	88
12) Phenanthrene	17.72	178	4415m	0.231	ng/ul	
13) Anthracene	17.80	178	749m	0.039	ng/ul	
15) Fluoranthene	19.68	202	12808m	0.492	ng/ul	
17) Pyrene	20.04	202	13580	0.644	ng/ul#	80
18) Benzo(a)anthracene	21.75	228	8194m	0.327	ng/ul	
19) Chrysene	21.80	228	6919	0.383	ng/ul	95
21) Benzo(b)fluoranthene	23.57	252	9117m	0.369	ng/ul	
22) Benzo(k)fluoranthene	23.62	252	3281m	0.133	ng/ul	
23) Benzo(a)pyrene	24.26	252	5660	0.238	ng/ul#	86
24) Indeno(1,2,3-cd)pyrene	27.16	276	4579	0.173	ng/ul#	74
25) Dibenzo(a,h)anthracene	27.18	278	1361	0.064	ng/ul#	81
26) Benzo(a,h,i)perylene	28.04	276	3389	0.153	ng/ul	97

SJ 4/23/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed