


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096091.D
Acq On : 23 Apr 2018 18:48
Operator : SJ/JU
Sample : J2355-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y24

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:16:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

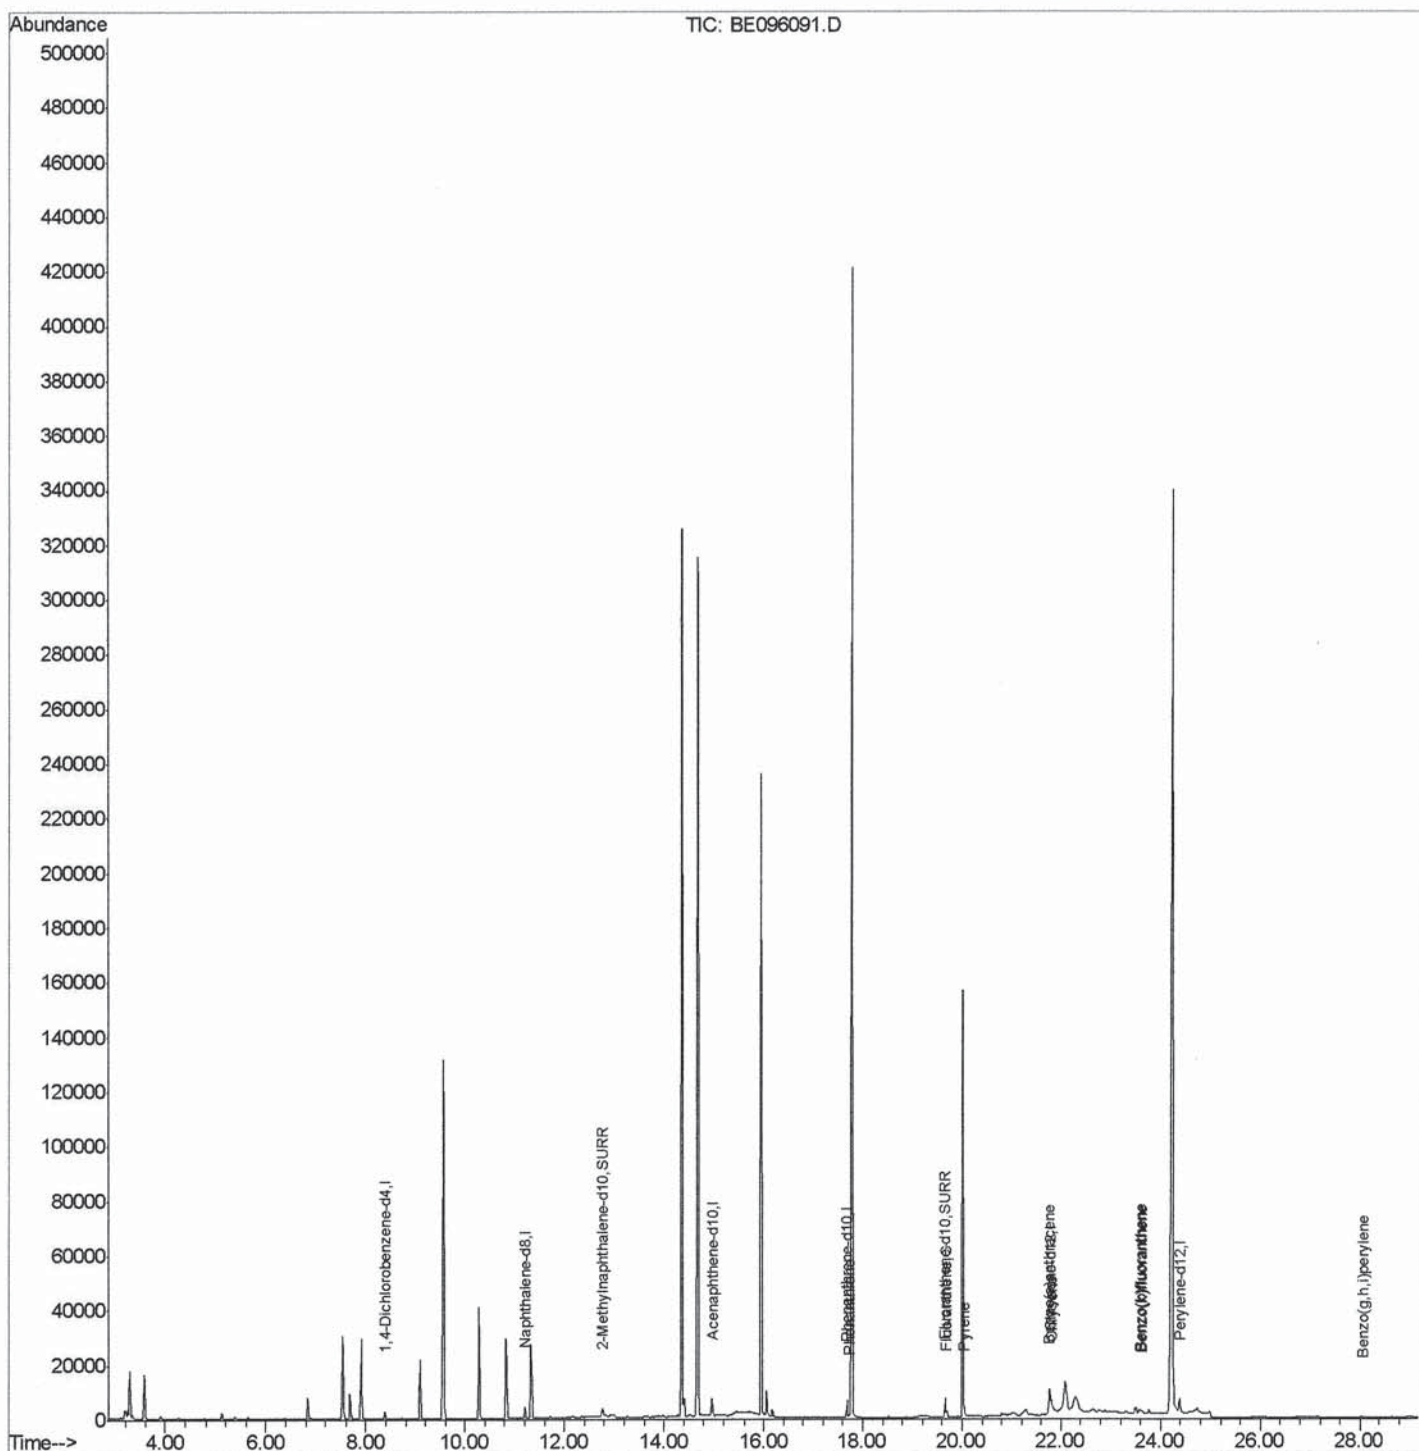

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096091.D
Acq On : 23 Apr 2018 18:48
Operator : SJ/JU
Sample : J2355-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y24

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:00:27 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

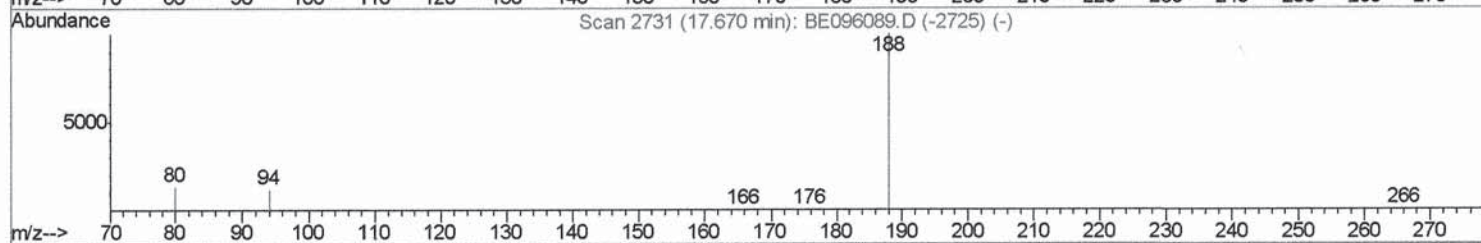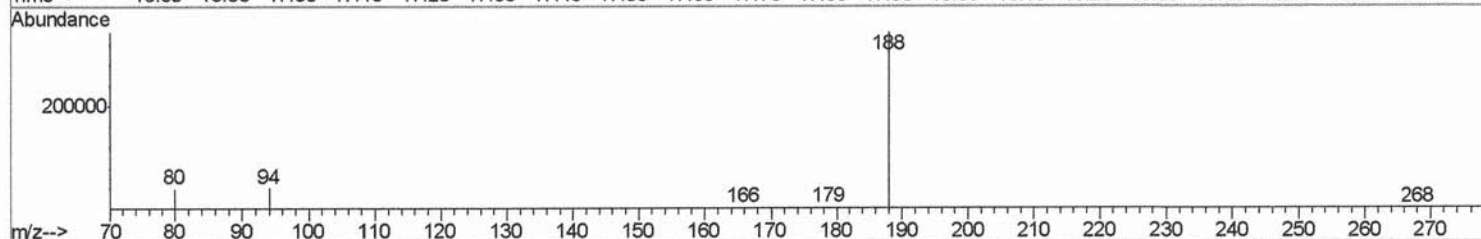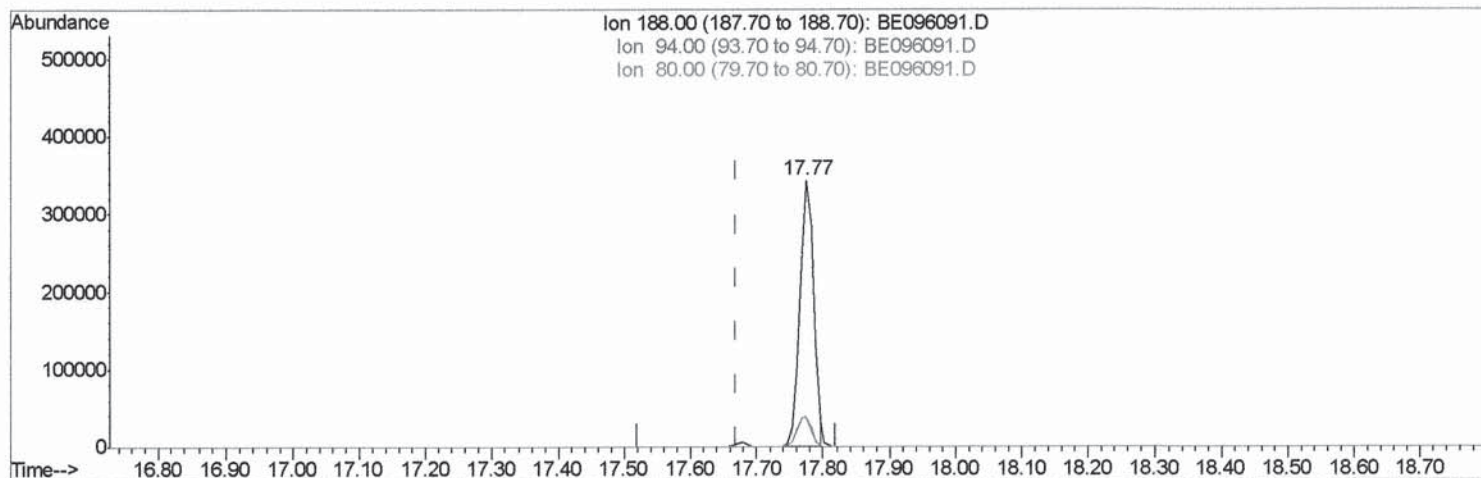

TIC: BE096091.D

(10) Phenanthrene-d10 (I)

17.774min (+0.103) 0.40ng/ul

response 489977

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.45
80.00	11.80	11.10
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:00:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

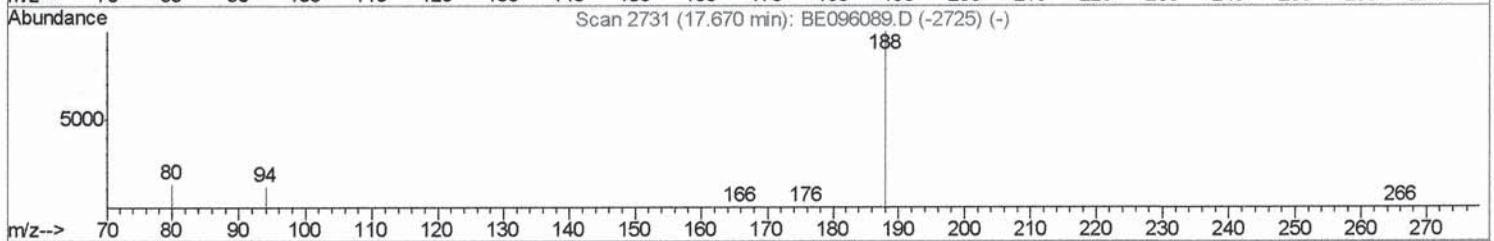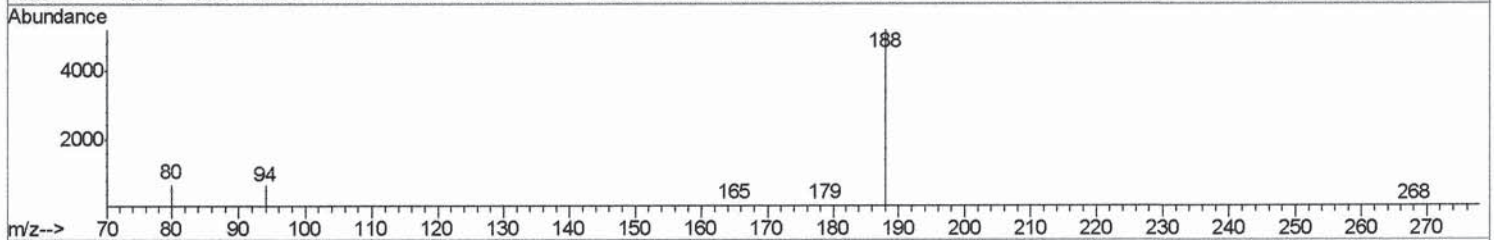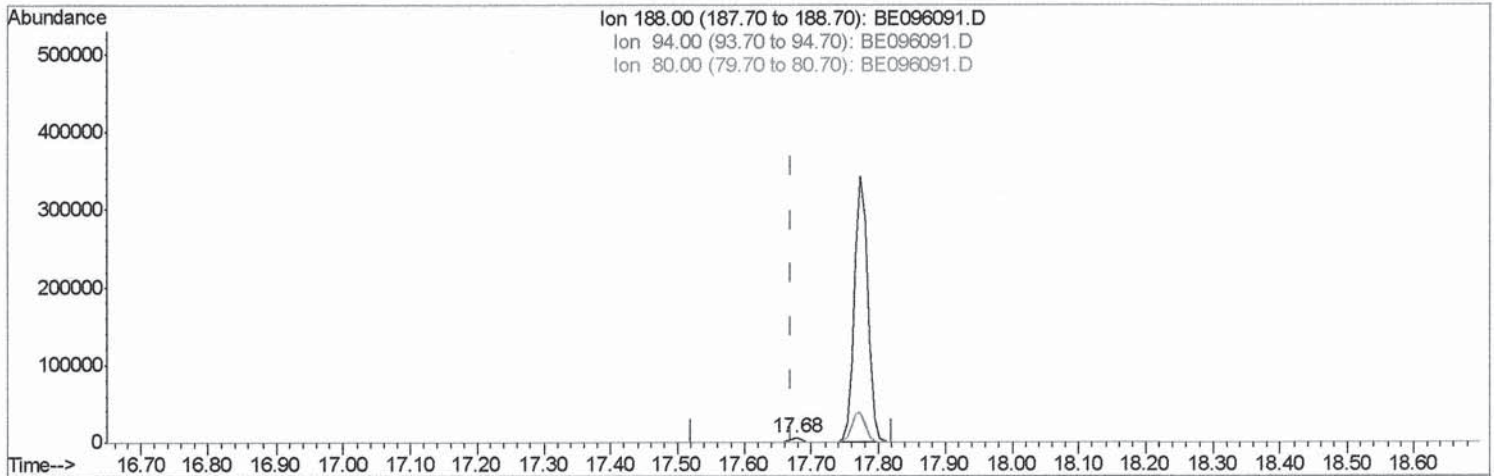

TIC: BE096091.D

(10) Phenanthrene-d10 (I)

17.675min (+0.005) 0.40ng/ul m> 57 4/24/18

response 7223

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.36
80.00	11.80	13.42
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

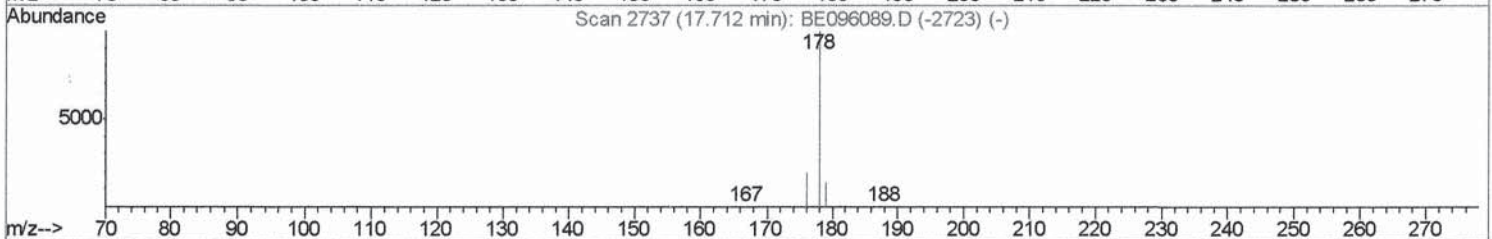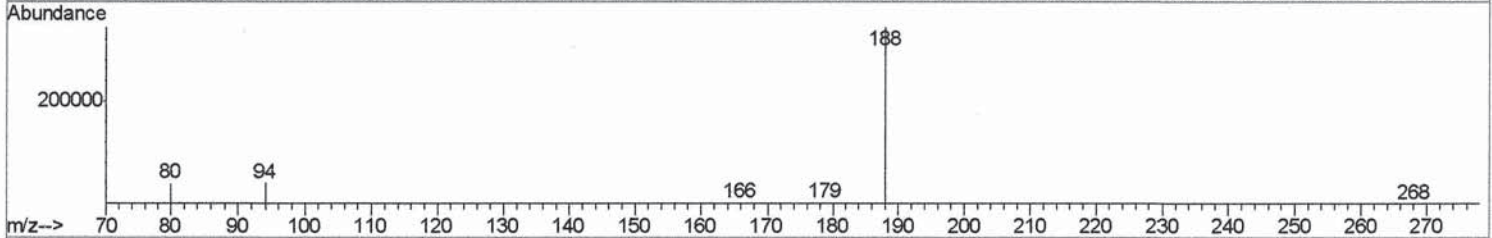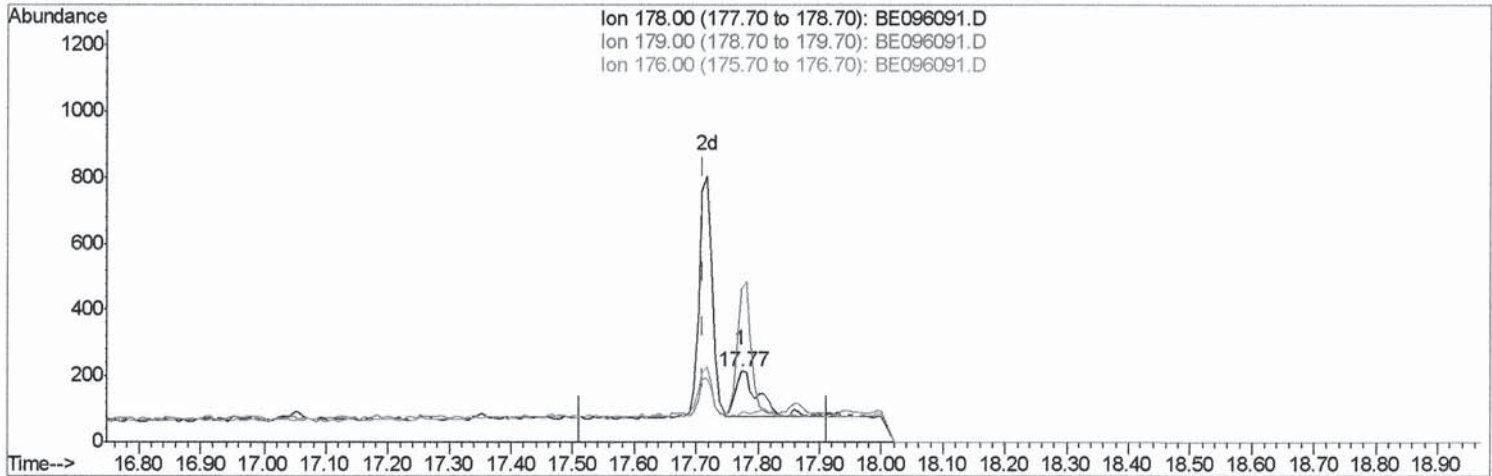

TIC: BE096091.D

(12) Phenanthrene

17.774min (+0.061) 0.02ng/ul

response 381

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	216.82#
176.00	17.00	42.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

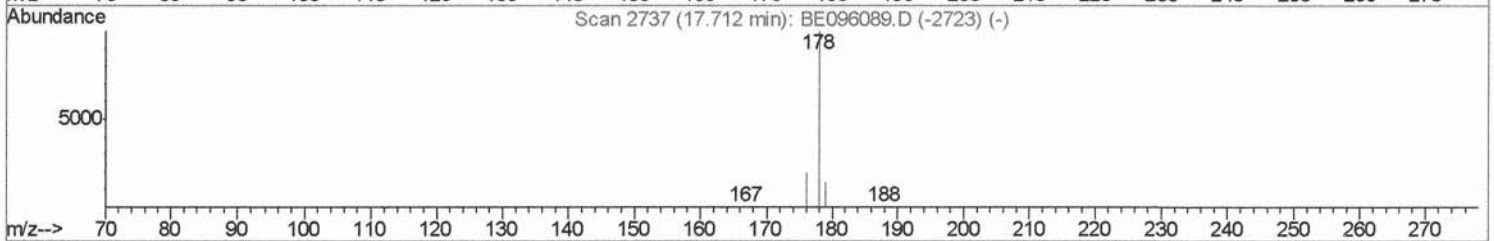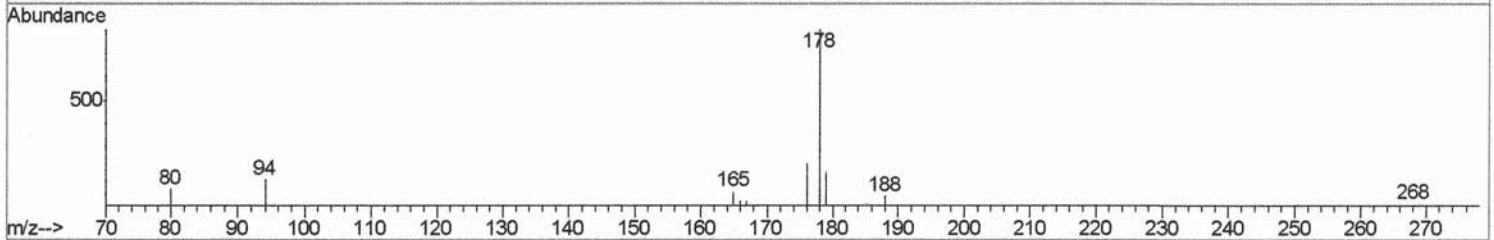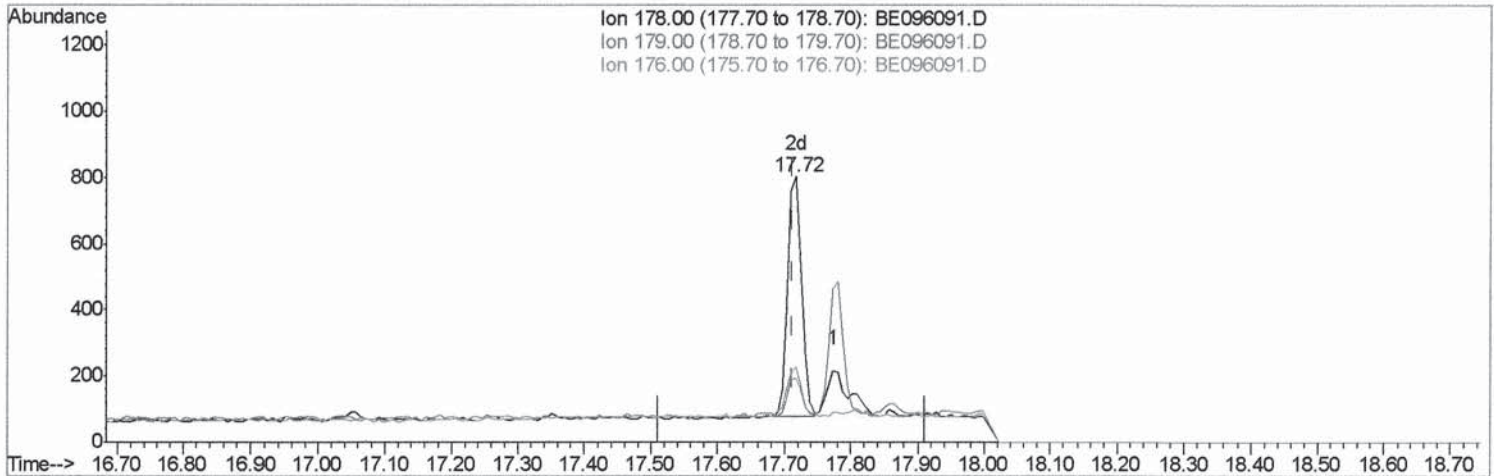

TIC: BE096091.D

(12) Phenanthrene

17.717min (+0.005) 0.05ng/ul m > 52 4K2118

response 1073

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.16
176.00	17.00	28.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

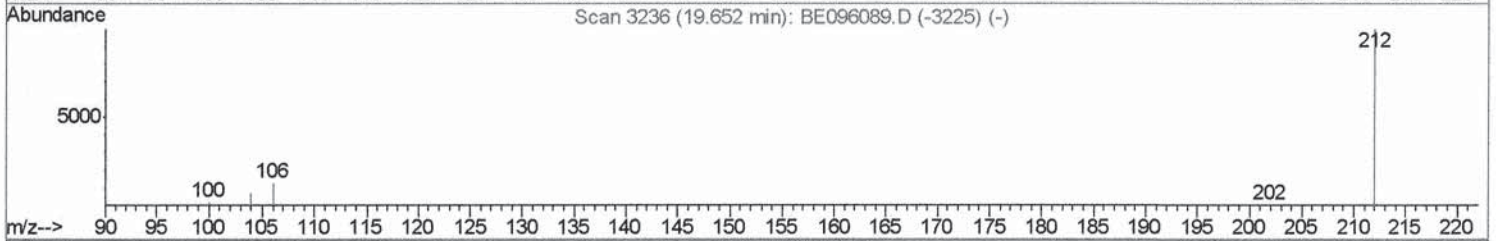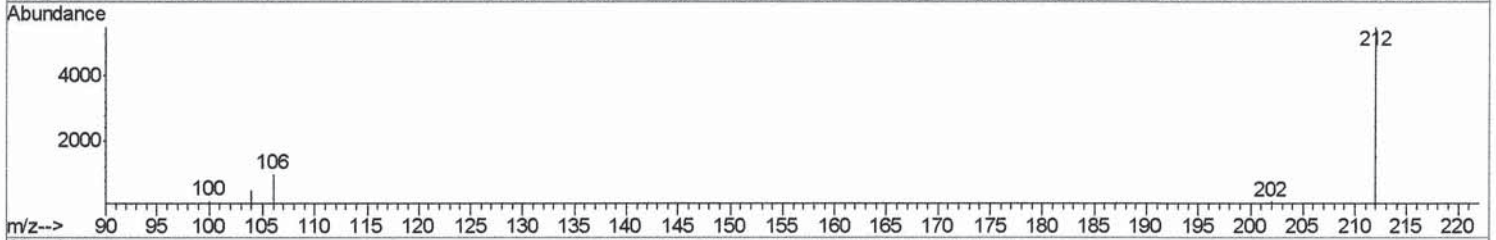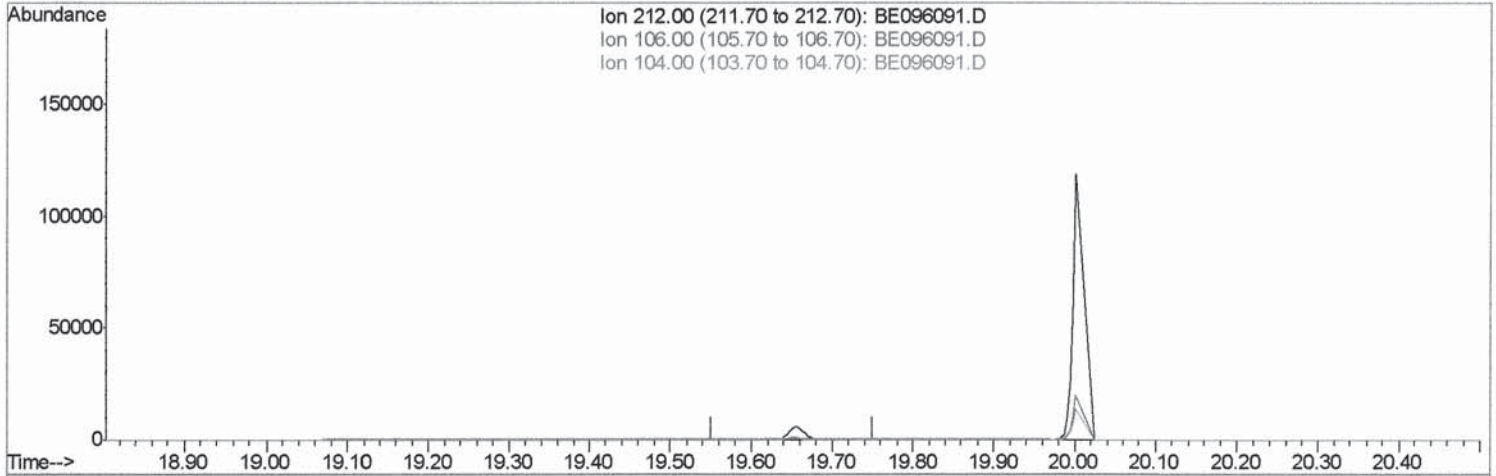

(14) Fluoranthene-d10 (SURR)

19.652min (-19.652) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

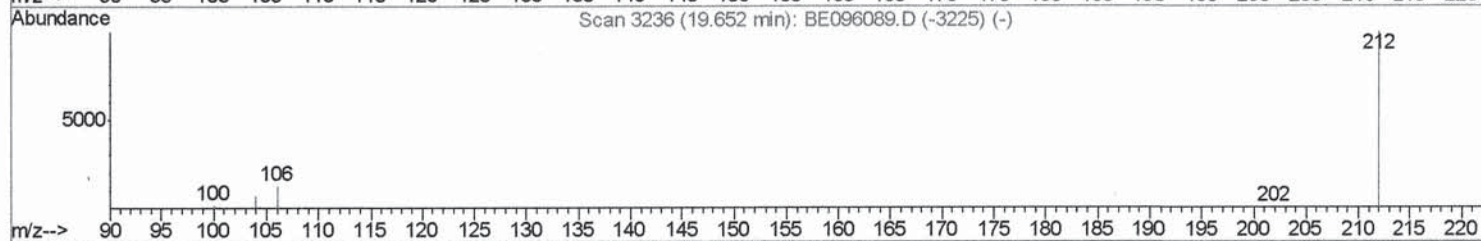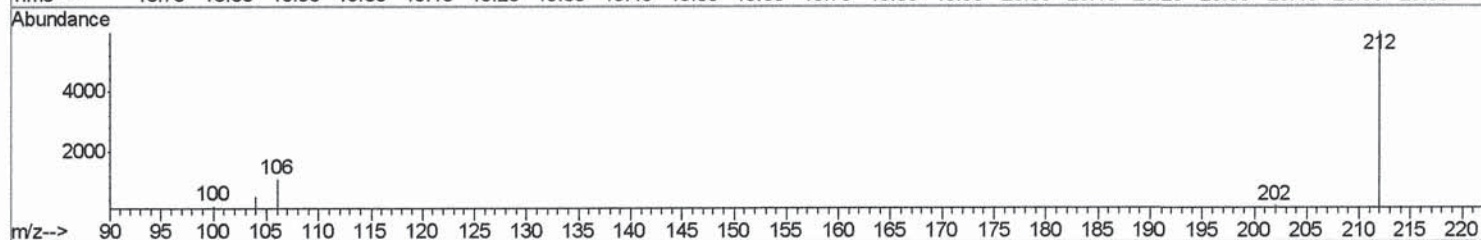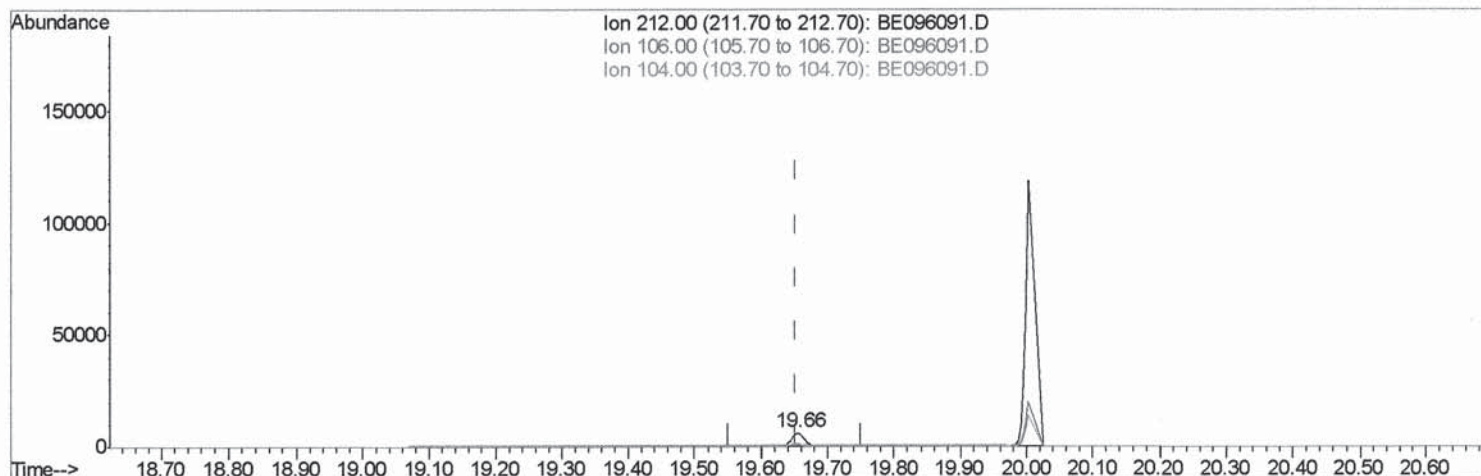

(14) Fluoranthene-d10 (SURR)

19.655min (+0.003) 0.27ng/ul m> SJ 4/22/18

response 7933

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

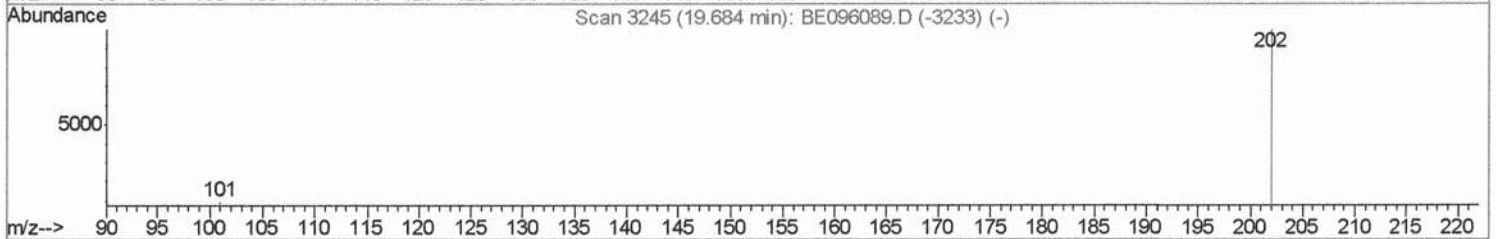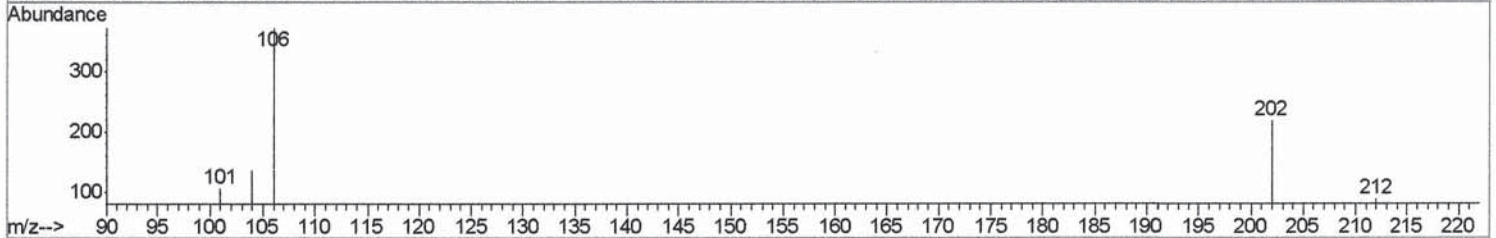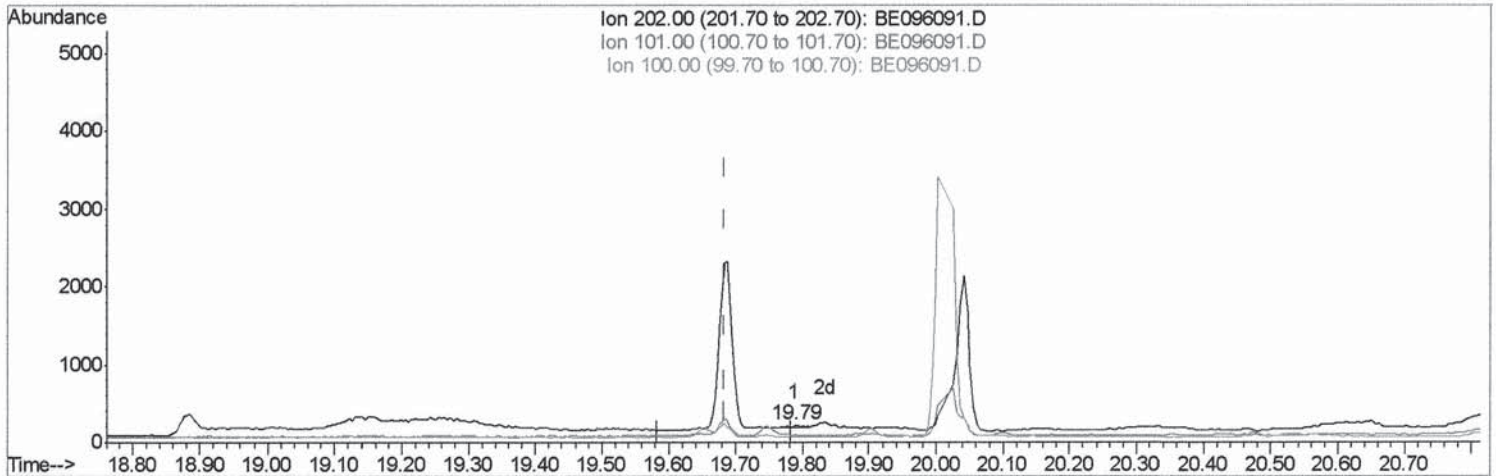

TIC: BE096091.D

(15) Fluoranthene (C)

19.787min (+0.103) 0.00ng/ul

response 79

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	48.62#
100.00	19.50	36.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

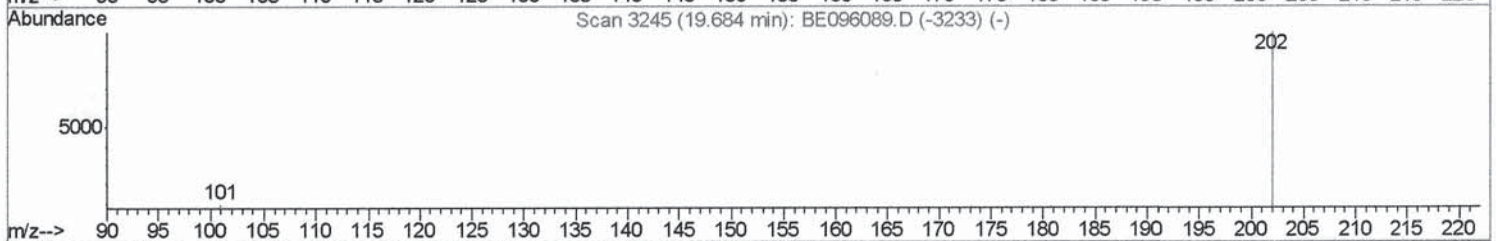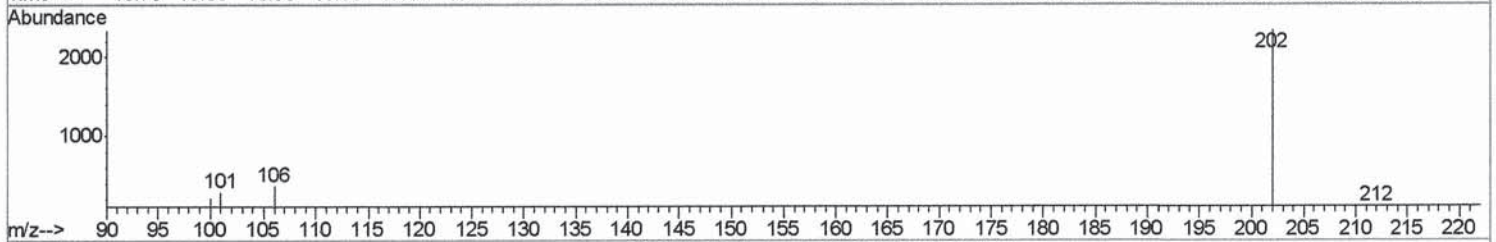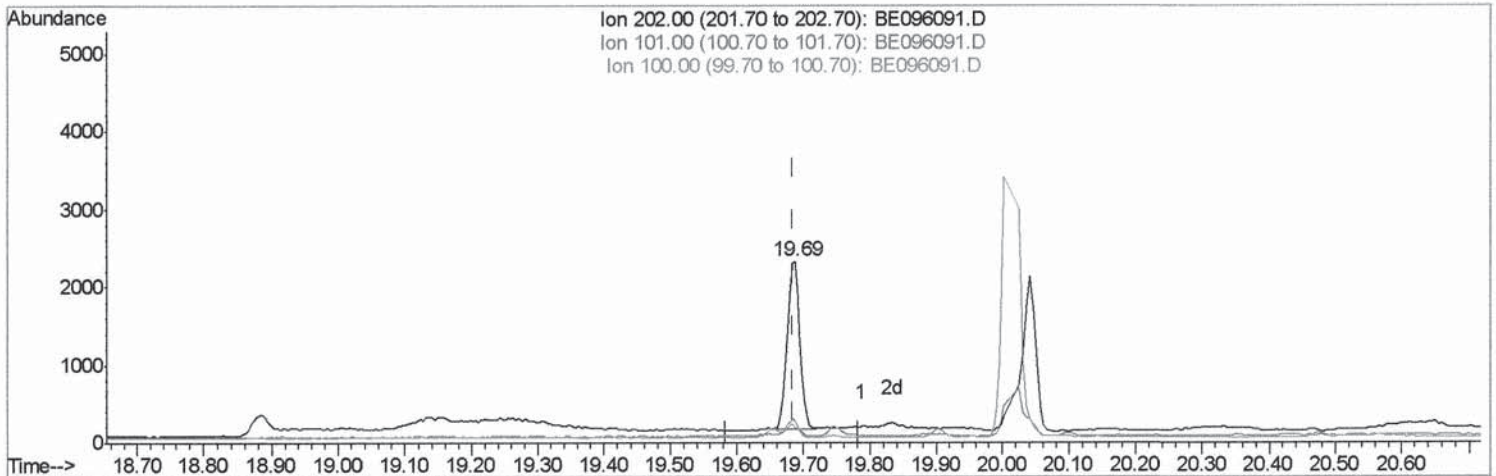

TIC: BE096091.D

(15) Fluoranthene (C)

19.687min (+0.003) 0.10ng/ul m > SJ 4/24/18

response 2834

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.30
100.00	19.50	8.96
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

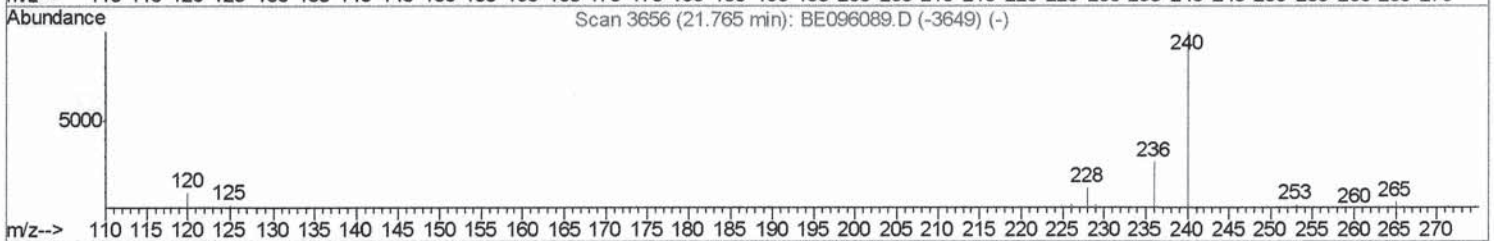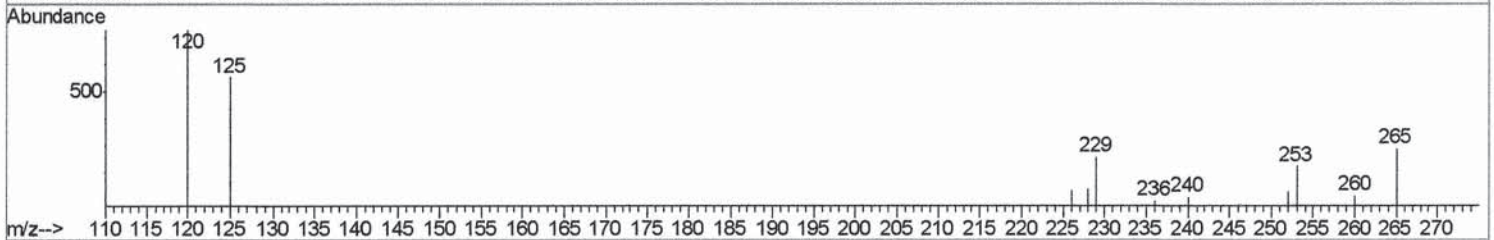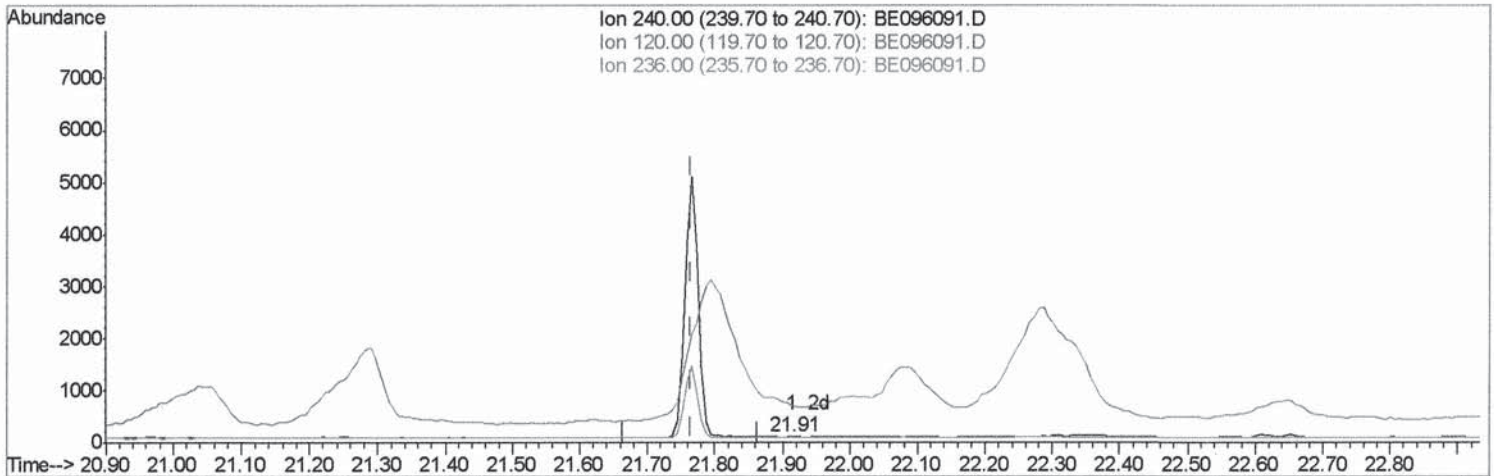

TIC: BE096091.D

(16) Chrysene-d12 (I)

21.913min (+0.148) 0.40ng/ul

response 8

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	662.73#
236.00	34.90	87.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:12:06 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

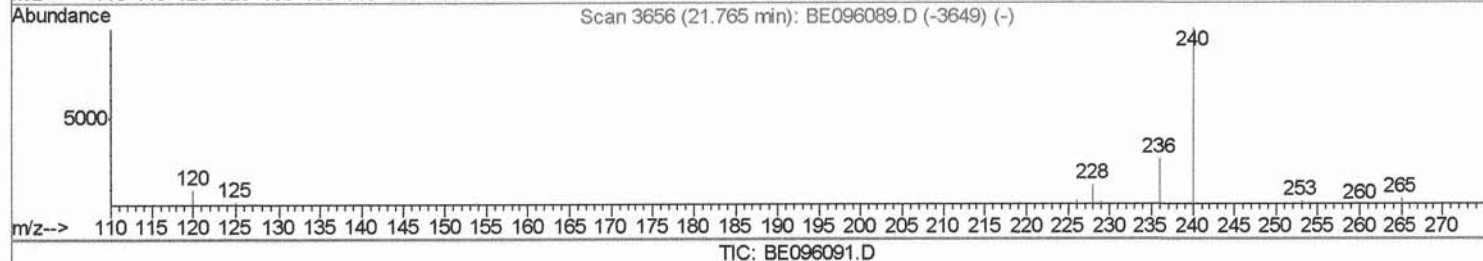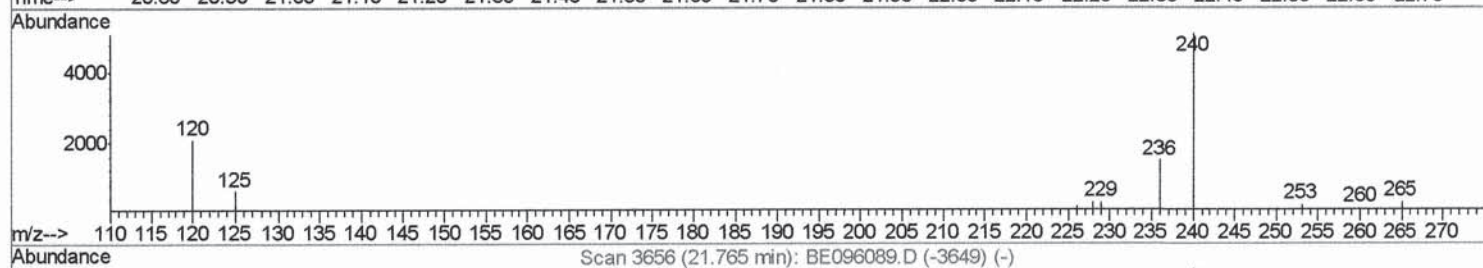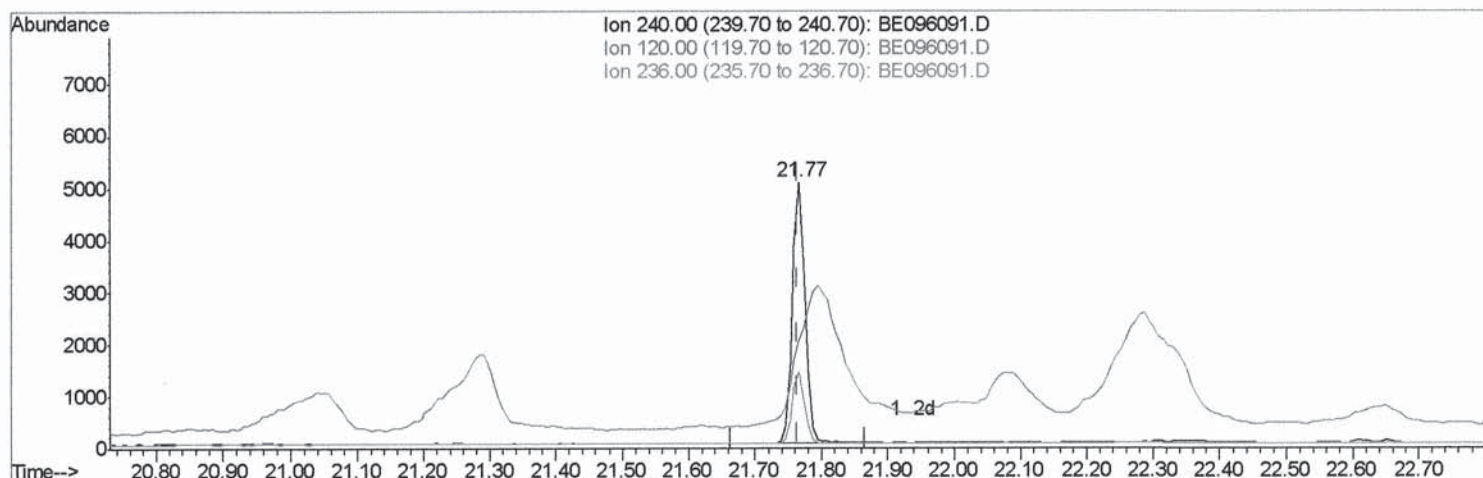

(16) Chrysene-d12 (I)

21.766min (+0.001) 0.40ng/ul m> SJ 4/24/18

response 6759

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	40.72#
236.00	34.90	29.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096091.D
Acq On : 23 Apr 2018 18:48
Operator : SJ/JU
Sample : J2355-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
A3Y24

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

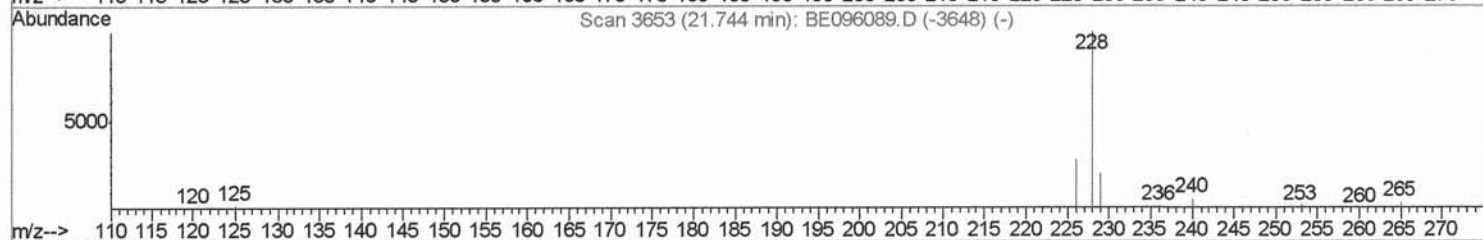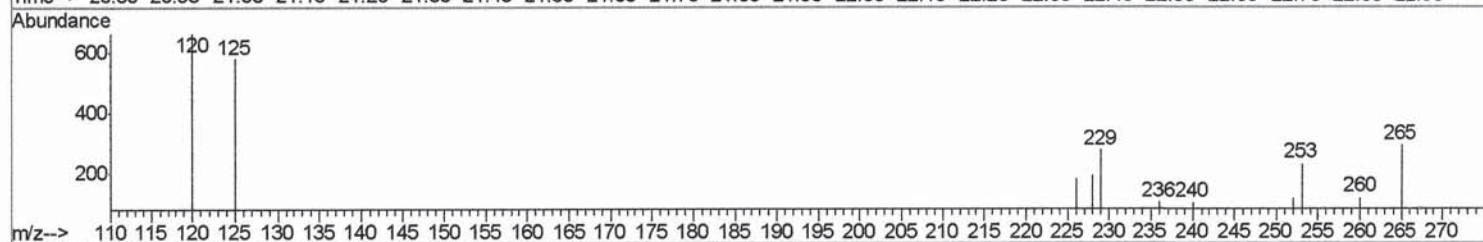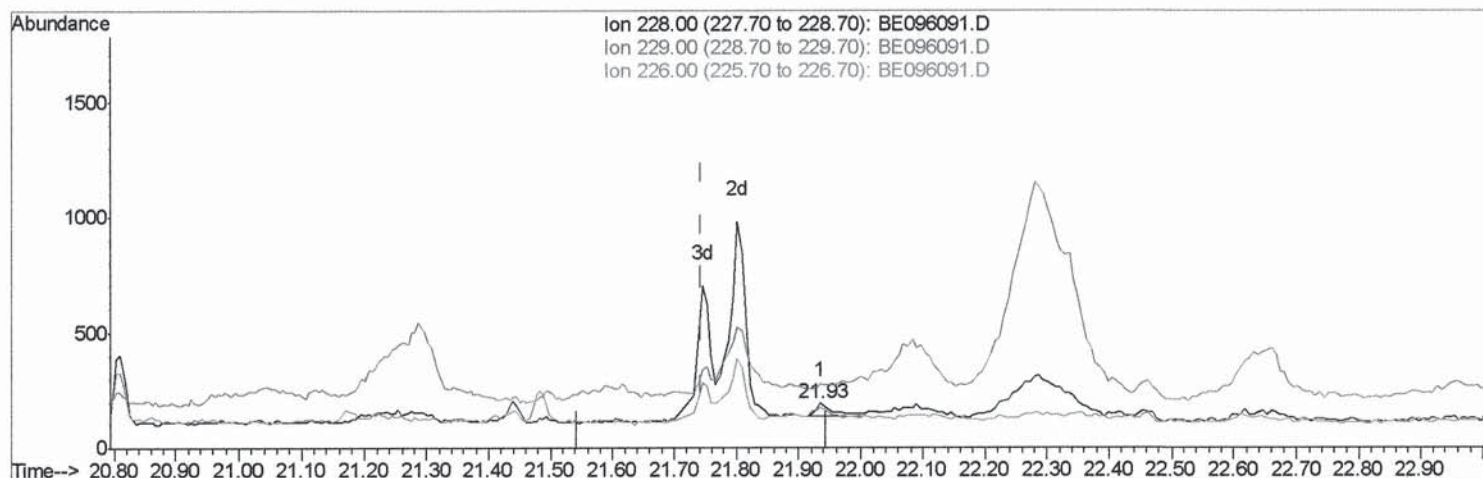

TIC: BE096091.D

(18) Benzo(a)anthracene

21.935min (+0.191) 0.00ng/ul

response 122

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	143.75#
226.00	21.30	93.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

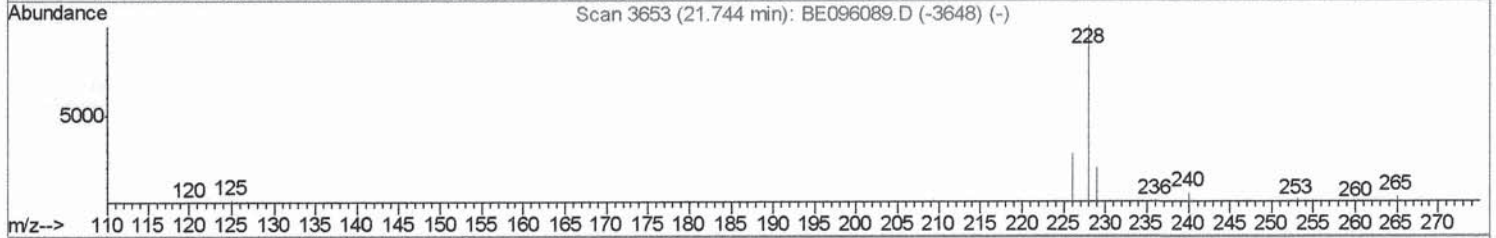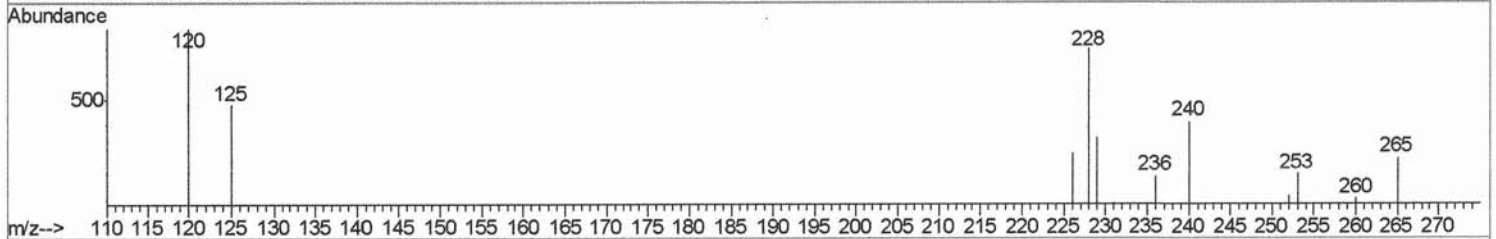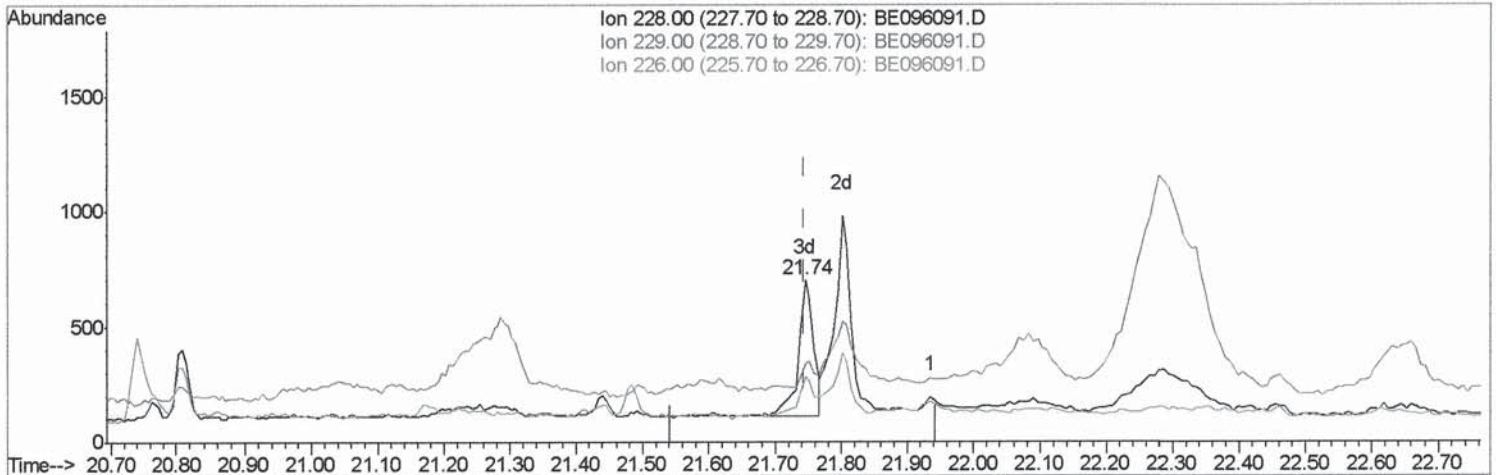

TIC: BE096091.D

(18) Benzo(a)anthracene

21.745min (+0.001) 0.04ng/ul m> SJ 4/24/18

response 1214

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	48.79#
226.00	21.30	40.54#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

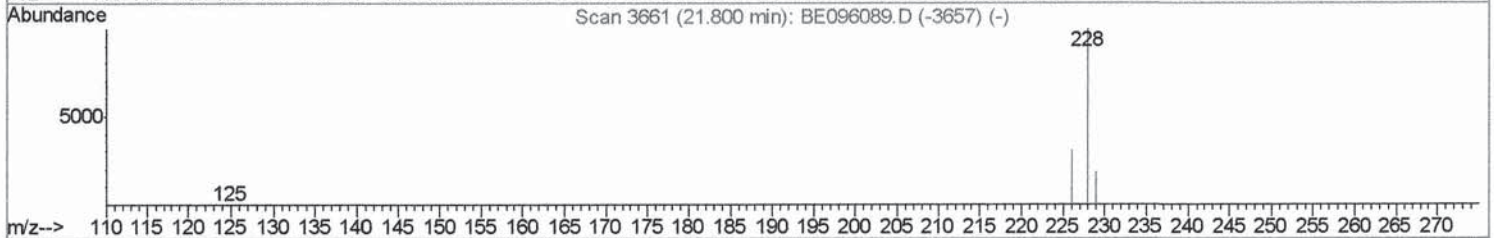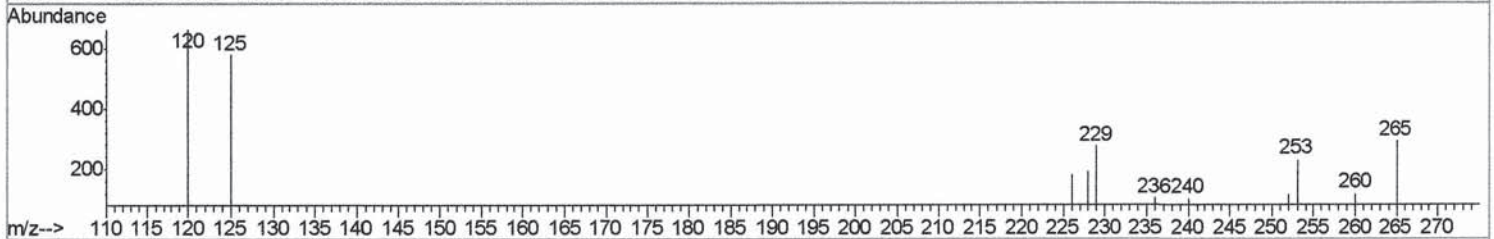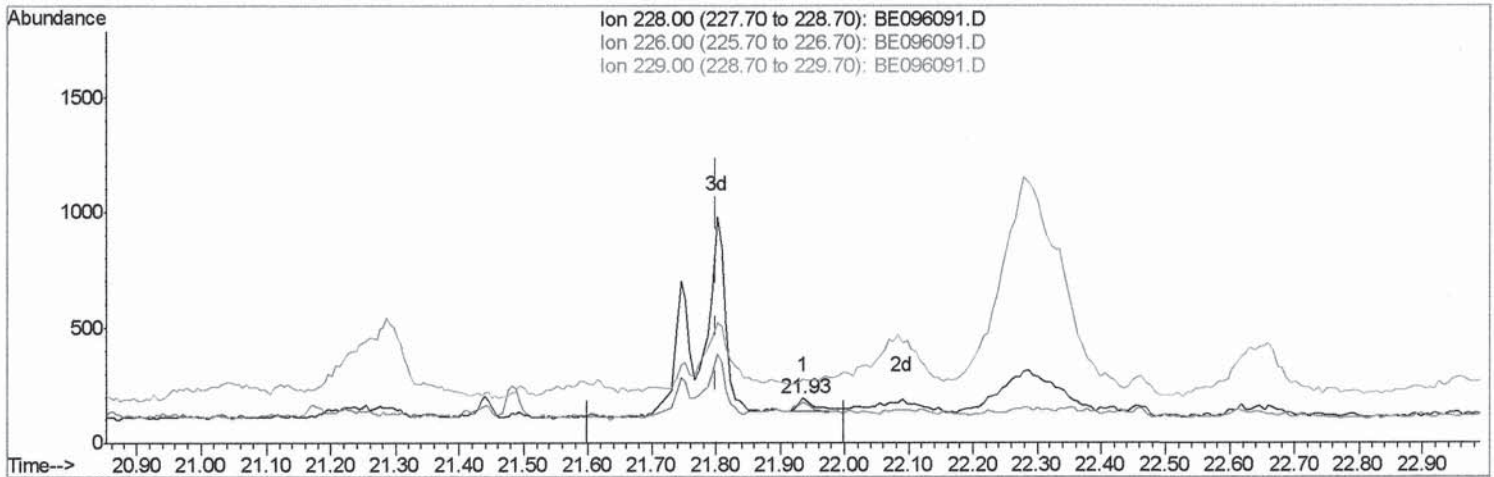

TIC: BE096091.D

(19) Chrysene

21.935min (+0.134) 0.01ng/ul

response 111

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	93.75#
229.00	22.10	143.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

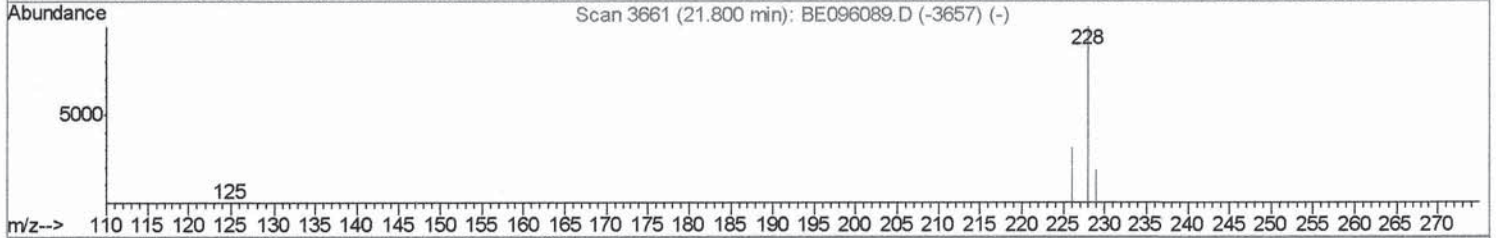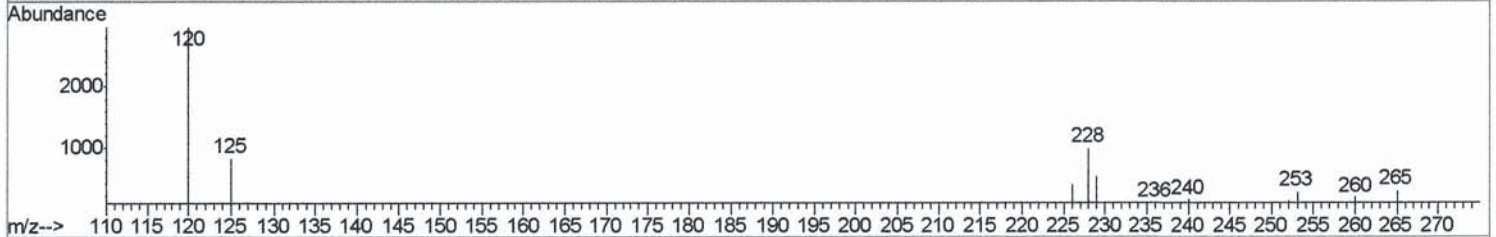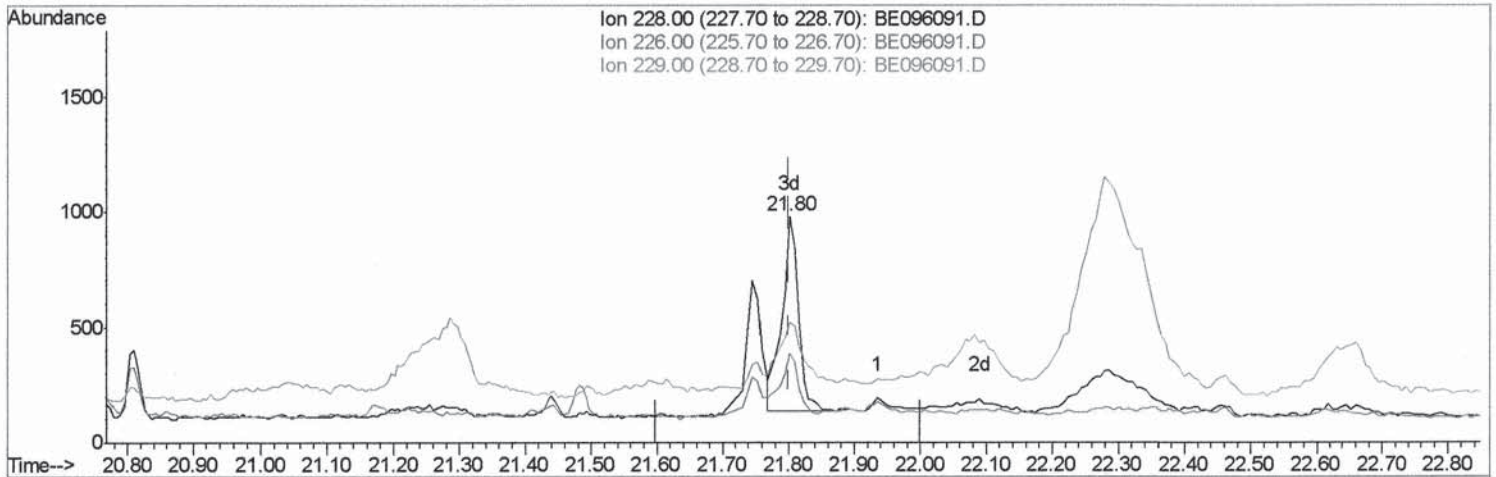

(19) Chrysene

21.801min (+0.001) 0.07ng/ul m > SJ 4/24/18

response 1470

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	39.76#
229.00	22.10	53.41#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

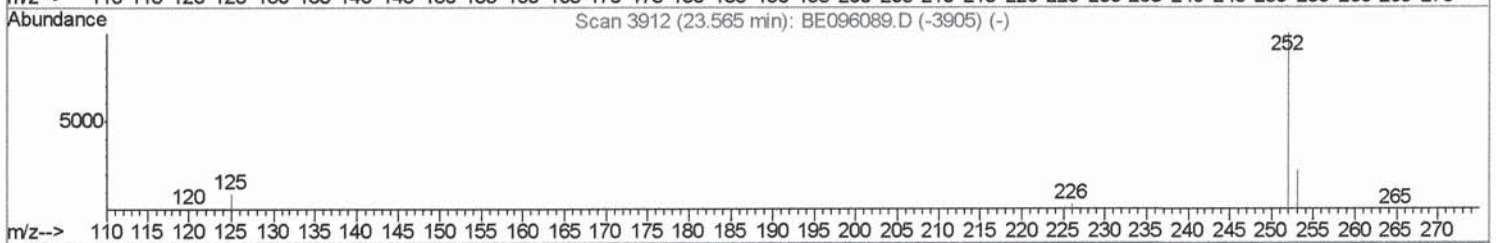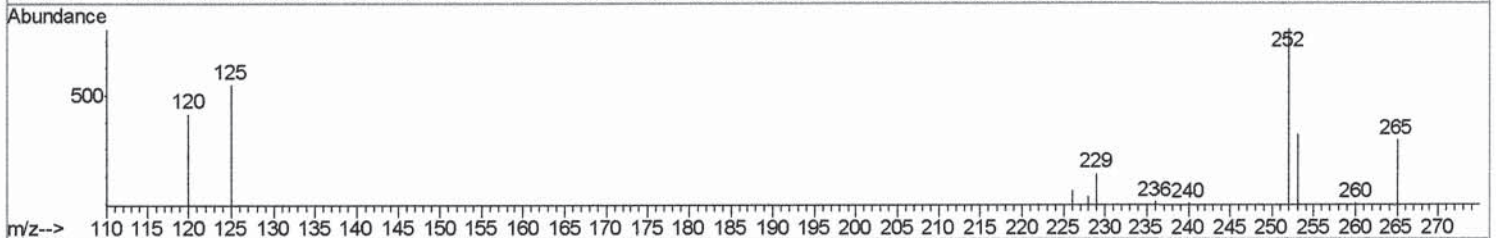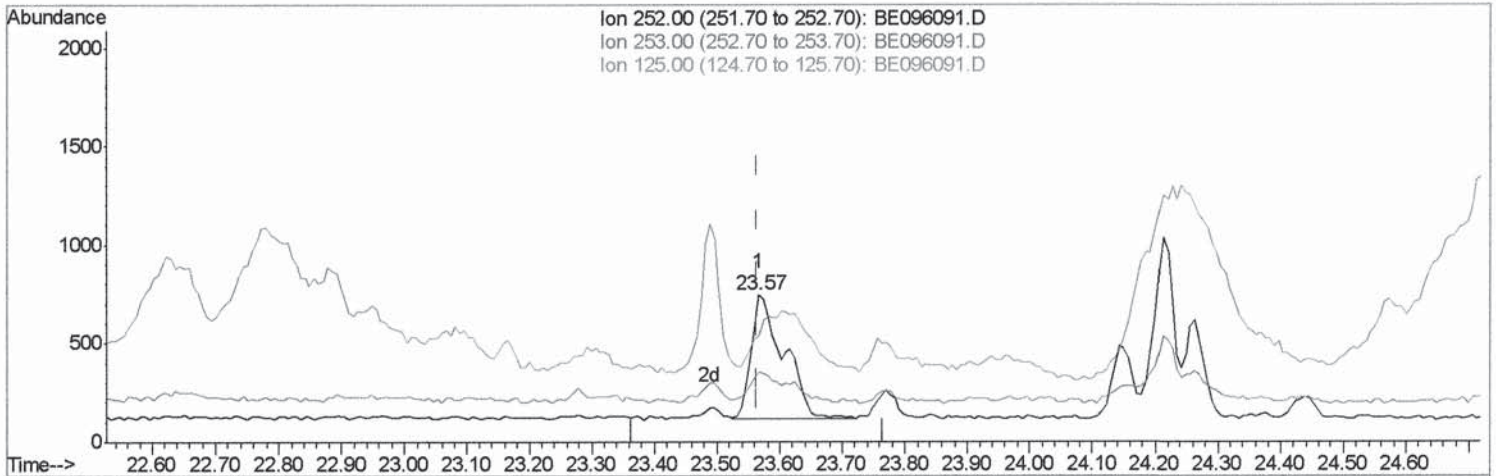

TIC: BE096091.D

(21) Benzo(b)fluoranthene
 23.566min (+0.001) 0.09ng/ul
 response 2250

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	47.52
125.00	17.50	72.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096091.D
Acq On : 23 Apr 2018 18:48
Operator : SJ/JU
Sample : J2355-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y24

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:13:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

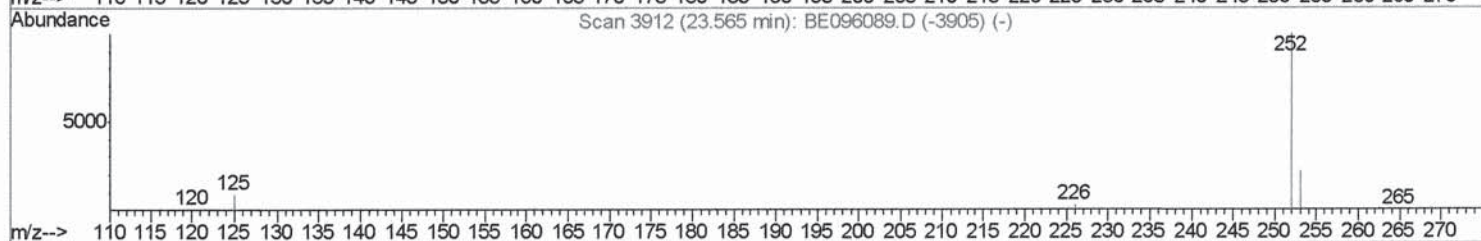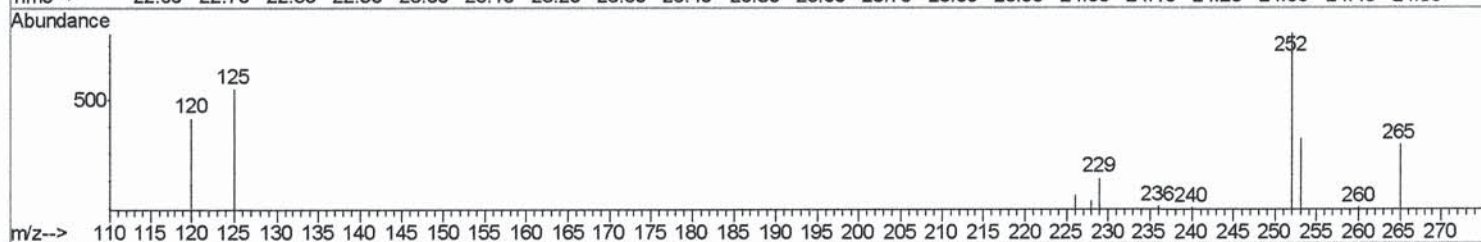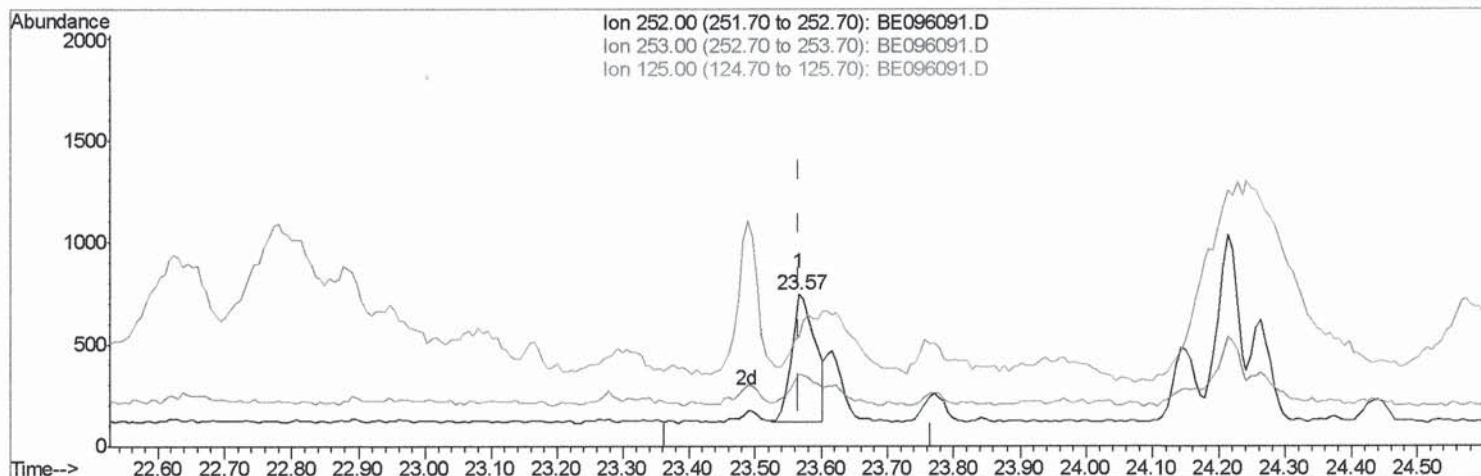

TIC: BE096091.D

(21) Benzo(b)fluoranthene

23.566min (+0.001) 0.06ng/ul m > SJ 4/24/18

response 1583

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	47.52
125.00	17.50	72.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:14:31 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

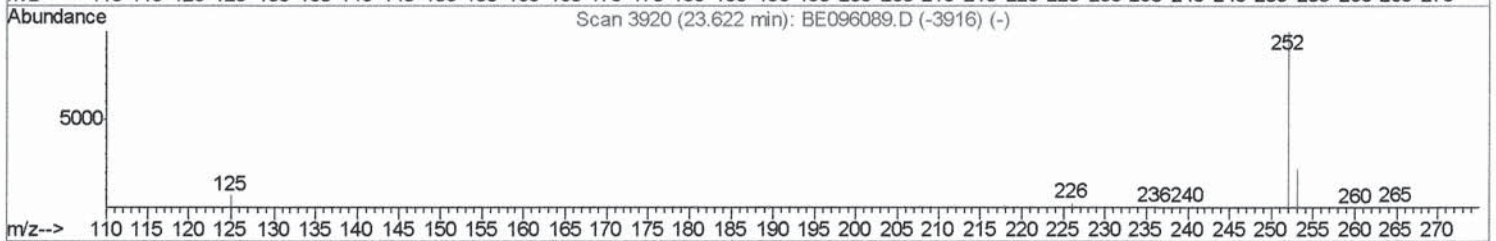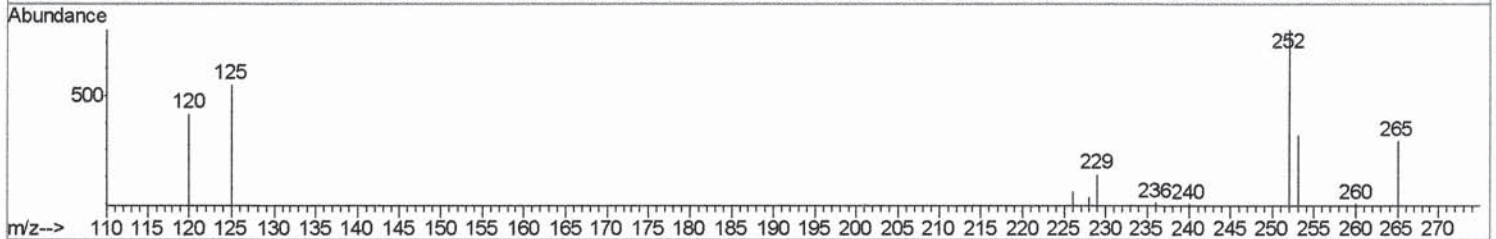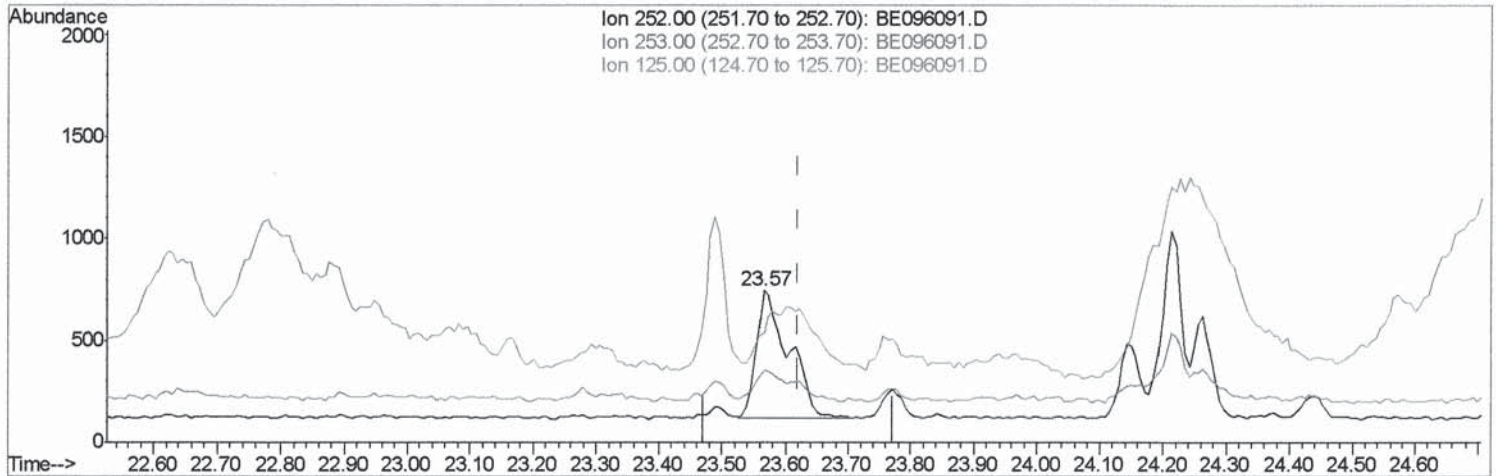

TIC: BE096091.D

(22) Benzo(k)fluoranthene
 23.566min (-0.056) 0.09ng/ul
 response 2212

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	47.52#
125.00	17.10	72.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:14:31 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

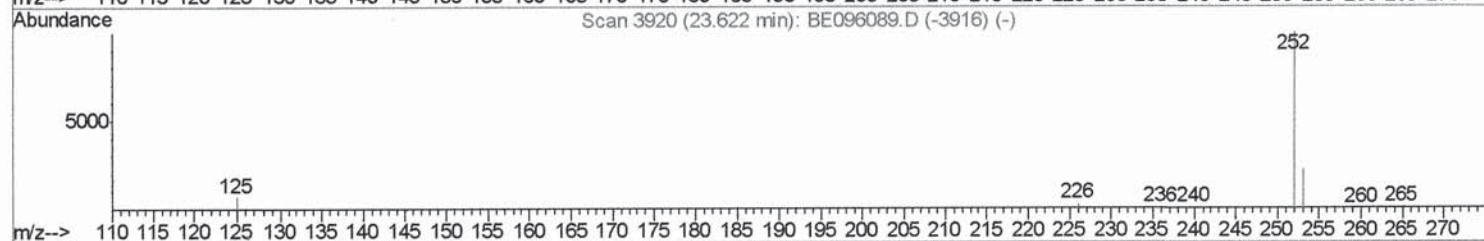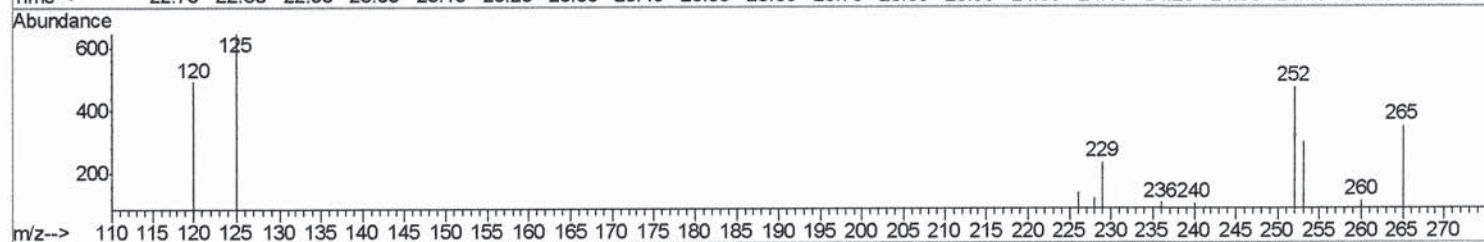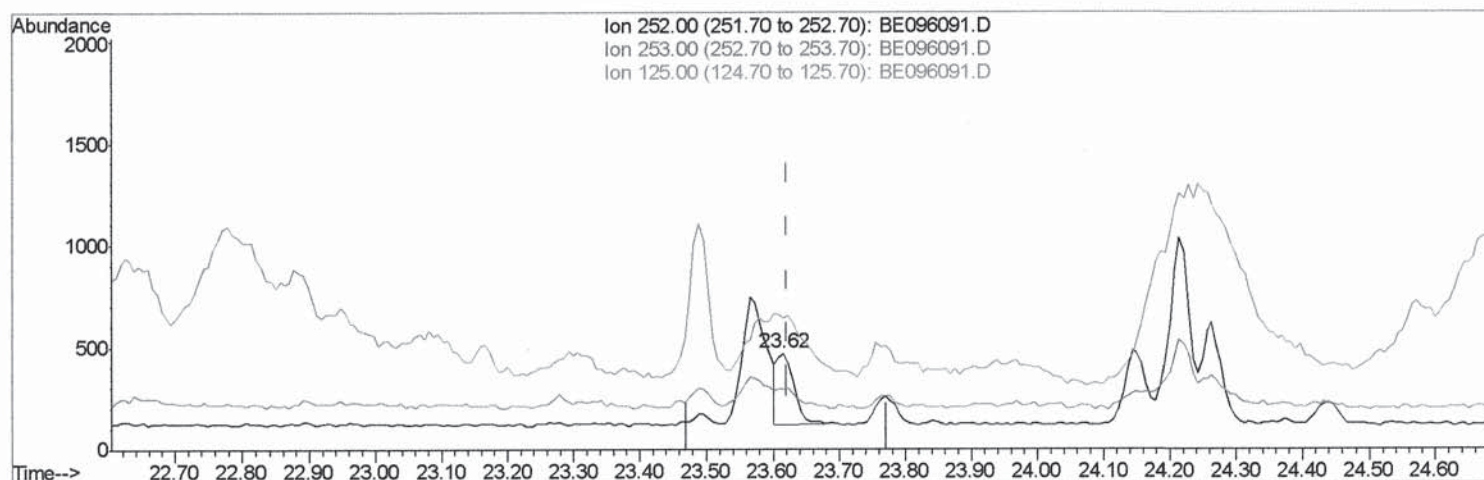

TIC: BE096091.D

(22) Benzo(k)fluoranthene

23.615min (-0.006) 0.03ng/ul m > SJ 4/24/18

response 613

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	62.77#
125.00	17.10	137.66#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:16:08 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

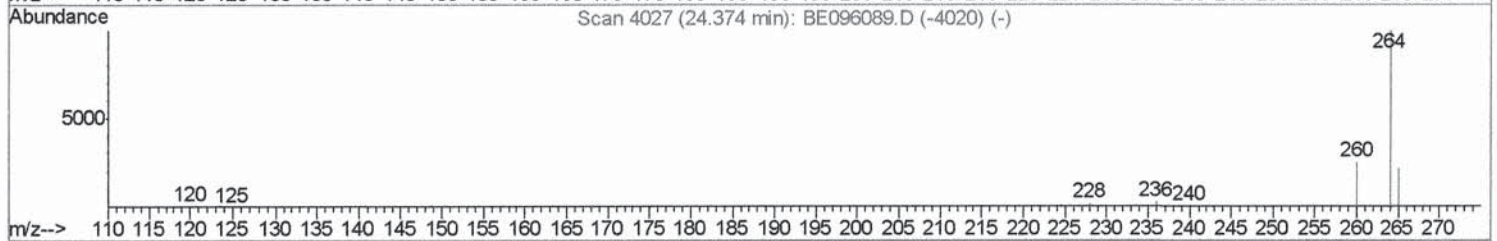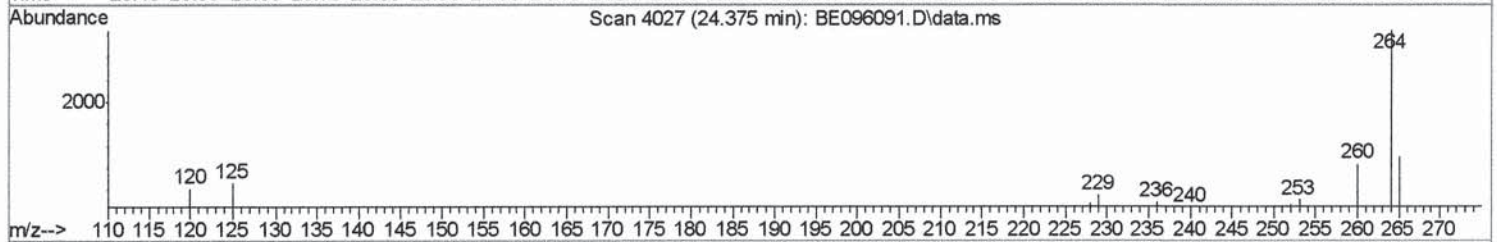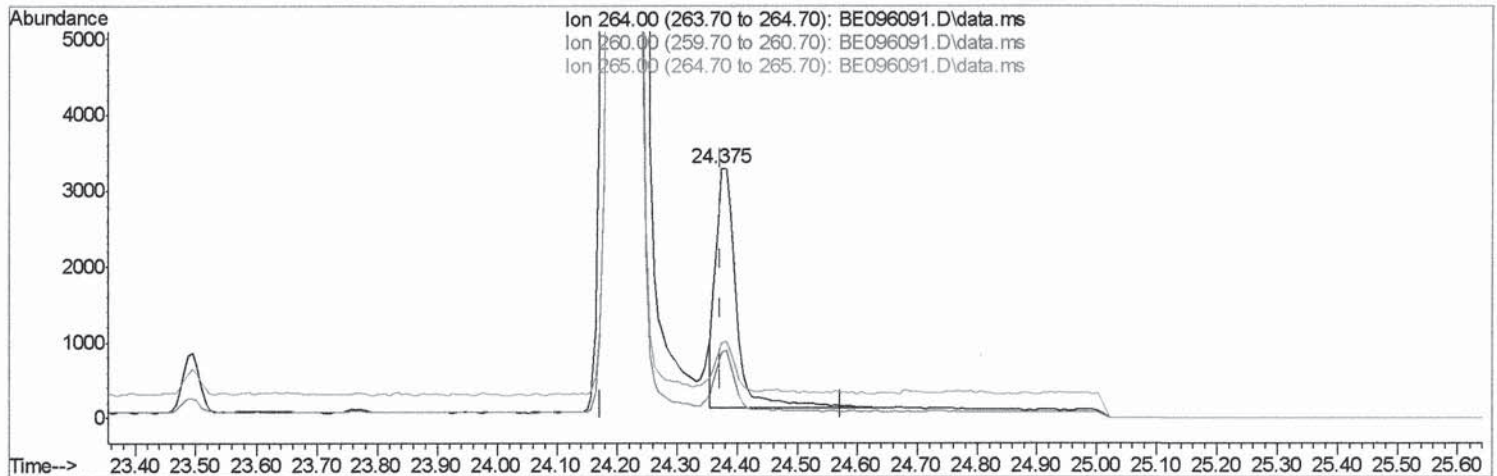

TIC: BE096091.D\data.ms

(20) Perylene-d12 (I)

24.375min (+0.001) 0.40 ng/ul

response 7547

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.37
265.00	103.50	30.10#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 07:16:08 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

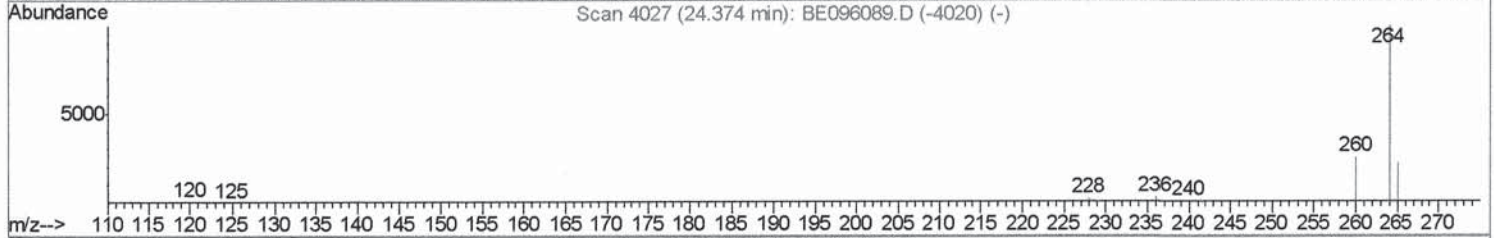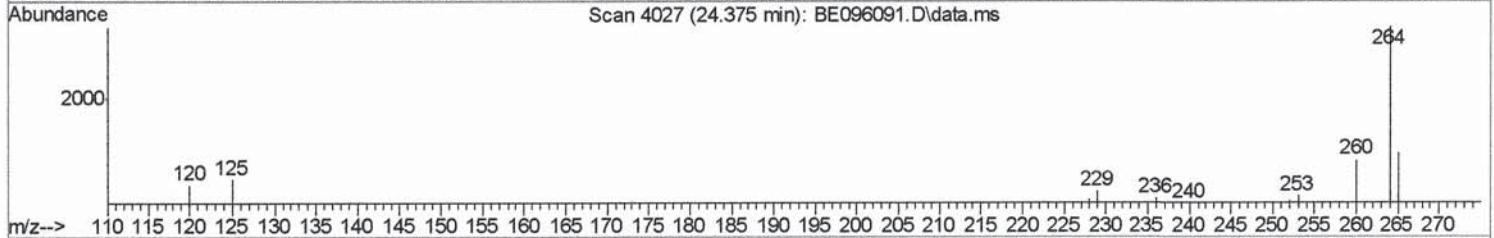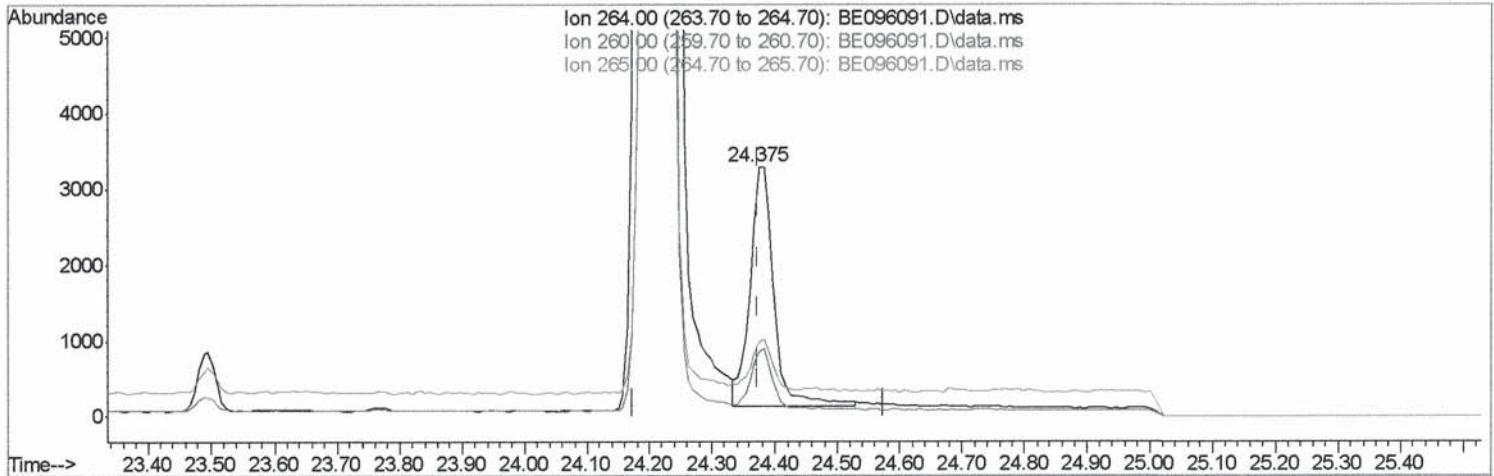

TIC: BE096091.D\data.ms

(20) Perylene-d12 (I)

24.375min (+0.001) 0.40 ng/ul m > SJ 4/24/18

response 8132

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.37
265.00	103.50	30.10#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE042318\
 Data File : BE096091.D
 Acq On : 23 Apr 2018 18:48
 Operator : SJ/JU
 Sample : J2355-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y24

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:37 PM

Quant Time: Apr 24 10:44:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.379	152	2000	0.40	ng/ul	0.00
2) Naphthalene-d8	11.203	136	5572	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.966	164	3510	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.675	188	7223m	0.40	ng/ul	0.00
16) Chrysene-d12	21.766	240	6759m	0.40	ng/ul	0.00
20) Perylene-d12	24.375	264	8132m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.757	152	3289	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.655	212	7933m	0.27	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.717	178	1073m	0.05	ng/ul	Ovalue
15) Fluoranthene	19.687	202	2834m	0.10	ng/ul	
17) Pyrene	20.040	202	2976	0.13	ng/ul#	86
18) Benzo(a)anthracene	21.745	228	1214m	0.04	ng/ul	SJ 4/24/18
19) Chrysene	21.801	228	1470m	0.07	ng/ul	
21) Benzo(b)fluoranthene	23.566	252	1583m	0.06	ng/ul	
22) Benzo(k)fluoranthene	23.615	252	613m	0.02	ng/ul	
26) Benzo(a,h,i)perylene	28.039	276	745	0.03	ng/ul#	57

(#) = qualifier out of range (m) = manual integration (+) = signals summed