


Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:30:50 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

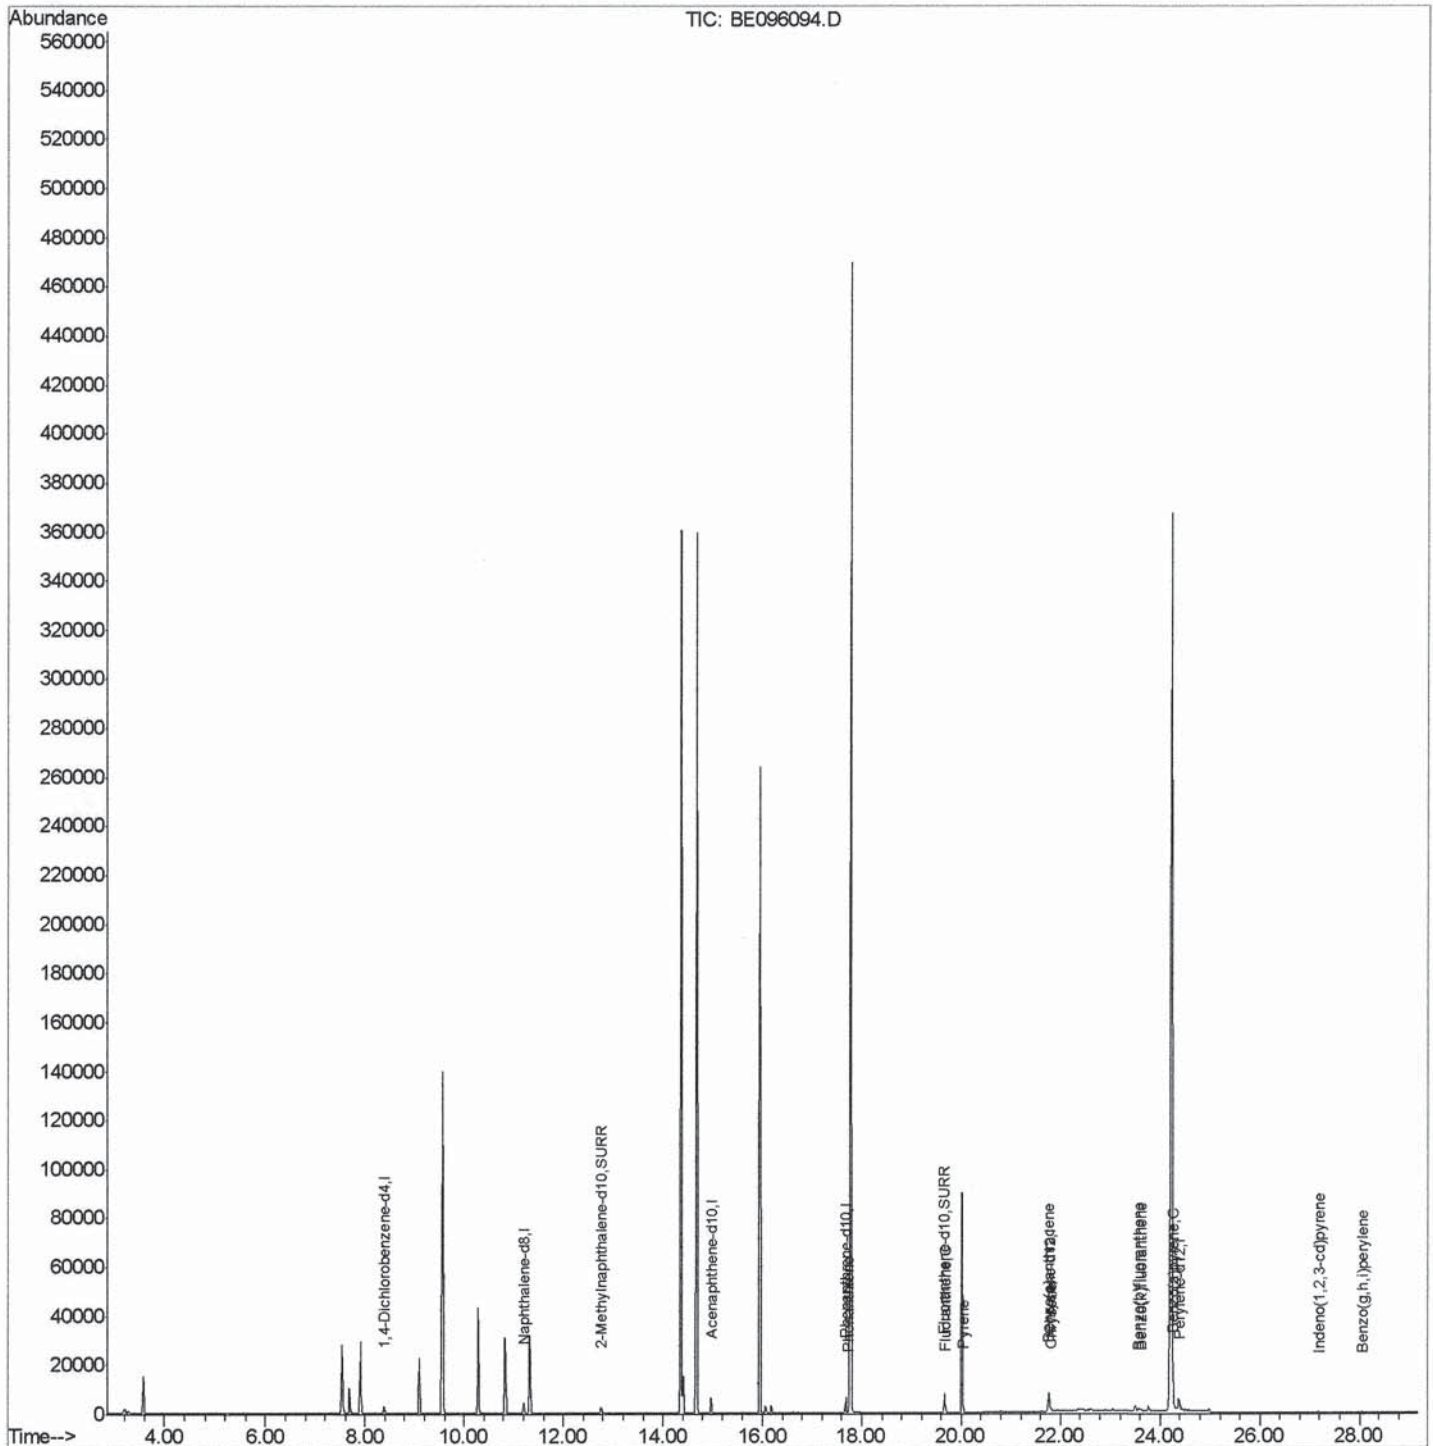

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:00:59 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

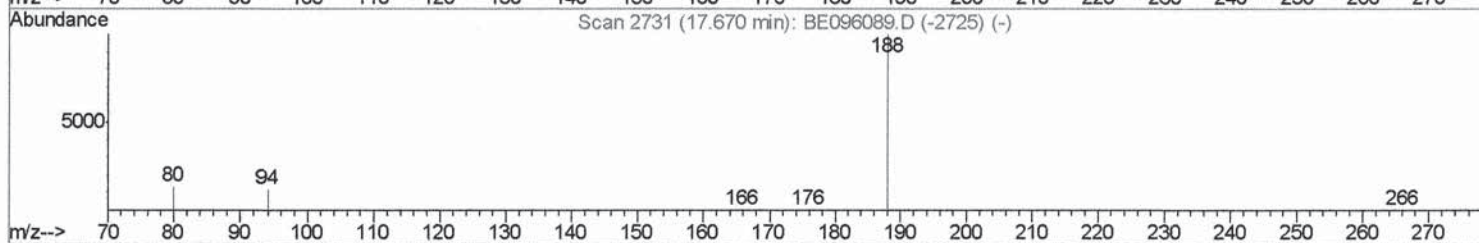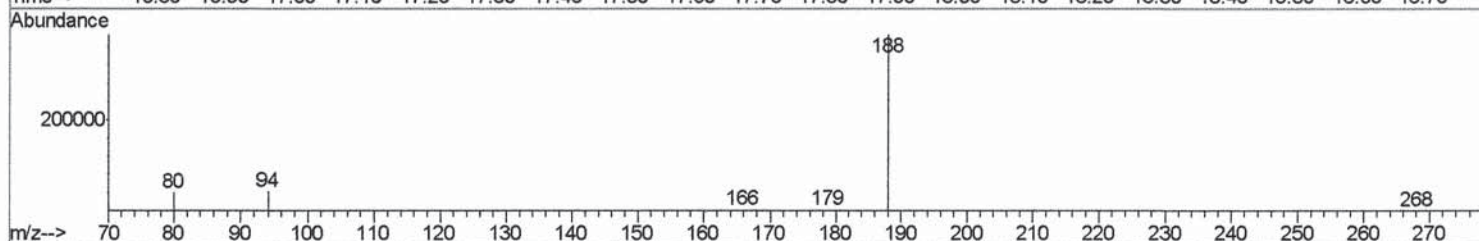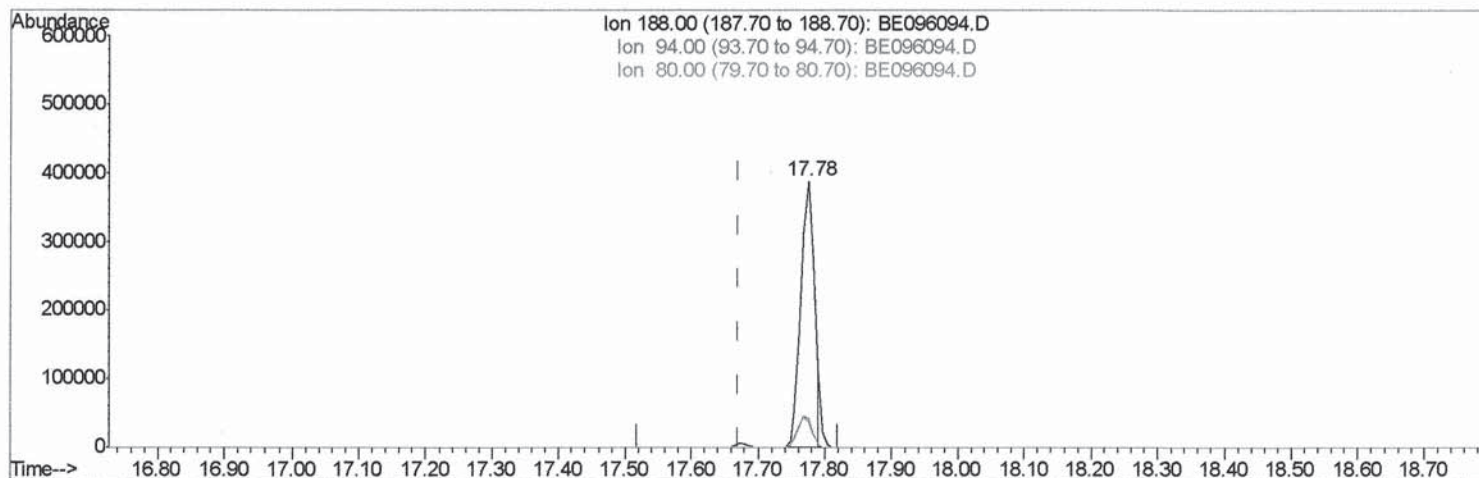

TIC: BE096094.D

(10) Phenanthrene-d10 (I)

17.775min (+0.105) 0.40ng/ul

response 552420

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.70
80.00	11.80	10.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:00:59 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

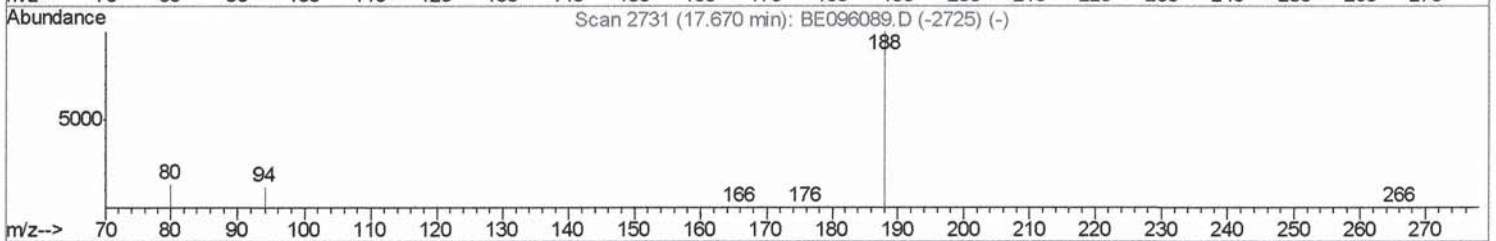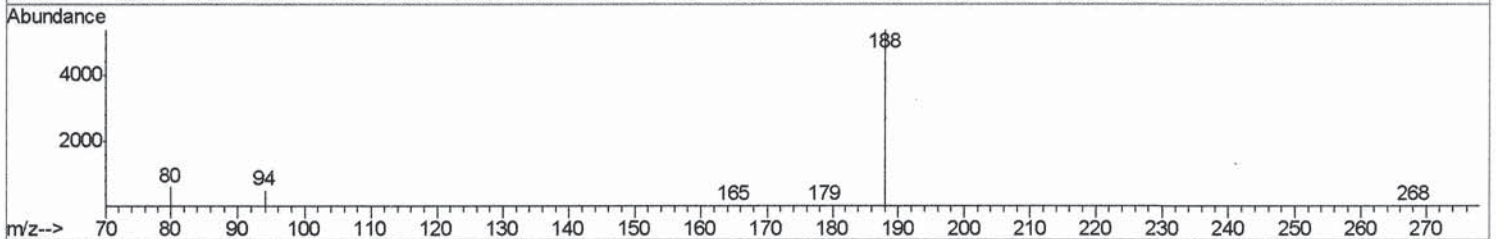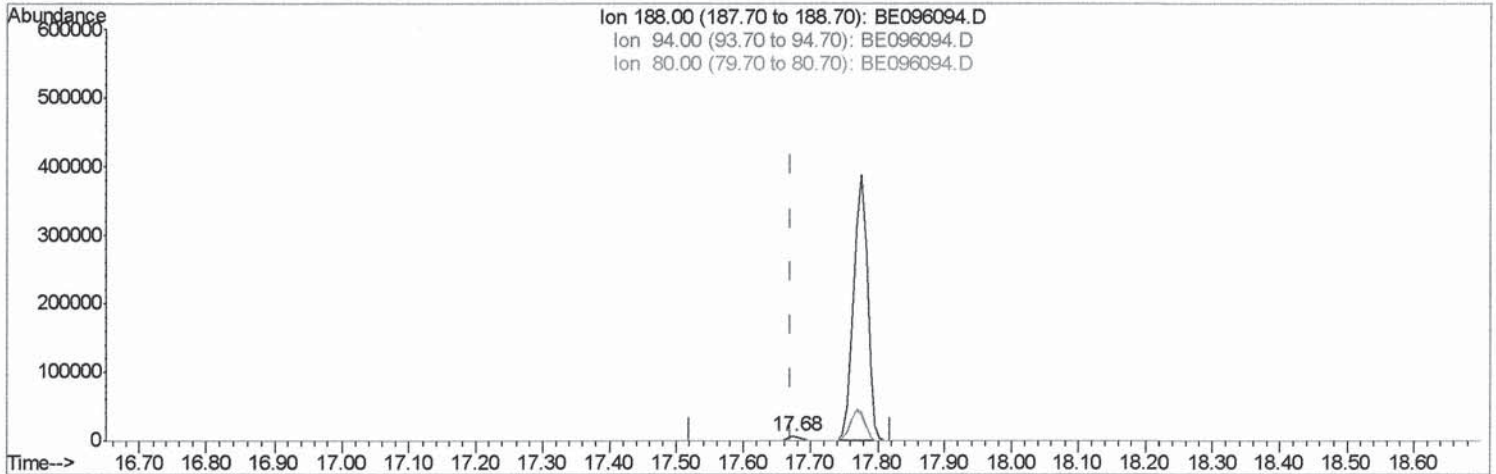

TIC: BE096094.D

(10) Phenanthrene-d10 (I)

17.677min (+0.006) 0.40ng/ul m> SJ 4/24/18

response 7513

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.96
80.00	11.80	11.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

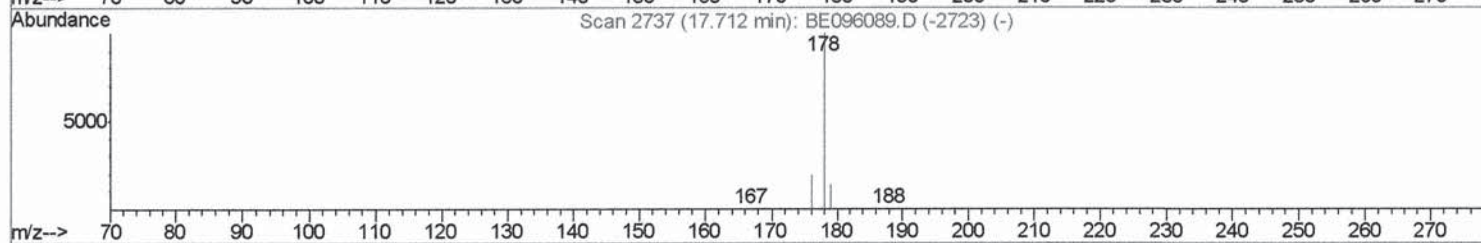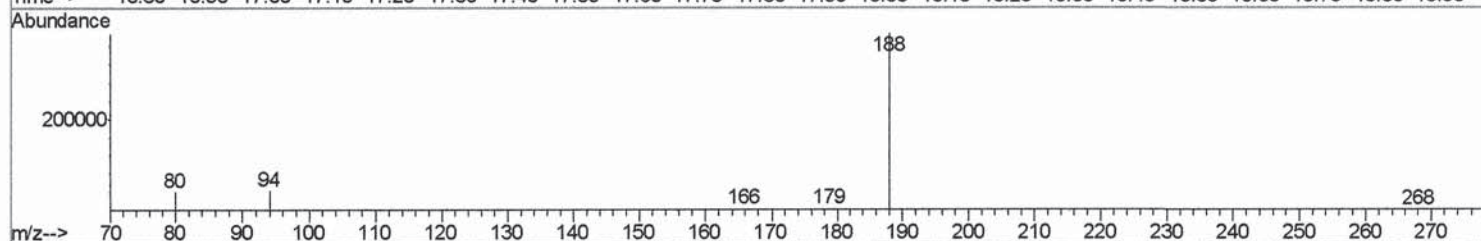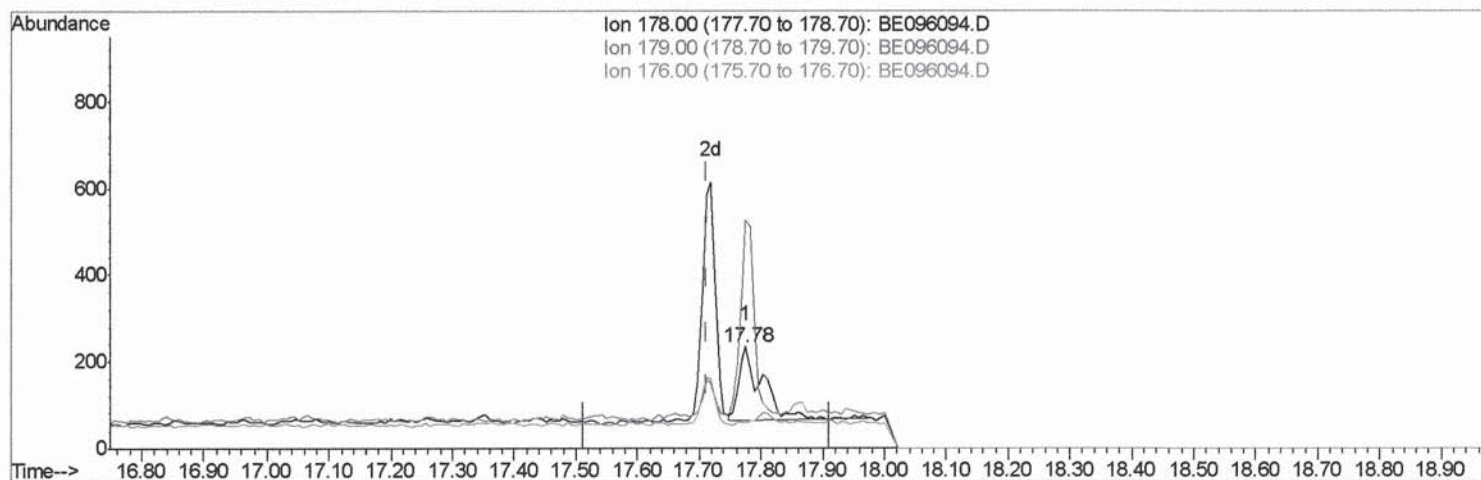

TIC: BE096094.D

(12) Phenanthrene

17.775min (+0.063) 0.02ng/ul

response 443

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	226.61#
176.00	17.00	25.32#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

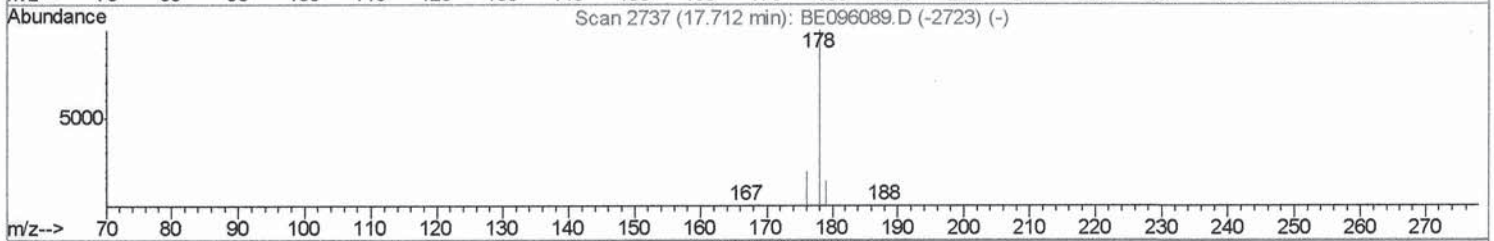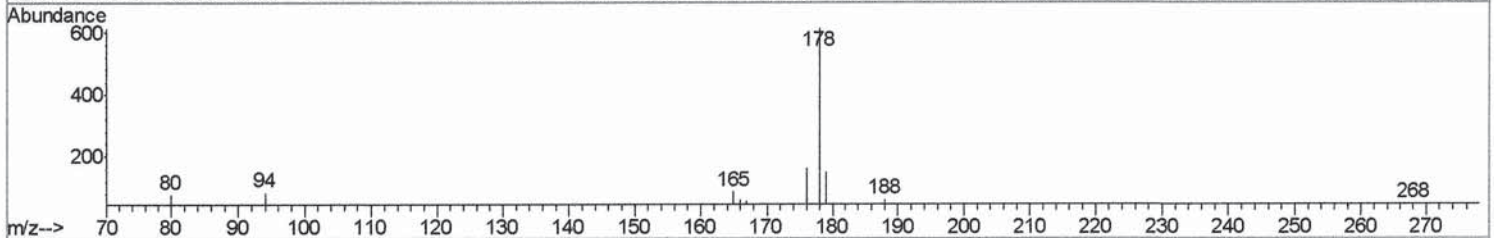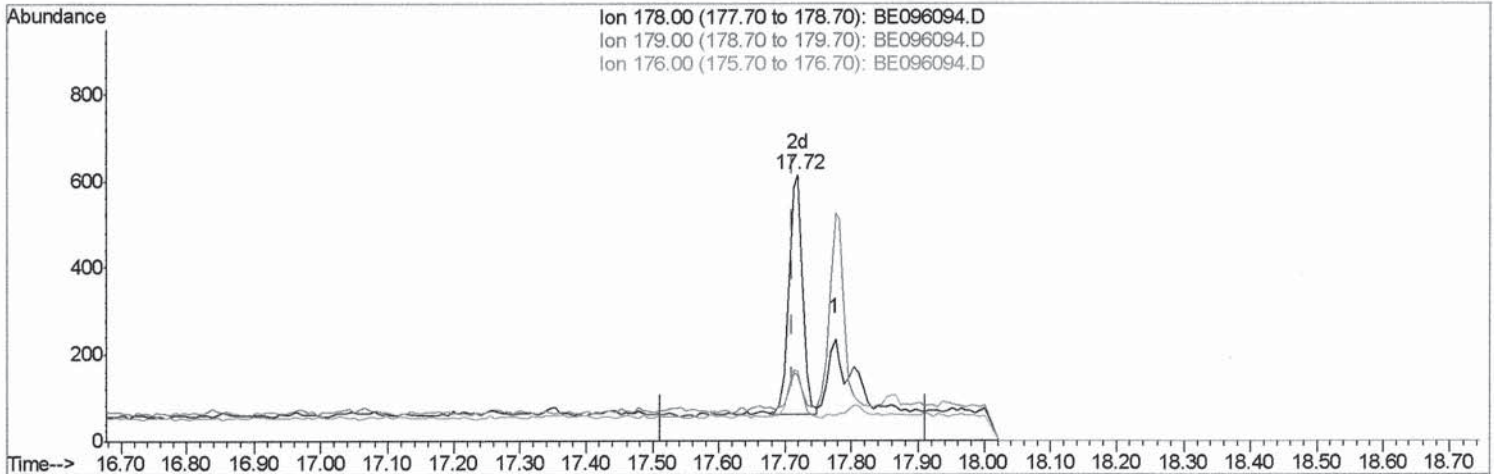

TIC: BE096094.D

(12) Phenanthrene

17.719min (+0.006) 0.04ng/ul m> SJ 4/24/18

response 816

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.63
176.00	17.00	26.43#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

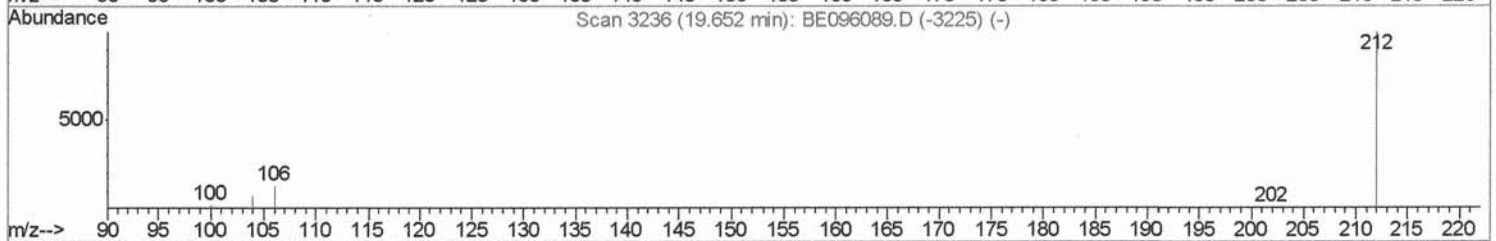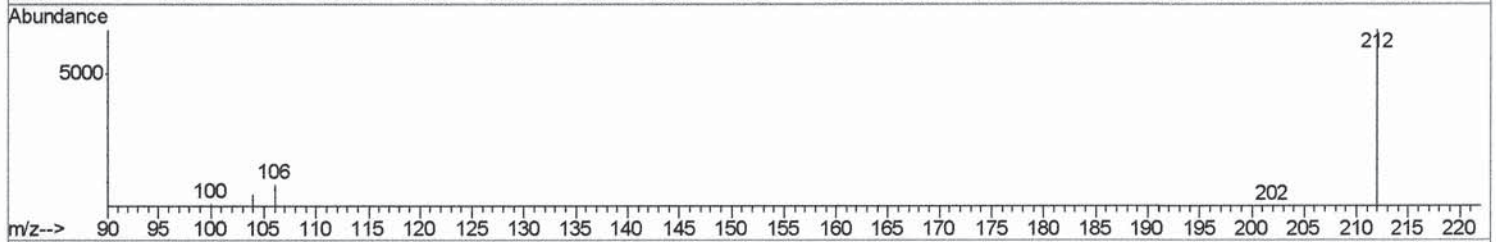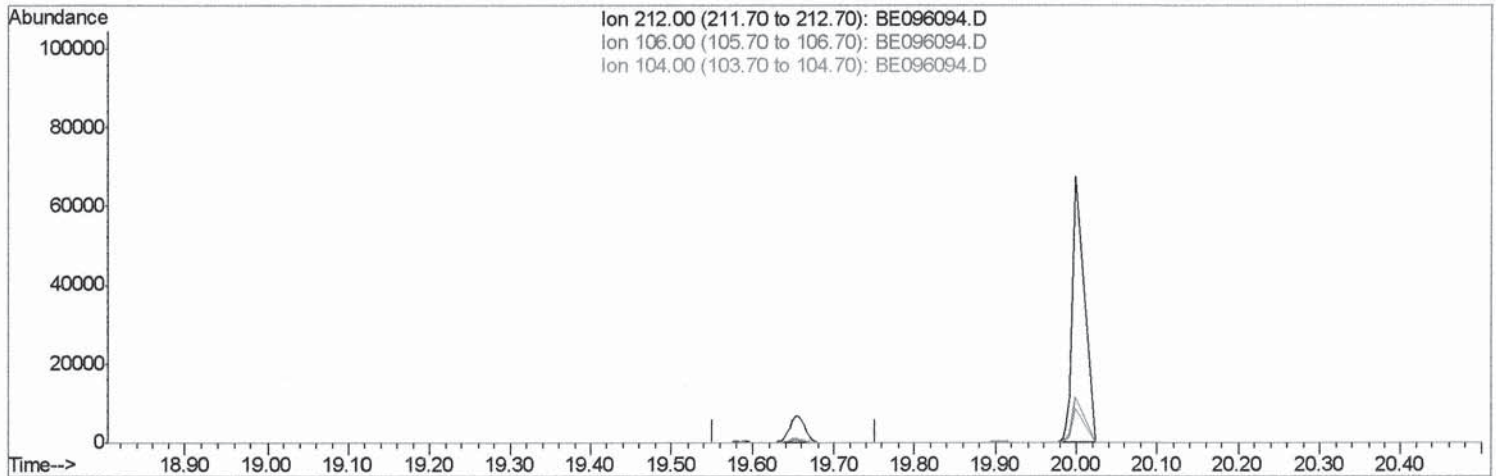

TIC: BE096094.D

(14) Fluoranthene-d10 (Surr)

19.652min (-19.652) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

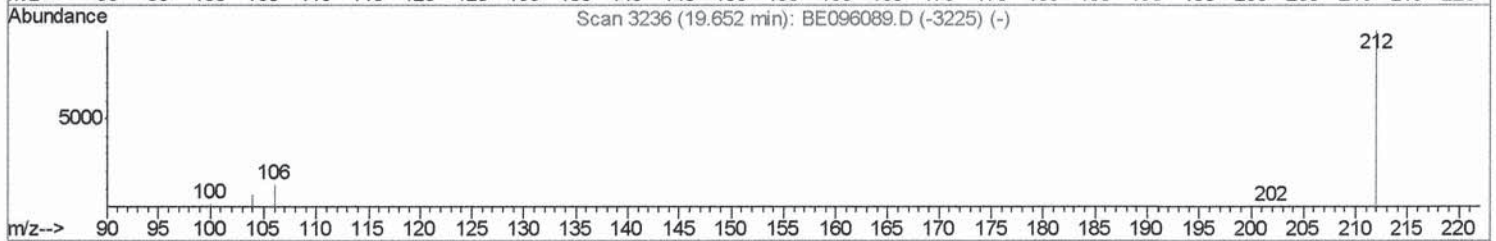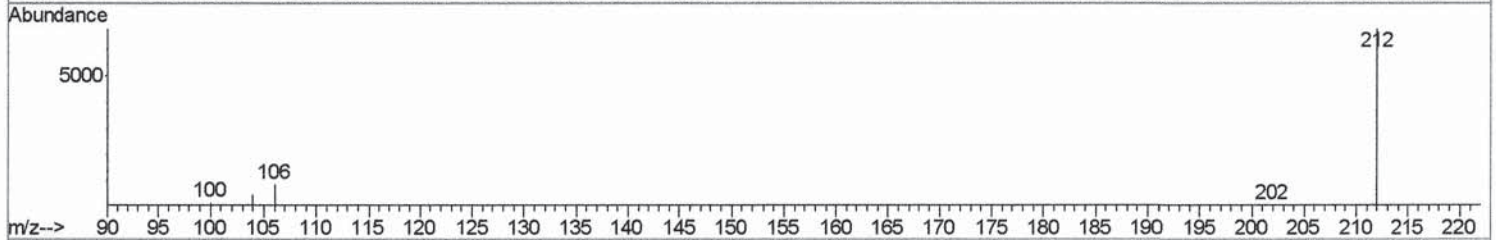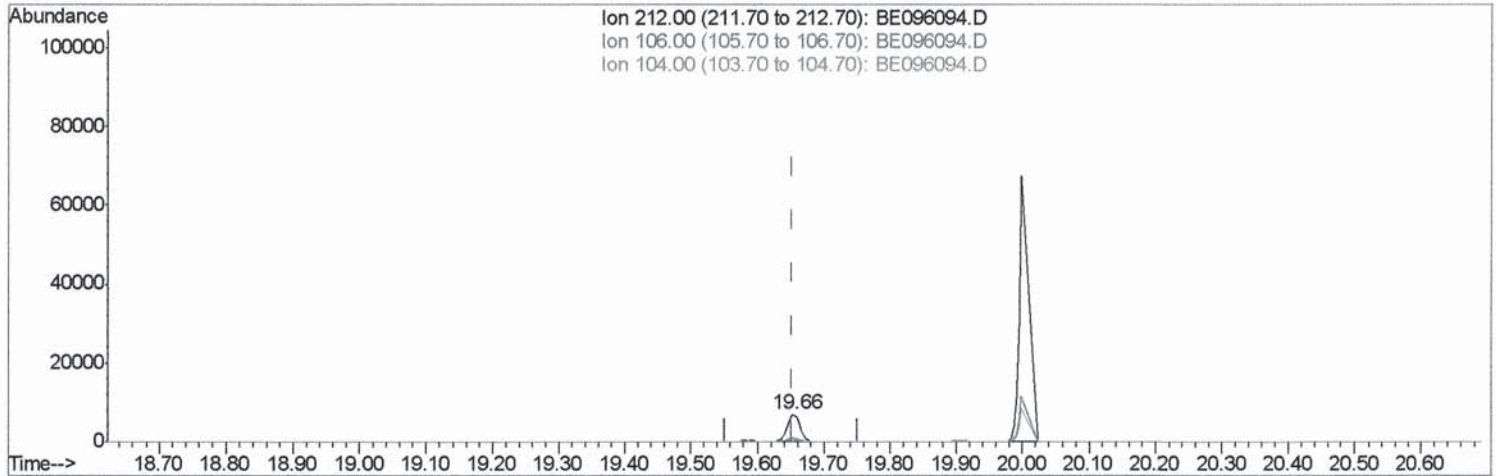

TIC: BE096094.D

(14) Fluoranthene-d10 (SURR)

19.655min (+0.003) 0.29ng/ul m) SJ 4/24/18

response 8948

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

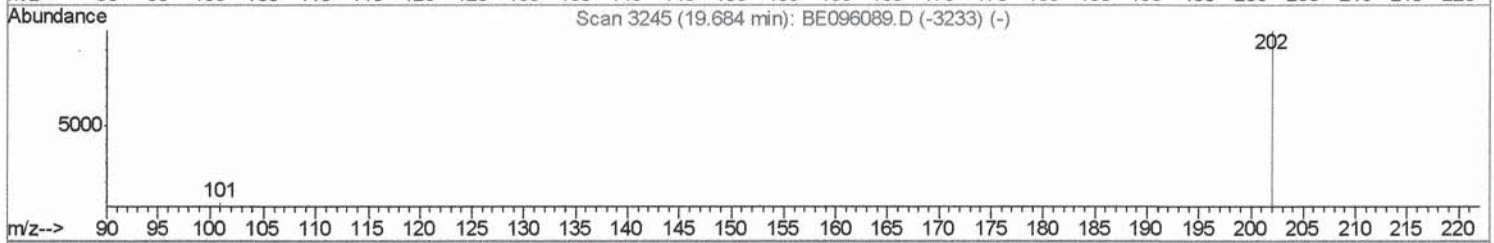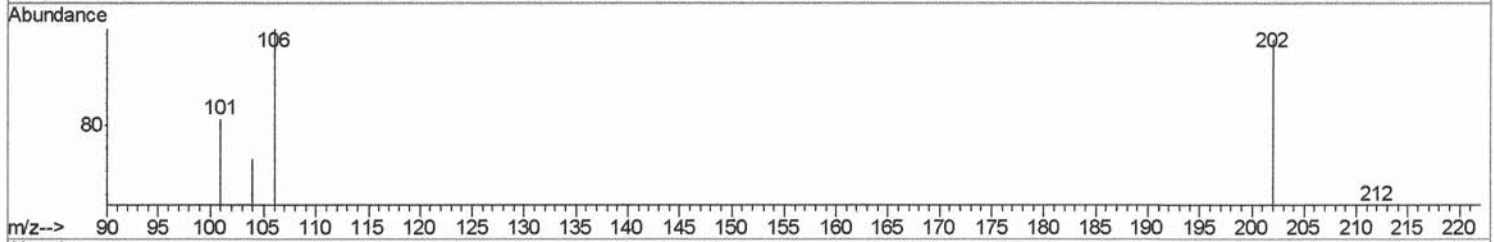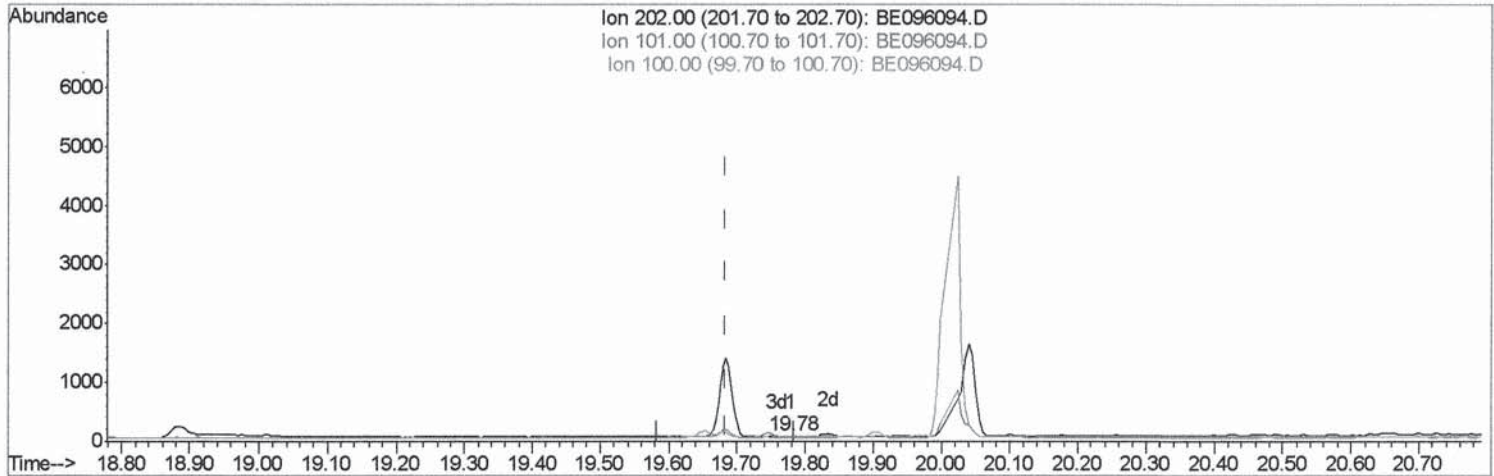

TIC: BE096094.D

(15) Fluoranthene (C)

19.780min (+0.096) 0.00ng/ul

response 6

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	85.26#
100.00	19.50	69.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

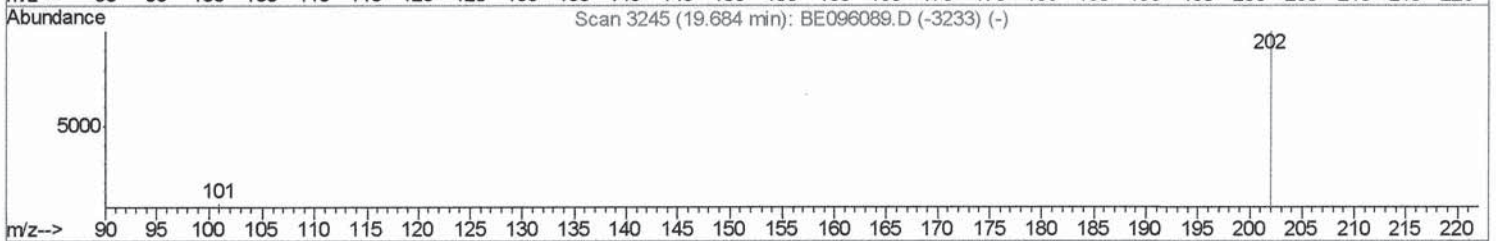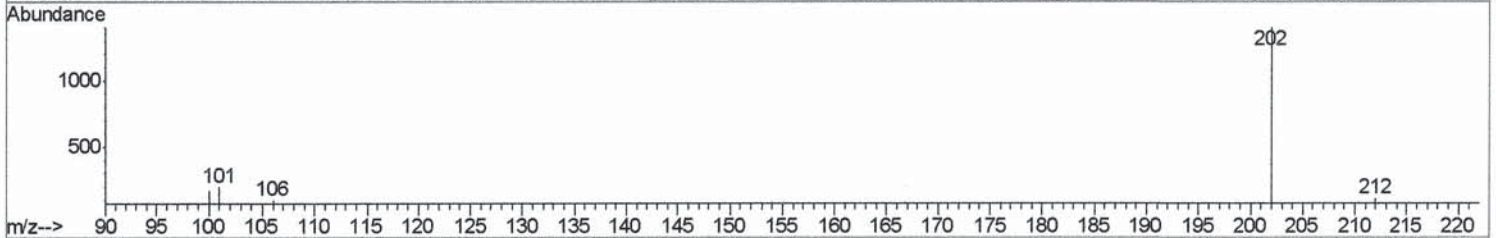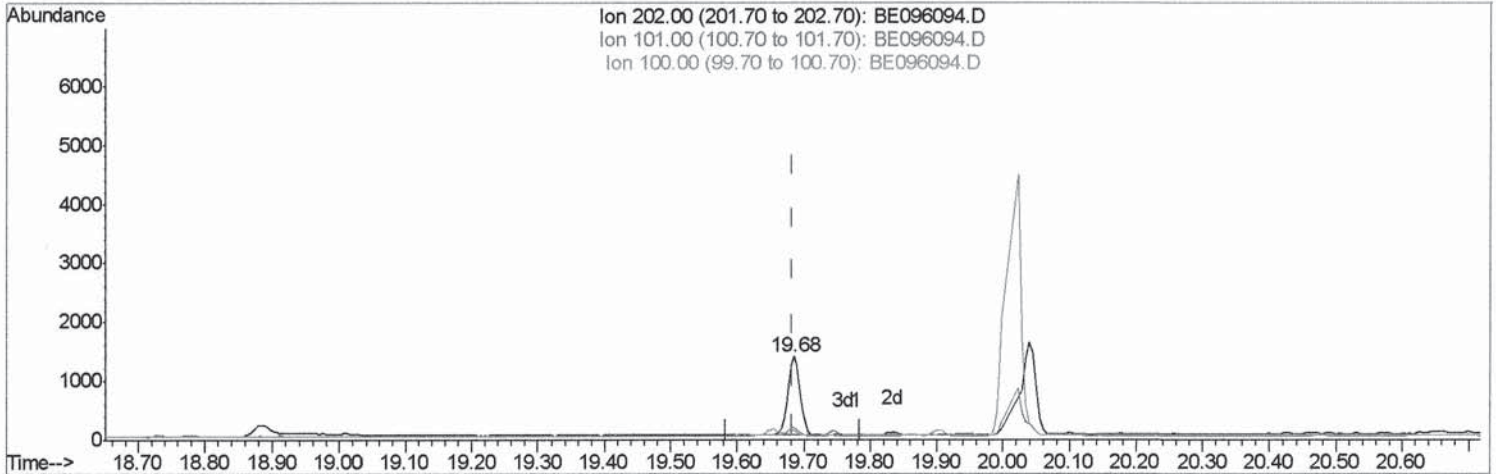

TIC: BE096094.D

(15) Fluoranthene (C)

19.684min (-0.000) 0.06ng/ul m> SJ 4/24/18

response 1697

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	14.25
100.00	19.50	12.18
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

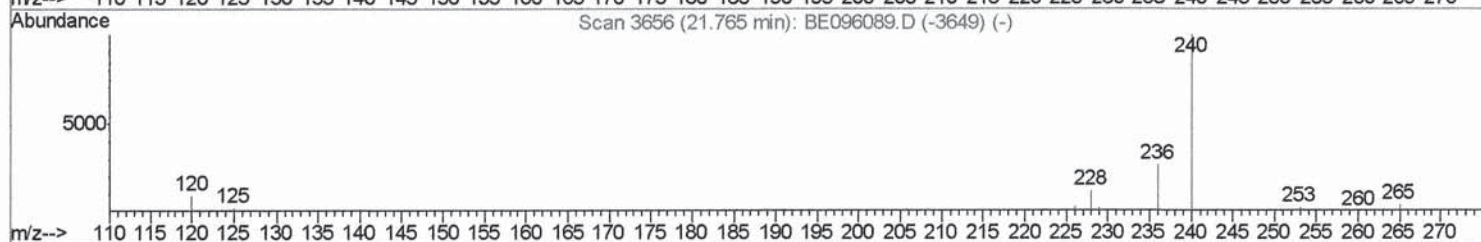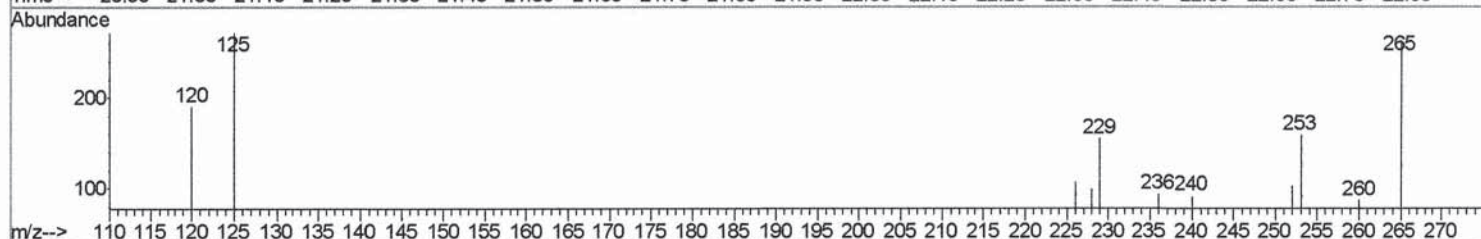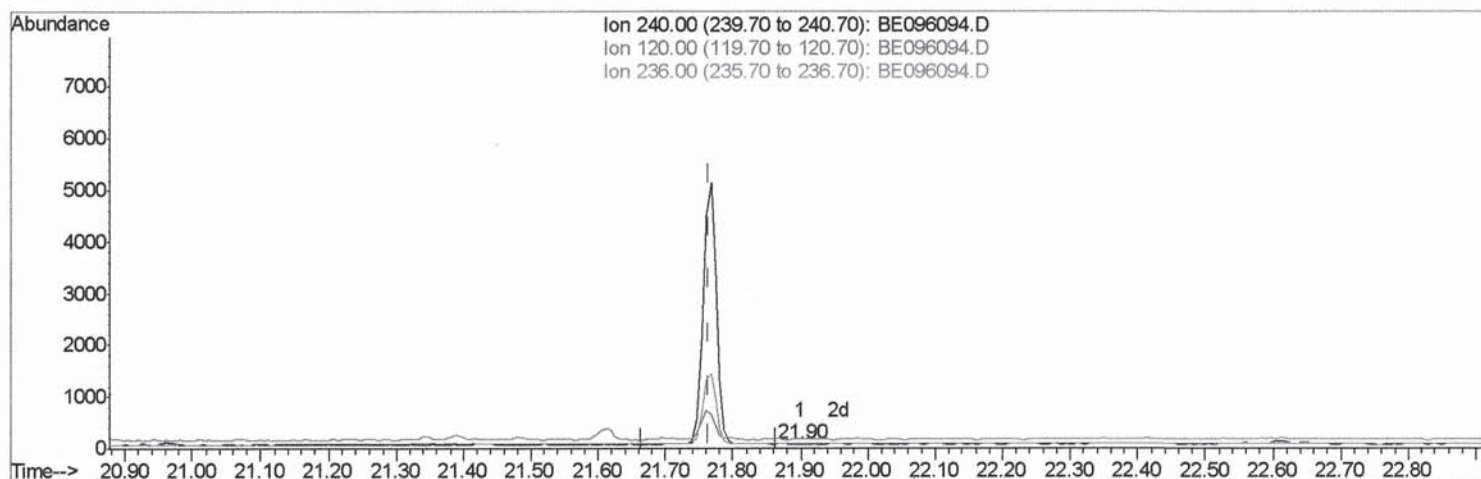

TIC: BE096094.D

(16) Chrysene-d12 (I)

21.900min (+0.135) 0.40ng/ul

response 11

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	208.79#
236.00	34.90	102.20#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:25:37 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

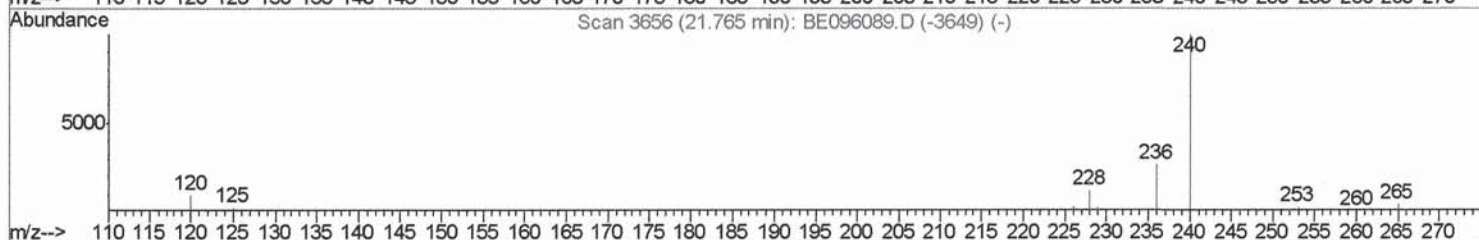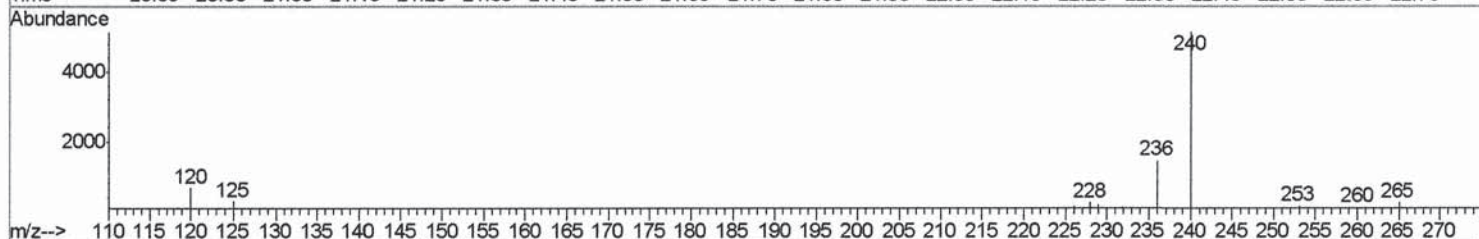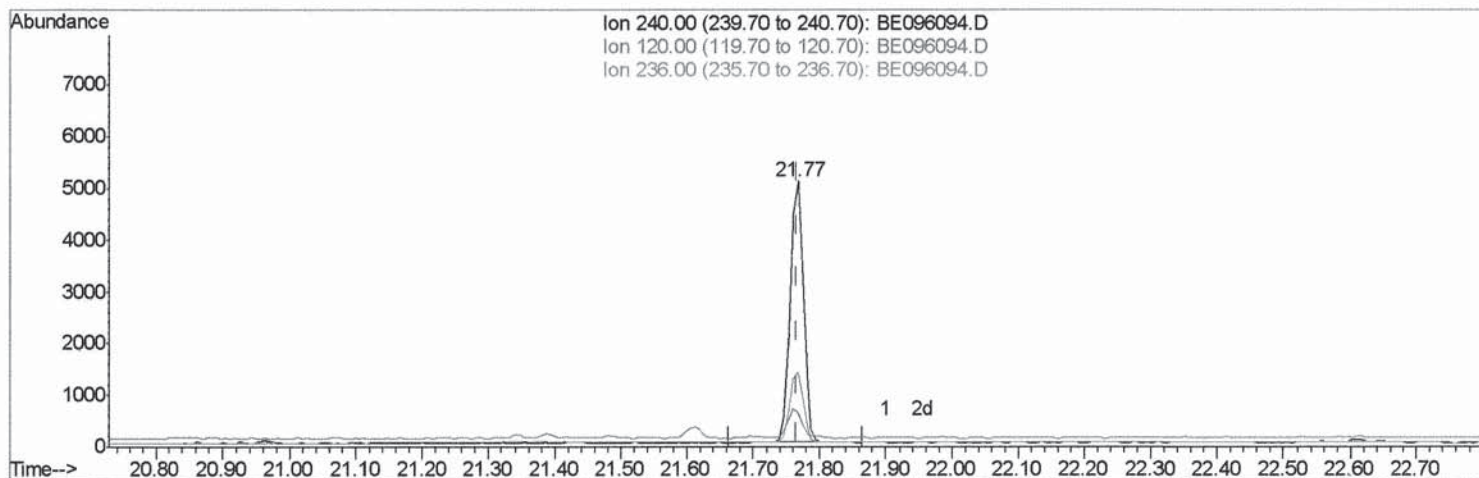

TIC: BE096094.D

(16) Chrysene-d12 (l)

21.766min (+0.001) 0.40ng/ul m > SJ 4/22/18

response 7086

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.82#
236.00	34.90	28.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

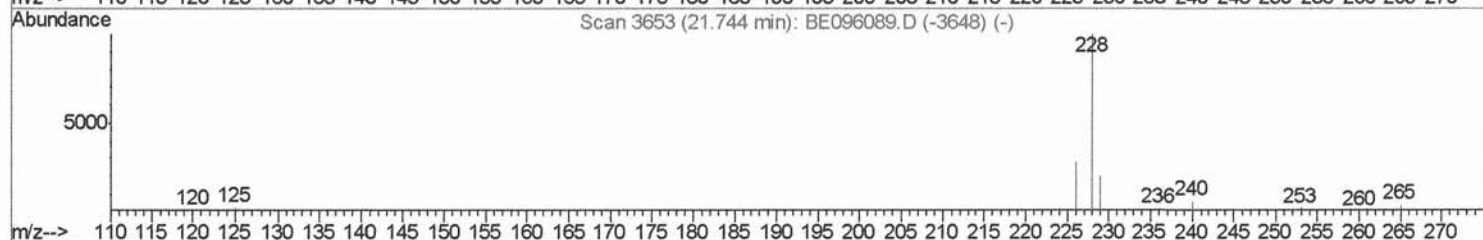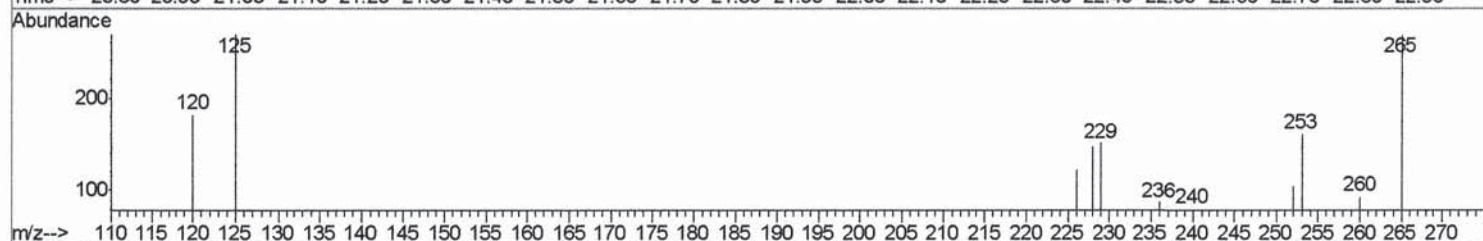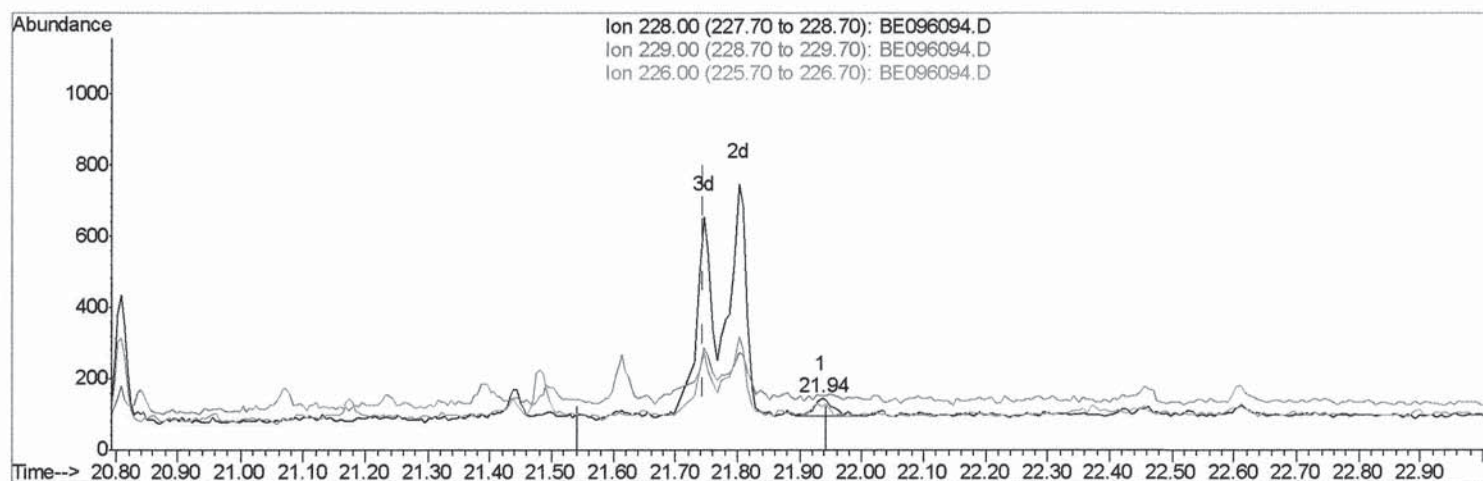

TIC: BE096094.D

(18) Benzo(a)anthracene

21.935min (+0.191) 0.00ng/ul

response 113

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	102.72#
226.00	21.30	83.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

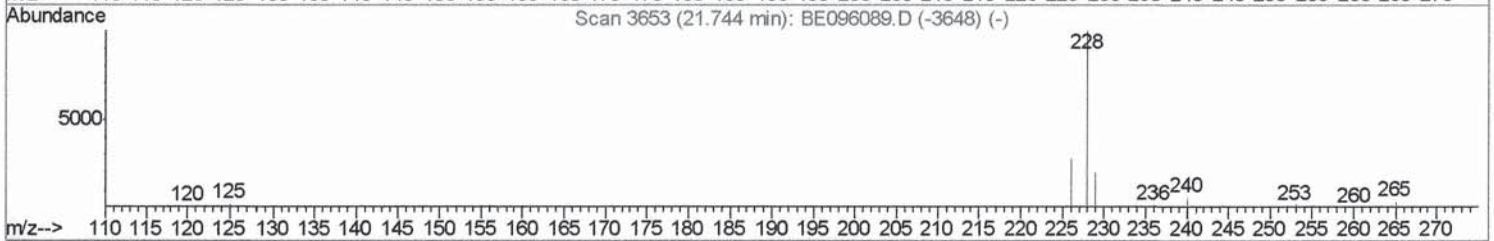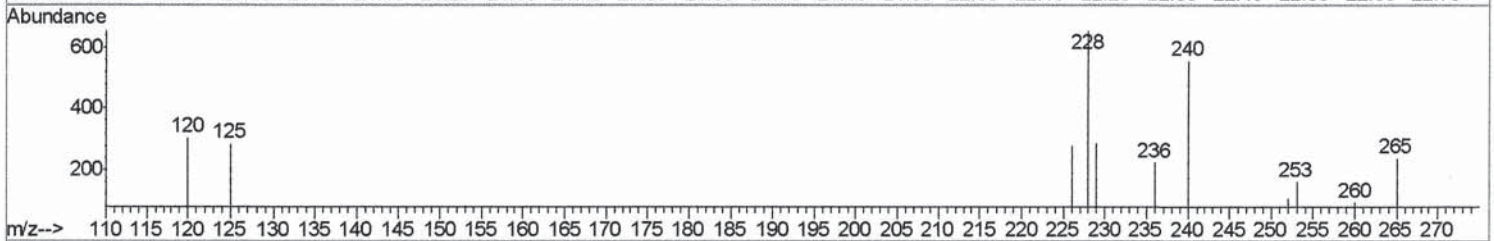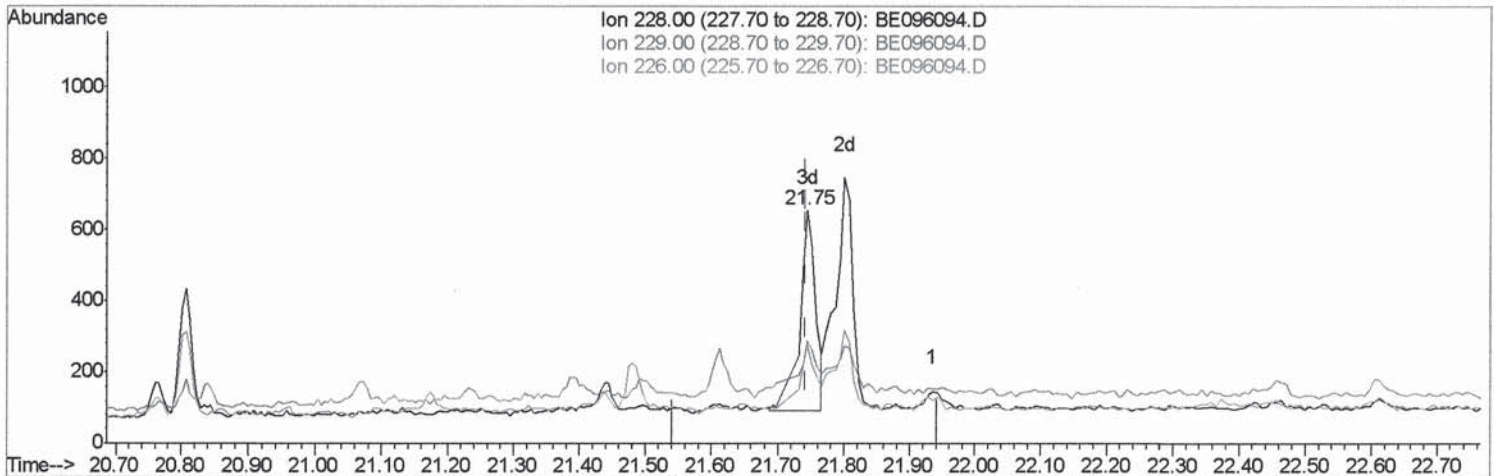

TIC: BE096094.D

(18) Benzo(a)anthracene

21.745min (+0.001) 0.04ng/ul m> SJ 4/24/18

response 1190

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	44.04#
226.00	21.30	42.35#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

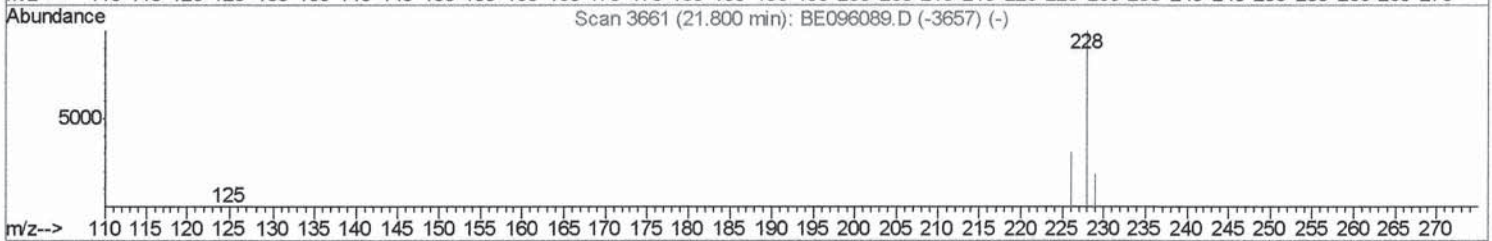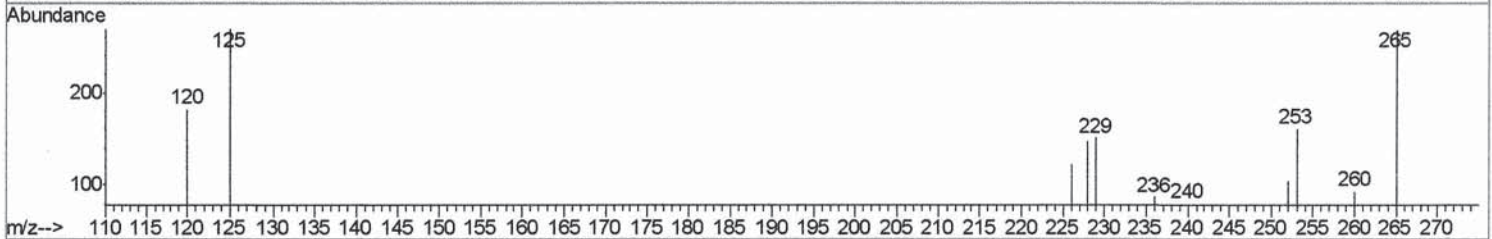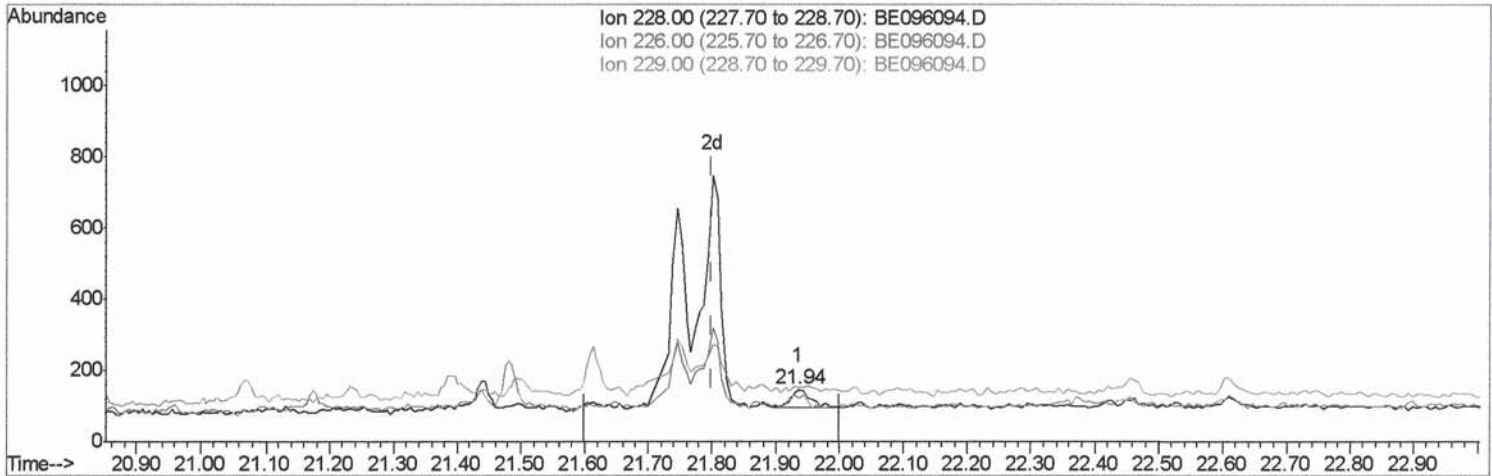

TIC: BE096094.D

(19) Chrysene

21.935min (+0.135) 0.01ng/ul

response 117

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	83.67#
229.00	22.10	102.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

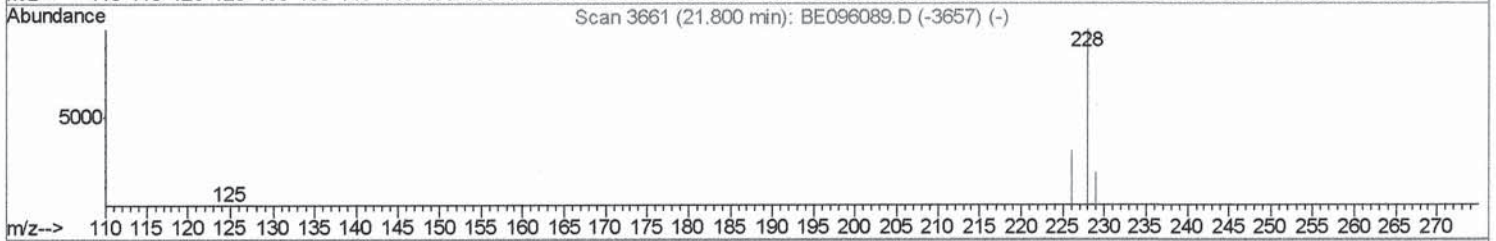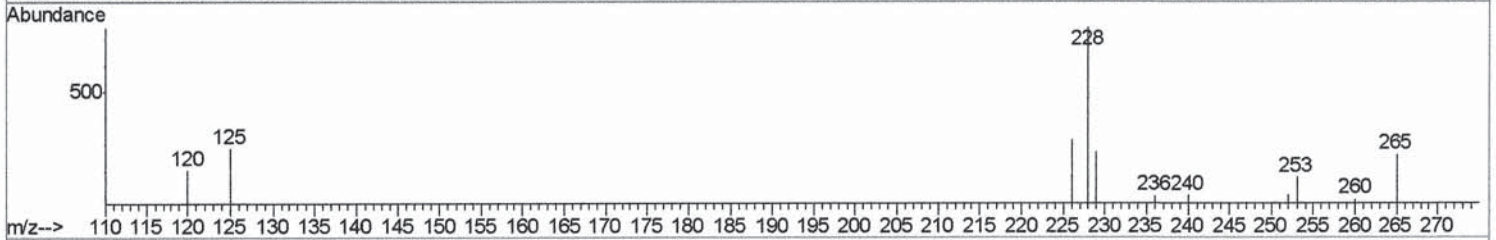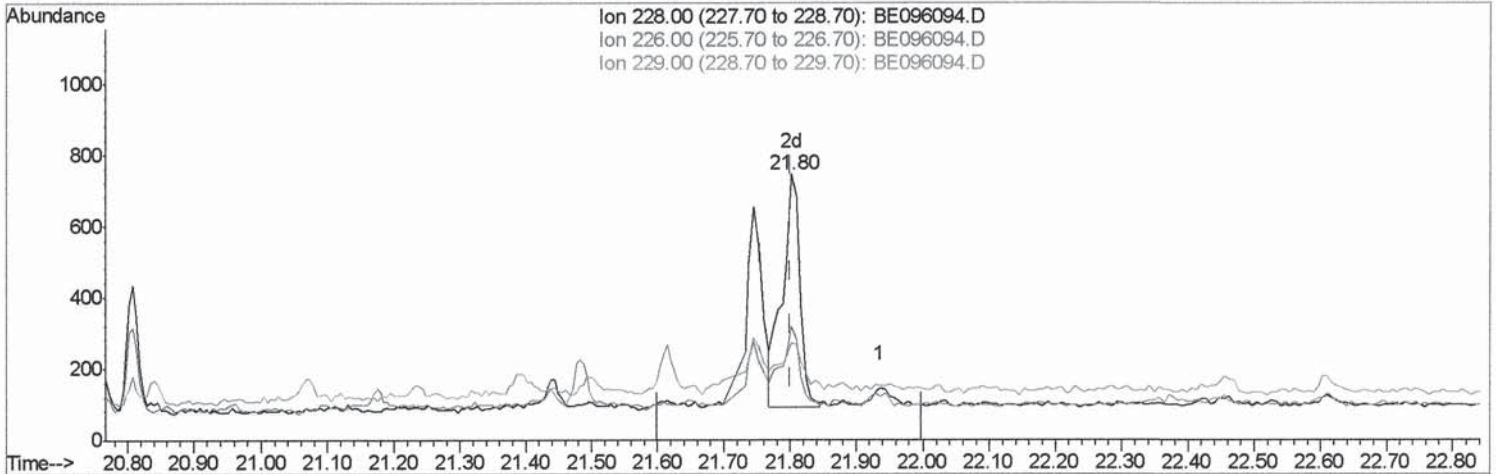

TIC: BE096094.D

(19) Chrysene

21.802min (+0.001) 0.06ng/ul m > 52 4/24/18

response 1217

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	42.82#
229.00	22.10	36.64#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

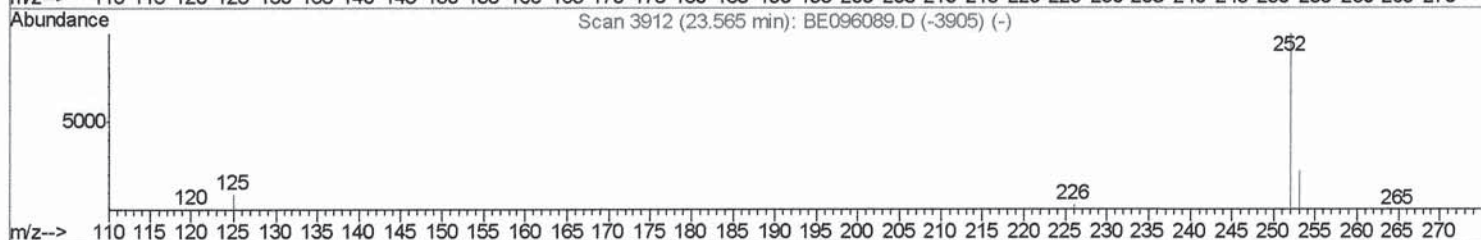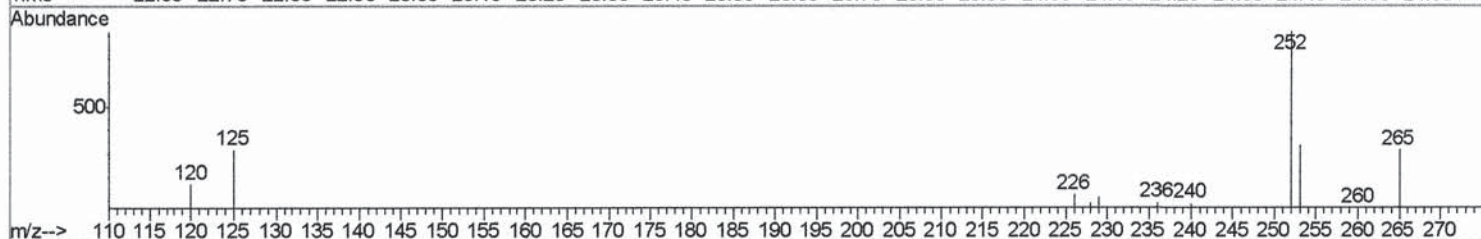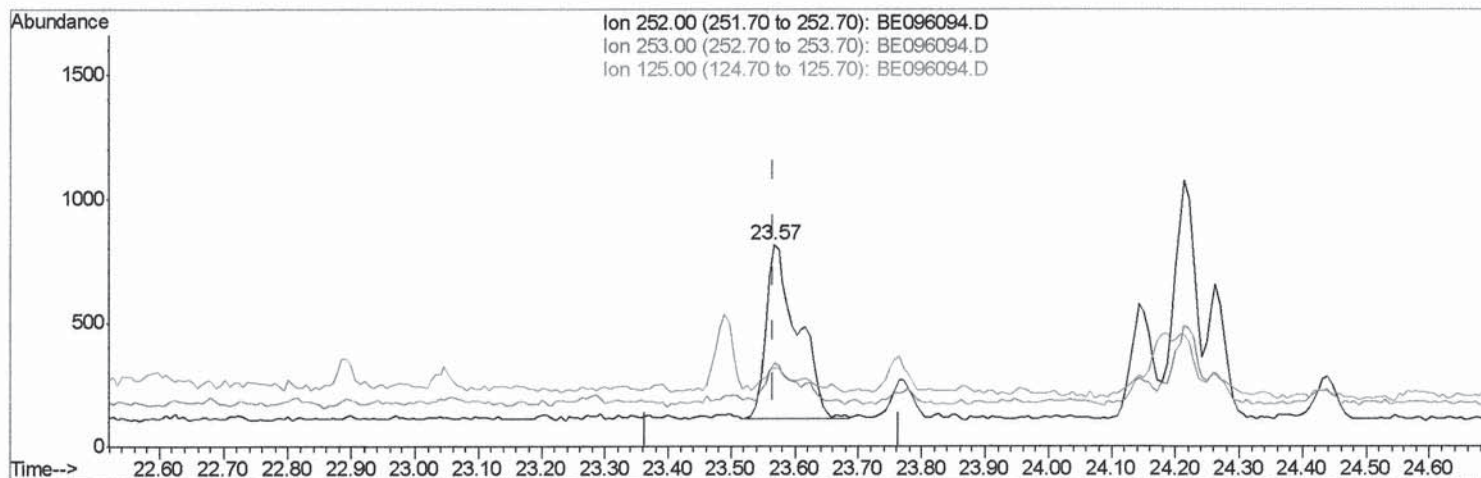

TIC: BE096094.D

(21) Benzo(b)fluoranthene

23.567min (+0.001) 0.09ng/ul

response 2421

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	41.15
125.00	17.50	38.94#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

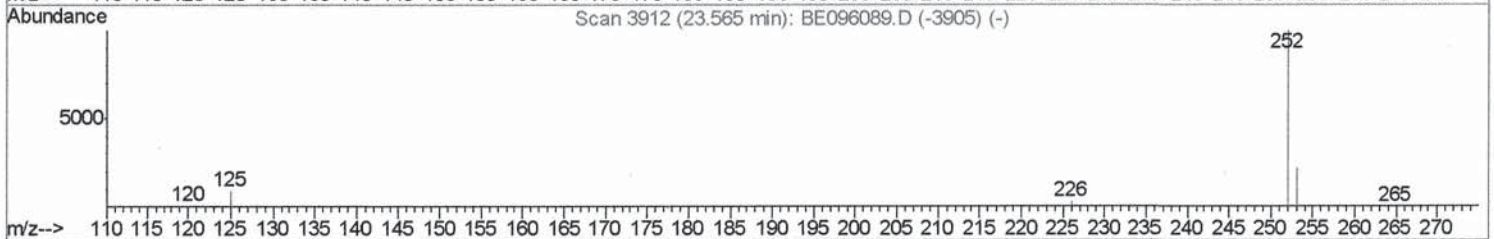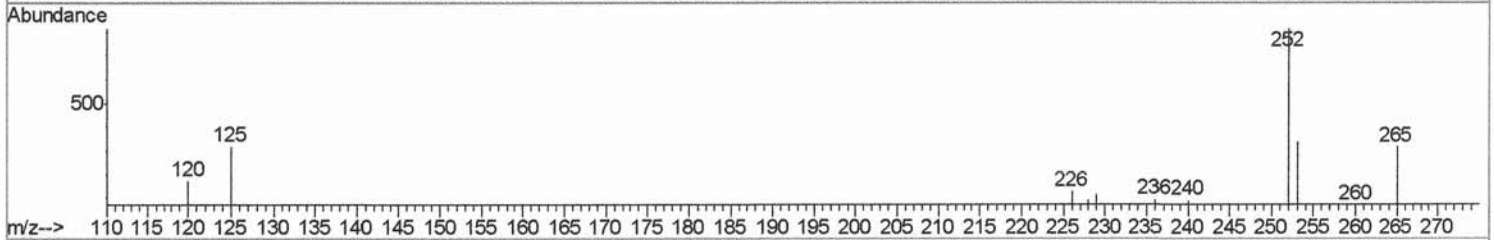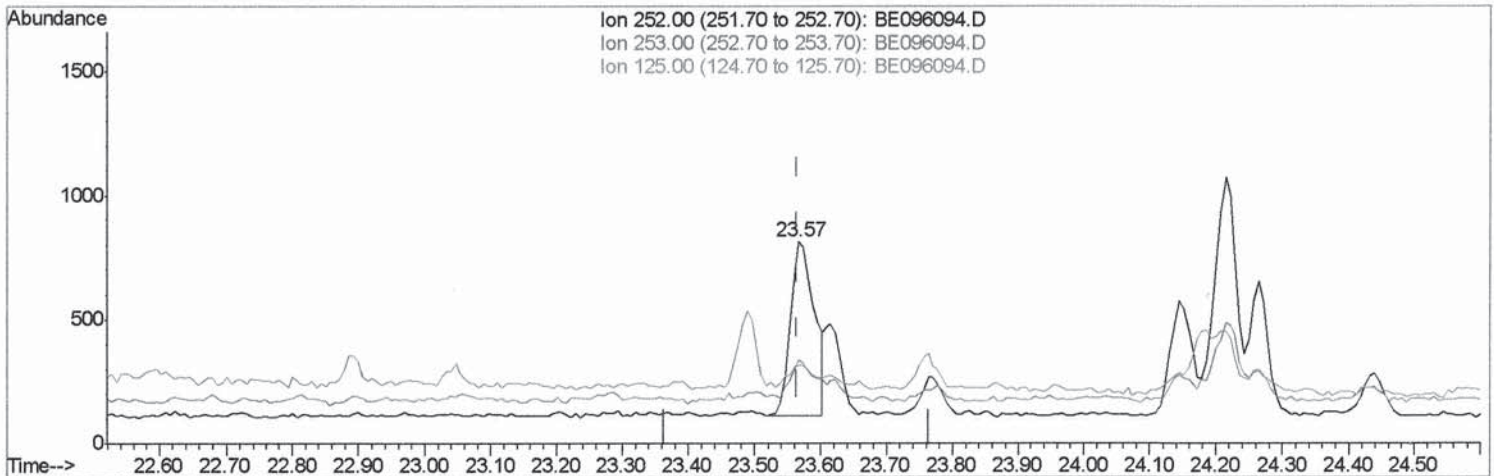

TIC: BE096094.D

(21) Benzo(b)fluoranthene

23.567min (+0.001) 0.06ng/ul m> SJ 4/24/18

response 1800

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	41.15
125.00	17.50	38.94#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

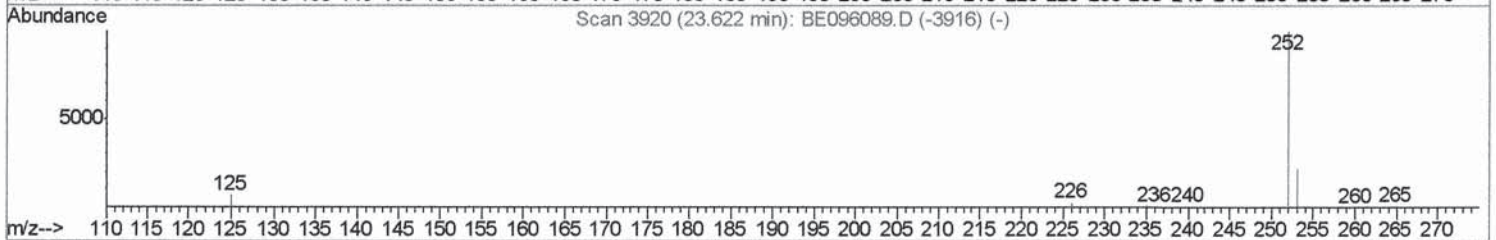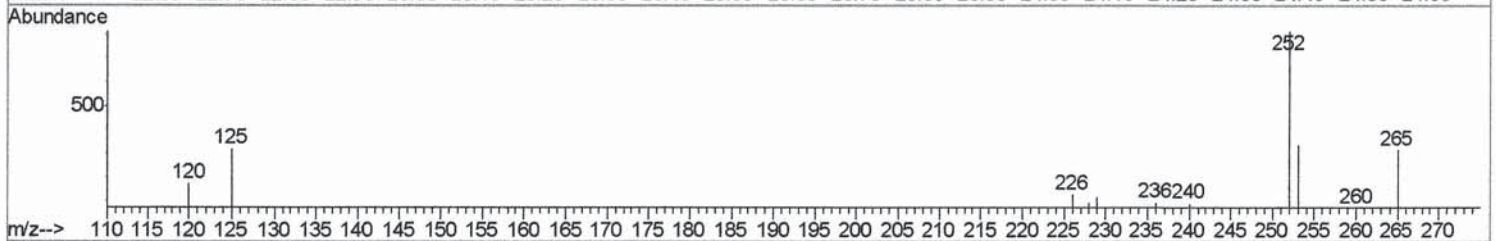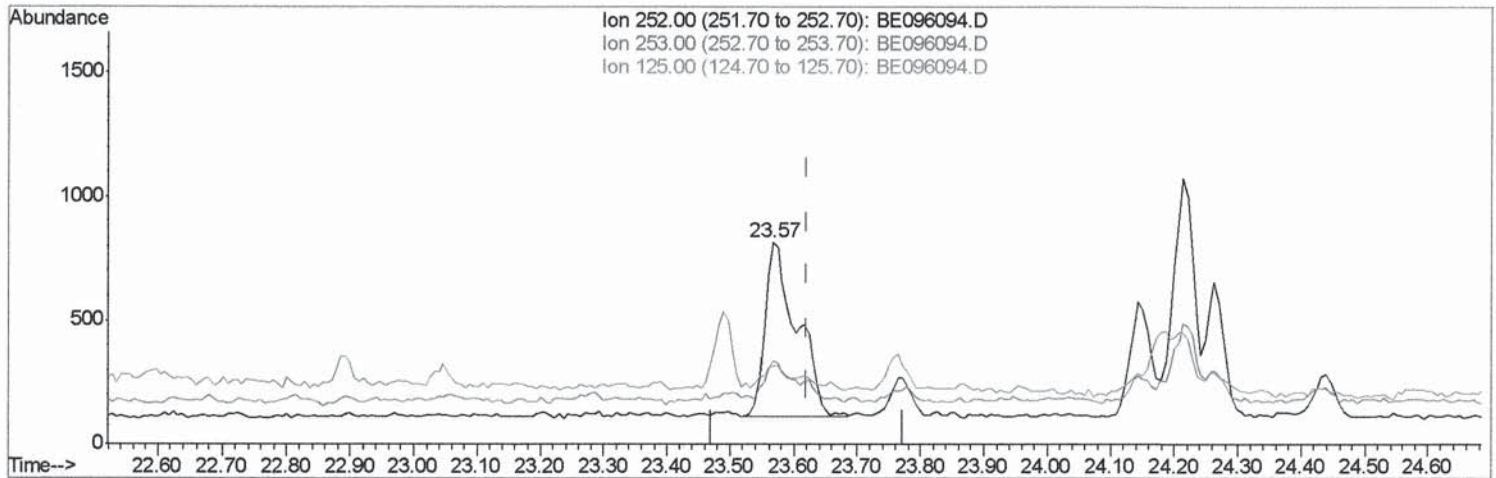

TIC: BE096094.D

(22) Benzo(k)fluoranthene
 23.567min (-0.055) 0.09ng/ul
 response 2421

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	41.15#
125.00	17.10	38.94#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
Data File : BE096094.D
Acq On : 23 Apr 2018 20:36
Operator : SJ/JU
Sample : J2355-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
A3Y28

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:29:24 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

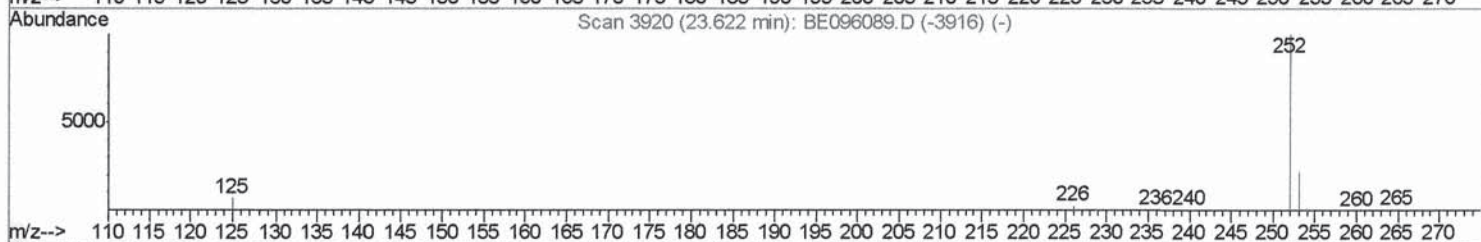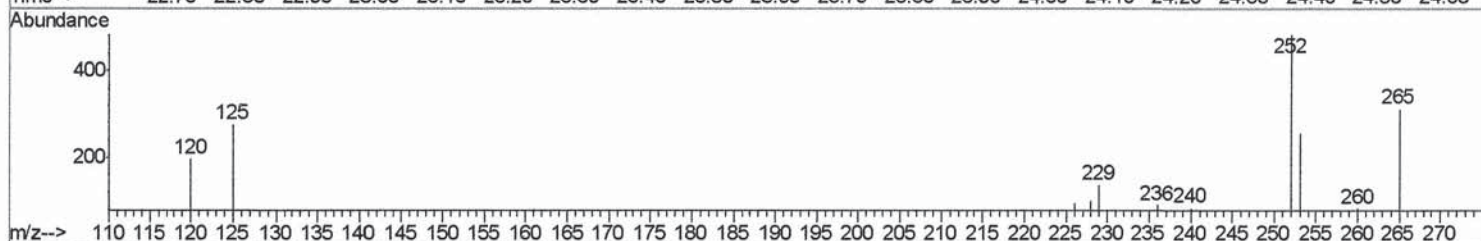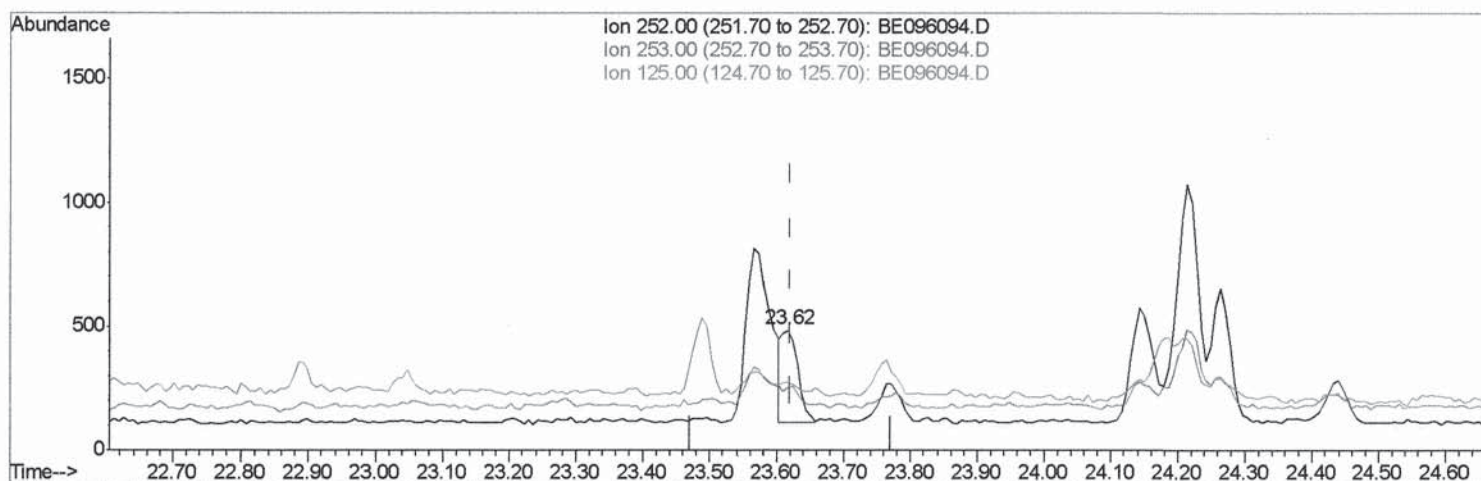

TIC: BE096094.D

(22) Benzo(k)fluoranthene

23.616min (-0.006) 0.02ng/ul m > SJ 4/24/18

response 635

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	52.69#
125.00	17.10	57.02#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE042318\
 Data File : BE096094.D
 Acq On : 23 Apr 2018 20:36
 Operator : SJ/JU
 Sample : J2355-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 A3Y28

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:47 PM

Quant Time: Apr 24 07:30:50 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	2076	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	5901	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3590	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	7513m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	7086m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	8746	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.76	152	3385	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	8948m	0.29	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) Phenanthrene	17.72	178	816m	0.037	ng/ul	
15) Fluoranthene	19.68	202	1697m	0.056	ng/ul	
17) Pyrene	20.04	202	2403	0.100	ng/ul#	93
18) Benzo(a)anthracene	21.75	228	1190m	0.042	ng/ul	
19) Chrysene	21.80	228	1217m	0.059	ng/ul	
21) Benzo(b)fluoranthene	23.57	252	1800m	0.064	ng/ul	
22) Benzo(k)fluoranthene	23.62	252	635m	0.023	ng/ul	
23) Benzo(a)pyrene	24.26	252	1019	0.037	ng/ul#	72
24) Indeno(1,2,3-cd)pyrene	27.16	276	1059	0.035	ng/ul#	72
26) Benzo(a,h,i)perylene	28.03	276	1043	0.041	ng/ul#	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed