


Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
Data File : BE096100.D
Acq On : 24 Apr 2018 00:14
Operator : SJ/JU
Sample : J2434-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AB6

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:49:16 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

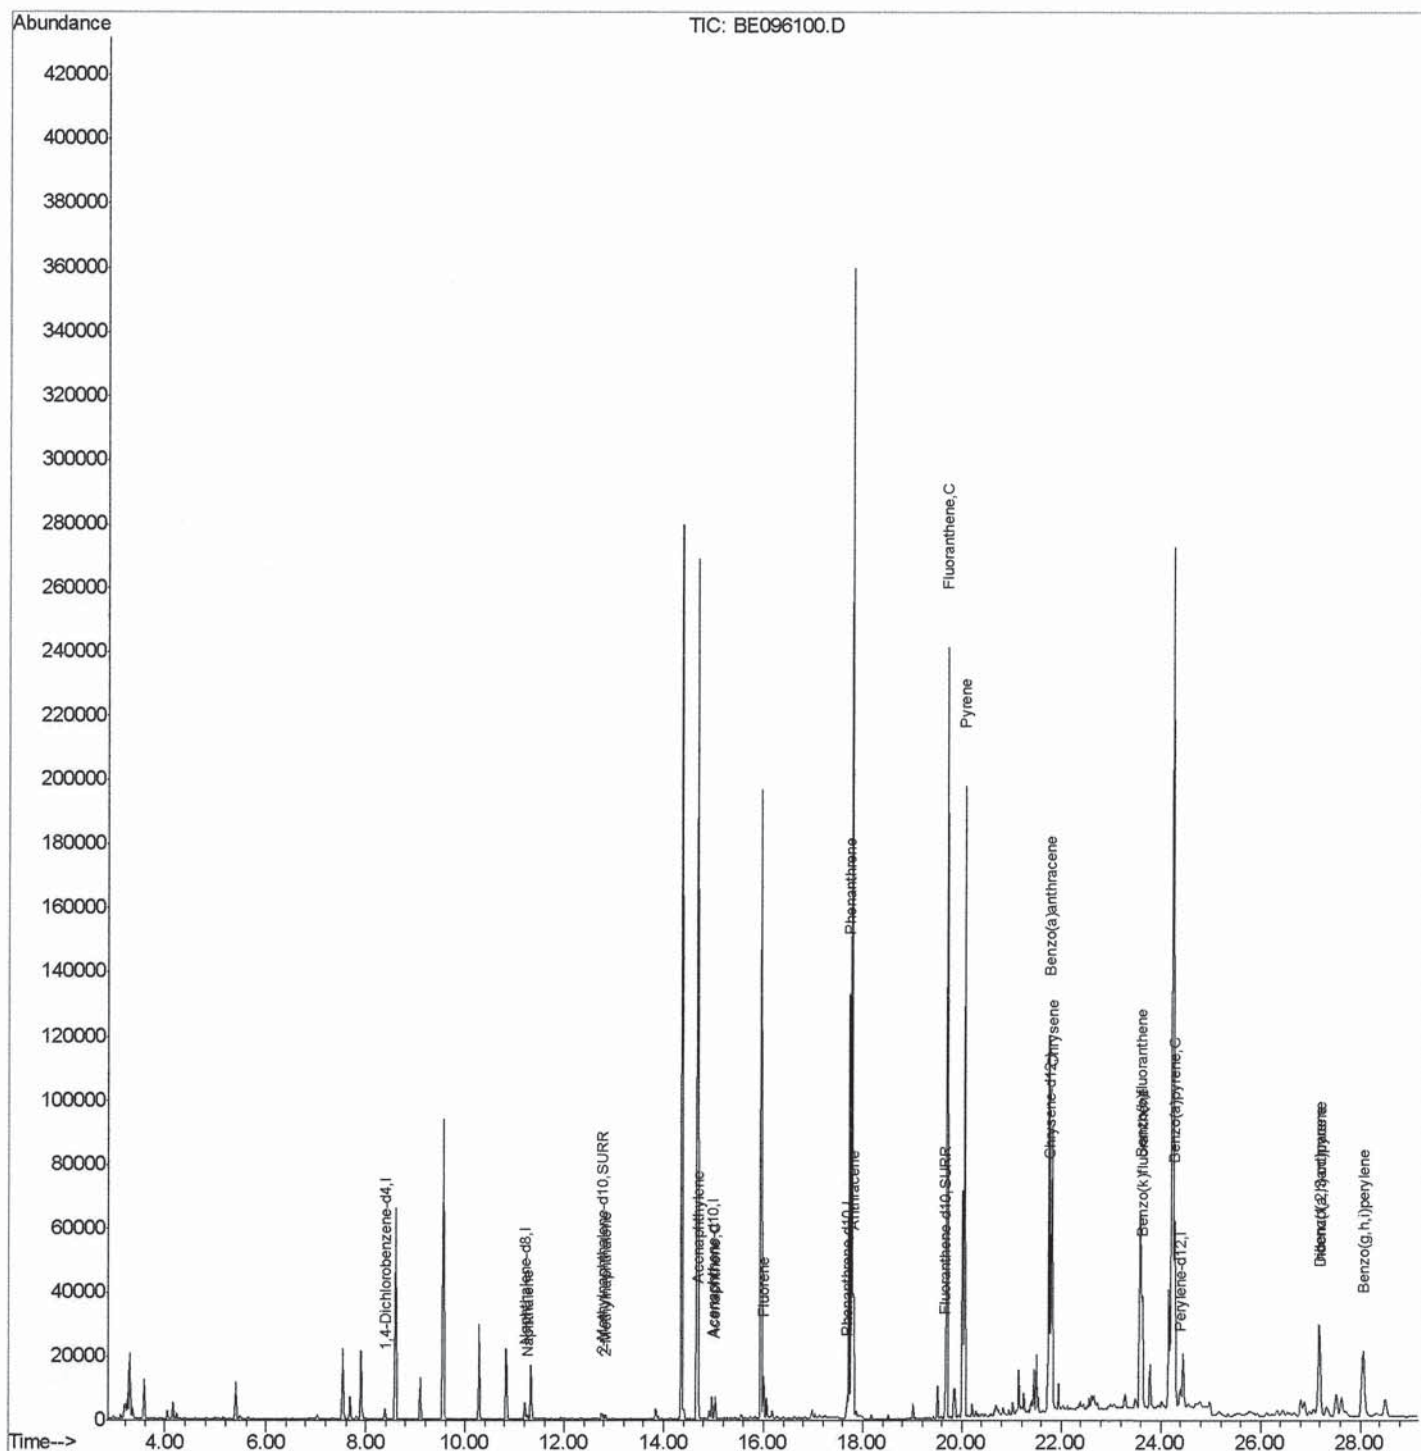

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:44:40 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

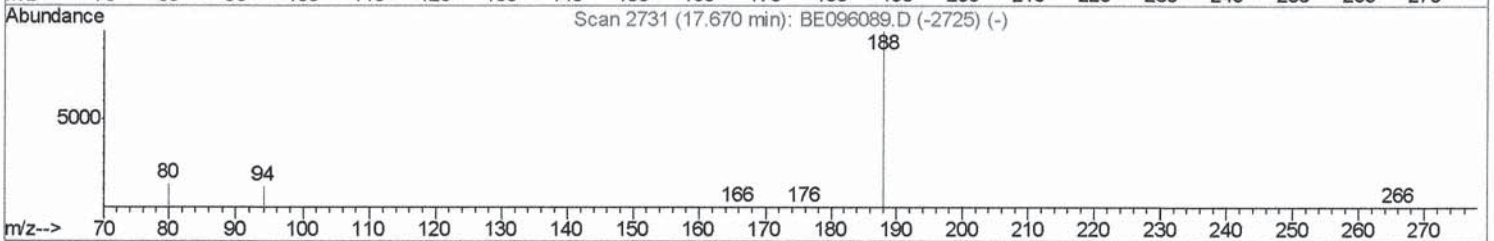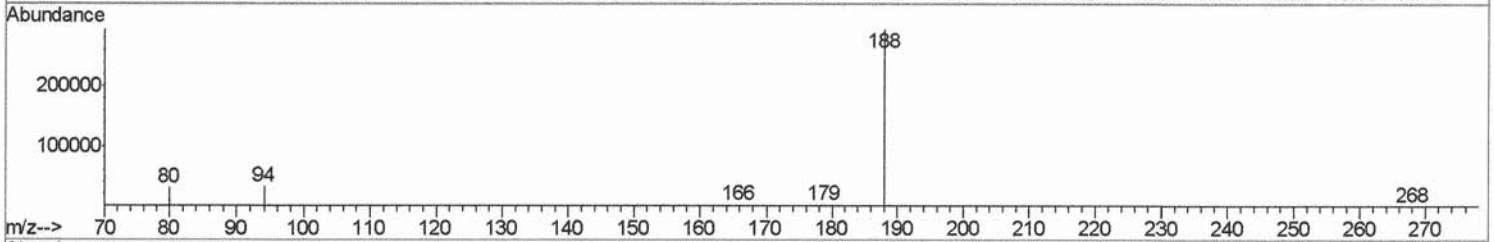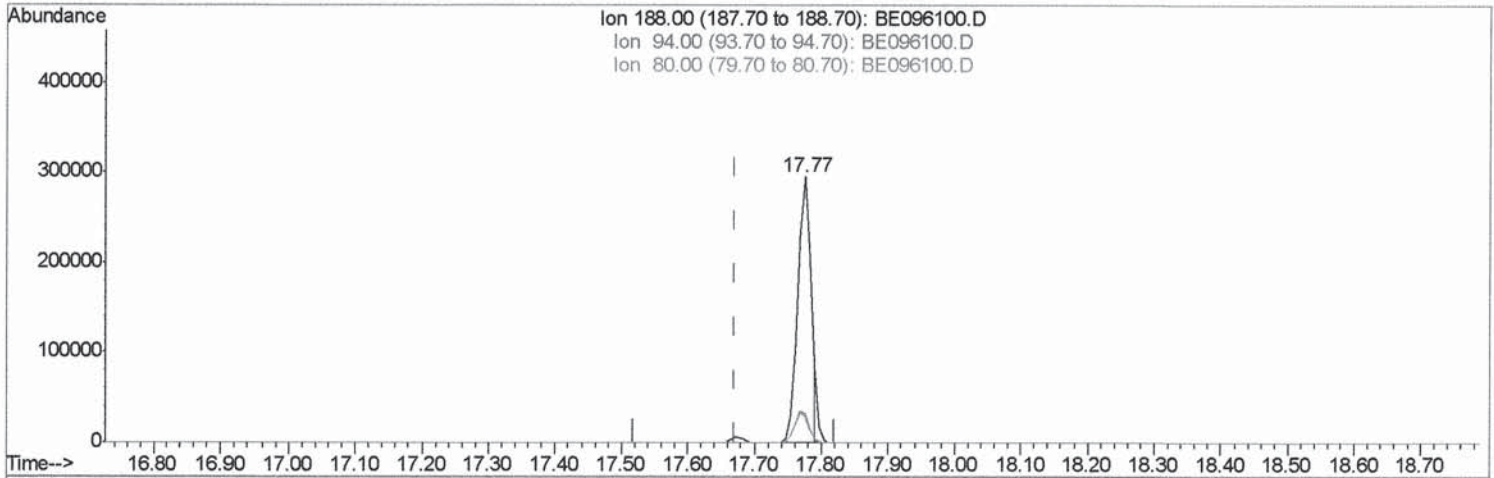

TIC: BE096100.D

(10) Phenanthrene-d10 (I)

17.775min (+0.104) 0.40ng/ul

response 403486

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.85
80.00	11.80	10.23
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:44:40 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

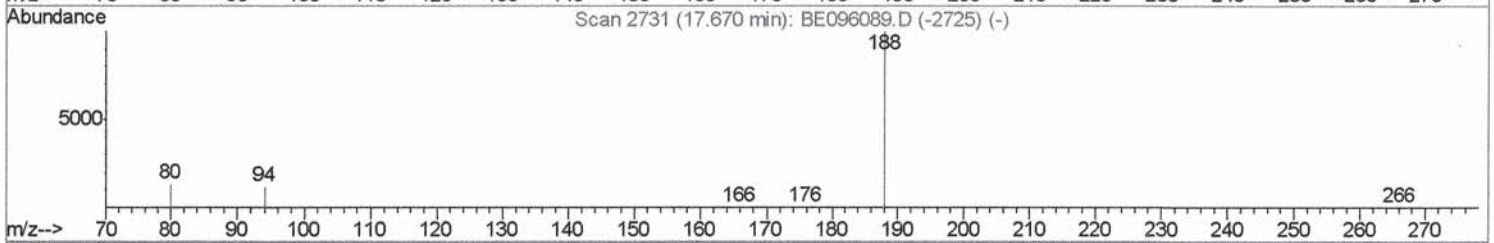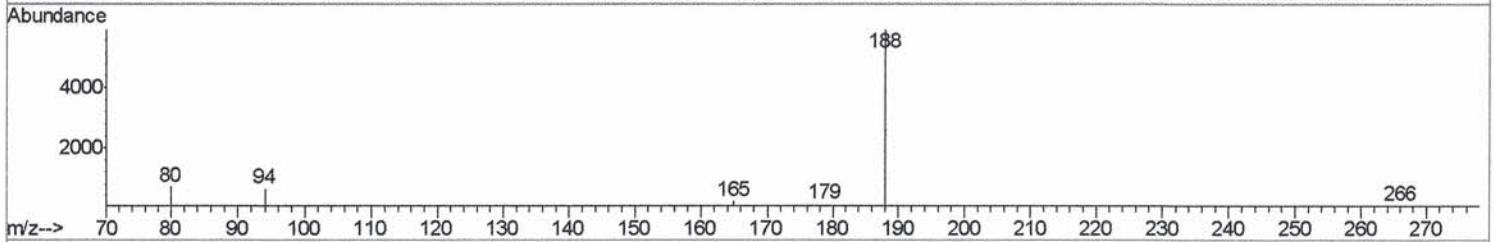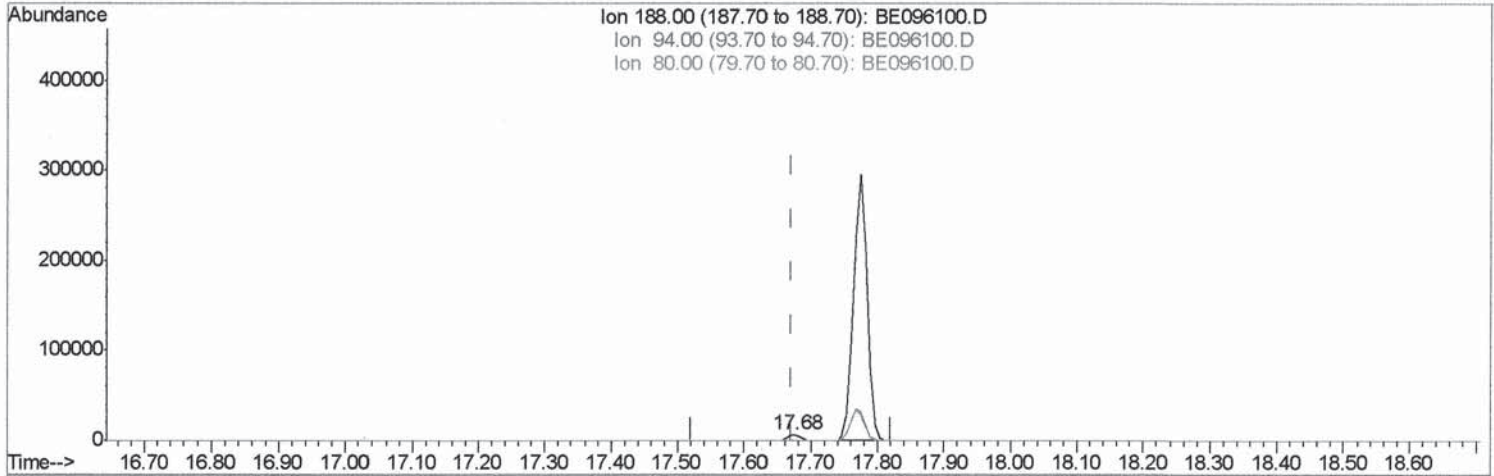

TIC: BE096100.D

(10) Phenanthrene-d10 (I)

17.676min (+0.006) 0.40ng/ul m > SJ 4/24/18

response 8524

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.66
80.00	11.80	11.59
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

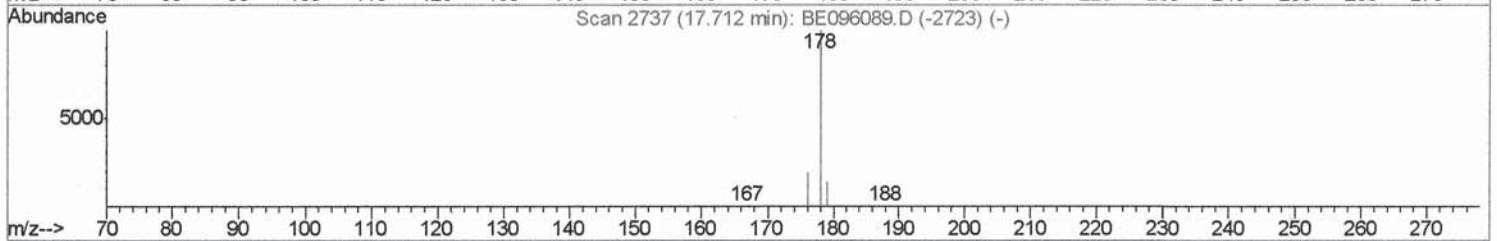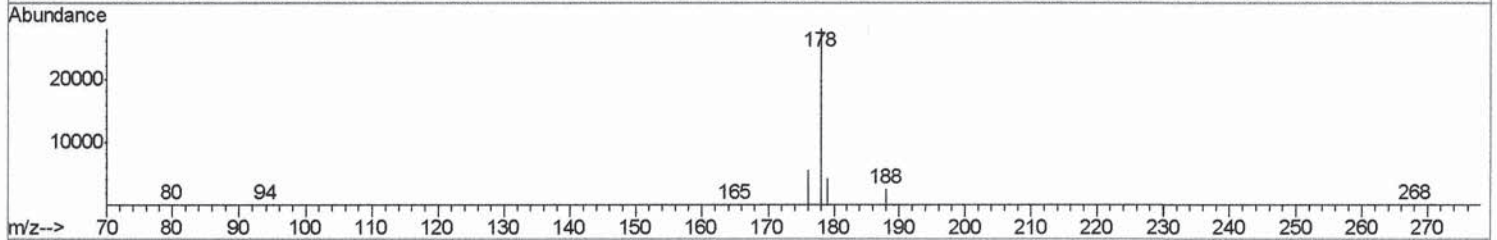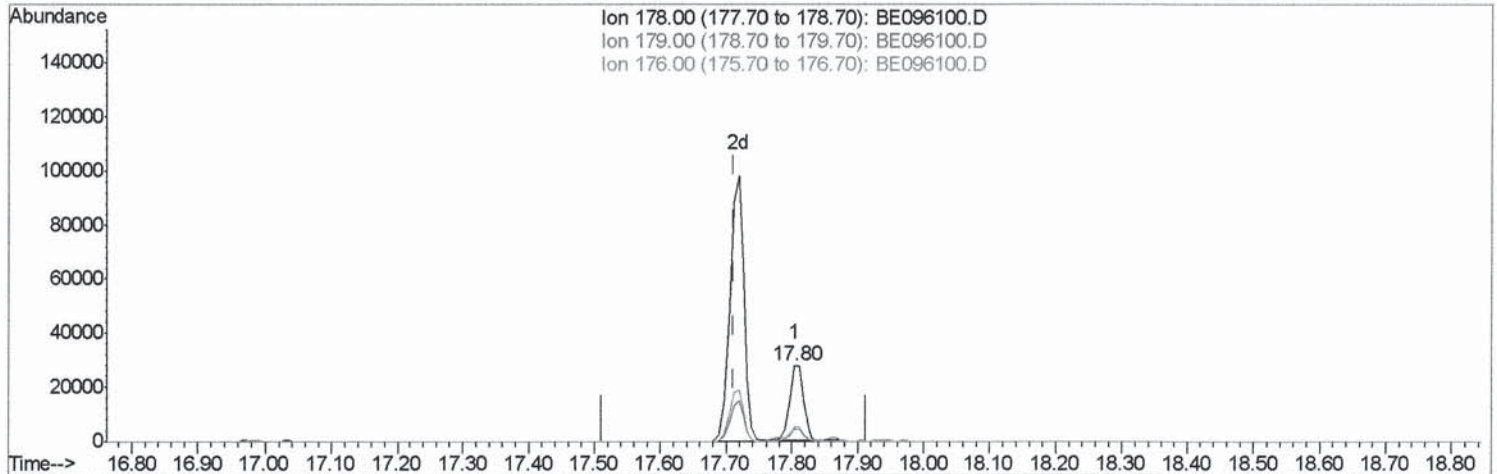

TIC: BE096100.D

(12) Phenanthrene

17.803min (+0.090) 1.60ng/ul

response 40267

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.51#
176.00	17.00	19.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
Data File : BE096100.D
Acq On : 24 Apr 2018 00:14
Operator : SJ/JU
Sample : J2434-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB6

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

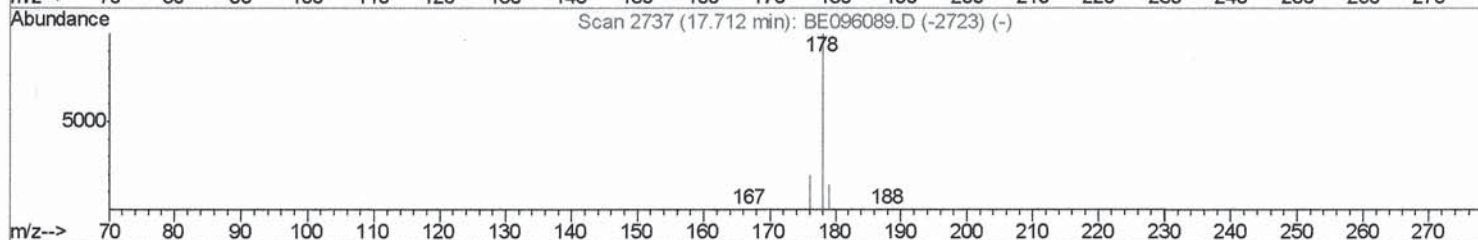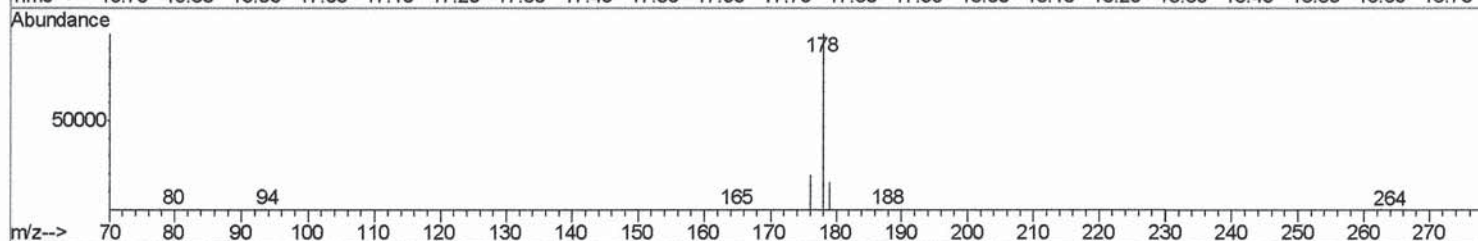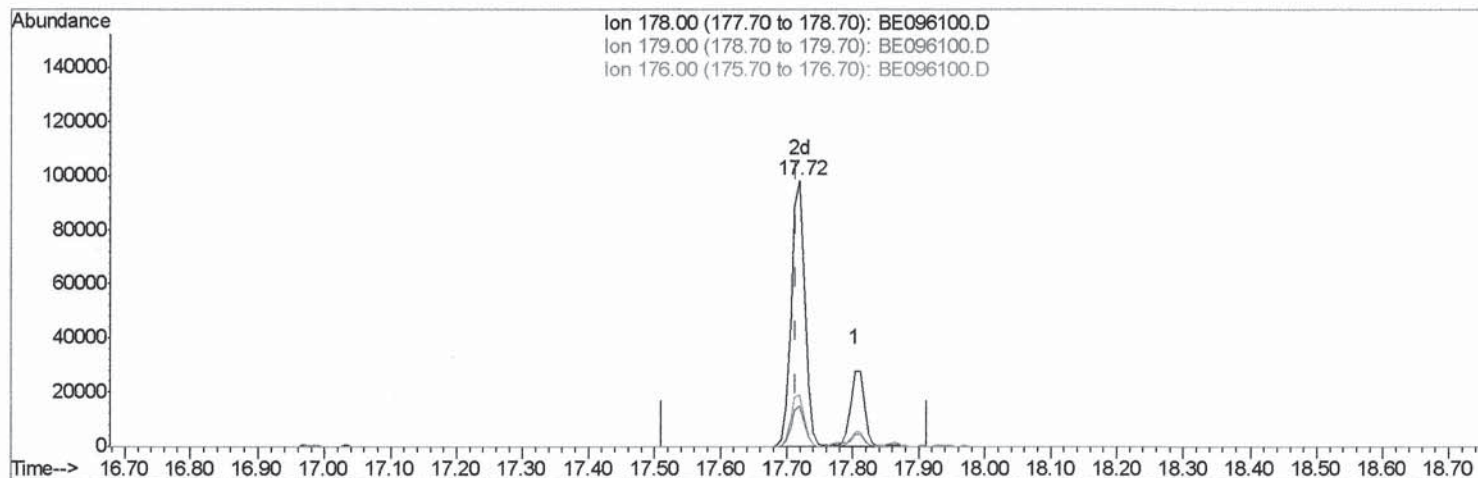

TIC: BE096100.D

(12) Phenanthrene

17.718min (+0.006) 5.76ng/ul m> SJ 4/22/18

response 144766

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.54#
176.00	17.00	19.77
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

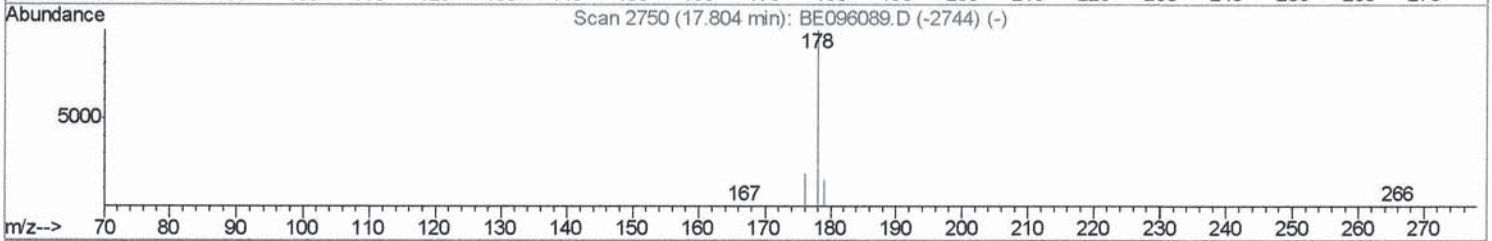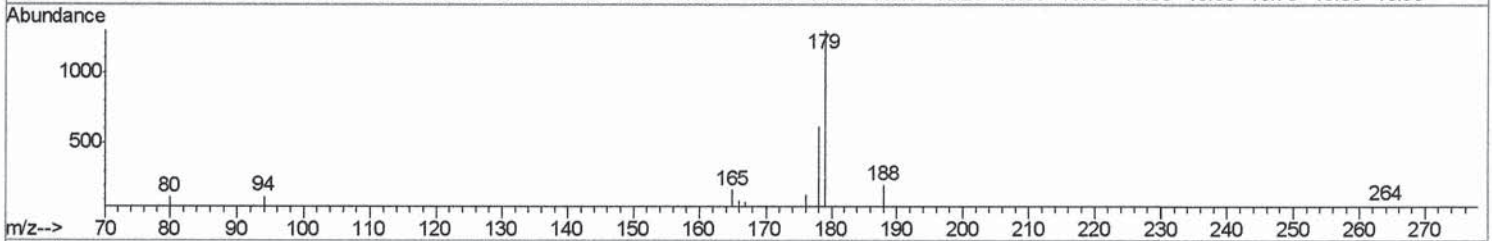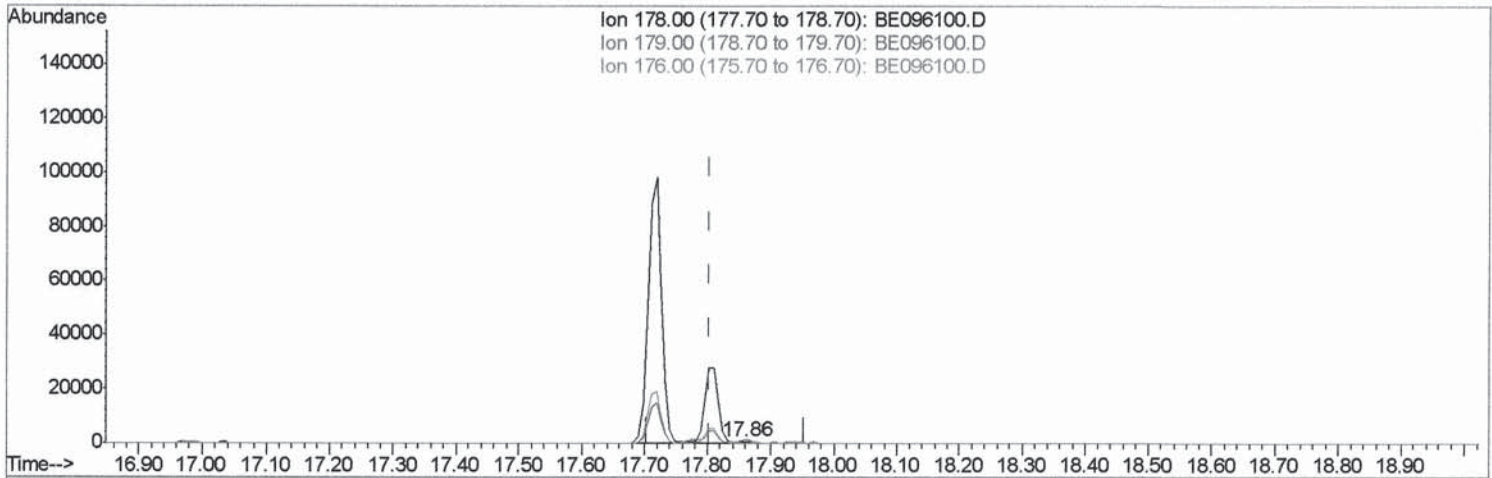

TIC: BE096100.D

(13) Anthracene

17.859min (+0.055) 0.10ng/ul

response 2484

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	209.87#
176.00	18.40	22.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

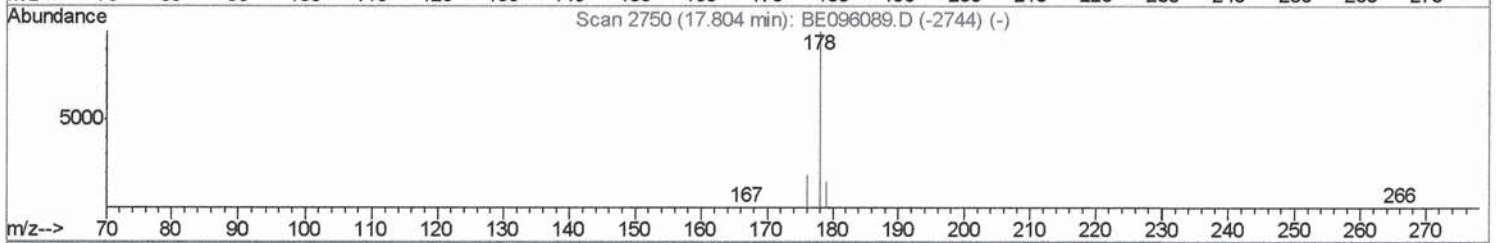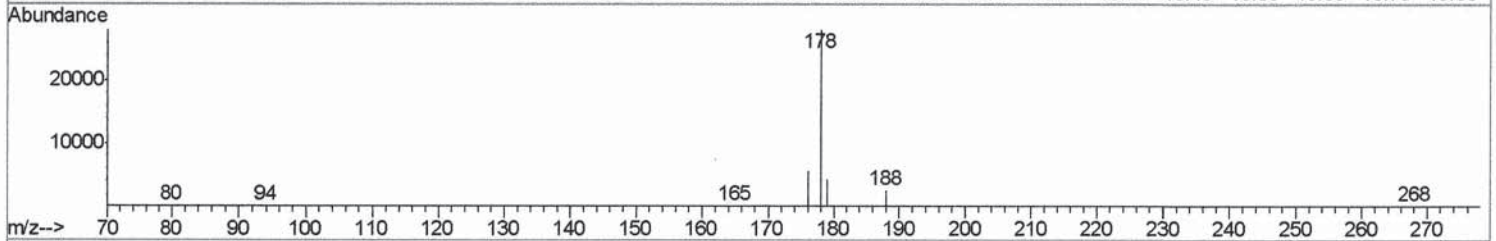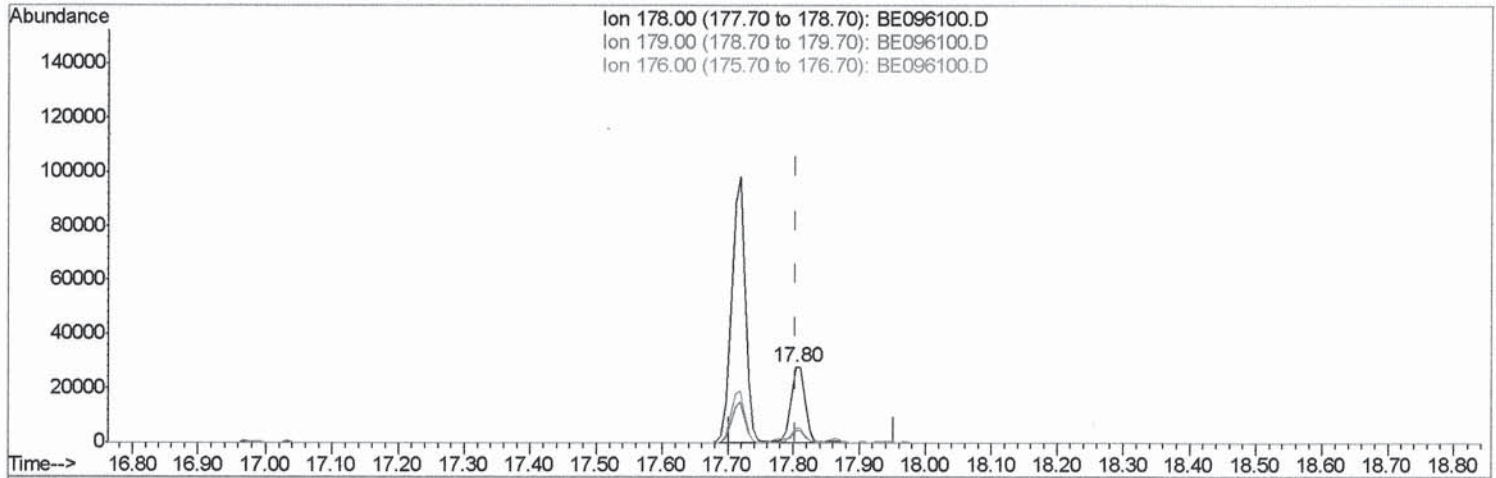

TIC: BE096100.D

(13) Anthracene

17.803min (-0.001) 1.66ng/ul m2 SJ 4/24/18

response 41602

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	15.51#
176.00	18.40	19.75
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
Data File : BE096100.D
Acq On : 24 Apr 2018 00:14
Operator : SJ/JU
Sample : J2434-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB6

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

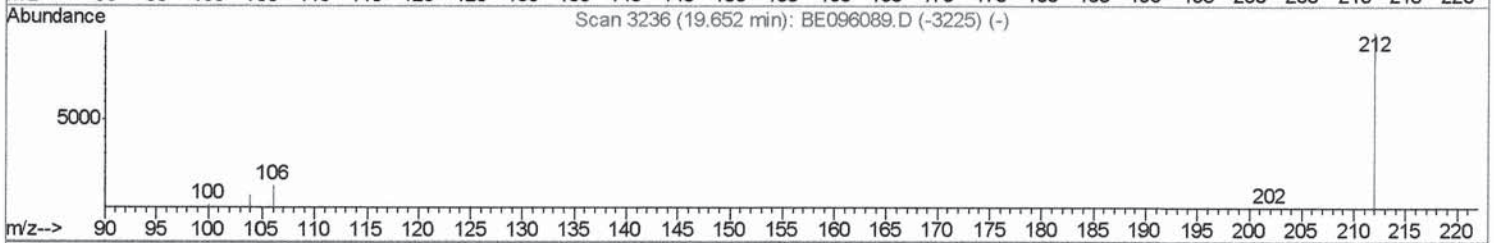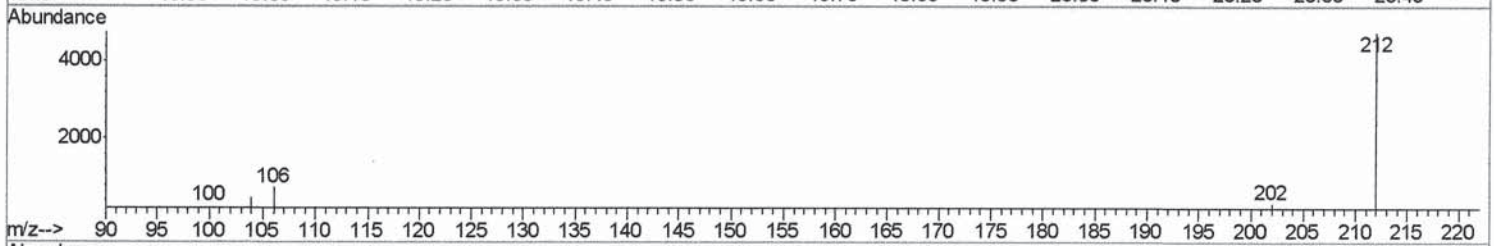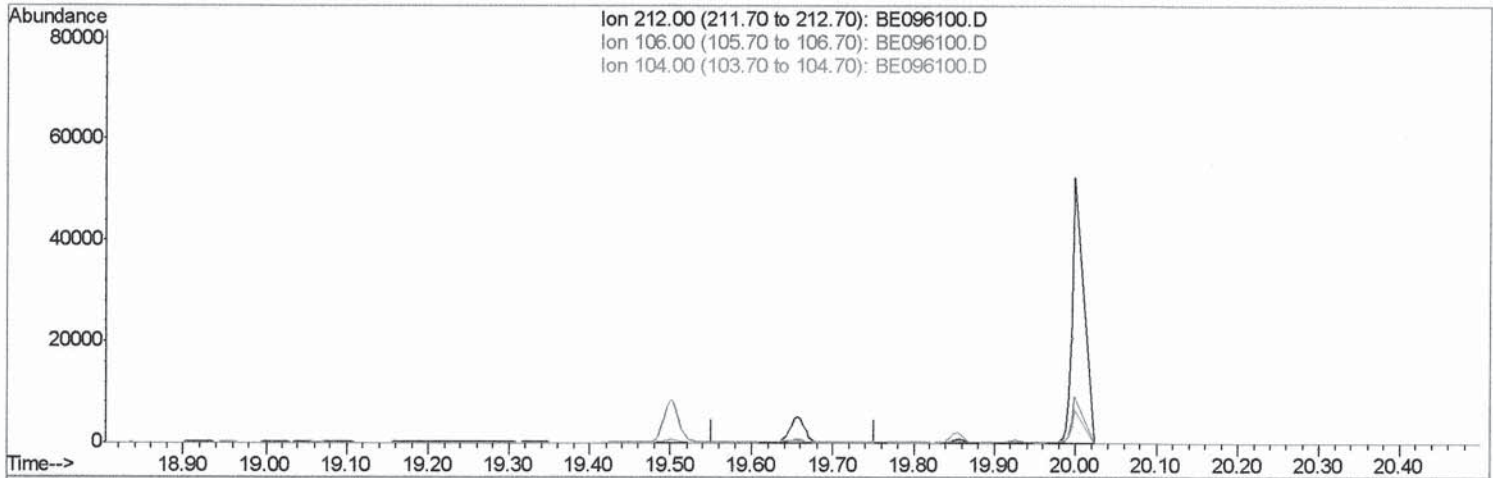

TIC: BE096100.D

(14) Fluoranthene-d10 (SURR)

19.652min (-19.652) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

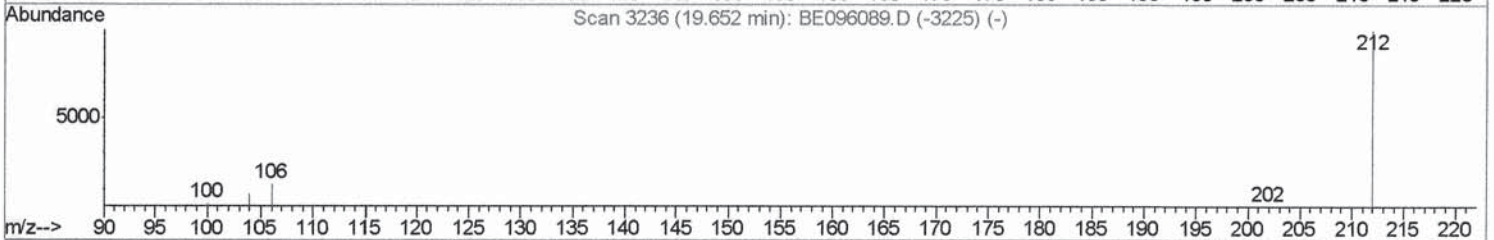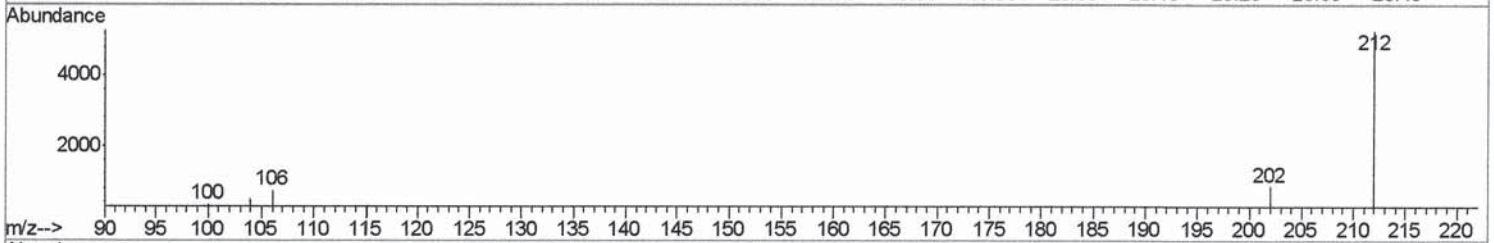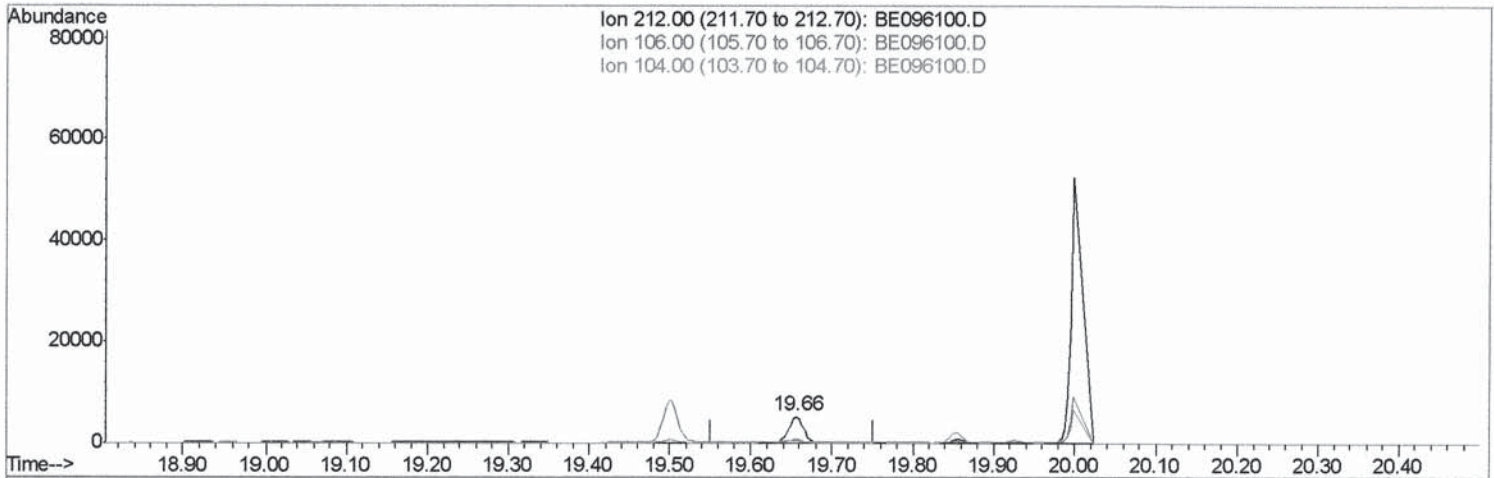

TIC: BE096100.D

(14) Fluoranthene-d10 (SURR)

19.656min (+0.004) 0.18ng/ul m> SJ 4/24/18

response 6491

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

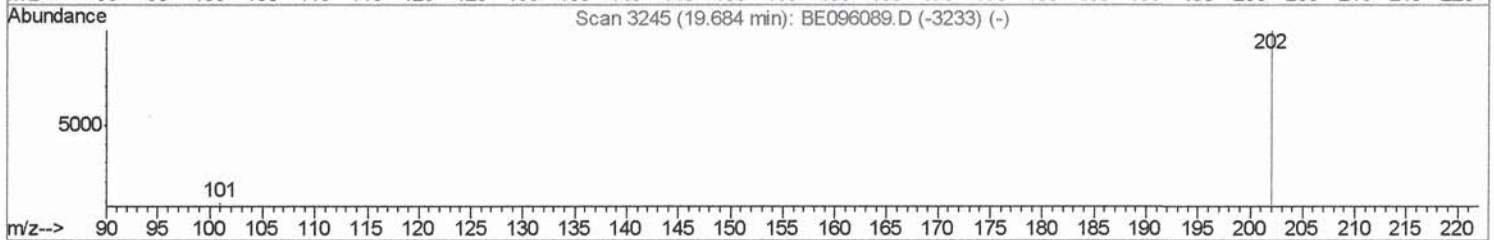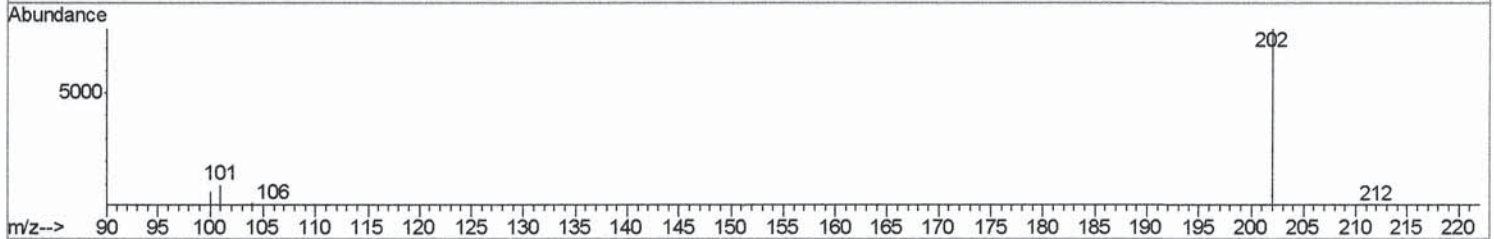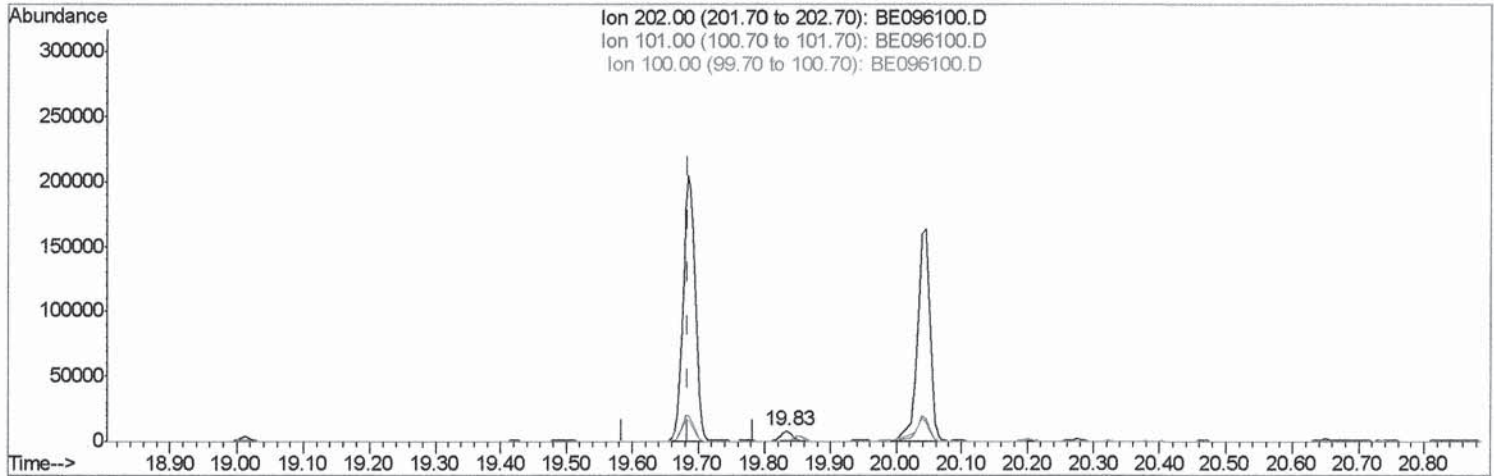

TIC: BE096100.D

(15) Fluoranthene (C)

19.834min (+0.150) 0.29ng/ui

response 10012

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.17
100.00	19.50	9.11
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

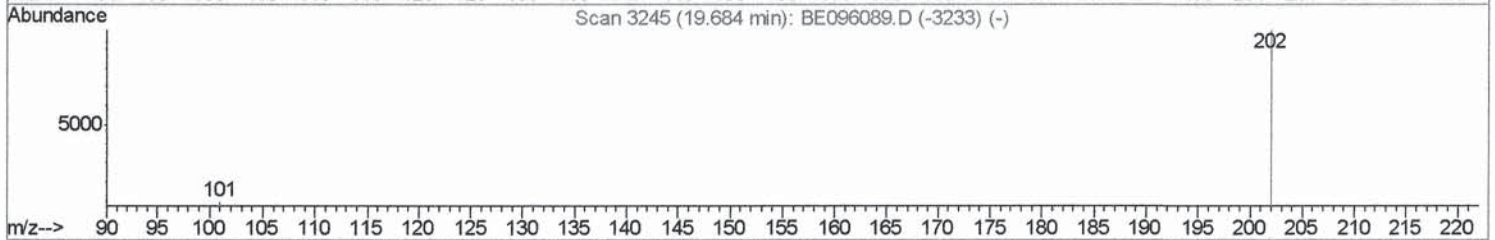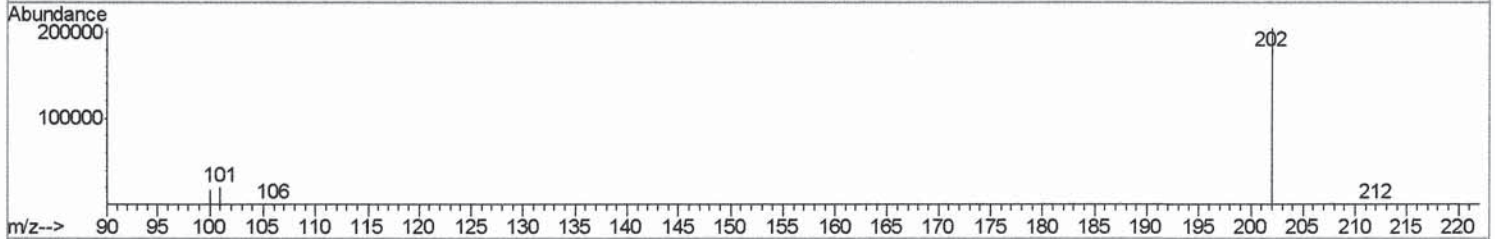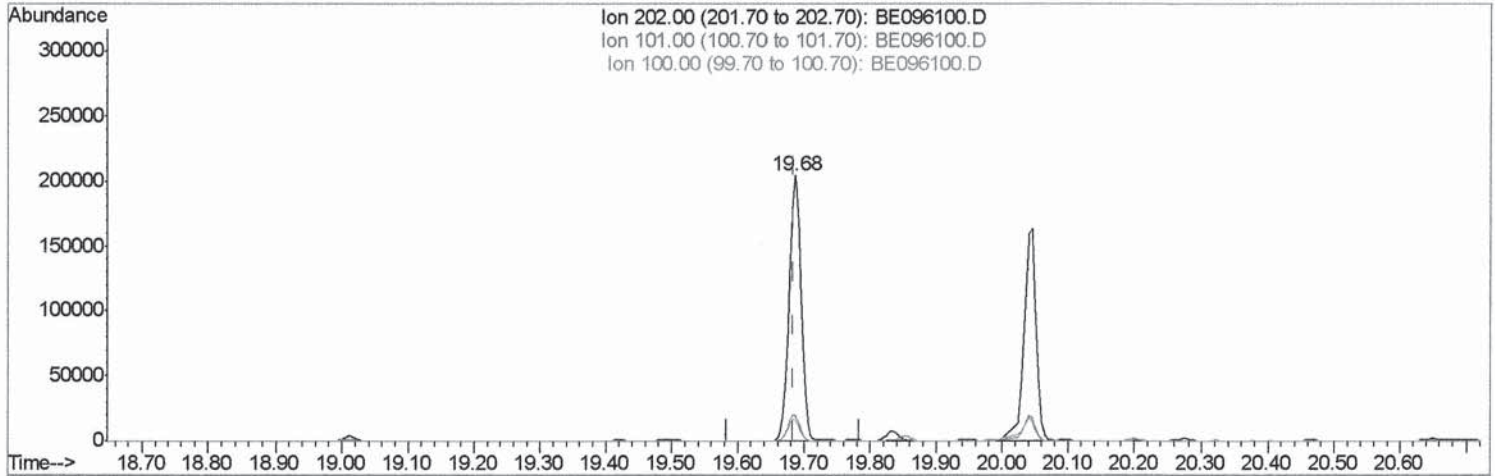

TIC: BE096100.D

(15) Fluoranthene (C)

19.684min (+0.000) 8.00ng/ul m> SJ 4/24/18

response 273360

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	9.80
100.00	19.50	8.14
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
Data File : BE096100.D
Acq On : 24 Apr 2018 00:14
Operator : SJ/JU
Sample : J2434-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB6

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

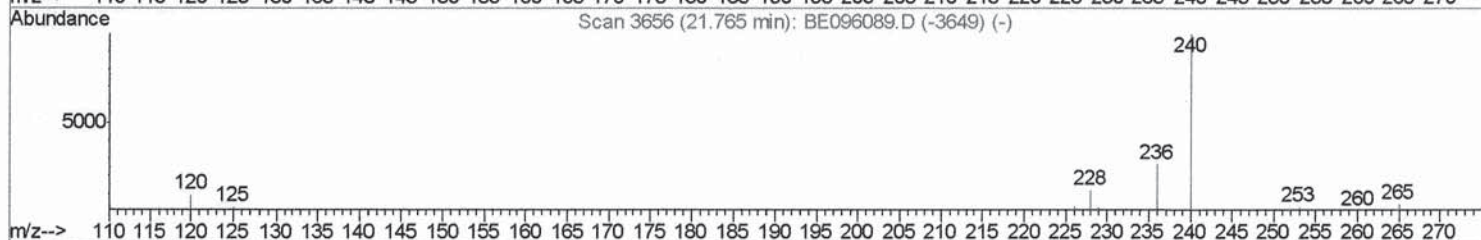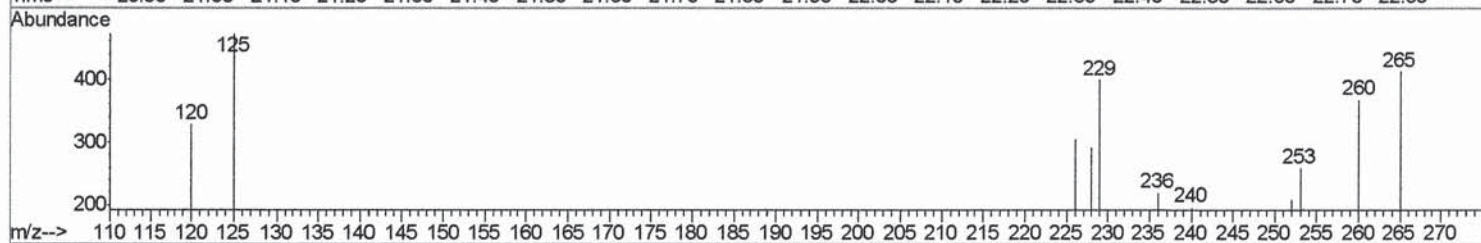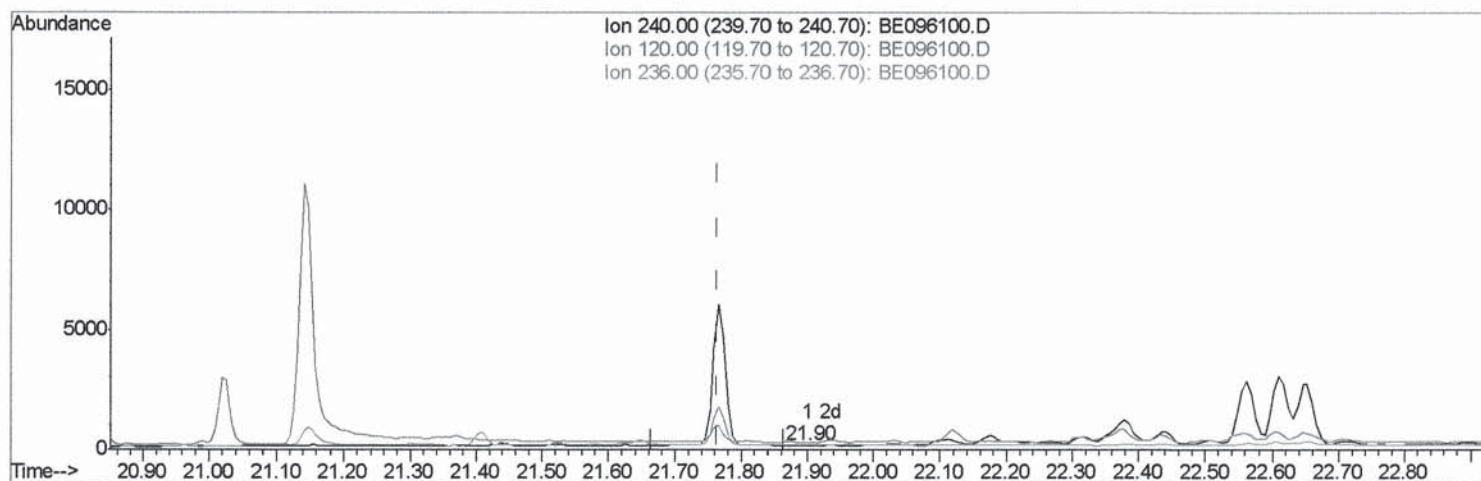

TIC: BE096100.D

(16) Chrysene-d12 (I)

21.900min (+0.135) 0.40ng/ul

response 108

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	167.35#
236.00	34.90	111.73#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:45:30 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

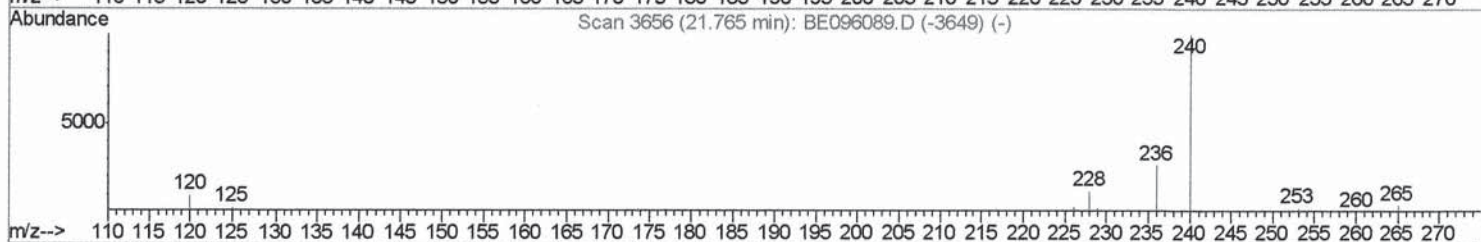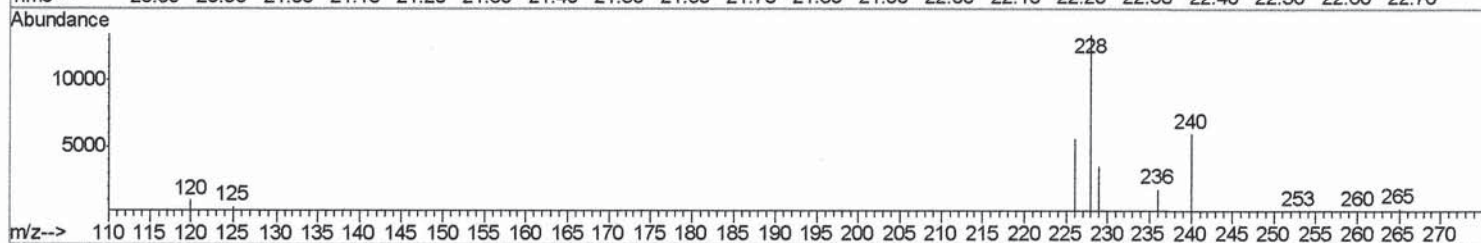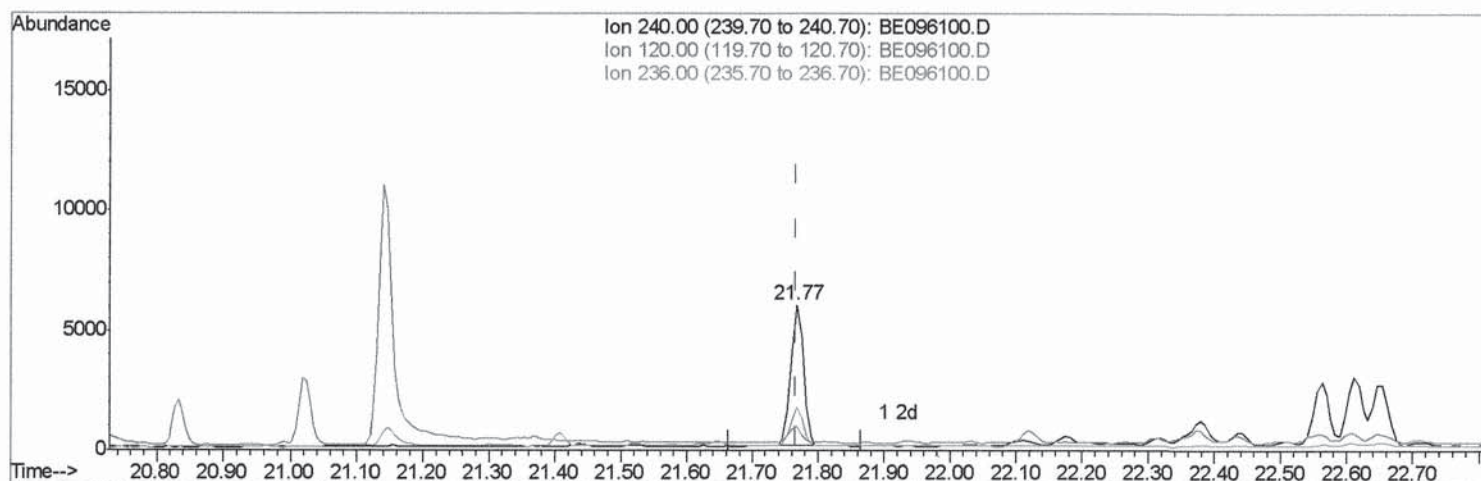

TIC: BE096100.D

(16) Chrysene-d12 (I)

21.766min (+0.001) 0.40ng/ul m > SJ 4/27/18

response 7705

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	16.47#
236.00	34.90	30.21
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

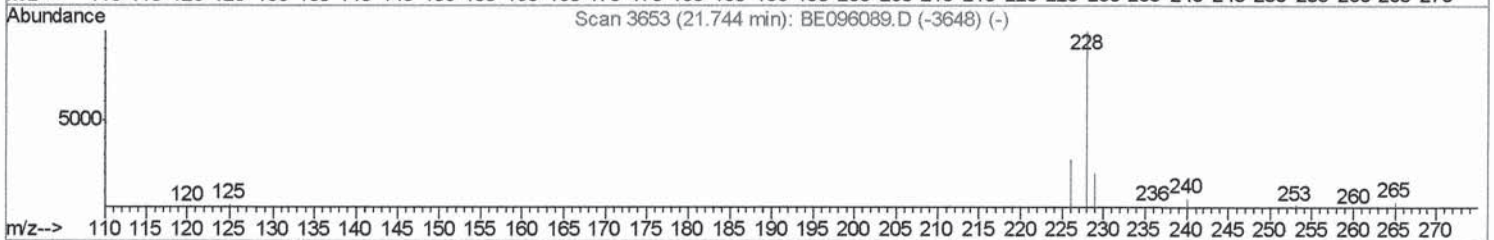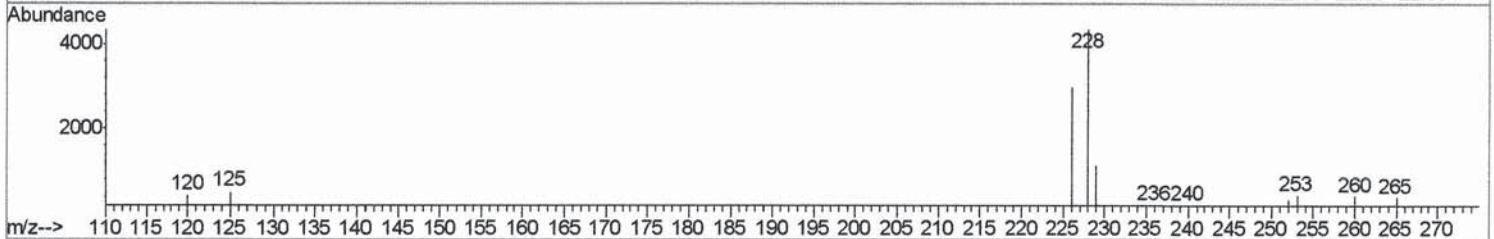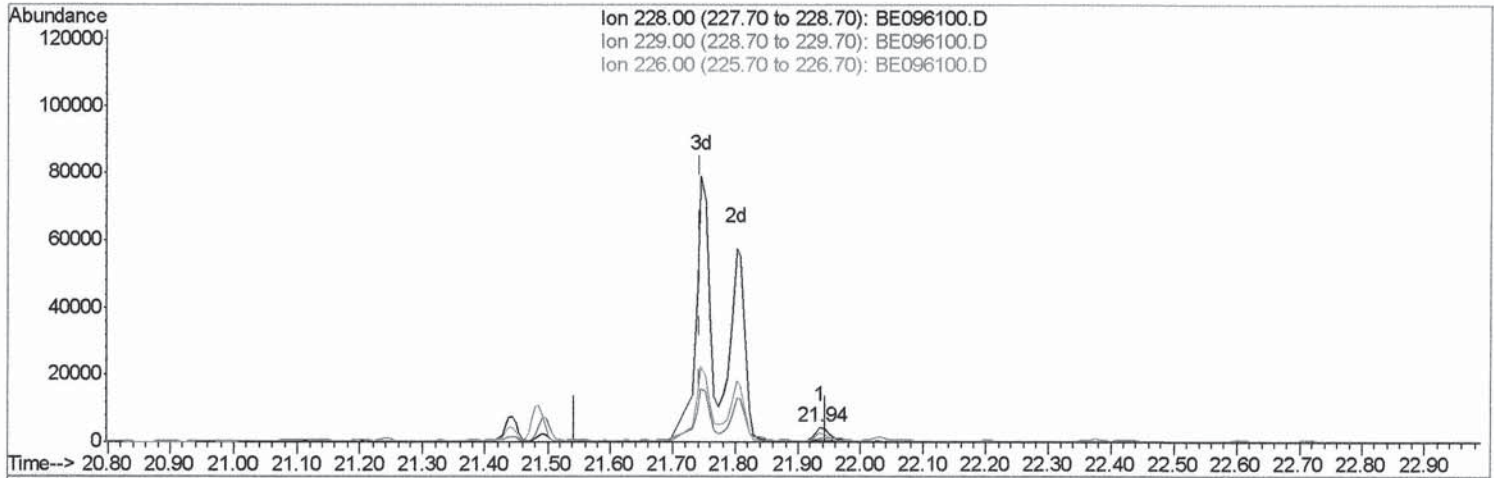

TIC: BE096100.D

(18) Benzo(a)anthracene
 21.935min (+0.191) 0.21ng/ul
 response 6595

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	26.12
226.00	21.30	68.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

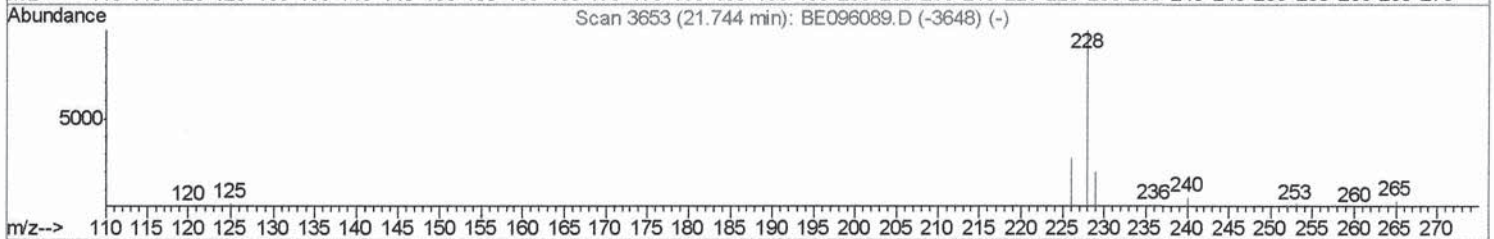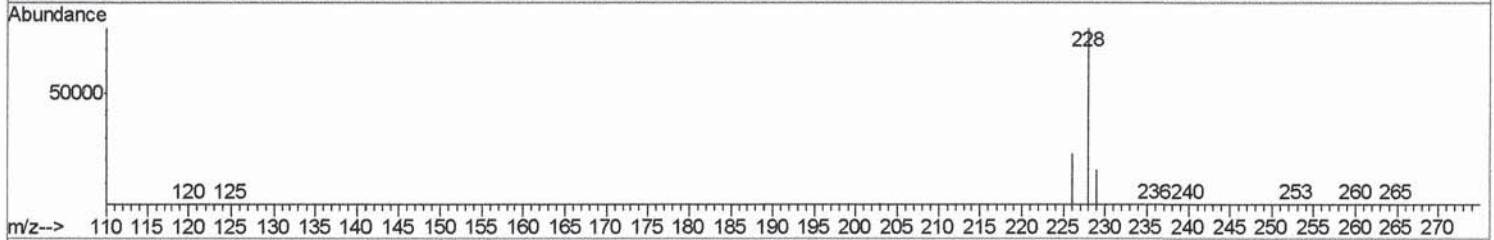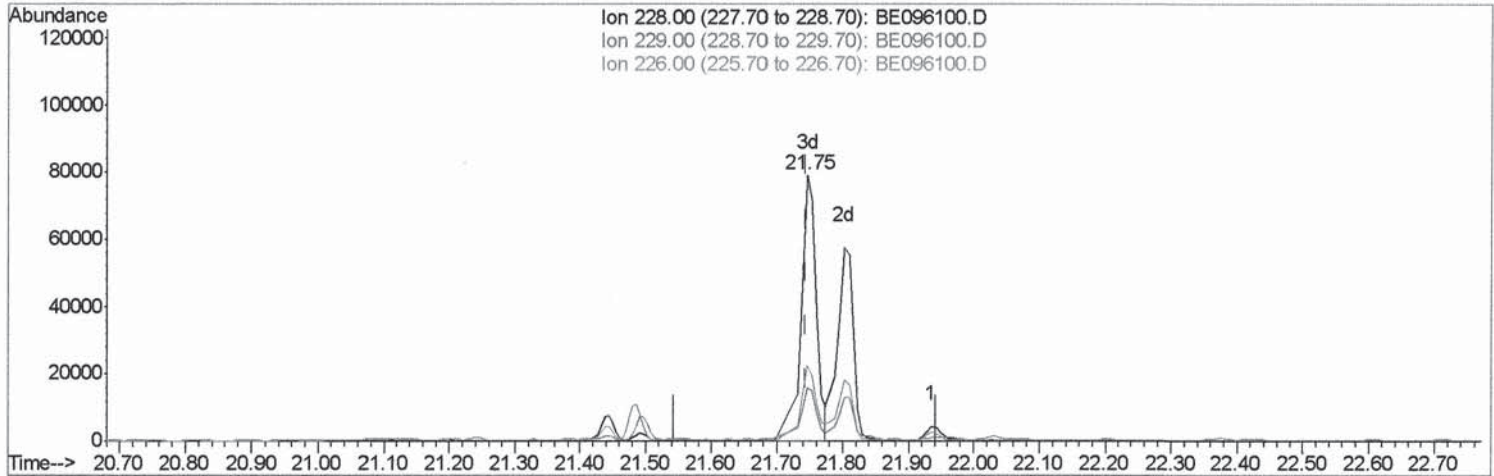

TIC: BE096100.D

(18) Benzo(a)anthracene

21.745min (+0.001) 4.82ng/ul m> SJ 4/24/18

response 149912

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.17#
226.00	21.30	28.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

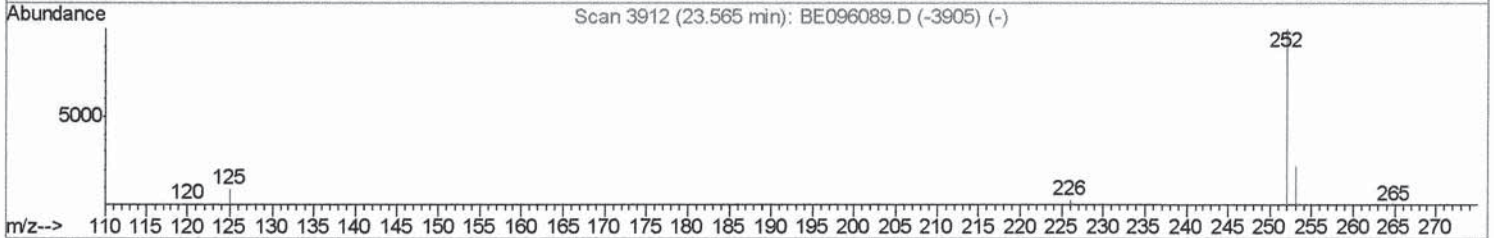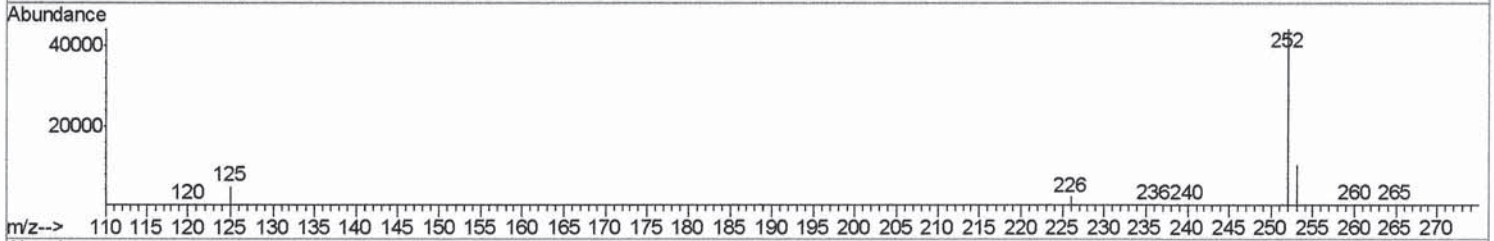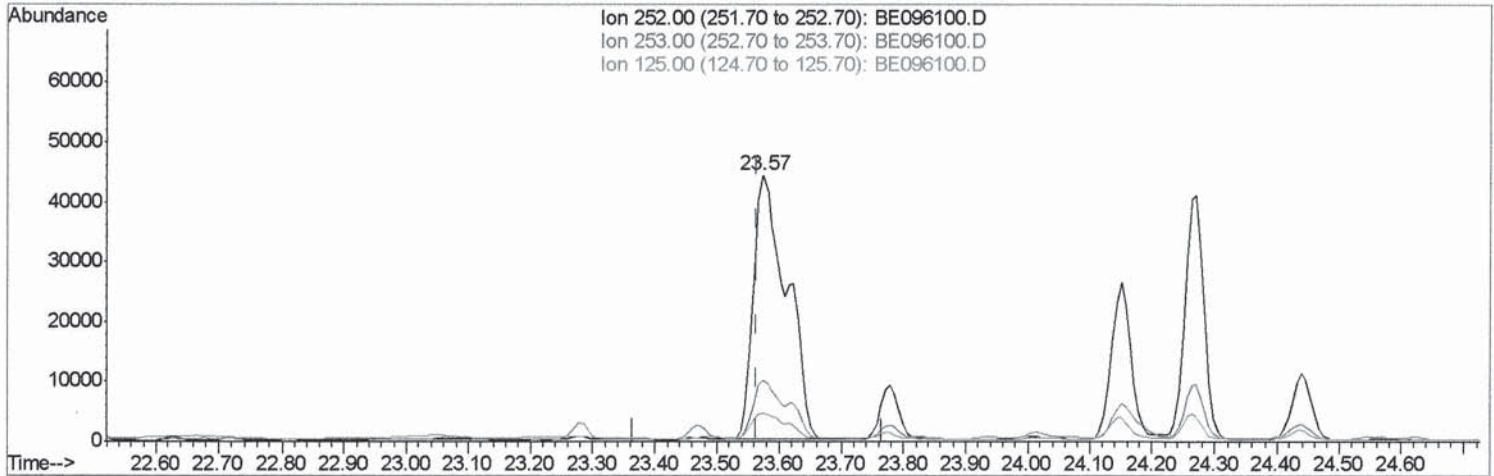

TIC: BE096100.D

(21) Benzo(b)fluoranthene
 23.574min (+0.008) 4.95ng/ul
 response 162517

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.11
125.00	17.50	10.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
Data File : BE096100.D
Acq On : 24 Apr 2018 00:14
Operator : SJ/JU
Sample : J2434-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AB6

Manual Integrations
APPROVED

Sohil
4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 24 06:59:54 2018
Response via : Initial Calibration

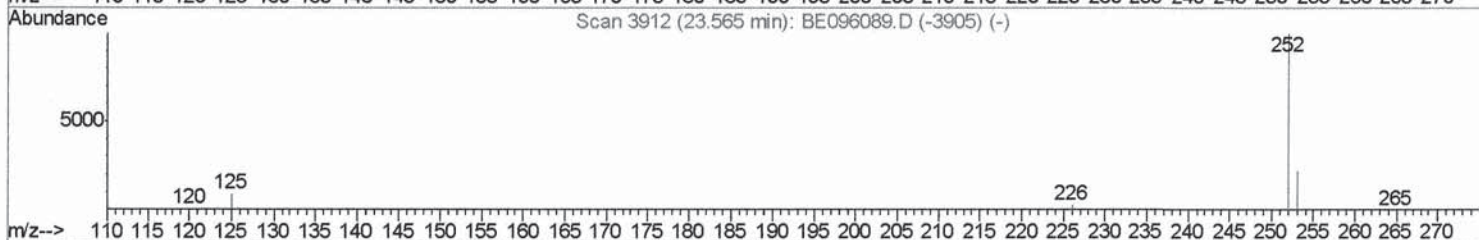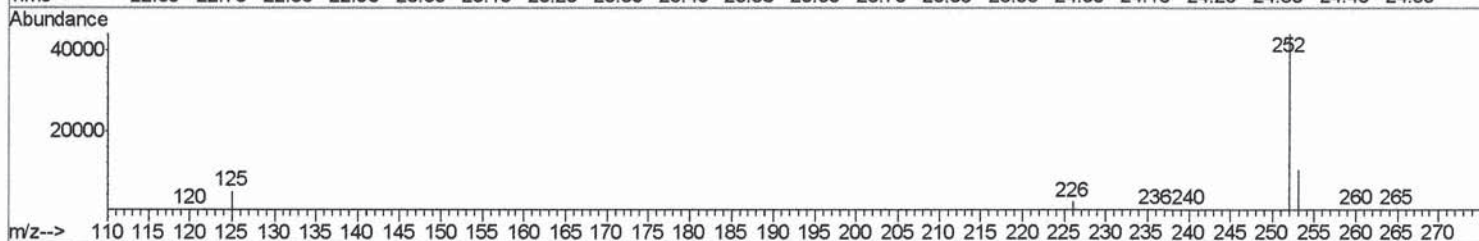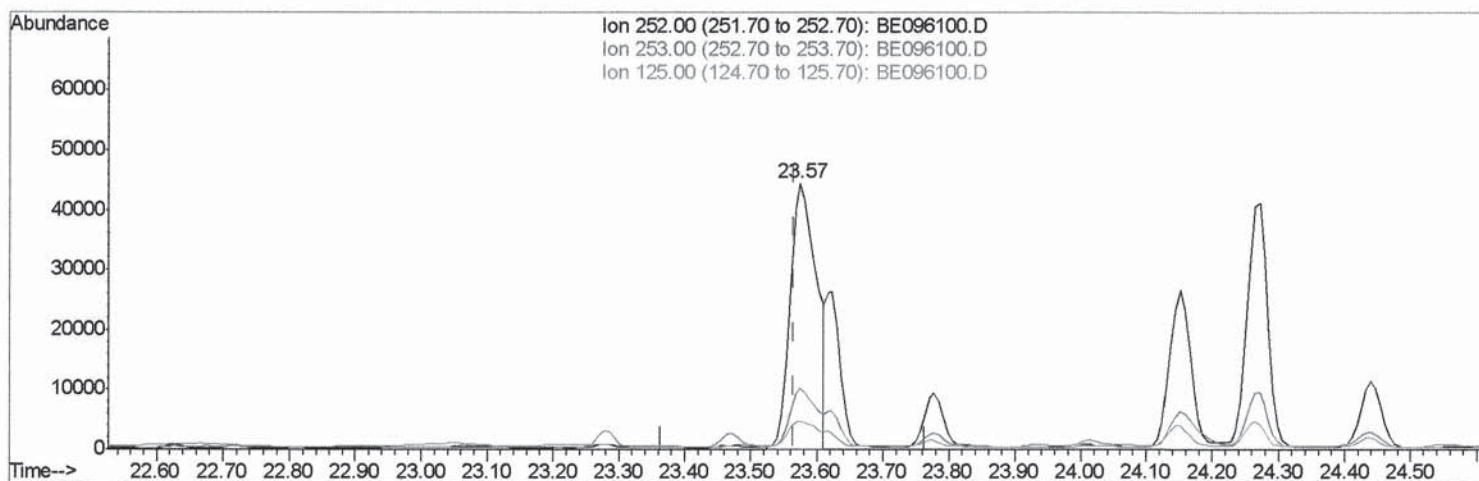

TIC: BE096100.D

(21) Benzo(b)fluoranthene

23.574min (+0.008) 3.79ng/ul m > SJ 4/24/18

response 124348

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.11
125.00	17.50	10.91
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

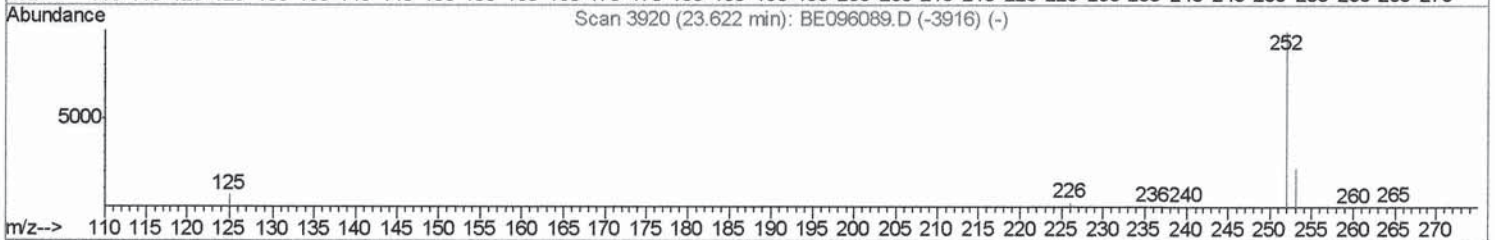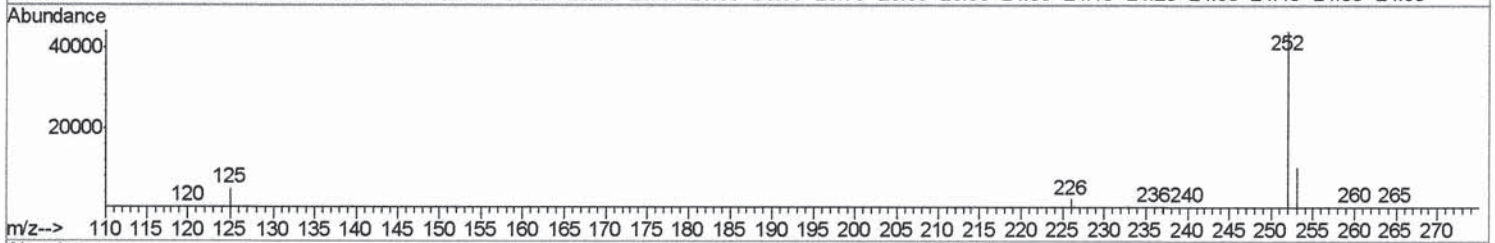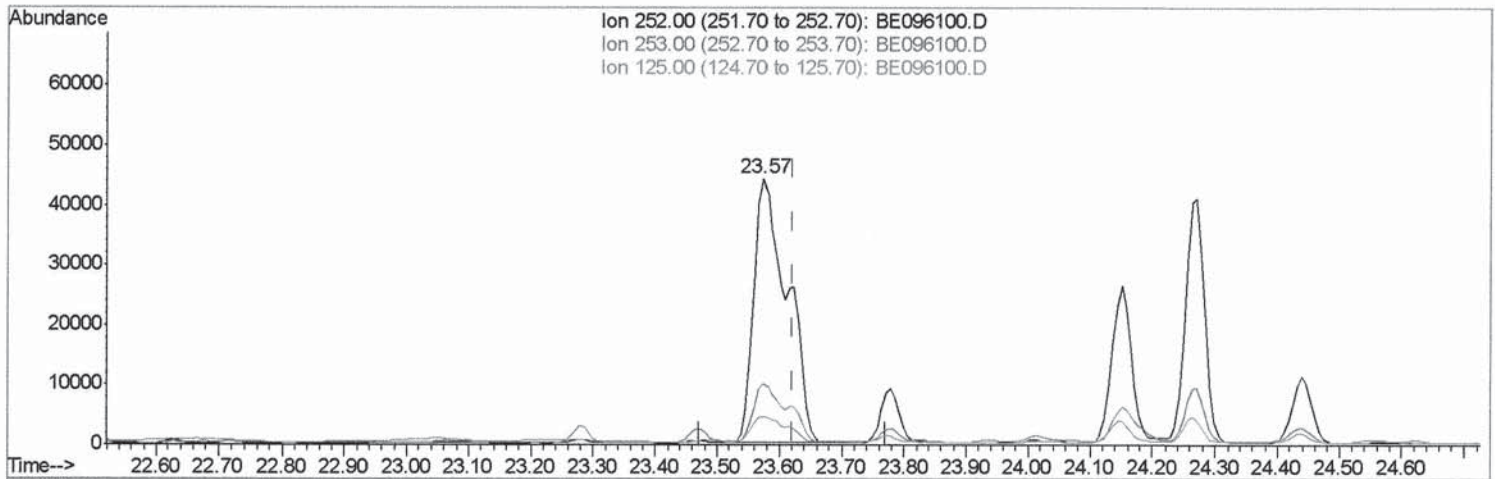

TIC: BE096100.D

(22) Benzo(k)fluoranthene

23.574min (-0.048) 4.97ng/ul

response 162517

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.11#
125.00	17.10	10.91#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:47:48 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

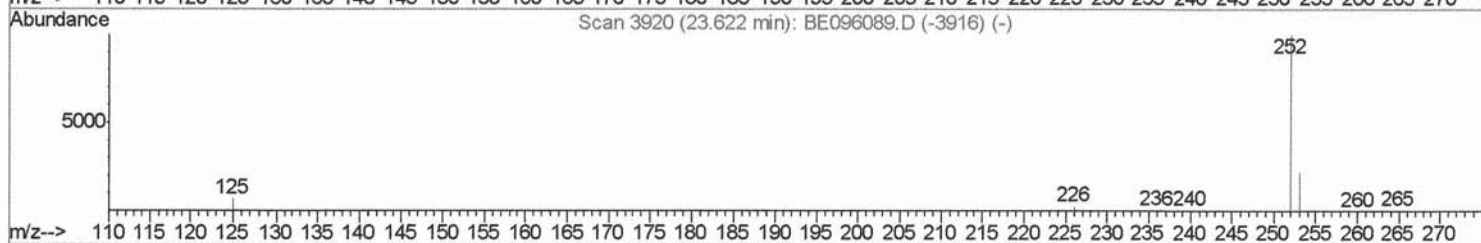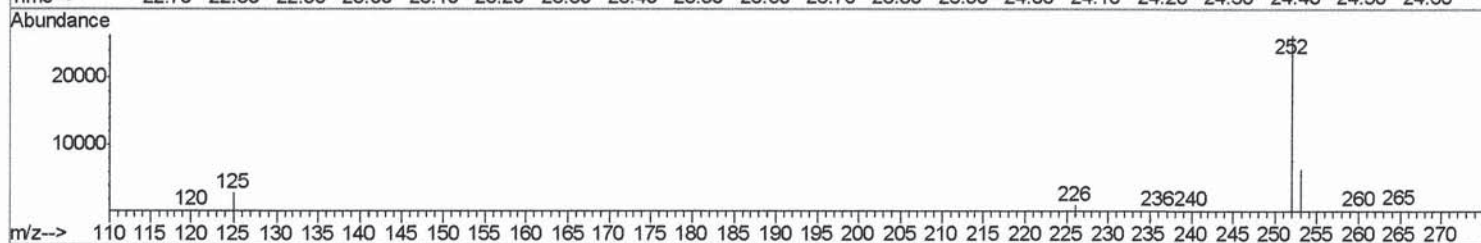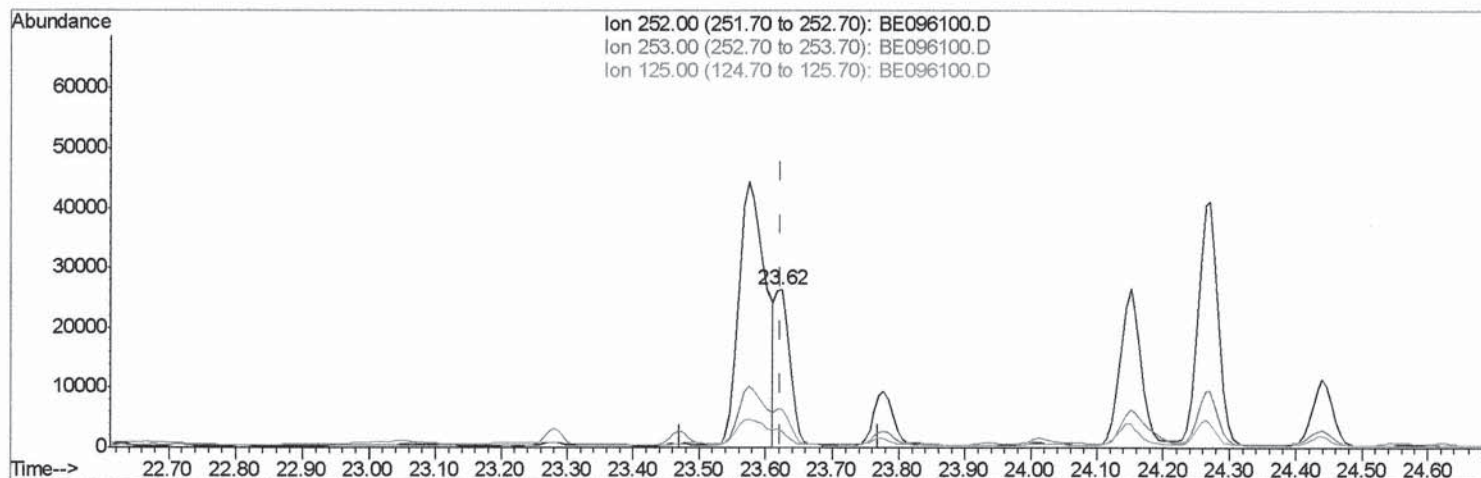

TIC: BE096100.D

(22) Benzo(k)fluoranthene

23.623min (+0.001) 1.25ng/ul m

> SJ 4/24/18

response 40928

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.85
125.00	17.10	10.77#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE042318\
 Data File : BE096100.D
 Acq On : 24 Apr 2018 00:14
 Operator : SJ/JU
 Sample : J2434-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB6

Manual Integrations
 APPROVED

Sohil
 4/24/2018 7:10:59 PM

Quant Time: Apr 24 14:49:16 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 24 06:59:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.38	152	2282	0.40	ng/ul	0.00
2) Naphthalene-d8	11.20	136	6599	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.97	164	3880	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.68	188	8524m	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	7705m	0.40	ng/ul	0.00
20) Perylene-d12	24.38	264	10144	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.76	152	2407	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.66	212	6491m	0.18	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	11.25	128	1784	0.097	ng/ul#	89
5) 2-Methylnaphthalene	12.83	142	1001	0.080	ng/ul	99
7) Acenaphthylene	14.70	152	5376	0.267	ng/ul	98
8) Acenaphthene	15.02	153	4072	0.282	ng/ul	93
9) Fluorene	15.99	166	8491	0.521	ng/ul#	89
12) Phenanthrene	17.72	178	144766m	5.762	ng/ul	
13) Anthracene	17.80	178	41602m	1.664	ng/ul	
15) Fluoranthene	19.68	202	273360m	7.997	ng/ul	
17) Pyrene	20.04	202	232996	8.899	ng/ul#	77
18) Benzo(a)anthracene	21.75	228	149912m	4.816	ng/ul	
19) Chrysene	21.80	228	94018	4.197	ng/ul	97
21) Benzo(b)fluoranthene	23.57	252	124348m	3.788	ng/ul	
22) Benzo(k)fluoranthene	23.62	252	40928m	1.252	ng/ul	
23) Benzo(a)pyrene	24.27	252	87538	2.764	ng/ul#	78
24) Indeno(1,2,3-cd)pyrene	27.17	276	55542	1.578	ng/ul#	74
25) Dibenzo(a,h)anthracene	27.18	278	14684	0.518	ng/ul	97
26) Benzo(g,h,i)perylene	28.05	276	53185	1.809	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed